

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014736.D
 Acq On : 25 May 2021 15:16
 Operator : CG/JU
 Sample : M2497-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014736.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	19	21	24	rBV3	9283	10601	0.17%	0.049%
2	3.240	24	26	28	rVV2	12315	8755	0.14%	0.041%
3	3.640	92	94	97	rBV4	6140	7337	0.12%	0.034%
4	3.781	116	118	121	rVB3	7884	6651	0.11%	0.031%
5	3.928	140	143	144	rVV2	6360	7102	0.11%	0.033%
6	3.952	144	147	153	rVV5	12464	21013	0.34%	0.097%
7	4.046	161	163	165	rBV3	6872	7423	0.12%	0.034%
8	4.110	172	174	179	rVB5	5548	7206	0.12%	0.033%
9	4.152	179	181	182	rBV	9314	6676	0.11%	0.031%
10	6.316	546	549	552	rVB4	6022	6697	0.11%	0.031%
11	6.651	602	606	607	rBV3	6808	7802	0.13%	0.036%
12	6.875	641	644	645	rVB	7927	7002	0.11%	0.032%
13	7.110	681	684	687	rBV3	5354	8057	0.13%	0.037%
14	7.710	777	786	796	rBV	712274	1182664	18.98%	5.487%
15	7.816	801	804	809	rVV5	5665	10955	0.18%	0.051%
16	8.010	835	837	841	rBV4	4676	6440	0.10%	0.030%
17	8.175	862	865	869	rVV4	6127	7014	0.11%	0.033%
18	8.481	913	917	920	rVB4	5651	7936	0.13%	0.037%
19	8.575	932	933	940	rVB5	5511	9269	0.15%	0.043%
20	9.516	1087	1093	1095	rVV3	3875	6412	0.10%	0.030%
21	9.910	1156	1160	1162	rVB3	4638	6345	0.10%	0.029%
22	9.957	1162	1168	1169	rBV3	5452	9845	0.16%	0.046%
23	10.281	1219	1223	1225	rVV4	4300	7092	0.11%	0.033%
24	10.498	1251	1260	1272	rBV	914021	1597985	25.65%	7.413%
25	10.875	1317	1324	1327	rBV4	4392	7146	0.11%	0.033%
26	11.951	1505	1507	1511	rBV4	6014	9392	0.15%	0.044%
27	13.581	1780	1784	1786	rBV4	5330	6561	0.11%	0.030%
28	14.363	1909	1917	1928	rBV	1682156	2512143	40.32%	11.654%
29	14.475	1933	1936	1938	rVB2	8324	7239	0.12%	0.034%
30	16.327	2248	2251	2254	rVB3	6012	6363	0.10%	0.030%
31	16.416	2263	2266	2269	rBV3	7157	9135	0.15%	0.042%
32	16.698	2310	2314	2317	rBV5	3966	6757	0.11%	0.031%
33	16.851	2333	2340	2342	rBV6	3687	8098	0.13%	0.038%
34	16.904	2345	2349	2354	rVB4	12808	20140	0.32%	0.093%
35	17.116	2379	2385	2395	rBV	2490265	3655352	58.67%	16.958%
36	17.222	2400	2403	2405	rVB3	6882	7959	0.13%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014736.D
 Acq On : 25 May 2021 15:16
 Operator : CG/JU
 Sample : M2497-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	17.939	2522	2525	2528	rBV5	5688	8550	0.14%	0.040%
38	18.092	2547	2551	2552	rBV3	6001	7021	0.11%	0.033%
39	18.416	2603	2606	2611	rVB5	4975	9517	0.15%	0.044%
40	18.610	2636	2639	2640	rBV3	7254	6850	0.11%	0.032%
41	18.710	2652	2656	2658	rBV3	7561	7843	0.13%	0.036%
42	18.851	2677	2680	2684	rBV4	5335	8280	0.13%	0.038%
43	19.068	2716	2717	2720	rBV2	7056	7139	0.11%	0.033%
44	19.421	2774	2777	2779	rVV4	7300	7561	0.12%	0.035%
45	19.515	2789	2793	2794	rVB4	6890	6686	0.11%	0.031%
46	19.539	2794	2797	2798	rBV3	10089	9828	0.16%	0.046%
47	19.610	2805	2809	2810	rBV4	8378	9104	0.15%	0.042%
48	19.745	2828	2832	2835	rVB5	8501	9819	0.16%	0.046%
49	19.786	2837	2839	2842	rVB4	7577	6750	0.11%	0.031%
50	19.886	2853	2856	2857	rBV2	7228	6235	0.10%	0.029%
51	20.057	2884	2885	2891	rVB6	9076	11106	0.18%	0.052%
52	20.110	2891	2894	2896	rBV4	8729	10969	0.18%	0.051%
53	20.257	2918	2919	2922	rBV3	10674	7955	0.13%	0.037%
54	20.439	2948	2950	2952	rBV3	7937	7936	0.13%	0.037%
55	20.474	2955	2956	2958	rBV2	12797	6972	0.11%	0.032%
56	20.533	2963	2966	2970	rVV6	20598	31177	0.50%	0.145%
57	20.615	2978	2980	2981	rBV2	12352	8103	0.13%	0.038%
58	20.727	2997	2999	3001	rBV3	12613	10324	0.17%	0.048%
59	20.780	3005	3008	3009	rBV3	14732	15147	0.24%	0.070%
60	20.821	3012	3015	3016	rBV3	12528	12301	0.20%	0.057%
61	20.839	3016	3018	3020	rVB3	16447	12634	0.20%	0.059%
62	21.104	3060	3063	3068	rBV6	36158	52398	0.84%	0.243%
63	21.315	3094	3099	3113	rBV	4237834	5483464	88.02%	25.439%
64	21.433	3117	3119	3120	rBV2	29750	19428	0.31%	0.090%
65	23.486	3464	3468	3474	rBV8	66947	114544	1.84%	0.531%
66	23.580	3476	3484	3496	rBV2	3162603	6229877	100.00%	28.901%
67	25.803	3856	3862	3867	rVB9	63085	146483	2.35%	0.680%
68	26.827	4034	4036	4037	rBV2	52591	43141	0.69%	0.200%




Sum of corrected areas: 21555706

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014736.D
Acq On : 25 May 2021 15:16
Operator : CG/JU
Sample : M2497-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

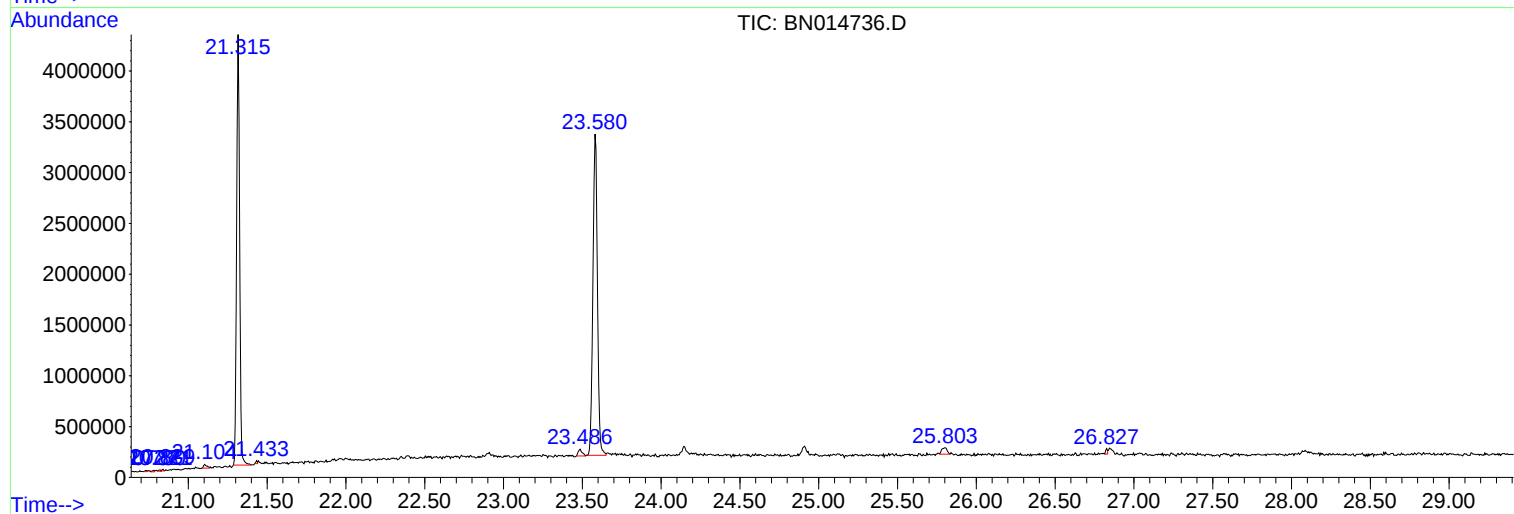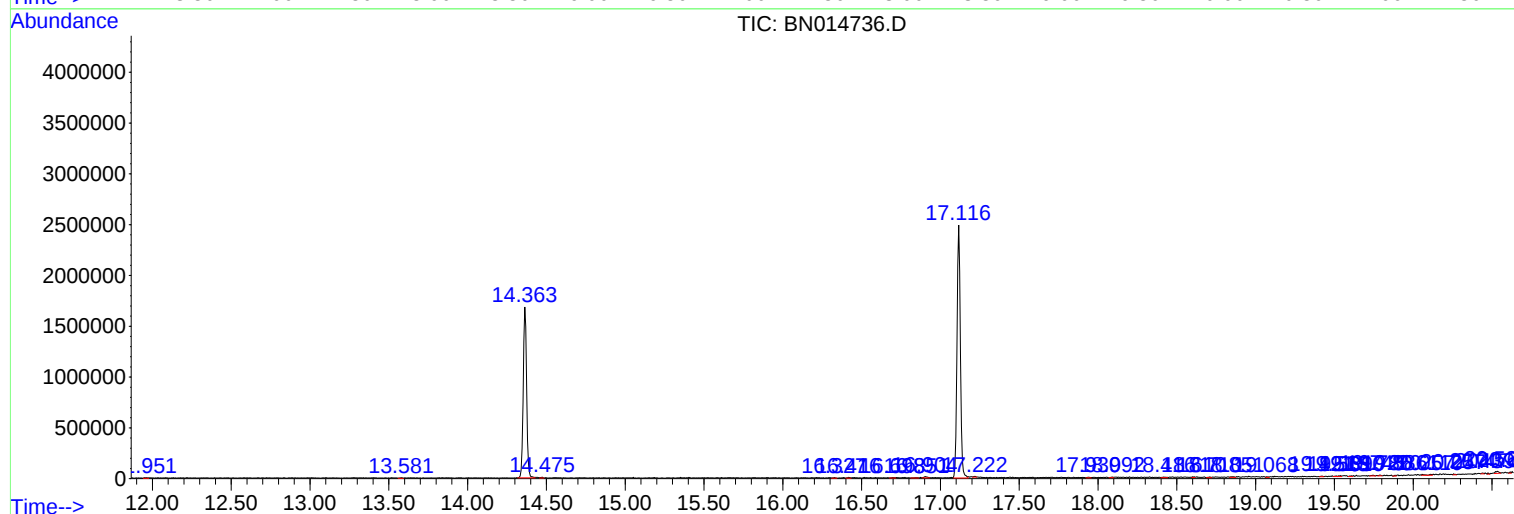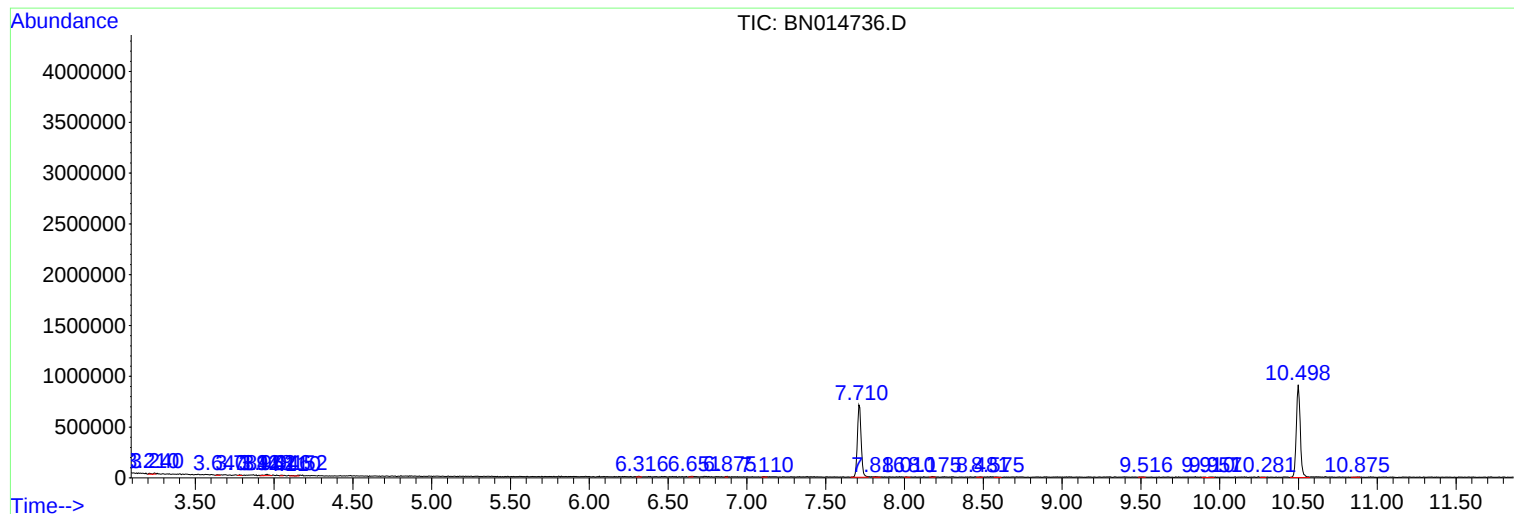

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014736.D
Acq On : 25 May 2021 15:16
Operator : CG/JU
Sample : M2497-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014736.D
Acq On : 25 May 2021 15:16
Operator : CG/JU
Sample : M2497-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
