

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014738.D
 Acq On : 25 May 2021 17:03
 Operator : CG/JU
 Sample : PB136607BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK607

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014738.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	19	24	34	rBV4	44229	86897	0.99%	0.150%
2	3.422	56	57	59	rBV2	11376	8848	0.10%	0.015%
3	3.469	61	65	67	rVV3	11374	13920	0.16%	0.024%
4	3.634	90	93	108	rBV	267570	590999	6.72%	1.023%
5	3.952	145	147	151	rBV4	8158	14395	0.16%	0.025%
6	4.634	261	263	266	rVB3	9355	9326	0.11%	0.016%
7	4.840	296	298	304	rVB4	8005	14861	0.17%	0.026%
8	4.899	304	308	310	rBV4	7681	12077	0.14%	0.021%
9	4.946	315	316	321	rBV3	6322	11524	0.13%	0.020%
10	5.052	330	334	338	rVB5	6685	12235	0.14%	0.021%
11	6.799	627	631	636	rBV4	6804	11233	0.13%	0.019%
12	6.887	641	646	658	rVV	666374	1129871	12.86%	1.955%
13	7.052	668	674	685	rBV	471057	857054	9.75%	1.483%
14	7.252	700	708	717	rBV	709596	1185129	13.48%	2.051%
15	7.716	777	787	795	rBV	475400	798405	9.08%	1.381%
16	7.963	826	829	834	rBV5	6237	9623	0.11%	0.017%
17	8.422	899	907	922	rBV	887749	1500418	17.07%	2.596%
18	8.804	969	972	974	rBV3	7244	8962	0.10%	0.016%
19	8.863	975	982	992	rVV	669475	1122543	12.77%	1.942%
20	9.587	1098	1105	1113	rBV	496352	859116	9.77%	1.486%
21	10.128	1189	1197	1208	rBV	844379	1563376	17.79%	2.705%
22	10.281	1222	1223	1230	rVB5	8304	10047	0.11%	0.017%
23	10.498	1253	1260	1268	rBV	663217	1101685	12.53%	1.906%
24	10.634	1275	1283	1293	rBV	854510	1525715	17.36%	2.640%
25	12.098	1523	1532	1537	rBV6	22456	39266	0.45%	0.068%
26	13.775	1810	1817	1825	rBV	1840540	2776326	31.59%	4.804%
27	14.051	1857	1864	1873	rBV	1921685	2924313	33.27%	5.060%
28	14.363	1911	1917	1923	rBV	1167411	1673040	19.04%	2.895%
29	14.581	1947	1954	1967	rBV	572942	1079563	12.28%	1.868%
30	15.363	2080	2087	2098	rBV	2746740	3965659	45.12%	6.861%
31	15.475	2100	2106	2114	rBV	689398	960109	10.92%	1.661%
32	15.604	2123	2128	2132	rBV6	32717	50771	0.58%	0.088%
33	16.151	2218	2221	2223	rVB4	10360	12002	0.14%	0.021%
34	16.428	2265	2268	2273	rBV5	5289	9476	0.11%	0.016%
35	16.733	2313	2320	2322	rBV6	5010	9683	0.11%	0.017%
36	16.904	2346	2349	2355	rBV4	13008	20498	0.23%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014738.D
 Acq On : 25 May 2021 17:03
 Operator : CG/JU
 Sample : PB136607BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK607

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	17.116	2378	2385	2396	rBV	1725042	2423761	27.58%	4.194%
38	17.216	2396	2402	2414	rBV	3362949	4707261	53.56%	8.145%
39	17.333	2419	2422	2425	rVV5	8194	11849	0.13%	0.021%
40	17.369	2425	2428	2431	rVB3	7081	9052	0.10%	0.016%
41	18.663	2644	2648	2652	rVB7	7589	11473	0.13%	0.020%
42	19.157	2725	2732	2735	rVV3	42789	67432	0.77%	0.117%
43	19.222	2739	2743	2746	rBV4	6734	12860	0.15%	0.022%
44	19.404	2770	2774	2780	rVB2	40997	62296	0.71%	0.108%
45	19.516	2787	2793	2802	rBV	4408508	6318817	71.89%	10.933%
46	19.774	2833	2837	2842	rBV7	13705	25278	0.29%	0.044%
47	20.080	2884	2889	2891	rBV5	9213	12742	0.14%	0.022%
48	20.357	2934	2936	2937	rBV2	13361	9075	0.10%	0.016%
49	20.416	2941	2946	2947	rBV5	12358	14221	0.16%	0.025%
50	20.492	2956	2959	2960	rBV3	11099	9028	0.10%	0.016%
51	20.533	2962	2966	2969	rBV6	23676	31245	0.36%	0.054%
52	20.692	2991	2993	2995	rVV3	13322	10620	0.12%	0.018%
53	20.851	3018	3020	3023	rBV4	16791	13697	0.16%	0.024%
54	20.921	3030	3032	3035	rBV4	11770	9104	0.10%	0.016%
55	21.045	3050	3053	3059	rBV8	18265	33394	0.38%	0.058%
56	21.104	3060	3063	3067	rVV4	27163	37490	0.43%	0.065%
57	21.316	3094	3099	3111	rBV	2851762	3704263	42.15%	6.409%
58	21.545	3137	3138	3140	rBV2	26363	20513	0.23%	0.035%
59	22.104	3231	3233	3234	rBV2	29284	16365	0.19%	0.028%
60	22.392	3279	3282	3286	rVB5	74449	77102	0.88%	0.133%
61	22.904	3367	3369	3374	rVB5	120026	143035	1.63%	0.247%
62	23.439	3452	3460	3466	rBV	4560337	8789109	100.00%	15.207%
63	23.580	3477	3484	3492	rVB2	2223067	4324620	49.20%	7.483%
64	24.145	3575	3580	3586	rVB6	168886	331767	3.77%	0.574%
65	24.904	3705	3709	3716	rVB7	165315	328899	3.74%	0.569%
66	25.798	3857	3861	3868	rVB10	119376	250555	2.85%	0.434%


Sum of corrected areas: 57795888

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014738.D
Acq On : 25 May 2021 17:03
Operator : CG/JU
Sample : PB136607BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK607

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

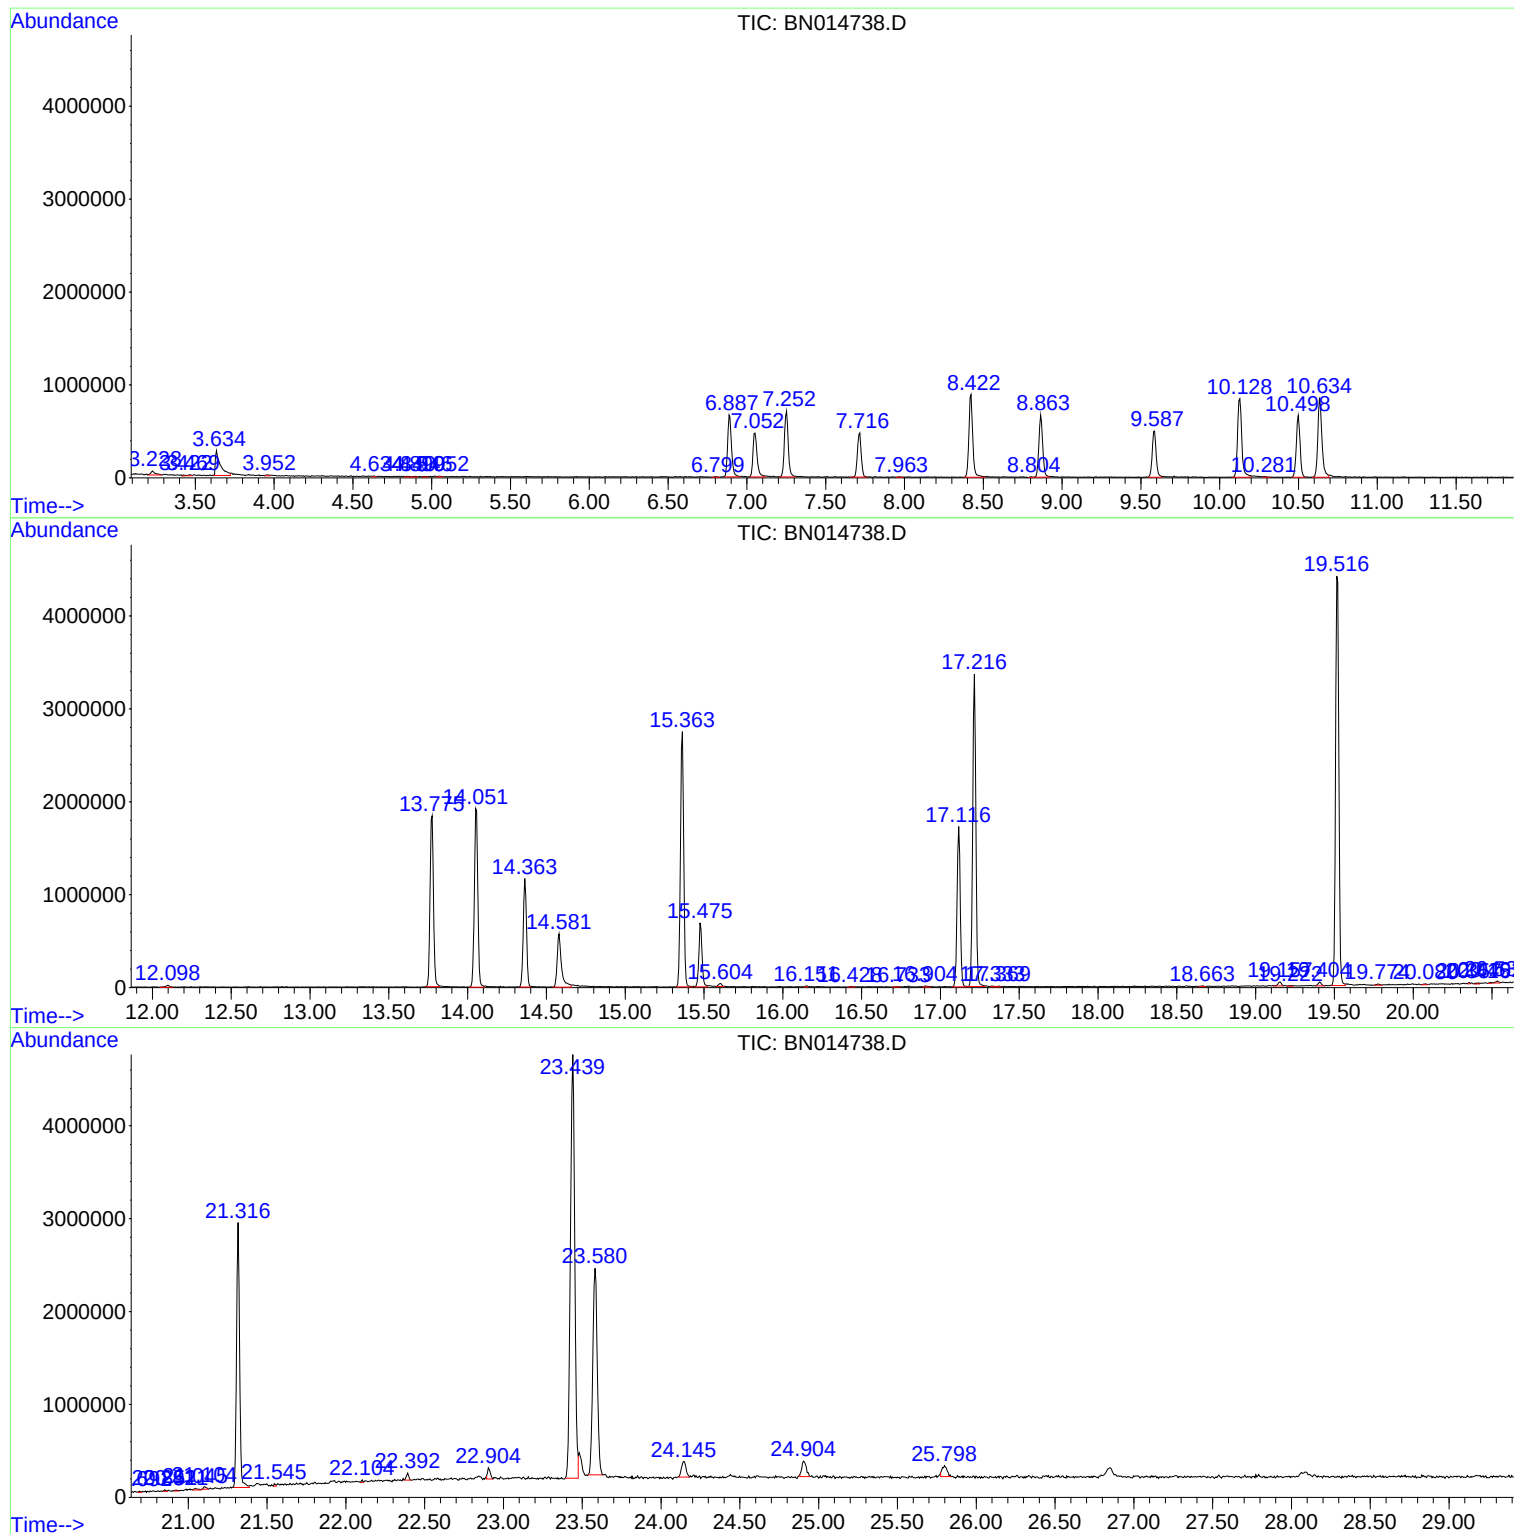

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014738.D
Acq On : 25 May 2021 17:03
Operator : CG/JU
Sample : PB136607BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK607

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014738.D
Acq On : 25 May 2021 17:03
Operator : CG/JU
Sample : PB136607BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK607

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------