

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014740.D
 Acq On : 25 May 2021 18:15
 Operator : CG/JU
 Sample : PB136630BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK630

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014740.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	32	rVB4	39305	62137	0.66%	0.093%
2	3.634	89	93	106	rBV	285909	654065	6.92%	0.980%
3	3.746	110	112	117	rVV4	16062	27529	0.29%	0.041%
4	3.905	138	139	143	rVB4	15149	11561	0.12%	0.017%
5	3.952	143	147	148	rBV3	11941	13734	0.15%	0.021%
6	4.046	160	163	165	rBV4	8422	11415	0.12%	0.017%
7	4.552	244	249	250	rBV3	8550	10598	0.11%	0.016%
8	5.264	367	370	374	rBV4	7760	12281	0.13%	0.018%
9	5.764	451	455	457	rVB4	7721	10004	0.11%	0.015%
10	6.887	639	646	655	rBV	744155	1249482	13.21%	1.873%
11	7.052	669	674	686	rBV	521306	917871	9.71%	1.376%
12	7.246	701	707	721	rVB	756058	1303911	13.79%	1.954%
13	7.711	779	786	795	rBV	596150	1008142	10.66%	1.511%
14	7.946	823	826	830	rVB5	5899	10172	0.11%	0.015%
15	7.987	830	833	837	rBV3	9867	12750	0.13%	0.019%
16	8.416	900	906	918	rBV	970881	1656400	17.52%	2.482%
17	8.863	972	982	991	rBV	739510	1267256	13.40%	1.899%
18	9.581	1098	1104	1114	rBV	592343	1004725	10.63%	1.506%
19	10.128	1188	1197	1210	rBV	989293	1754907	18.56%	2.630%
20	10.499	1254	1260	1268	rVB	826769	1378921	14.58%	2.067%
21	10.634	1276	1283	1296	rBV	935439	1725190	18.24%	2.586%
22	12.099	1528	1532	1540	rVB5	19070	36945	0.39%	0.055%
23	13.775	1809	1817	1829	rBV	2127003	3141357	33.22%	4.708%
24	14.051	1856	1864	1874	rVV	2198490	3300421	34.90%	4.946%
25	14.363	1910	1917	1924	rBV	1517095	2216208	23.44%	3.321%
26	14.575	1947	1953	1974	rBV	697852	1294670	13.69%	1.940%
27	15.363	2078	2087	2094	rBV	2915431	4441770	46.97%	6.657%
28	15.475	2098	2106	2113	rBV	828184	1162591	12.29%	1.742%
29	15.604	2124	2128	2132	rVB4	45236	64535	0.68%	0.097%
30	16.151	2215	2221	2224	rBV6	17390	29394	0.31%	0.044%
31	16.892	2344	2347	2349	rBV3	12440	11983	0.13%	0.018%
32	17.116	2379	2385	2393	rVB	2167033	3079440	32.57%	4.615%
33	17.216	2395	2402	2411	rBV	3692450	5315947	56.22%	7.967%
34	17.545	2453	2458	2460	rVB5	8054	10534	0.11%	0.016%
35	18.086	2545	2550	2554	rBV6	9054	13556	0.14%	0.020%
36	19.145	2725	2730	2735	rBV3	50527	81176	0.86%	0.122%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014740.D
 Acq On : 25 May 2021 18:15
 Operator : CG/JU
 Sample : PB136630BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK630

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	19.322	2756	2760	2763	rBV4	8346	13514	0.14%	0.020%
38	19.404	2770	2774	2779	rBV2	46549	69241	0.73%	0.104%
39	19.516	2787	2793	2805	rBV	5186734	7152316	75.64%	10.719%
40	19.698	2821	2824	2826	rBV3	8779	11788	0.12%	0.018%
41	19.969	2867	2870	2871	rBV3	10786	11171	0.12%	0.017%
42	20.339	2931	2933	2940	rVB7	13579	22251	0.24%	0.033%
43	20.398	2940	2943	2948	rBV6	12600	24804	0.26%	0.037%
44	20.445	2948	2951	2952	rBV3	14228	12405	0.13%	0.019%
45	20.469	2952	2955	2956	rBV3	8124	10173	0.11%	0.015%
46	20.528	2961	2965	2970	rVV8	23978	43731	0.46%	0.066%
47	20.669	2987	2989	2992	rVB4	12440	11023	0.12%	0.017%
48	21.033	3049	3051	3052	rBV2	12736	9969	0.11%	0.015%
49	21.092	3059	3061	3062	rBV2	25417	18217	0.19%	0.027%
50	21.310	3093	3098	3108	rBV	3460991	4682789	49.52%	7.018%
51	21.427	3116	3118	3121	rBV4	30638	33719	0.36%	0.051%
52	22.904	3365	3369	3374	rVB6	105724	154835	1.64%	0.232%
53	23.433	3450	3459	3466	rBV	4787327	9455907	100.00%	14.172%
54	23.580	3476	3484	3496	rVB2	2700733	5546521	58.66%	8.313%
55	24.139	3574	3579	3586	rBV5	190273	398836	4.22%	0.598%
56	24.904	3703	3709	3717	rVB7	192570	432045	4.57%	0.648%
57	25.792	3857	3860	3869	rVB8	137881	305034	3.23%	0.457%


Sum of corrected areas: 66723867

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014740.D
Acq On : 25 May 2021 18:15
Operator : CG/JU
Sample : PB136630BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK630

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

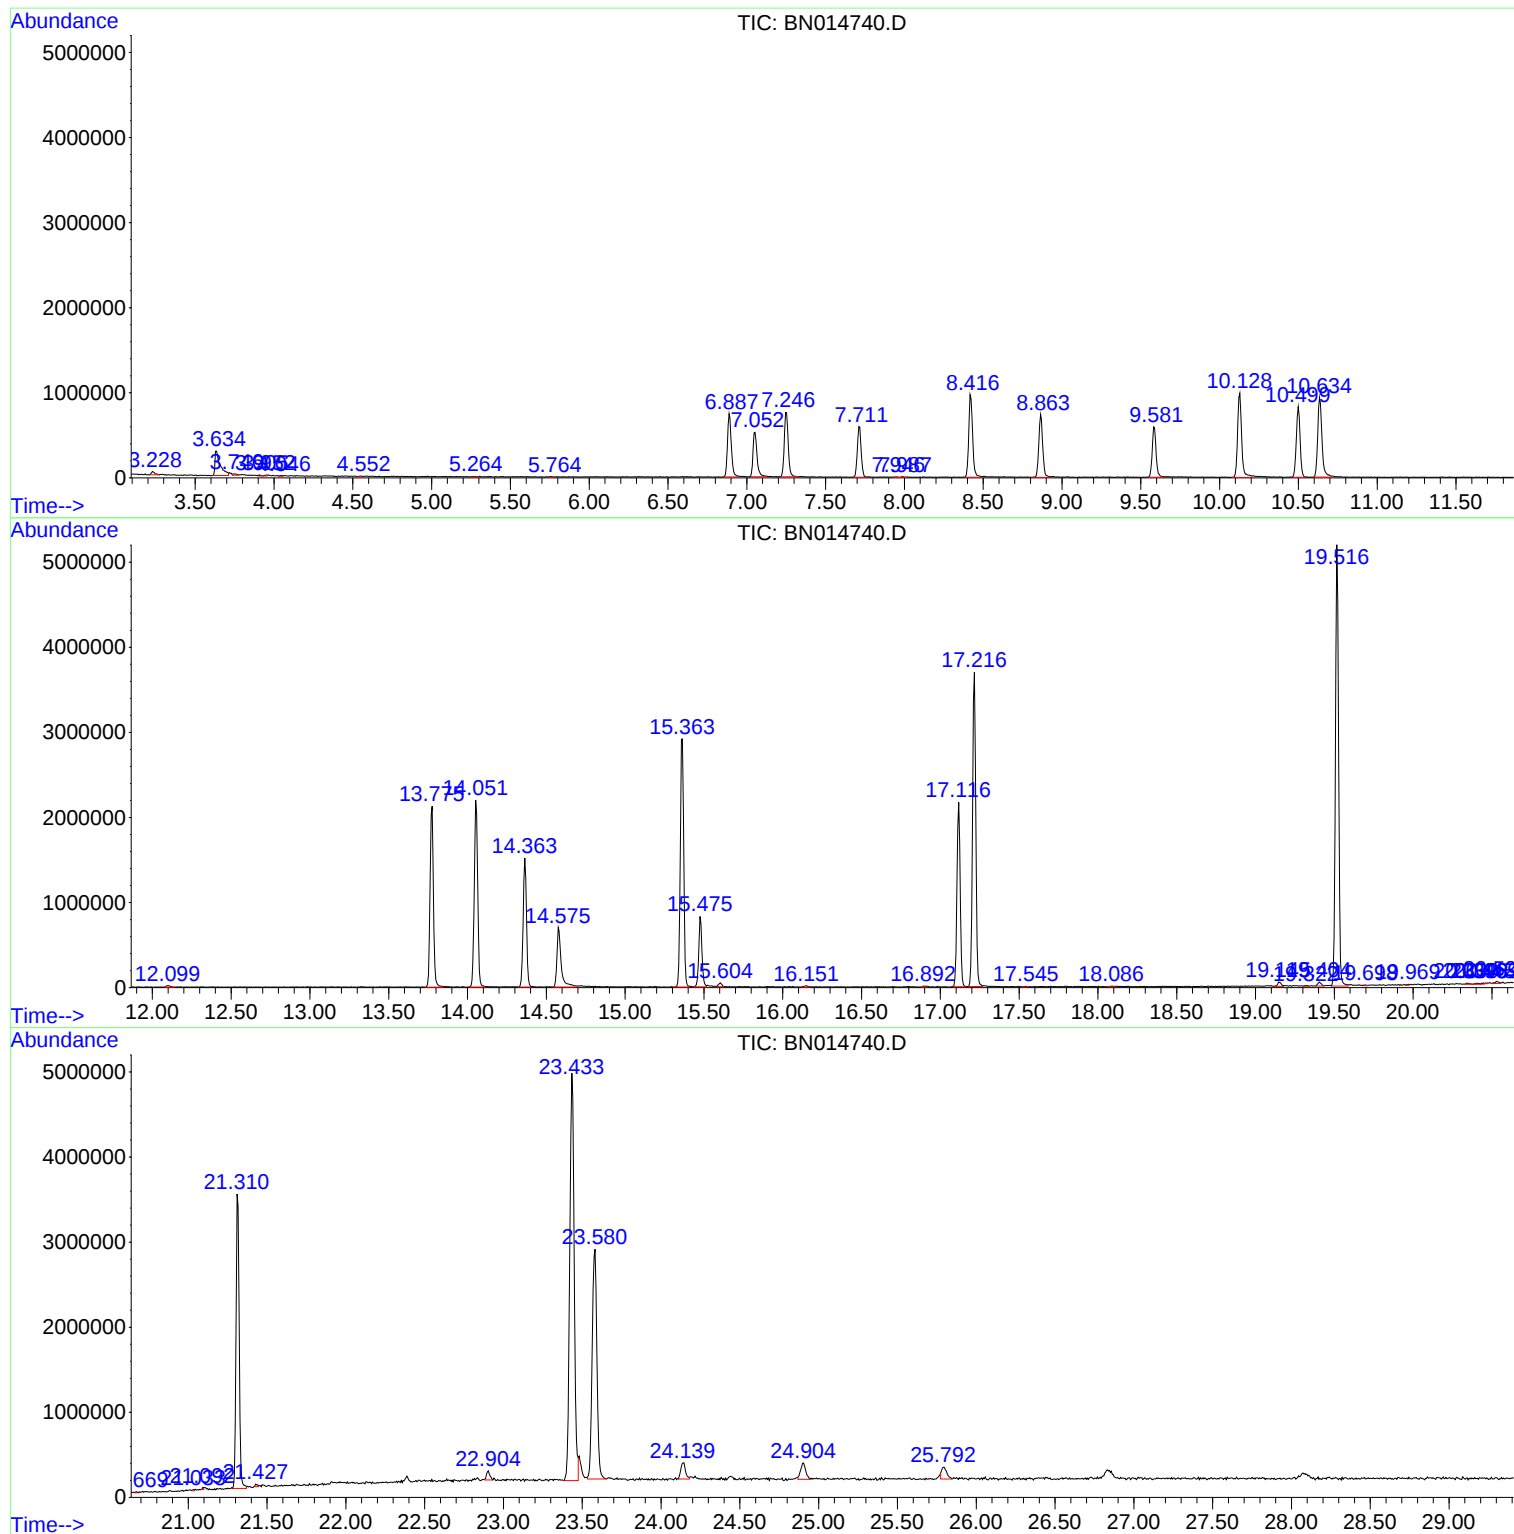

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014740.D
Acq On : 25 May 2021 18:15
Operator : CG/JU
Sample : PB136630BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK630

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014740.D
Acq On : 25 May 2021 18:15
Operator : CG/JU
Sample : PB136630BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK630

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc