

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014746.D
 Acq On : 25 May 2021 21:49
 Operator : CG/JU
 Sample : M2493-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB420

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014746.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	22	24	28	rBV3	33503	44871	0.35%	0.048%
2	3.858	125	131	135	rBV4	36012	68496	0.53%	0.073%
3	3.952	145	147	151	rVB4	16913	16339	0.13%	0.017%
4	4.052	161	164	169	rBV5	15734	24115	0.19%	0.026%
5	4.469	231	235	245	rVB4	94686	173439	1.35%	0.185%
6	4.858	295	301	304	rBV5	13112	20771	0.16%	0.022%
7	6.887	638	646	656	rBV	265283	462568	3.60%	0.494%
8	7.052	668	674	688	rBV	881473	1484356	11.56%	1.585%
9	7.246	700	707	720	rBV	1043697	1744020	13.59%	1.862%
10	7.710	776	786	794	rBV	1115245	1780511	13.87%	1.901%
11	8.416	898	906	917	rBV	863012	1448055	11.28%	1.546%
12	8.863	972	982	995	rBV	1217543	2049514	15.97%	2.188%
13	9.587	1097	1105	1114	rBV	966312	1670381	13.01%	1.783%
14	10.122	1189	1196	1209	rBV	1561131	2785229	21.70%	2.974%
15	10.498	1253	1260	1271	rBV	1411678	2362545	18.41%	2.522%
16	10.646	1279	1285	1289	rBV9	18936	33622	0.26%	0.036%
17	12.093	1526	1531	1538	rVB2	36288	60521	0.47%	0.065%
18	12.316	1563	1569	1575	rBV7	7103	13309	0.10%	0.014%
19	13.328	1738	1741	1745	rBV4	10192	15705	0.12%	0.017%
20	13.775	1810	1817	1831	rBV	3387430	4876798	37.99%	5.207%
21	14.051	1856	1864	1876	rBV	3477933	5289164	41.21%	5.647%
22	14.363	1909	1917	1924	rBV	2442529	3679197	28.66%	3.928%
23	14.581	1946	1954	1967	rBV3	208722	457793	3.57%	0.489%
24	15.192	2052	2058	2062	rVB3	24485	39895	0.31%	0.043%
25	15.363	2078	2087	2097	rBV	4677396	7031794	54.78%	7.508%
26	15.475	2099	2106	2114	rBV	1653144	2252664	17.55%	2.405%
27	15.598	2122	2127	2135	rVB3	70441	120574	0.94%	0.129%
28	15.734	2146	2150	2155	rBV6	12653	19172	0.15%	0.020%
29	15.928	2179	2183	2187	rBV4	10713	15393	0.12%	0.016%
30	16.151	2215	2221	2227	rVB4	37091	64171	0.50%	0.069%
31	16.322	2246	2250	2256	rBV7	7277	14348	0.11%	0.015%
32	16.716	2316	2317	2321	rVB4	12565	13753	0.11%	0.015%
33	16.798	2327	2331	2335	rBV4	13958	22824	0.18%	0.024%
34	16.904	2342	2349	2352	rBV5	20607	31264	0.24%	0.033%
35	17.116	2379	2385	2394	rBV	3419513	4813556	37.50%	5.139%
36	17.216	2395	2402	2415	rVV	5751569	8397191	65.42%	8.966%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014746.D
 Acq On : 25 May 2021 21:49
 Operator : CG/JU
 Sample : M2493-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB420

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	17.398	2429	2433	2437	rBV5	18849	37106	0.29%	0.040%
38	17.792	2496	2500	2505	rBV7	66274	85952	0.67%	0.092%
39	17.904	2517	2519	2523	rVV4	14221	19547	0.15%	0.021%
40	17.963	2525	2529	2532	rVV5	10018	16607	0.13%	0.018%
41	18.022	2535	2539	2547	rVV4	133126	243624	1.90%	0.260%
42	18.092	2547	2551	2554	rVV4	33910	59013	0.46%	0.063%
43	18.239	2572	2576	2578	rBV5	19780	22805	0.18%	0.024%
44	18.604	2634	2638	2642	rBV5	23680	27683	0.22%	0.030%
45	18.792	2665	2670	2673	rBV7	10951	18750	0.15%	0.020%
46	18.898	2684	2688	2693	rVB8	9094	13009	0.10%	0.014%
47	19.151	2727	2731	2741	rVB	92625	151281	1.18%	0.162%
48	19.310	2753	2758	2769	rBV3	247544	397695	3.10%	0.425%
49	19.404	2769	2774	2780	rVV	79239	124855	0.97%	0.133%
50	19.516	2787	2793	2802	rBV2	7566423	10733563	83.62%	11.460%
51	20.533	2963	2966	2969	rVV4	26699	31337	0.24%	0.033%
52	20.574	2971	2973	2976	rVB4	13705	13461	0.10%	0.014%
53	21.039	3050	3052	3056	rBV5	31143	29462	0.23%	0.031%
54	21.239	3083	3086	3089	rVB5	50191	59812	0.47%	0.064%
55	21.310	3093	3098	3108	rBV	4619393	6422328	50.03%	6.857%
56	21.916	3198	3201	3204	rBV5	50126	66183	0.52%	0.071%
57	22.174	3242	3245	3248	rBV4	81590	99941	0.78%	0.107%
58	22.386	3278	3281	3287	rVB6	103465	131915	1.03%	0.141%
59	22.904	3365	3369	3374	rVB5	142007	194726	1.52%	0.208%
60	23.433	3451	3459	3475	rBV2	6138722	12835813	100.00%	13.705%
61	23.580	3476	3484	3496	rVB2	3497822	6899896	53.76%	7.367%
62	24.139	3573	3579	3584	rBV6	230739	464726	3.62%	0.496%
63	24.433	3627	3629	3635	rVB7	64422	99171	0.77%	0.106%
64	24.904	3704	3709	3718	rVB6	192371	417843	3.26%	0.446%
65	25.798	3855	3861	3867	rVB9	120219	292450	2.28%	0.312%
66	26.833	4035	4037	4047	rVB8	126530	250944	1.96%	0.268%


Sum of corrected areas: 93659416

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014746.D
Acq On : 25 May 2021 21:49
Operator : CG/JU
Sample : M2493-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB420

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

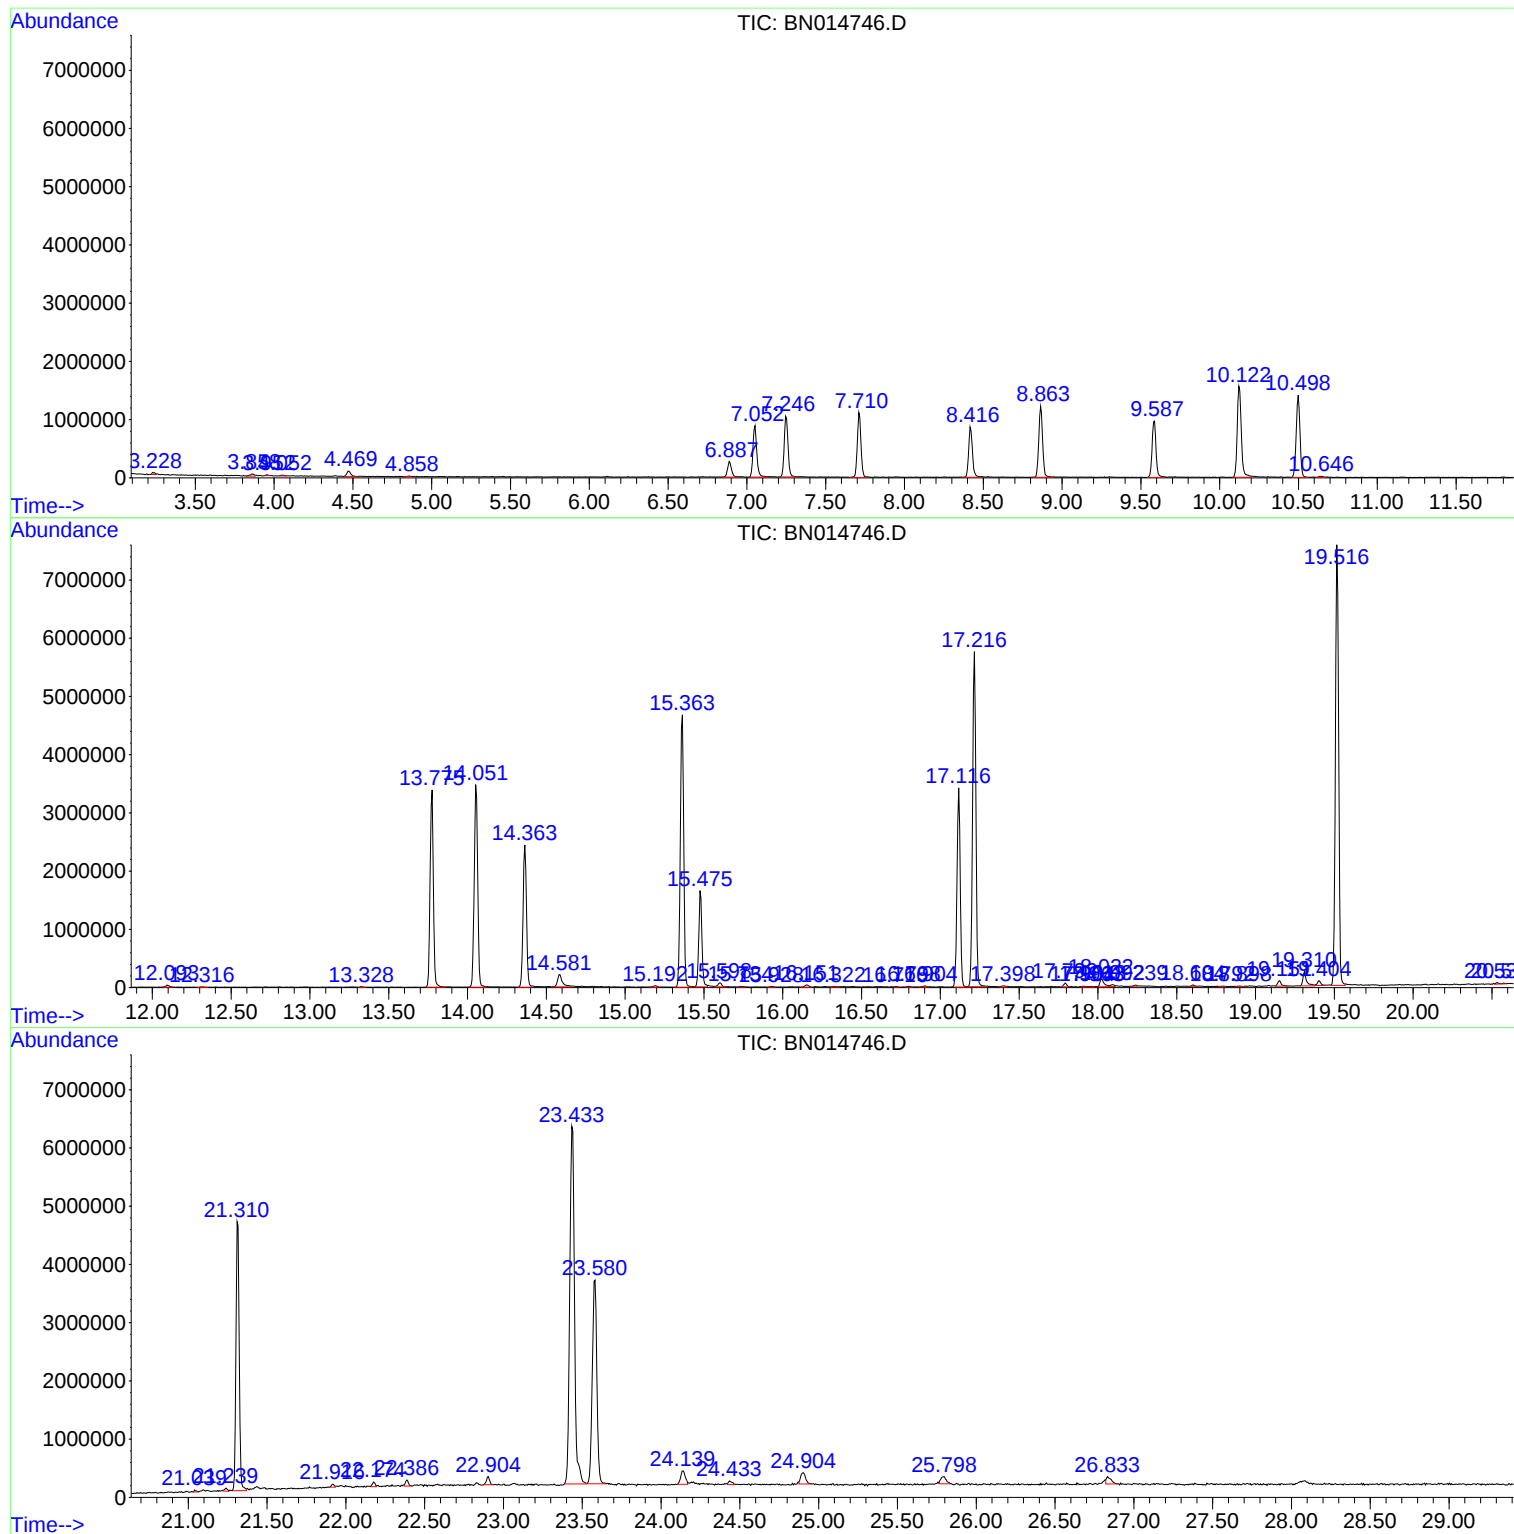

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014746.D
Acq On : 25 May 2021 21:49
Operator : CG/JU
Sample : M2493-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB420

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014746.D
Acq On : 25 May 2021 21:49
Operator : CG/JU
Sample : M2493-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB420

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
