

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014755.D
 Acq On : 26 May 2021 03:45
 Operator : CG/JU
 Sample : M2493-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB426

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014755.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.946	144	146	147	rBV	15039	7809	0.14%	0.026%
2	4.187	185	187	192	rVB4	8853	9770	0.18%	0.033%
3	4.281	202	203	207	rBV4	9998	12678	0.23%	0.043%
4	4.340	211	213	215	rBV3	9553	10112	0.19%	0.034%
5	4.558	248	250	253	rVB4	8952	8139	0.15%	0.027%
6	5.752	452	453	456	rBV3	10839	8643	0.16%	0.029%
7	6.334	551	552	555	rBV3	10055	7776	0.14%	0.026%
8	6.852	638	640	642	rBV3	6838	7761	0.14%	0.026%
9	6.893	642	647	650	rBV3	31412	53800	0.99%	0.181%
10	7.052	668	674	683	rBV2	114285	223785	4.11%	0.755%
11	7.252	700	708	716	rVB2	137035	257140	4.73%	0.867%
12	7.452	741	742	747	rVB4	6841	7821	0.14%	0.026%
13	7.710	779	786	797	rBV	632101	1053734	19.37%	3.553%
14	8.246	875	877	880	rBV4	8147	9239	0.17%	0.031%
15	8.422	898	907	920	rBV2	97994	209695	3.86%	0.707%
16	8.628	941	942	947	rVB3	5476	7187	0.13%	0.024%
17	8.863	975	982	993	rBV	149472	278286	5.12%	0.938%
18	9.493	1086	1089	1095	rVB6	4628	9318	0.17%	0.031%
19	9.581	1098	1104	1110	rBV3	103597	189411	3.48%	0.639%
20	9.681	1119	1121	1124	rBV4	6374	7732	0.14%	0.026%
21	10.128	1189	1197	1207	rBV2	156904	335568	6.17%	1.132%
22	10.199	1207	1209	1214	rVB5	10036	15022	0.28%	0.051%
23	10.499	1253	1260	1273	rBV	794006	1428942	26.27%	4.818%
24	10.651	1278	1286	1290	rBV7	12031	25792	0.47%	0.087%
25	10.987	1342	1343	1347	rVB3	7531	7080	0.13%	0.024%
26	11.334	1398	1402	1404	rBV4	7153	7584	0.14%	0.026%
27	11.504	1426	1431	1433	rBV4	5741	7556	0.14%	0.025%
28	12.022	1516	1519	1523	rVB5	6128	10304	0.19%	0.035%
29	13.269	1724	1731	1734	rBV5	5991	10875	0.20%	0.037%
30	13.769	1810	1816	1821	rBV	544118	776045	14.27%	2.617%
31	13.916	1839	1841	1845	rVB3	7585	7150	0.13%	0.024%
32	14.051	1857	1864	1870	rBV	519868	756070	13.90%	2.549%
33	14.287	1902	1904	1910	rBV4	5296	8663	0.16%	0.029%
34	14.363	1910	1917	1929	rVB	1504943	2250606	41.38%	7.589%
35	14.504	1939	1941	1944	rVB3	7749	8346	0.15%	0.028%
36	14.598	1953	1957	1958	rBV3	10171	8901	0.16%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014755.D
 Acq On : 26 May 2021 03:45
 Operator : CG/JU
 Sample : M2493-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB426

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	15.104	2039	2043	2045	rBV4	9641	13260	0.24%	0.045%
38	15.357	2079	2086	2095	rBV	800702	1180975	21.71%	3.982%
39	15.475	2102	2106	2111	rBV6	48489	68913	1.27%	0.232%
40	15.592	2125	2126	2130	rBV4	9803	10305	0.19%	0.035%
41	16.904	2343	2349	2351	rVB7	14066	21949	0.40%	0.074%
42	17.116	2376	2385	2395	rBV	2209396	3215455	59.12%	10.842%
43	17.210	2395	2401	2415	rVB	1049821	1623640	29.85%	5.475%
44	17.486	2446	2448	2452	rBV4	7134	7827	0.14%	0.026%
45	17.575	2462	2463	2465	rBV	11264	8134	0.15%	0.027%
46	17.922	2517	2522	2523	rBV4	6157	9810	0.18%	0.033%
47	18.022	2537	2539	2546	rVB7	13092	17426	0.32%	0.059%
48	18.339	2589	2593	2594	rBV4	6429	7829	0.14%	0.026%
49	18.363	2595	2597	2602	rVB6	9264	8335	0.15%	0.028%
50	18.539	2624	2627	2629	rBV4	7299	11456	0.21%	0.039%
51	18.616	2637	2640	2643	rBV4	7648	9994	0.18%	0.034%
52	18.722	2655	2658	2661	rBV3	6191	11339	0.21%	0.038%
53	18.792	2665	2670	2671	rBV4	8034	10601	0.19%	0.036%
54	19.151	2728	2731	2738	rVB7	16996	31672	0.58%	0.107%
55	19.404	2770	2774	2777	rBV6	13821	18074	0.33%	0.061%
56	19.516	2787	2793	2800	rBV	1596791	2258671	41.53%	7.616%
57	19.657	2815	2817	2820	rBV4	9108	8874	0.16%	0.030%
58	21.033	3047	3051	3053	rBV5	47695	68954	1.27%	0.233%
59	21.310	3093	3098	3106	rBV2	3572843	4694961	86.33%	15.831%
60	23.427	3452	3458	3464	rBV2	1543554	2854715	52.49%	9.626%
61	23.574	3476	3483	3492	rVB	2828205	5438686	100.00%	18.339%




Sum of corrected areas: 29656195

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014755.D
Acq On : 26 May 2021 03:45
Operator : CG/JU
Sample : M2493-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

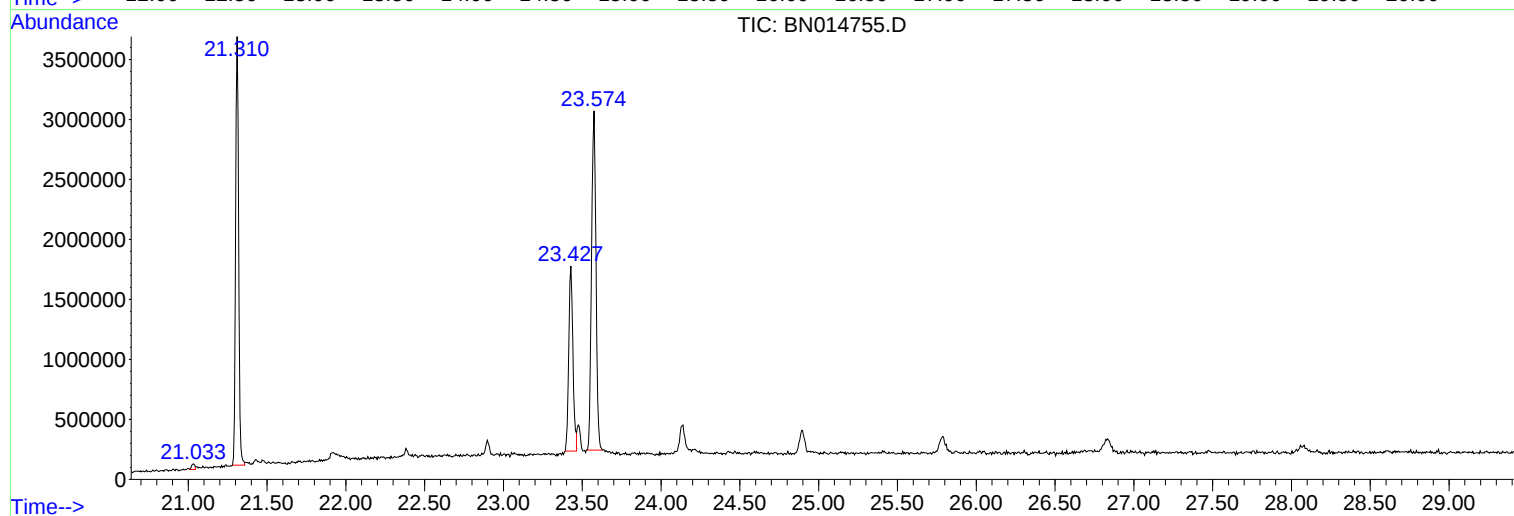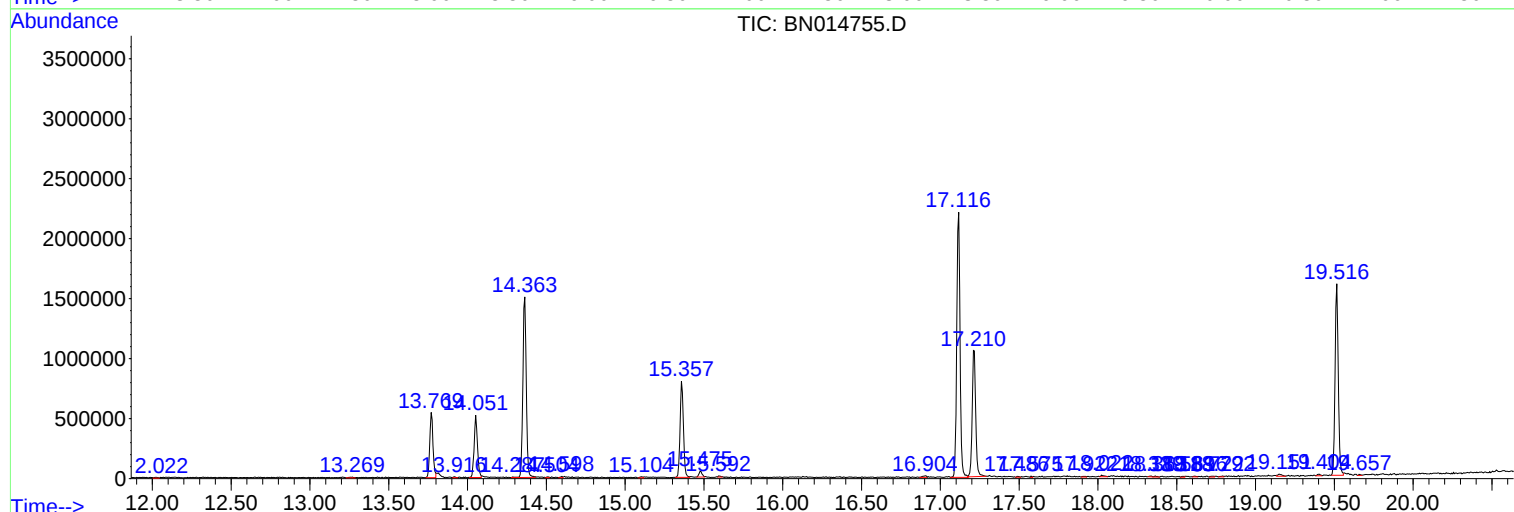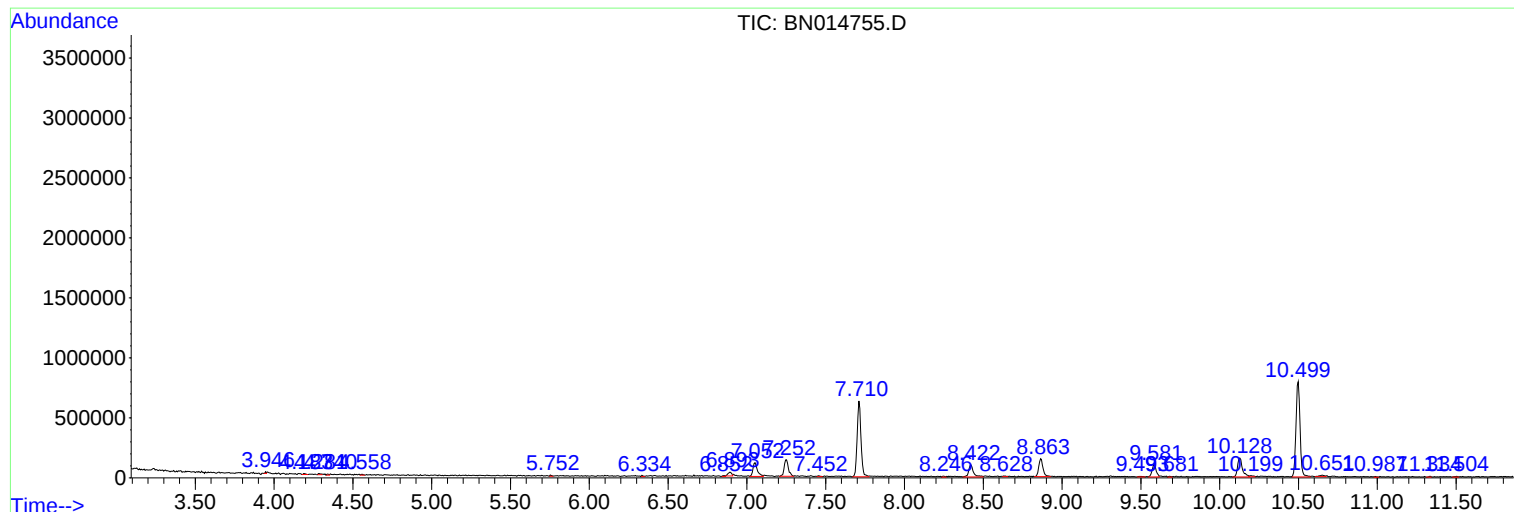

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014755.D
Acq On : 26 May 2021 03:45
Operator : CG/JU
Sample : M2493-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014755.D
Acq On : 26 May 2021 03:45
Operator : CG/JU
Sample : M2493-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
