

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014757.D
 Acq On : 26 May 2021 04:55
 Operator : CG/JU
 Sample : M2493-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB429

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014757.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	27	rBV3	24693	32472	0.24%	0.037%
2	3.581	83	84	90	rVB6	10175	14127	0.10%	0.016%
3	3.864	127	132	139	rVB6	32407	60602	0.44%	0.069%
4	4.846	290	299	304	rBV7	12903	28486	0.21%	0.032%
5	6.110	508	514	518	rBV8	15831	23500	0.17%	0.027%
6	6.887	638	646	659	rVV	237806	438174	3.19%	0.499%
7	7.046	667	673	686	rBV	712929	1233108	8.97%	1.403%
8	7.246	700	707	720	rVV	883226	1435497	10.44%	1.634%
9	7.710	779	786	797	rBV	850693	1349003	9.81%	1.535%
10	8.416	899	906	914	rBV2	727000	1195791	8.70%	1.361%
11	8.863	975	982	995	rBV	1024038	1707647	12.42%	1.943%
12	9.299	1054	1056	1065	rVB4	14293	19651	0.14%	0.022%
13	9.581	1096	1104	1115	rBV	863815	1417227	10.31%	1.613%
14	10.122	1189	1196	1210	rBV	1333426	2324334	16.91%	2.645%
15	10.493	1252	1259	1271	rVB	1128473	1924288	14.00%	2.190%
16	10.640	1278	1284	1293	rBV2	106285	201676	1.47%	0.229%
17	12.087	1526	1530	1531	rBV3	25919	27031	0.20%	0.031%
18	13.269	1726	1731	1733	rBV5	13209	21163	0.15%	0.024%
19	13.769	1807	1816	1821	rBV	3075050	4363573	31.74%	4.966%
20	13.816	1821	1824	1829	rVB	141867	202024	1.47%	0.230%
21	14.051	1857	1864	1875	rBV	3163638	4660354	33.90%	5.303%
22	14.122	1875	1876	1881	rVB3	11080	15137	0.11%	0.017%
23	14.275	1898	1902	1907	rVB6	9663	16486	0.12%	0.019%
24	14.363	1910	1917	1926	rBV	2000015	2950655	21.46%	3.358%
25	14.581	1947	1954	1962	rBV3	210198	418238	3.04%	0.476%
26	15.110	2039	2044	2051	rBV	120559	162379	1.18%	0.185%
27	15.357	2080	2086	2096	rBV	4268014	6403890	46.58%	7.287%
28	15.475	2100	2106	2117	rBV	1468490	2013179	14.64%	2.291%
29	15.598	2121	2127	2133	rVV3	58426	86836	0.63%	0.099%
30	16.039	2199	2202	2207	rVV7	15055	19231	0.14%	0.022%
31	16.086	2207	2210	2214	rVV6	9727	15220	0.11%	0.017%
32	16.151	2216	2221	2225	rVB5	26726	38894	0.28%	0.044%
33	16.357	2250	2256	2260	rBV5	26224	35899	0.26%	0.041%
34	16.516	2279	2283	2288	rVB6	9731	17011	0.12%	0.019%
35	16.792	2328	2330	2334	rVB4	15819	18063	0.13%	0.021%
36	16.904	2345	2349	2351	rBV4	14105	17052	0.12%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014757.D
 Acq On : 26 May 2021 04:55
 Operator : CG/JU
 Sample : M2493-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB429

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	17.116	2378	2385	2394	rBV	2851846	4184494	30.44%	4.762%
38	17.210	2394	2401	2416	rVV2	5232691	8007969	58.25%	9.113%
39	17.316	2416	2419	2423	rVB6	12282	18531	0.13%	0.021%
40	17.792	2496	2500	2502	rBV5	11376	13885	0.10%	0.016%
41	18.022	2534	2539	2544	rBV3	155049	239151	1.74%	0.272%
42	19.145	2724	2730	2736	rBV	88467	129325	0.94%	0.147%
43	19.310	2754	2758	2761	rBV6	24265	30721	0.22%	0.035%
44	19.339	2761	2763	2768	rVB6	14027	23380	0.17%	0.027%
45	19.398	2768	2773	2779	rBV3	78680	135397	0.98%	0.154%
46	19.463	2779	2784	2787	rBV7	8424	13988	0.10%	0.016%
47	19.516	2787	2793	2800	rBV	7072936	10440013	75.94%	11.880%
48	19.857	2849	2851	2856	rBV5	15894	21346	0.16%	0.024%
49	19.898	2856	2858	2861	rBV4	17285	21497	0.16%	0.024%
50	19.969	2868	2870	2875	rBV6	11045	14384	0.10%	0.016%
51	20.345	2931	2934	2941	rVB8	14562	28477	0.21%	0.032%
52	20.404	2941	2944	2949	rBV6	15813	23138	0.17%	0.026%
53	21.027	3046	3050	3061	rBV	572615	912461	6.64%	1.038%
54	21.310	3092	3098	3110	rBV	4618338	5959296	43.35%	6.781%
55	21.433	3116	3119	3122	rBV5	57101	65366	0.48%	0.074%
56	21.474	3124	3126	3130	rVB4	48550	44974	0.33%	0.051%
57	21.851	3188	3190	3191	rBV2	29212	28932	0.21%	0.033%
58	21.916	3199	3201	3204	rBV4	49356	63123	0.46%	0.072%
59	22.380	3277	3280	3288	rVB6	91662	126365	0.92%	0.144%
60	22.898	3364	3368	3373	rVB3	164830	225837	1.64%	0.257%
61	23.433	3450	3459	3474	rBV2	6556754	13747022	100.00%	15.643%
62	23.574	3475	3483	3494	rVB2	3390733	6698864	48.73%	7.623%
63	24.133	3572	3578	3585	rBV4	290761	600826	4.37%	0.684%
64	24.215	3588	3592	3598	rVB9	124378	225673	1.64%	0.257%
65	24.898	3701	3708	3713	rBV3	235336	514023	3.74%	0.585%
66	25.786	3854	3859	3865	rVB9	167437	383856	2.79%	0.437%
67	27.415	4134	4136	4137	rBV2	38143	26716	0.19%	0.030%


Sum of corrected areas: 87876928

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014757.D
Acq On : 26 May 2021 04:55
Operator : CG/JU
Sample : M2493-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB429

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

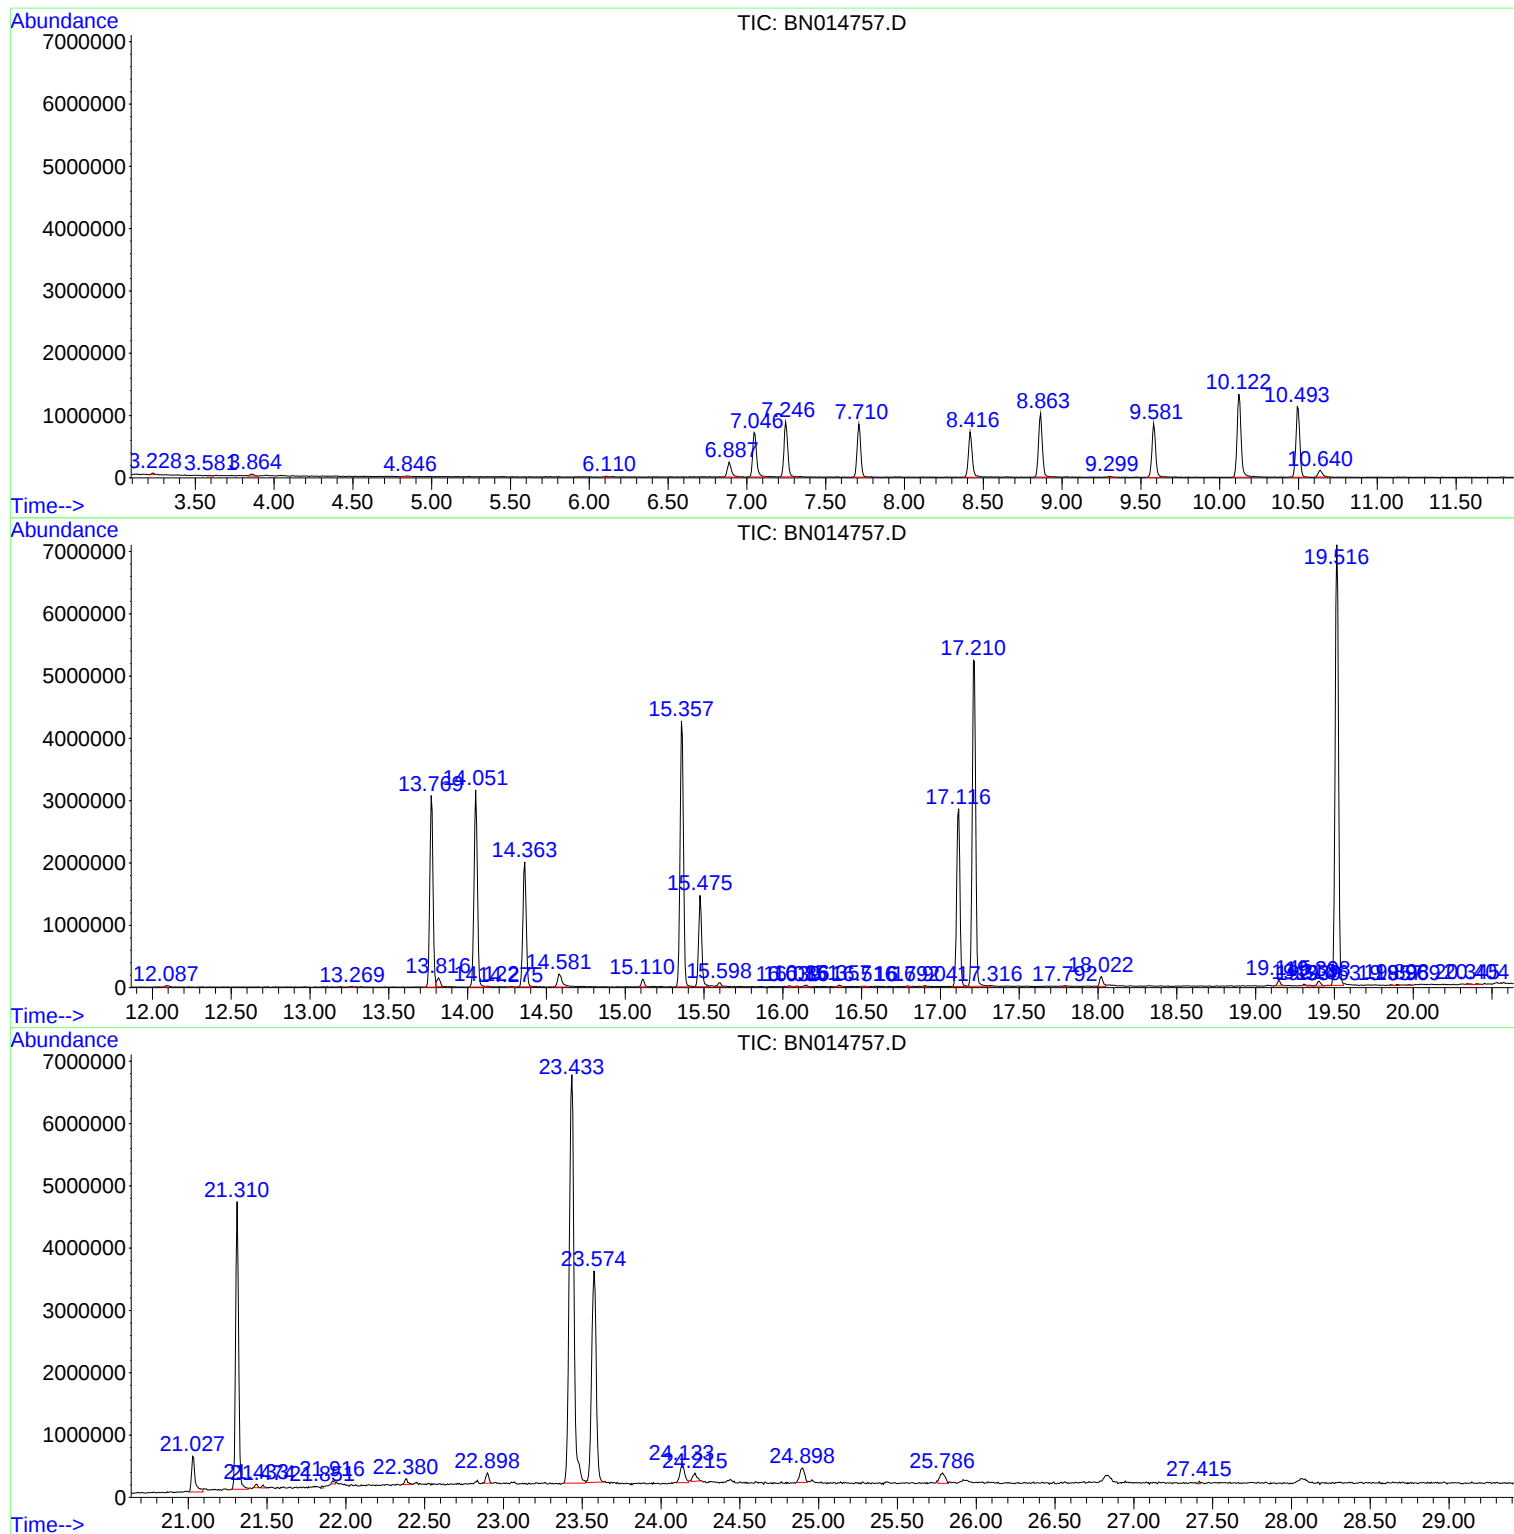

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014757.D
Acq On : 26 May 2021 04:55
Operator : CG/JU
Sample : M2493-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB429










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.03 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.030	3.06 ng/ul	912461	Chrysene-d12	21.310

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cycloeicosane	280	C20H40	000296-56-0	94
2			3-Eicosene, (E)-	280	C20H40	074685-33-9	91
3			4-Trifluoroacetoxyhexadecane	338	C18H33F3O2	1000215-97-5	91
4			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	91
5			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	91

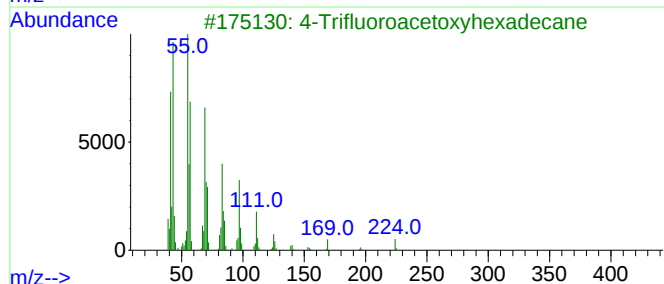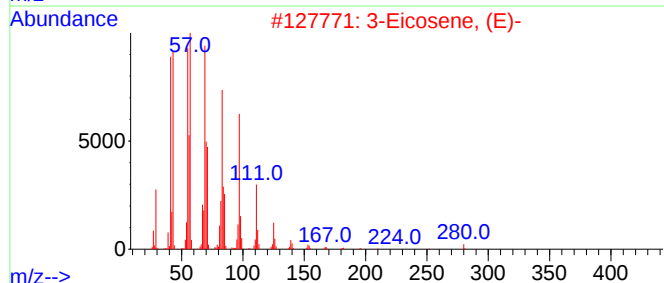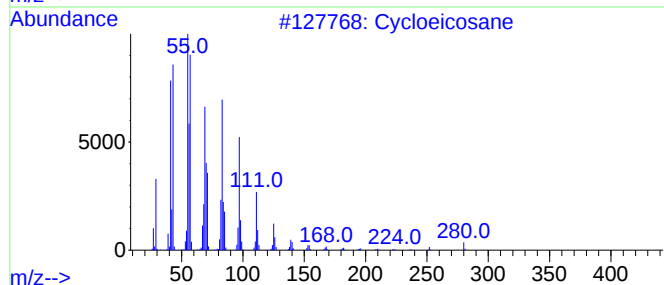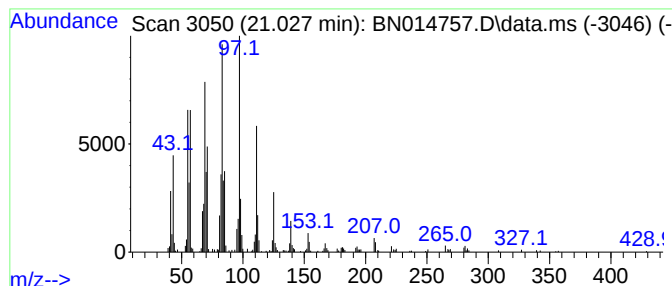

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014757.D
Acq On : 26 May 2021 04:55
Operator : CG/JU
Sample : M2493-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB429

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.030	3.1	ng/u1	912461	5	21.310	5959300	20.0