

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014764.D
 Acq On : 26 May 2021 09:19
 Operator : CG/JU
 Sample : PB136631BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK631

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	31	rVB5	26872	48506	0.53%	0.076%
2	3.340	41	43	46	rVB4	16307	12809	0.14%	0.020%
3	3.634	91	93	110	rBV	279088	638729	7.00%	0.999%
4	3.958	145	148	151	rVB5	9894	10746	0.12%	0.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014764.D
 Acq On : 26 May 2021 09:19
 Operator : CG/JU
 Sample : PB136631BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK631

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION


37	16.310	2244	2248	2256	rVB5	8926	21539	0.24%	0.034%
38	16.792	2326	2330	2331	rBV3	12673	9283	0.10%	0.015%
39	17.116	2379	2385	2395	rBV	2173370	3016421	33.03%	4.719%
40	17.216	2395	2402	2413	rVV	3638413	5153507	56.44%	8.062%
41	17.298	2413	2416	2421	rVB7	11538	14131	0.15%	0.022%
42	17.428	2433	2438	2442	rVB7	7568	13015	0.14%	0.020%
43	17.528	2452	2455	2458	rBV5	7317	9353	0.10%	0.015%
44	17.934	2518	2524	2528	rVV7	8037	12706	0.14%	0.020%
45	18.092	2548	2551						

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014764.D
Acq On : 26 May 2021 09:19
Operator : CG/JU
Sample : PB136631BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK631

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

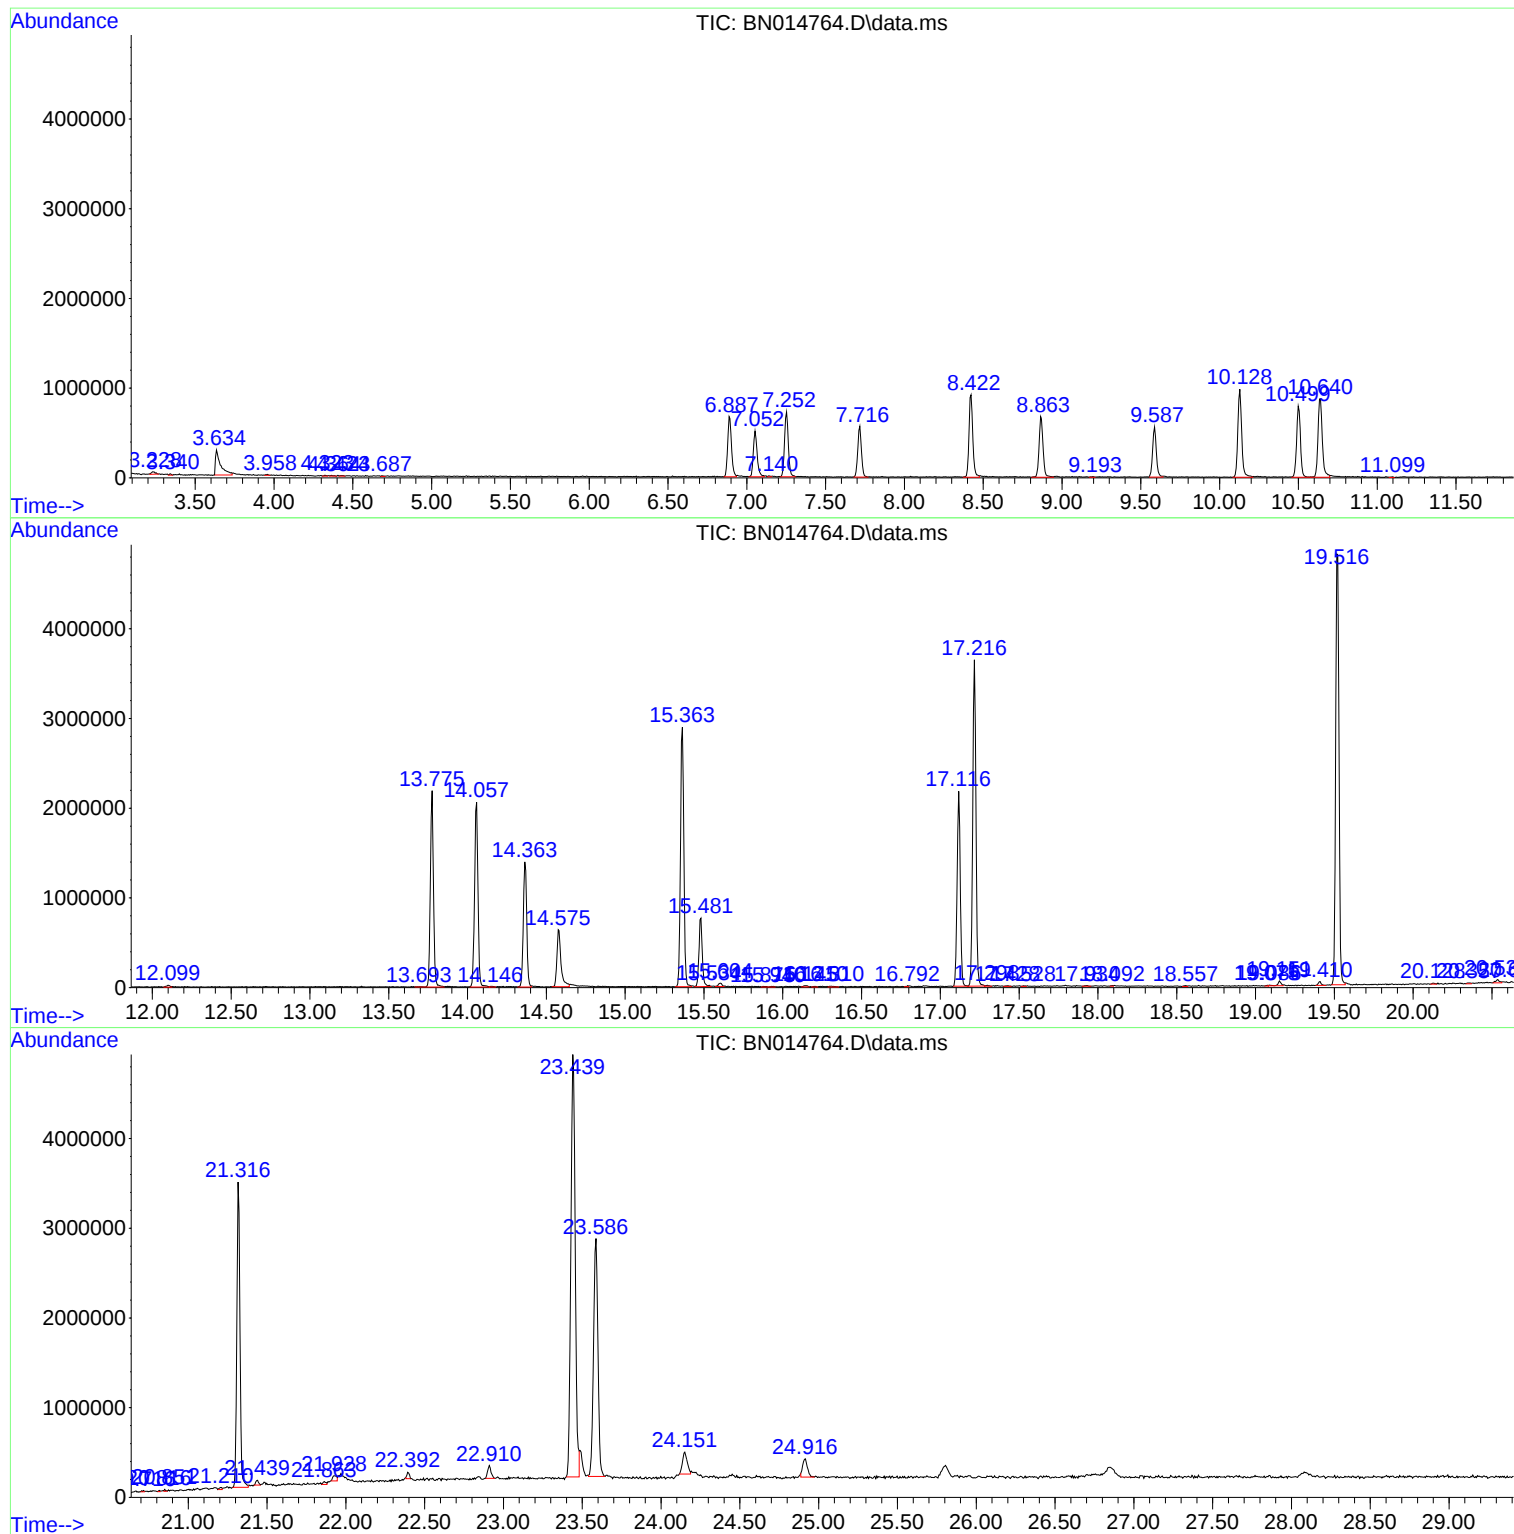

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014764.D
Acq On : 26 May 2021 09:19
Operator : CG/JU
Sample : PB136631BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK631

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014764.D
Acq On : 26 May 2021 09:19
Operator : CG/JU
Sample : PB136631BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK631

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc