

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014765.D
 Acq On : 26 May 2021 11:36
 Operator : CG/JU
 Sample : M2493-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

Signal : TIC: BN014765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	34	37	39	rVB4	8299	8469	0.11%	0.016%
2	4.270	198	201	203	rVV4	8386	7735	0.10%	0.015%
3	4.334	210	212	215	rVB4	9309	9566	0.12%	0.018%
4	4.381	218	220	224	rVB4	7585	8482	0.11%	0.016%
5	5.081	335	339	342	rBV4	7896	11808	0.15%	0.023%
6	5.640	427	434	435	rBV5	6408	8609	0.11%	0.017%
7	6.546	586	588	595	rVB6	7491	14061	0.18%	0.027%
8	6.769	623	626	632	rVB4	8149	10787	0.14%	0.021%
9	6.893	641	647	655	rBV	228323	397051	5.16%	0.765%
10	7.052	666	674	684	rBV	246872	452401	5.87%	0.872%
11	7.252	702	708	718	rBV	315786	538257	6.99%	1.037%
12	7.364	724	727	730	rVB4	8205	9336	0.12%	0.018%
13	7.717	779	787	795	rBV	797387	1340735	17.41%	2.583%
14	8.422	901	907	915	rBV2	356634	620490	8.06%	1.196%
15	8.769	964	966	970	rBV2	7355	8547	0.11%	0.016%
16	8.869	976	983	991	rBV	329630	578690	7.51%	1.115%
17	8.922	991	992	997	rVB5	8020	10946	0.14%	0.021%
18	8.958	997	998	1002	rBV3	6243	8097	0.11%	0.016%
19	9.587	1099	1105	1116	rVB2	261206	447862	5.82%	0.863%
20	9.946	1163	1166	1169	rBV4	5940	7988	0.10%	0.015%
21	10.128	1189	1197	1206	rBV2	466905	835956	10.85%	1.611%
22	10.499	1253	1260	1267	rBV	1080551	1891750	24.56%	3.645%
23	10.640	1277	1284	1299	rBV2	267464	534738	6.94%	1.030%
24	11.163	1370	1373	1377	rVB3	7058	10945	0.14%	0.021%
25	13.328	1740	1741	1746	rVB4	7447	10075	0.13%	0.019%
26	13.775	1810	1817	1823	rBV	1169274	1618344	21.01%	3.118%
27	13.816	1823	1824	1831	rVV3	37773	42928	0.56%	0.083%
28	14.057	1857	1865	1872	rVV	1111126	1660299	21.56%	3.199%
29	14.104	1872	1873	1878	rVV5	9799	14342	0.19%	0.028%
30	14.363	1909	1917	1928	rBV	2018626	3107441	40.35%	5.988%
31	14.587	1949	1955	1970	rBV2	129605	287627	3.73%	0.554%
32	15.110	2040	2044	2047	rVB5	9629	12313	0.16%	0.024%
33	15.363	2080	2087	2095	rBV	1682083	2445278	31.75%	4.712%
34	15.481	2100	2107	2115	rVV	241673	361797	4.70%	0.697%
35	15.598	2124	2127	2133	rVB5	21041	29184	0.38%	0.056%
36	15.869	2169	2173	2175	rVB4	8266	10597	0.14%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014765.D
 Acq On : 26 May 2021 11:36
 Operator : CG/JU
 Sample : M2493-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

37	16.045	2202	2203	2208	rVB5	6838	8556	0.11%	0.016%
38	16.151	2217	2221	2224	rVB5	8014	12302	0.16%	0.024%
39	16.628	2300	2302	2305	rVB3	12706	9928	0.13%	0.019%
40	16.681	2308	2311	2314	rVB4	8566	9628	0.13%	0.019%
41	16.904	2346	2349	2352	rBV2	12800	17371	0.23%	0.033%
42	17.116	2379	2385	2395	rBV	3041513	4414678	57.32%	8.506%
43	17.216	2395	2402	2412	rVV	2254806	3096764	40.21%	5.967%
44	17.310	2417	2418	2424	rVB5	10909	11578	0.15%	0.022%
45	17.698	2482	2484	2488	rBV5	12464	12149	0.16%	0.023%
46	17.798	2495	2501	2506	rVB8	8219	19022	0.25%	0.037%
47	17.922	2517	2522	2524	rBV5	5523	8600	0.11%	0.017%
48	18.022	2535	2539	2540	rBV3	8566	9569	0.12%	0.018%
49	18.034	2540	2541	2545	rVV3	13150	11768	0.15%	0.023%
50	18.157	2561	2562	2567	rBV5	9214	11090	0.14%	0.021%
51	18.322	2588	2590	2595	rVB5	8111	12194	0.16%	0.023%
52	18.492	2615	2619	2622	rBV5	9045	11755	0.15%	0.023%
53	18.528	2622	2625	2627	rVV3	5468	7720	0.10%	0.015%
54	18.563	2627	2631	2634	rVB6	12632	19701	0.26%	0.038%
55	18.604	2634	2638	2640	rBV3	5899	9007	0.12%	0.017%
56	18.657	2640	2647	2650	rBV8	8498	15701	0.20%	0.030%
57	18.828	2673	2676	2678	rVB4	7684	9602	0.12%	0.019%
58	19.057	2712	2715	2717	rBV4	8609	10840	0.14%	0.021%
59	19.081	2717	2719	2721	rBV3	10736	12341	0.16%	0.024%
60	19.151	2729	2731	2736	rBV6	10720	16292	0.21%	0.031%
61	19.404	2769	2774	2780	rVB4	25732	39450	0.51%	0.076%
62	19.457	2780	2783	2787	rBV5	12502	15361	0.20%	0.030%
63	19.522	2787	2794	2804	rBV	2956091	4242089	55.08%	8.174%
64	19.916	2860	2861	2864	rBV3	10790	8490	0.11%	0.016%
65	20.157	2899	2902	2903	rBV3	12546	13824	0.18%	0.027%
66	20.239	2914	2916	2918	rBV3	15377	17079	0.22%	0.033%
67	20.328	2929	2931	2934	rBV4	11738	7851	0.10%	0.015%
68	20.375	2936	2939	2940	rVB3	13133	9804	0.13%	0.019%
69	20.539	2962	2967	2970	rBV4	65105	82637	1.07%	0.159%
70	20.722	2997	2998	3001	rBV3	18105	13576	0.18%	0.026%
71	20.957	3034	3038	3042	rBV6	20911	31589	0.41%	0.061%
72	21.045	3049	3053	3057	rBV6	47886	79548	1.03%	0.153%
73	21.239	3084	3086	3088	rBV3	19950	20356	0.26%	0.039%
74	21.263	3088	3090	3092	rBV3	17247	12159	0.16%	0.023%
75	21.322	3094	3100	3109	rBV	5197145	6629512	86.08%	12.774%
76	21.439	3116	3120	3124	rBV4	99961	155160	2.01%	0.299%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
 Data File : BN014765.D
 Acq On : 26 May 2021 11:36
 Operator : CG/JU
 Sample : M2493-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GB426

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Title : SVOA CALIBRATION

77	21.486	3126	3128	3133	rVB6	37409	54341	0.71%	0.105%
78	22.398	3280	3283	3292	rVB8	116810	152307	1.98%	0.293%
79	22.910	3367	3370	3375	rBV5	149675	206609	2.68%	0.398%
80	23.445	3453	3461	3467	rBV	2927646	5688221	73.86%	10.960%
81	23.592	3478	3486	3495	rBV2	3908867	7701716	100.00%	14.840%
82	24.157	3576	3582	3589	rBV2	289169	532424	6.91%	1.026%
83	24.916	3705	3711	3721	rVB6	260331	586746	7.62%	1.131%
84	25.810	3857	3863	3873	rVB9	177319	446164	5.79%	0.860%




Sum of corrected areas: 51898700

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014765.D
Acq On : 26 May 2021 11:36
Operator : CG/JU
Sample : M2493-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

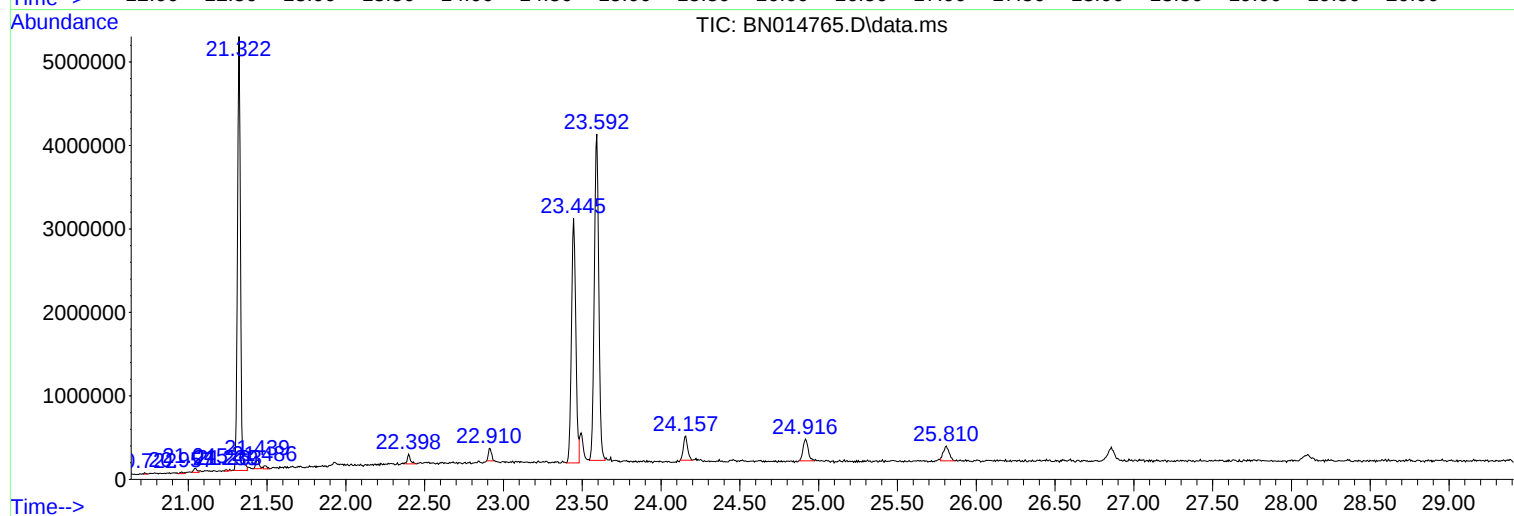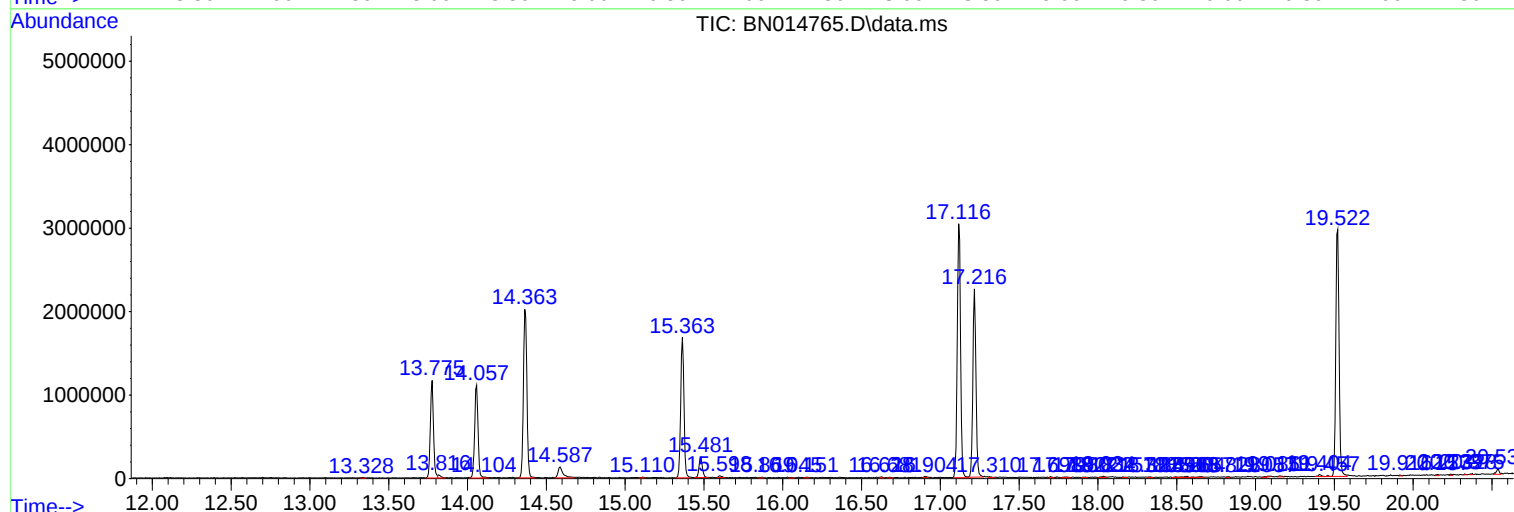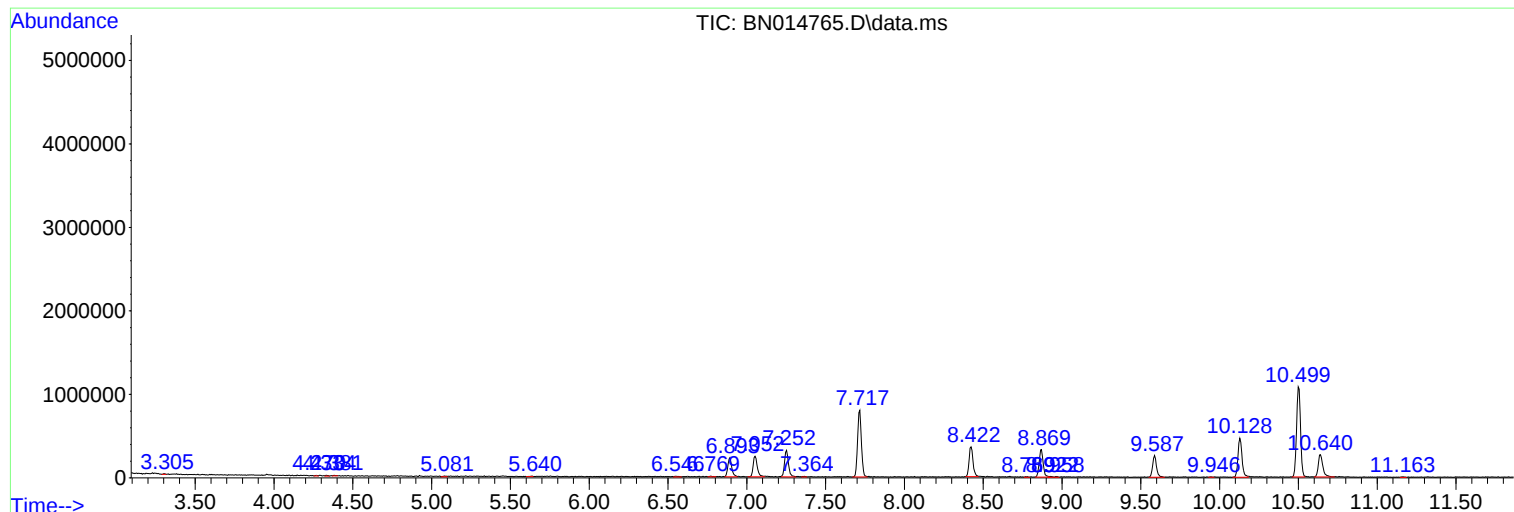

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014765.D
Acq On : 26 May 2021 11:36
Operator : CG/JU
Sample : M2493-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052521\
Data File : BN014765.D
Acq On : 26 May 2021 11:36
Operator : CG/JU
Sample : M2493-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GB426

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
