

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025659.D
 Acq On : 28 May 2023 00:10
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: May 29 00:55:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 29 00:47:45 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.019	152	6251	0.400	ng	0.00
7) Naphthalene-d8	10.835	136	18138	0.400	ng	# 0.00
13) Acenaphthene-d10	14.651	164	10773	0.400	ng	0.00
19) Phenanthrene-d10	17.393	188	23238	0.400	ng	# 0.00
29) Chrysene-d12	21.578	240	15484	0.400	ng	# 0.00
35) Perylene-d12	24.054	264	13446	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.557	112	6589	0.411	ng	0.00
5) Phenol-d6	7.174	99	7884	0.411	ng	0.00
8) Nitrobenzene-d5	9.191	82	5859	0.386	ng	0.00
11) 2-Methylnaphthalene-d10	12.423	152	10866	0.420	ng	0.00
14) 2,4,6-Tribromophenol	16.152	330	1145	0.526	ng	0.00
15) 2-Fluorobiphenyl	13.283	172	17751	0.399	ng	0.00
27) Fluoranthene-d10	19.421	212	21637	0.411	ng	0.00
31) Terphenyl-d14	20.015	244	13761	0.406	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.397	88	3041	0.420	ng	99
3) n-Nitrosodimethylamine	3.744	42	2729	0.350	ng	# 87
6) bis(2-Chloroethyl)ether	7.434	93	7809	0.395	ng	94
9) Naphthalene	10.889	128	20703	0.417	ng	98
10) Hexachlorobutadiene	11.177	225	3560	0.414	ng	# 96
12) 2-Methylnaphthalene	12.495	142	14247	0.417	ng	99
16) Acenaphthylene	14.373	152	20046	0.394	ng	100
17) Acenaphthene	14.715	154	13739	0.410	ng	99
18) Fluorene	15.693	166	18389	0.415	ng	99
20) 4,6-Dinitro-2-methylph...	15.780	198	1230	0.494	ng	# 55
21) 4-Bromophenyl-phenylether	16.586	248	5267	0.399	ng	# 88
22) Hexachlorobenzene	16.698	284	4825	0.400	ng	99
23) Atrazine	16.847	200	4196	0.399	ng	95
24) Pentachlorophenol	17.070	266	876	0.848	ng	# 86
25) Phenanthrene	17.430	178	29111	0.412	ng	99
26) Anthracene	17.530	178	25780	0.403	ng	99
28) Fluoranthene	19.453	202	31640	0.410	ng	99
30) Pyrene	19.816	202	32041	0.425	ng	99
32) Benzo(a)anthracene	21.560	228	23248	0.403	ng	99
33) Chrysene	21.614	228	26576	0.425	ng	99
34) Bis(2-ethylhexyl)phtha...	21.471	149	15230	0.434	ng	# 98
36) Indeno(1,2,3-cd)pyrene	26.647	276	20895	0.405	ng	# 64
37) Benzo(b)fluoranthene	23.297	252	22148	0.433	ng	94
38) Benzo(k)fluoranthene	23.344	252	22118	0.415	ng	95
39) Benzo(a)pyrene	23.946	252	20256	0.414	ng	94
40) Dibenzo(a,h)anthracene	26.668	278	16417	0.402	ng	95
41) Benzo(g,h,i)perylene	27.437	276	18665	0.400	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025659.D
Acq On : 28 May 2023 00:10
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: May 29 00:55:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 00:47:45 2023
Response via : Initial Calibration

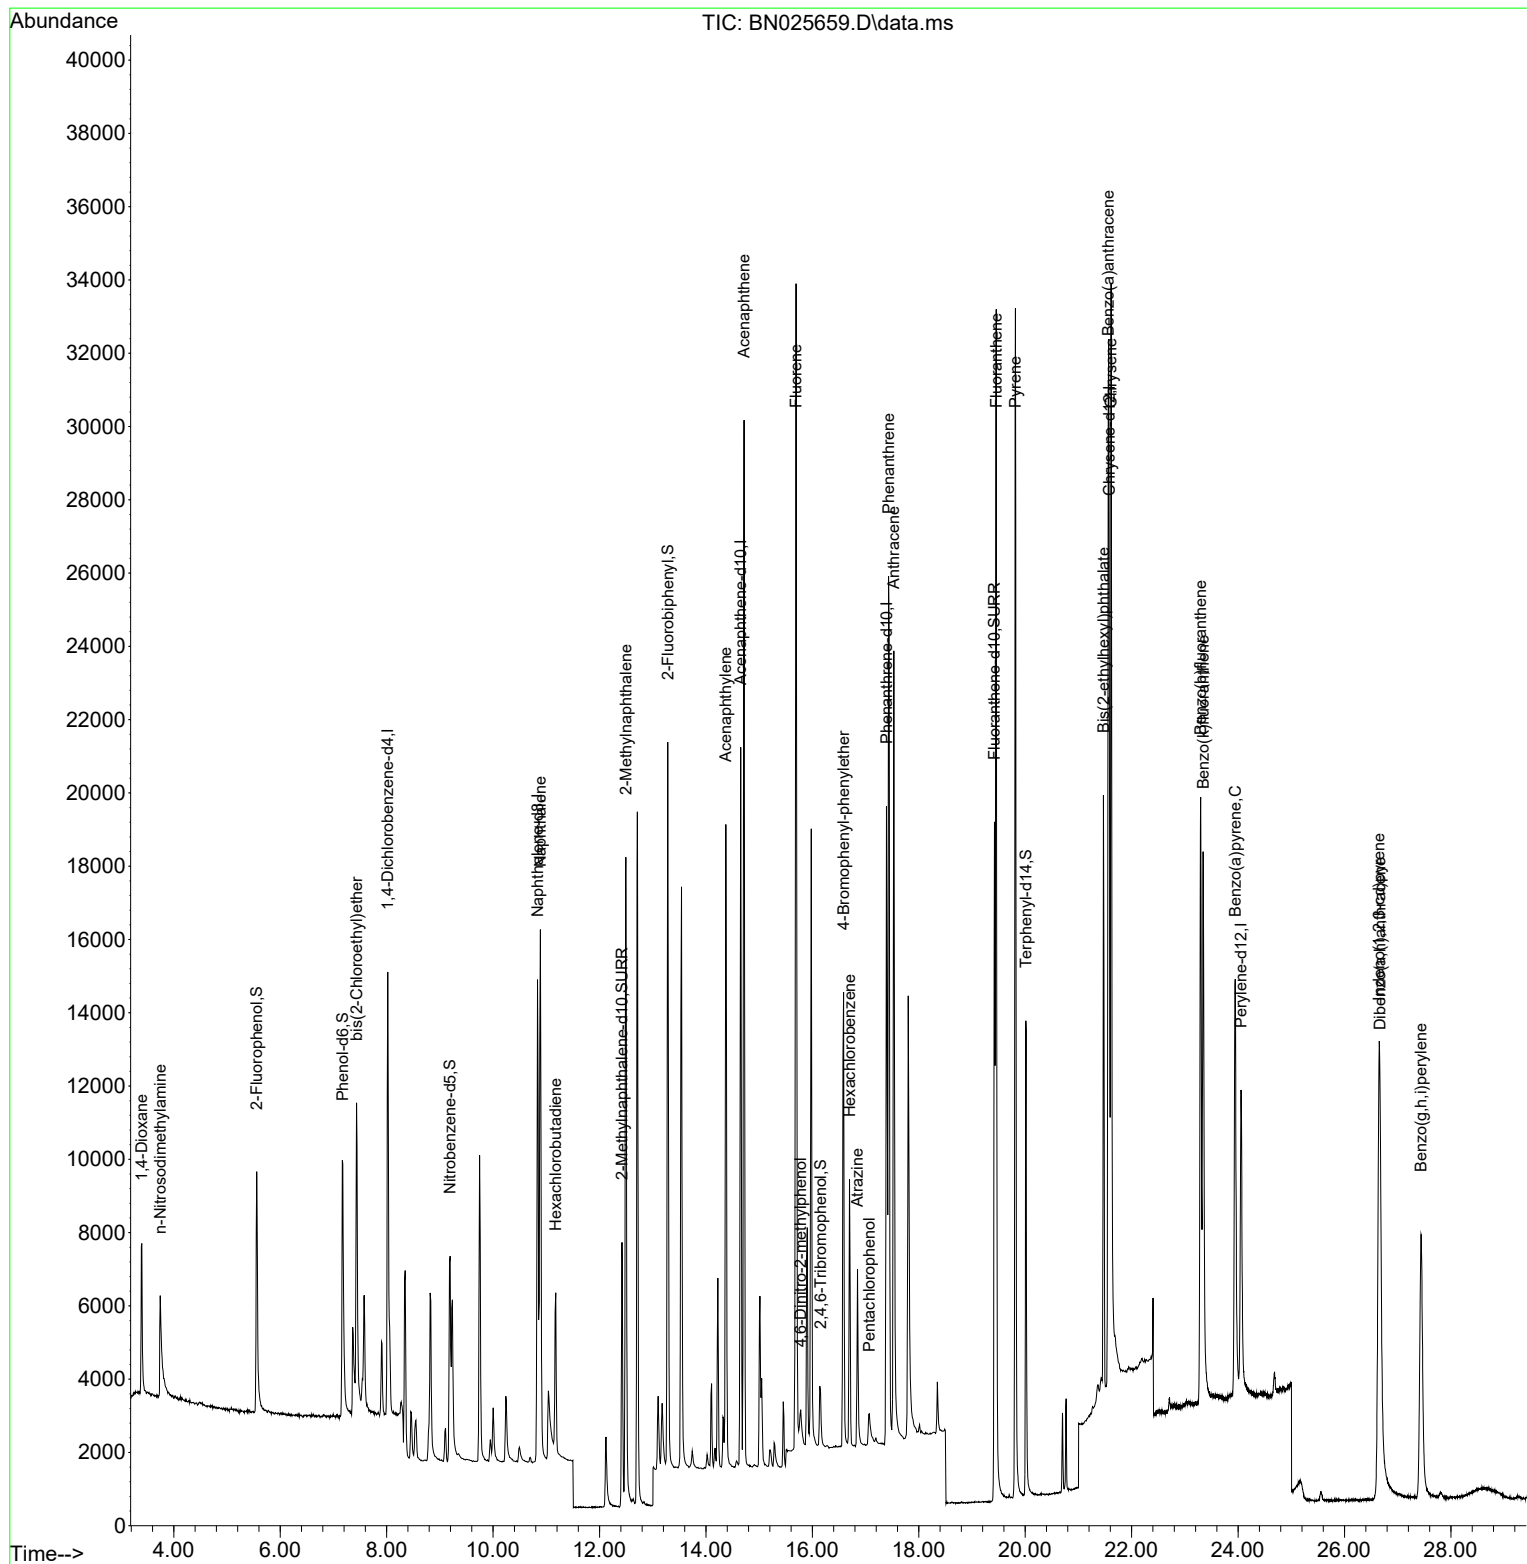





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.019 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



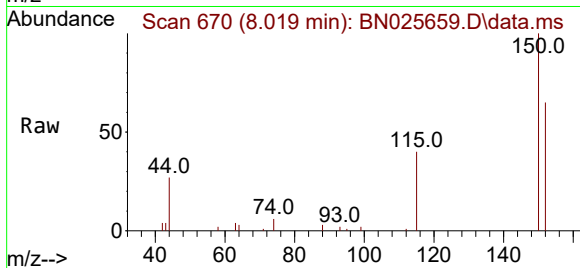



Tgt Ion:152 Resp: 6251
Ion Ratio Lower Upper
152 100
150 155.0 121.0 181.6
115 62.2 48.5 72.7

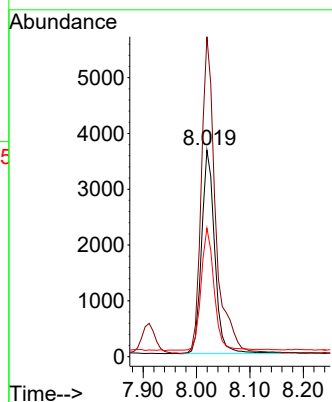

#2
1,4-Dioxane
Concen: 0.420 ng
RT: 3.397 min Scan# 30
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion: 88 Resp: 3041
Ion Ratio Lower Upper
88 100
43 31.9 26.5 39.7
58 71.6 56.8 85.2


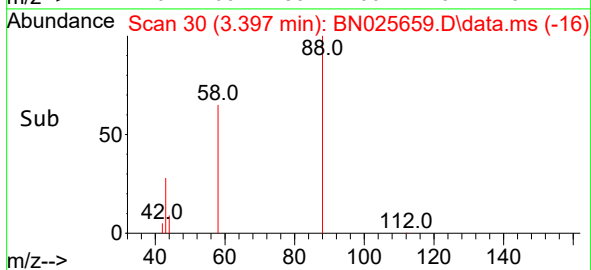
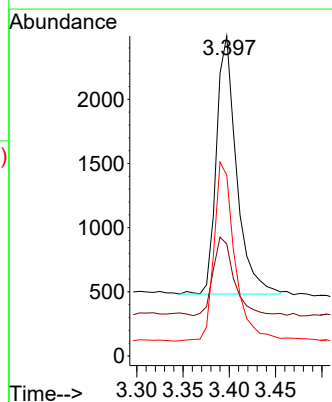
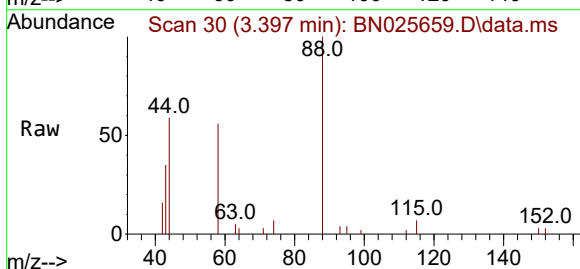


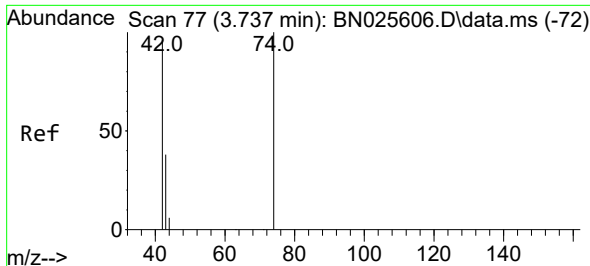

#3
n-Nitrosodimethylamine
Concen: 0.350 ng
RT: 3.744 min Scan# 71
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 2729
Ion Ratio Lower Upper
42 100
74 115.6 82.2 123.2
44 11.0 0.0 0.0#

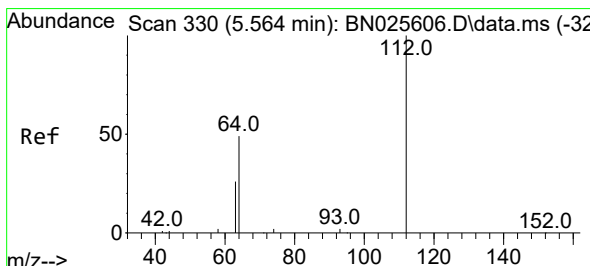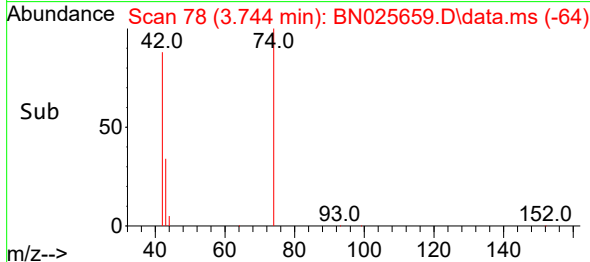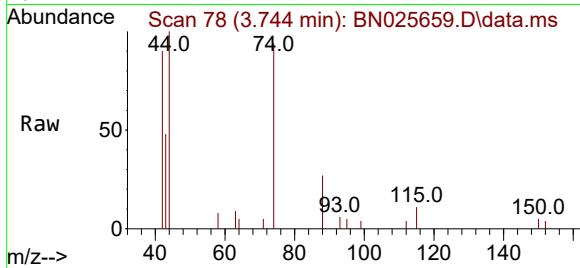

#4
2-Fluorophenol
Concen: 0.411 ng
RT: 5.557 min Scan# 329
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion: 112 Resp: 6589
Ion Ratio Lower Upper
112 100
64 58.6 45.7 68.5
63 32.1 26.2 39.2


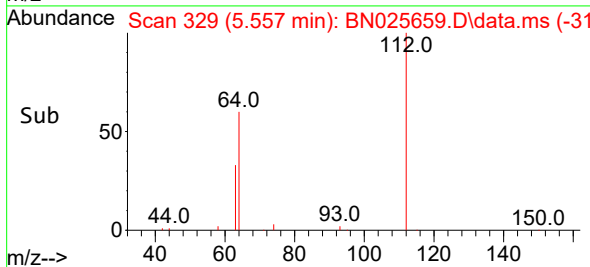

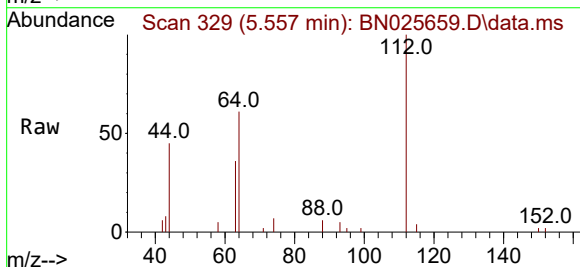




#5
Phenol-d6
Concen: 0.411 ng
RT: 7.174 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 7884
Ion Ratio Lower Upper
99 100
42 22.2 17.1 25.7
71 37.2 29.3 43.9



#6
bis(2-Chloroethyl)ether
Concen: 0.395 ng
RT: 7.434 min Scan# 589
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion: 93 Resp: 7809
Ion Ratio Lower Upper
93 100
63 66.9 49.1 73.7
95 29.6 22.6 33.8


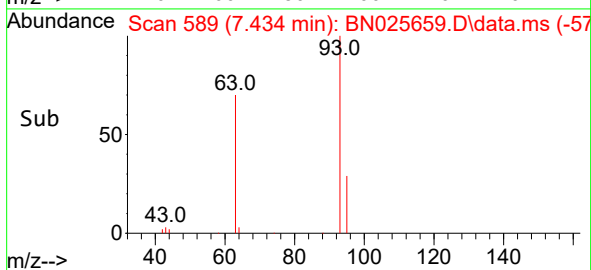






#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.835 min Scan# 948
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	18138
Ion Ratio	Lower	Upper	
136	100		
137	11.3	9.1	13.7
54	9.4	5.4	8.0#
68	7.1	4.3	6.5#

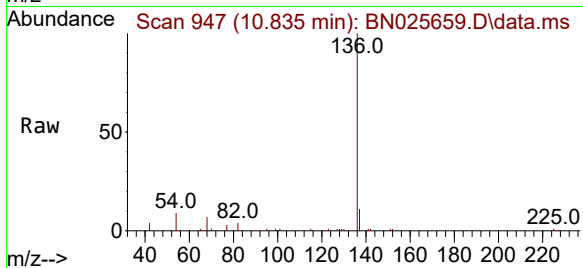

#8
Nitrobenzene-d5
Concen: 0.386 ng
RT: 9.191 min Scan# 793
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion:	82	Resp:	5859
Ion Ratio	Lower	Upper	
82	100		
128	44.0	32.5	48.7
54	48.8	40.6	60.8

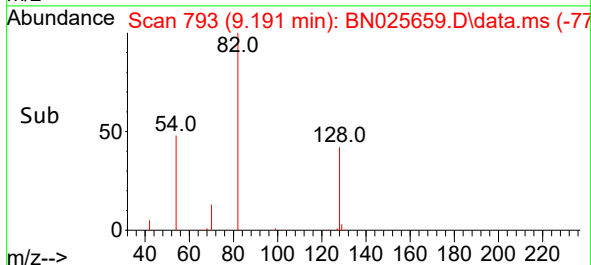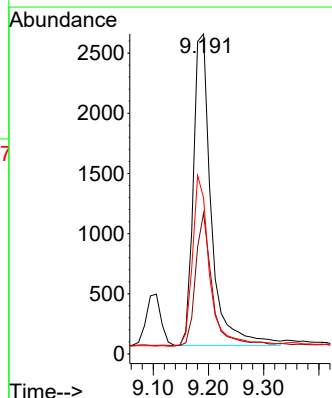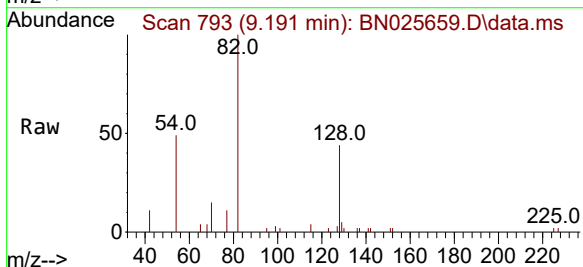



#9

Naphthalene

Concen: 0.417 ng

RT: 10.889 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:128 Resp: 20703

Ion Ratio Lower Upper

128 100

129 11.1 9.3 13.9

127 13.0 11.0 16.6

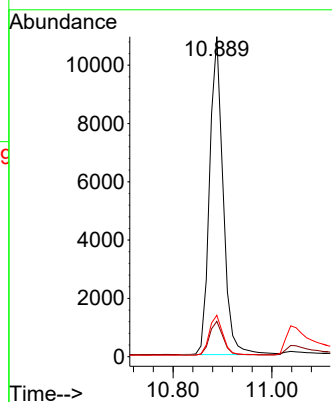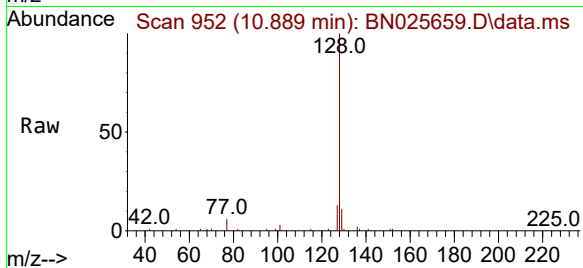

#10

Hexachlorobutadiene

Concen: 0.414 ng

RT: 11.177 min Scan# 979

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:225 Resp: 3560

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.3 48.4 72.6

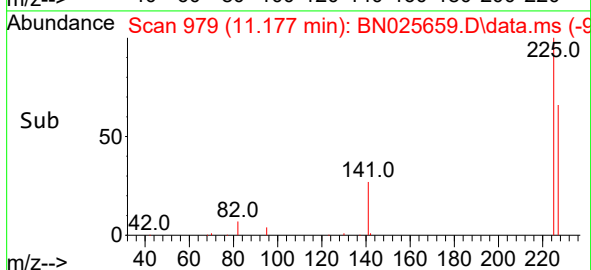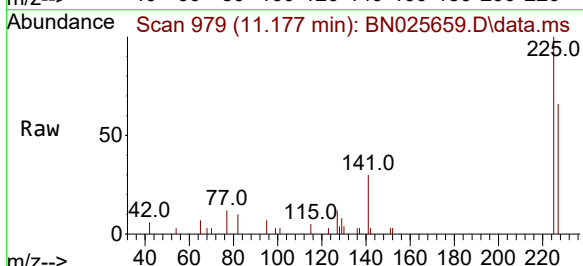



#11

2-Methylnaphthalene-d10

Concen: 0.420 ng

RT: 12.423 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :





SSTDCCC0.4EC

Tgt Ion:152 Resp: 10866

Ion Ratio Lower Upper

152 100

151 20.3 16.1 24.1

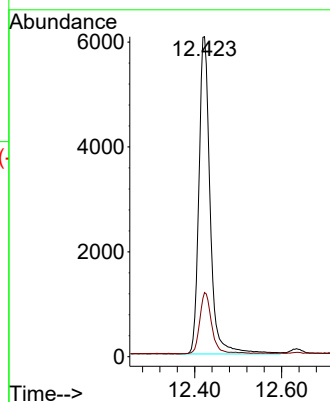

#12

2-Methylnaphthalene

Concen: 0.417 ng

RT: 12.495 min Scan# 1271

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:142 Resp: 14247


Ion Ratio Lower Upper

142 100

141 88.3 70.7 106.1

115 40.3 31.5 47.3

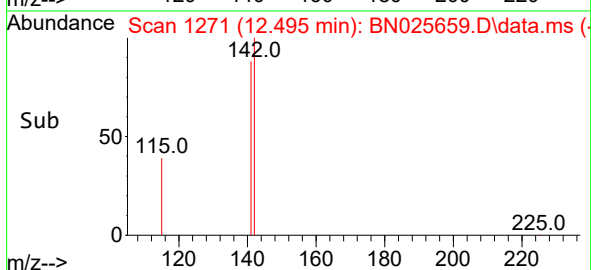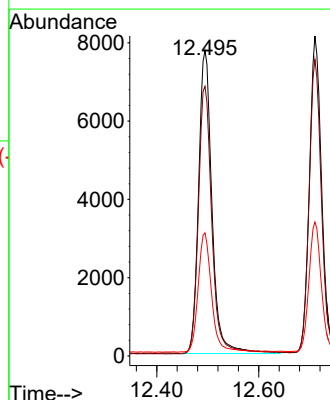

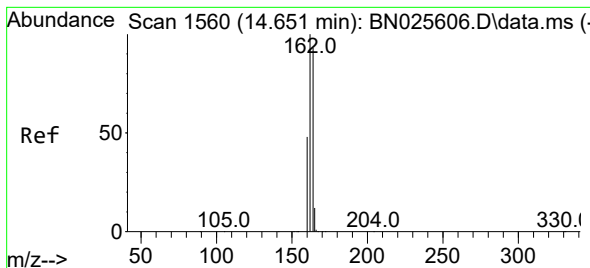

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.651 min Scan# 1560

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:164 Resp: 10773

Ion Ratio Lower Upper

164 100

162 106.8 86.4 129.6

160 50.3 41.9 62.9

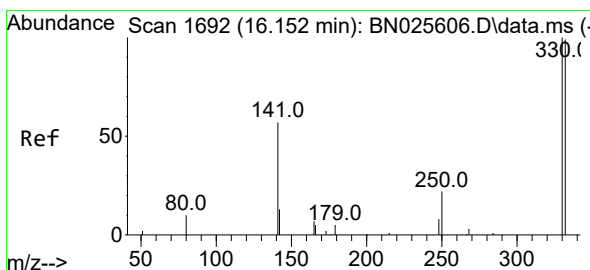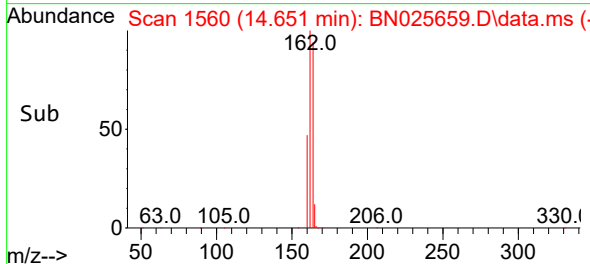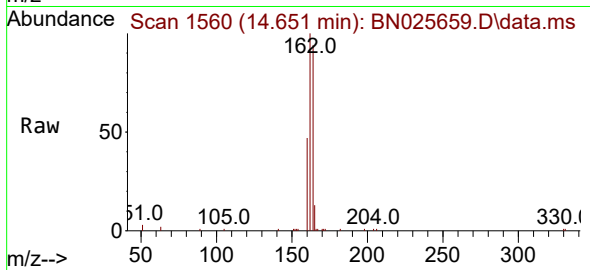

#14

2,4,6-Tribromophenol

Concen: 0.526 ng

RT: 16.152 min Scan# 1692

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:330 Resp: 1145


Ion Ratio Lower Upper

330 100

332 96.2 80.0 120.0

141 57.8 45.8 68.6


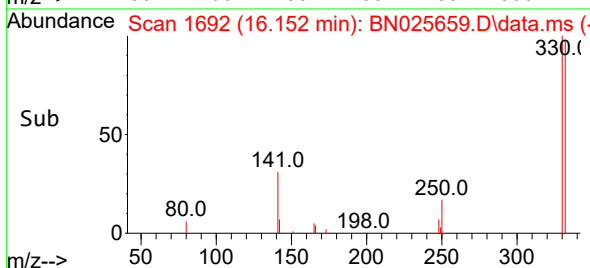

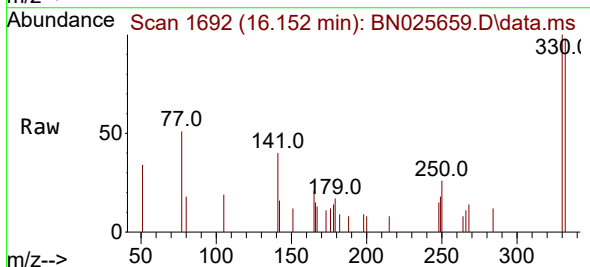


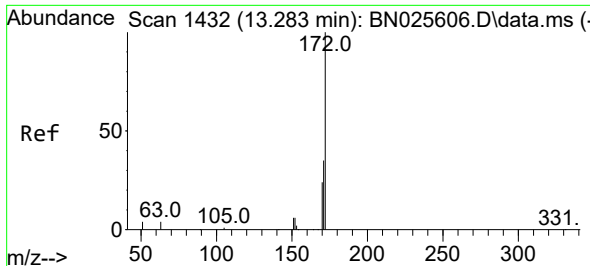

#15
2-Fluorobiphenyl
Concen: 0.399 ng
RT: 13.283 min Scan# 1432
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 17751
Ion Ratio Lower Upper
172 100
171 34.8 28.6 42.8
170 23.5 19.7 29.5

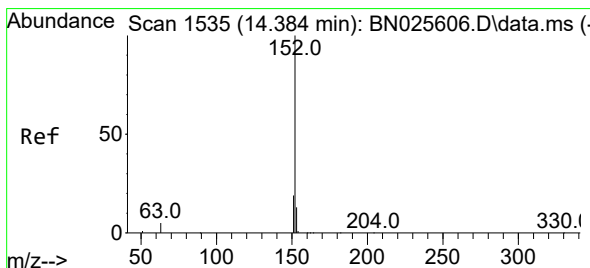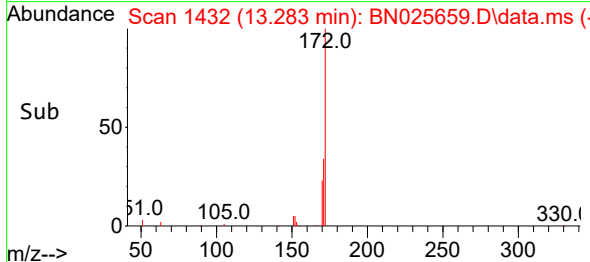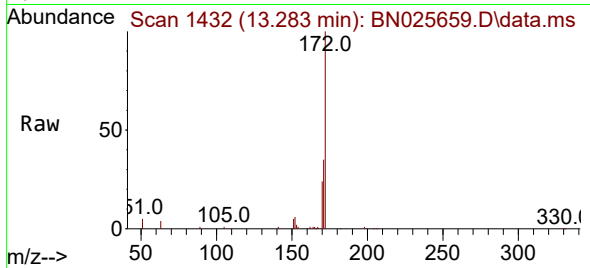

#16
Acenaphthylene
Concen: 0.394 ng
RT: 14.373 min Scan# 1534
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion:152 Resp: 20046
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.6
153 13.0 10.6 15.8

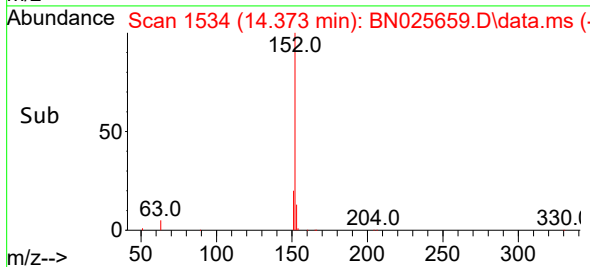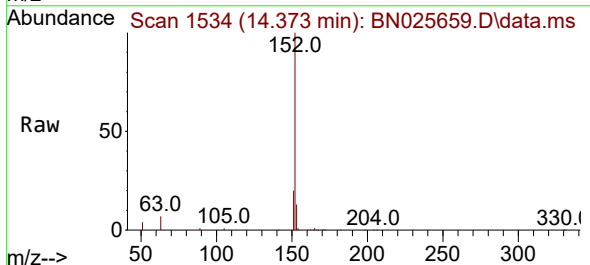



#17

Acenaphthene

Concen: 0.410 ng

RT: 14.715 min Scan# 1566

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:154 Resp: 13739

Ion Ratio Lower Upper

154 100

153 116.2 91.9 137.9

152 57.0 45.4 68.2

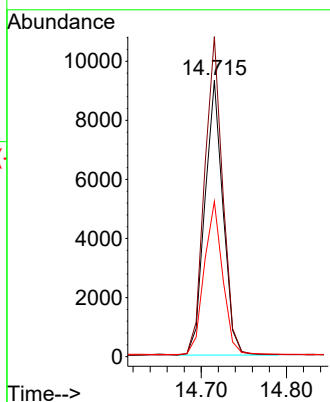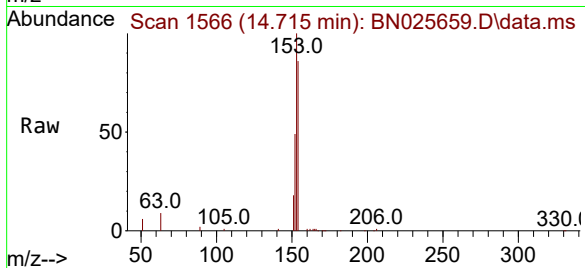

#18

Fluorene

Concen: 0.415 ng

RT: 15.693 min Scan# 1655

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:166 Resp: 18389


Ion Ratio Lower Upper

166 100

165 98.2 79.3 118.9

167 13.4 10.7 16.1

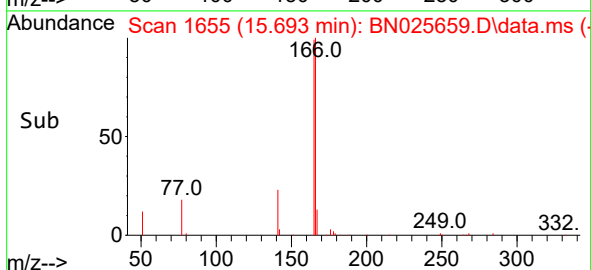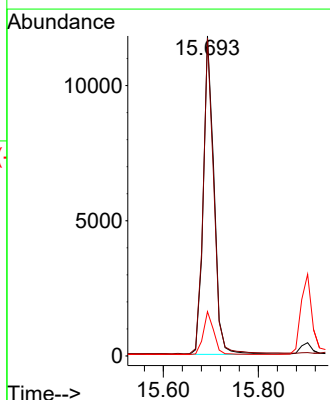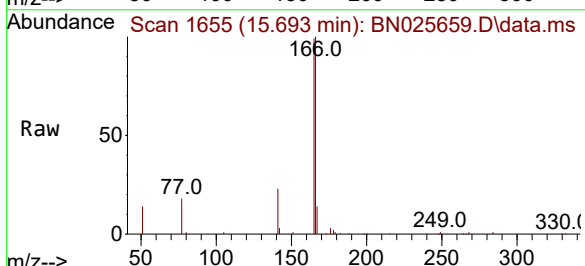



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.393 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:188 Resp: 23238

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 11.8 12.2 18.2#

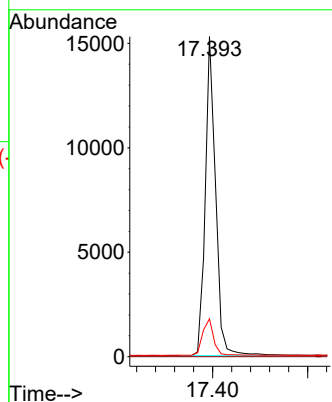

#20

4,6-Dinitro-2-methylphenol

Concen: 0.494 ng

RT: 15.780 min Scan# 1662

Delta R.T. -0.013 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:198 Resp: 1230


Ion Ratio Lower Upper

198 100

51 70.4 110.8 166.2#

105 56.0 61.9 92.9#


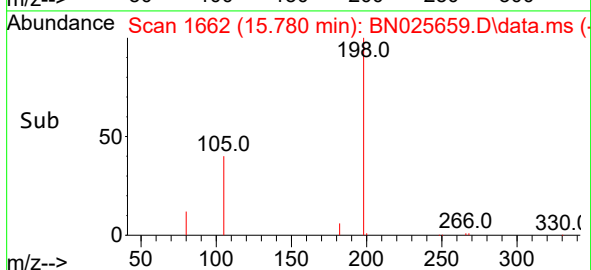






#21
4-Bromophenyl-phenylether
Concen: 0.399 ng
RT: 16.586 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 5267
Ion Ratio Lower Upper
248 100
250 99.6 77.5 116.3
141 59.9 64.0 96.0#

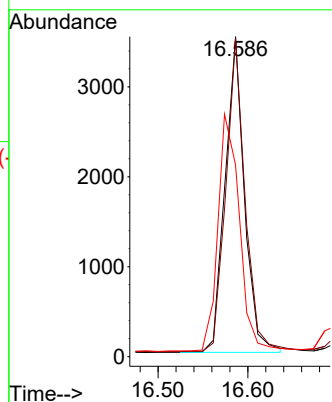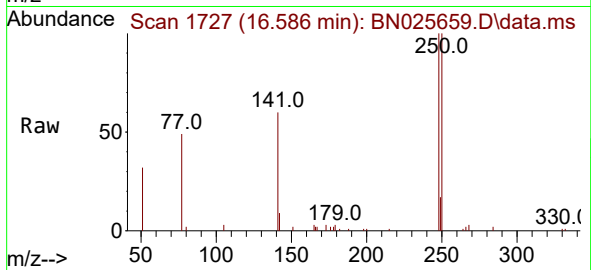

#22
Hexachlorobenzene
Concen: 0.400 ng
RT: 16.698 min Scan# 1736
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion:284 Resp: 4825
Ion Ratio Lower Upper
284 100
142 53.6 42.0 63.0
249 35.4 28.6 43.0


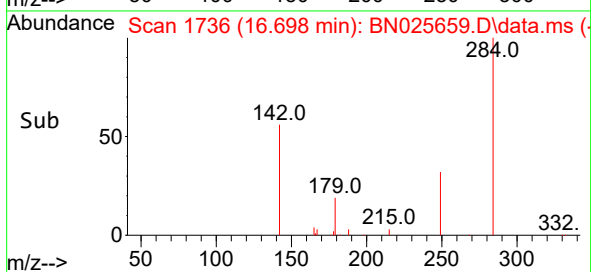






#23
 Atrazine
 Concen: 0.399 ng
 RT: 16.847 min Scan# 1766
 Delta R.T. -0.000 min
 Lab File: BN025659.D
 Acq: 28 May 2023 00:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:200 Resp: 4196
 Ion Ratio Lower Upper
 200 100
 173 28.8 27.9 41.9
 215 44.3 35.1 52.7



#24
 Pentachlorophenol
 Concen: 0.848 ng
 RT: 17.070 min Scan# 1766
 Delta R.T. -0.000 min
 Lab File: BN025659.D
 Acq: 28 May 2023 00:10

Tgt Ion:266 Resp: 876
 Ion Ratio Lower Upper
 266 100
 264 63.2 60.0 90.0
 268 69.6 0.0 0.0#

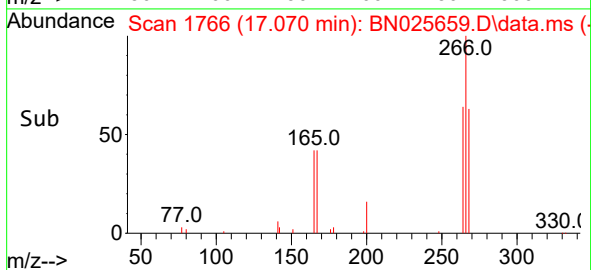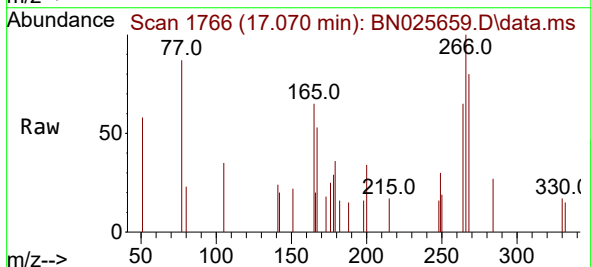



#25

Phenanthrene

Concen: 0.412 ng

RT: 17.430 min Scan# 1796

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:178 Resp: 29111

Ion Ratio Lower Upper

178 100

176 19.4 15.4 23.2

179 15.3 12.6 19.0



#26

Anthracene

Concen: 0.403 ng

RT: 17.530 min Scan# 1803

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:178 Resp: 25780


Ion Ratio Lower Upper

178 100

176 18.6 14.8 22.2

179 14.9 12.2 18.2


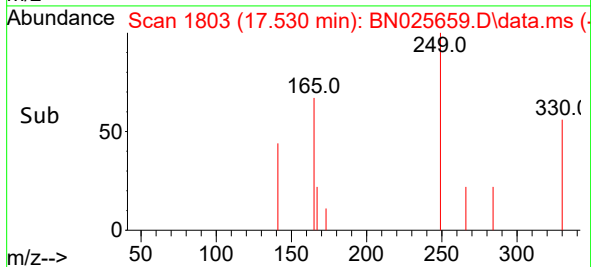

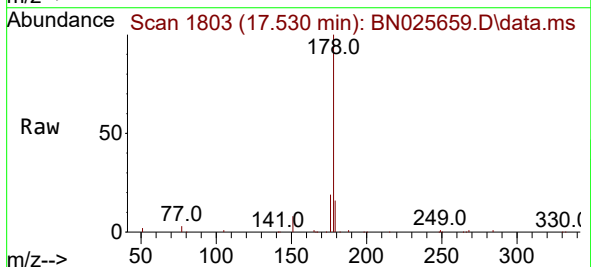




#27
Fluoranthene-d10
Concen: 0.411 ng
RT: 19.421 min Scan# 2078
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 21637
Ion Ratio Lower Upper
212 100
106 15.5 12.3 18.5
104 9.2 7.2 10.8

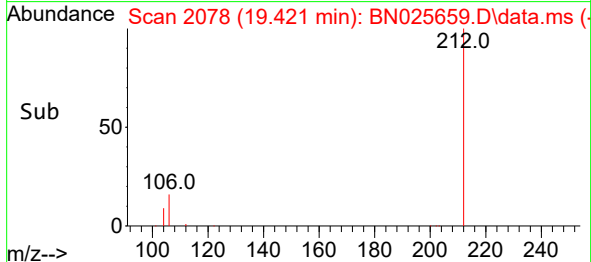

#28
Fluoranthene
Concen: 0.410 ng
RT: 19.453 min Scan# 2085
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion:202 Resp: 31640
Ion Ratio Lower Upper
202 100
101 11.3 9.2 13.8
203 16.9 13.3 19.9

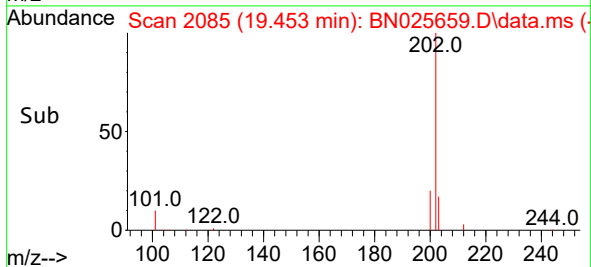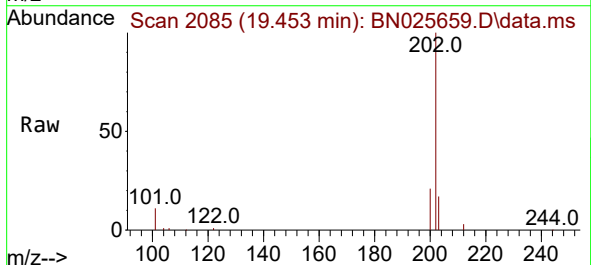

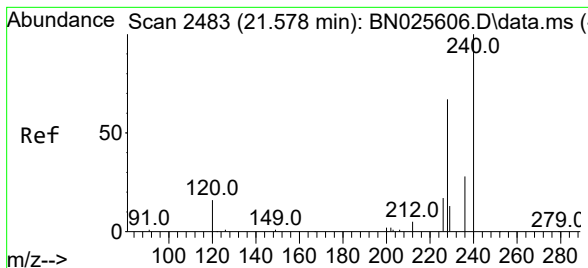

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.578 min Scan# 2483

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:240 Resp: 15484

Ion Ratio Lower Upper

240 100

120 15.2 15.4 23.0#

236 29.2 23.2 34.8

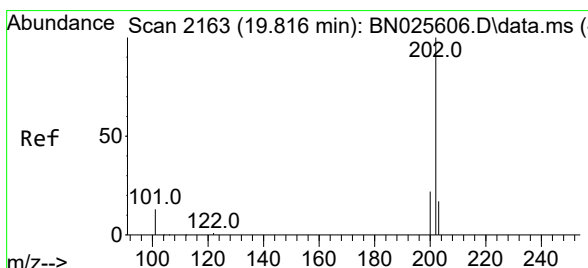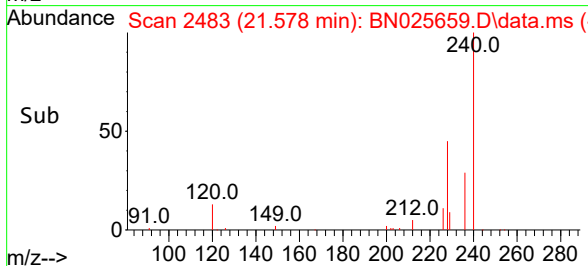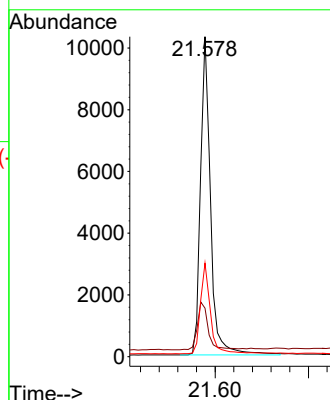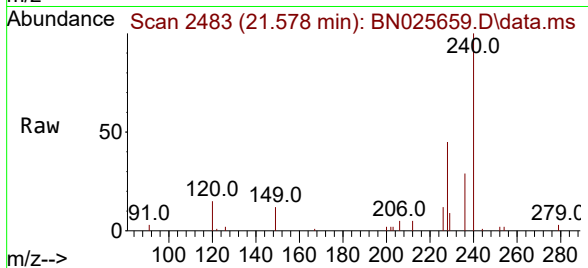

#30

Pyrene

Concen: 0.425 ng

RT: 19.816 min Scan# 2163

Delta R.T. -0.000 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:202 Resp: 32041


Ion Ratio Lower Upper

202 100

200 21.0 17.1 25.7

203 17.6 14.5 21.7


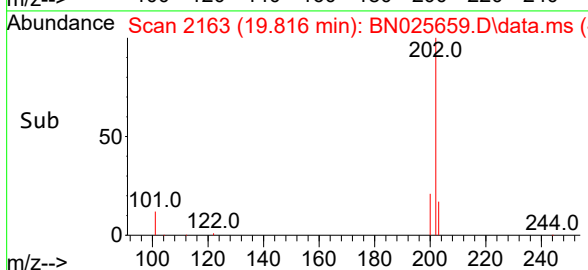
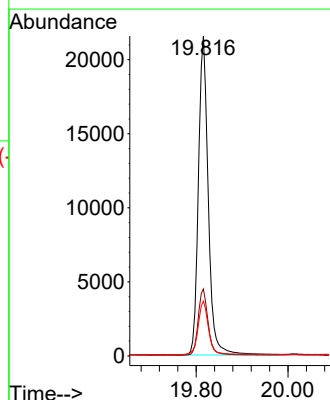
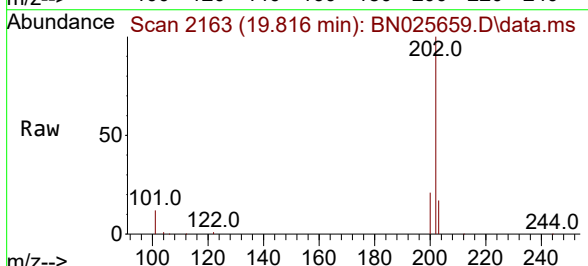




#31
 Terphenyl-d14
 Concen: 0.406 ng
 RT: 20.015 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN025659.D
 Acq: 28 May 2023 00:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:244 Resp: 13761
 Ion Ratio Lower Upper
 244 100
 212 9.9 8.5 12.7
 122 16.1 14.9 22.3

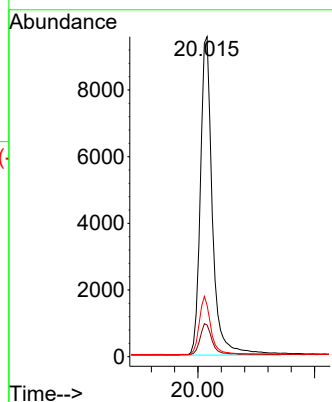

#32
 Benzo(a)anthracene
 Concen: 0.403 ng
 RT: 21.560 min Scan# 2481
 Delta R.T. -0.000 min
 Lab File: BN025659.D
 Acq: 28 May 2023 00:10

Tgt Ion:228 Resp: 23248
 Ion Ratio Lower Upper
 228 100
 226 28.2 22.9 34.3
 229 19.6 15.9 23.9


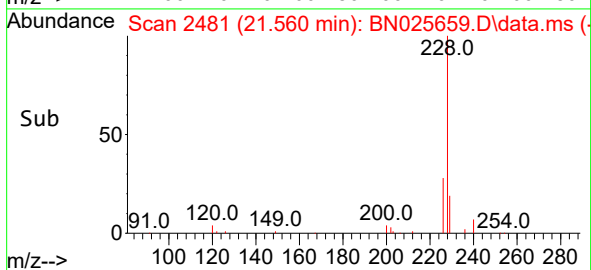
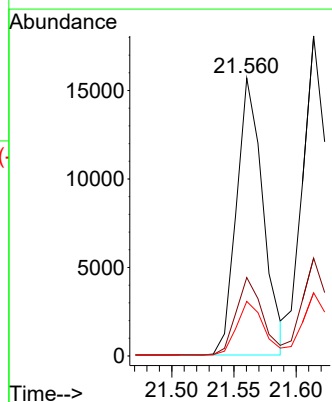



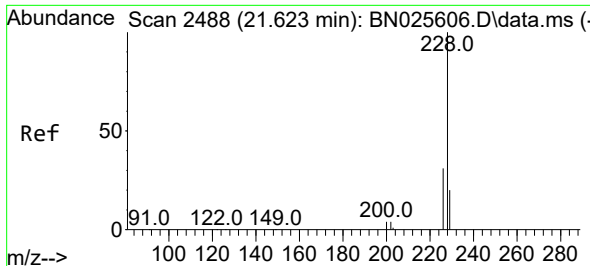

#33
Chrysene
Concen: 0.425 ng
RT: 21.614 min Scan# 2487
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:228 Resp: 26576
Ion Ratio Lower Upper
228 100
226 30.6 24.5 36.7
229 19.7 16.2 24.4

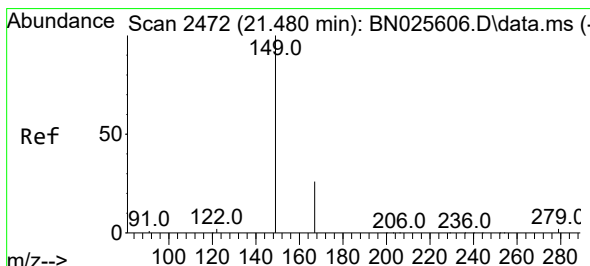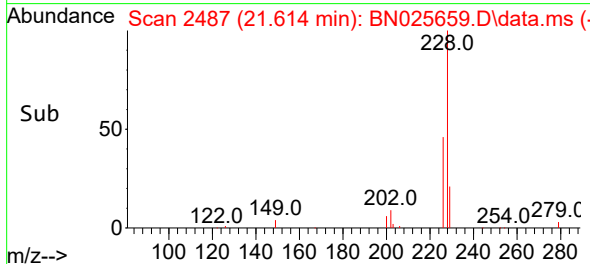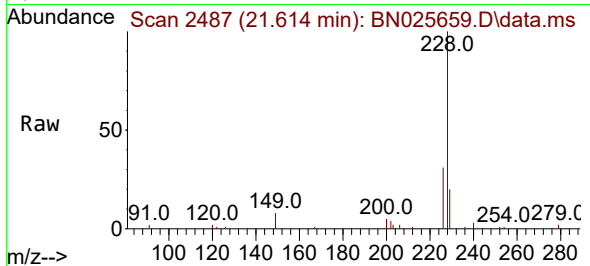

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.434 ng
RT: 21.471 min Scan# 2471
Delta R.T. -0.000 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion:149 Resp: 15230
Ion Ratio Lower Upper
149 100
167 26.4 20.4 30.6
279 2.7 3.3 4.9

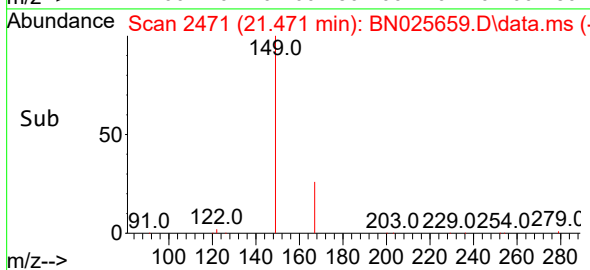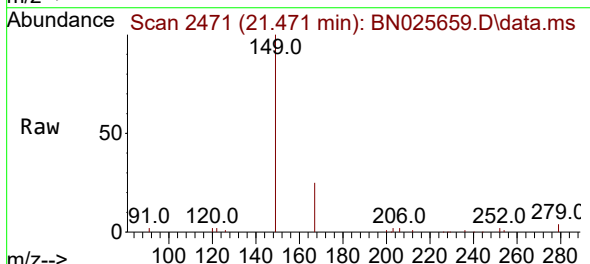



#35

Perylene-d12

Concen: 0.400 ng

RT: 24.054 min Scan# 31

Delta R.T. -0.015 min

Lab File: BN025659.D


Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

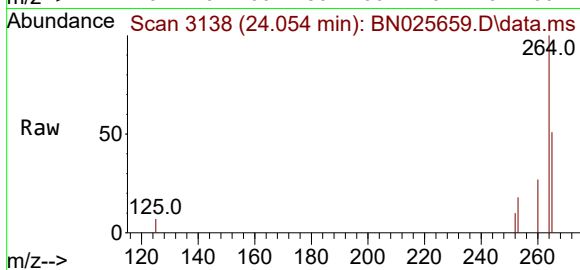




Tgt Ion:264 Resp: 13446

Ion Ratio Lower Upper

264 100

260 27.2 22.3 33.5

265 50.7 54.3 81.5#

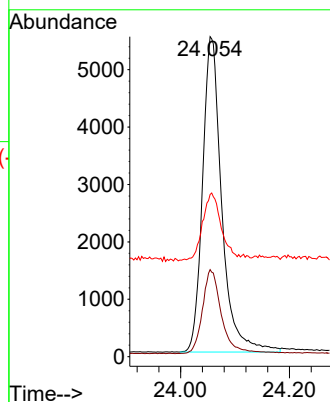

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.405 ng

RT: 26.647 min Scan# 4025

Delta R.T. -0.032 min

Lab File: BN025659.D

Acq: 28 May 2023 00:10




Tgt Ion:276 Resp: 20895


Ion Ratio Lower Upper

276 100

138 28.5 10.5 15.7#


277 24.3 9.2 13.8#

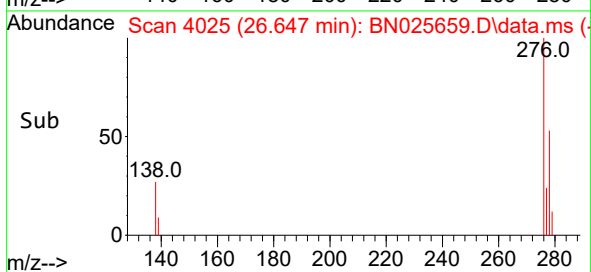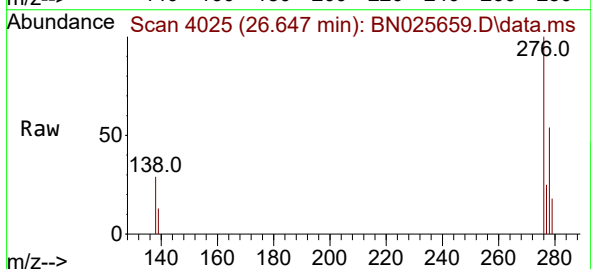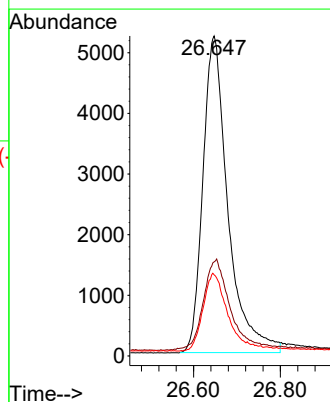





#37
Benzo(b)fluoranthene
Concen: 0.433 ng
RT: 23.297 min Scan# 2879
Delta R.T. -0.006 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 22148
Ion Ratio Lower Upper
252 100
253 28.2 26.2 39.4
125 14.8 12.9 19.3



#38
Benzo(k)fluoranthene
Concen: 0.415 ng
RT: 23.344 min Scan# 2895
Delta R.T. -0.012 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10


Tgt Ion:252 Resp: 22118
Ion Ratio Lower Upper
252 100
253 29.3 26.1 39.1
125 14.4 12.5 18.7

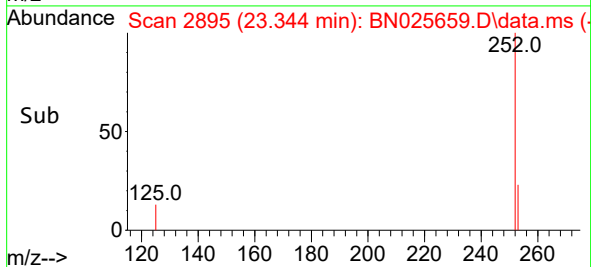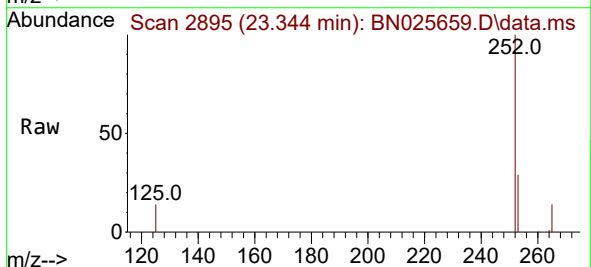






#39
Benzo(a)pyrene
Concen: 0.414 ng
RT: 23.946 min Scan# 3107
Delta R.T. -0.009 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 20256
Ion Ratio Lower Upper
252 100
253 32.6 30.2 45.2
125 18.8 14.8 22.2

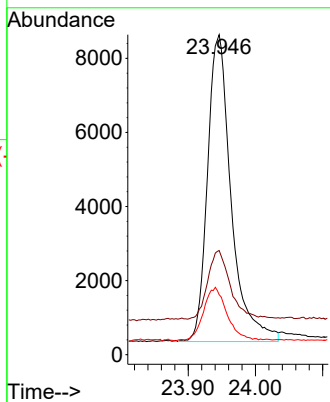

#40
Dibenzo(a,h)anthracene
Concen: 0.402 ng
RT: 26.668 min Scan# 4032
Delta R.T. -0.035 min
Lab File: BN025659.D
Acq: 28 May 2023 00:10

Tgt Ion:278 Resp: 16417
Ion Ratio Lower Upper
278 100
139 21.9 18.6 28.0
279 31.2 27.8 41.8

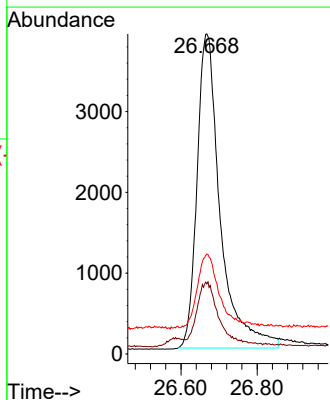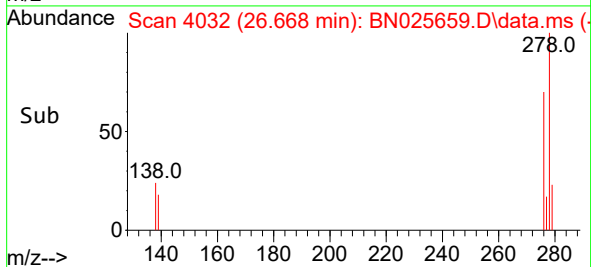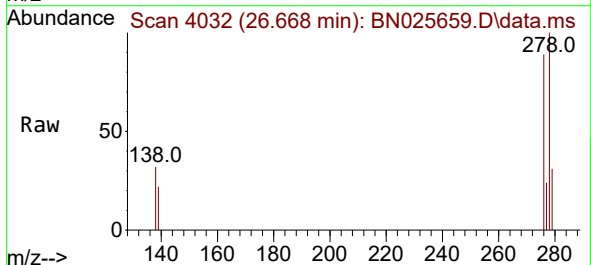

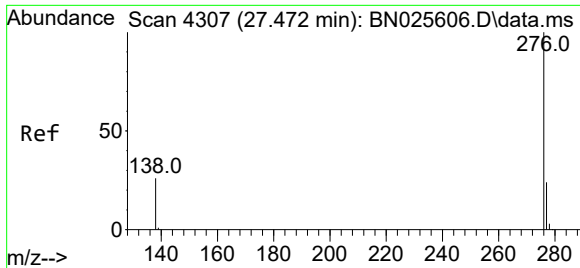

#41

Benzo(g,h,i)perylene

Concen: 0.400 ng

RT: 27.437 min Scan# 41

Delta R.T. -0.032 min

Lab File: BN025659.D


Acq: 28 May 2023 00:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

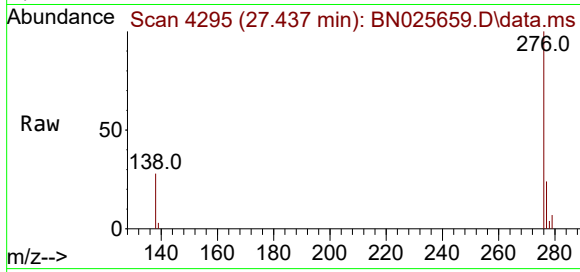

Tgt Ion:276 Resp: 18665

Ion Ratio Lower Upper

276 100

277 24.1 21.4 32.0

138 28.0 22.8 34.2

