
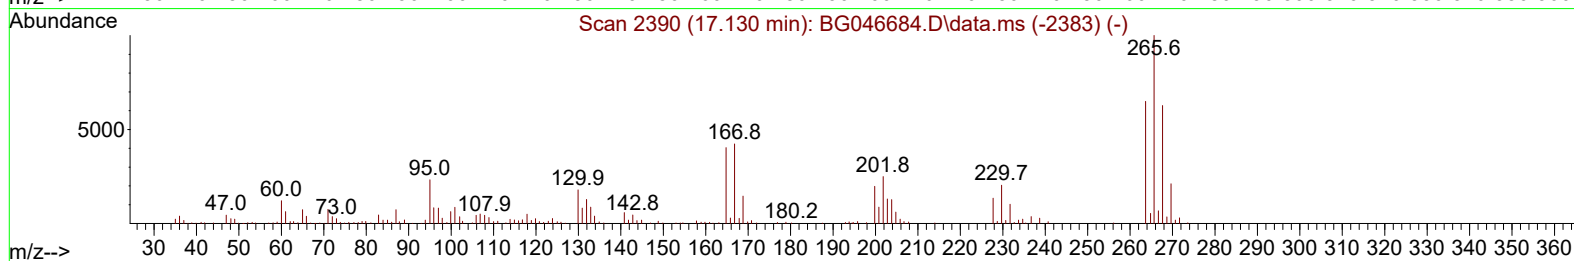
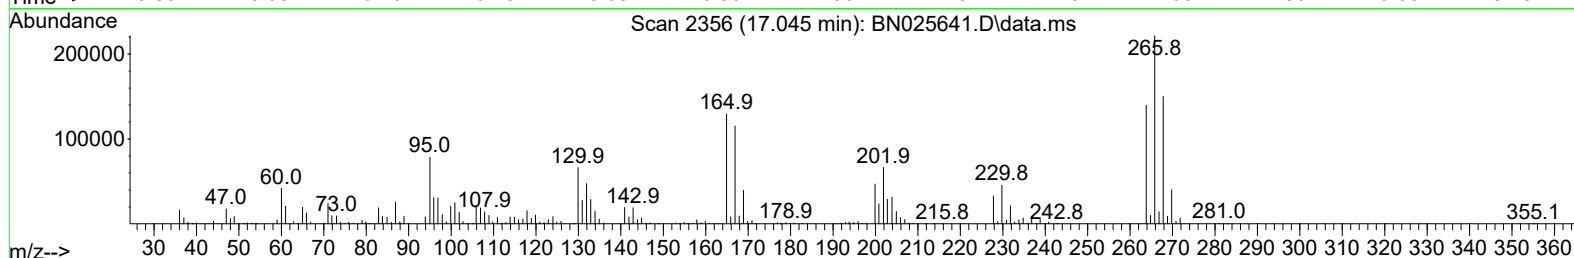


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025641.D
Acq On : 27 May 2023 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: May 29 03:15:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

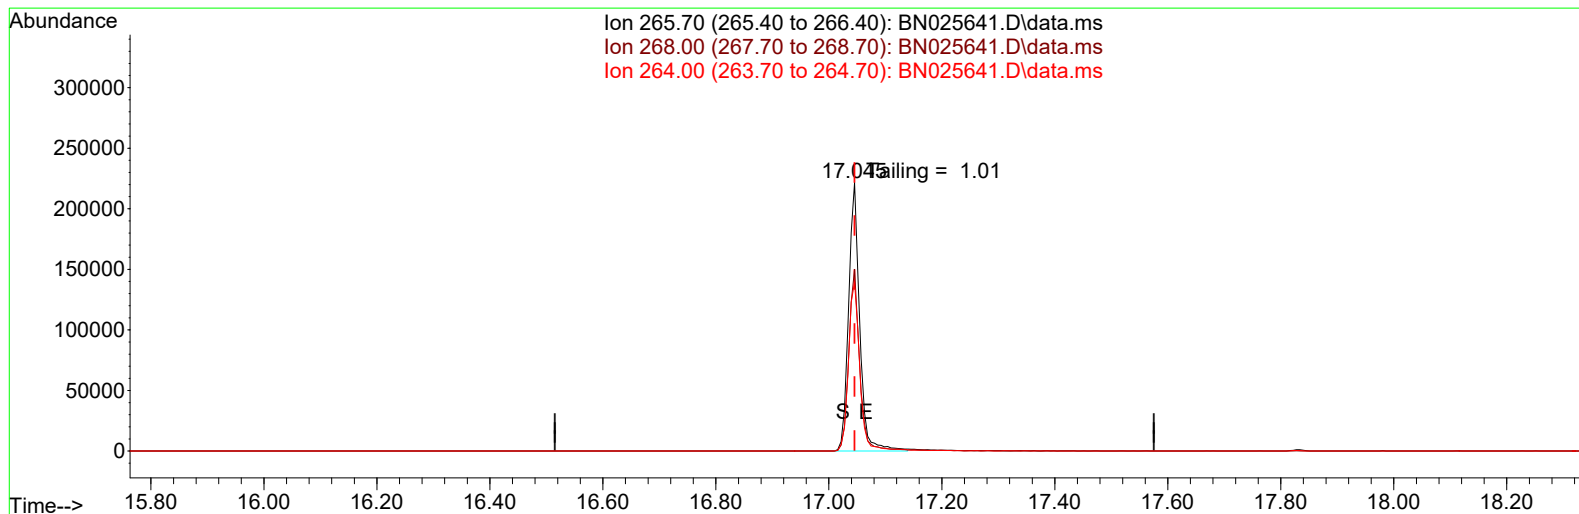

TIC: BN025641.D\data.ms

(70) Pentachlorophenol (C)




17.045min (0.000) 13799.42 ng

response 307881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.65
264.00	61.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025641.D
Acq On : 27 May 2023 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: May 29 03:15:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

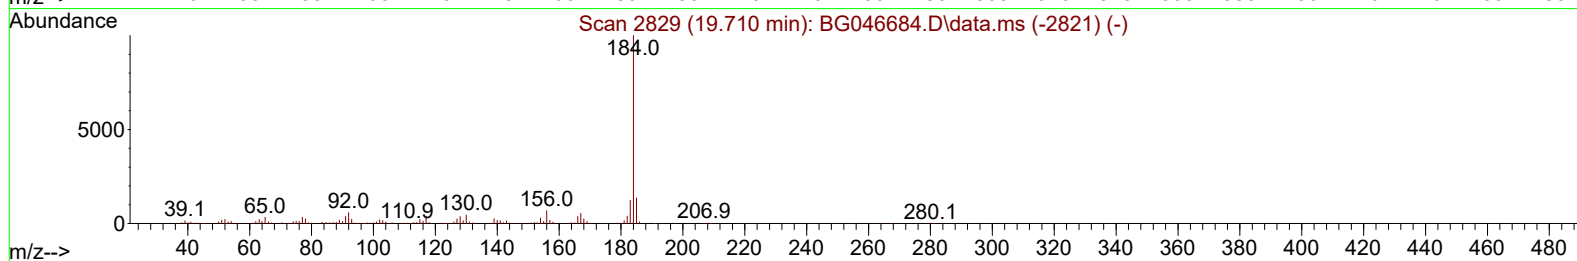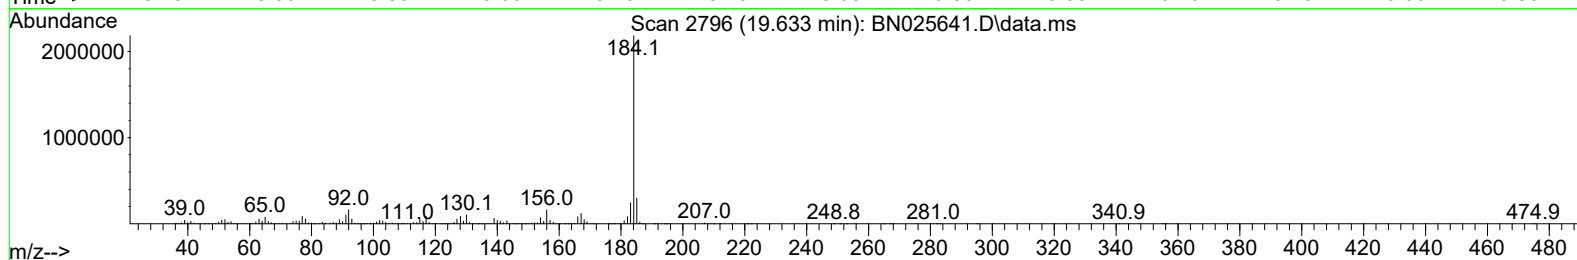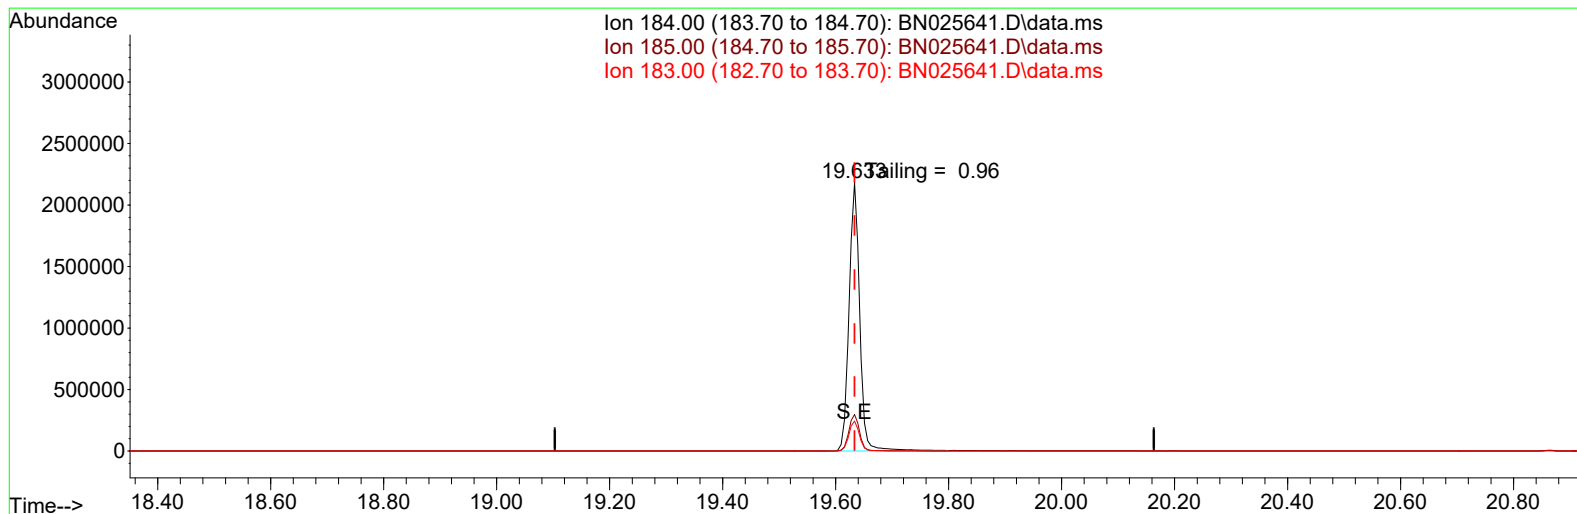

TIC: BN025641.D\data.ms

(77) Benzidine

19.633min (0.000) 0.00 ng

response 2868976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.14
0.00	0.00	0.00