
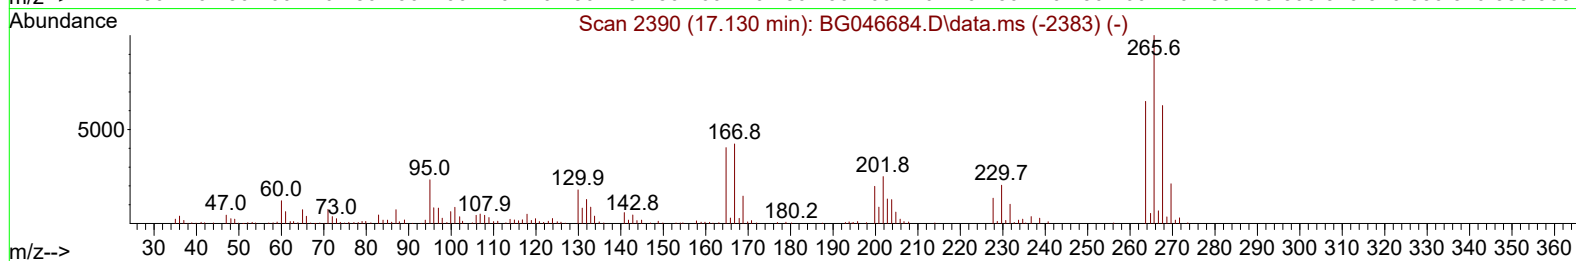
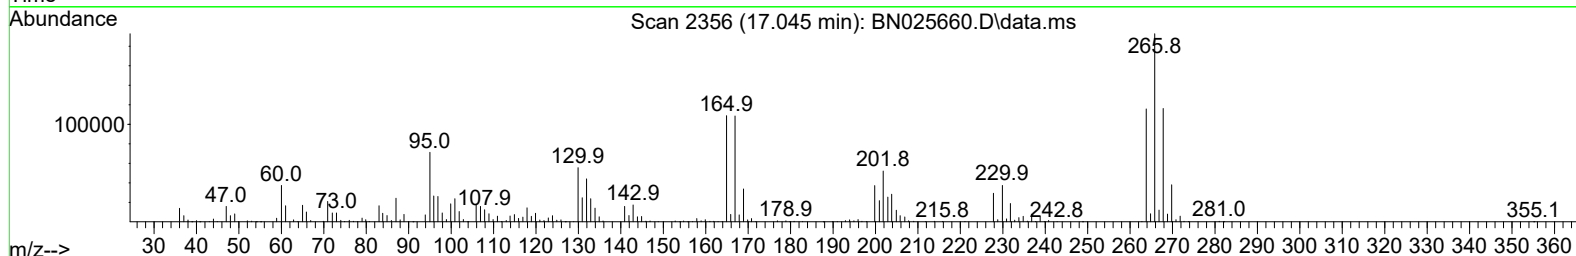


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025660.D
Acq On : 28 May 2023 00:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Quant Time: May 29 03:16:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

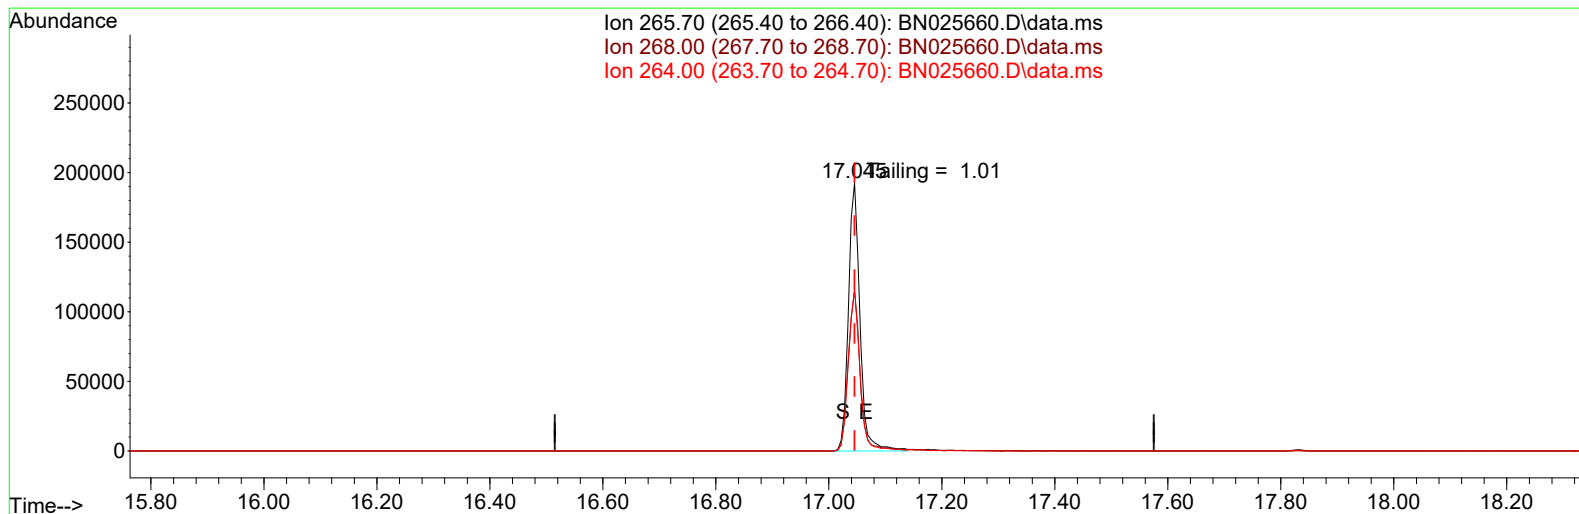

TIC: BN025660.D\data.ms

(70) Pentachlorophenol (C)




17.045min (+ 0.000) 13468.22 ng

response 276393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.25
264.00	61.60	60.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025660.D
Acq On : 28 May 2023 00:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Quant Time: May 29 03:16:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

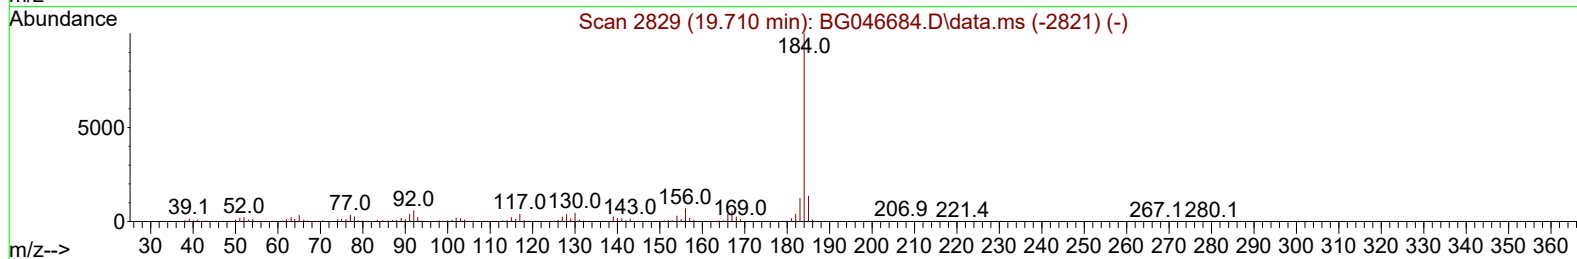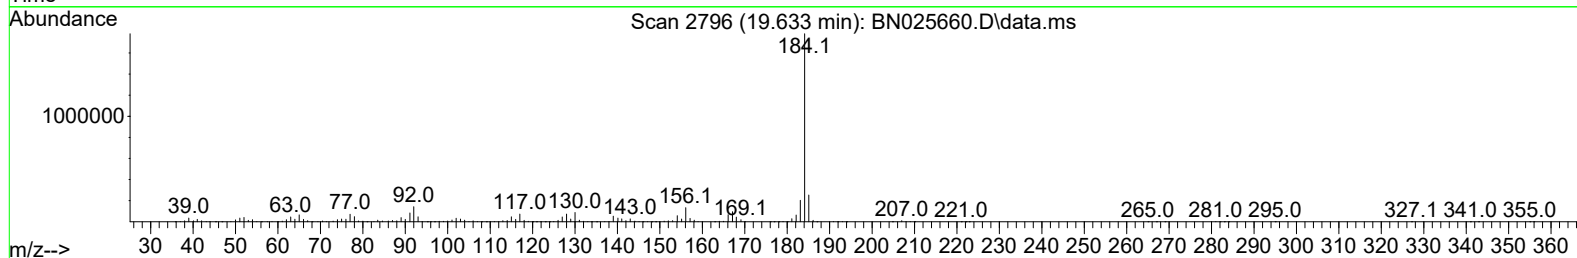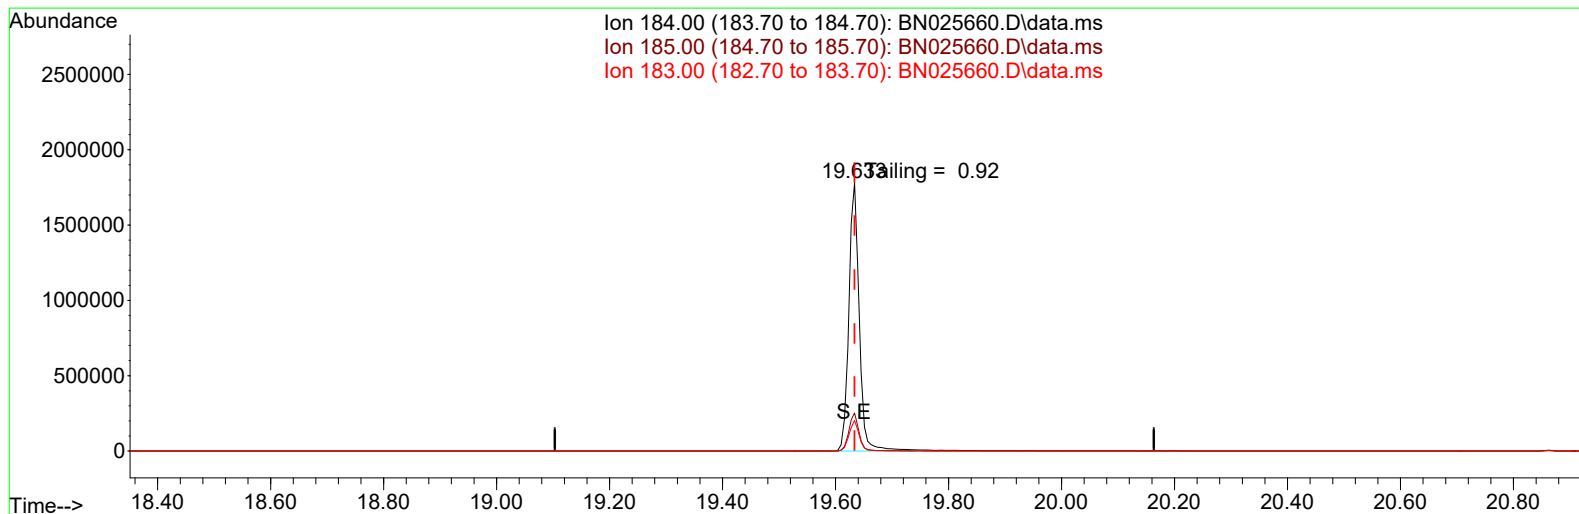

TIC: BN025660.D\data.ms

(77) Benzidine**19.633min (+ 0.000) 0.00 ng****response 2308669**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	11.39
0.00	0.00	0.00