
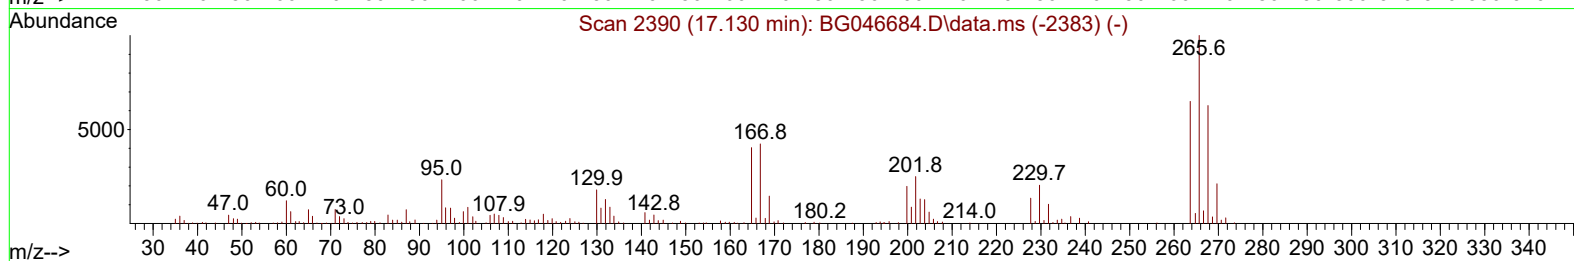
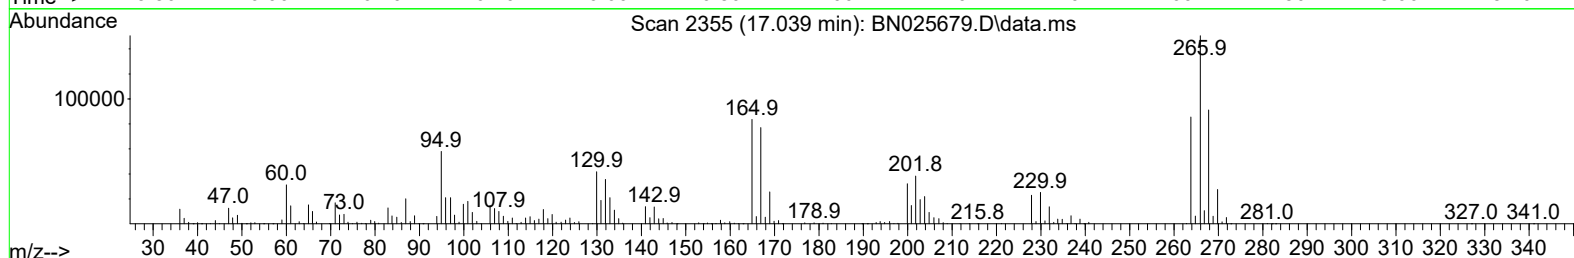


Quant Time: May 29 03:17:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 29 03:15:08 2023  
Response via : Initial Calibration

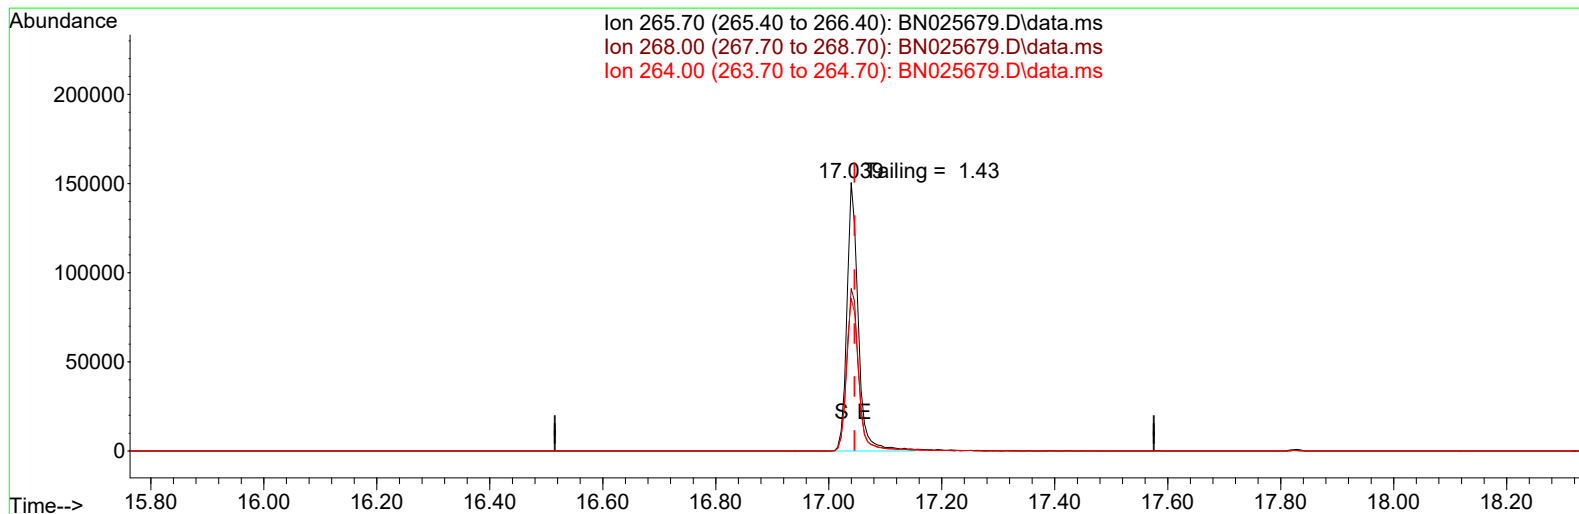

TIC: BN025679.D\data.ms

(70) Pentachlorophenol (C)




17.039min (-0.006) 13409.45 ng

**response**      **208258**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 60.51  |
| 264.00 | 61.60  | 56.83  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052623\  
Data File : BN025679.D  
Acq On : 28 May 2023 13:15  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 77 Sample Multiplier: 1

Quant Time: May 29 03:17:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 29 03:15:08 2023  
Response via : Initial Calibration

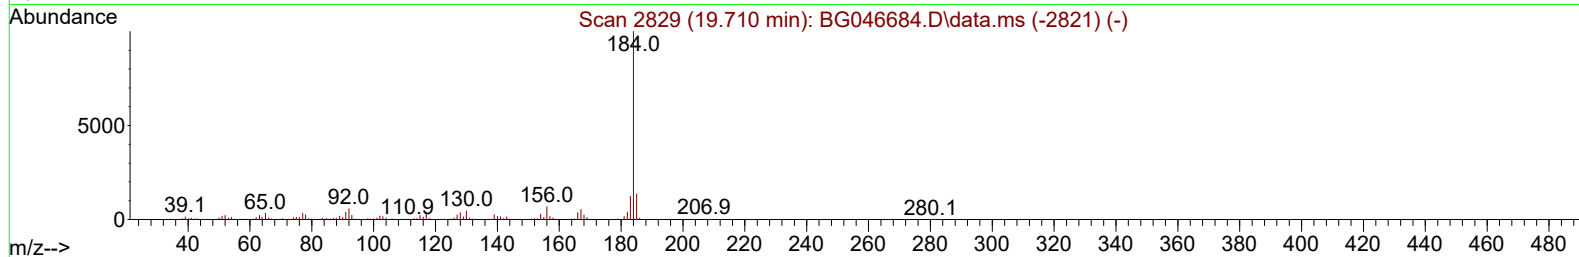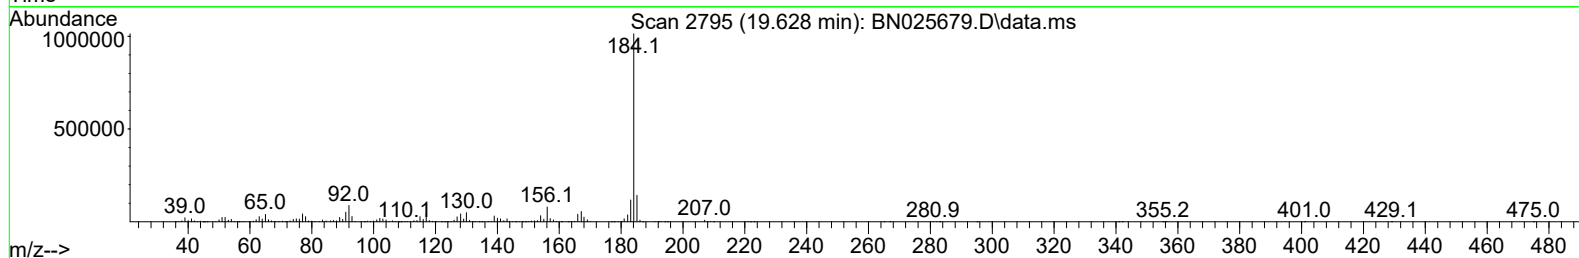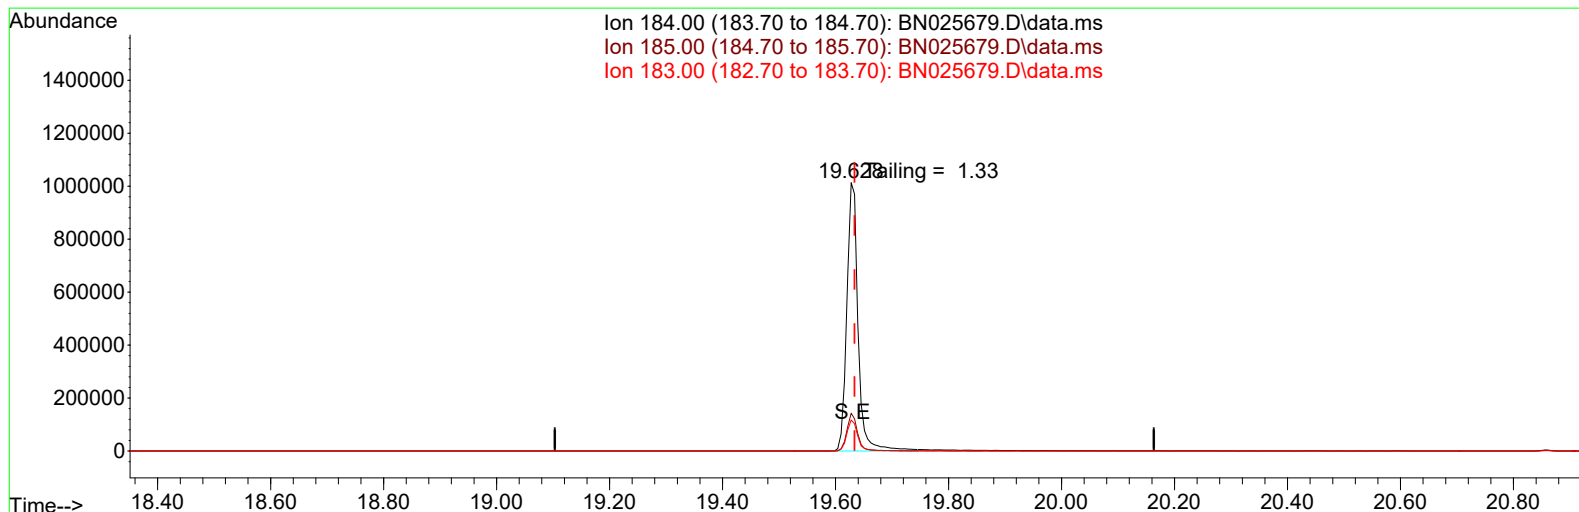

TIC: BN025679.D\data.ms

**(77) Benzidine****19.628min (-0.006) 0.00 ng****response 1422064**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.10  |
| 183.00 | 13.20  | 11.61  |
| 0.00   | 0.00   | 0.00   |