
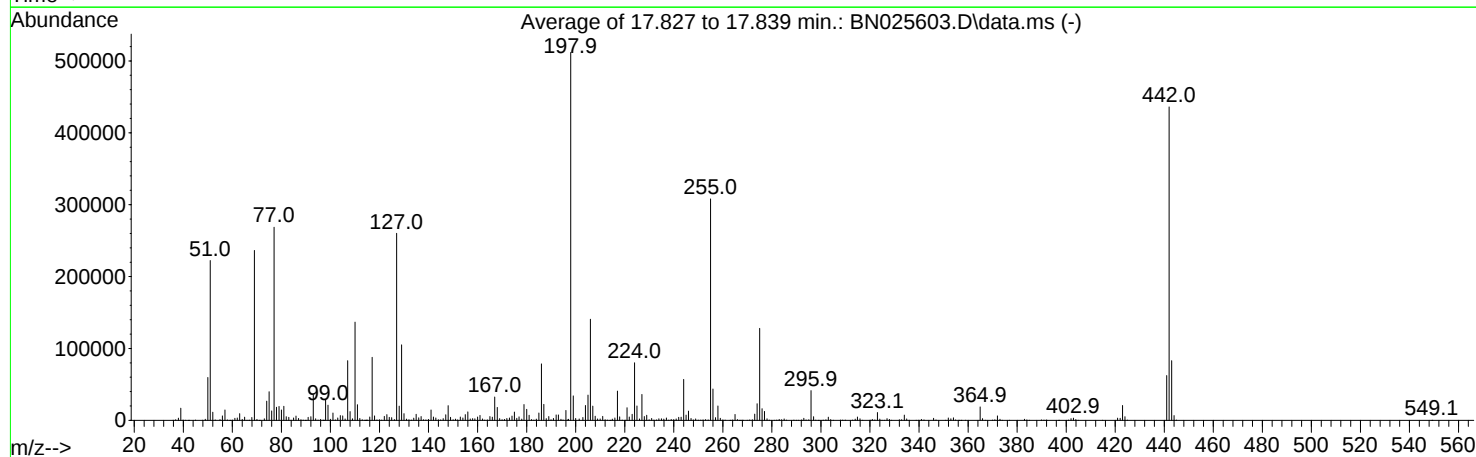


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025603.D
Acq On : 26 May 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 29 00:47:45 2023

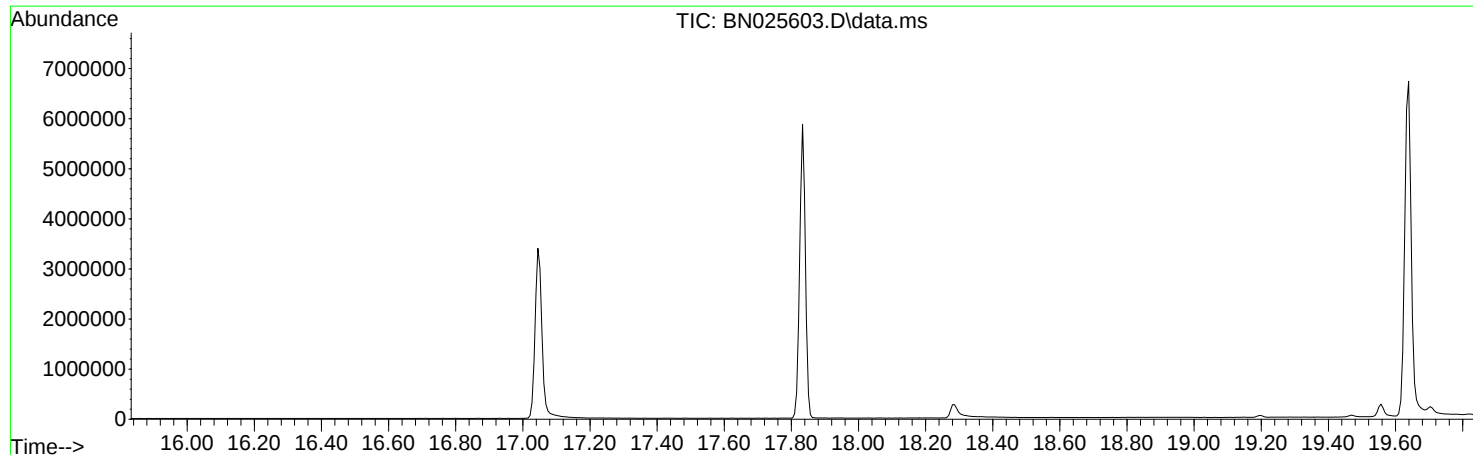

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	222322	PASS
68	69	0.00	2	1.7	4078	PASS
69	198	0.00	100	46.2	236463	PASS
70	69	0.00	2	0.6	1331	PASS
127	198	10	80	50.8	260096	PASS
197	198	0.00	2	0.3	1578	PASS
198	198	100	100	100.0	511723	PASS
199	198	5	9	6.7	34128	PASS
275	198	10	60	25.0	128083	PASS
365	198	1	100	3.7	18802	PASS
441	198	0.01	100	12.2	62363	PASS
442	442	50	100	100.0	436053	PASS
443	442	15	24	19.0	82987	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_N	<u>BN025603.D</u>
Compound Name	Response	Retention Time
DDT	1504938	20.874
DDD	32636	20.486
DDE	0	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32636	1537574	2.12

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025603.D
Acq On : 26 May 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 27 06:26:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 27 06:25:38 2023
Response via : Initial Calibration

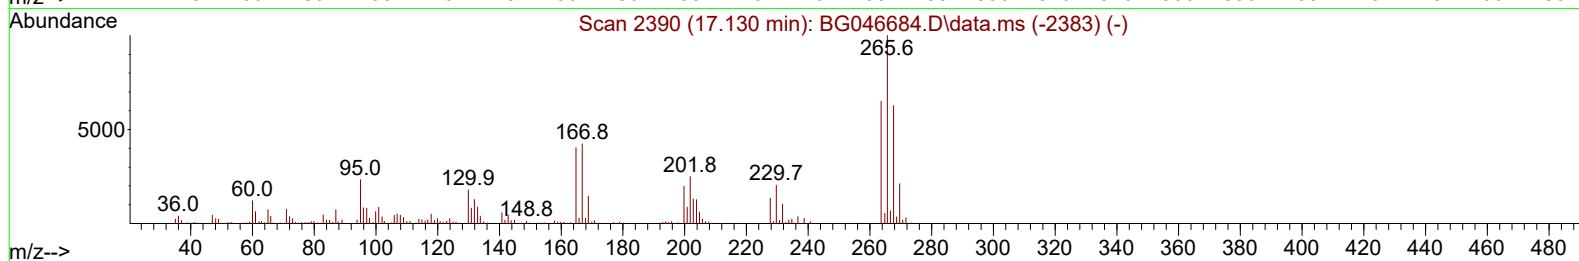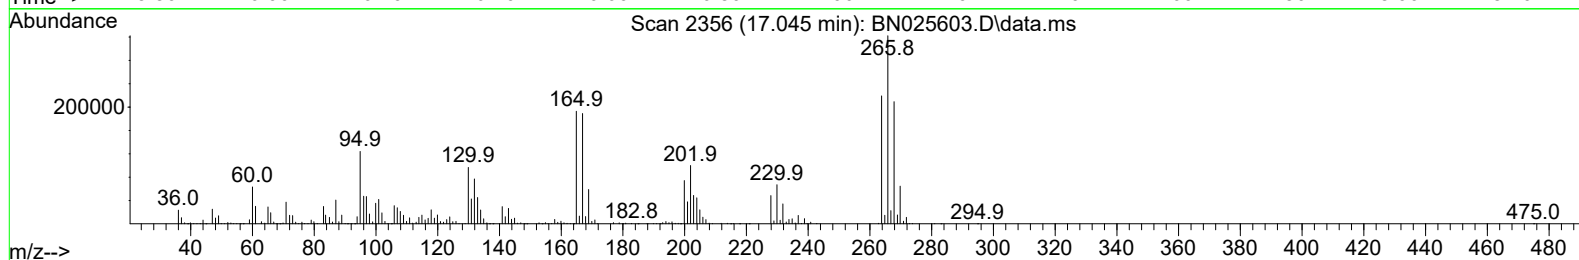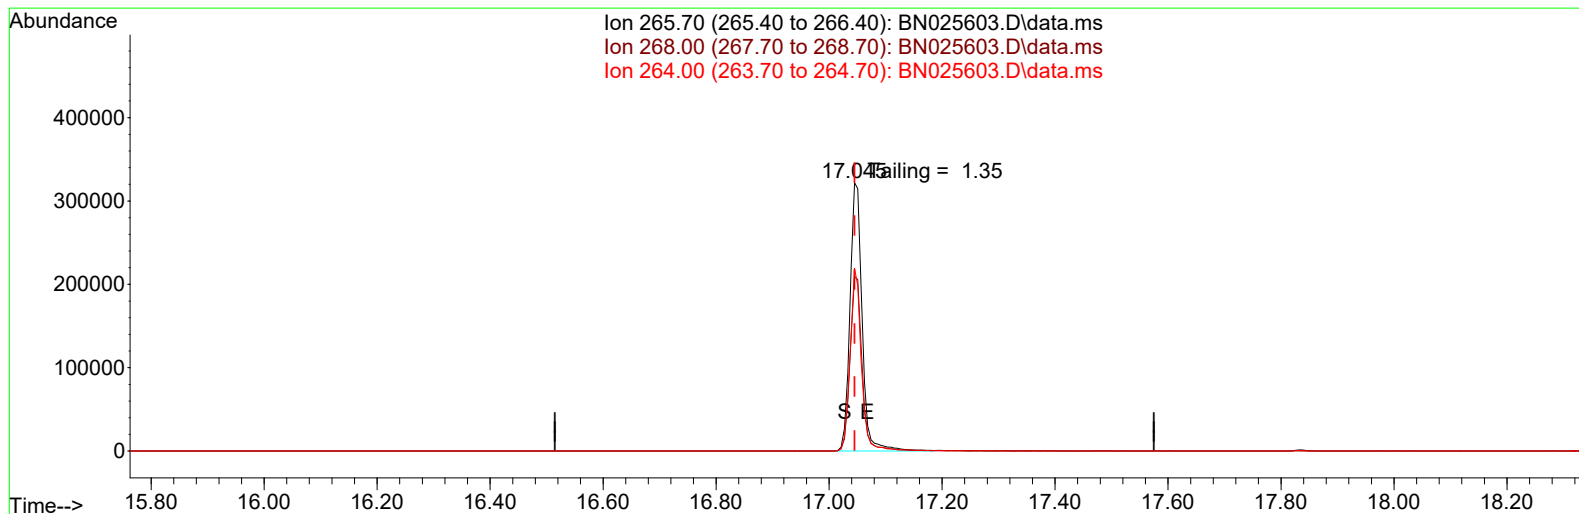

TIC: BN025603.D\data.ms

(70) Pentachlorophenol (C)

17.045min (0.000) 17239.71 ng




response 482725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.94
264.00	61.60	68.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025603.D
Acq On : 26 May 2023 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 27 06:26:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 27 06:25:38 2023
Response via : Initial Calibration

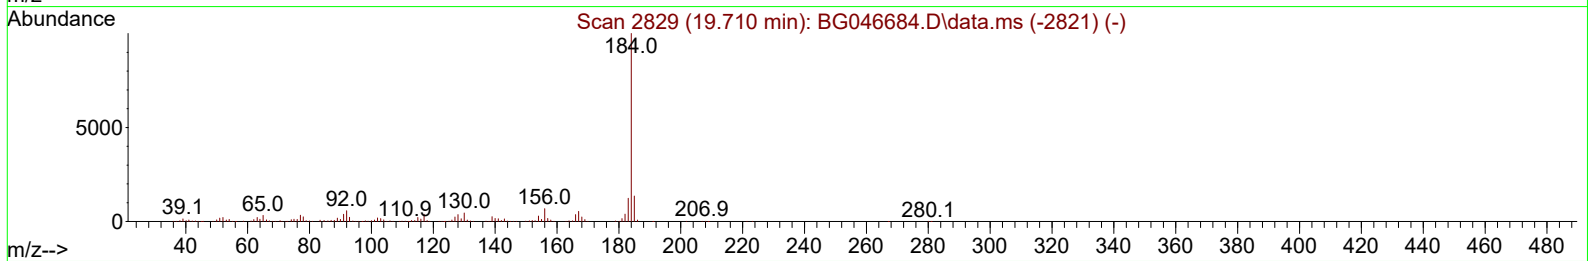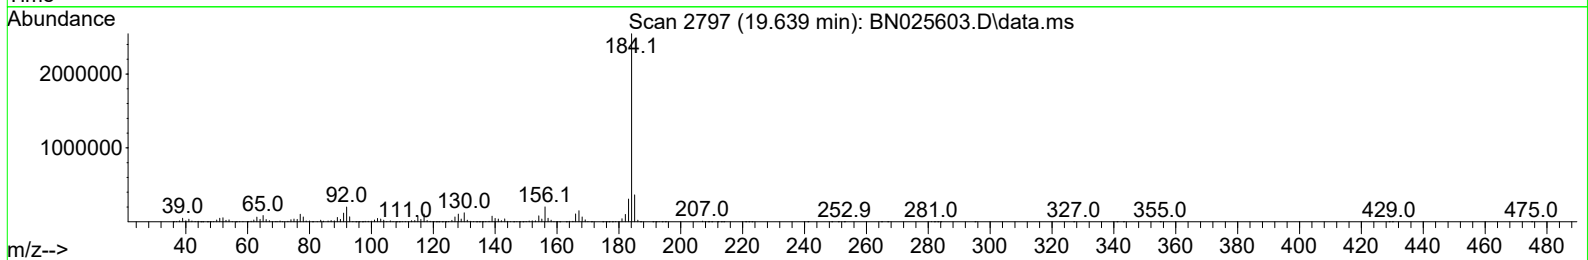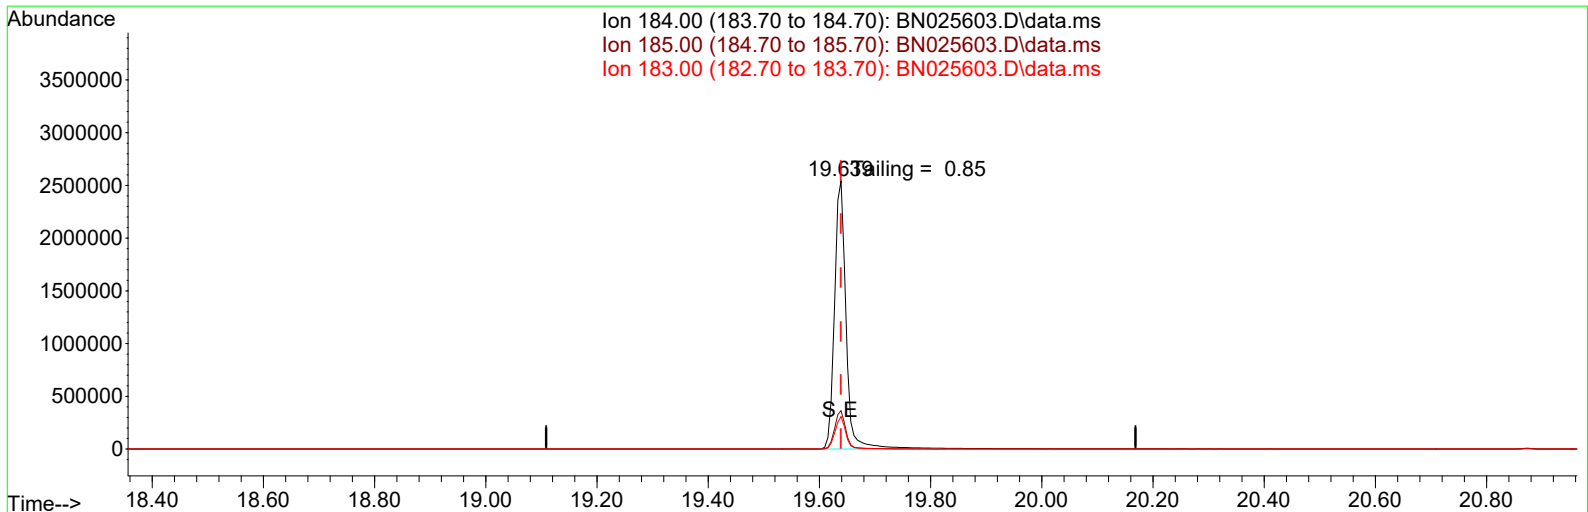

TIC: BN025603.D\data.ms

(77) Benzidine

19.639min (0.000) 0.00 ng

response 3701443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.11
0.00	0.00	0.00