
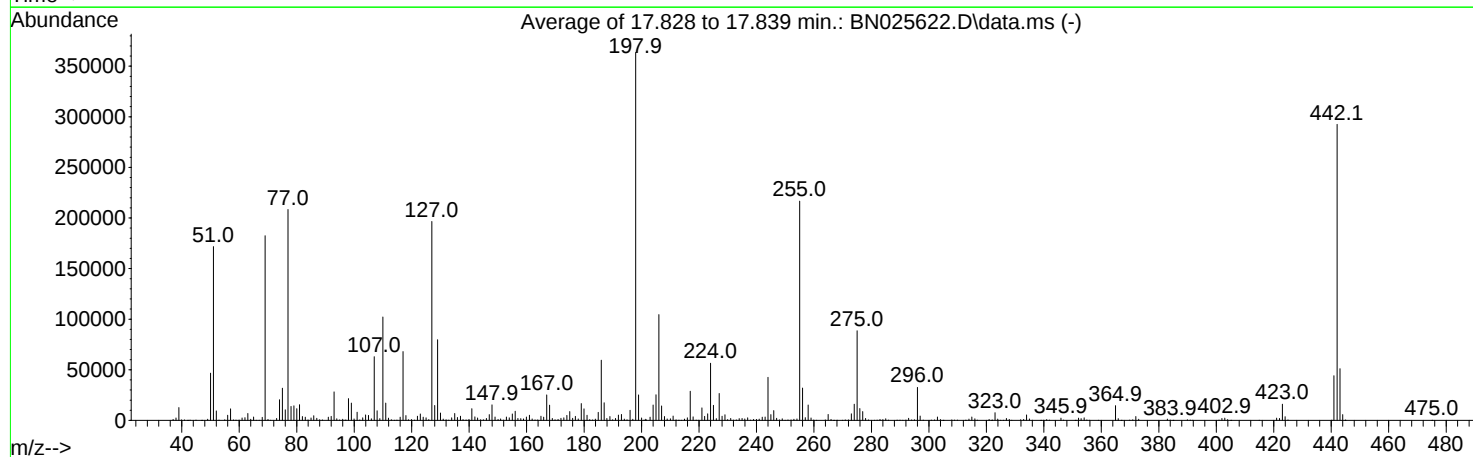


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025622.D
 Acq On : 26 May 2023 23:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 29 00:47:45 2023

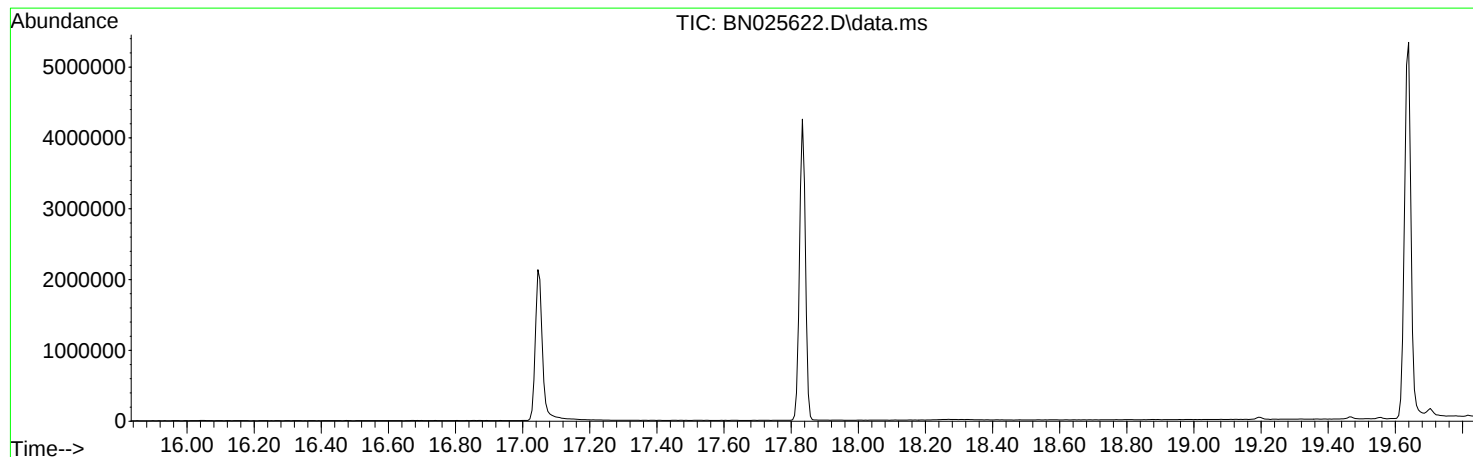

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	171755	PASS
68	69	0.00	2	1.6	2977	PASS
69	198	0.00	100	50.2	182528	PASS
70	69	0.00	2	0.6	1035	PASS
127	198	10	80	54.1	196629	PASS
197	198	0.00	2	0.3	1084	PASS
198	198	100	100	100.0	363520	PASS
199	198	5	9	6.9	25091	PASS
275	198	10	60	24.4	88555	PASS
365	198	1	100	4.0	14491	PASS
441	198	0.01	100	12.1	44163	PASS
442	442	50	100	100.0	292523	PASS
443	442	15	24	17.5	51165	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_N	<u>BN025622.D</u>
Compound Name	Response	Retention Time
DDT	1045347	20.869
DDD	36148	20.48
DDE	0	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36148	1081495	3.34

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025622.D
 Acq On : 26 May 2023 23:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 27 06:28:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 27 06:25:38 2023
 Response via : Initial Calibration

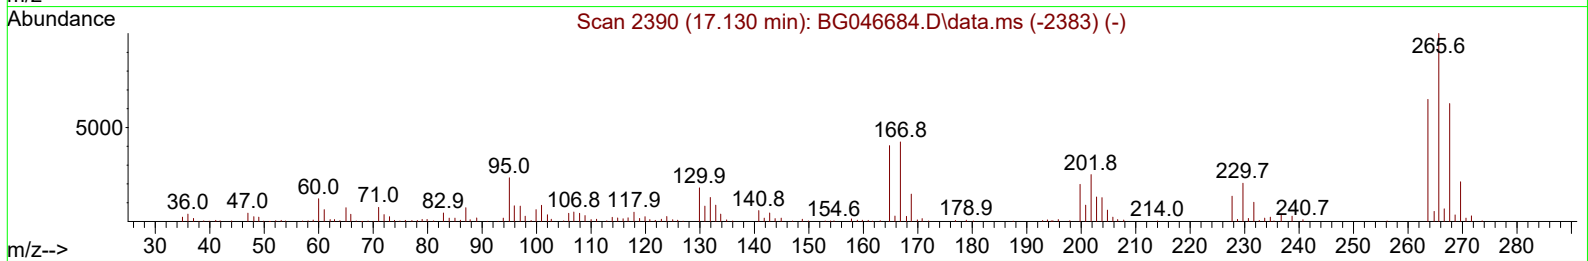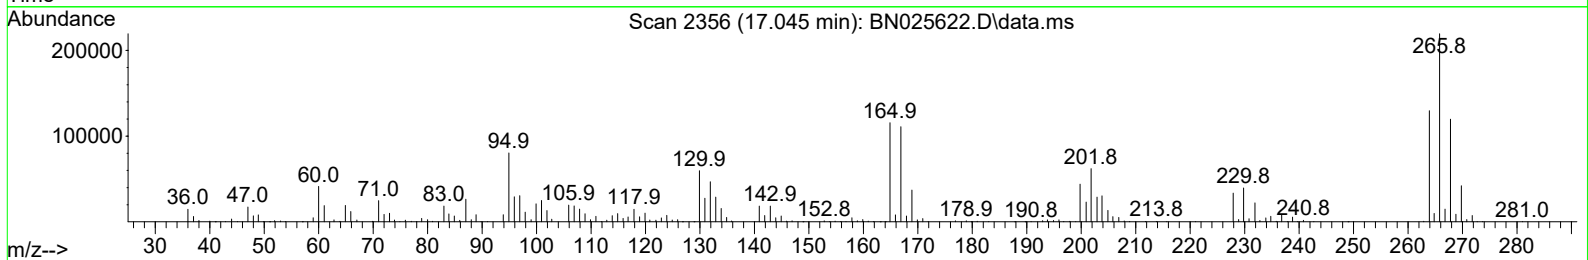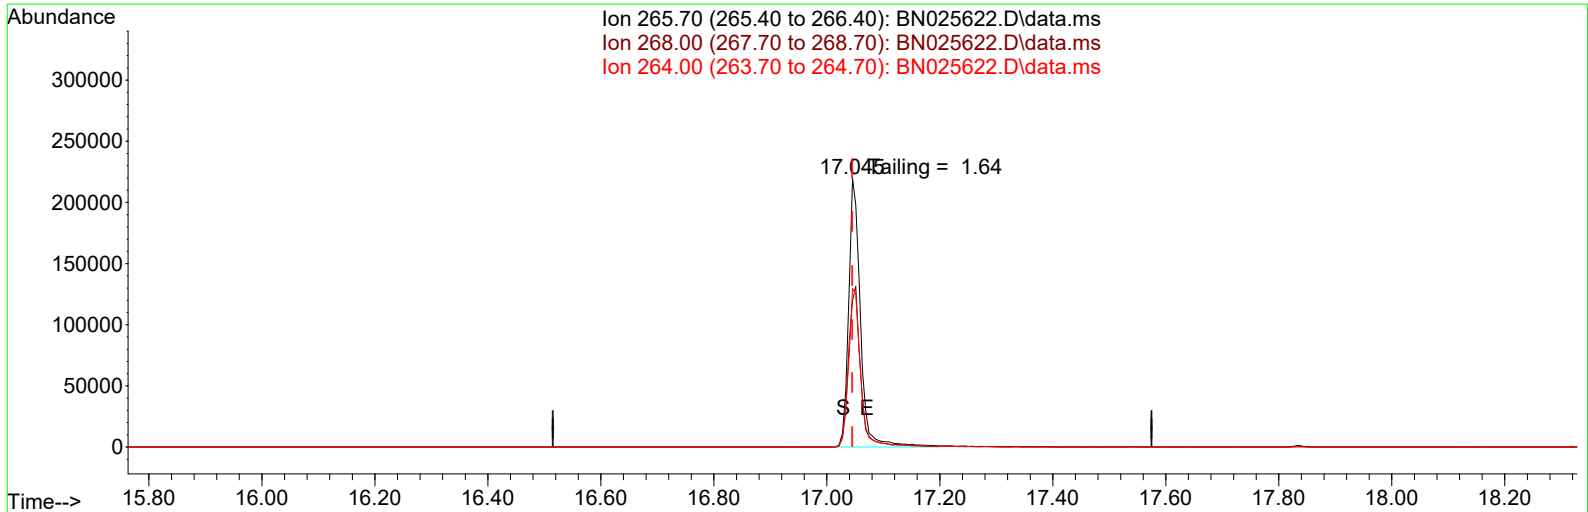

TIC: BN025622.D\data.ms

(70) Pentachlorophenol (C)

17.045min (+ 0.000) 15137.93 ng




response 321588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	54.62
264.00	61.60	59.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025622.D
Acq On : 26 May 2023 23:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 27 06:28:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 27 06:25:38 2023
Response via : Initial Calibration

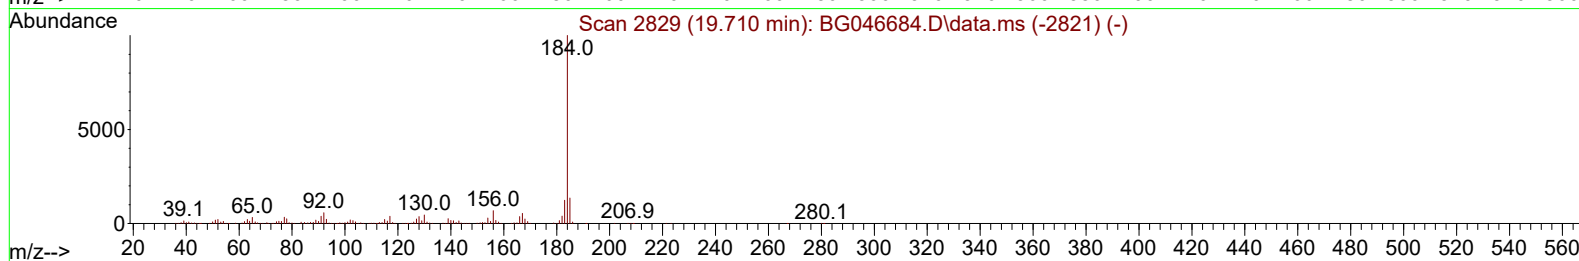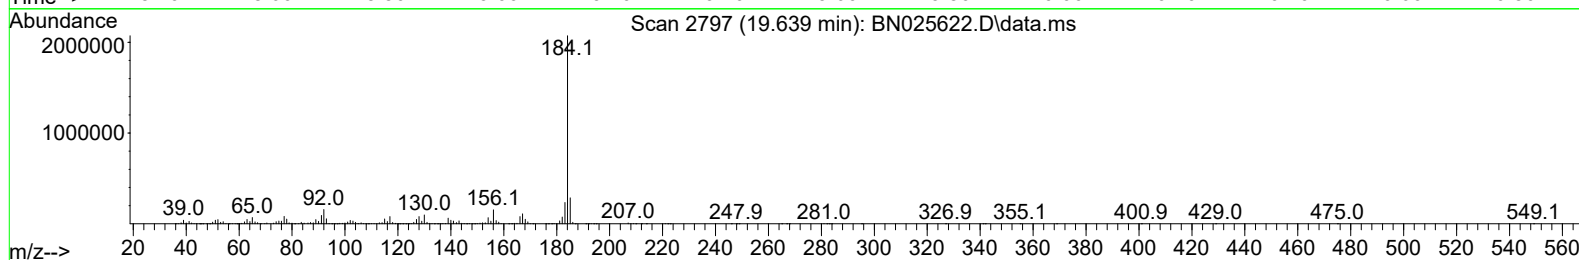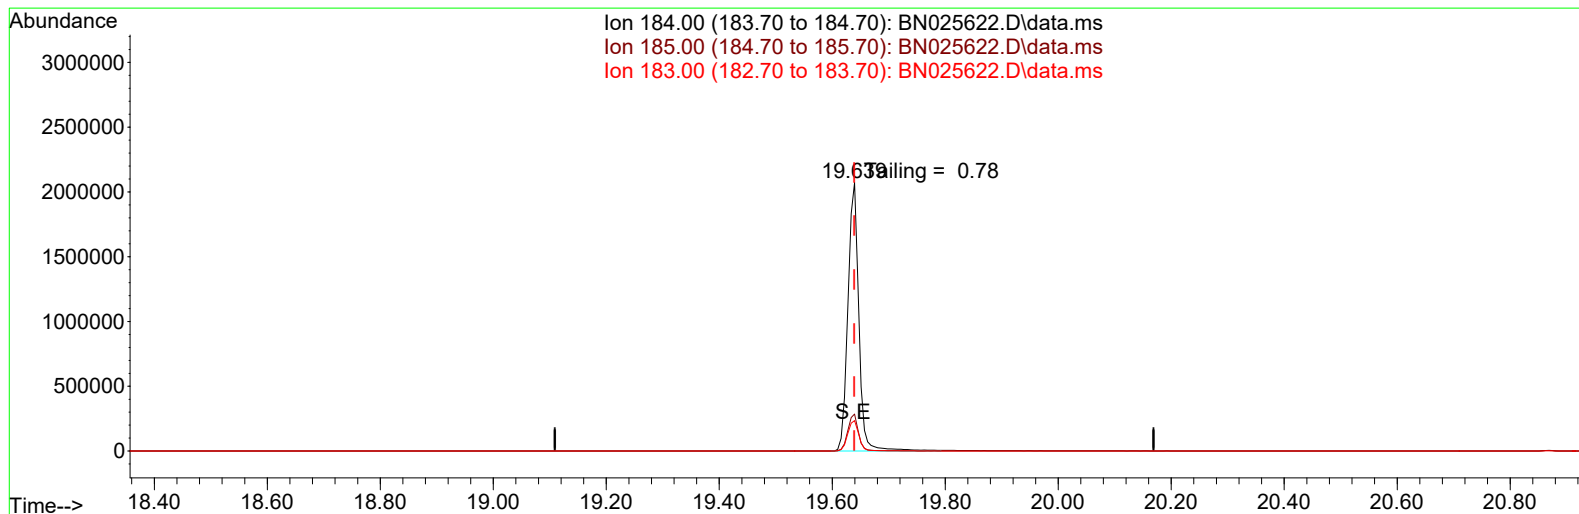

TIC: BN025622.D\data.ms

(77) Benzidine

19.639min (+ 0.000) 0.00 ng

response 2816397

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	11.34
0.00	0.00	0.00