
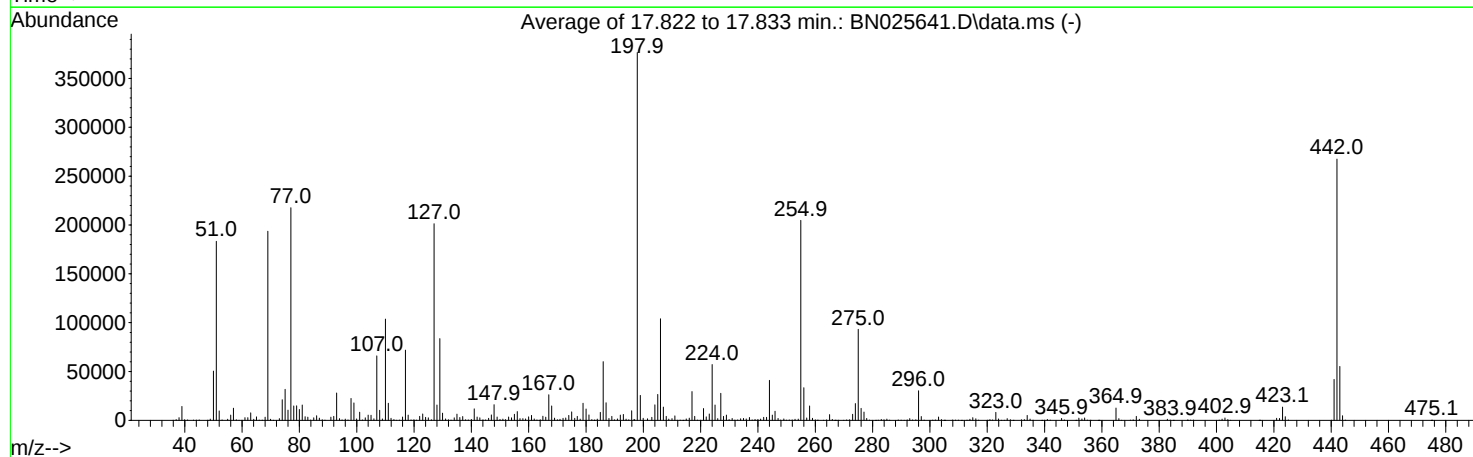


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025641.D
 Acq On : 27 May 2023 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 29 00:47:45 2023

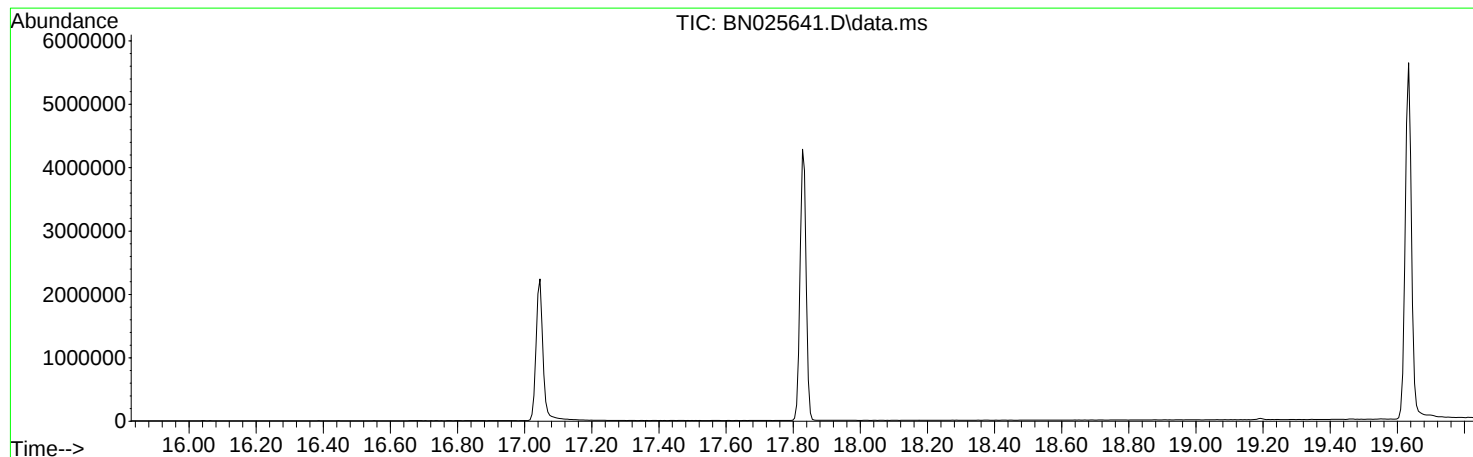

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	183317	PASS
68	69	0.00	2	1.7	3234	PASS
69	198	0.00	100	51.4	193685	PASS
70	69	0.00	2	0.6	1128	PASS
127	198	10	80	53.4	201237	PASS
197	198	0.00	2	0.3	1065	PASS
198	198	100	100	100.0	376576	PASS
199	198	5	9	6.8	25536	PASS
275	198	10	60	24.7	93168	PASS
365	198	1	100	3.4	12669	PASS
441	198	0.01	100	11.1	41917	PASS
442	442	50	100	100.0	267456	PASS
443	442	15	24	20.7	55232	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_N	<u>BN025641.D</u>
Compound Name	Response	Retention Time
DDT	1127850	20.863
DDD	30563	20.422
DDE	340	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30903	1158753	2.67

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025641.D
 Acq On : 27 May 2023 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 29 03:15:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 29 03:15:08 2023
 Response via : Initial Calibration

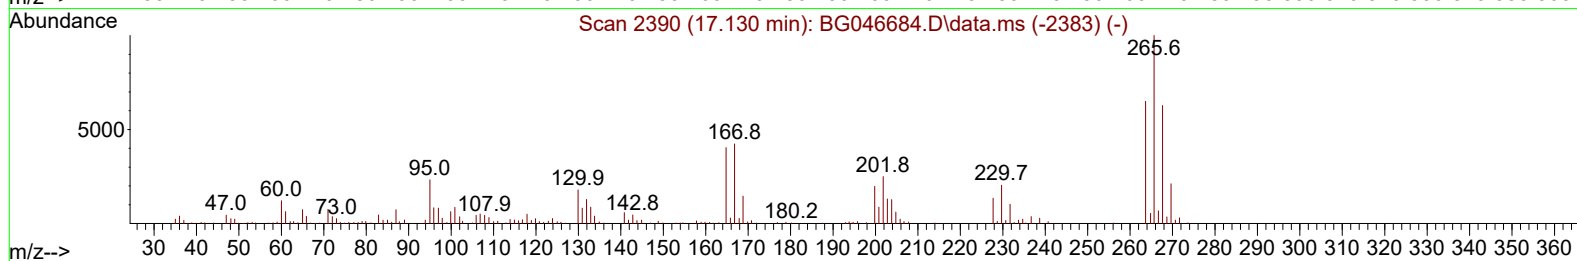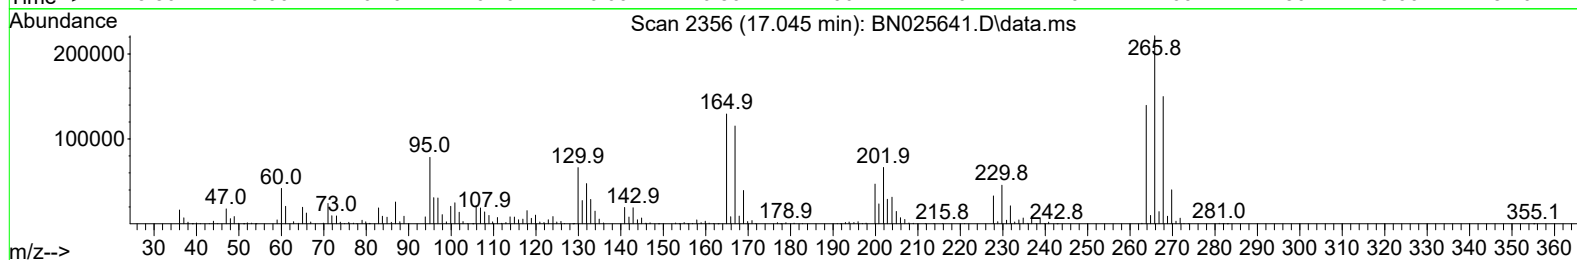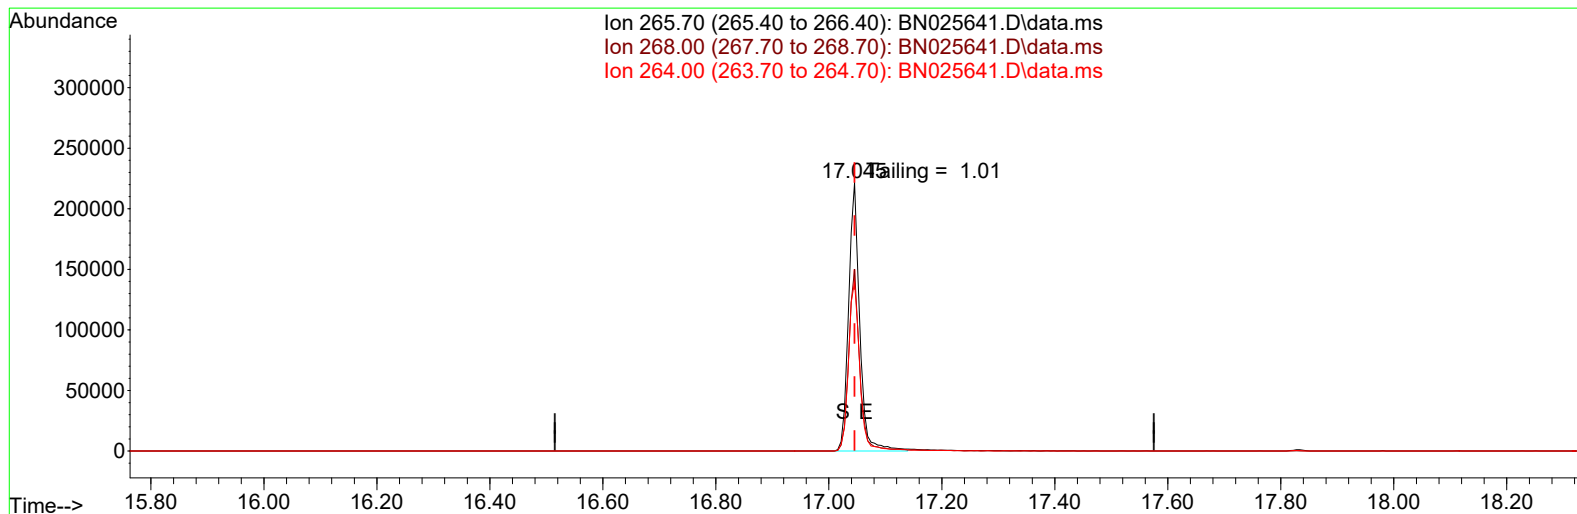

TIC: BN025641.D\data.ms

(70) Pentachlorophenol (C)

17.045min (0.000) 13799.42 ng




response 307881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.65
264.00	61.60	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025641.D
Acq On : 27 May 2023 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 29 03:15:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

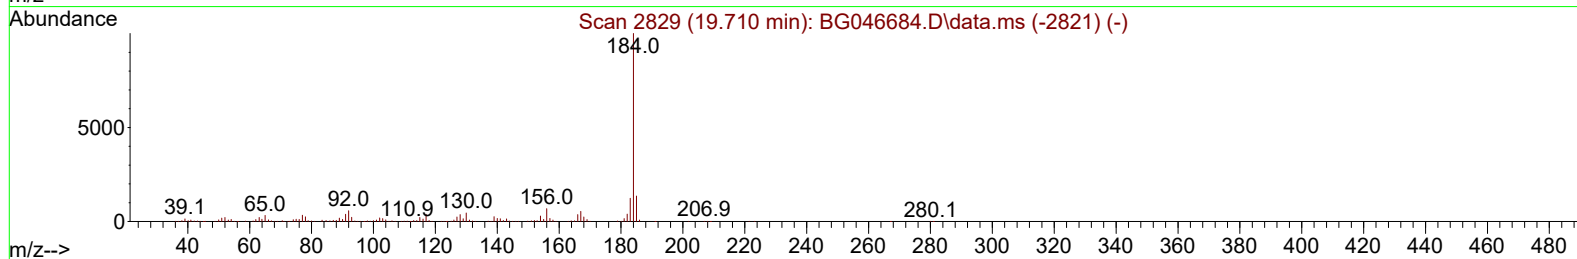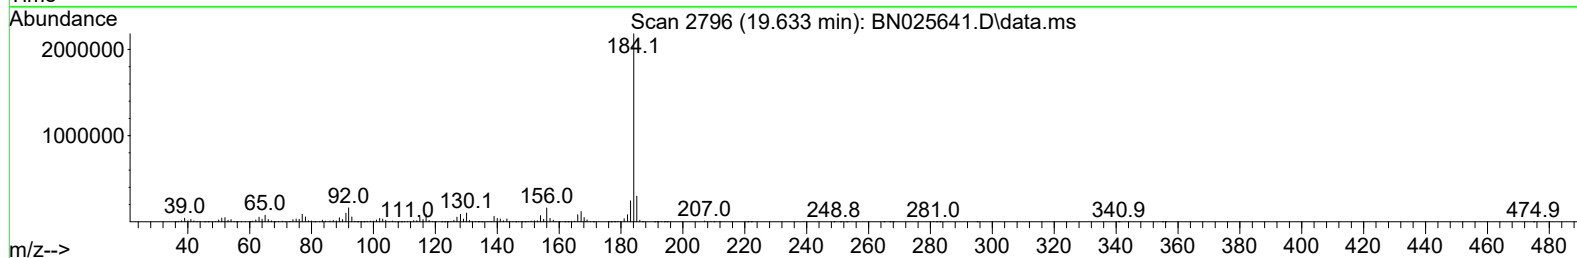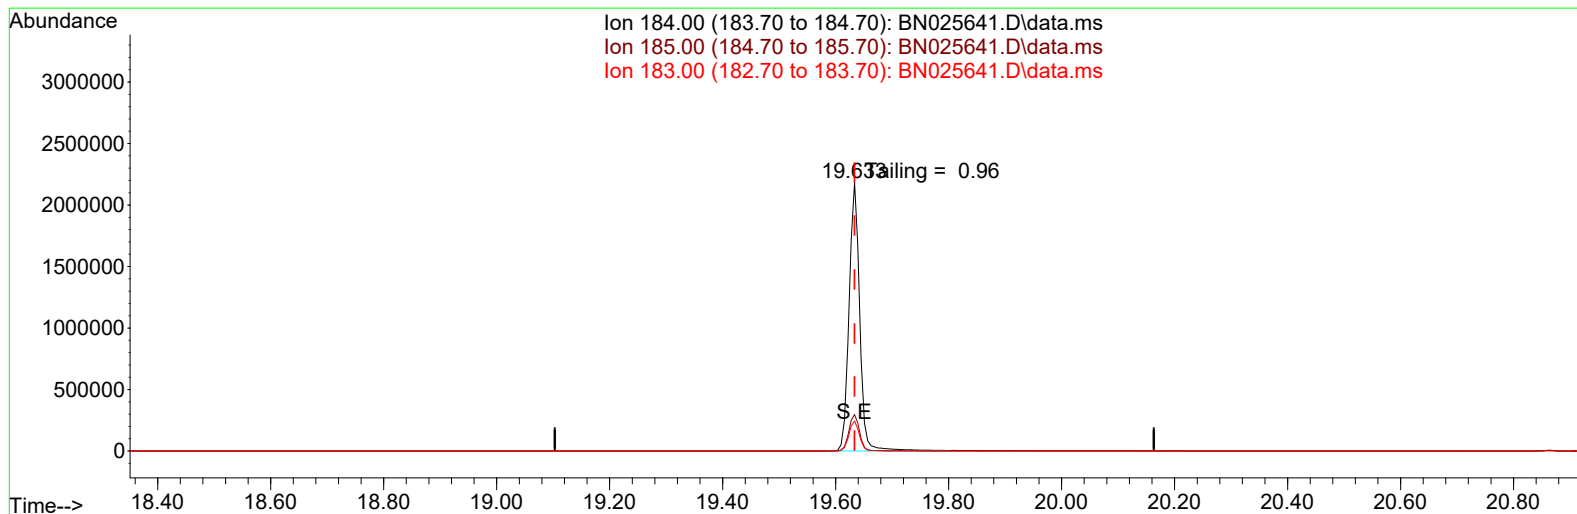

TIC: BN025641.D\data.ms

(77) Benzidine

19.633min (0.000) 0.00 ng

response 2868976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.14
0.00	0.00	0.00