
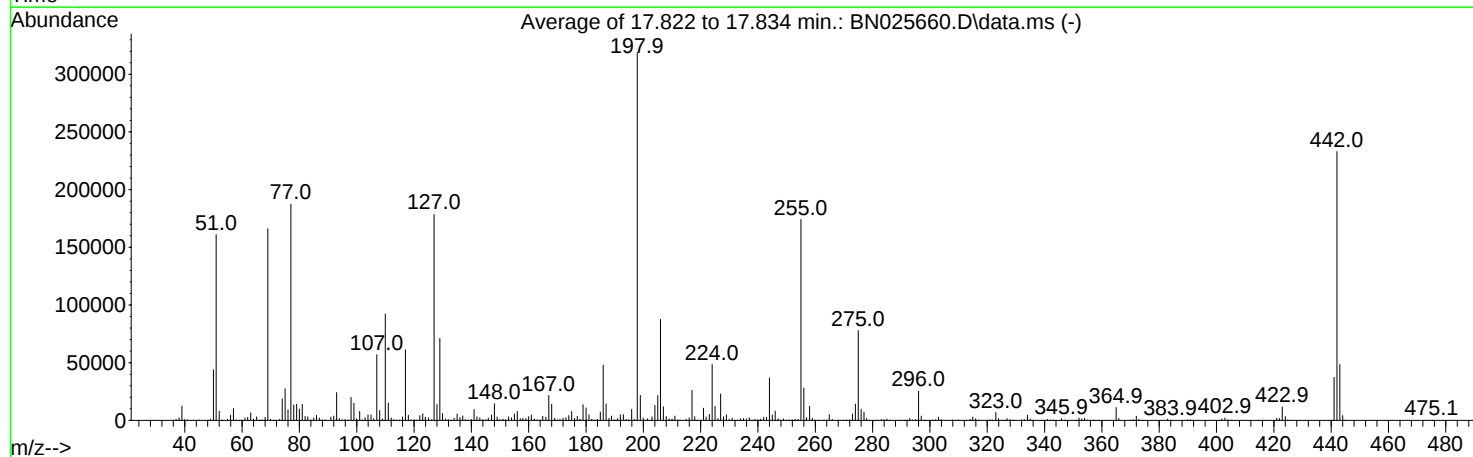


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025660.D
Acq On : 28 May 2023 00:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 29 00:47:45 2023

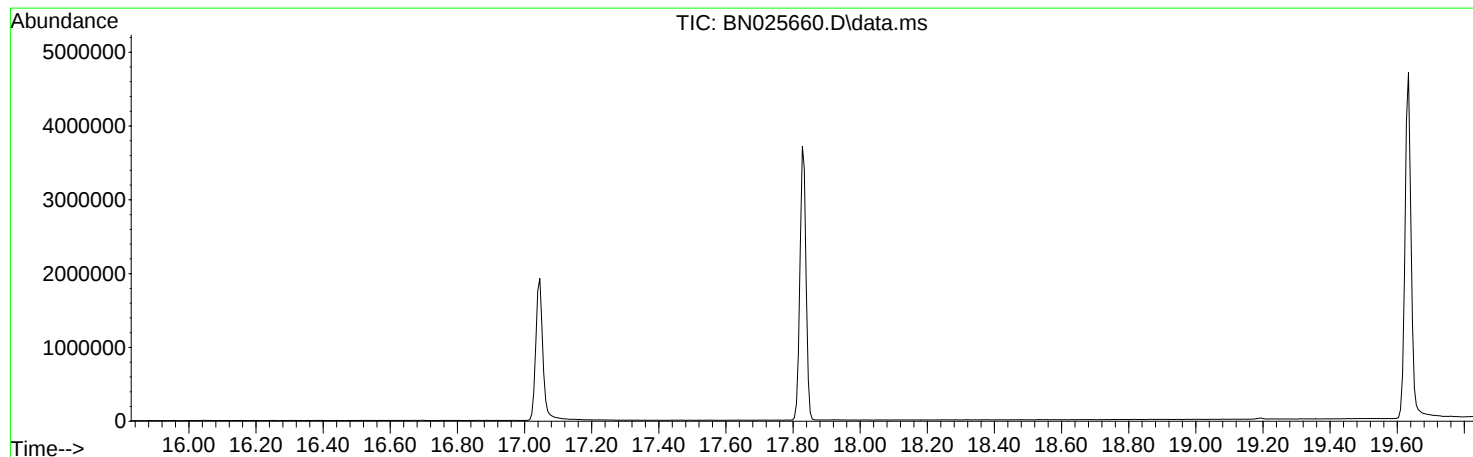

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	161077	PASS
68	69	0.00	2	1.6	2621	PASS
69	198	0.00	100	52.1	166101	PASS
70	69	0.00	2	0.5	801	PASS
127	198	10	80	56.0	178496	PASS
197	198	0.00	2	0.3	895	PASS
198	198	100	100	100.0	318848	PASS
199	198	5	9	6.8	21696	PASS
275	198	10	60	24.4	77883	PASS
365	198	1	100	3.5	11187	PASS
441	198	0.01	100	11.7	37272	PASS
442	442	50	100	100.0	233069	PASS
443	442	15	24	20.8	48469	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_N	<u>BN025660.D</u>
Compound Name	Response	Retention Time
DDT	954173	20.863
DDD	23644	20.422
DDE	484	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24128	978301	2.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025660.D
 Acq On : 28 May 2023 00:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 29 03:16:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 29 03:15:08 2023
 Response via : Initial Calibration

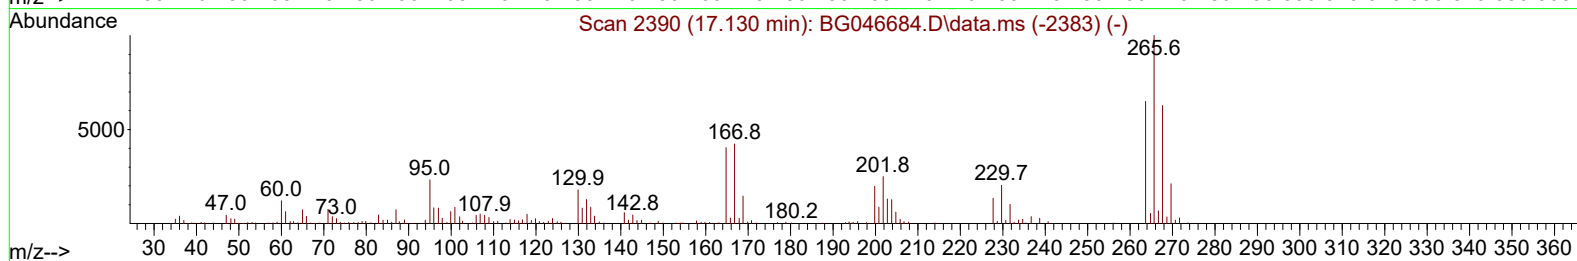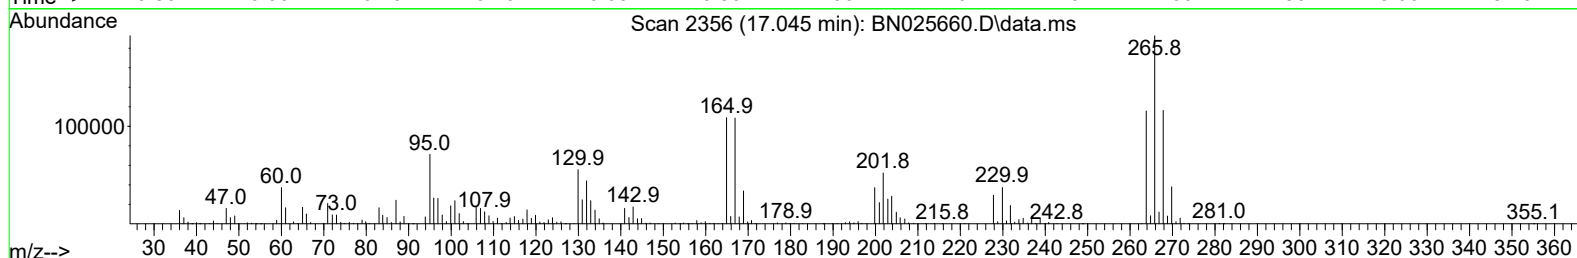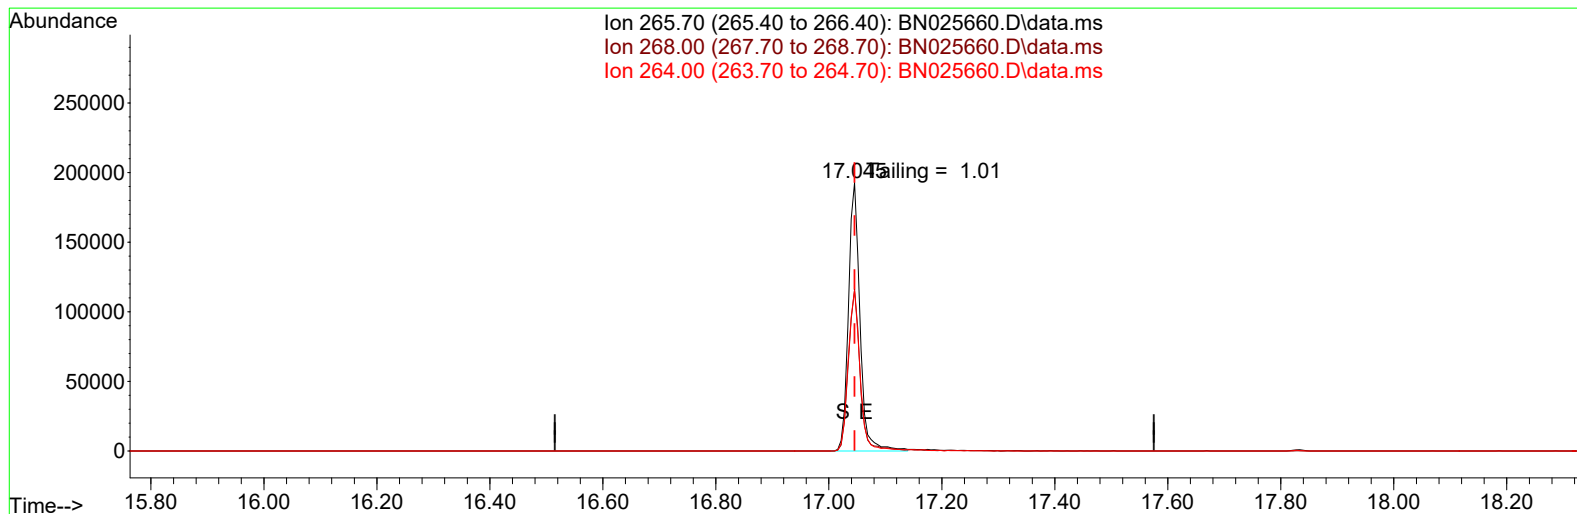

TIC: BN025660.D\data.ms

(70) Pentachlorophenol (C)

17.045min (+ 0.000) 13468.22 ng




response 276393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.25
264.00	61.60	60.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025660.D
Acq On : 28 May 2023 00:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 29 03:16:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

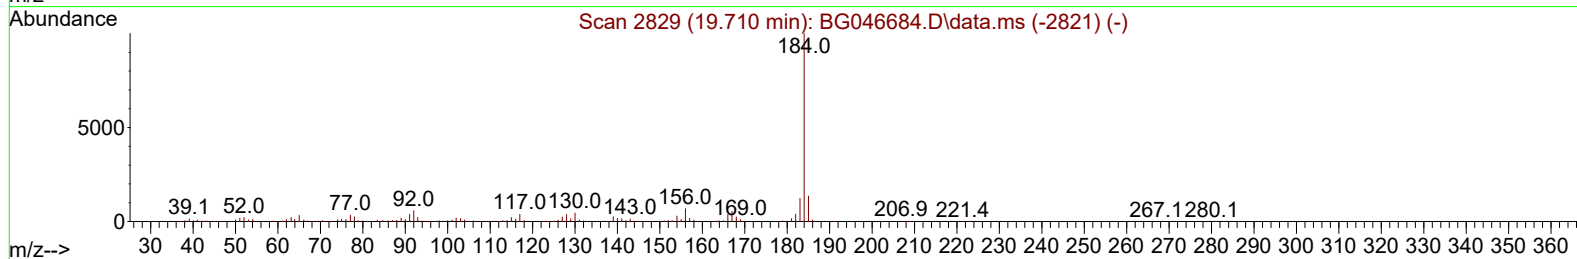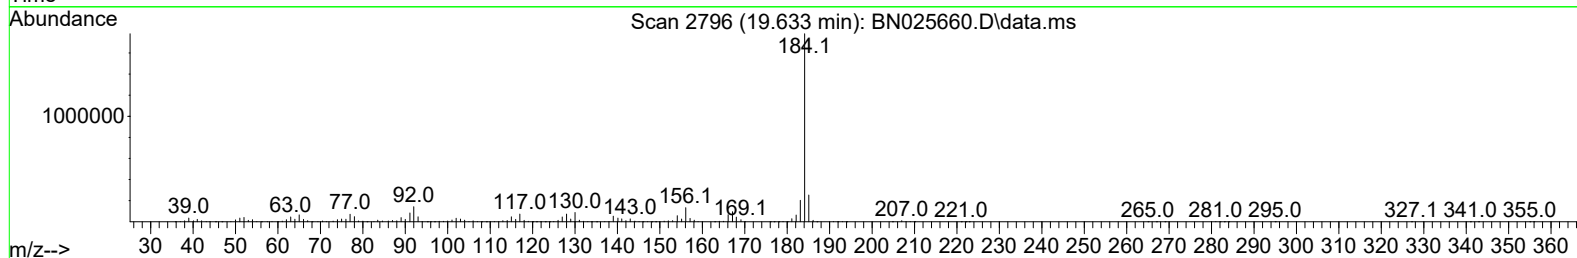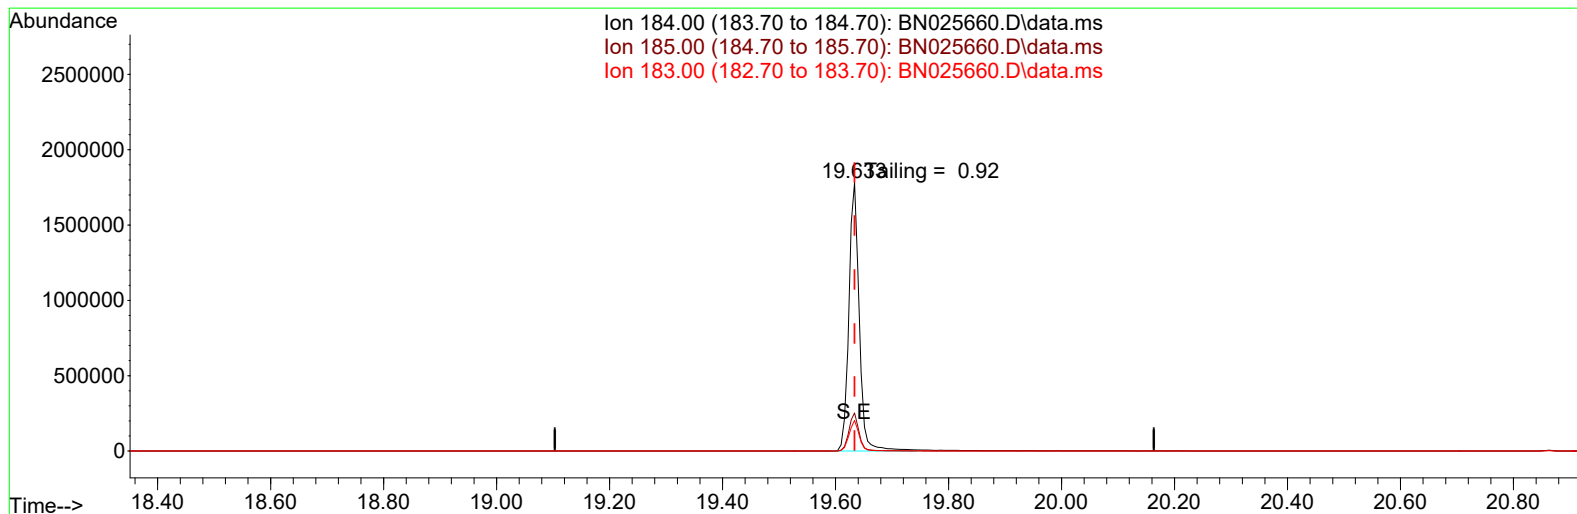

TIC: BN025660.D\data.ms

(77) Benzidine

19.633min (+ 0.000) 0.00 ng

response 2308669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	11.39
0.00	0.00	0.00