
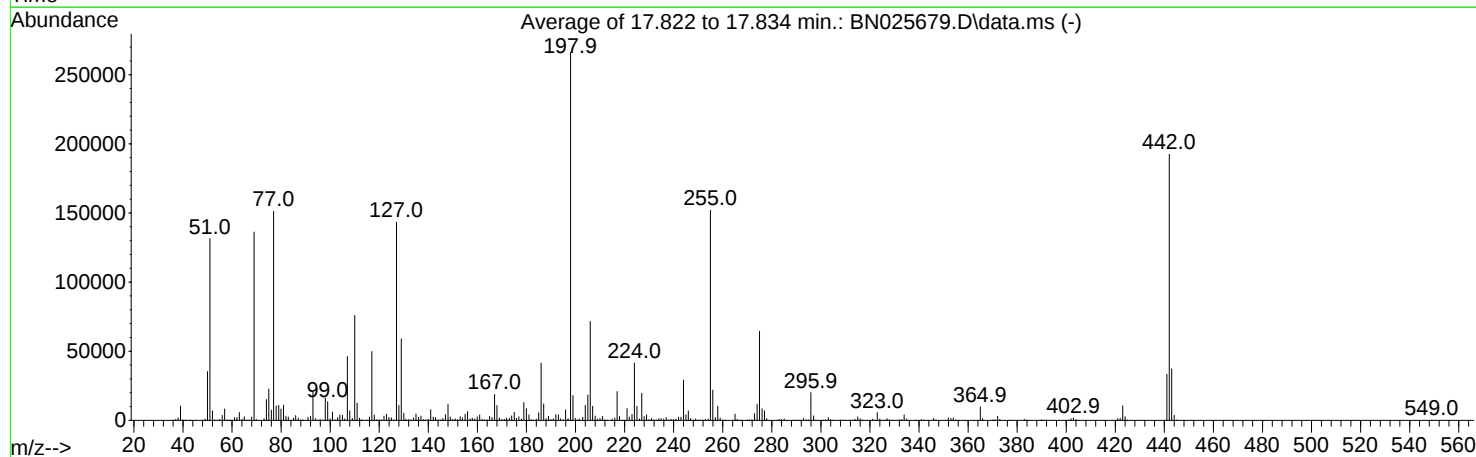


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025679.D
Acq On : 28 May 2023 13:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 29 00:47:45 2023

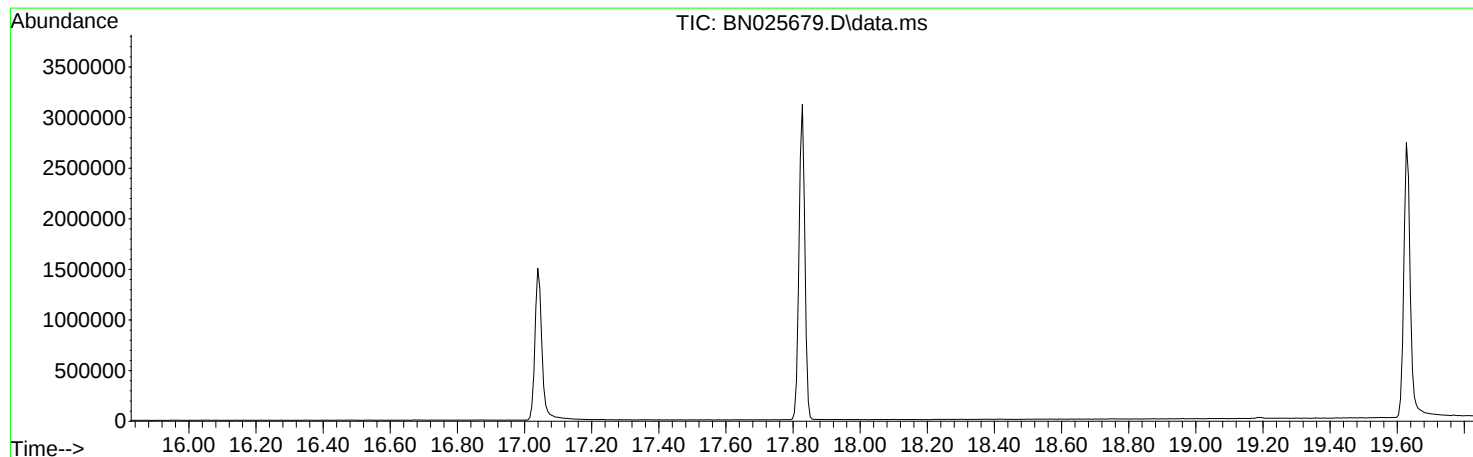

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	131496	PASS
68	69	0.00	2	1.8	2396	PASS
69	198	0.00	100	51.2	136264	PASS
70	69	0.00	2	0.5	662	PASS
127	198	10	80	53.9	143323	PASS
197	198	0.00	2	0.4	1191	PASS
198	198	100	100	100.0	266091	PASS
199	198	5	9	6.8	17983	PASS
275	198	10	60	24.2	64461	PASS
365	198	1	100	3.7	9713	PASS
441	198	0.01	100	12.5	33341	PASS
442	442	50	100	100.0	192533	PASS
443	442	15	24	19.4	37341	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_N	<u>BN025679.D</u>
Compound Name	Response	Retention Time
DDT	679199	20.857
DDD	14669	20.422
DDE	266	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14935	694134	2.15

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025679.D
 Acq On : 28 May 2023 13:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 29 03:17:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 29 03:15:08 2023
 Response via : Initial Calibration

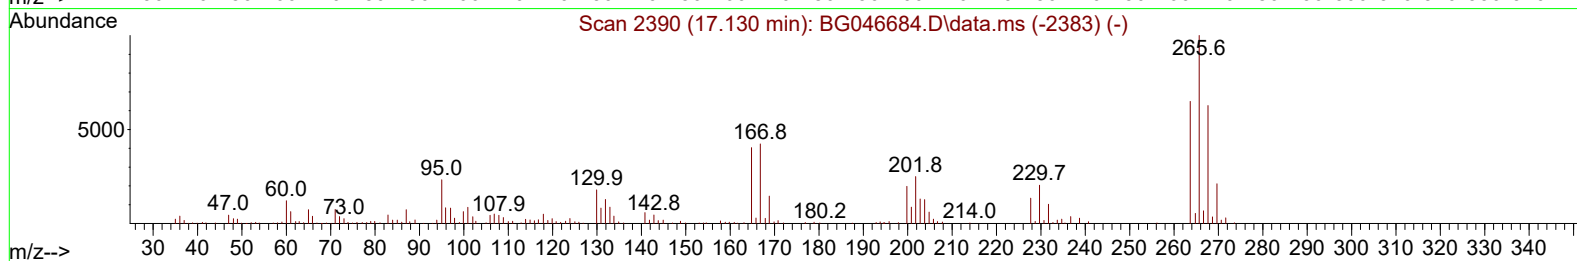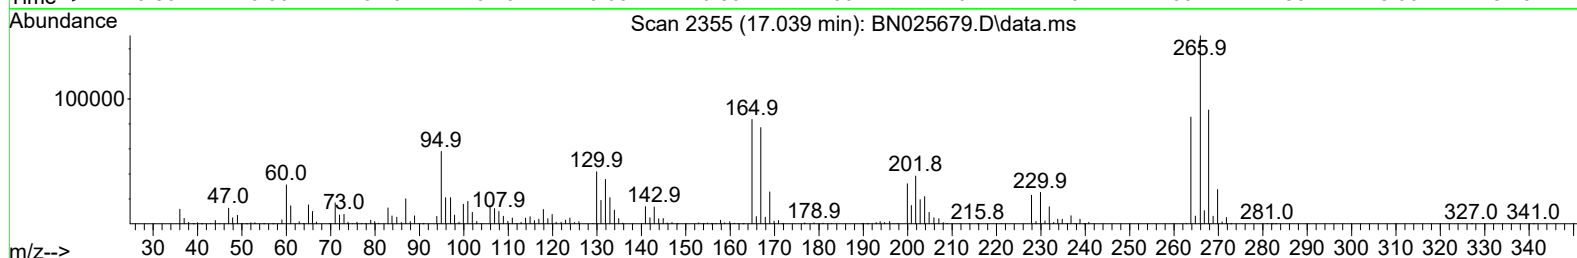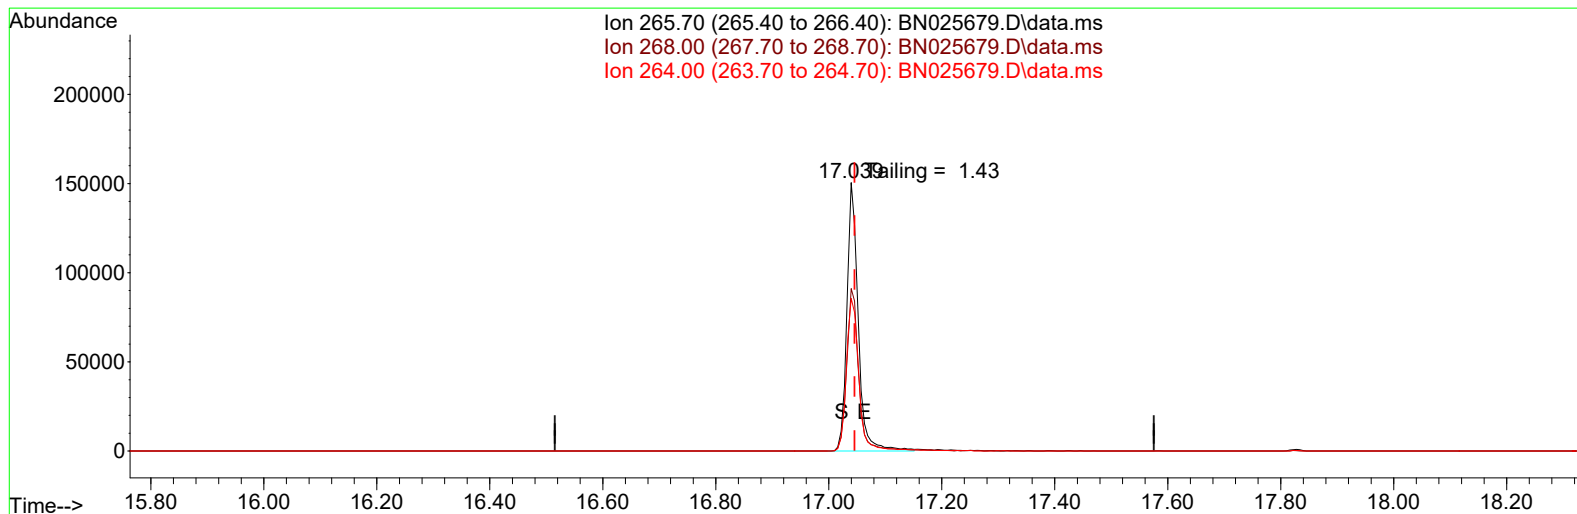

TIC: BN025679.D\data.ms

(70) Pentachlorophenol (C)

17.039min (-0.006) 13409.45 ng




response 208258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.51
264.00	61.60	56.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025679.D
 Acq On : 28 May 2023 13:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 29 03:17:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 29 03:15:08 2023
 Response via : Initial Calibration

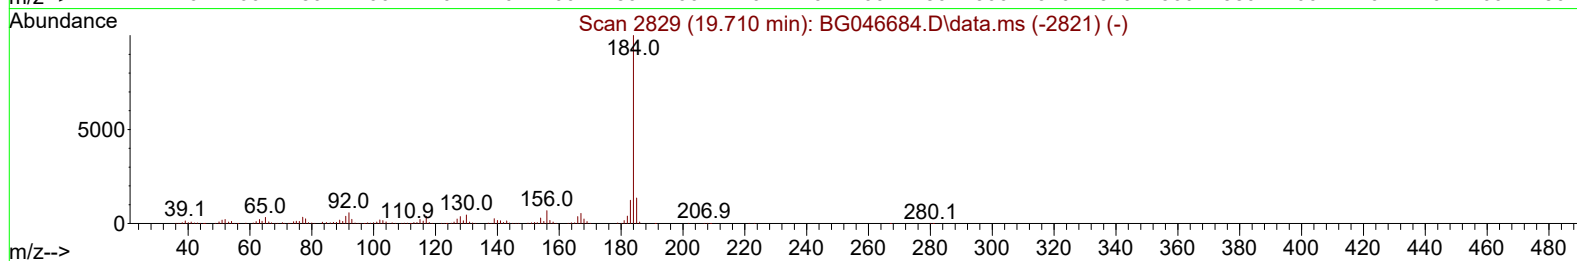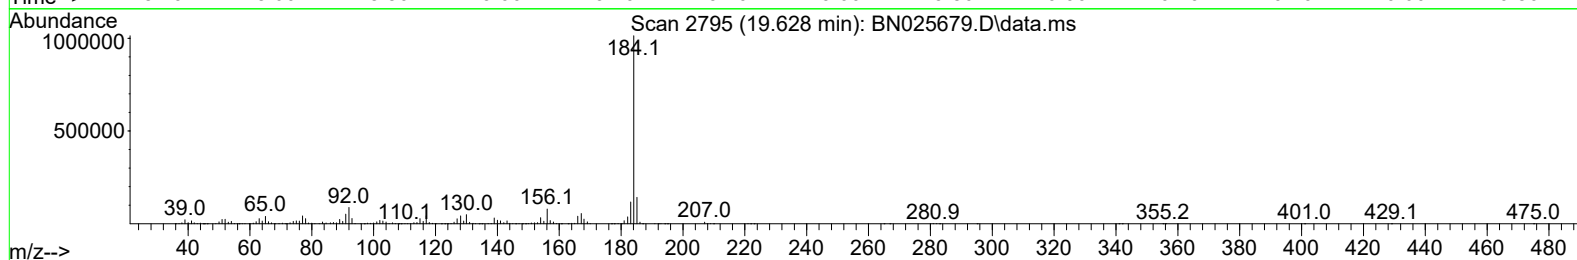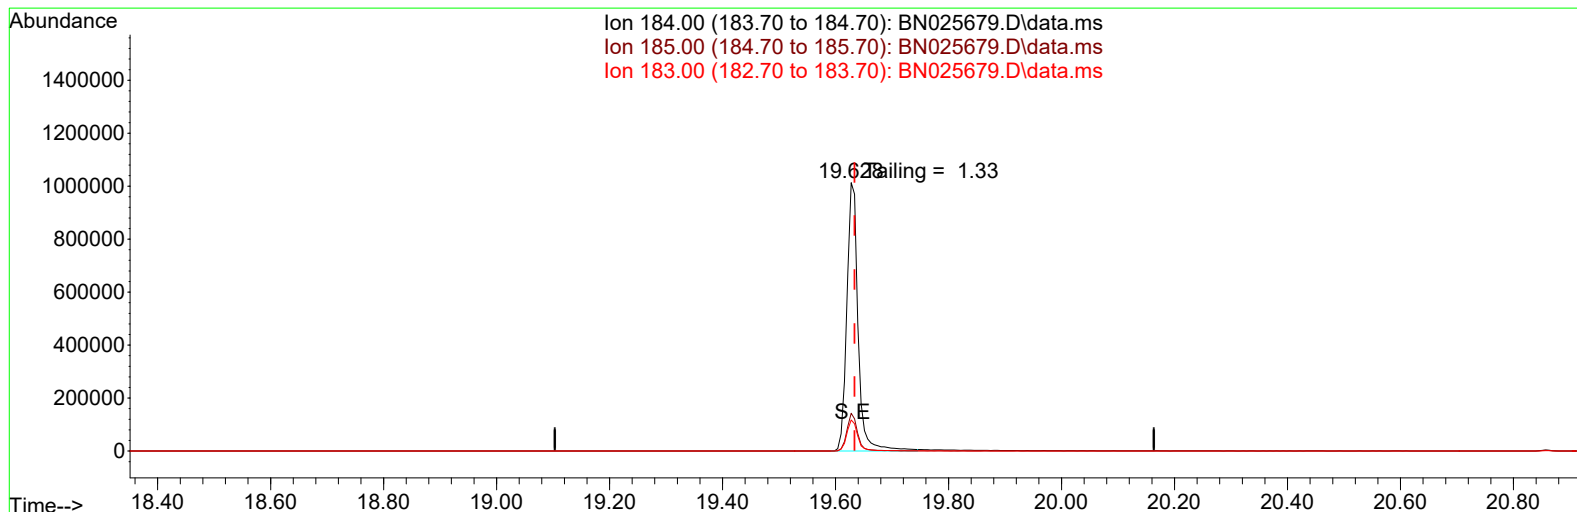

TIC: BN025679.D\data.ms

(77) Benzidine

19.628min (-0.006) 0.00 ng

response 1422064

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.61
0.00	0.00	0.00