


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
 Data File : BN025698.D
 Acq On : 29 May 2023 01:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 29 00:47:45 2023

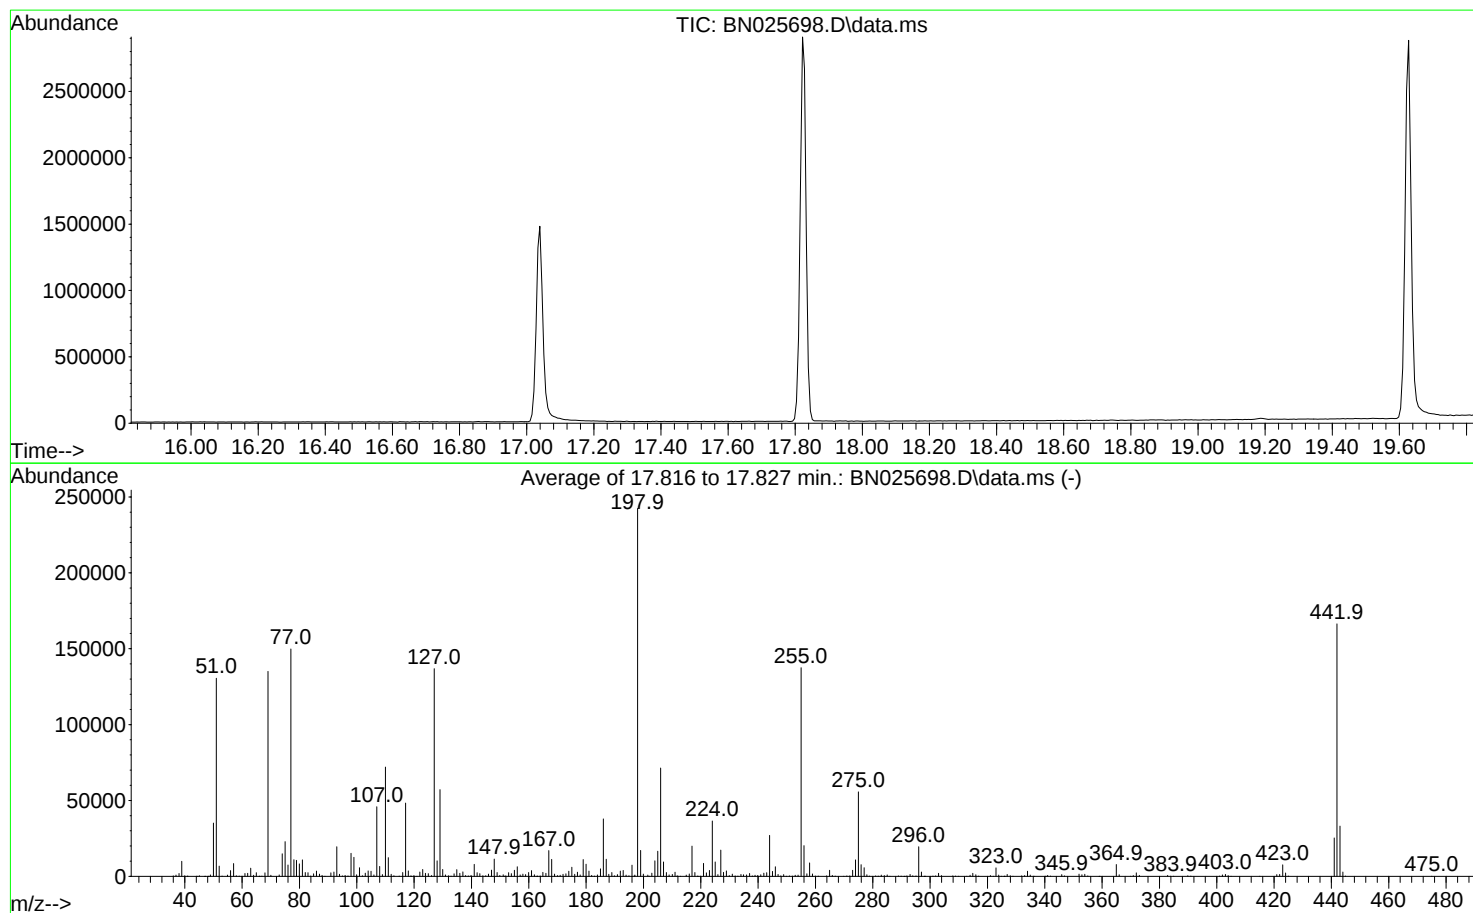

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	130485	PASS
68	69	0.00	2	1.8	2369	PASS
69	198	0.00	100	55.7	135029	PASS
70	69	0.00	2	0.5	714	PASS
127	198	10	80	56.5	136888	PASS
197	198	0.00	2	0.3	809	PASS
198	198	100	100	100.0	242389	PASS
199	198	5	9	7.0	17085	PASS
275	198	10	60	23.0	55651	PASS
365	198	1	100	3.2	7845	PASS
441	198	0.01	100	10.4	25264	PASS
442	442	50	100	100.0	166379	PASS
443	442	15	24	19.9	33152	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_N	<u>BN025698.D</u>
Compound Name	Response	Retention Time
DDT	430422	20.857
DDD	9923	20.416
DDE	0	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9923	440345	2.25

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025698.D
Acq On : 29 May 2023 01:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 29 03:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

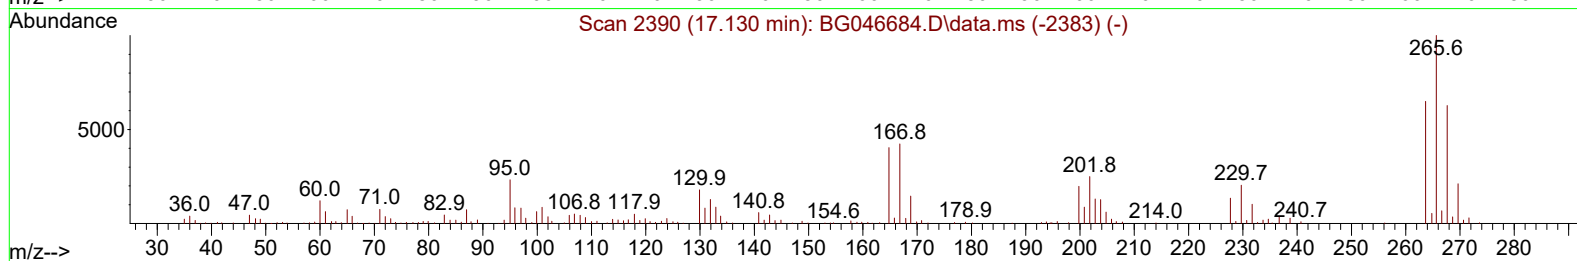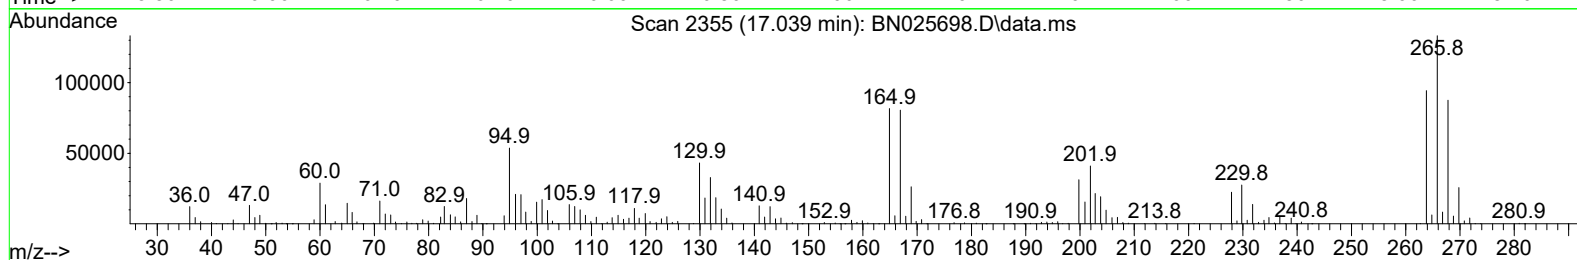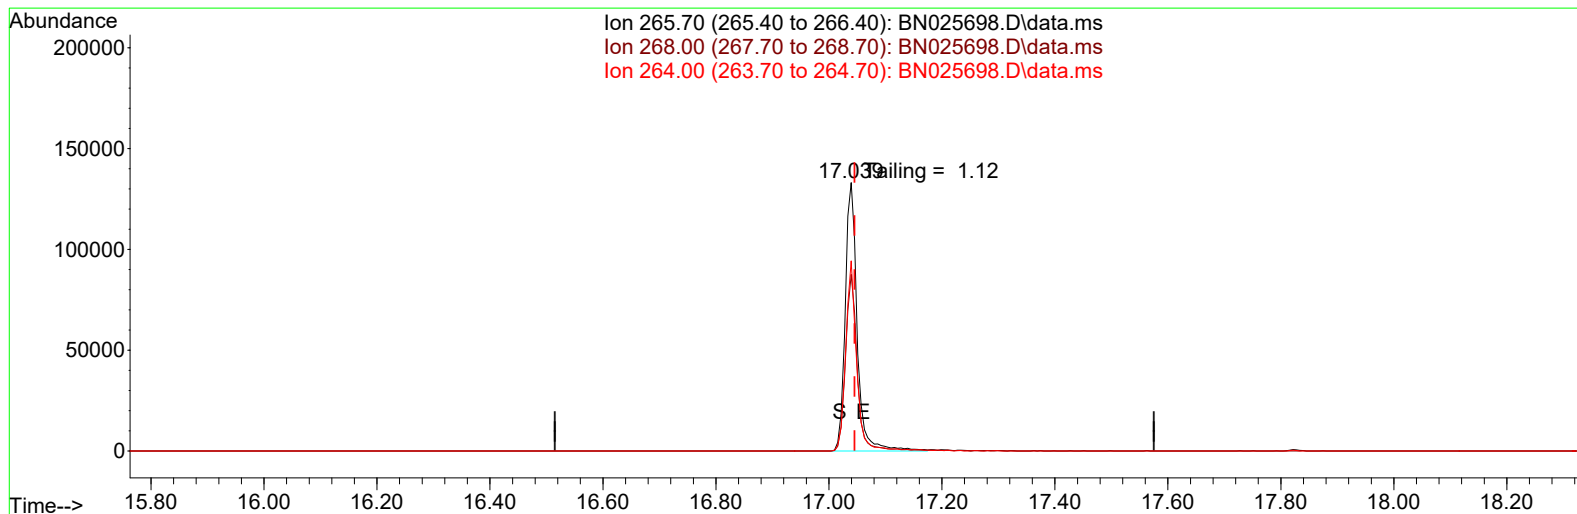

TIC: BN025698.D\data.ms

(70) Pentachlorophenol (C)

17.039min (-0.006) 12331.19 ng




response 196157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.75
264.00	61.60	70.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052623\
Data File : BN025698.D
Acq On : 29 May 2023 01:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 29 03:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 29 03:15:08 2023
Response via : Initial Calibration

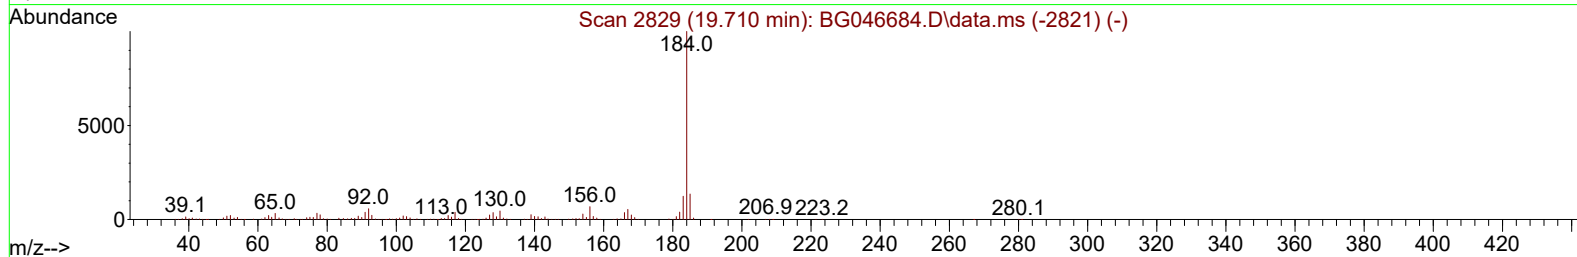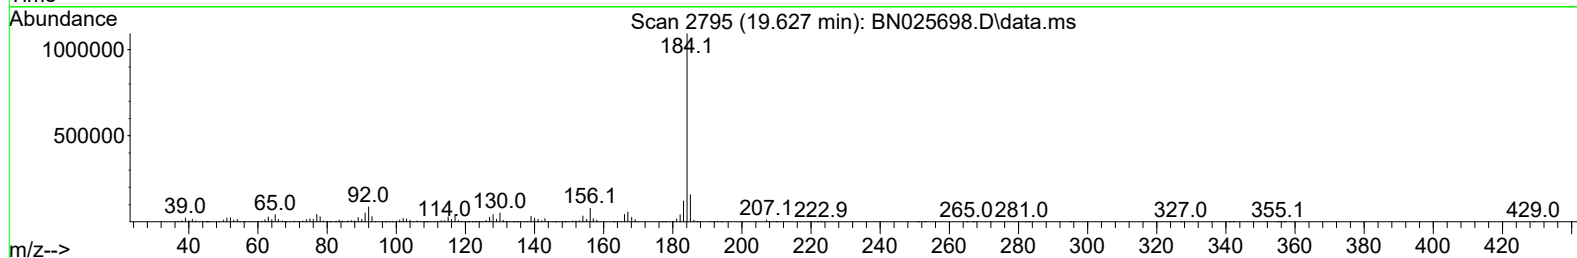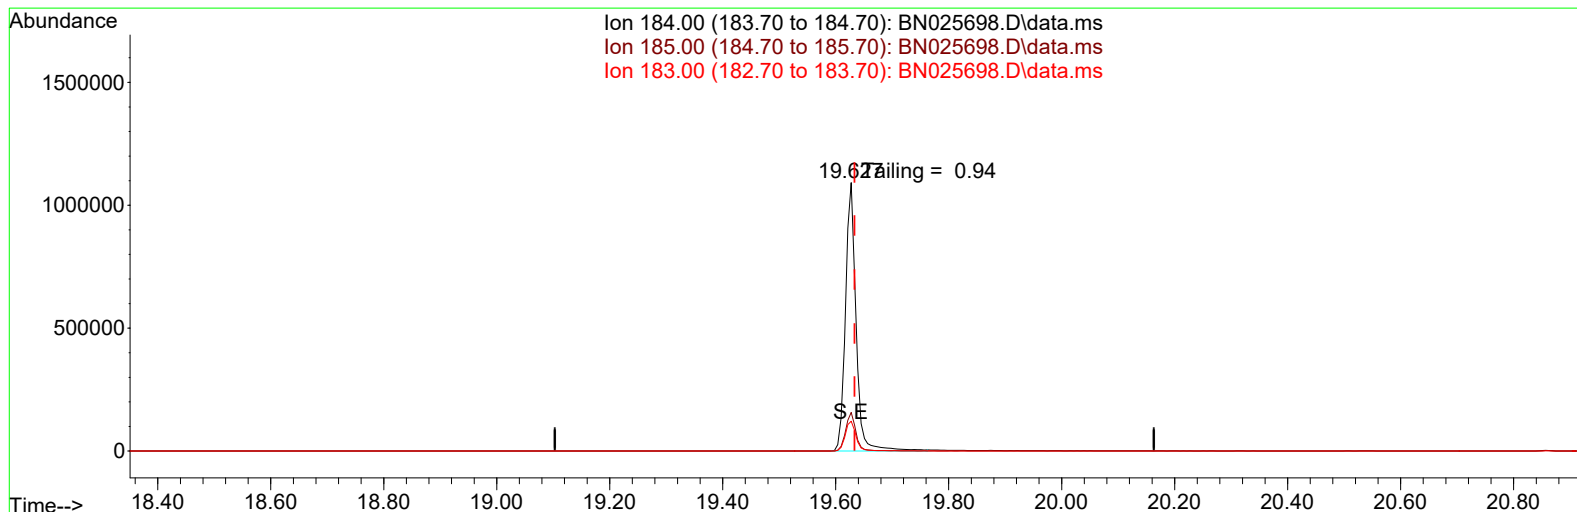

TIC: BN025698.D\data.ms

(77) Benzidine

19.627min (-0.006) 0.00 ng

response 1408458

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	11.10
0.00	0.00	0.00