

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052919\
 Data File : BN005923.D
 Acq On : 29 May 2019 10:59
 Operator : JU/SJ
 Sample : K2924-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4271

Quant Time: May 29 13:13:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 29 02:28:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	357208	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	1654419	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	1013570	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	2383501	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	2494936	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	2852021	20.00	ng/ul	0.02

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	44807	5.52	ng/uL	0.00
5) Phenol-d5	6.89	99	958460	30.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	582741	32.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	743331	30.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	730575	28.59	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	368880	34.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	373242	37.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	719440	30.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	1079901	35.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	2585535	34.60	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	3072367	32.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	445479	32.76	ng/ul	0.00
57) Fluorene-d10	15.36	176	2182921	34.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	277252	28.54	ng/ul	0.00
70) Anthracene-d10	17.22	188	3447960	33.99	ng/ul	0.00
78) Pyrene-d10	19.53	212	4119474	32.69	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.47	264	4443563	34.92	ng/ul	0.02


Target Compounds					Ovalue	
44) Dimethylphthalate	13.83	163	768726	10.293	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052919\
Data File : BN005923.D
Acq On : 29 May 2019 10:59
Operator : JU/SJ
Sample : K2924-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4271

Quant Time: May 29 13:13:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 29 02:28:30 2019
Response via : Initial Calibration

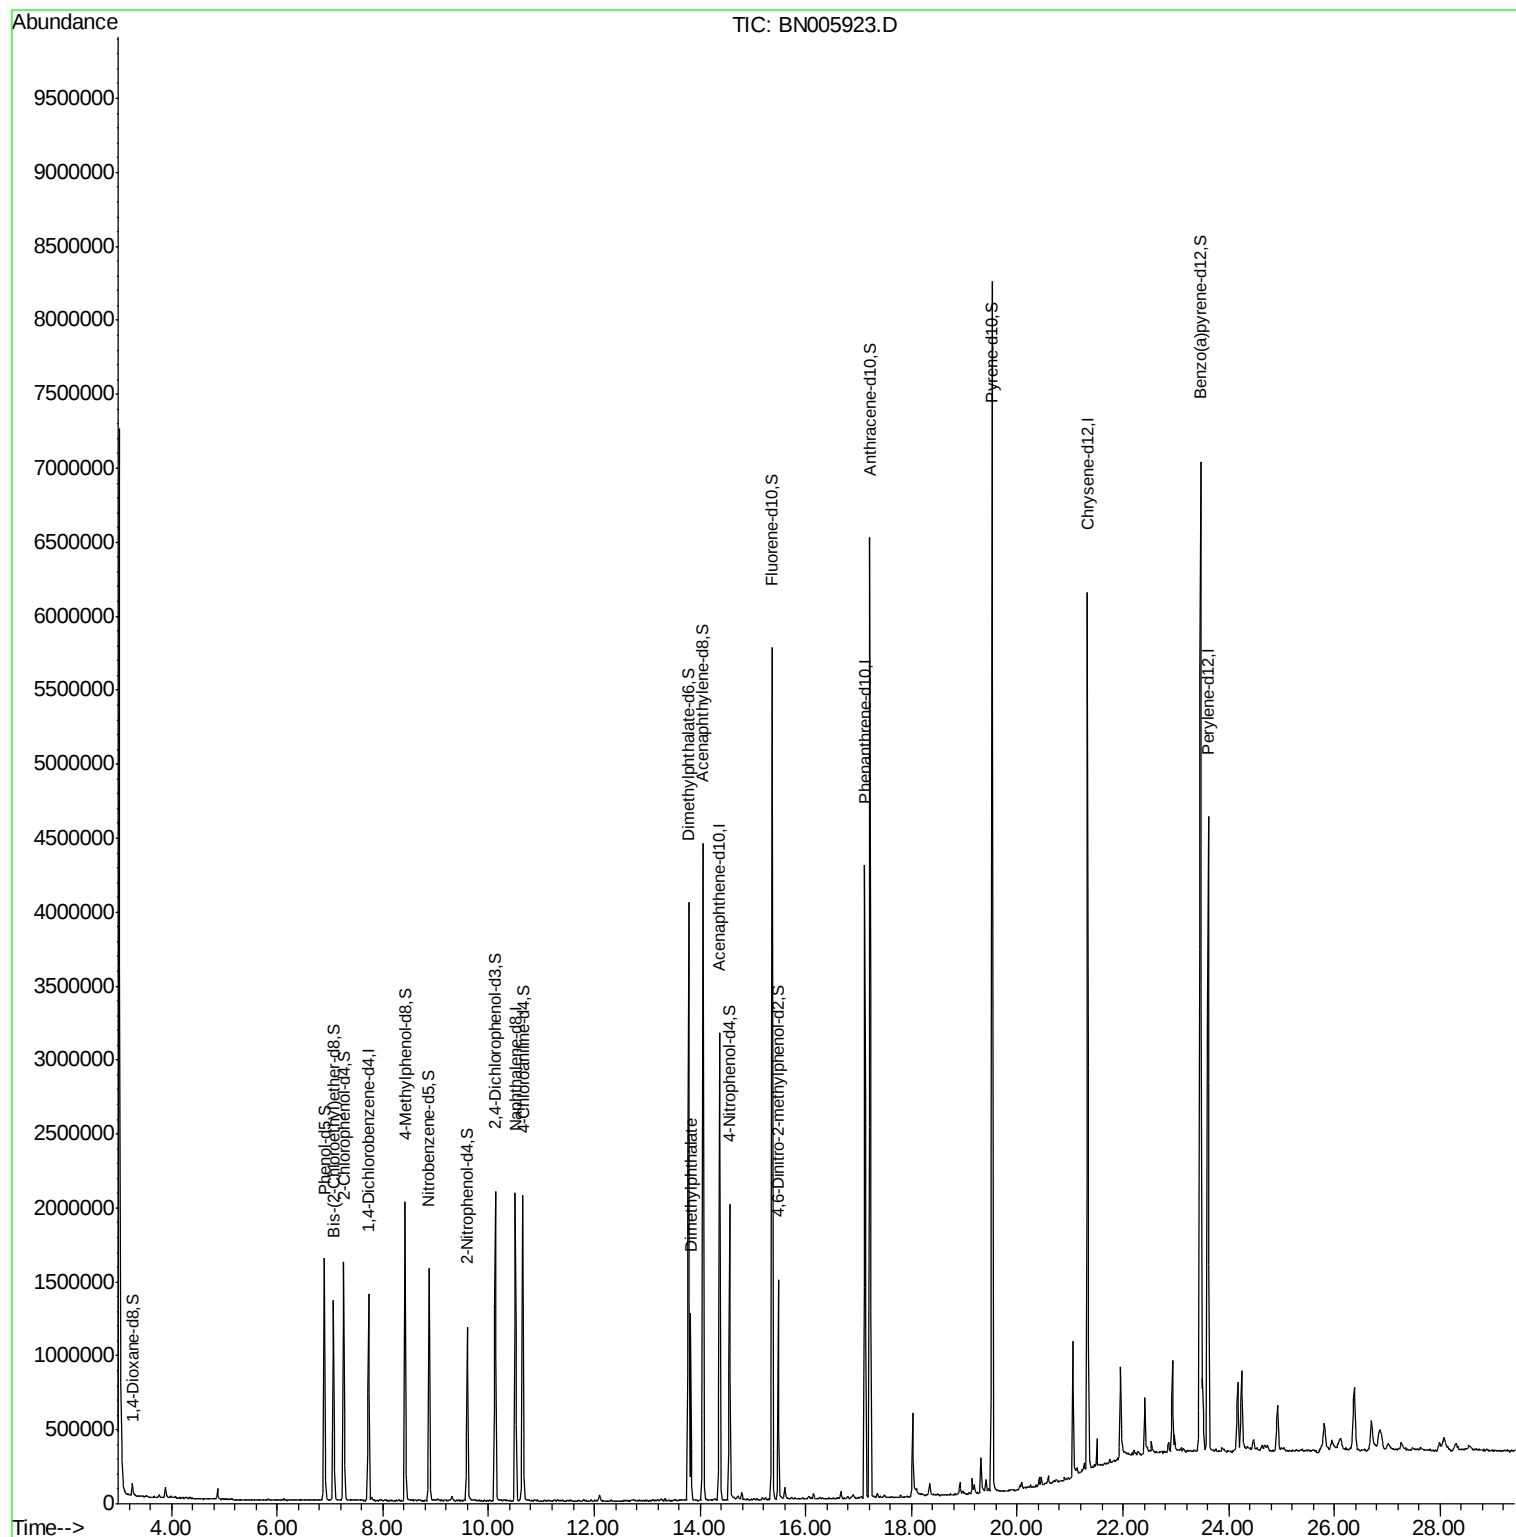

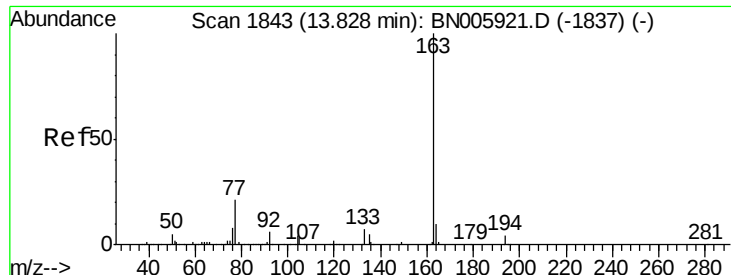

#44

Dimethylphthalate

Concen: 10.293 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.00 min

Lab File: BN005923.D

Acq: 29 May 2019 10:59

Instrument :

BNA_N

ClientSampleId :

A4271


Tot Ion:163 Resp: 768726

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 9.9 8.1 12.1

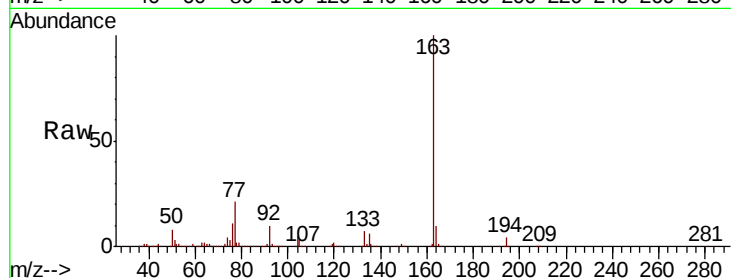

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

