

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052919\
 Data File : BN005934.D
 Acq On : 29 May 2019 17:21
 Operator : JU/SJ
 Sample : K2924-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4273

Quant Time: May 29 18:23:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 29 02:28:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	412807	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	1863642	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	1091328	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	2528630	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	2698032	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	2919284	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	55132	5.88	ng/uL	0.00
5) Phenol-d5	6.89	99	1108266	30.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	673006	32.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	877201	31.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	860781	29.14	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	429214	35.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	442977	39.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	839896	31.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	1204875	34.94	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	2729661	33.93	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	3391748	33.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	450116	30.74	ng/ul	0.00
57) Fluorene-d10	15.36	176	2349928	34.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	266466	25.85	ng/ul	0.00
70) Anthracene-d10	17.22	188	3674431	34.14	ng/ul	0.00
78) Pyrene-d10	19.52	212	4595318	33.72	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	4742782	36.41	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.82	163	948890	11.800	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052919\
Data File : BN005934.D
Acq On : 29 May 2019 17:21
Operator : JU/SJ
Sample : K2924-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4273

Quant Time: May 29 18:23:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 29 02:28:30 2019
Response via : Initial Calibration

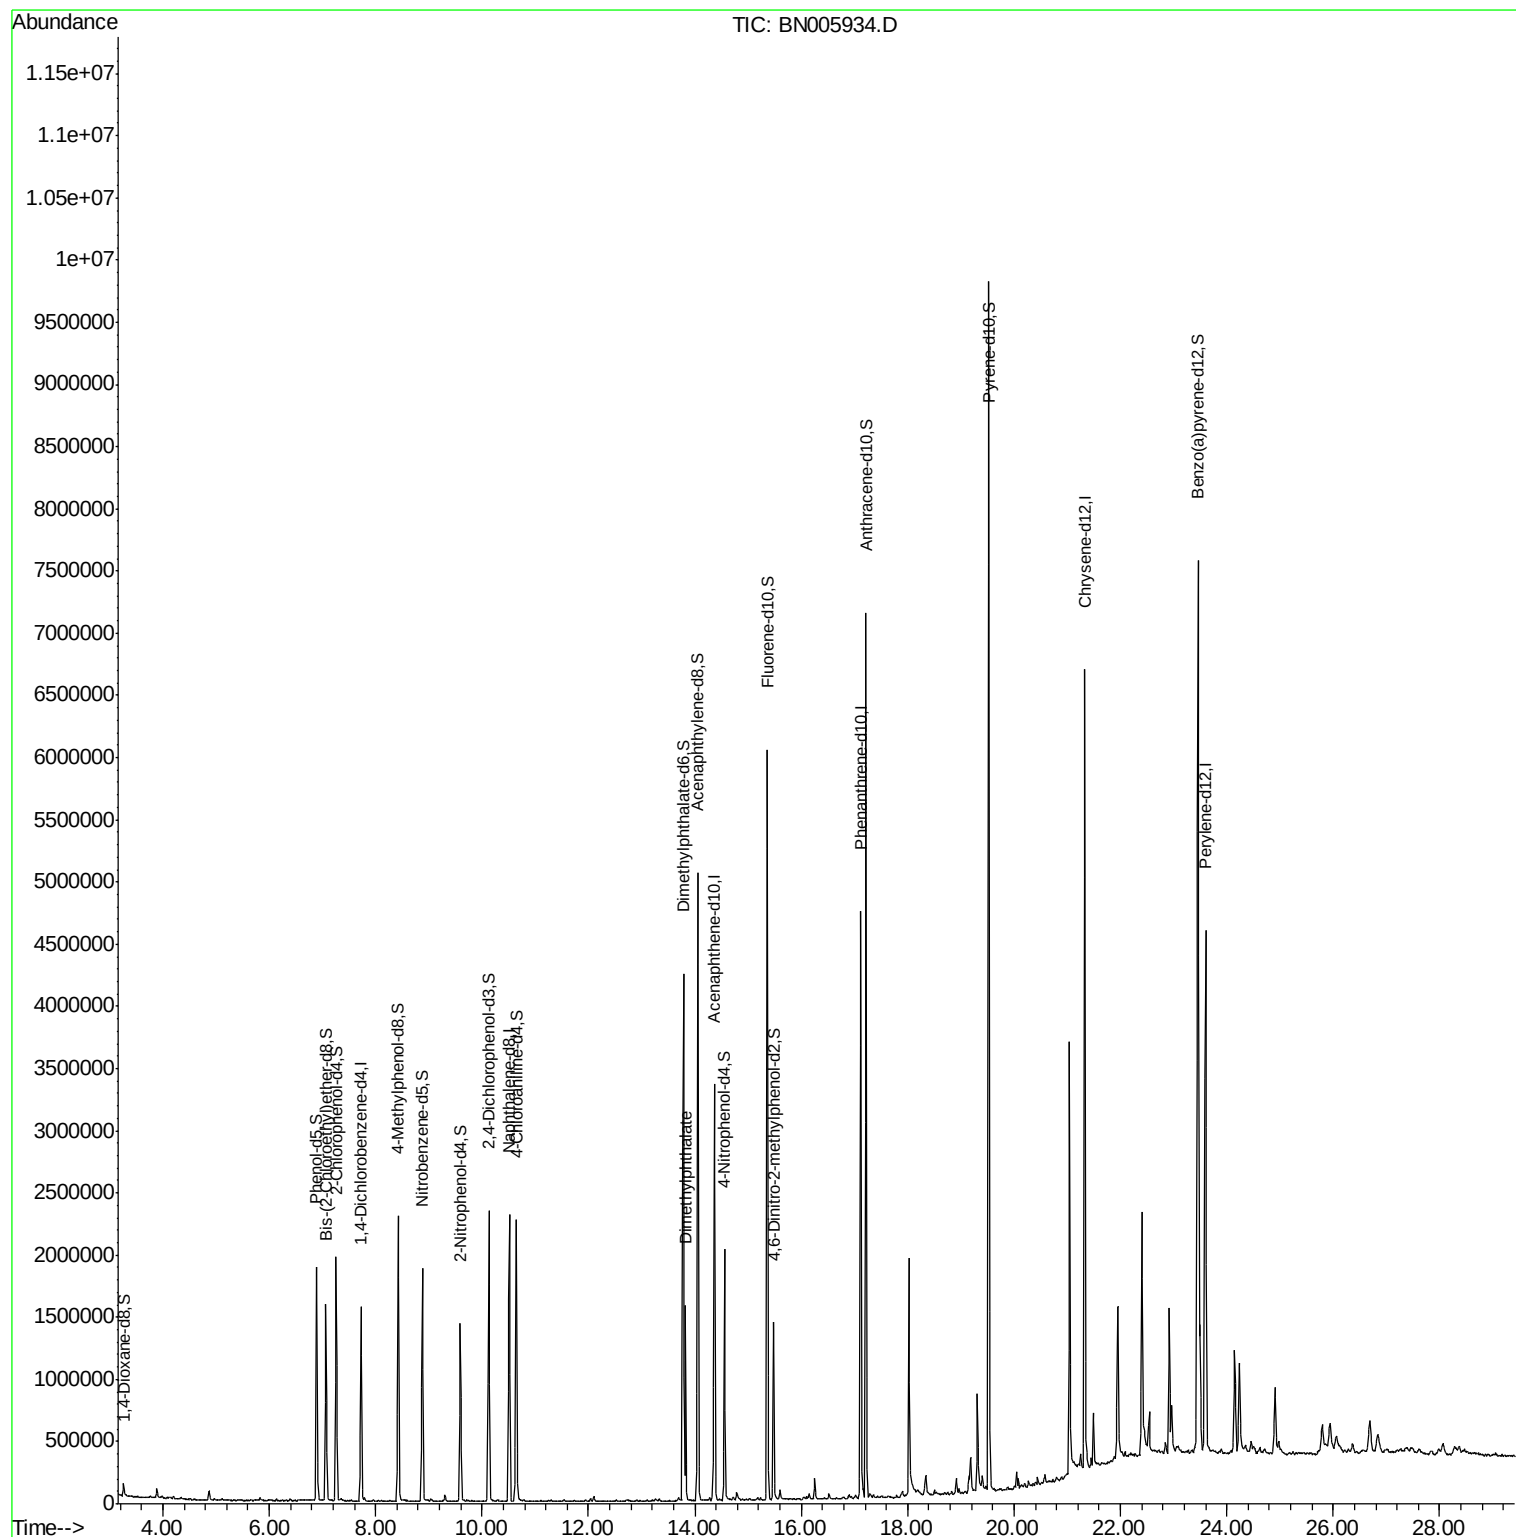

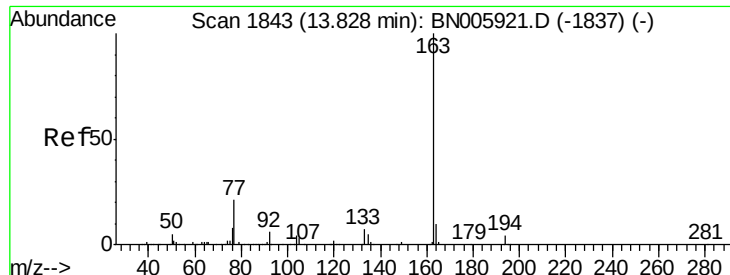

#44

Dimethylphthalate

Concen: 11.800 ng/ul

RT: 13.82 min Scan# 1814

Delta R.T. -0.00 min

Lab File: BN005934.D

Acq: 29 May 2019 17:21

Instrument :

BNA_N

ClientSampleId :

A4273


Tot Ion:163 Resp: 948890

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.3 8.1 12.1

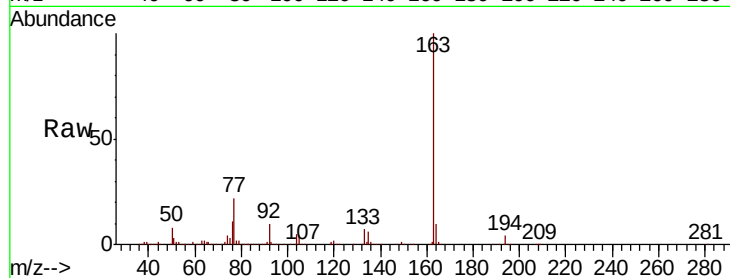

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

