

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN053019\
 Data File : BN005968.D
 Acq On : 30 May 2019 20:23
 Operator : JU/SJ
 Sample : K2853-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 31 01:07:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 30 15:28:35 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	8211	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	31575	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.39	164	16508	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	1831767	0.40	ng/ul	0.10
16) Chrysene-d12	21.46	240	35	0.40	ng/ul	0.11
20) Perylene-d12	23.64	264	20978	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	14570	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
17) Pyrene	19.57	202	1452	7.876	ng/ul#	41
18) Benzo(a)anthracene	21.39	228	1099	7.099	ng/ul#	14
19) Chrysene	21.51	228	79	0.544	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN053019\
Data File : BN005968.D
Acq On : 30 May 2019 20:23
Operator : JU/SJ
Sample : K2853-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 31 01:07:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 15:28:35 2019
Response via : Initial Calibration




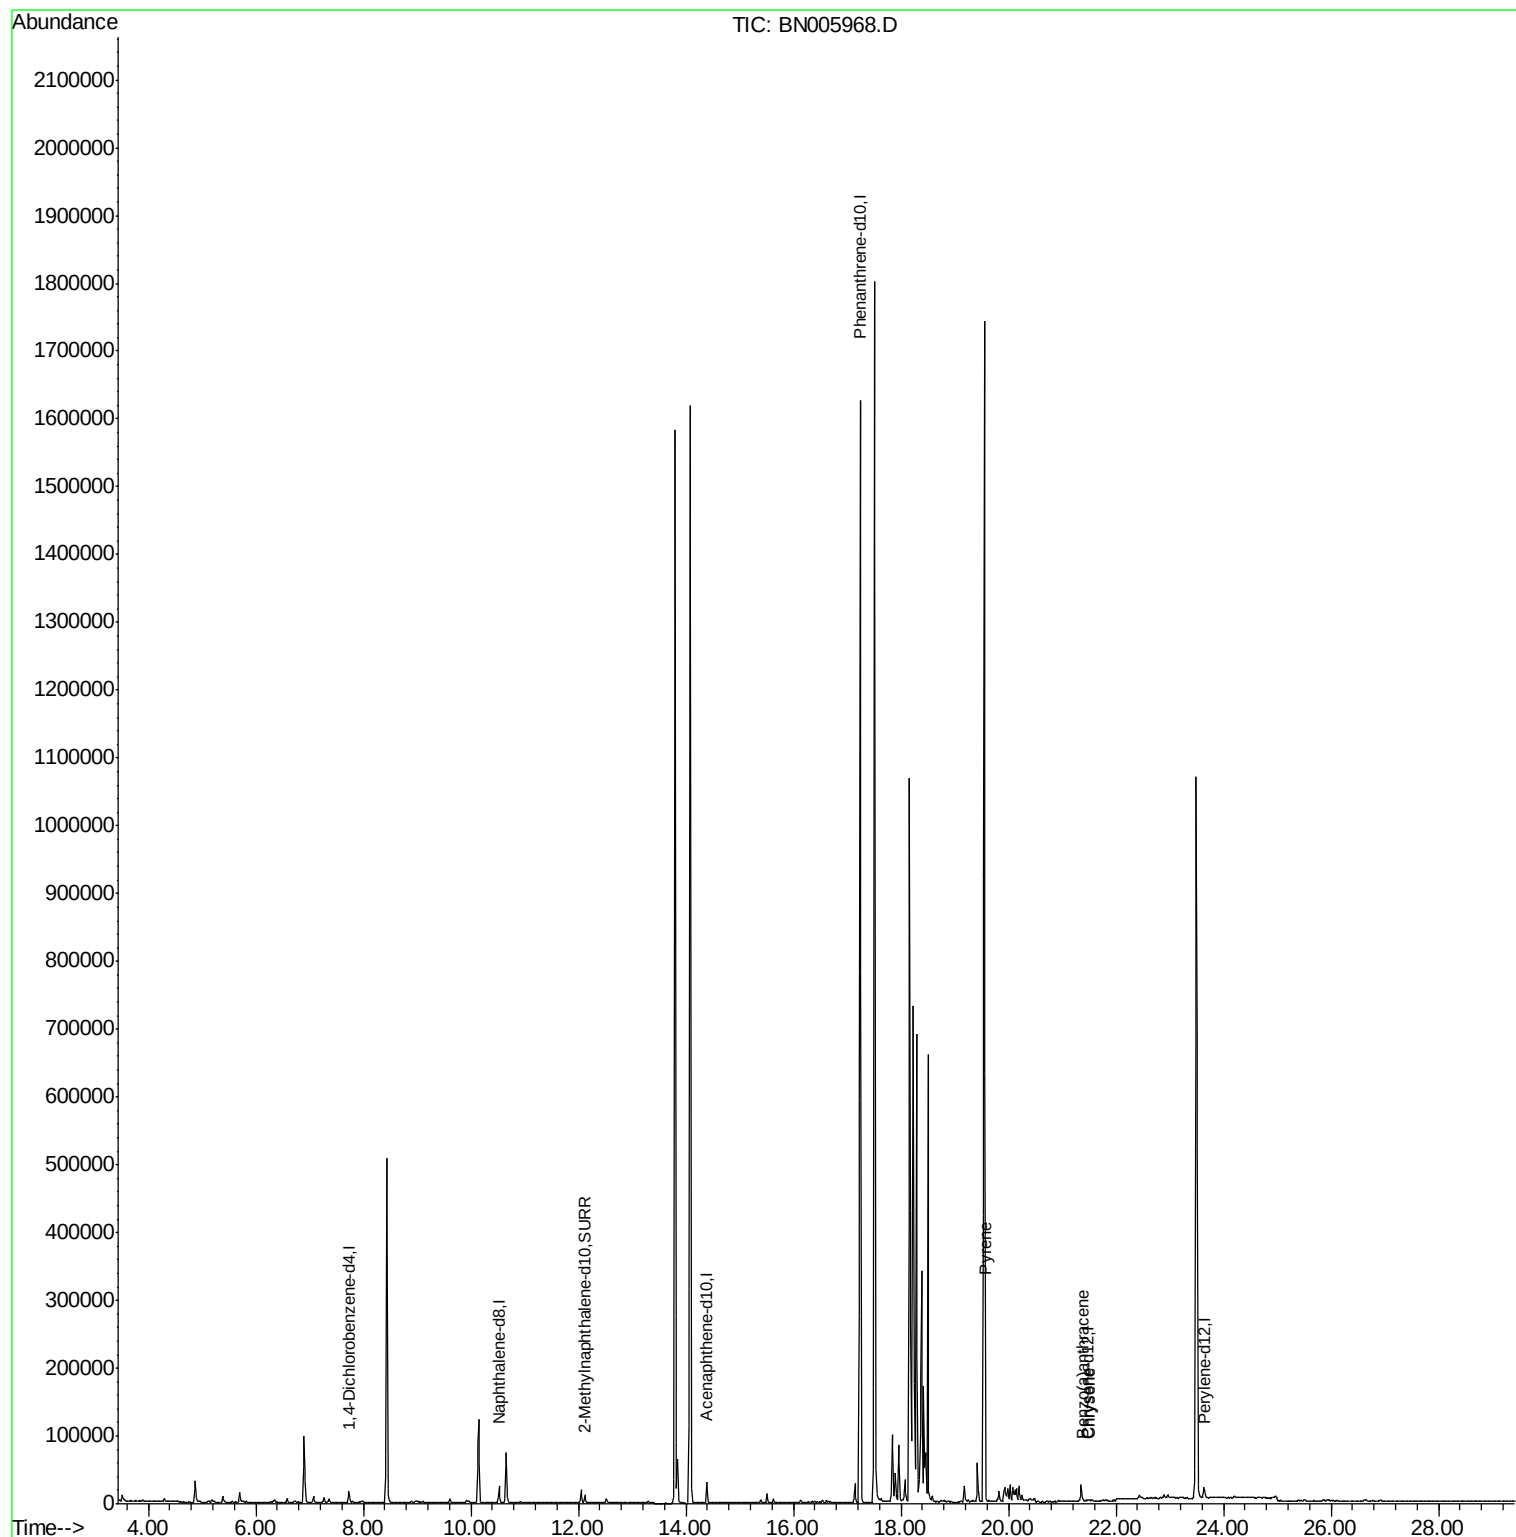


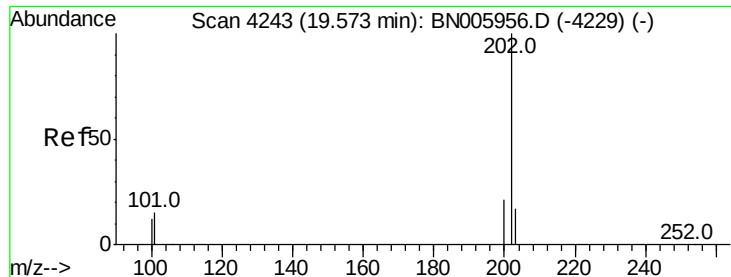

#17
Pvrene
Concen: 7.876 ng/ul
RT: 19.57 min Scan# 4243
Delta R.T. 0.00 min
Lab File: BN005968.D
Acq: 30 May 2019 20:23




Instrument :
BNA_N
ClientSampleId :


Tot Ion:202 Resp: 1452
Ion Ratio Lower Upper
202 100
101 41.3 12.2 18.2#
100 33.8 9.8 14.6#

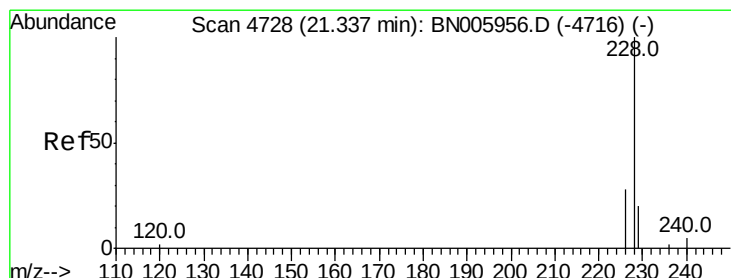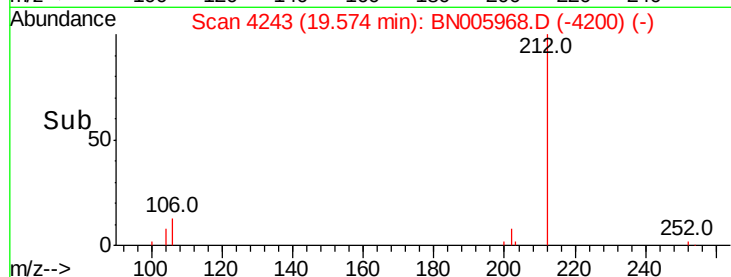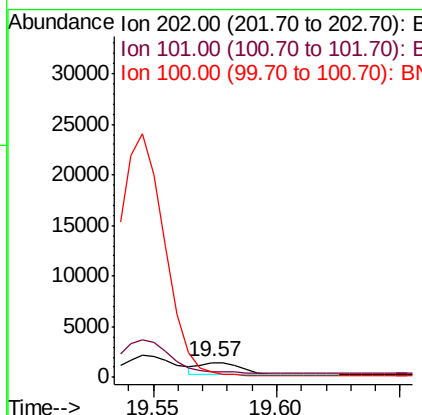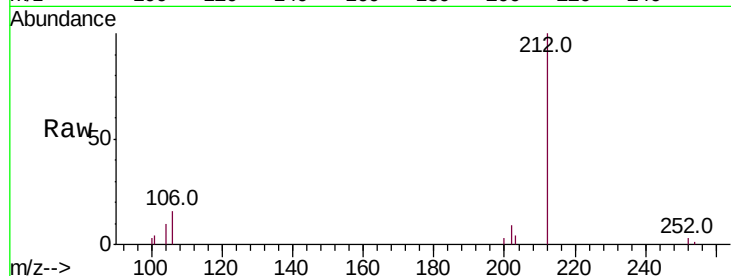

#18
Benzo(a)anthracene
Concen: 7.099 ng/ul
RT: 21.39 min Scan# 4747
Delta R.T. 0.05 min
Lab File: BN005968.D
Acq: 30 May 2019 20:23

Tgt Ion:228 Resp: 1099
Ion Ratio Lower Upper
228 100
229 68.0 16.5 24.7#
226 68.3 22.8 34.2#

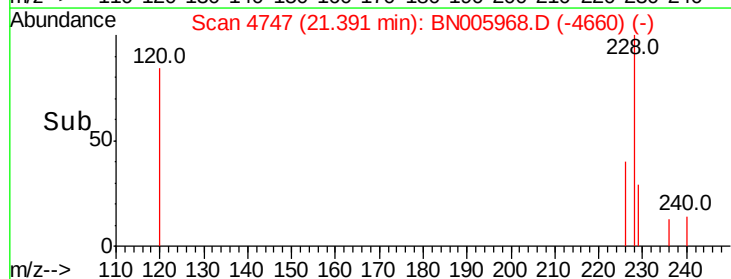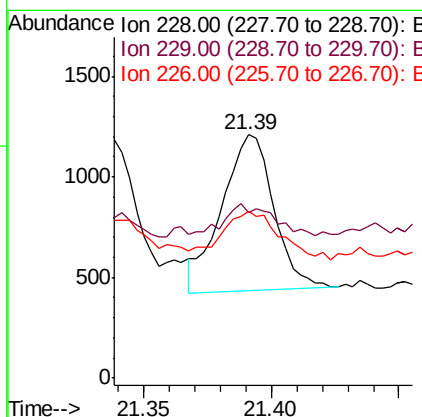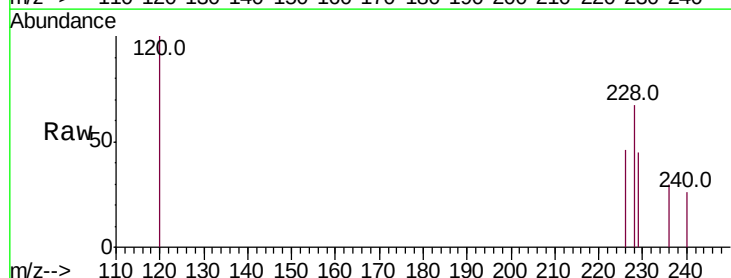

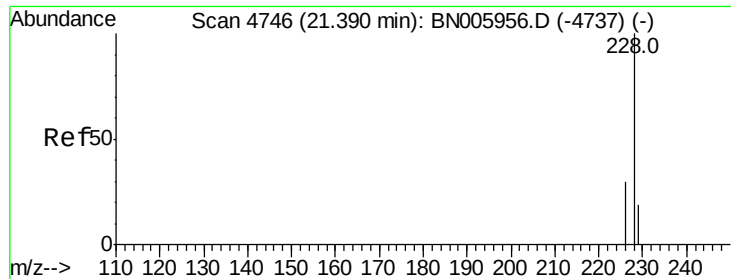

#19

Chrysene

Concen: 0.544 ng/ul

RT: 21.51 min Scan# 4789

Delta R.T. 0.12 min

Lab File: BN005968.D

Acq: 30 May 2019 20:23

Instrument :

BNA_N

ClientSampleId :

Tot Ion:228 Resp: 79

Ion Ratio Lower Upper

228 100

226 128.0 25.0 37.6#

229 142.9 16.3 24.5#

