

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN053119\
 Data File : BN005978.D
 Acq On : 31 May 2019 12:43
 Operator : JU/SJ
 Sample : K2928-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A42B7

Quant Time: May 31 14:17:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 31 14:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	569962	20.00	ng/ul	0.01
18) Naphthalene-d8	10.54	136	2200935	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.41	164	992245	20.00	ng/ul	0.02
61) Phenanthrene-d10	17.16	188	1754693	20.00	ng/ul	0.02
77) Chrysene-d12	21.38	240	1331238	20.00	ng/ul	0.02
85) Perylene-d12	23.69	264	1624166	20.00	ng/ul	0.05

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	50995	3.94	ng/uL	0.01
5) Phenol-d5	6.92	99	1044941	20.68	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.08	67	628368	21.80	ng/ul	0.01
9) 2-Chlorophenol-d4	7.28	132	857722	22.29	ng/ul	0.01
13) 4-Methylphenol-d8	8.45	113	795650	19.51	ng/ul	0.02
19) Nitrobenzene-d5	8.90	128	404248	28.62	ng/ul	0.01
22) 2-Nitrophenol-d4	9.62	143	403301	30.65	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.16	165	730980	23.53	ng/ul	0.02
29) 4-Chloroaniline-d4	10.67	131	391054	9.60	ng/ul	0.01
43) Dimethylphthalate-d6	13.81	166	1932468	26.42	ng/ul	0.02
46) Acenaphthylene-d8	14.09	160	2280209	24.92	ng/ul	0.02
51) 4-Nitrophenol-d4	14.61	143	232235	17.45	ng/ul	0.02
57) Fluorene-d10	15.40	176	1538310	25.08	ng/ul	0.02
62) 4,6-Dinitro-2-methylphenol	15.54	200	40432	5.65	ng/ul	0.03
70) Anthracene-d10	17.26	188	1899856	25.44	ng/ul	0.02
78) Pyrene-d10	19.56	212	1731614	25.76	ng/ul	0.02
89) Benzo(a)pyrene-d12	23.55	264	1722991	23.77	ng/ul	0.05

Target Compounds


					Ovalue	
44) Dimethylphthalate	13.85	163	605297	8.279	ng/ul	99
69) Phenanthrene	17.20	178	499787	5.749	ng/ul	100
71) Anthracene	17.29	178	138636	1.571	ng/ul	97
76) Fluoranthene	19.23	202	766686	8.261	ng/ul	98
79) Pyrene	19.59	202	640151	7.591	ng/ul	97
82) Benzo(a)anthracene	21.36	228	333335	3.983	ng/ul#	85
83) Bis(2-ethylhexyl)phthalate	21.29	149	146043	2.659	ng/ul#	85
84) Chrysene	21.42	228	315841	4.047	ng/ul#	85
87) Benzo(b)fluoranthene	23.00	252	413793	4.536	ng/ul#	61
90) Benzo(a)pyrene	23.59	252	289886	3.370	ng/ul#	56
91) Indeno(1,2,3-cd)pyrene	26.02	276	205288	2.034	ng/ul#	71
93) Benzo(g,h,i)perylene	26.72	276	187940	2.211	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN053119\
Data File : BN005978.D
Acq On : 31 May 2019 12:43
Operator : JU/SJ
Sample : K2928-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A42B7

Quant Time: May 31 14:17:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 31 14:10:13 2019
Response via : Initial Calibration

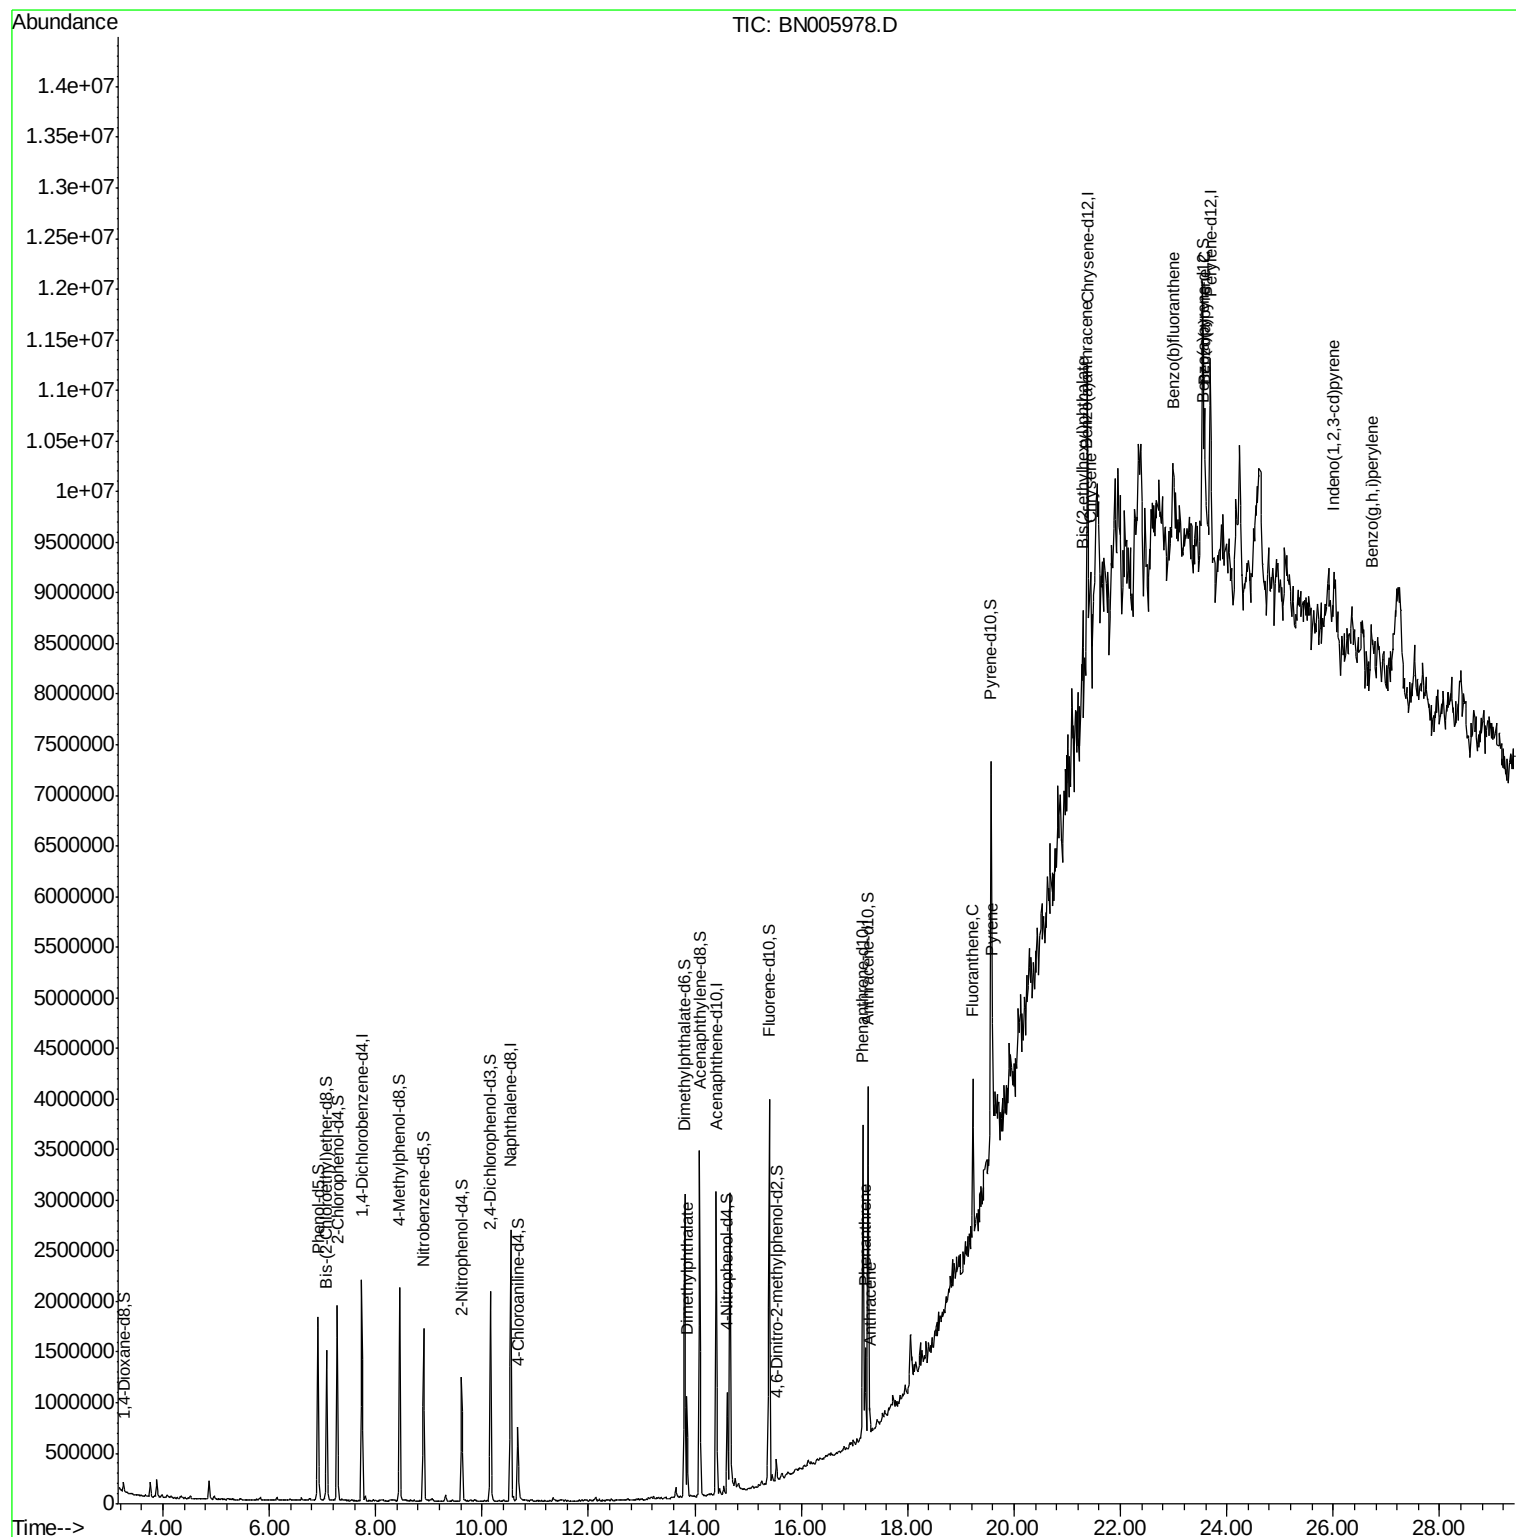

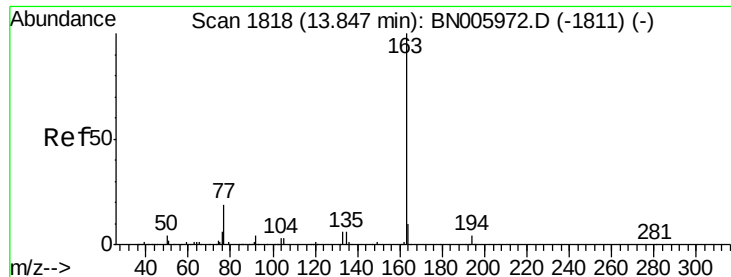

#44

Dimethylphthalate

Concen: 8.279 ng/ul

RT: 13.85 min Scan# 1819

Delta R.T. 0.01 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43

Instrument :

BNA_N

ClientSampleId :

A42B7


Tot Ion:163 Resp: 605297

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0




164 10.6 8.1 12.1

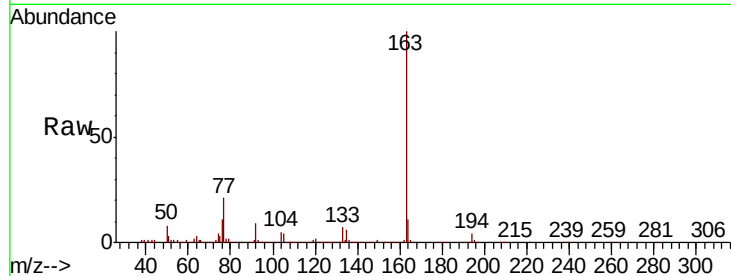

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

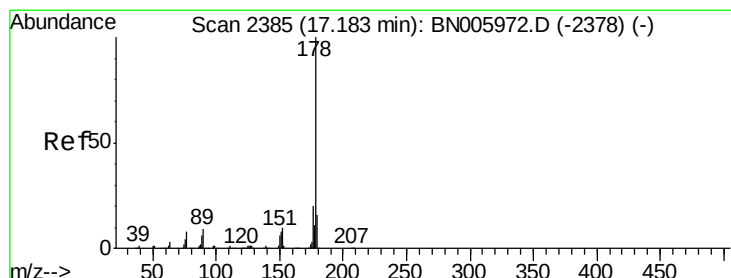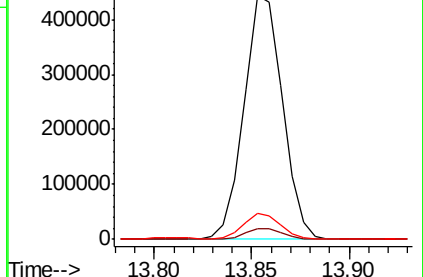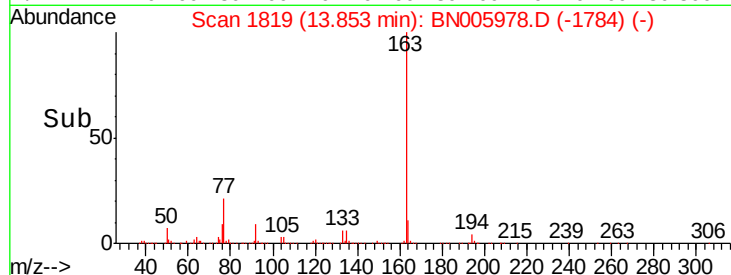

#69

Phenanthrene

Concen: 5.749 ng/ul

RT: 17.20 min Scan# 2388

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43


Tgt Ion:178 Resp: 499787

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.4



176 18.7 15.1 22.7

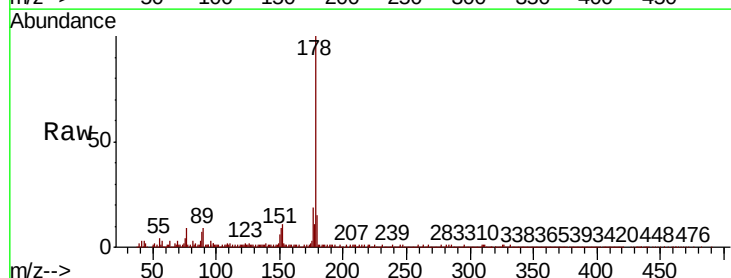


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

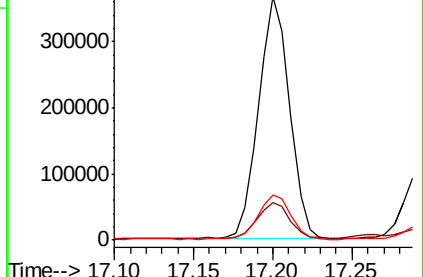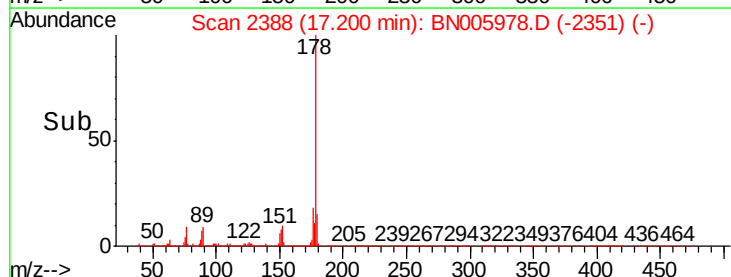

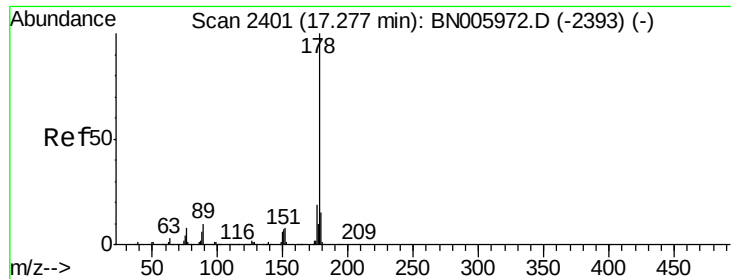

#71

Anthracene

Concen: 1.571 ng/ul

RT: 17.29 min Scan# 2404

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43

Instrument :

BNA_N

ClientSampleId :

A42B7


Tot Ion:178 Resp: 138636

Ion Ratio Lower Upper

178 100

179 17.2 12.3 18.5




176 19.6 15.1 22.7

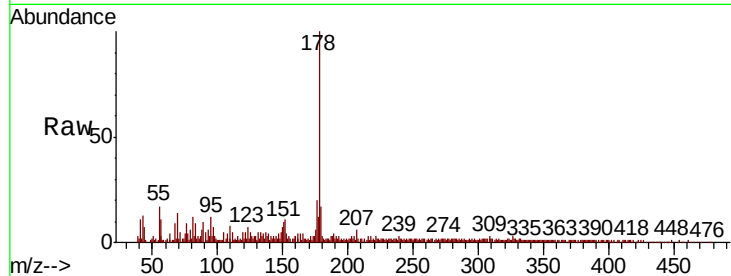

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

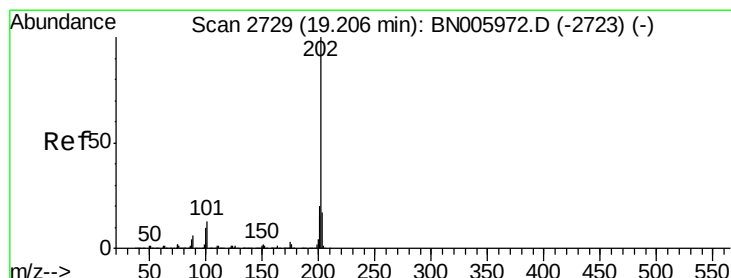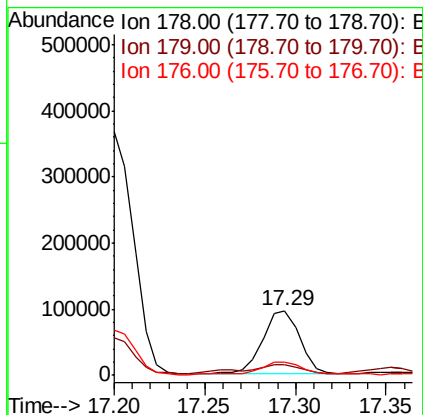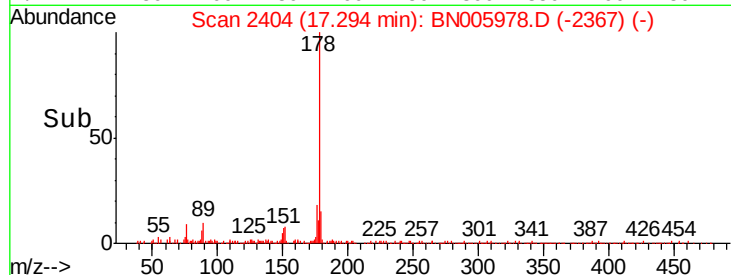

#76

Fluoranthene

Concen: 8.261 ng/ul

RT: 19.23 min Scan# 2733

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43


Tgt Ion:202 Resp: 766686

Ion Ratio Lower Upper

202 100

101 11.4 8.6 12.8



100 8.7 6.3 9.5

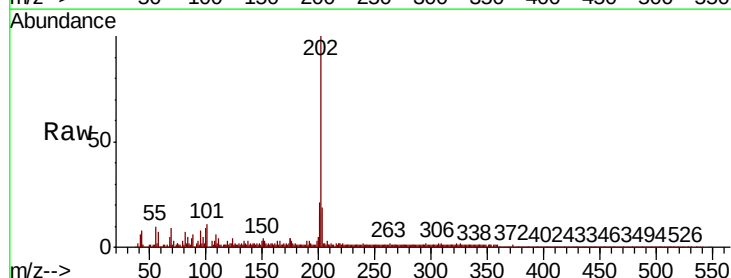


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

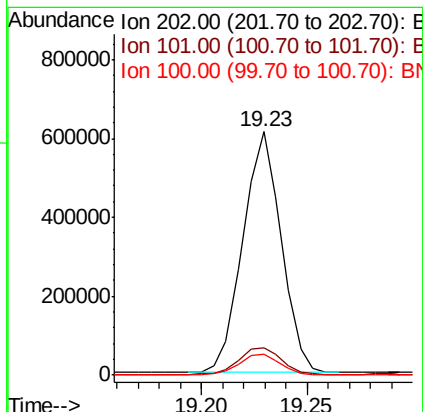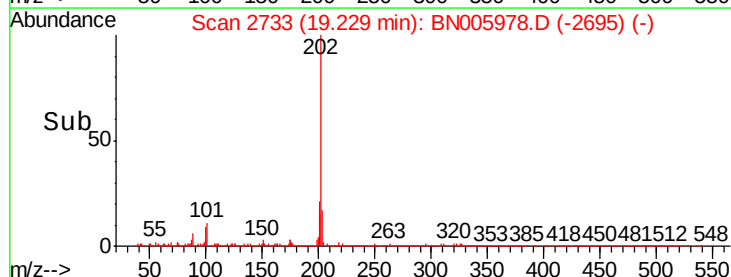

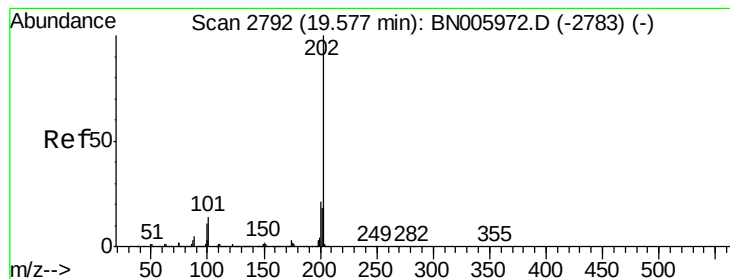

#79

Pvrene

Concen: 7.591 ng/ul

RT: 19.59 min Scan# 2795

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43

Instrument :

BNA_N

ClientSampleId :

A42B7


Tot Ion:202 Resp: 640151

Ion Ratio Lower Upper

202 100

101 13.8 10.3 15.5




100 11.5 7.9 11.9

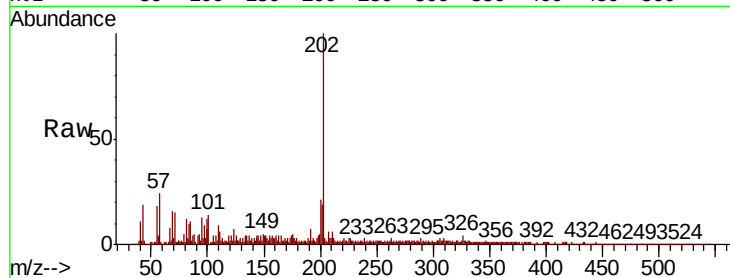

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

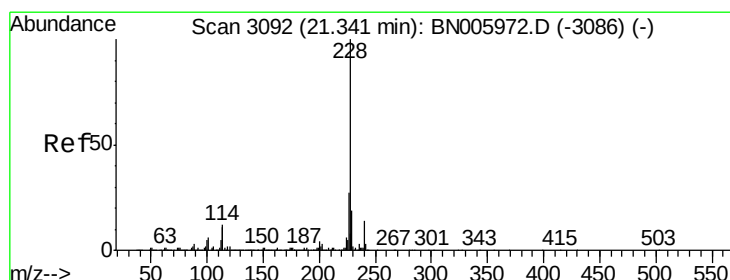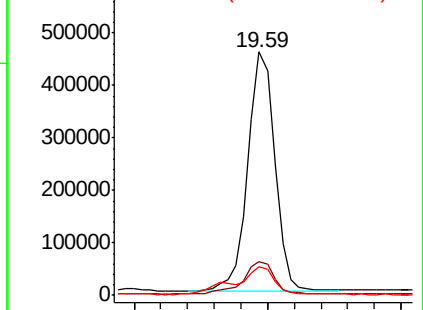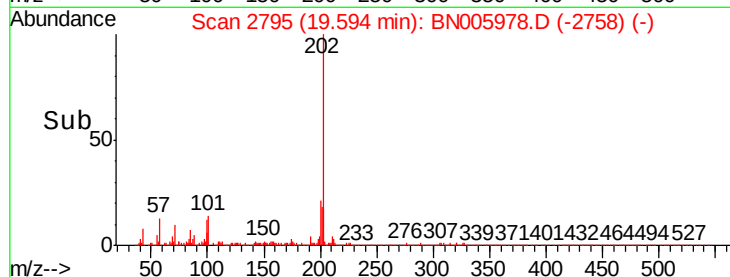

#82

Benzo(a)anthracene

Concen: 3.983 ng/ul

RT: 21.36 min Scan# 3096

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43


Tgt Ion:228 Resp: 333335

Ion Ratio Lower Upper

228 100

229 28.5 15.8 23.6#



226 32.8 21.4 32.2#

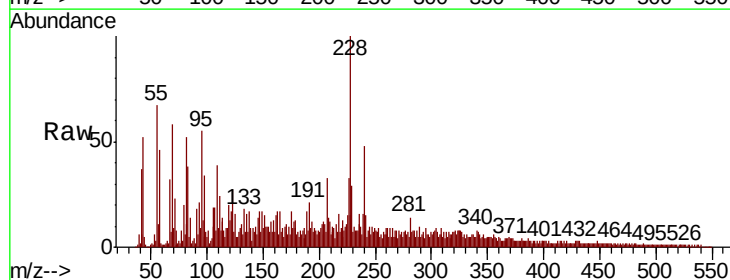


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

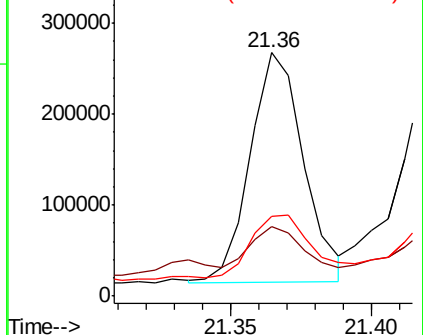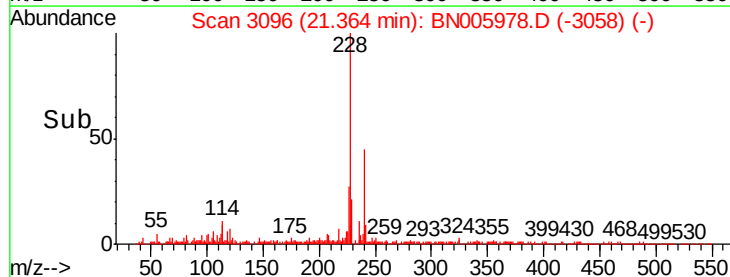

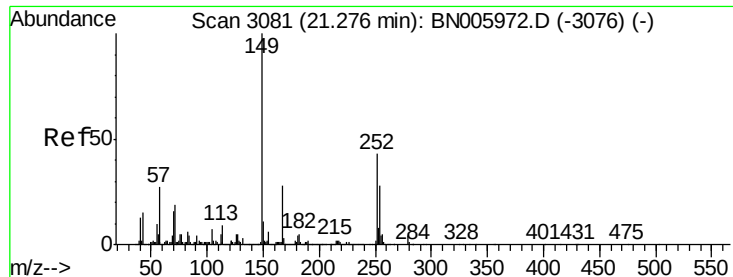

#83

Bis(2-ethylhexyl)phthalate

Concen: 2.659 ng/ul

RT: 21.29 min Scan# 3084

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43

Instrument :

BNA_N

ClientSampleId :

A42B7





Tot Ion:149 Resp: 146043

Ion Ratio Lower Upper

149 100

167 34.3 22.3 33.5#

279 14.5 3.3 4.9#

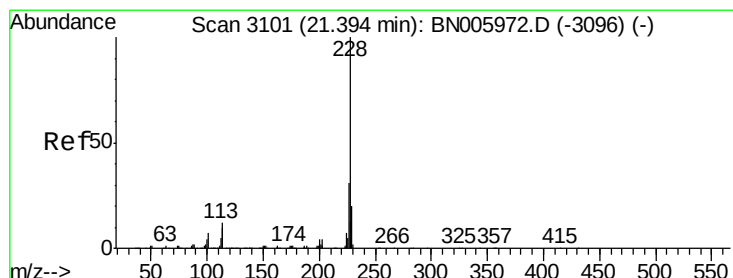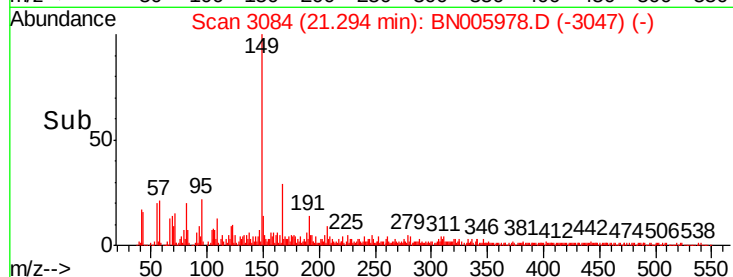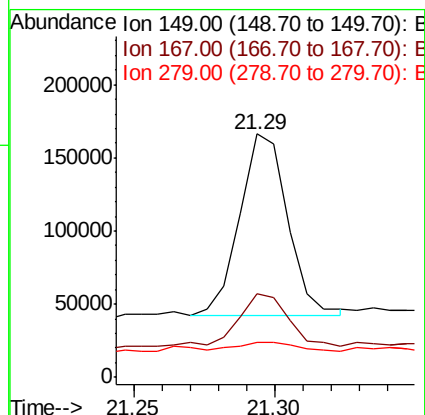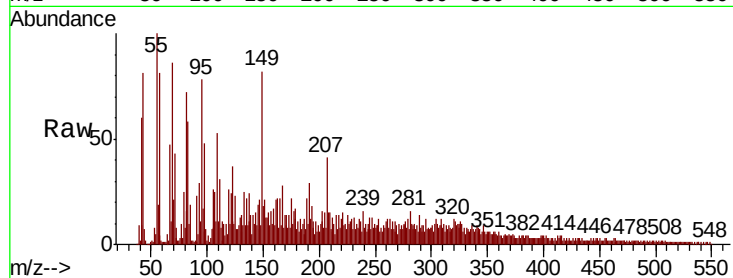

#84

Chrysene

Concen: 4.047 ng/ul

RT: 21.42 min Scan# 3105

Delta R.T. 0.02 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43




Tgt Ion:228 Resp: 315841


Ion Ratio Lower Upper

228 100

226 35.0 24.0 36.0

229 29.8 15.4 23.0#

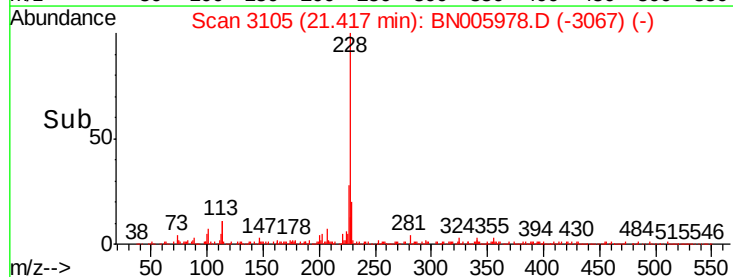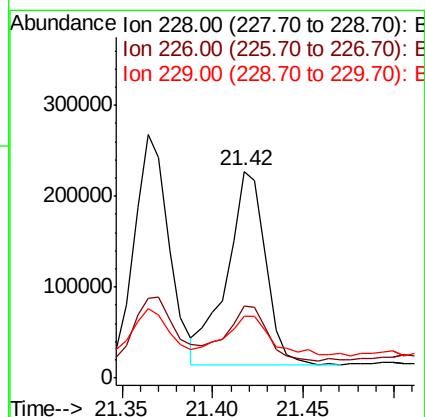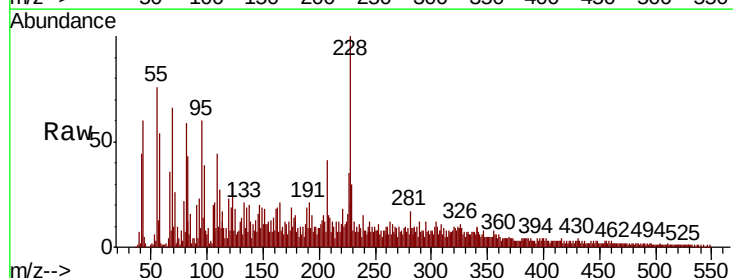

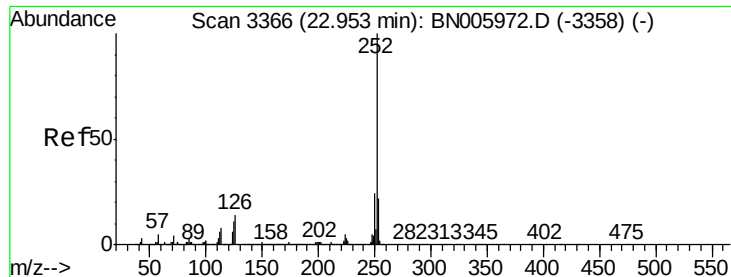

#87

Benzo(b)fluoranthene

Concen: 4.536 ng/ul

RT: 23.00 min Scan# 3374

Delta R.T. 0.05 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43

Instrument :

BNA_N

ClientSampleId :

A42B7





Tot Ion:252 Resp: 413793

Ion Ratio Lower Upper

252 100

253 34.9 17.7 26.5#

125 35.2 8.4 12.6#

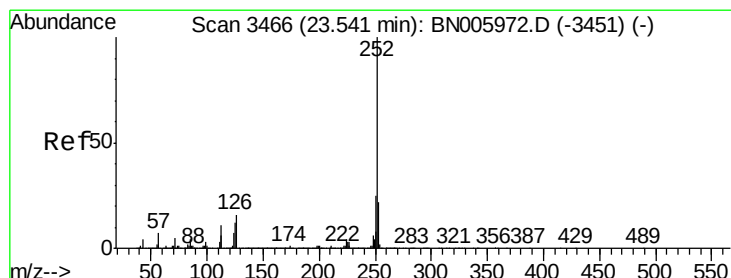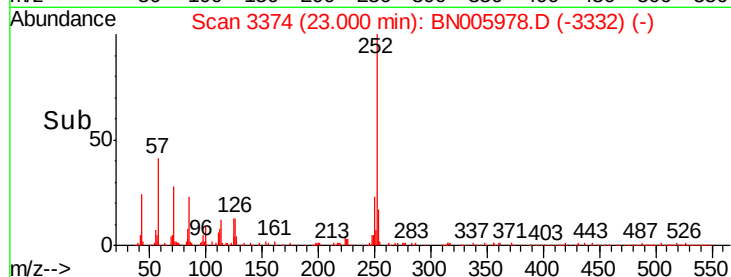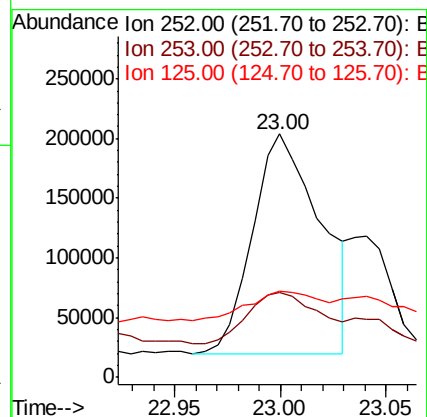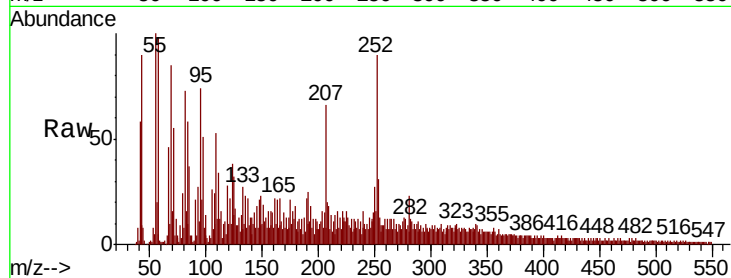

#90

Benzo(a)pyrene

Concen: 3.370 ng/ul

RT: 23.59 min Scan# 3475

Delta R.T. 0.05 min

Lab File: BN005978.D

Acq: 31 May 2019 12:43




Tgt Ion:252 Resp: 289886


Ion Ratio Lower Upper

252 100

253 35.6 17.3 25.9#

125 38.8 8.6 13.0#

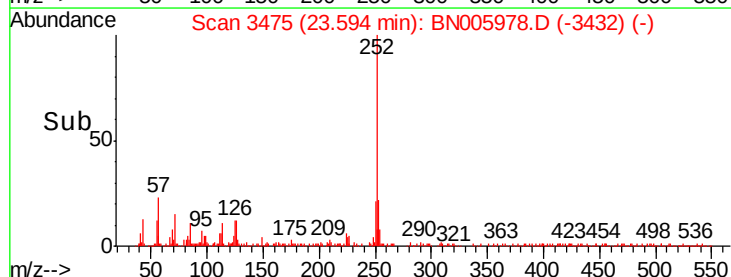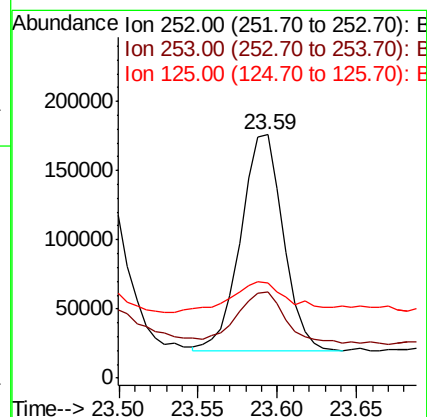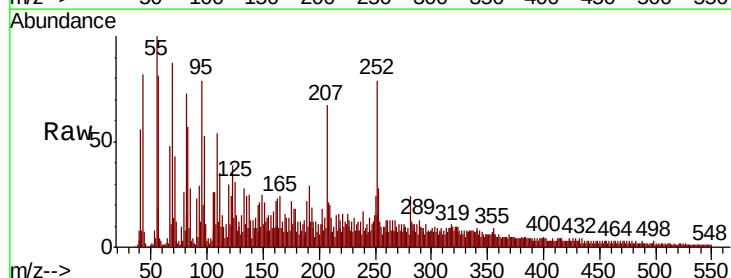




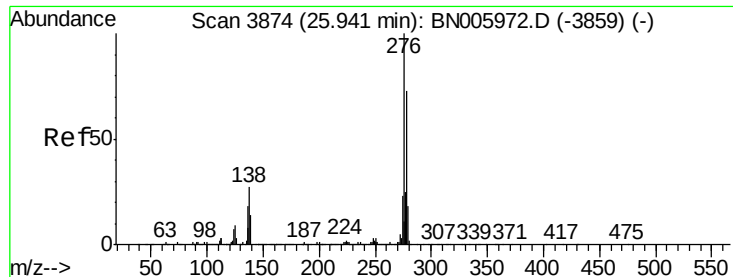


#91

Indeno(1,2,3-cd)pyrene
Concen: 2.034 ng/ul
RT: 26.02 min Scan# 3887
Delta R.T. 0.08 min
Lab File: BN005978.D
Acq: 31 May 2019 12:43

Instrument :
BNA_N
ClientSampleId :
A42B7

Tot Ion:276 Resp: 205288
Ion Ratio Lower Upper
276 100
138 35.7 17.9 26.9#
277 39.7 19.7 29.5#

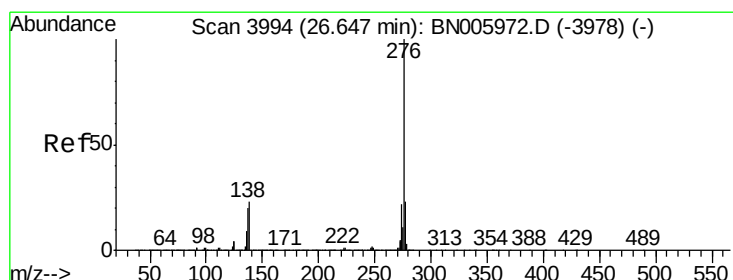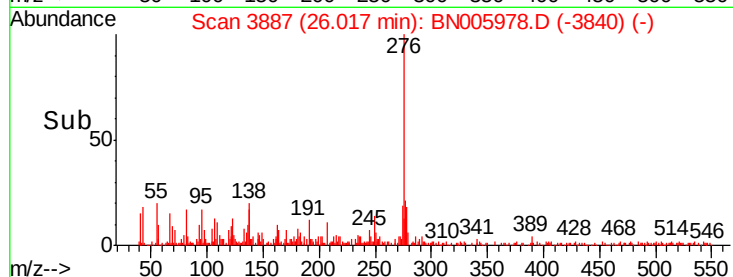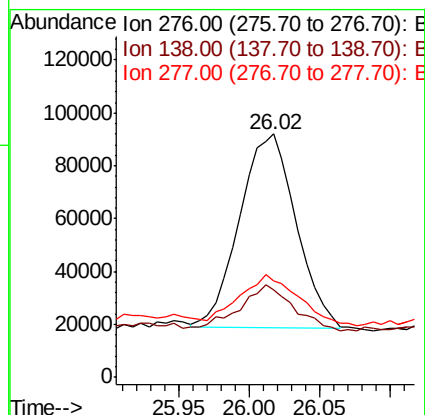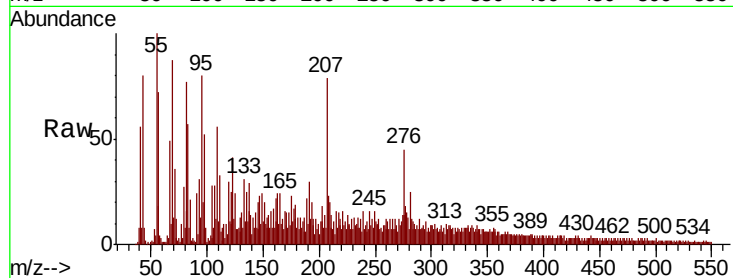

#93

Benzo(g,h,i)perylene
Concen: 2.211 ng/ul
RT: 26.72 min Scan# 4007
Delta R.T. 0.08 min
Lab File: BN005978.D
Acq: 31 May 2019 12:43

Tgt Ion:276 Resp: 187940
Ion Ratio Lower Upper
276 100
138 37.4 16.7 25.1#
277 42.0 18.2 27.2#

