

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN053119\
 Data File : BN005982.D
 Acq On : 31 May 2019 15:01
 Operator : JU/SJ
 Sample : K2924-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4282

Quant Time: May 31 15:52:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 31 15:02:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	594840	20.00	ng/ul	0.01
18) Naphthalene-d8	10.54	136	2226155	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.40	164	1032045	20.00	ng/ul	0.01
61) Phenanthrene-d10	17.16	188	2051731	20.00	ng/ul	0.02
77) Chrysene-d12	21.39	240	1733365	20.00	ng/ul	0.03
85) Perylene-d12	23.70	264	2067137	20.00	ng/ul	0.06

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	78464	5.80	ng/uL	0.00
5) Phenol-d5	6.91	99	1523072	28.89	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.08	67	947054	31.48	ng/ul	0.01
9) 2-Chlorophenol-d4	7.28	132	1267093	31.55	ng/ul	0.01
13) 4-Methylphenol-d8	8.45	113	1163672	27.34	ng/ul	0.01
19) Nitrobenzene-d5	8.90	128	592583	41.47	ng/ul	0.01
22) 2-Nitrophenol-d4	9.62	143	564790	42.44	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.16	165	1028007	32.72	ng/ul	0.02
29) 4-Chloroaniline-d4	10.67	131	1398616	33.95	ng/ul	0.01
43) Dimethylphthalate-d6	13.81	166	2682015	35.25	ng/ul	0.02
46) Acenaphthylene-d8	14.09	160	3245369	34.10	ng/ul	0.02
51) 4-Nitrophenol-d4	14.61	143	383524	27.70	ng/ul	0.02
57) Fluorene-d10	15.40	176	2097207	32.87	ng/ul	0.02
62) 4,6-Dinitro-2-methylphenol	15.54	200	52377	6.26	ng/ul	0.03
70) Anthracene-d10	17.26	188	2962624	33.93	ng/ul	0.02
78) Pyrene-d10	19.57	212	3154824	36.04	ng/ul	0.02
89) Benzo(a)pyrene-d12	23.55	264	3191757	34.60	ng/ul	0.06


Target Compounds					Ovalue	
44) Dimethylphthalate	13.85	163	163610	2.152	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN053119\
Data File : BN005982.D
Acq On : 31 May 2019 15:01
Operator : JU/SJ
Sample : K2924-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4282

Quant Time: May 31 15:52:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 31 15:02:18 2019
Response via : Initial Calibration

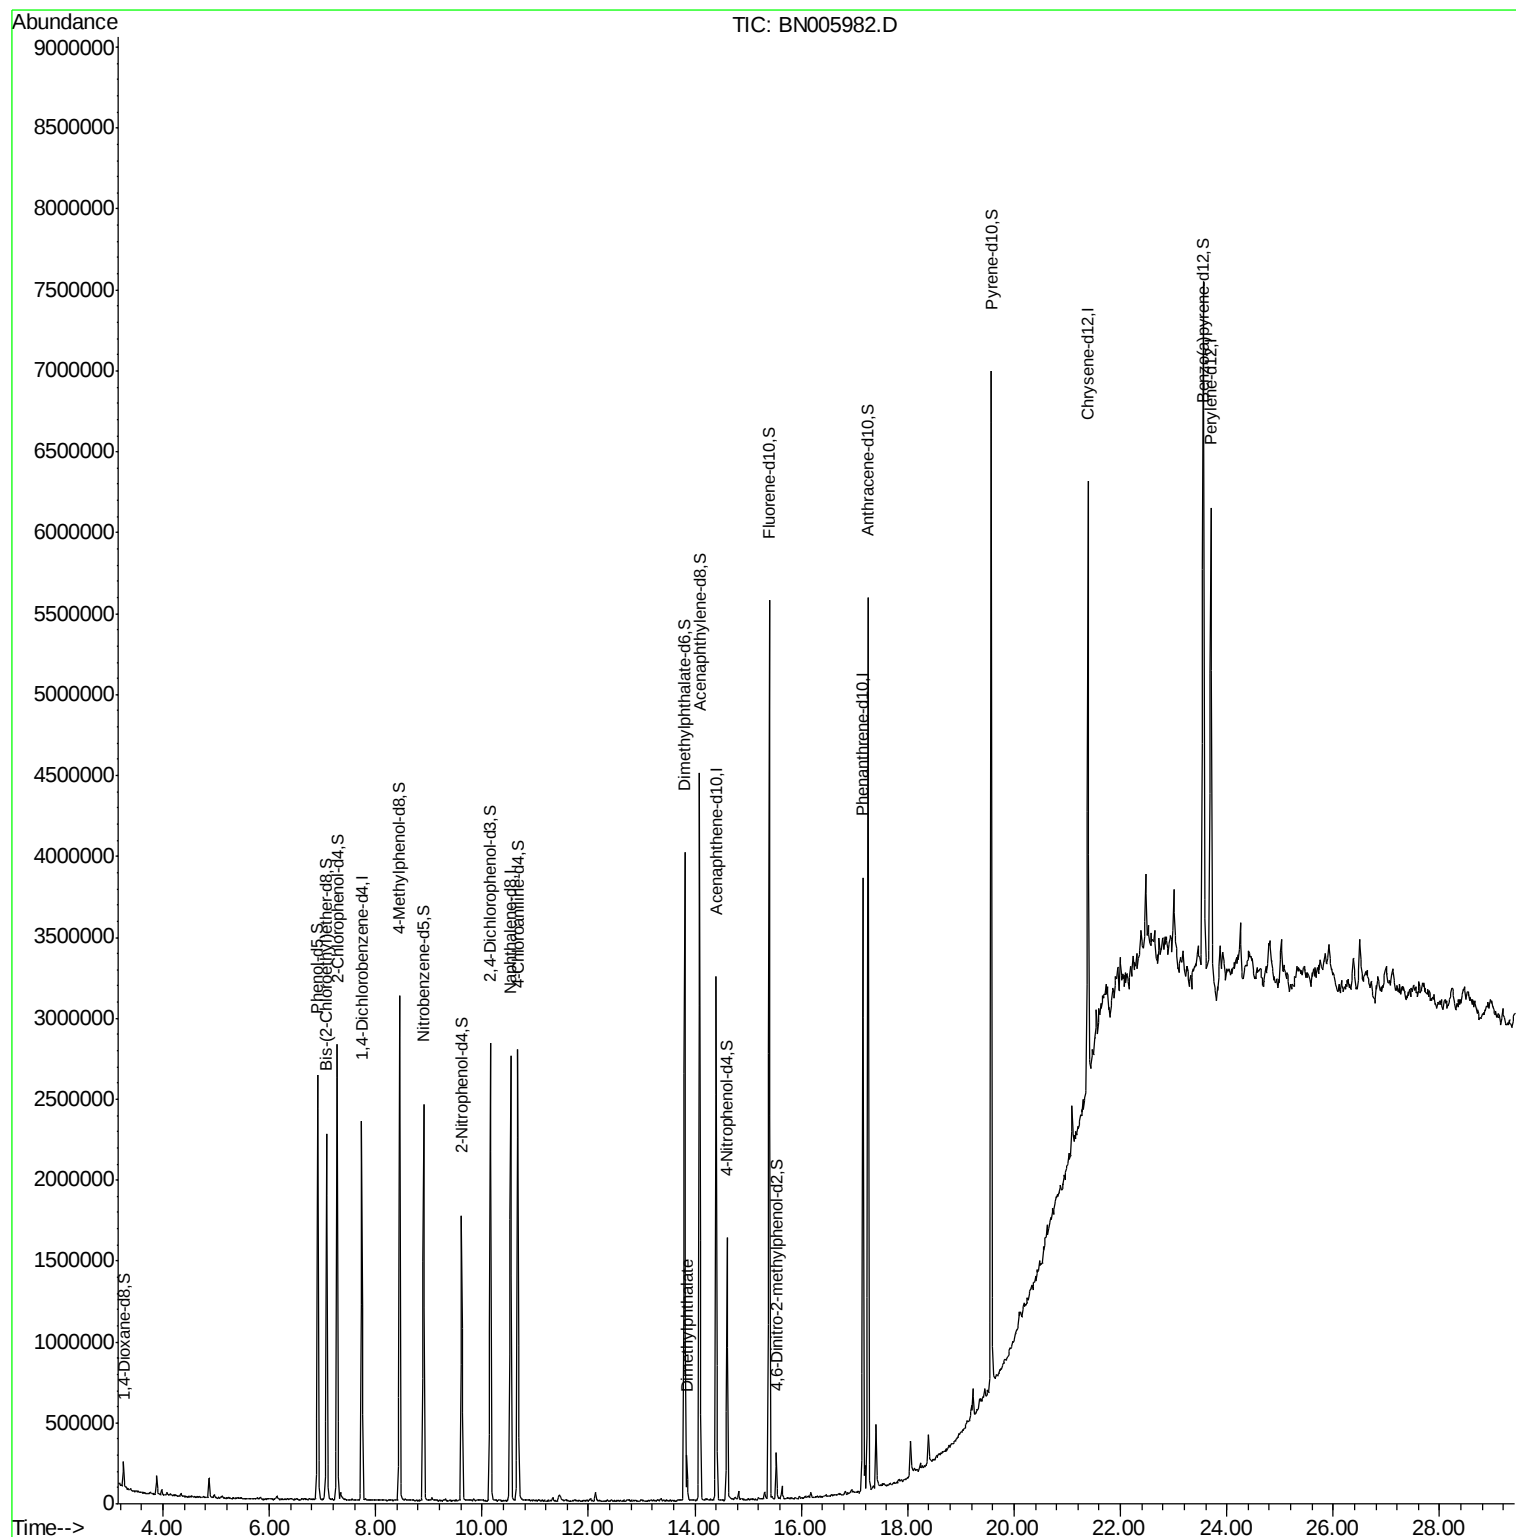

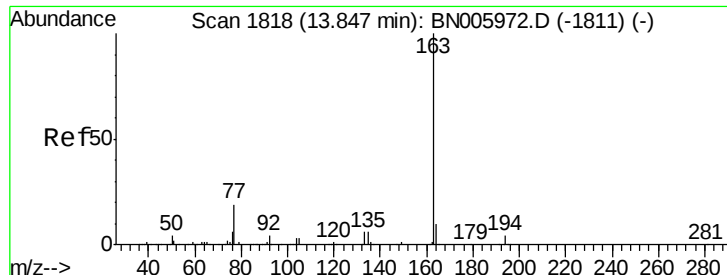

#44

Dimethylphthalate

Concen: 2.152 ng/ul

RT: 13.85 min Scan# 1819

Delta R.T. 0.01 min

Lab File: BN005982.D

Acq: 31 May 2019 15:01

Instrument :

BNA_N

ClientSampleId :

A4282


Tot Ion:163 Resp: 163610

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 9.9 8.1 12.1

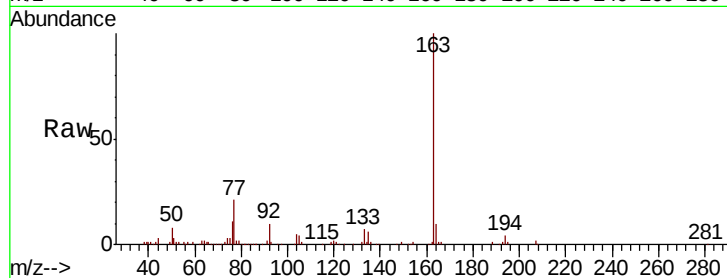

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

