
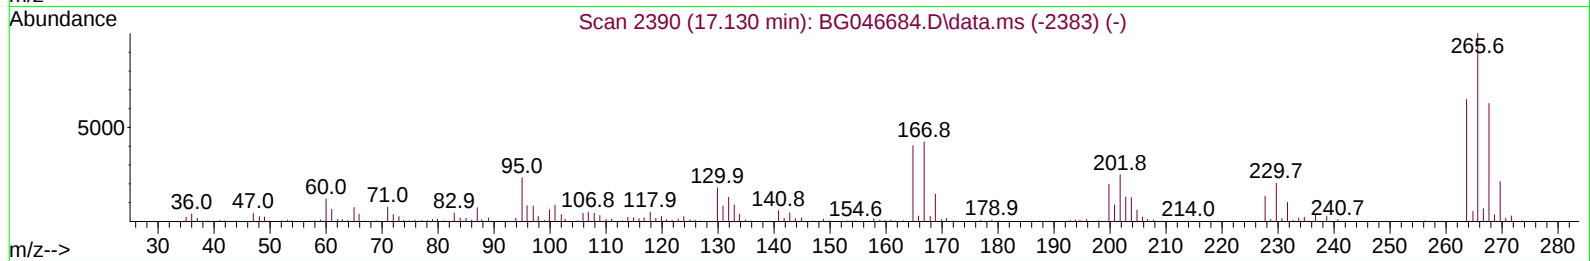
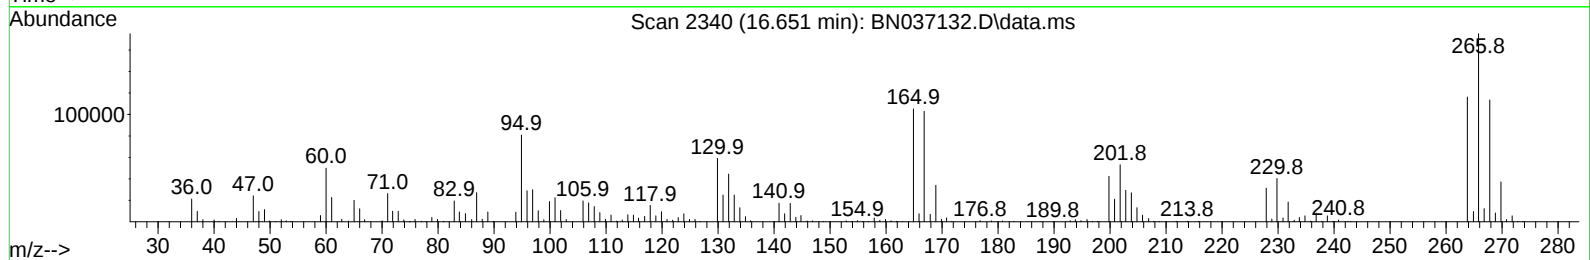


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060225\
Data File : BN037132.D
Acq On : 02 Jun 2025 15:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 05:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

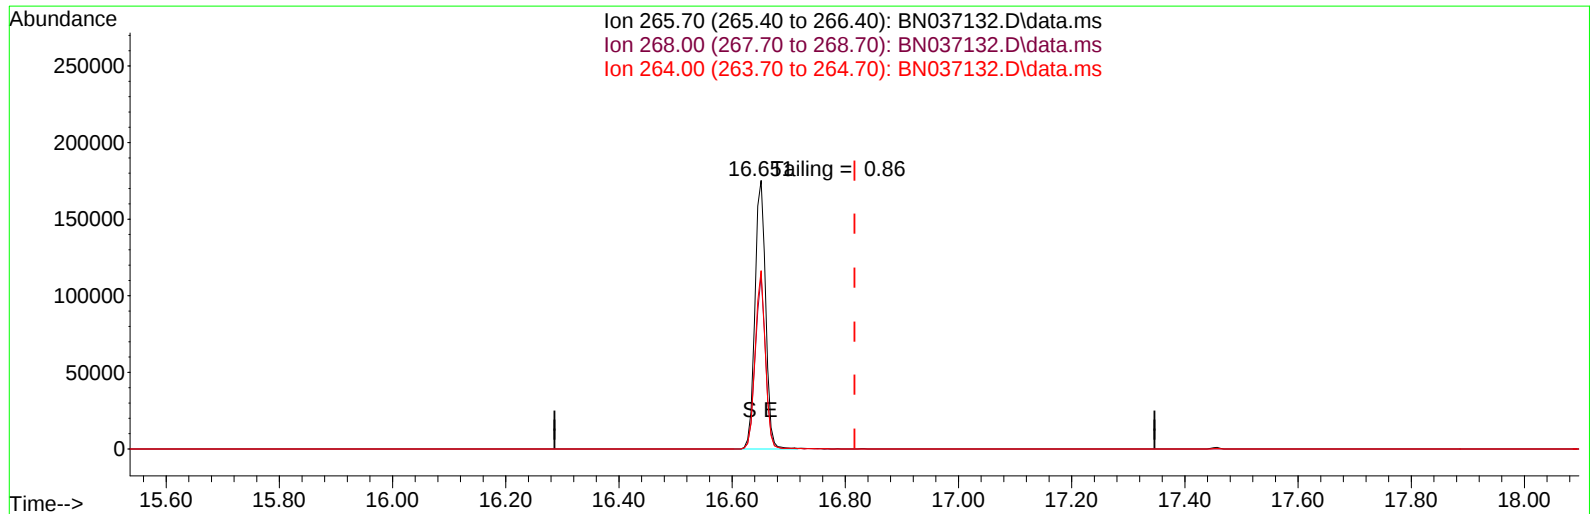

TIC: BN037132.D\data.ms

(70) Pentachlorophenol (C)




16.651min (-0.165) 17486.22 ng

response 231091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.78
264.00	61.60	66.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060225\
Data File : BN037132.D
Acq On : 02 Jun 2025 15:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 05:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

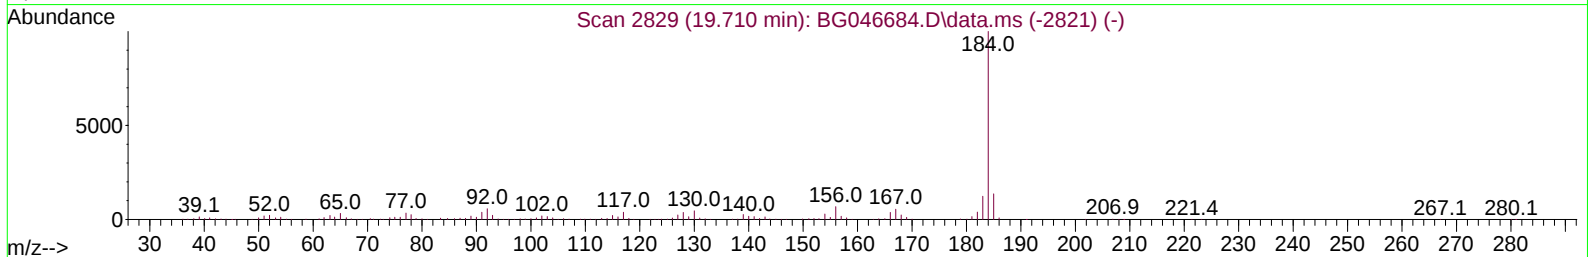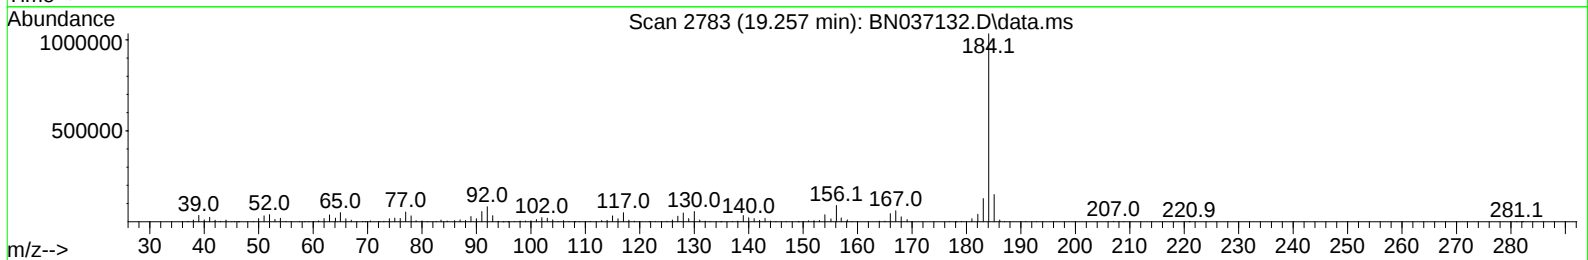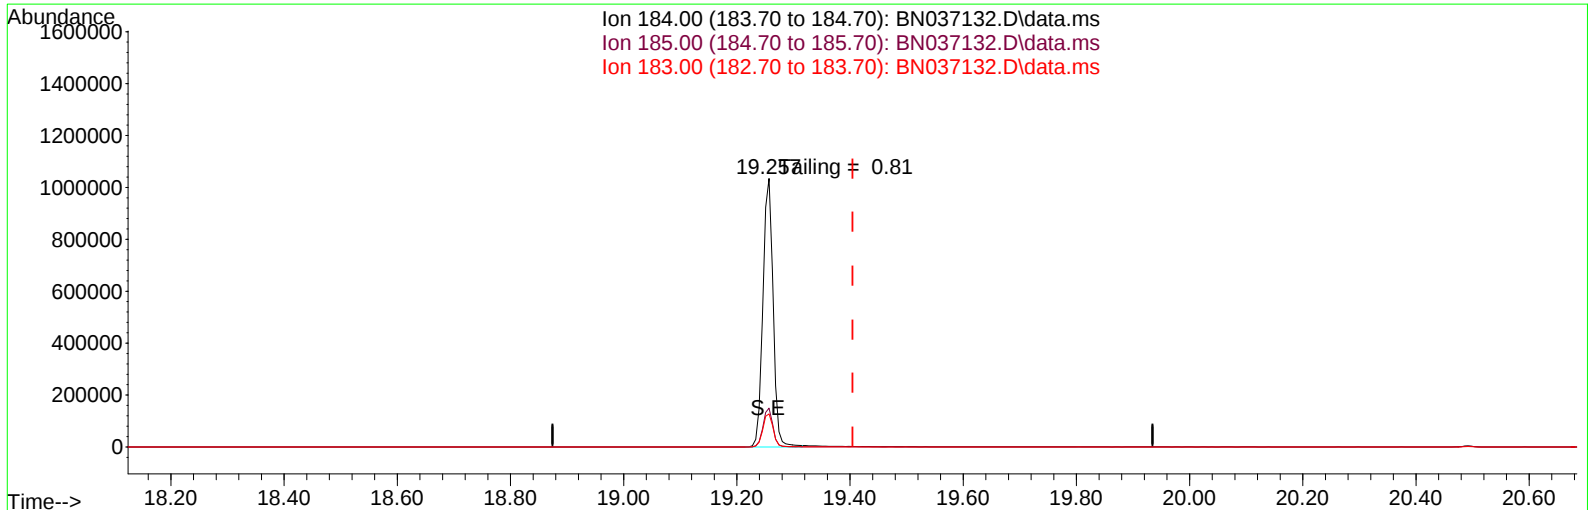

TIC: BN037132.D\data.ms

(77) Benzidine

19.257min (-0.147) 0.00 ng

response 1317247

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.34
0.00	0.00	0.00