
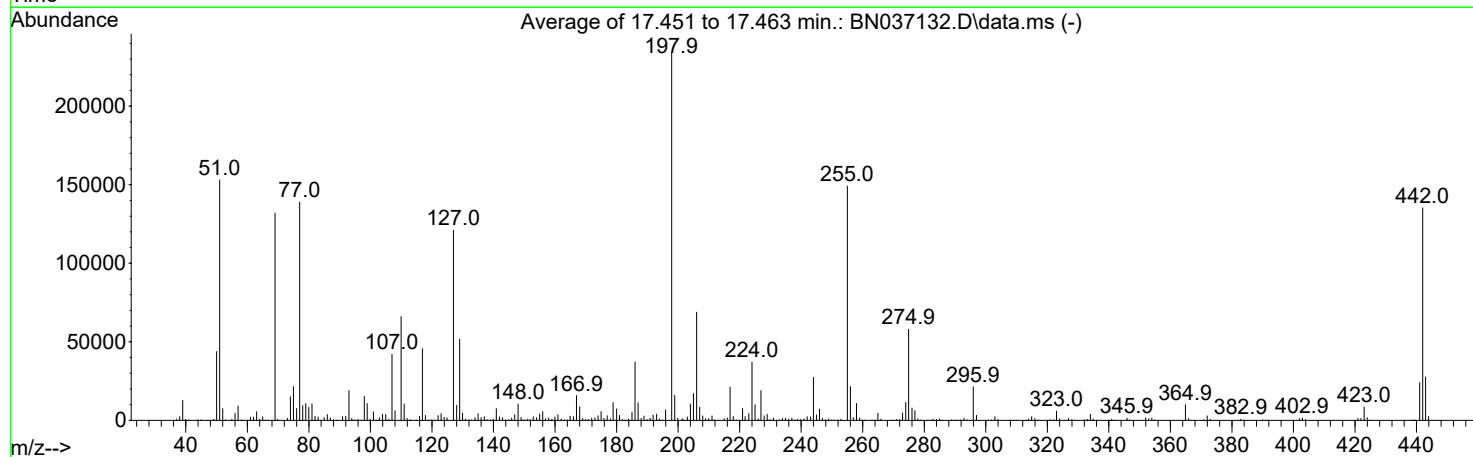


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060225\
Data File : BN037132.D
Acq On : 02 Jun 2025 15:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 03 05:41:05 2025

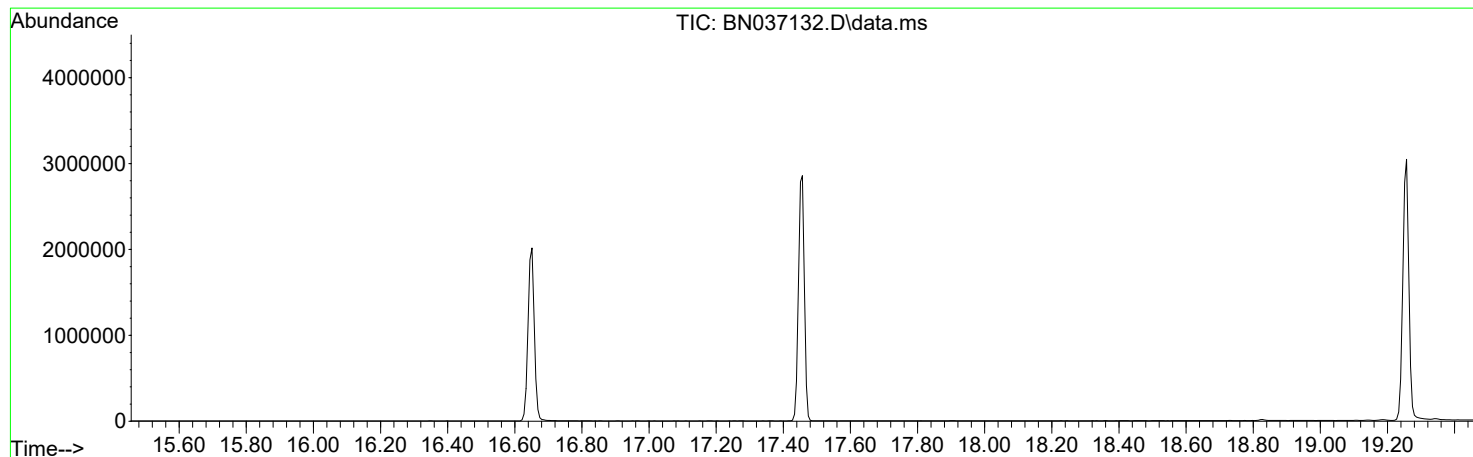

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.3	153011	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.3	131888	PASS
70	69	0.00	2	0.6	763	PASS
127	198	10	80	51.7	120965	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	234176	PASS
199	198	5	9	6.8	15859	PASS
275	198	10	60	24.8	57960	PASS
365	198	1	100	4.2	9938	PASS
441	198	0.01	100	10.3	24045	PASS
442	442	50	100	100.0	135280	PASS
443	442	15	24	20.4	27576	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/2/2025	BNA_N	<u>BN037132.D</u>
Compound Name	Response	Retention Time
DDT	735260	20.492
DDD	9195	20.104
DDE	677	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9872	745132	1.32

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060225\
Data File : BN037132.D
Acq On : 02 Jun 2025 15:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 03 05:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

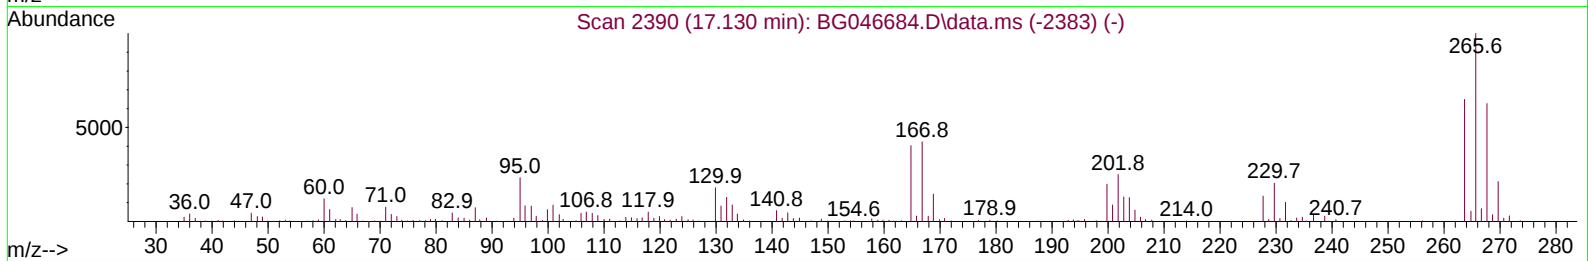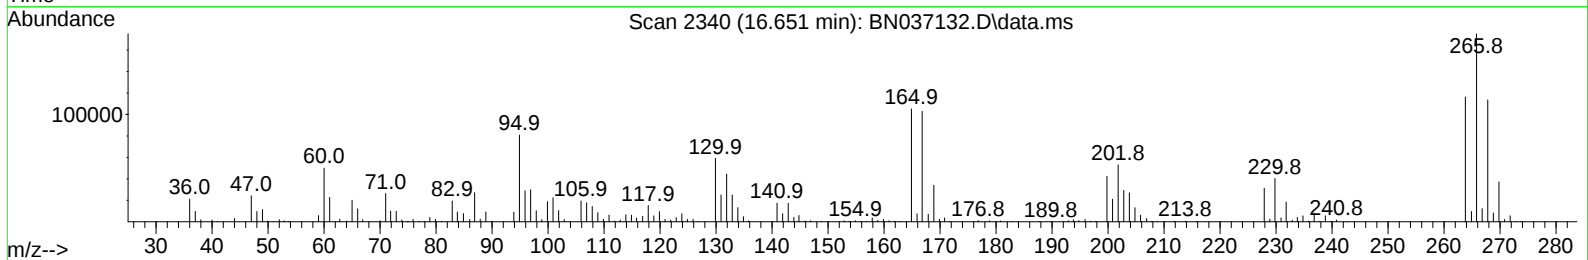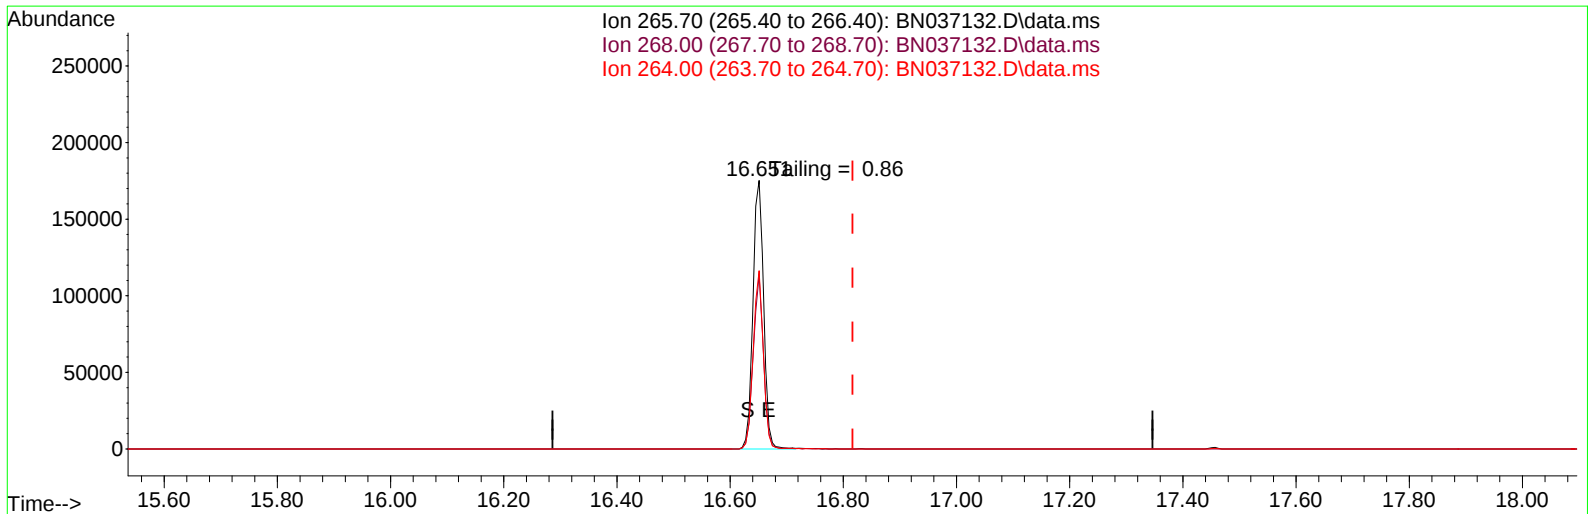

TIC: BN037132.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.165) 17486.22 ng




response 231091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.78
264.00	61.60	66.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060225\
Data File : BN037132.D
Acq On : 02 Jun 2025 15:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 03 05:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

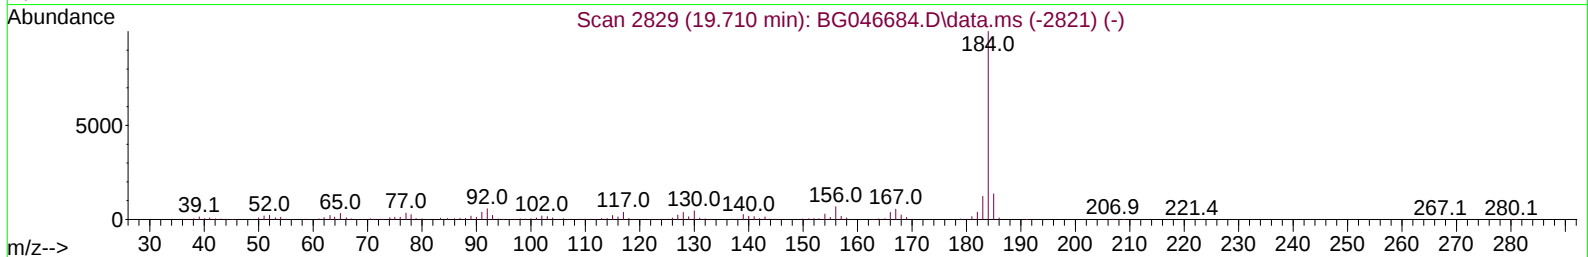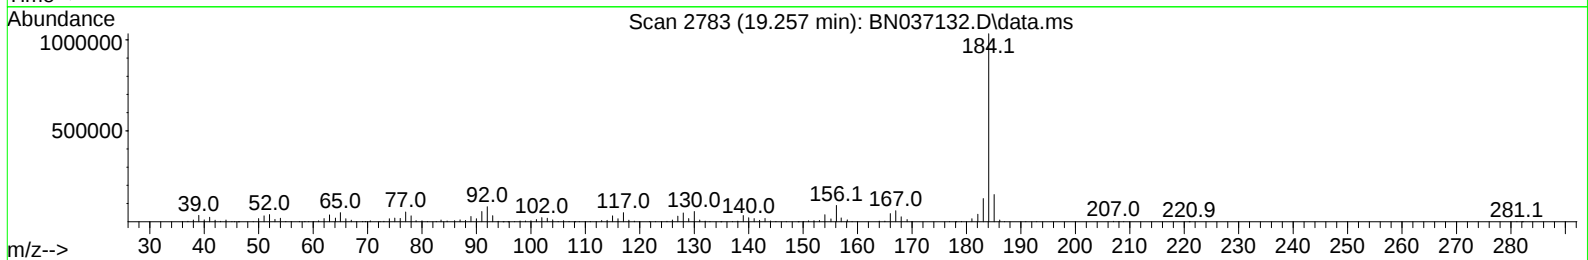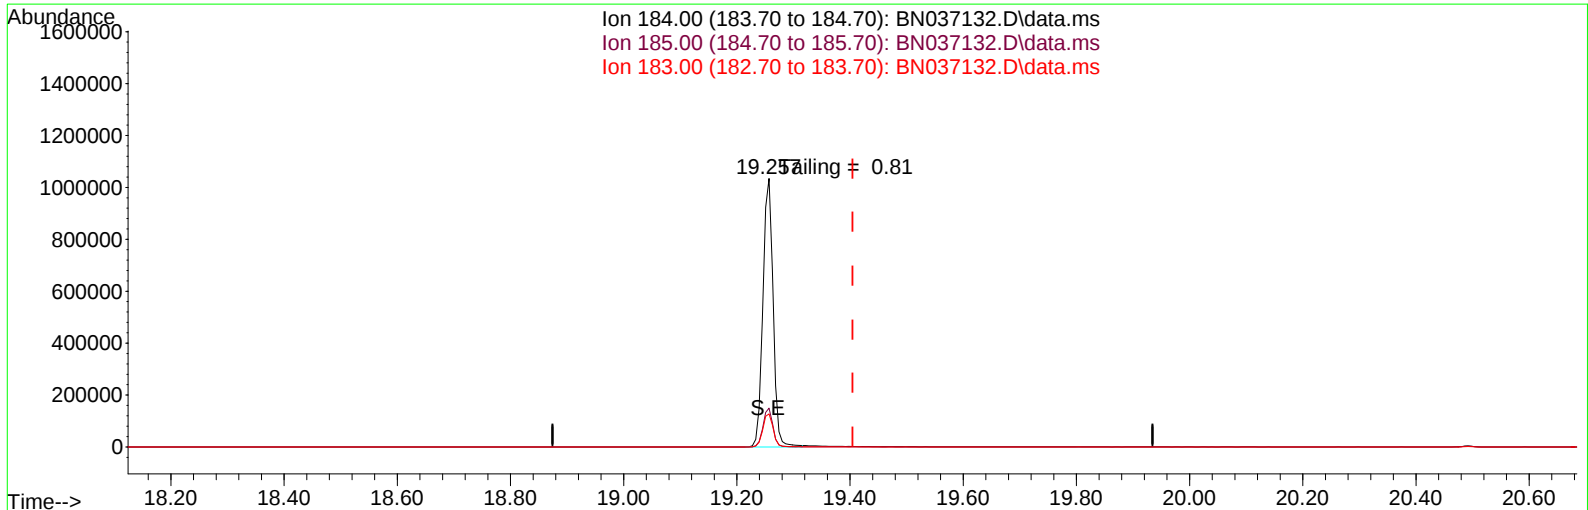

TIC: BN037132.D\data.ms

(77) Benzidine

19.257min (-0.147) 0.00 ng

response 1317247

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	12.34
0.00	0.00	0.00