

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060419\
 Data File : BN006074.D
 Acq On : 04 Jun 2019 21:23
 Operator : JU/SJ
 Sample : K2948-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHA8

Quant Time: Jun 05 01:21:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN060419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 04 17:47:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	268638	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1178981	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	669034	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1470485	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	1348610	20.00	ng/ul	0.00
85) Perylene-d12	23.50	264	1529645	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	28127	4.54	ng/uL	0.00
5) Phenol-d5	6.82	99	499955	23.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	306395	24.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	414287	24.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	370771	22.29	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	203912	24.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	227379	24.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	394151	23.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	534411	26.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1279880	26.97	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1515303	24.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	145259	17.33	ng/ul	0.00
57) Fluorene-d10	15.30	176	1063190	26.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	84963	10.33	ng/ul	0.00
70) Anthracene-d10	17.16	188	1609841	25.66	ng/ul	0.00
78) Pyrene-d10	19.46	212	1773259	27.21	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	1715976	25.19	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.76	163	163091	3.464	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060419\
Data File : BN006074.D
Acq On : 04 Jun 2019 21:23
Operator : JU/SJ
Sample : K2948-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHA8

Quant Time: Jun 05 01:21:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN060419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 04 17:47:25 2019
Response via : Initial Calibration

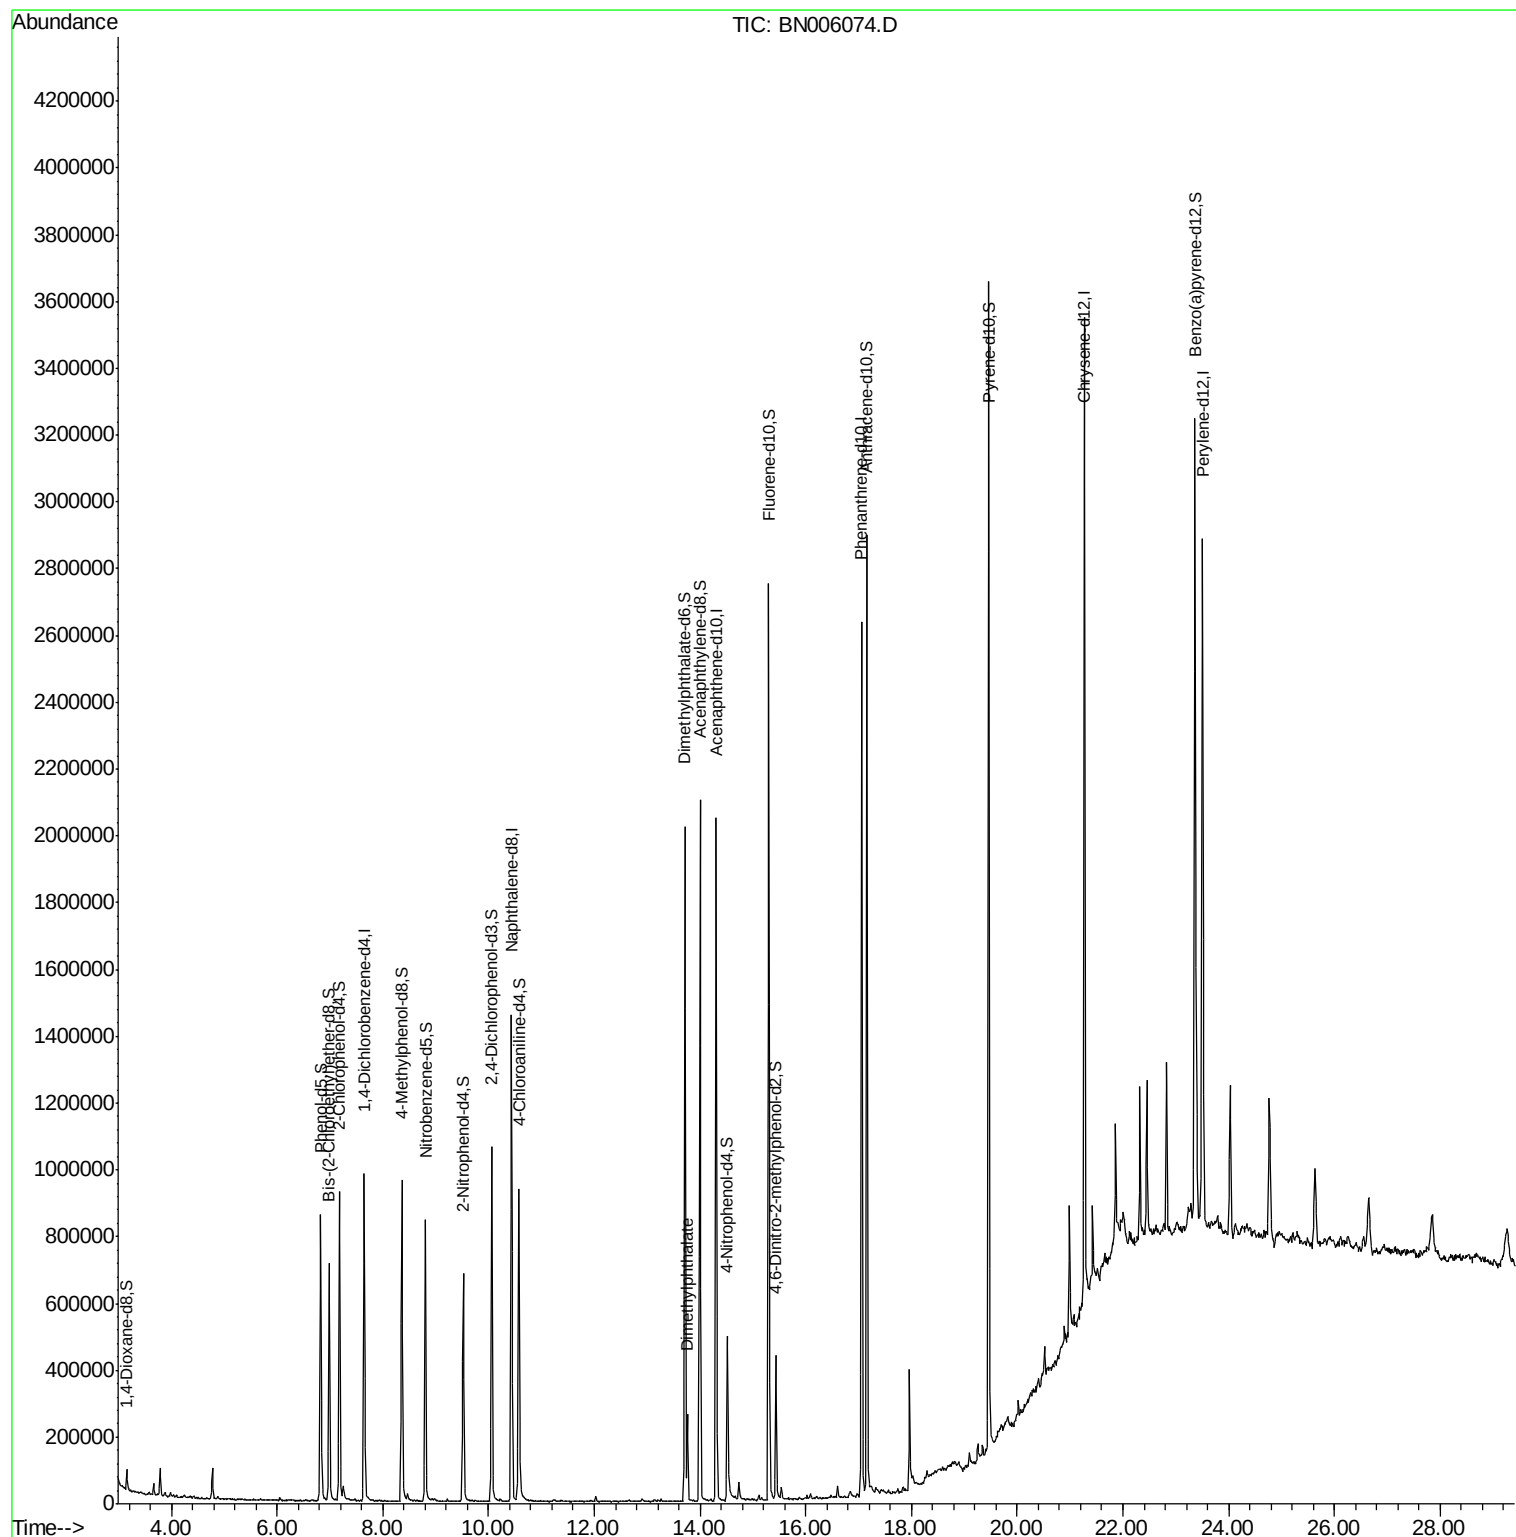

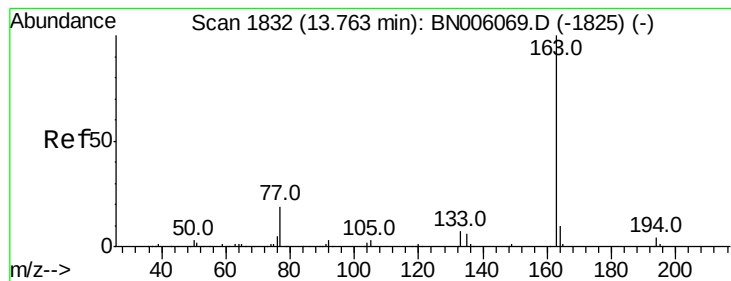

#44

Dimethylphthalate

Concen: 3.464 ng/ul

RT: 13.76 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BN006074.D

Acq: 04 Jun 2019 21:23

Instrument :

BNA_N

ClientSampleId :

BFHA8


Tot Ion:163 Resp: 163091

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.2 8.2 12.2

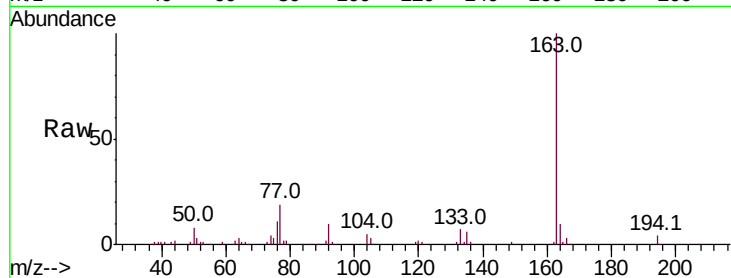

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

