

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060419\
 Data File : BN006076.D
 Acq On : 04 Jun 2019 22:33
 Operator : JU/SJ
 Sample : K2948-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHA6

Quant Time: Jun 05 01:22:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN060419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 04 17:47:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	271339	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1170753	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	652679	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1385494	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	1247134	20.00	ng/ul	0.00
85) Perylene-d12	23.51	264	1404281	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	21256	3.39	ng/uL	0.00
5) Phenol-d5	6.82	99	352852	16.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	231461	18.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	298389	17.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	288542	17.18	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	149572	17.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	160275	17.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	262079	15.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	357613	17.87	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	887347	19.16	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1009108	16.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	94040	11.50	ng/ul	0.00
57) Fluorene-d10	15.30	176	715821	18.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	55474	7.16	ng/ul	0.00
70) Anthracene-d10	17.16	188	1063290	17.99	ng/ul	0.00
78) Pyrene-d10	19.46	212	1073265	17.81	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.37	264	1023603	16.37	ng/ul	0.00


Target Compounds				Ovalue
44) Dimethylphthalate	13.76	163	102259	2.227 ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060419\
Data File : BN006076.D
Acq On : 04 Jun 2019 22:33
Operator : JU/SJ
Sample : K2948-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHA6

Quant Time: Jun 05 01:22:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN060419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 04 17:47:25 2019
Response via : Initial Calibration

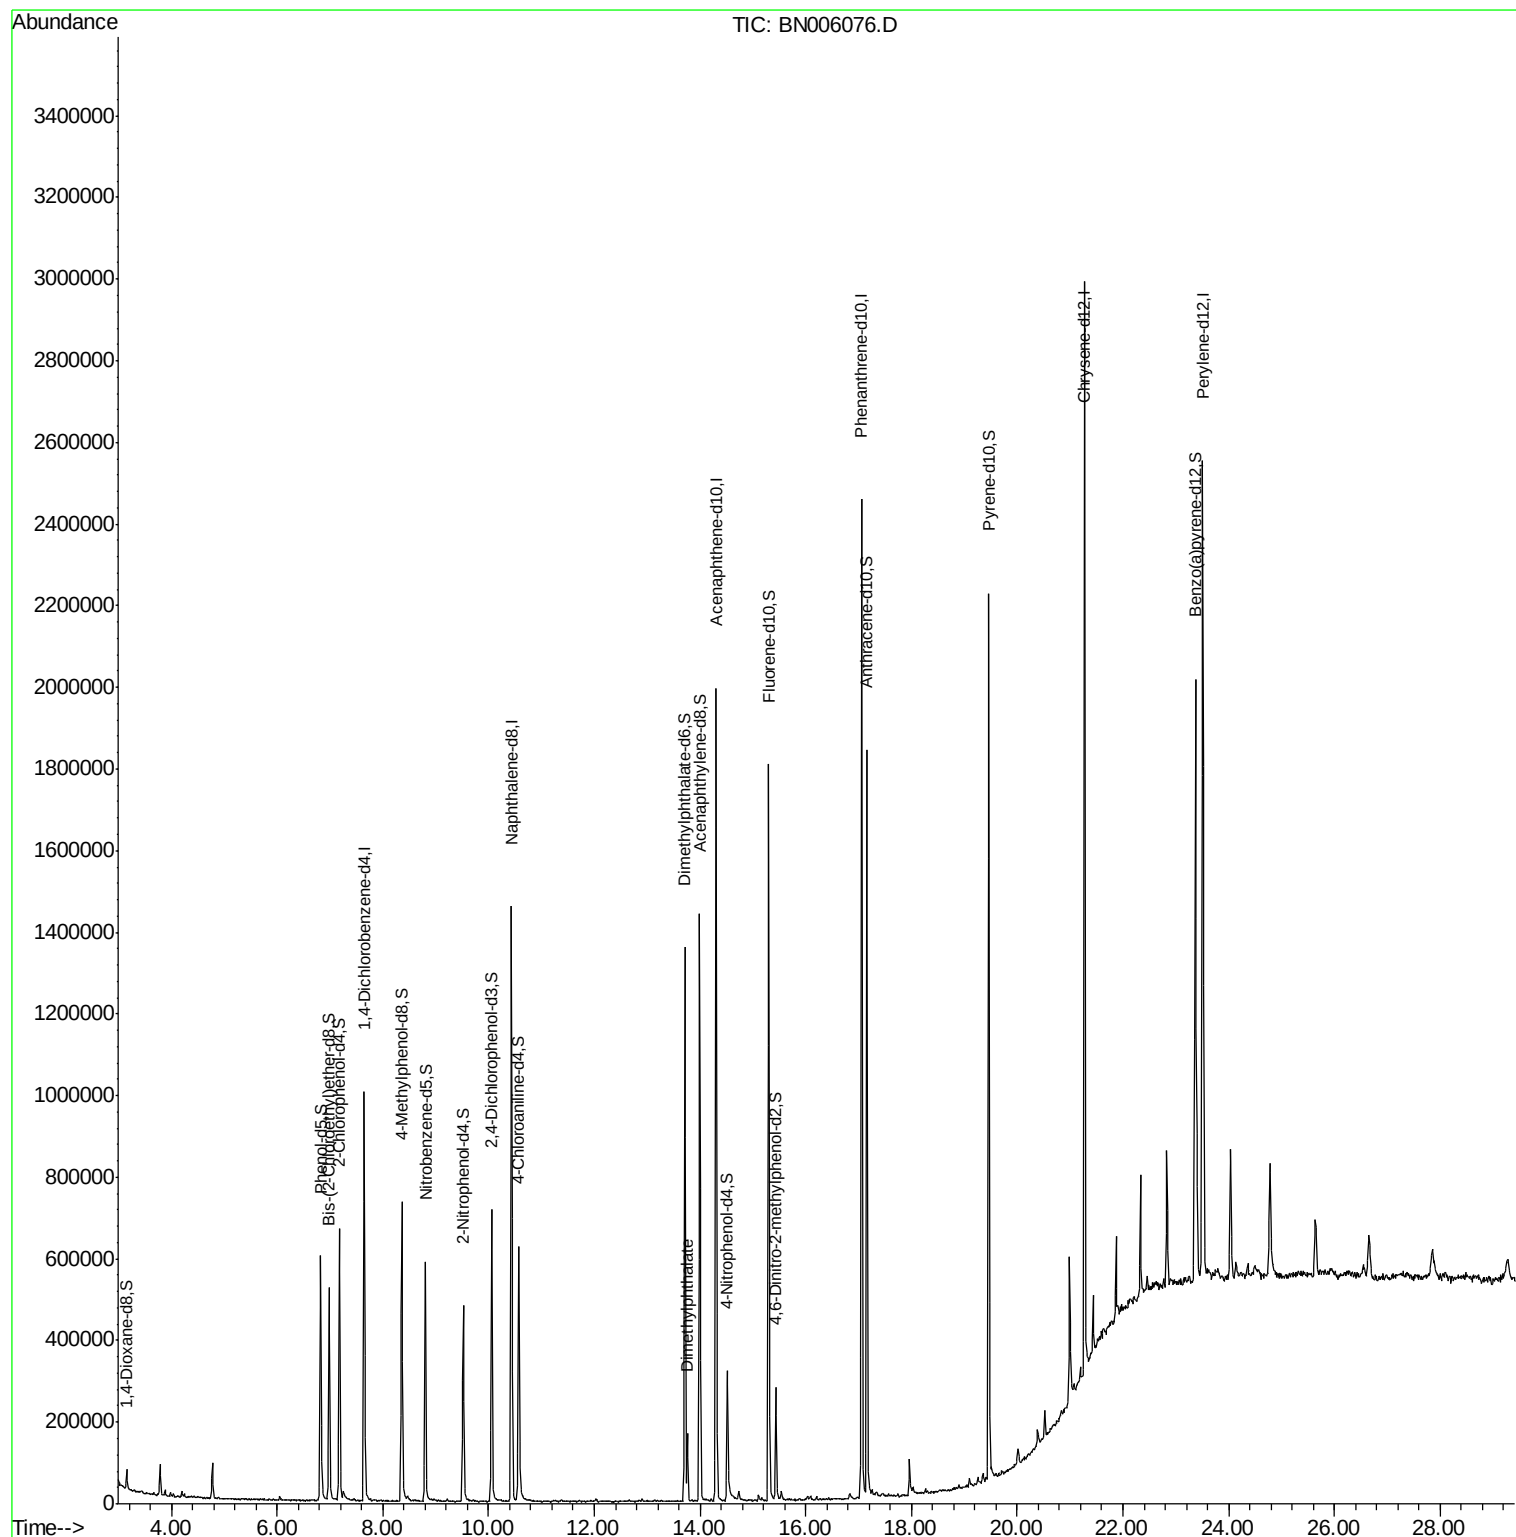

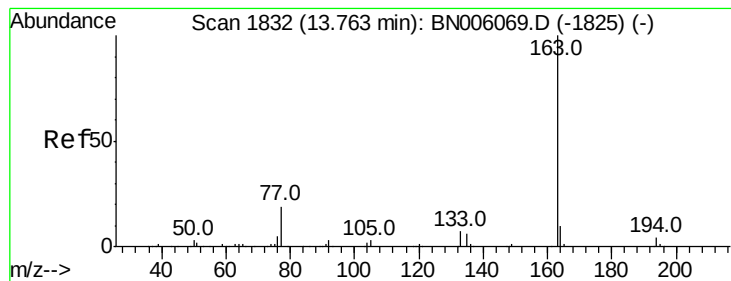

#44

Dimethylphthalate

Concen: 2.227 ng/ul

RT: 13.76 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BN006076.D

Acq: 04 Jun 2019 22:33

Instrument :

BNA_N

ClientSampleId :

BFHA6


Tot Ion:163 Resp: 102259

Ion Ratio Lower Upper

163 100

194 5.1 3.4 5.2

164 10.0 8.2 12.2

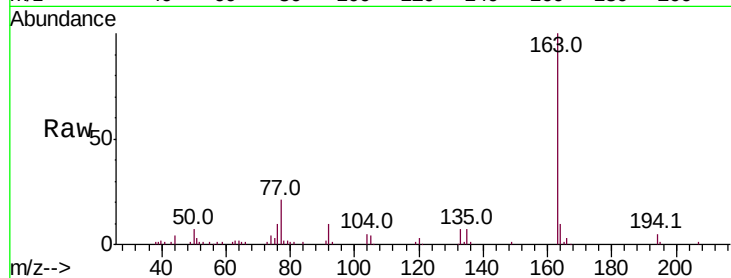

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

