

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060419\
 Data File : BN006079.D
 Acq On : 05 Jun 2019 00:17
 Operator : JU/SJ
 Sample : K2948-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFH97

Quant Time: Jun 05 01:22:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN060419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 04 17:47:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	250171	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1066851	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	593975	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1308306	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	1233613	20.00	ng/ul	0.00
85) Perylene-d12	23.50	264	1384725	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	48521	8.40	ng/uL	0.00
5) Phenol-d5	6.82	99	896098	44.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	527577	46.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	720800	44.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	706618	45.62	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	360441	47.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	399548	47.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	676453	44.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	956033	52.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1954773	46.39	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2549874	46.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	292812	39.35	ng/ul	0.00
57) Fluorene-d10	15.30	176	1666908	46.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	190572	26.03	ng/ul	0.00
70) Anthracene-d10	17.16	188	2621101	46.95	ng/ul	0.00
78) Pyrene-d10	19.46	212	2819364	47.30	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.36	264	2835224	45.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.76	163	162092	3.878	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060419\
Data File : BN006079.D
Acq On : 05 Jun 2019 00:17
Operator : JU/SJ
Sample : K2948-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFH97

Quant Time: Jun 05 01:22:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN060419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 04 17:47:25 2019
Response via : Initial Calibration

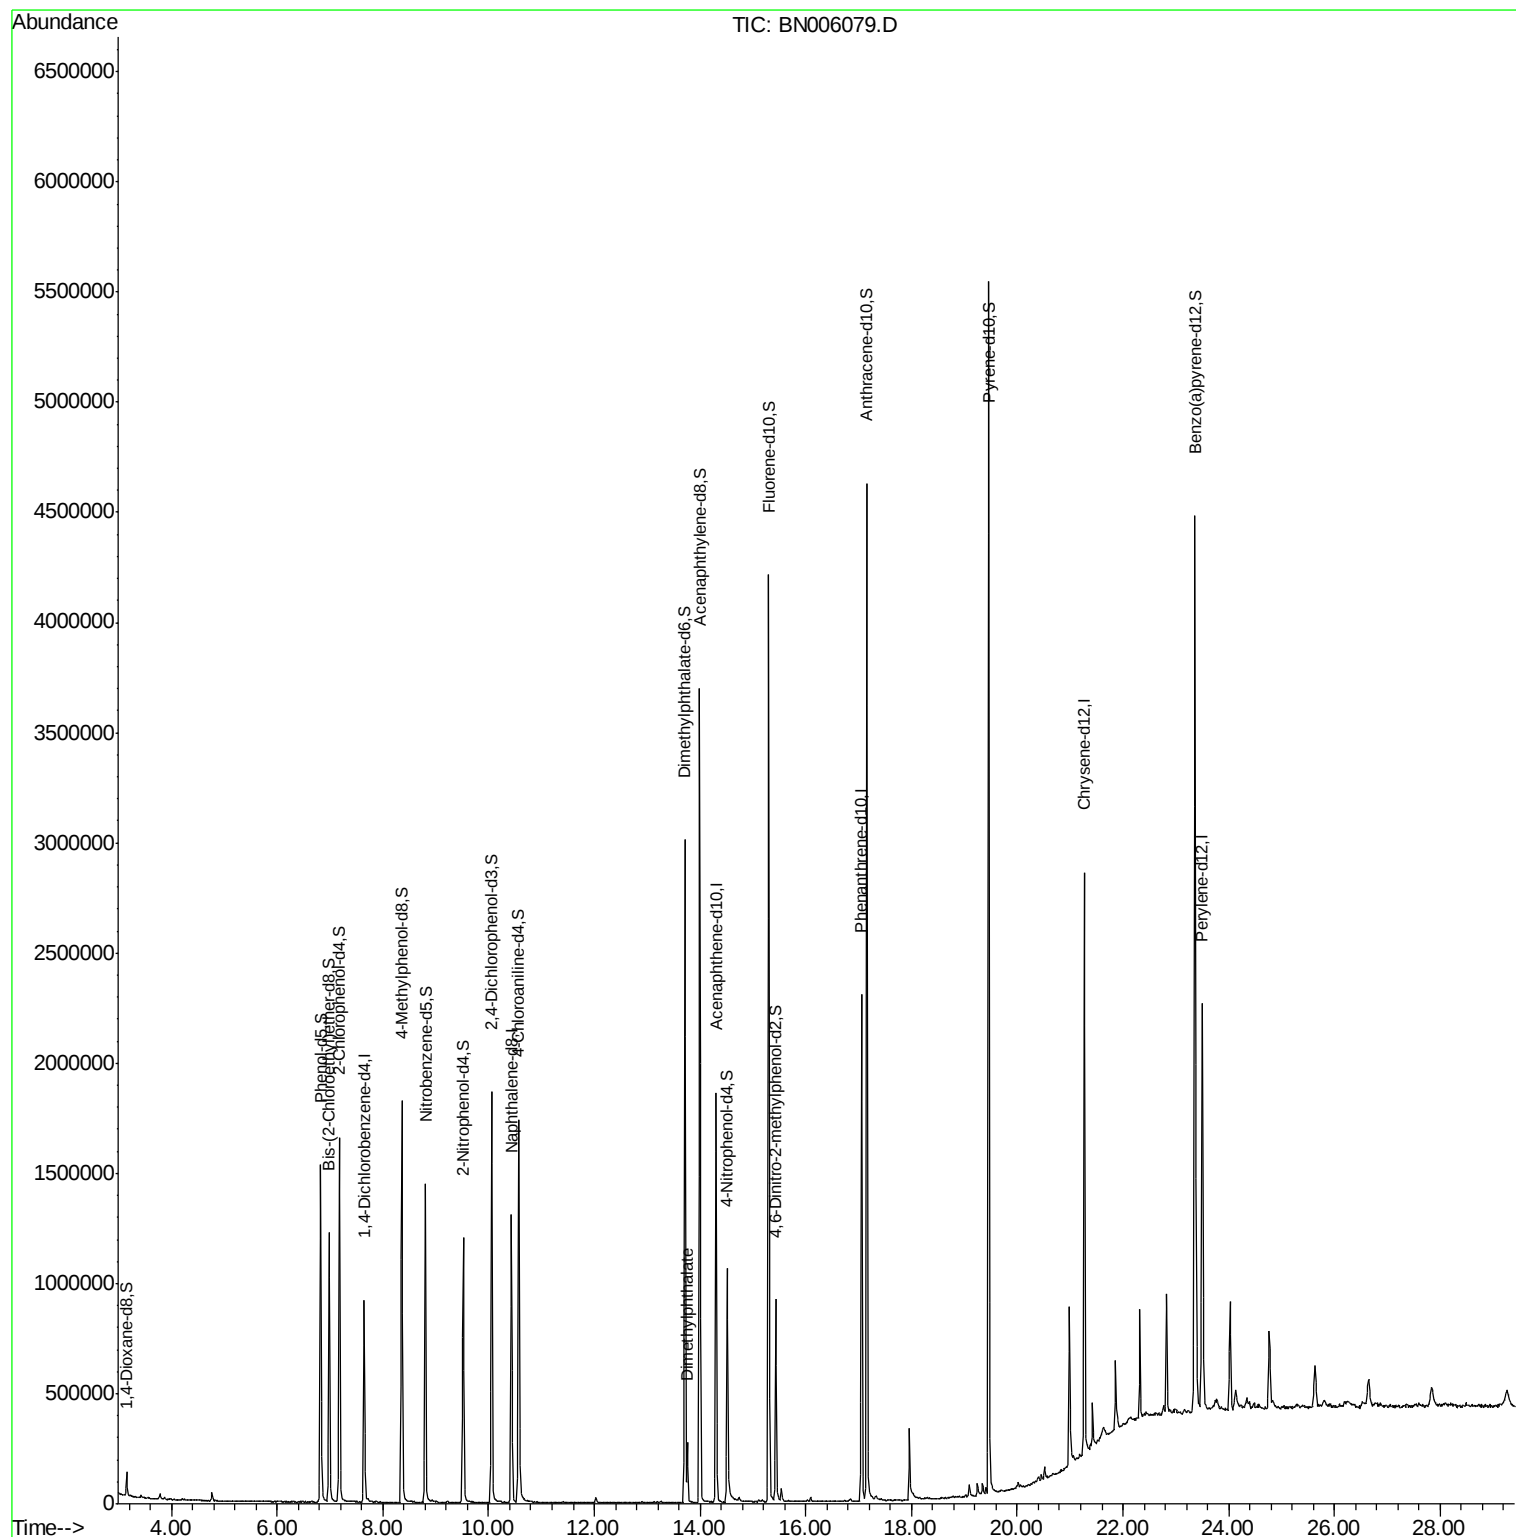

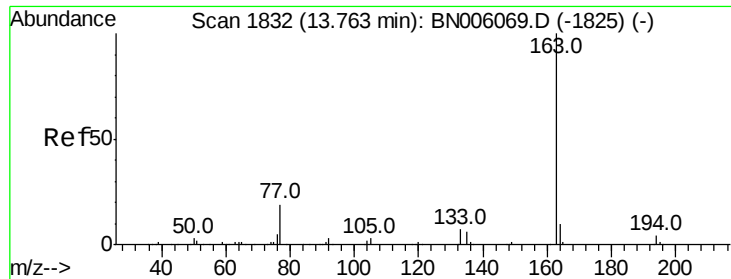

#44

Dimethylphthalate

Concen: 3.878 ng/ul

RT: 13.76 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BN006079.D

Acq: 05 Jun 2019 00:17

Instrument :

BNA_N

ClientSampleId :

BFH97


Tot Ion:163 Resp: 162092

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 10.3 8.2 12.2

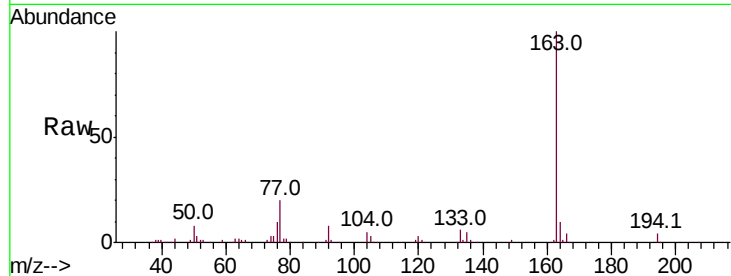

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

