

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
 Data File : BN031780.D
 Acq On : 04 Jun 2024 17:33
 Operator : MA/JU
 Sample : PB161200BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	43	rBV	107951	158041	1.65%	0.138%
2	3.593	100	103	124	rBV	1672018	2636361	27.46%	2.298%
3	3.911	153	157	164	rVB	24251	39443	0.41%	0.034%
4	6.687	621	629	635	rBV	6024	15484	0.16%	0.013%
5	6.852	647	657	668	rBV	2163161	3503482	36.49%	3.054%
6	7.022	677	686	695	rVB	1725906	2771825	28.87%	2.416%
7	7.211	711	718	733	rBV	2200350	3488548	36.34%	3.041%
8	7.675	790	797	808	rVB	1633397	2675505	27.87%	2.332%
9	8.381	909	917	928	rBV	2872767	4655530	48.49%	4.059%
10	8.834	985	994	1005	rBV	2199171	3512179	36.58%	3.062%
11	9.552	1104	1116	1127	rBV	1701970	2805030	29.22%	2.445%
12	10.081	1196	1206	1223	rBV	2710606	4680450	48.75%	4.080%
13	10.463	1262	1271	1279	rBV	2541439	4327069	45.07%	3.772%
14	10.605	1286	1295	1309	rBV	2896626	4987617	51.95%	4.348%
15	12.051	1535	1541	1548	rVB2	48905	87600	0.91%	0.076%
16	13.287	1746	1751	1757	rVB4	8614	16576	0.17%	0.014%
17	13.734	1819	1827	1837	rBV	4557275	6470114	67.40%	5.641%
18	14.010	1867	1874	1884	rBV	5368366	8209893	85.52%	7.157%
19	14.322	1919	1927	1935	rBV	3841645	5689471	59.26%	4.960%
20	14.522	1955	1961	1980	rBV	1865592	2852846	29.72%	2.487%
21	15.316	2089	2096	2105	rVV	6757877	9600278	100.00%	8.369%
22	15.440	2109	2117	2128	rVV	887183	1247754	13.00%	1.088%
23	15.551	2132	2136	2142	rVB	31596	54477	0.57%	0.047%
24	15.887	2188	2193	2199	rBV6	6082	11418	0.12%	0.010%
25	16.098	2224	2229	2233	rBV7	8395	11308	0.12%	0.010%
26	16.745	2335	2339	2346	rBV7	10089	17706	0.18%	0.015%
27	16.851	2353	2357	2361	rBV2	10638	16523	0.17%	0.014%
28	17.069	2387	2394	2402	rVB	4098152	5808558	60.50%	5.064%
29	17.169	2404	2411	2419	rBV	6343780	9259309	96.45%	8.072%
30	17.322	2432	2437	2452	rBV2	43923	116418	1.21%	0.101%
31	17.445	2455	2458	2463	rVB2	9222	14176	0.15%	0.012%
32	19.028	2723	2727	2733	rVB	74589	99490	1.04%	0.087%
33	19.098	2735	2739	2744	rVV	67180	93387	0.97%	0.081%
34	19.463	2795	2801	2809	rBV	6293973	8577936	89.35%	7.478%
35	21.298	3108	3113	3120	rBV2	2822414	4285001	44.63%	3.736%
36	24.039	3570	3579	3591	rVB2	3132040	7455824	77.66%	6.500%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031780.D
Acq On : 04 Jun 2024 17:33
Operator : MA/JU
Sample : PB161200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	24.233	3605	3612	3623	rVB	1739666	4453078	46.38%	3.882%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 114705705

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031780.D
Acq On : 04 Jun 2024 17:33
Operator : MA/JU
Sample : PB161200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

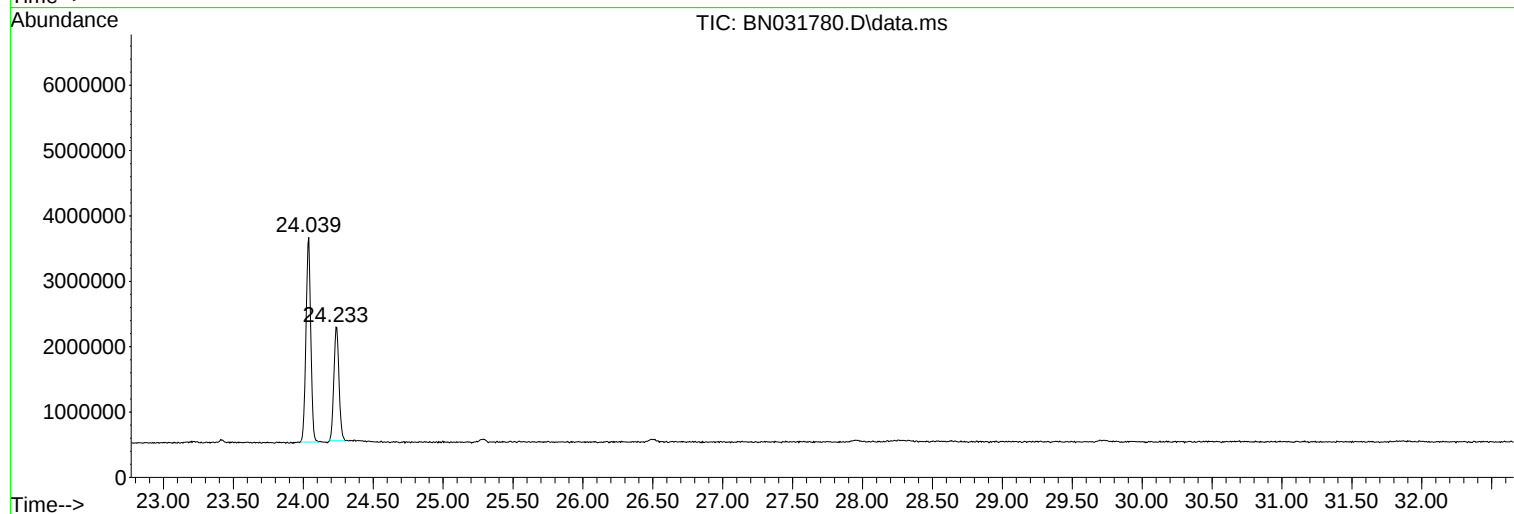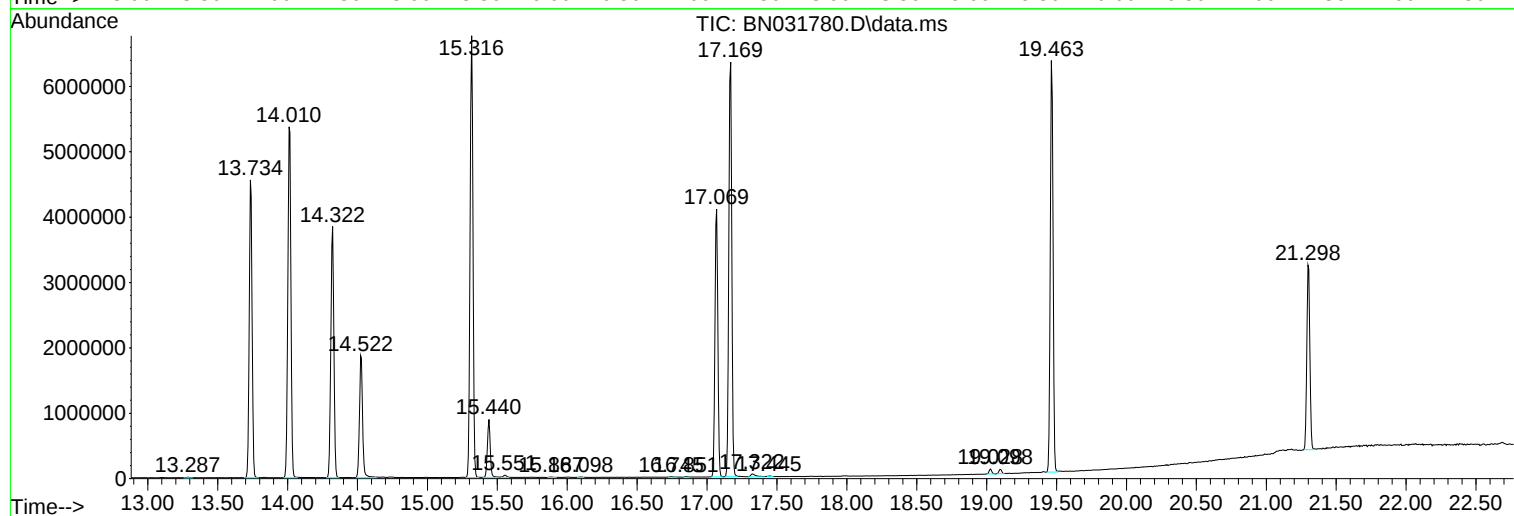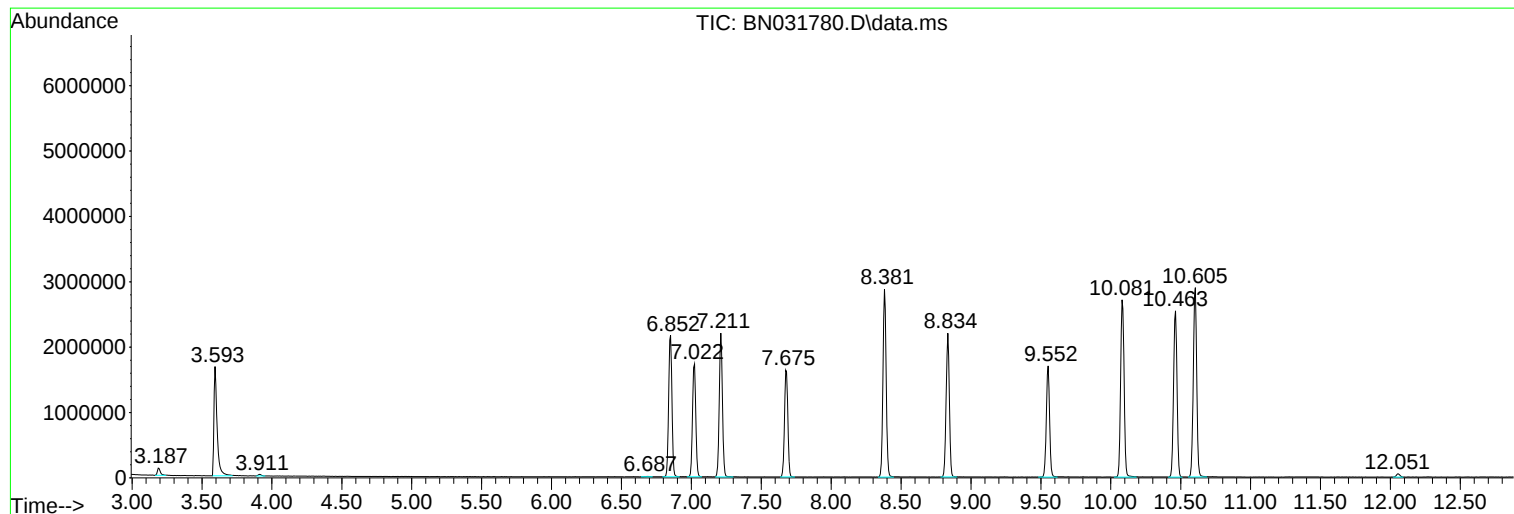

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031780.D
Acq On : 04 Jun 2024 17:33
Operator : MA/JU
Sample : PB161200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031780.D
Acq On : 04 Jun 2024 17:33
Operator : MA/JU
Sample : PB161200BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc