

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
 Data File : BN031797.D
 Acq On : 05 Jun 2024 13:09
 Operator : MA/JU
 Sample : PB161224BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	45	rVB	55977	91459	1.03%	0.116%
2	3.587	99	102	125	rBV	739786	1240430	13.94%	1.573%
3	3.905	153	156	161	rVB	9963	13454	0.15%	0.017%
4	6.846	646	656	670	rBV	957244	1521542	17.10%	1.930%
5	7.016	678	685	695	rVB	793978	1262468	14.19%	1.601%
6	7.205	709	717	727	rBV	926628	1545203	17.37%	1.960%
7	7.675	790	797	808	rVB	909403	1474363	16.57%	1.870%
8	8.381	908	917	928	rBV	1188559	1997780	22.46%	2.534%
9	8.828	983	993	1004	rBV	914309	1542904	17.34%	1.957%
10	9.546	1106	1115	1128	rBV	754342	1274764	14.33%	1.617%
11	10.081	1198	1206	1226	rBV	1136547	1968080	22.12%	2.496%
12	10.457	1262	1270	1278	rBV	1375211	2313167	26.00%	2.934%
13	10.599	1286	1294	1305	rBV	1305271	2248219	25.27%	2.852%
14	12.046	1536	1540	1547	rVB2	21256	39025	0.44%	0.050%
15	13.734	1819	1827	1841	rBV	2532740	3632677	40.83%	4.608%
16	14.010	1865	1874	1883	rBV	2798336	4124113	46.36%	5.231%
17	14.316	1918	1926	1934	rBV	2434056	3544005	39.84%	4.495%
18	14.428	1940	1945	1950	rBV8	5402	10021	0.11%	0.013%
19	14.528	1953	1962	1984	rBV	1298304	2050350	23.05%	2.601%
20	15.310	2088	2095	2102	rBV	3504668	5201451	58.47%	6.598%
21	15.440	2109	2117	2132	rBV	1187225	1688349	18.98%	2.142%
22	15.551	2132	2136	2145	rVB2	22108	36477	0.41%	0.046%
23	16.092	2225	2228	2235	rVB7	6847	12375	0.14%	0.016%
24	16.851	2353	2357	2361	rBV3	8386	11934	0.13%	0.015%
25	17.063	2387	2393	2403	rVB	3209457	4601721	51.72%	5.837%
26	17.163	2403	2410	2422	rBV2	4223182	6145392	69.08%	7.795%
27	17.445	2454	2458	2465	rVB3	10223	17320	0.19%	0.022%
28	17.963	2542	2546	2554	rBV4	30590	65810	0.74%	0.083%
29	19.028	2723	2727	2734	rBV3	63893	103743	1.17%	0.132%
30	19.092	2735	2738	2746	rVV	56568	93255	1.05%	0.118%
31	19.257	2763	2766	2770	rBV5	33322	45569	0.51%	0.058%
32	19.463	2795	2801	2808	rBV	5592582	7550551	84.87%	9.577%
33	21.304	3108	3114	3122	rBV	3769220	5628910	63.27%	7.140%
34	24.039	3570	3579	3590	rVB2	3600909	8896541	100.00%	11.285%
35	24.245	3605	3614	3626	rVB	2652825	6844949	76.94%	8.682%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031797.D
Acq On : 05 Jun 2024 13:09
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK224

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 78838371

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031797.D
Acq On : 05 Jun 2024 13:09
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

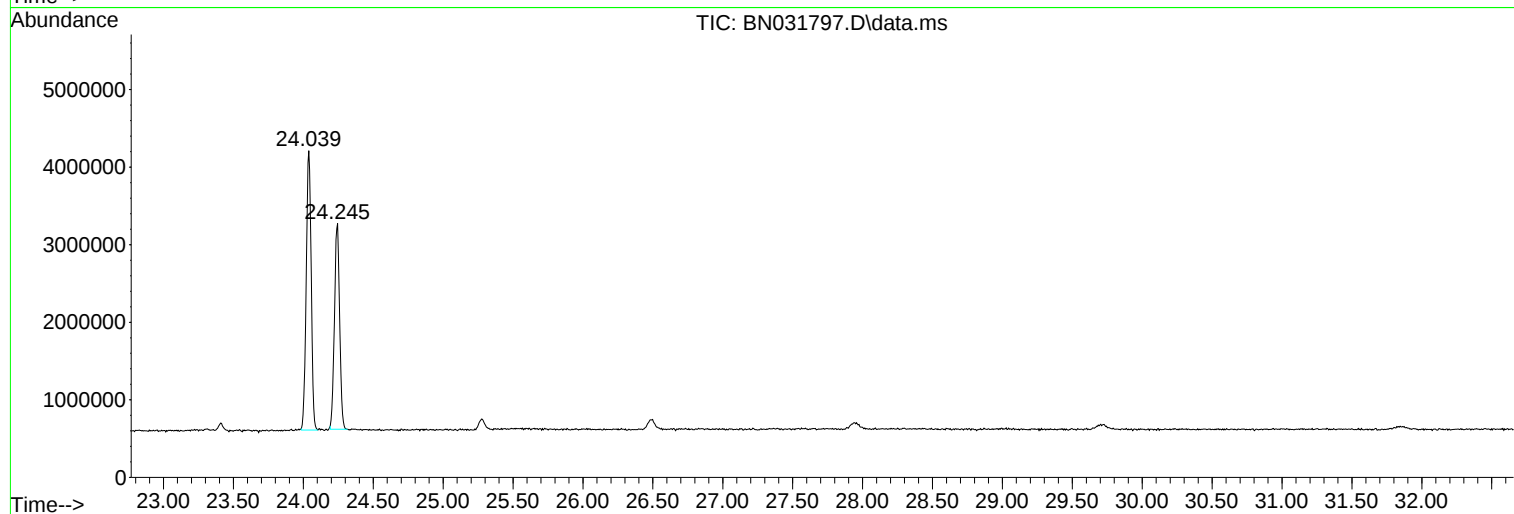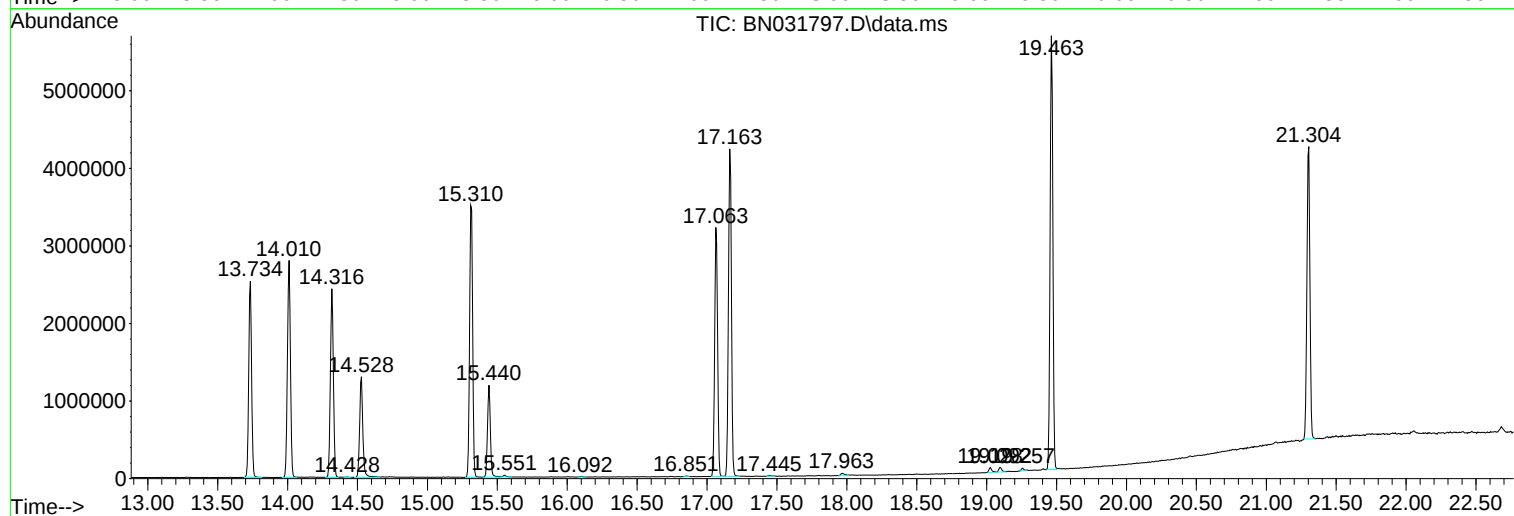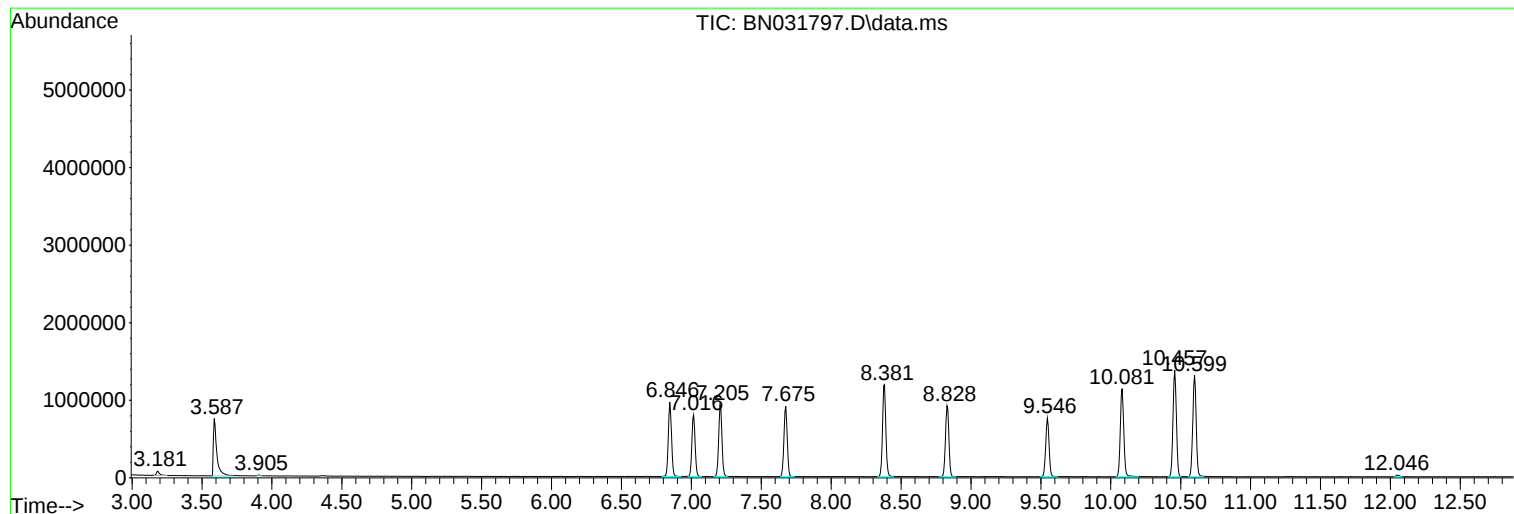

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031797.D
Acq On : 05 Jun 2024 13:09
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060524\
Data File : BN031797.D
Acq On : 05 Jun 2024 13:09
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc