

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006154.D
 Acq On : 07 Jun 2019 02:56
 Operator : JU/SJ
 Sample : K3016-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C7

Quant Time: Jun 07 03:55:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	5066	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	19091	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	9837	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1154676	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.35	264	1003092	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	7287	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
7) Acenaphthylene	14.01	152	2466	0.045	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006154.D
Acq On : 07 Jun 2019 02:56
Operator : JU/SJ
Sample : K3016-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C7

Quant Time: Jun 07 03:55:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

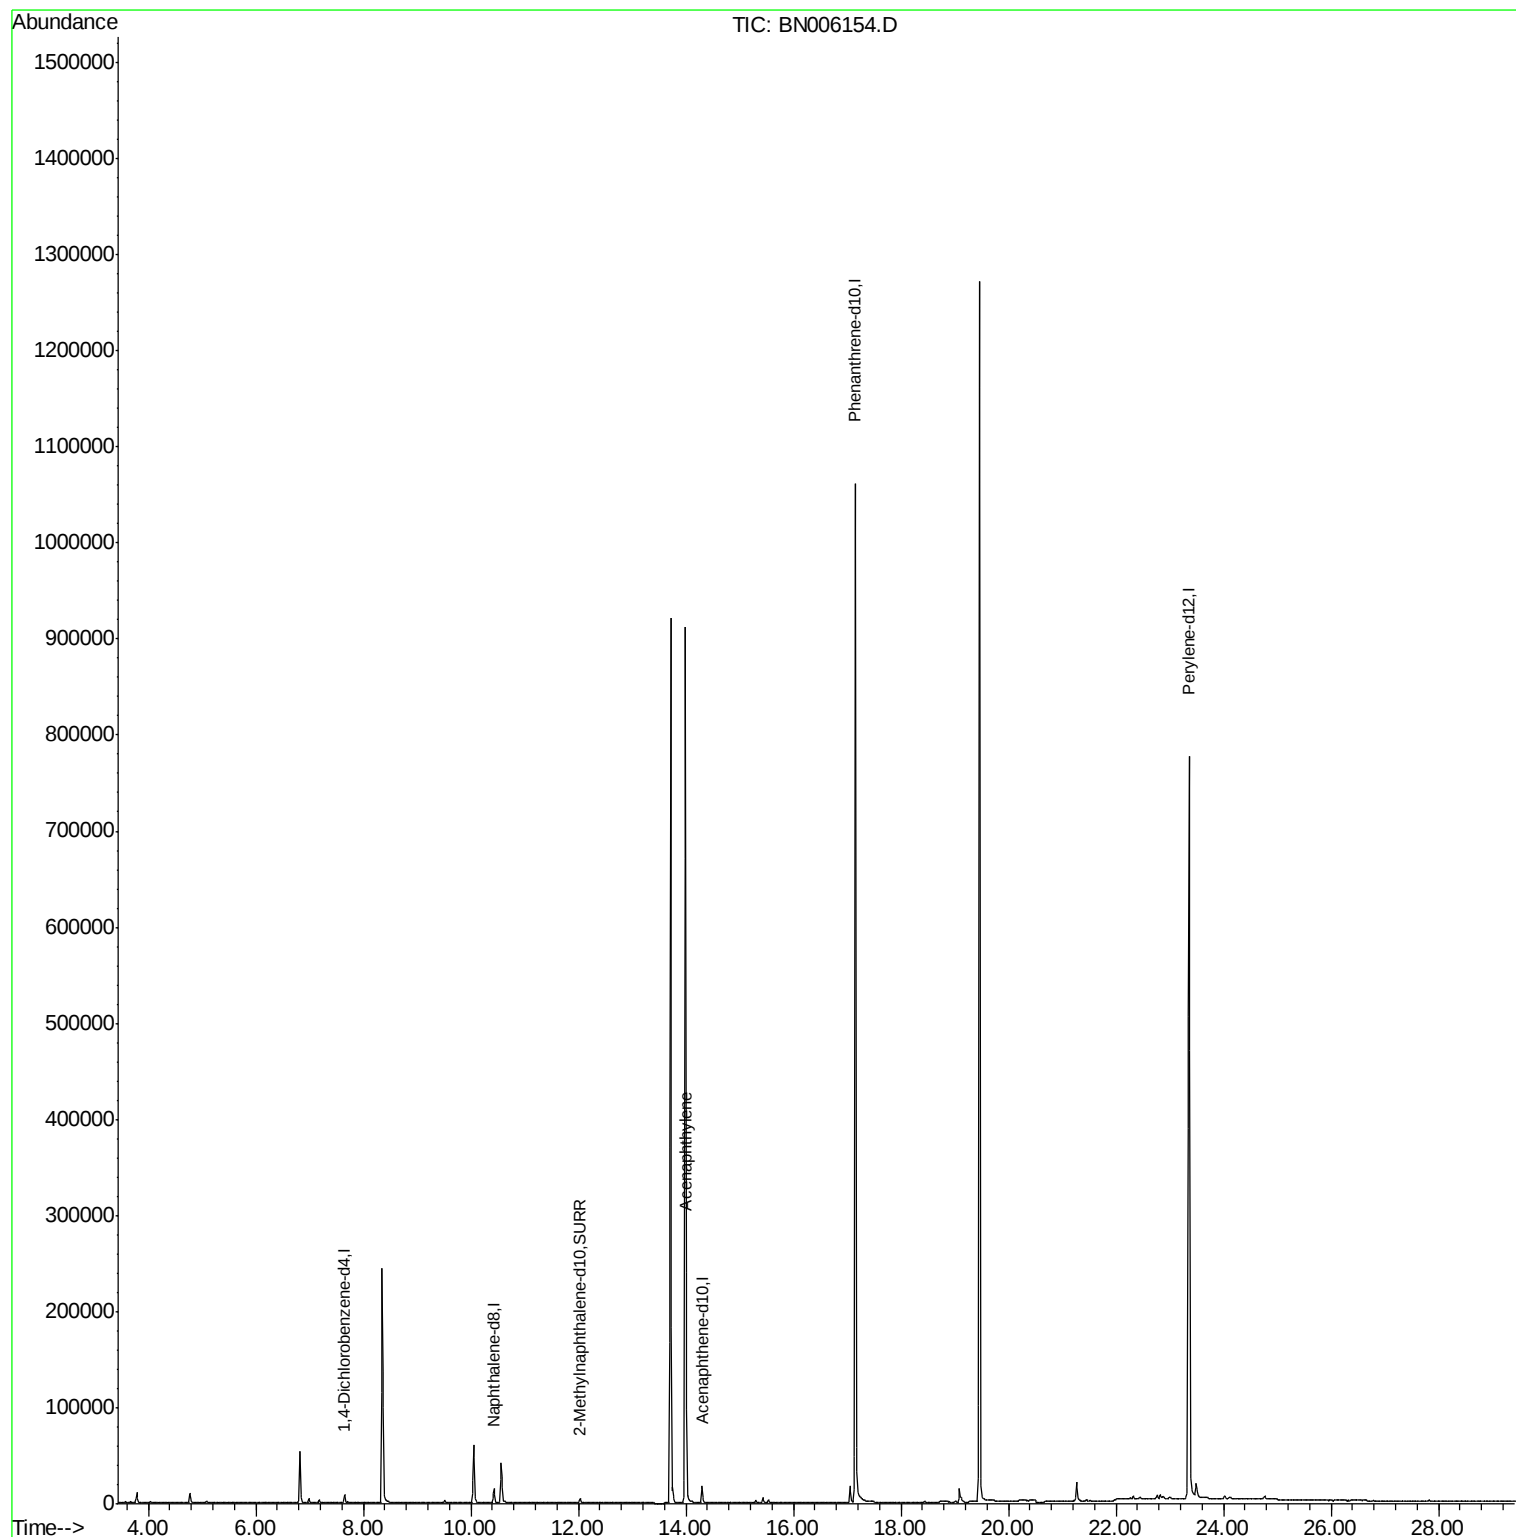

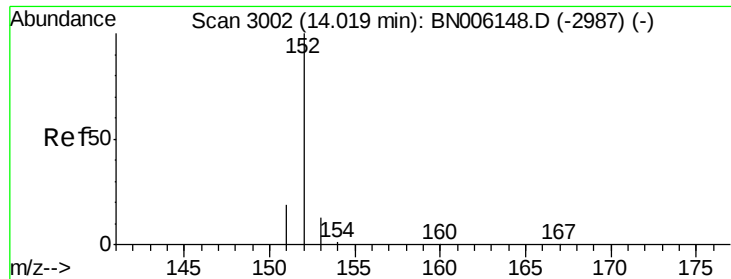

#7

Acenaphthylene

Concen: 0.045 ng/ul

RT: 14.01 min Scan# 3001

Delta R.T. -0.00 min

Lab File: BN006154.D

Acq: 07 Jun 2019 02:56

Instrument :

BNA_N

ClientSampleId :

A51C7

Tgt Ion:152 Resp: 2466

Ion Ratio Lower Upper

152 100

151 26.7 15.8 23.8#

153 20.9 10.8 16.2#

