

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006160.D
 Acq On : 07 Jun 2019 06:23
 Operator : JU/SJ
 Sample : K3016-19
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51D6

Quant Time: Jun 07 06:57:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	5778	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	21467	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10996	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1011322	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.50	264	29379	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	5409	0.16	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.36	252	3218	0.028	ng/ul#	Qvalue 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006160.D
Acq On : 07 Jun 2019 06:23
Operator : JU/SJ
Sample : K3016-19
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D6

Quant Time: Jun 07 06:57:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

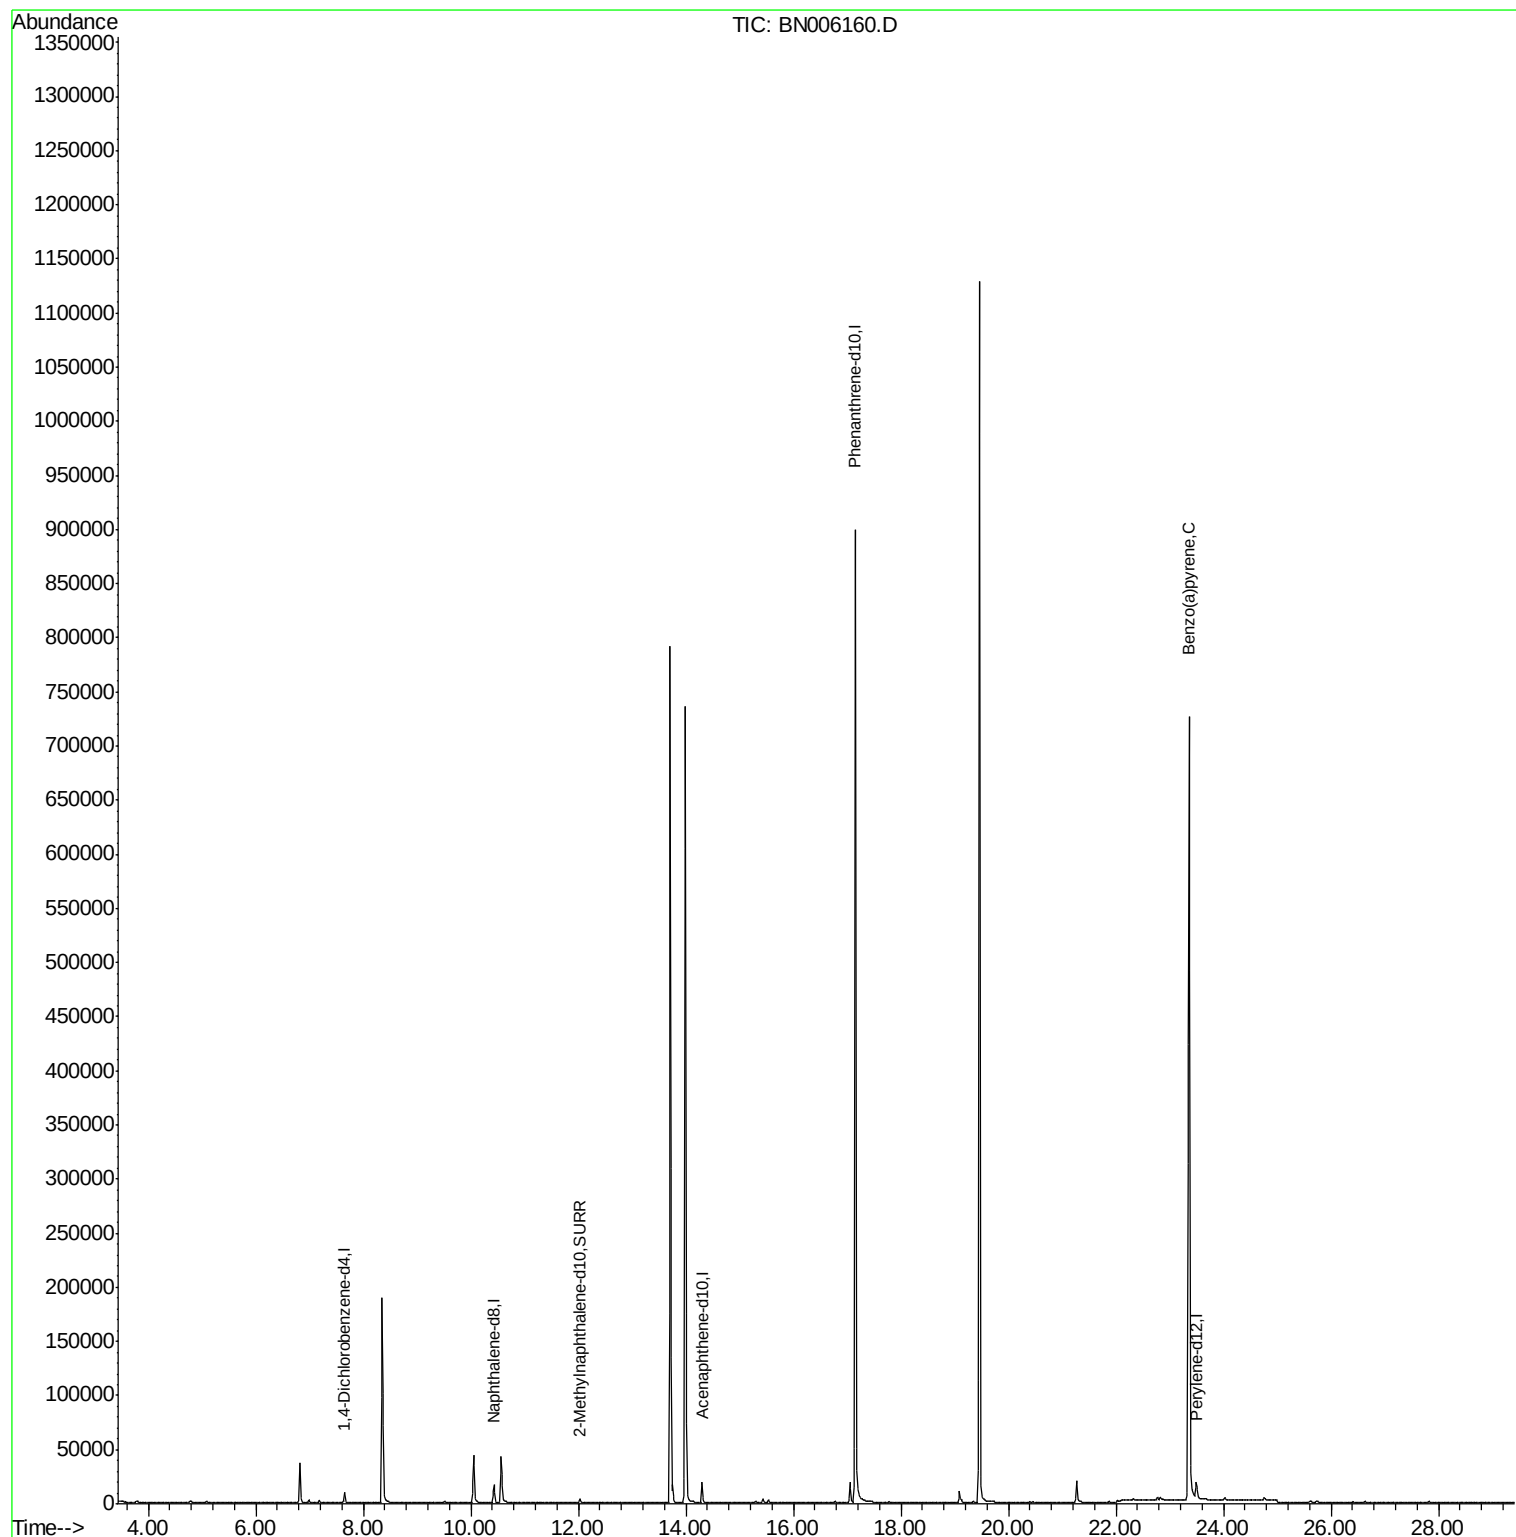

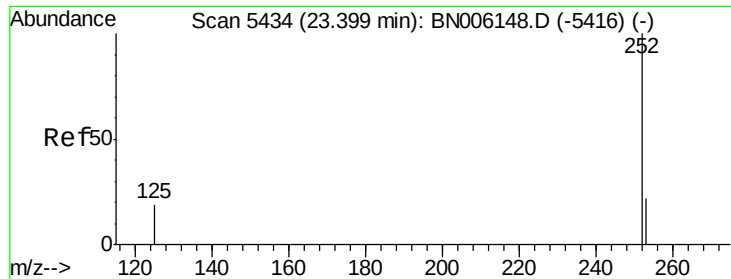

#23

Benzo(a)pyrene

Concen: 0.028 ng/ul

RT: 23.36 min Scan# 5419

Delta R.T. -0.04 min

Lab File: BN006160.D


Acq: 07 Jun 2019 06:23

Instrument :

BNA_N

ClientSampleId :

A51D6

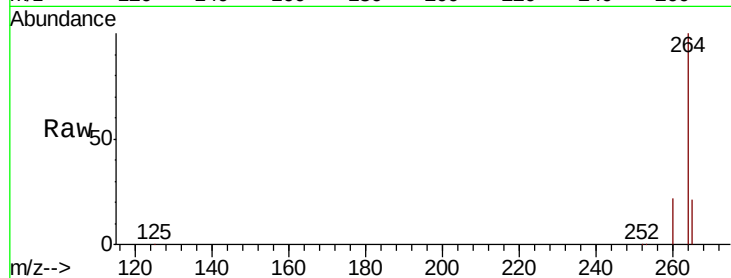


Tgt Ion: 252 Resp: 3218

Ion Ratio Lower Upper

252 100

253 47.0 21.1 31.7#

125 50.5 20.3 30.5#

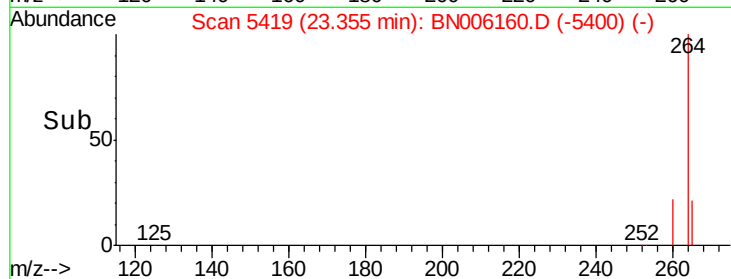

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

