

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:51:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

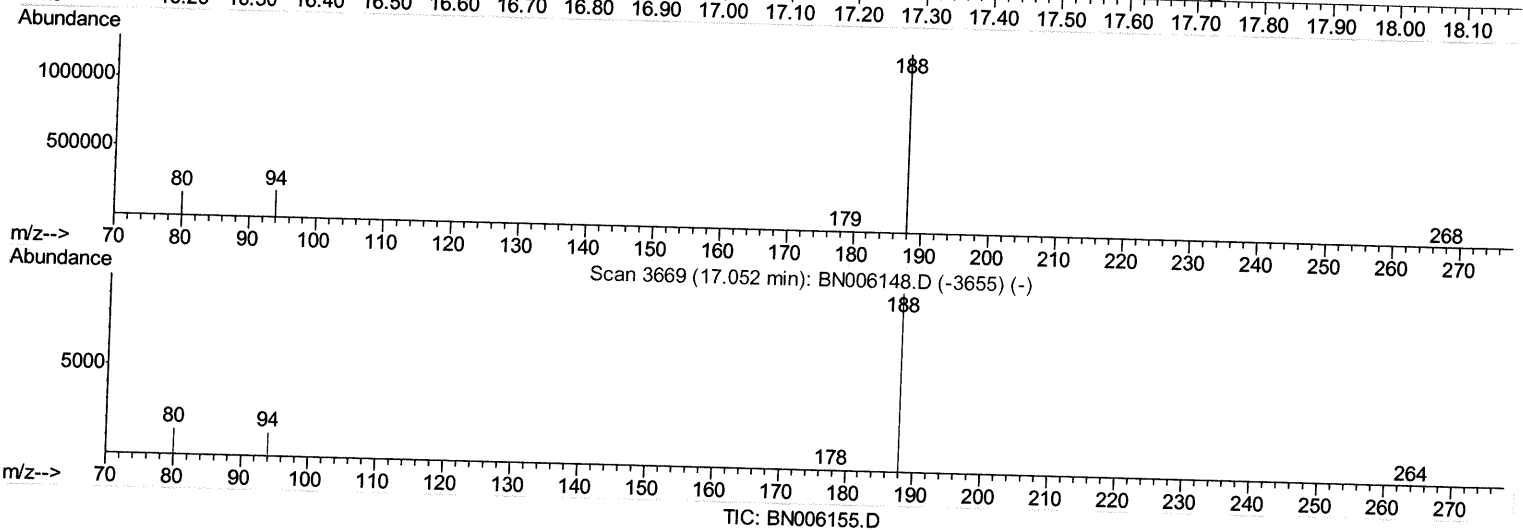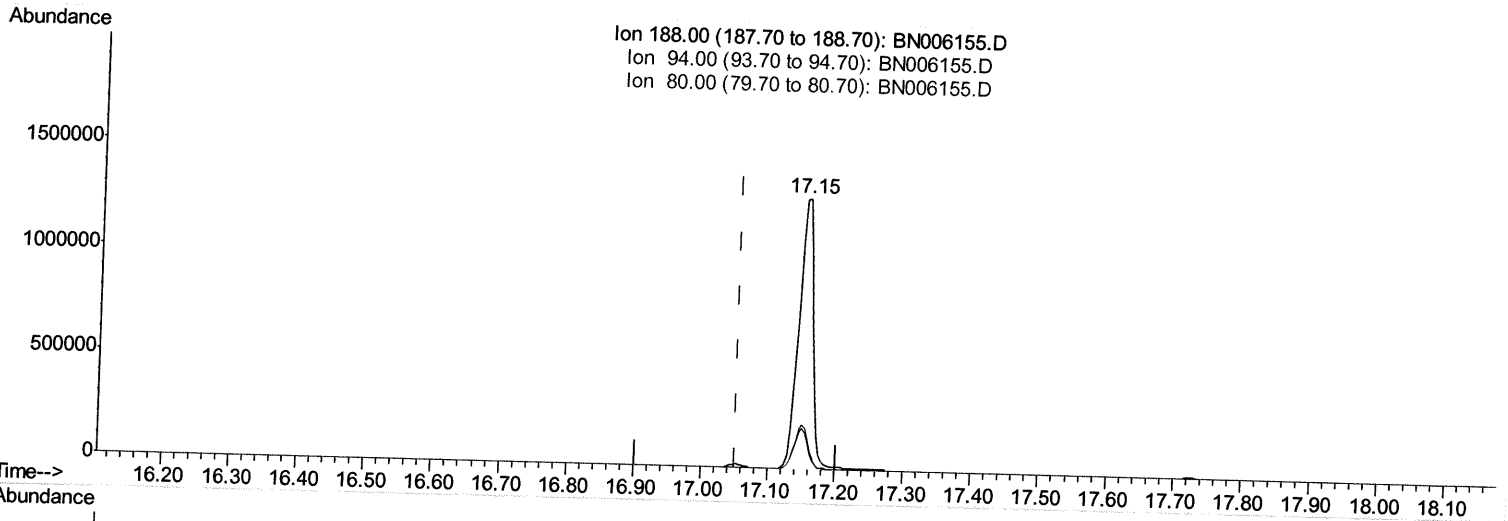

(10) Phenanthrene-d10 (I)

17.154min (+0.101) 0.40ng/ul

response 1879437

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.95
80.00	13.60	13.32
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:51:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

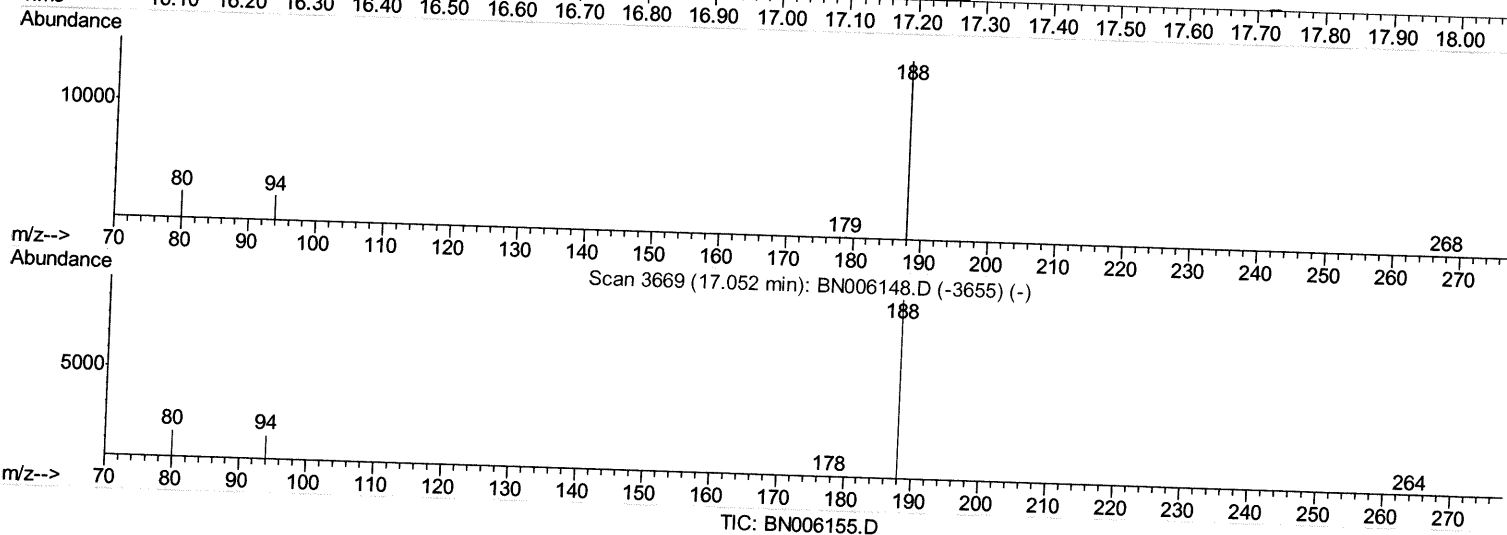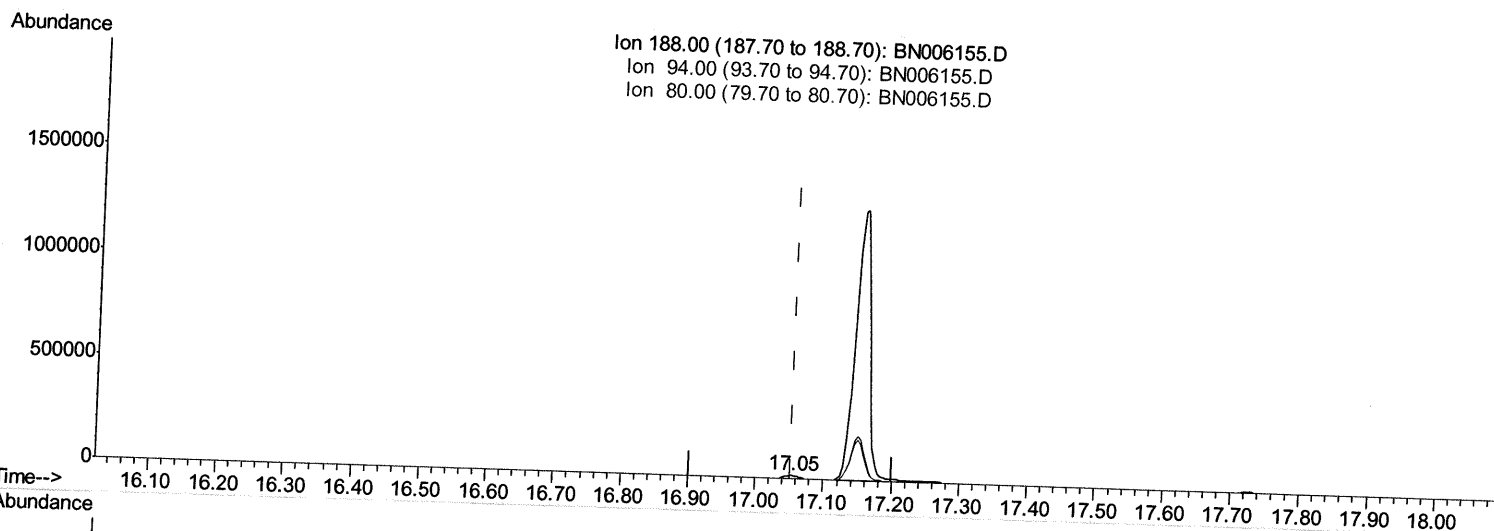

(10) Phenanthrene-d10 (I)

17.052min (+0.000) 0.40ng/ul m 06/10/19

response 21461

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.76
80.00	13.60	15.11
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:52:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

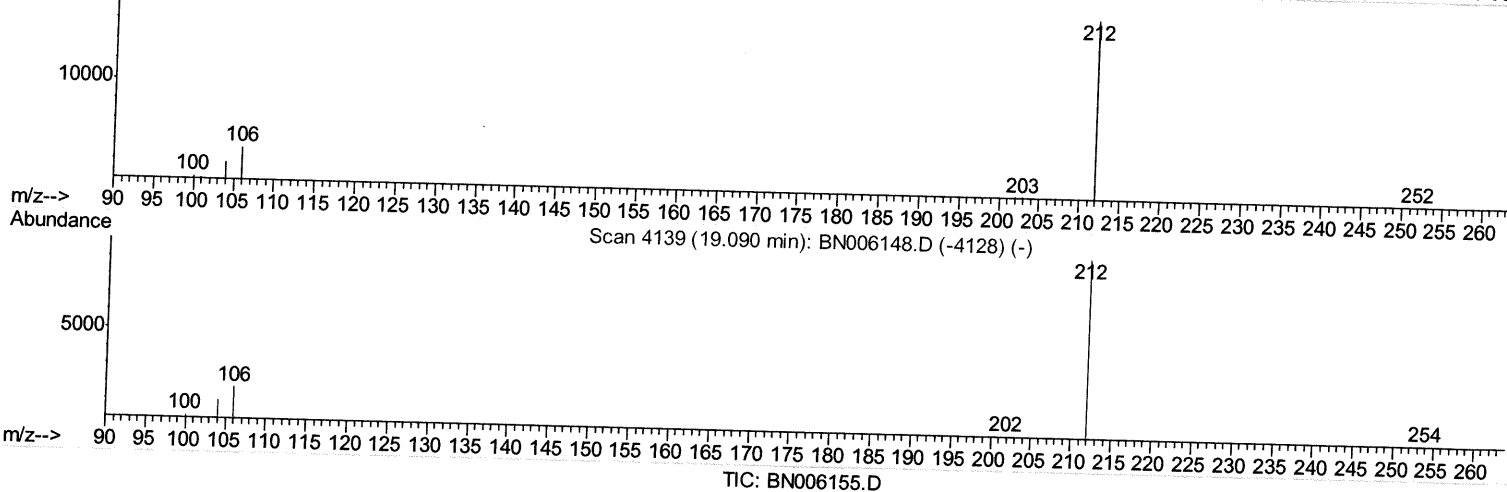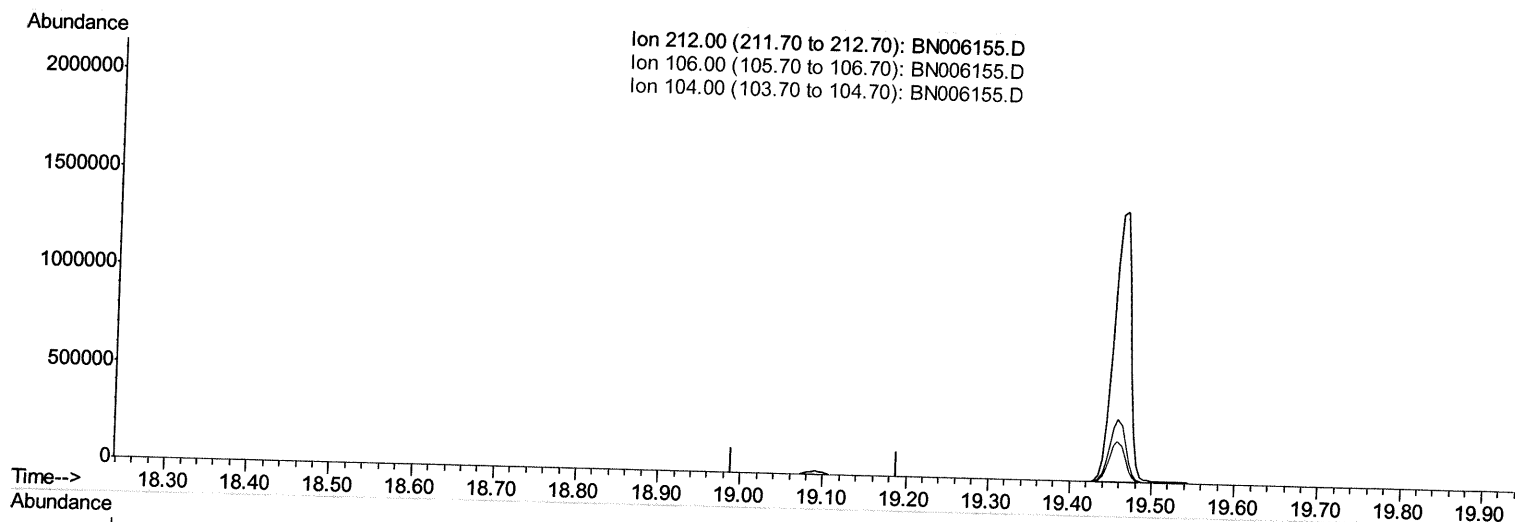

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006155.D
Acq On : 07 Jun 2019 03:30
Operator : JU/SJ
Sample : K3017-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51G1

Manual Integrations
APPROVED

mohammad
6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:52:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

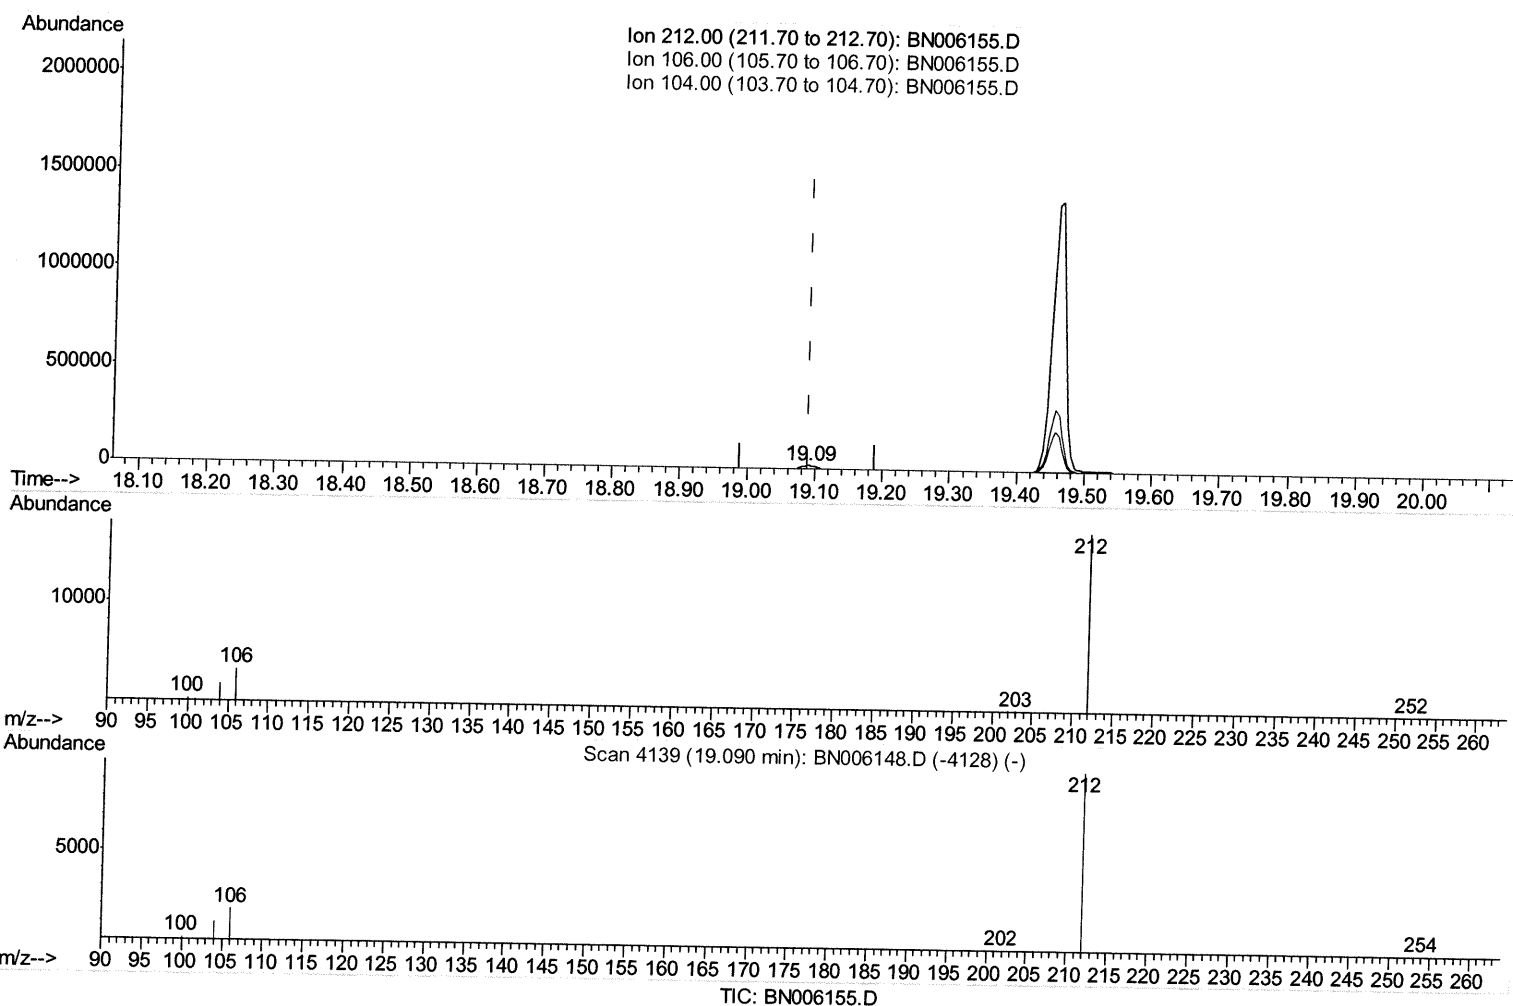

(14) Fluoranthene-d10 (SURR)

19.090min (+0.000) 0.43ng/ul m

JU
06/10/19

response 24529

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:52:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

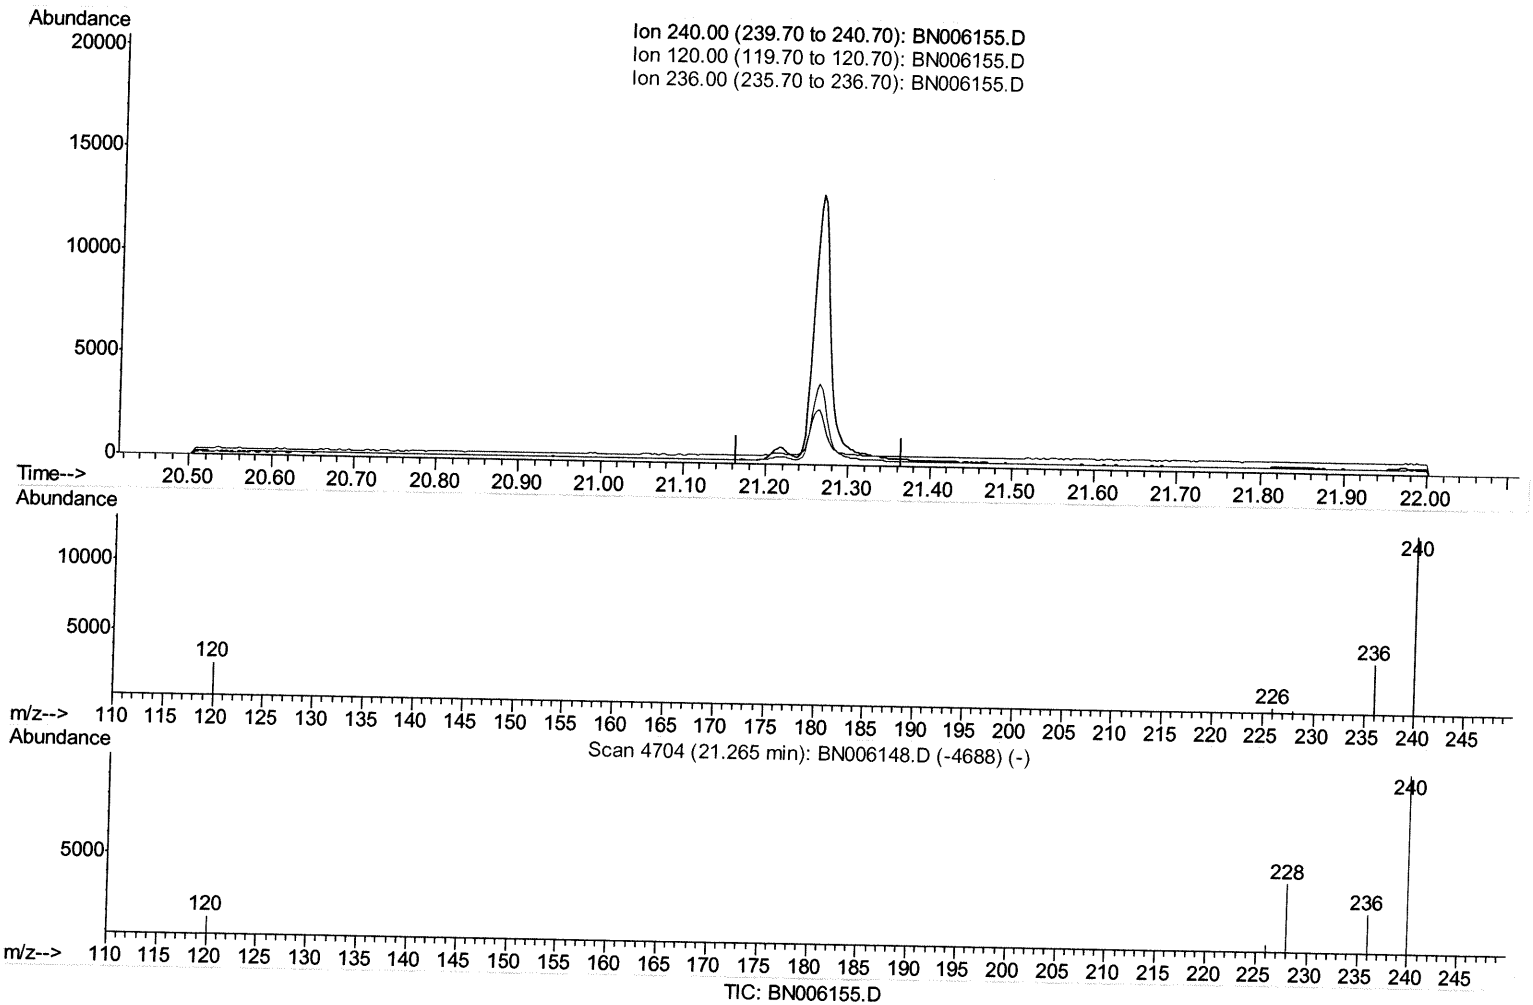

(16) Chrysene-d12 (I)

21.265min (-21.265) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:52:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

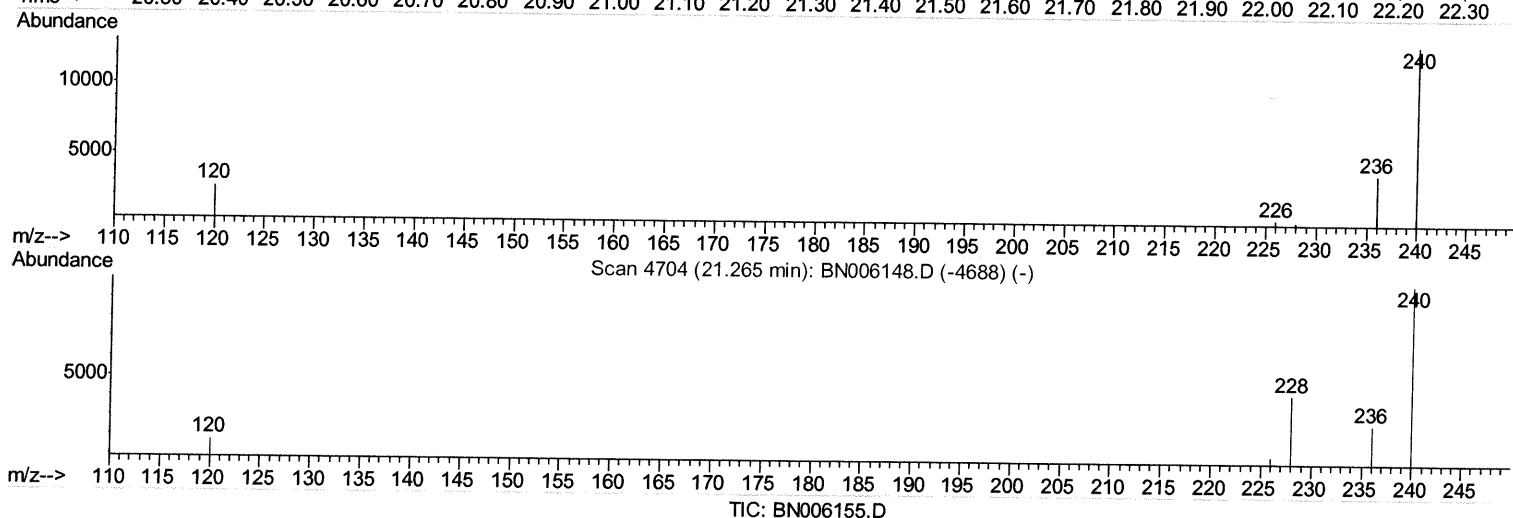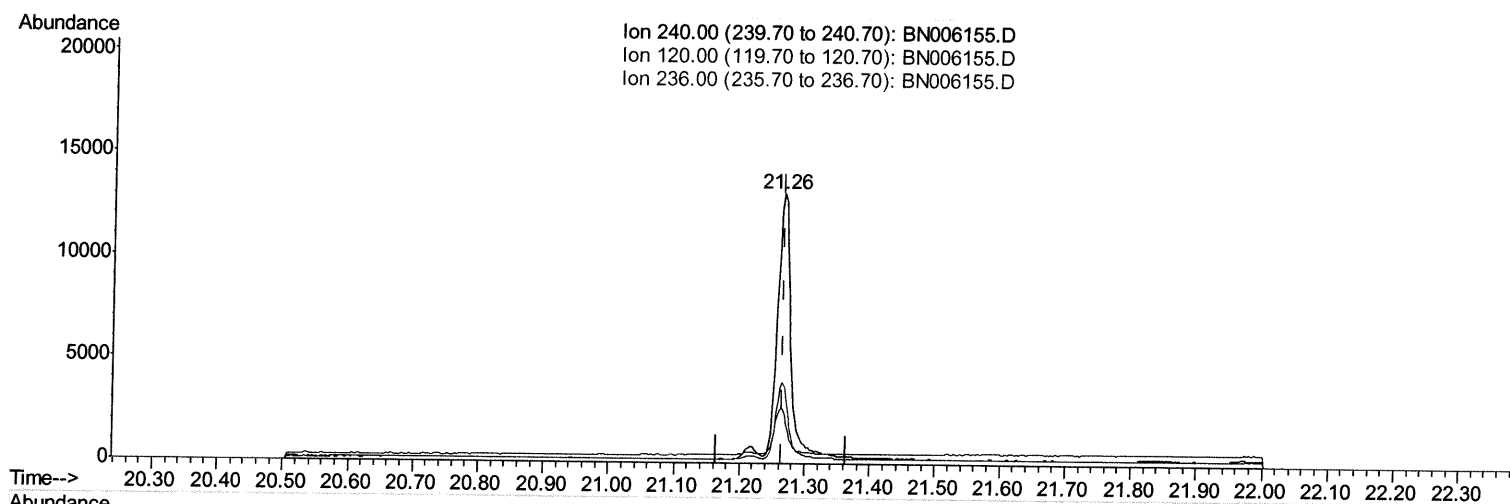

(16) Chrysene-d12 (I)

21.264min (-0.001) 0.40ng/ul m

response 19257

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	20.40
236.00	30.10	29.81
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:53:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

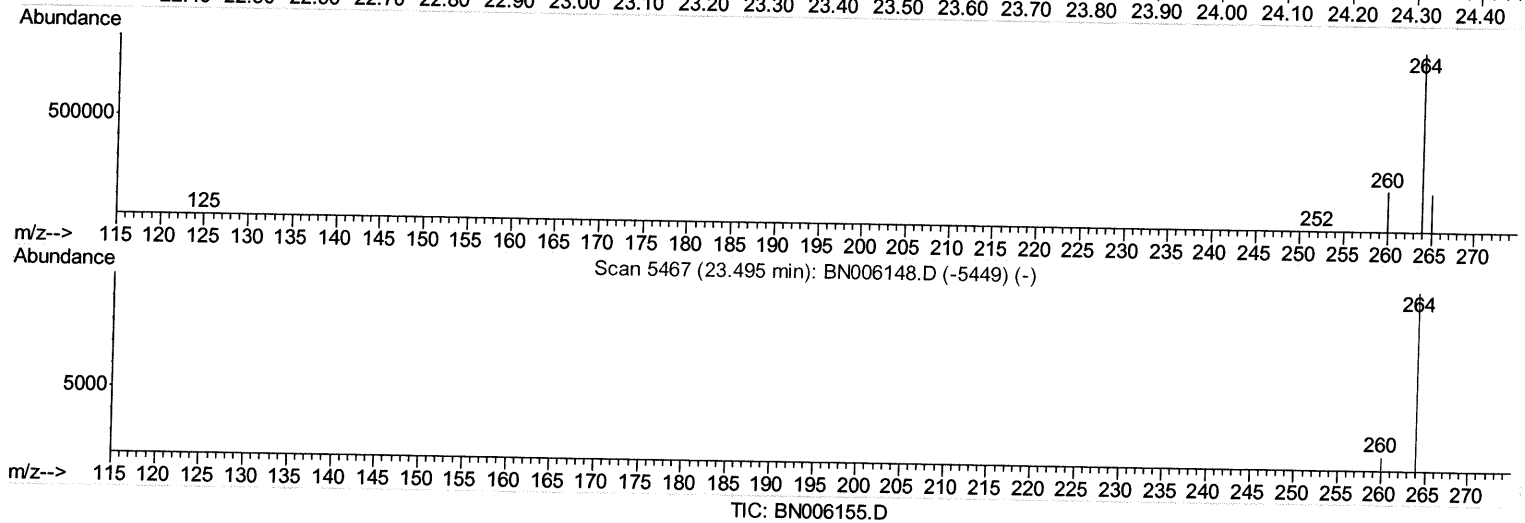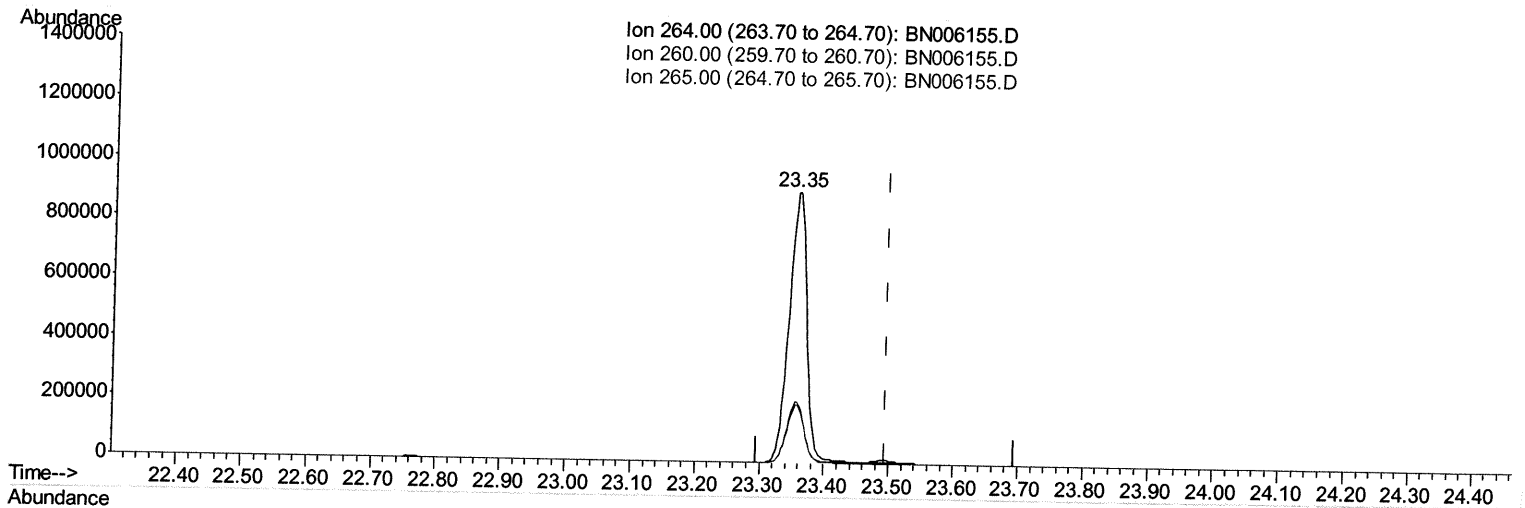

(20) Perylene-d12 (I)

23.354min (-0.141) 0.40ng/ul

response 1732362

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	22.52#
265.00	44.70	21.39#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006155.D
Acq On : 07 Jun 2019 03:30
Operator : JU/SJ
Sample : K3017-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51G1

Manual Integrations
APPROVED

mohammad
6/11/2019 5:07:56 PM

Quant Time: Jun 07 04:53:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

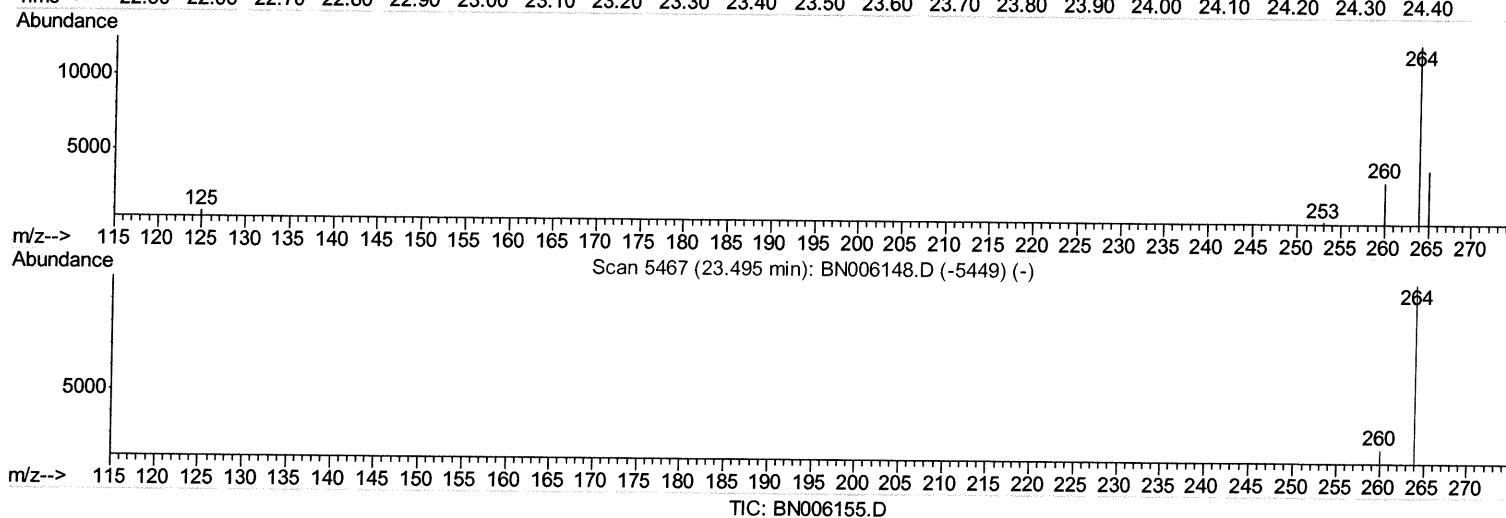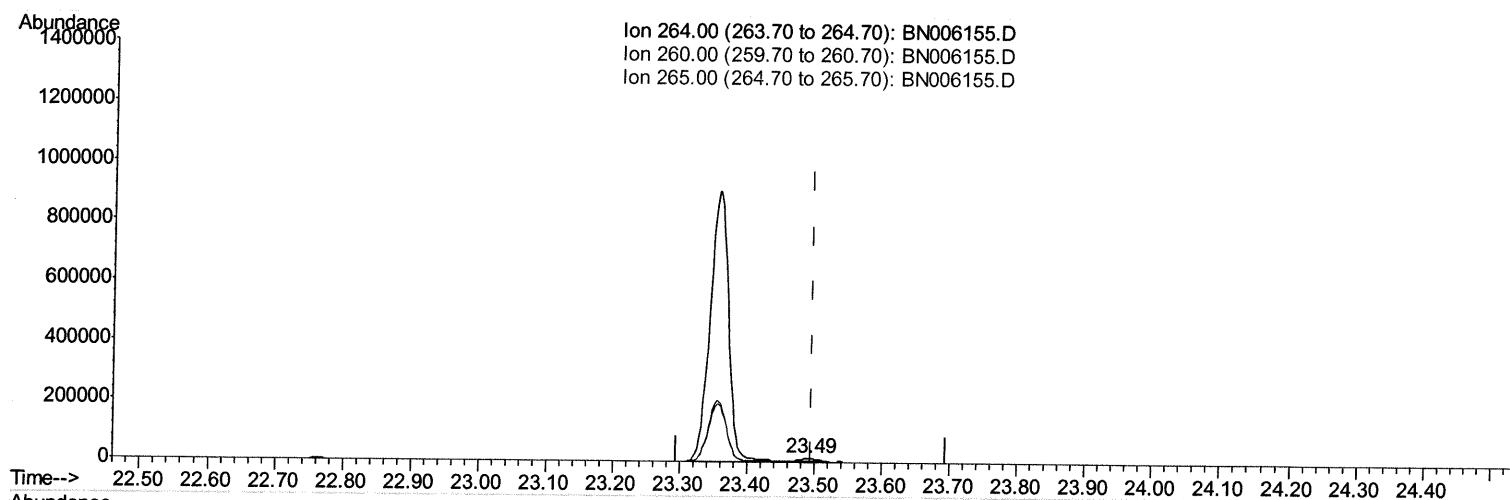

(20) Perylene-d12 (I)

23.491min (-0.004) 0.40ng/ul m

JU
06/10/19

response 15213

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.39
265.00	44.70	33.03#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060619\
 Data File : BN006155.D
 Acq On : 07 Jun 2019 03:30
 Operator : JU/SJ
 Sample : K3017-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 07 12:31:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 A51G1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:07:56 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	5919	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	22083	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	11633	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	21461m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	19257m	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	15213m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	12055	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	24529m	0.43	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.48	128	20988	0.344	ng/ul	Ovalue 100
7) Acenaphthylene	14.01	152	1594	0.025	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 06/10/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060619\
Data File : BN006155.D
Acq On : 07 Jun 2019 03:30
Operator : JU/SJ
Sample : K3017-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 07 12:31:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
A51G1

Manual Integrations
APPROVED

mohammad
6/11/2019 5:07:56 PM

