


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006157.D
Acq On : 07 Jun 2019 04:39
Operator : JU/SJ
Sample : K3016-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C6

Manual Integrations
APPROVED

mohammad
6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:44:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

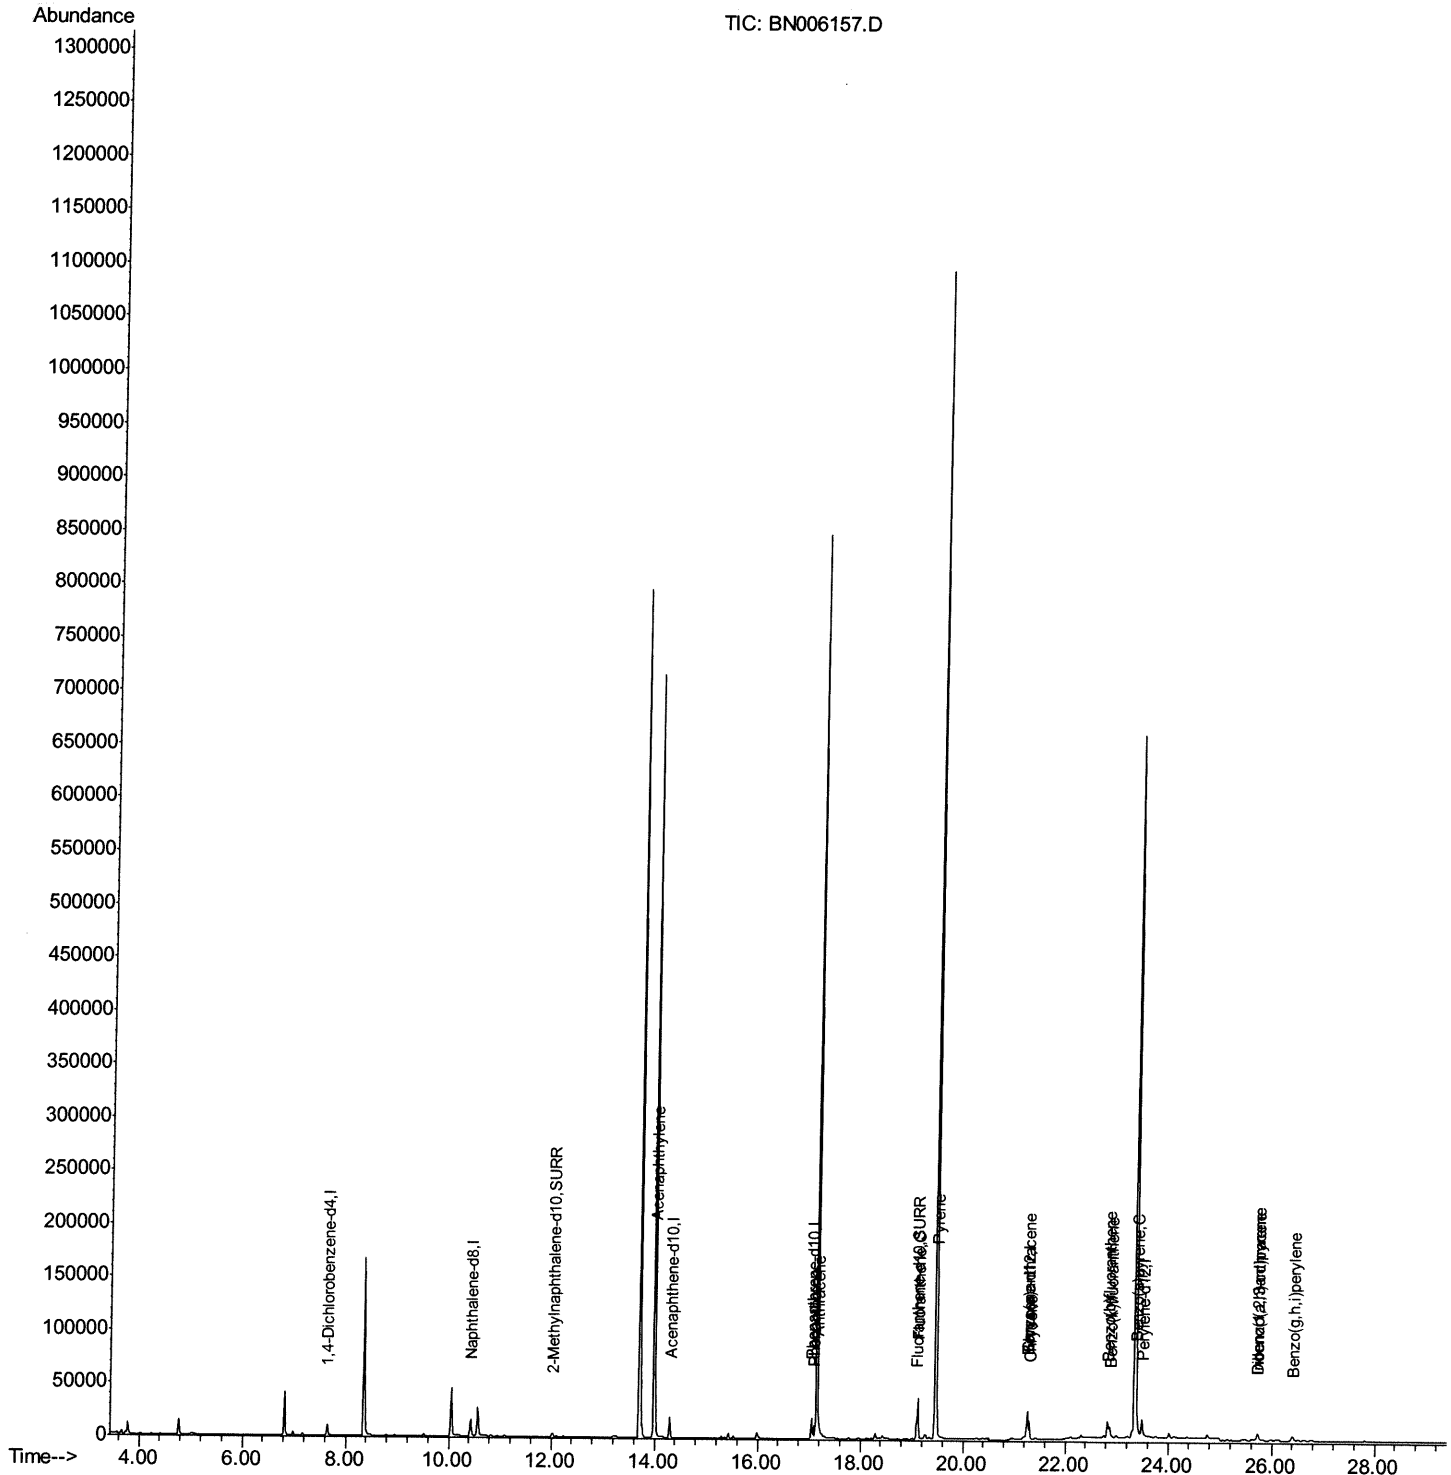

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:39:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

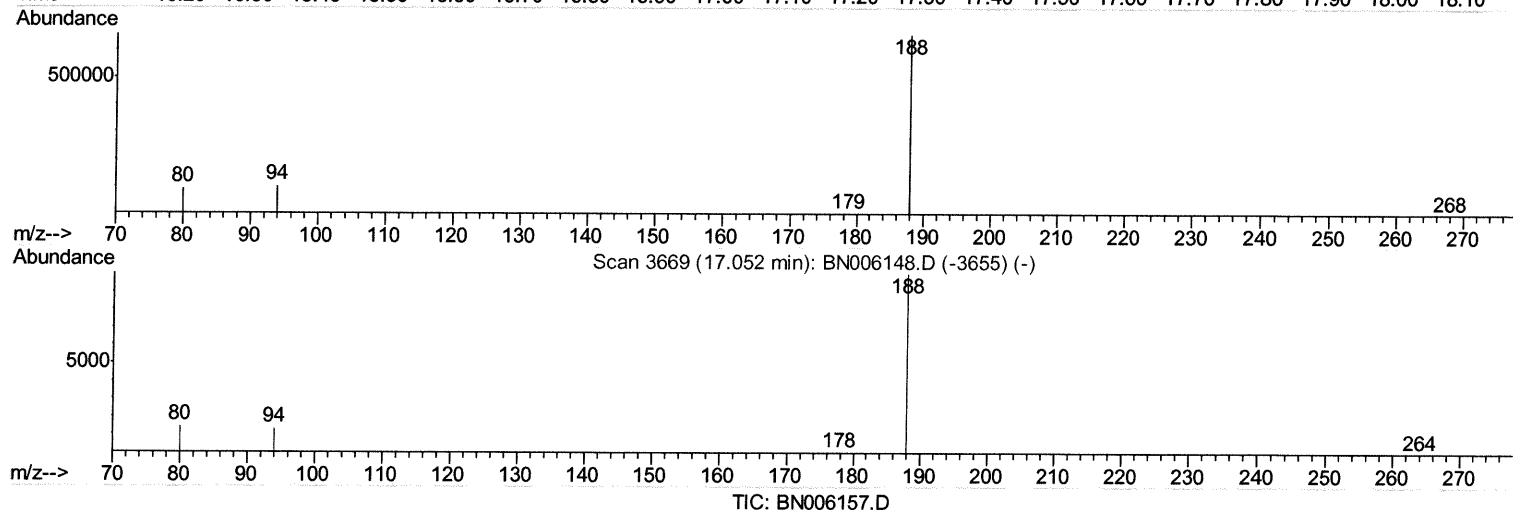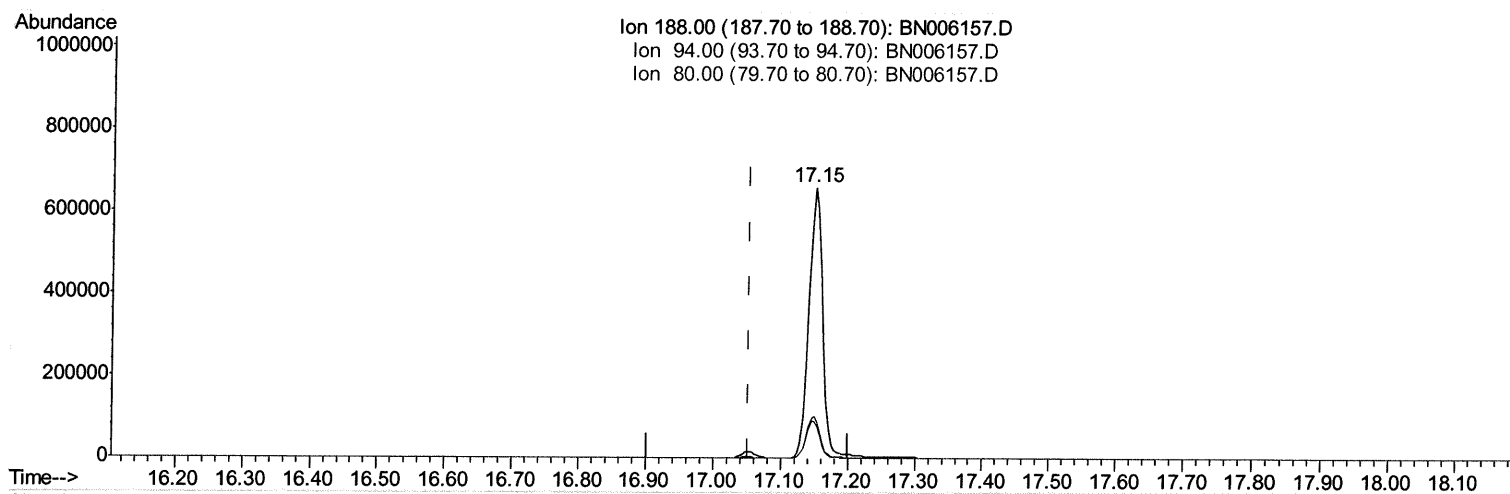

(10) Phenanthrene-d10 (I)

17.150min (+0.097) 0.40ng/ul

response 914602

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.41
80.00	13.60	13.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:39:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

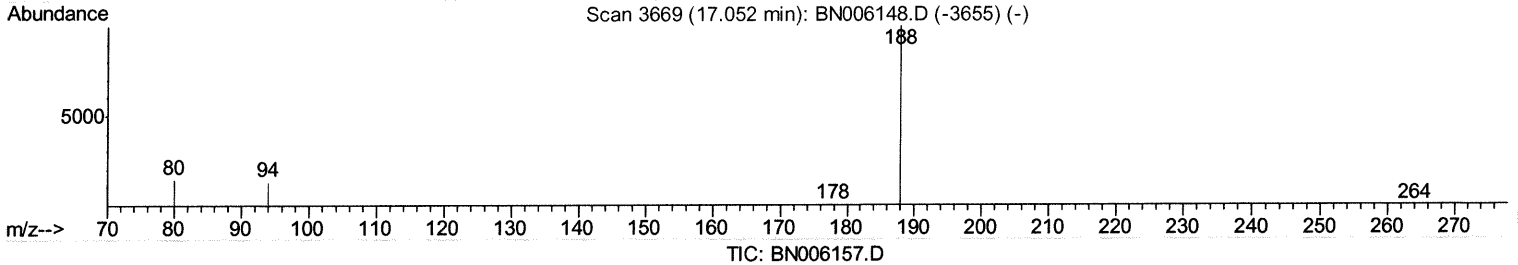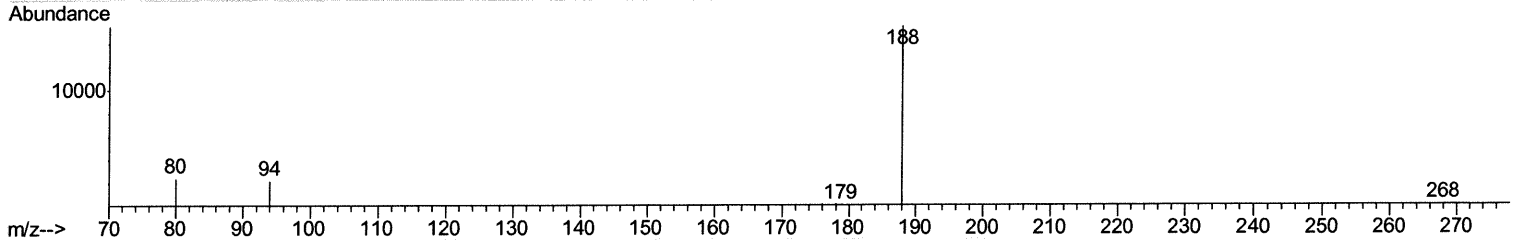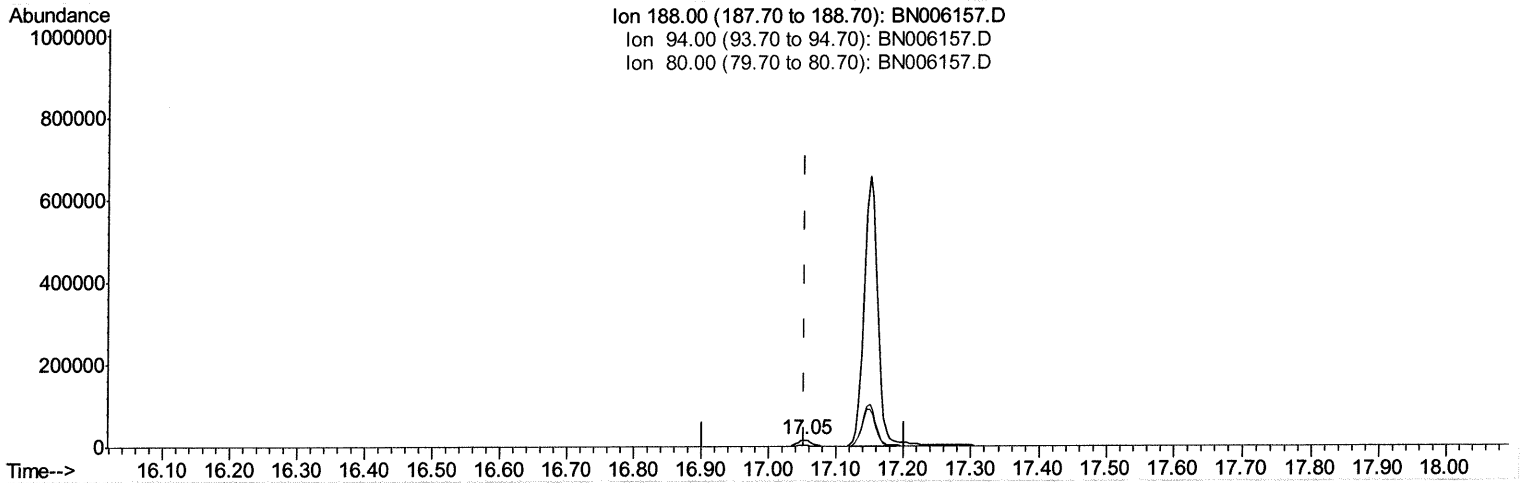

(10) Phenanthrene-d10 (I)

17.052min (+0.000) 0.40ng/ul m *JU* 06/10/19

response 22335

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.02
80.00	13.60	15.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

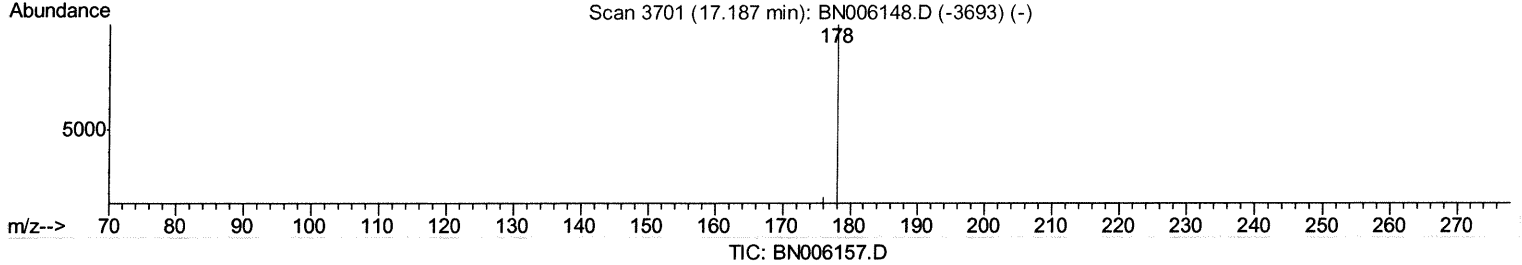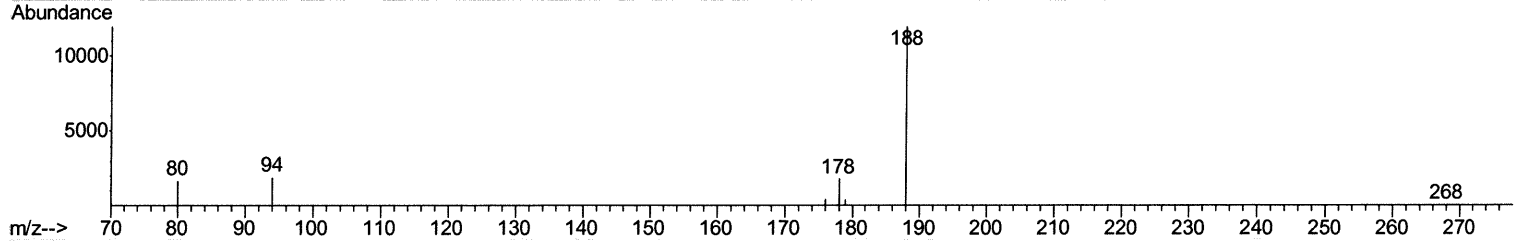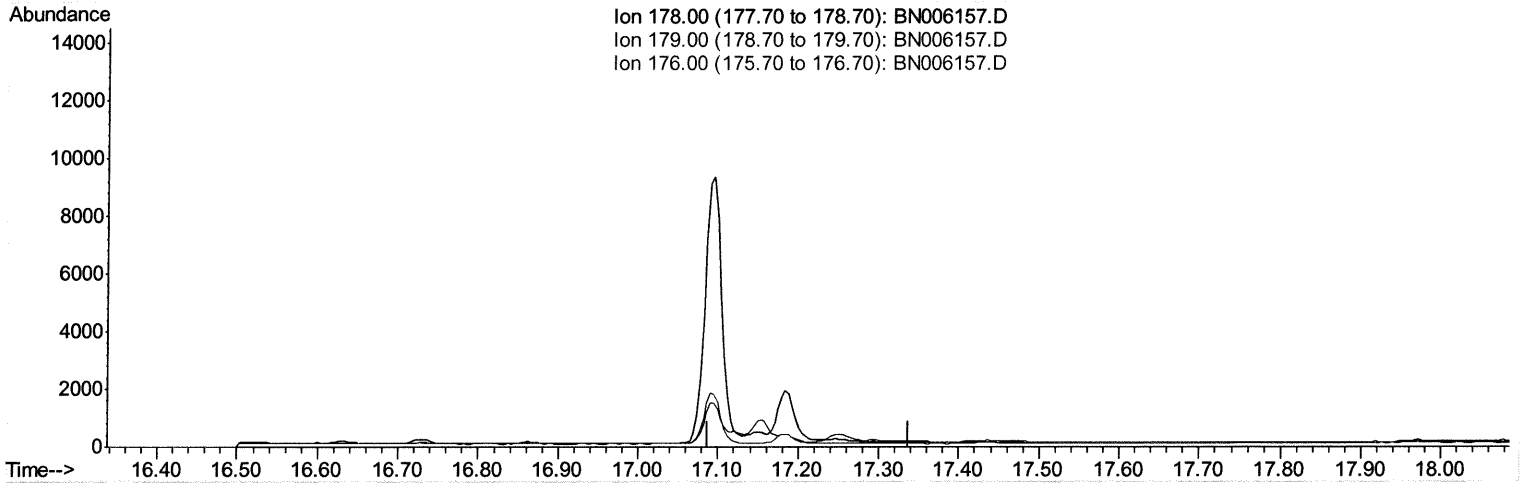

TIC: BN006157.D

(13) Anthracene

17.187min (-17.187) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.30	0.00#
176.00	18.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

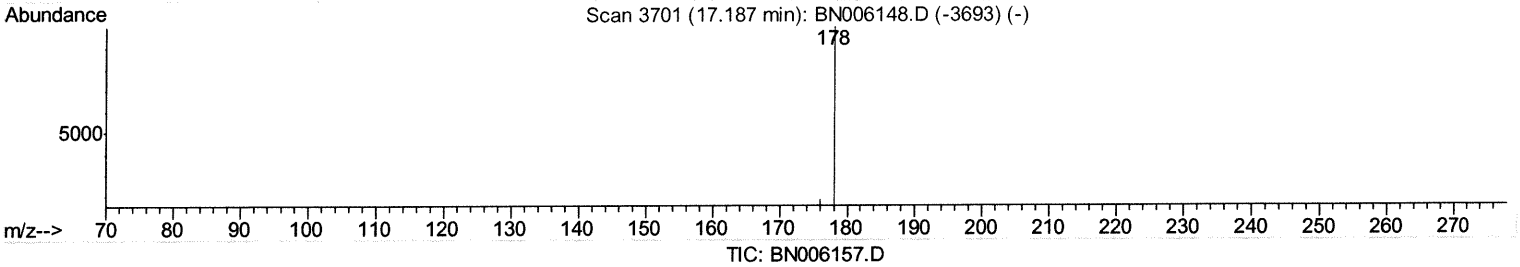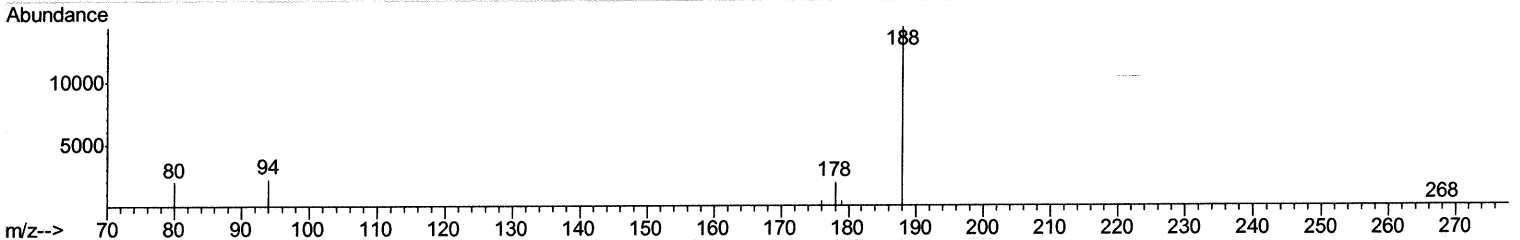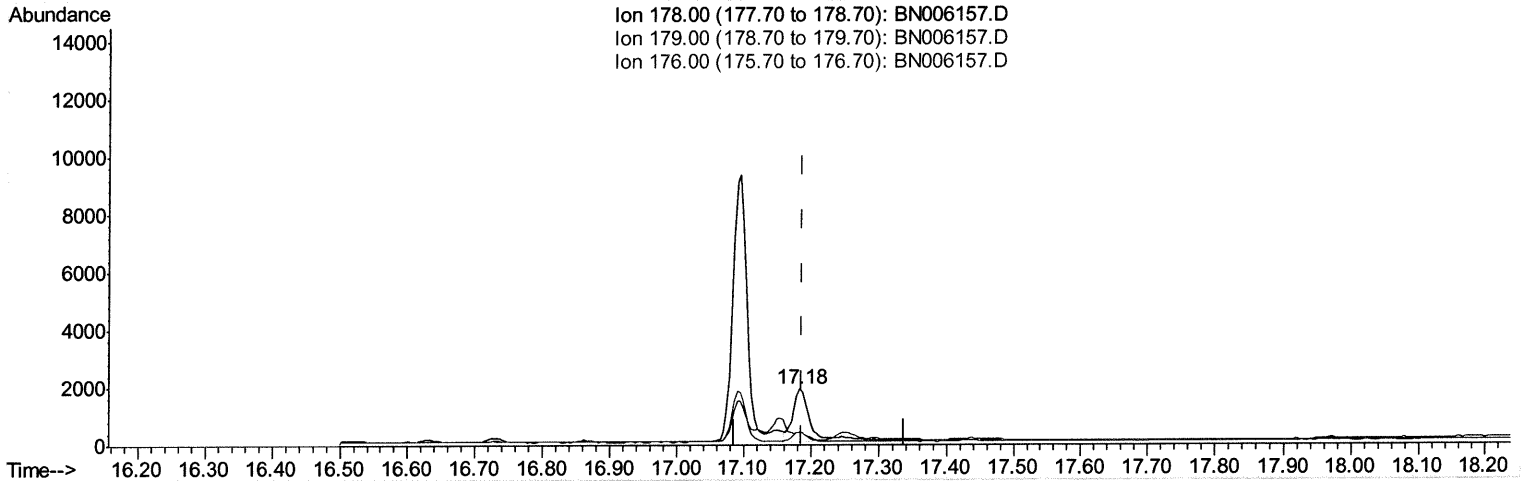

(13) Anthracene

17.183min (-0.004) 0.05ng/ul m 06/10/19

response 3217

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	22.63#
176.00	18.90	22.63
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

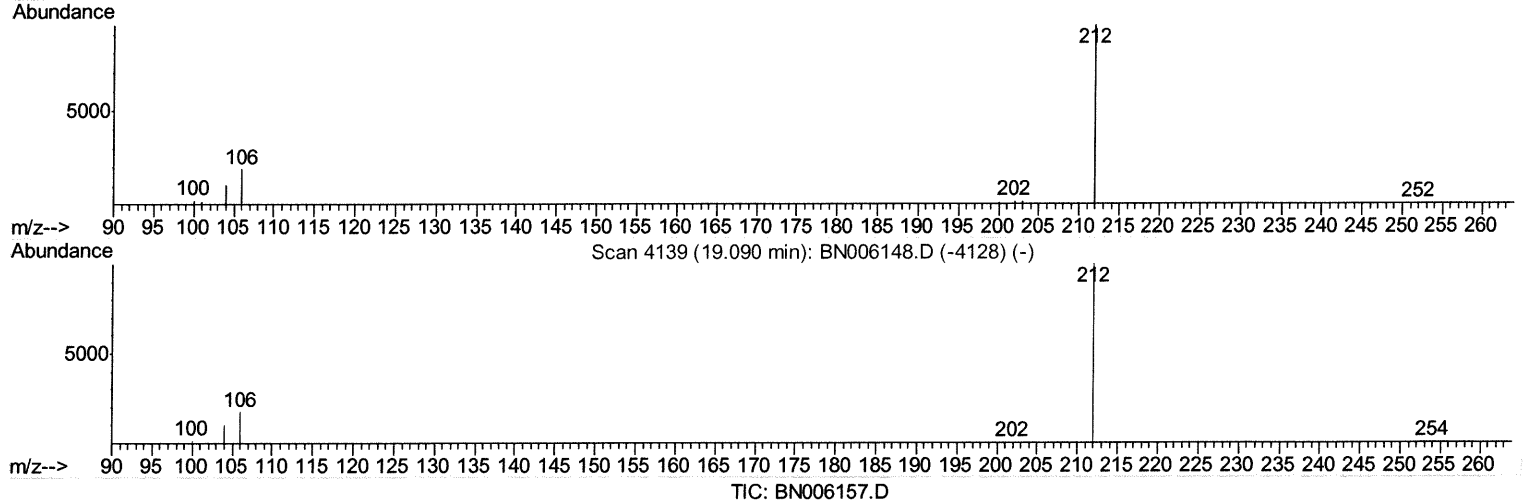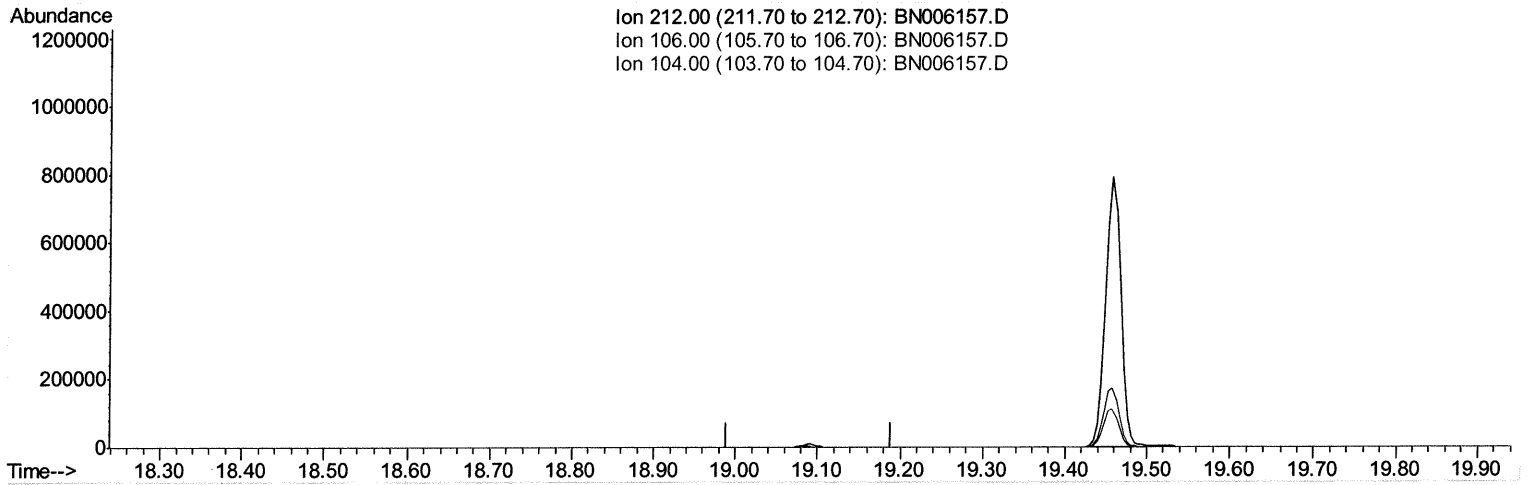

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

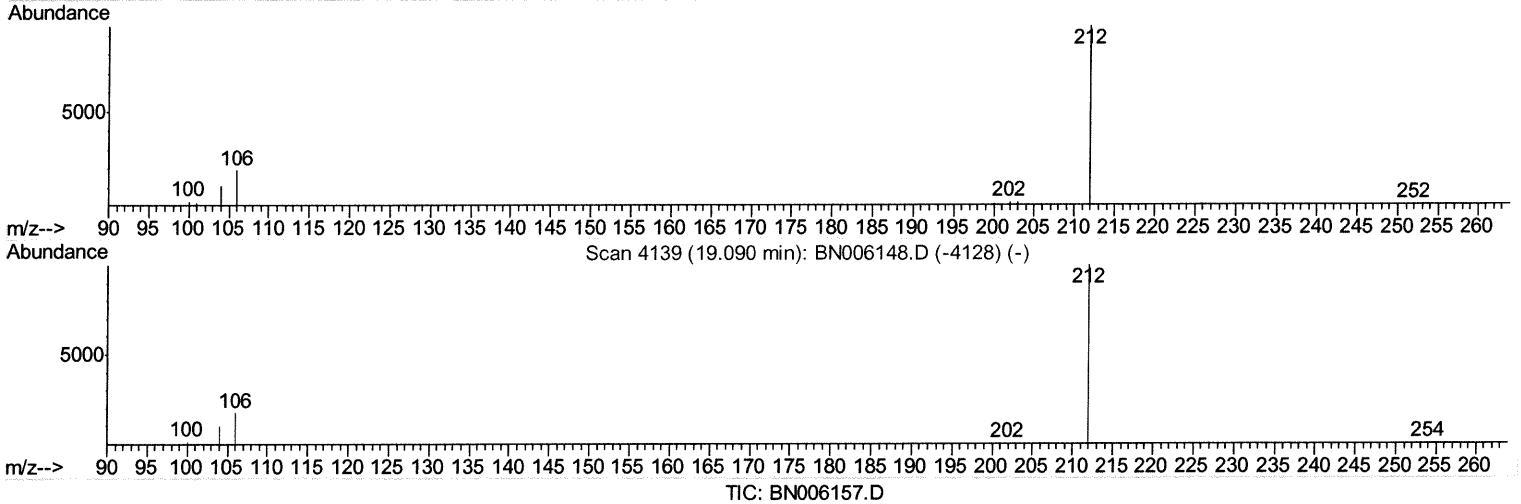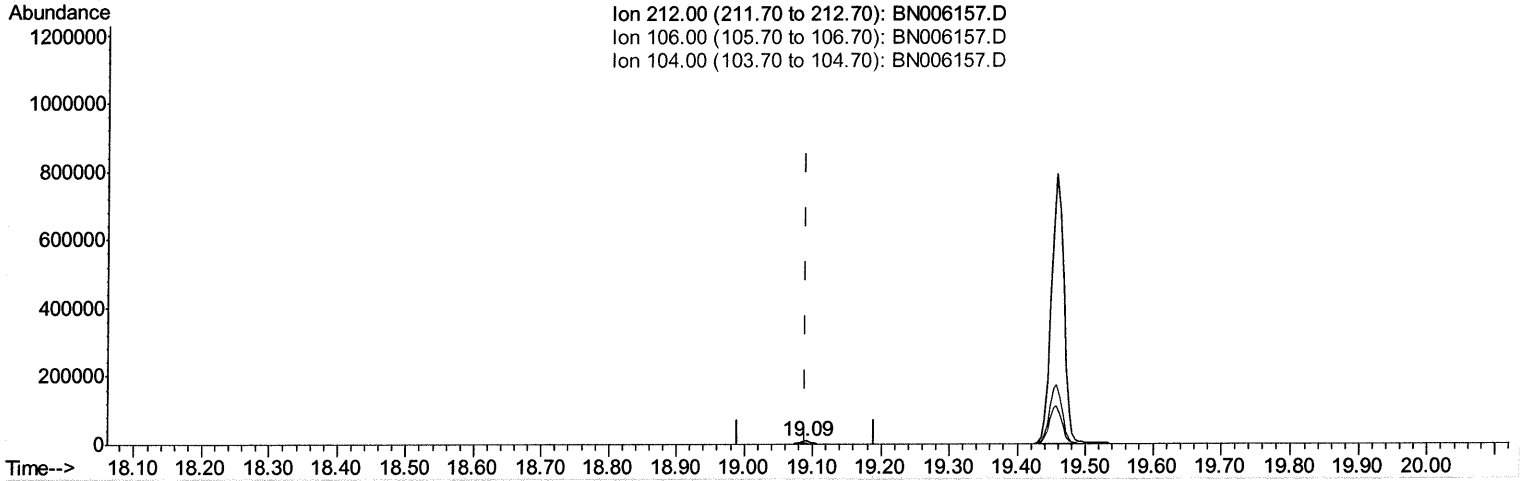

(14) Fluoranthene-d10 (SURR) JU
 19.090min (+0.000) 0.22ng/ul m 06/10/19

response 12917

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006157.D
Acq On : 07 Jun 2019 04:39
Operator : JU/SJ
Sample : K3016-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C6

Manual Integrations
APPROVED

mohammad
6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

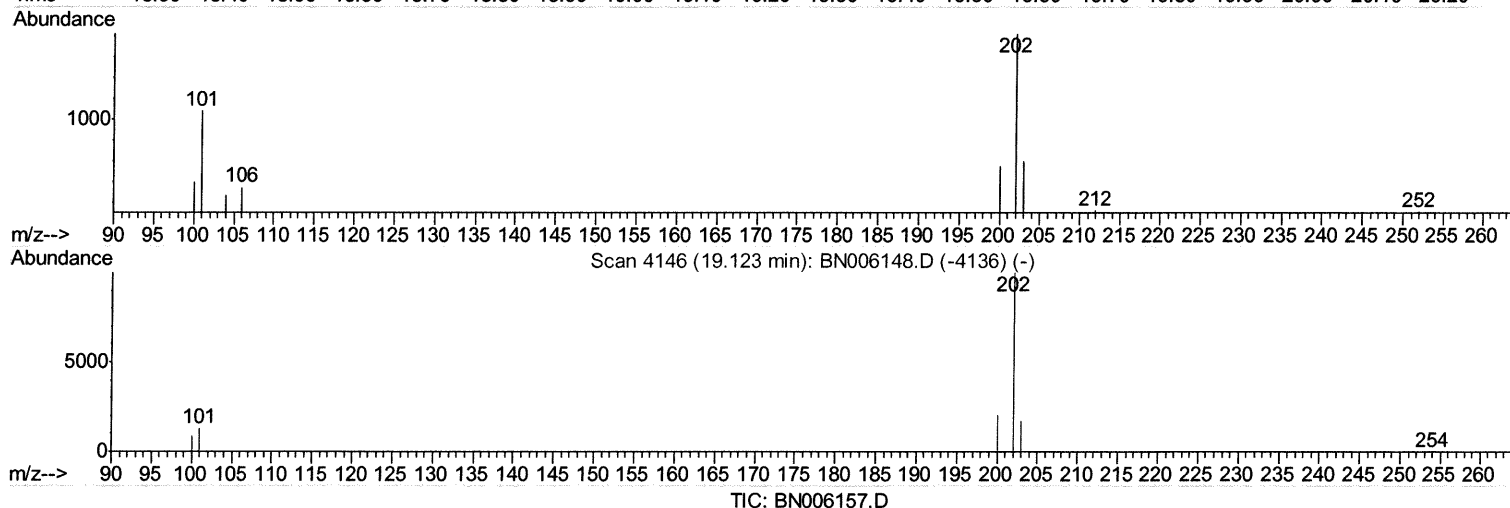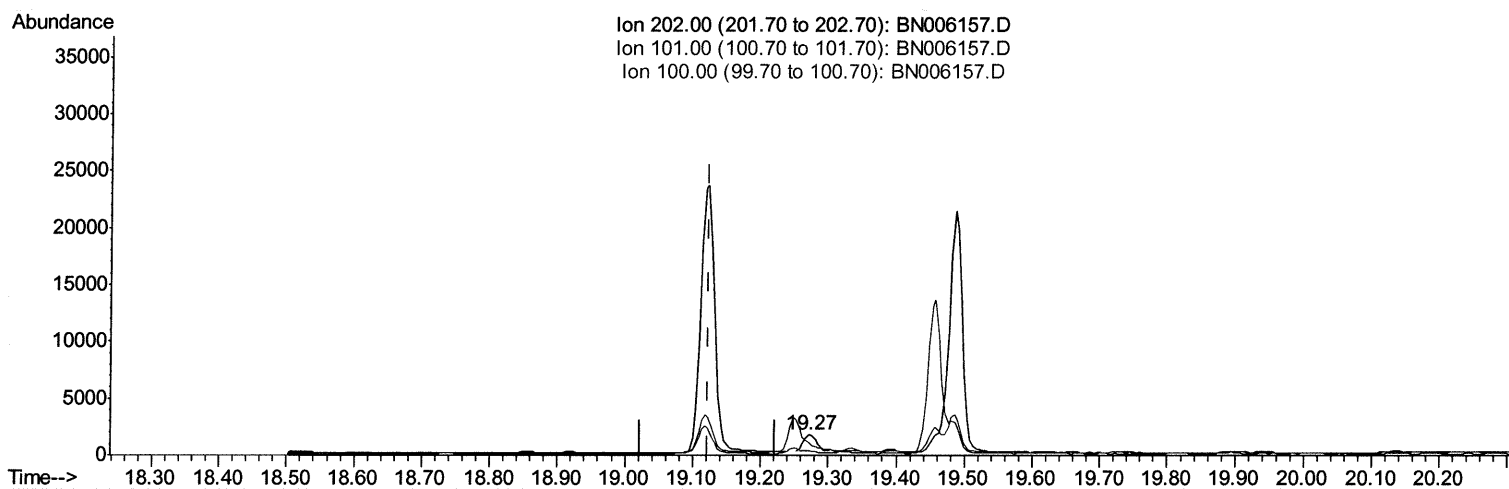

(15) Fluoranthene (C)

19.272min (+0.149) 0.03ng/ul

response 2127

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	59.33#
100.00	8.70	21.95
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

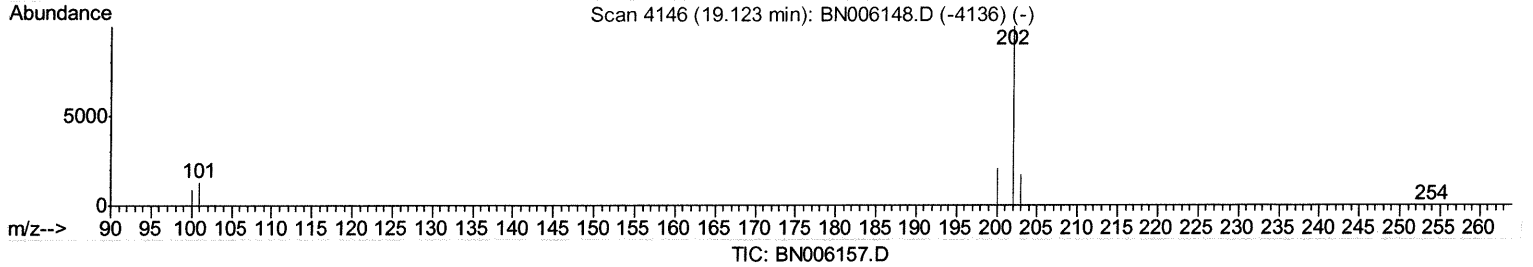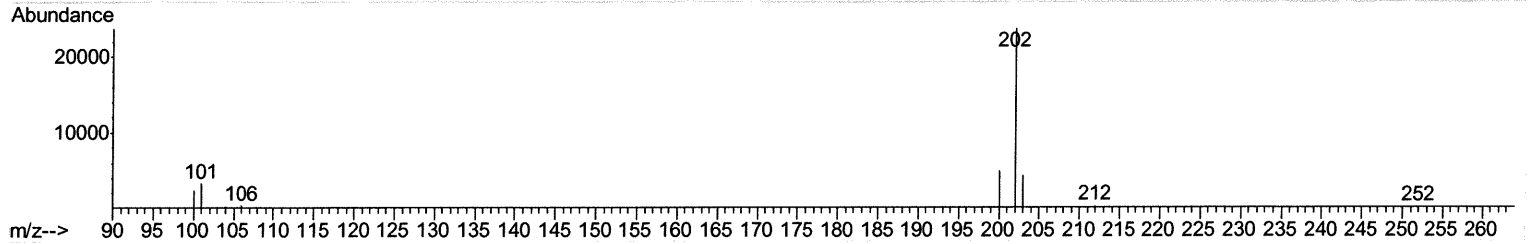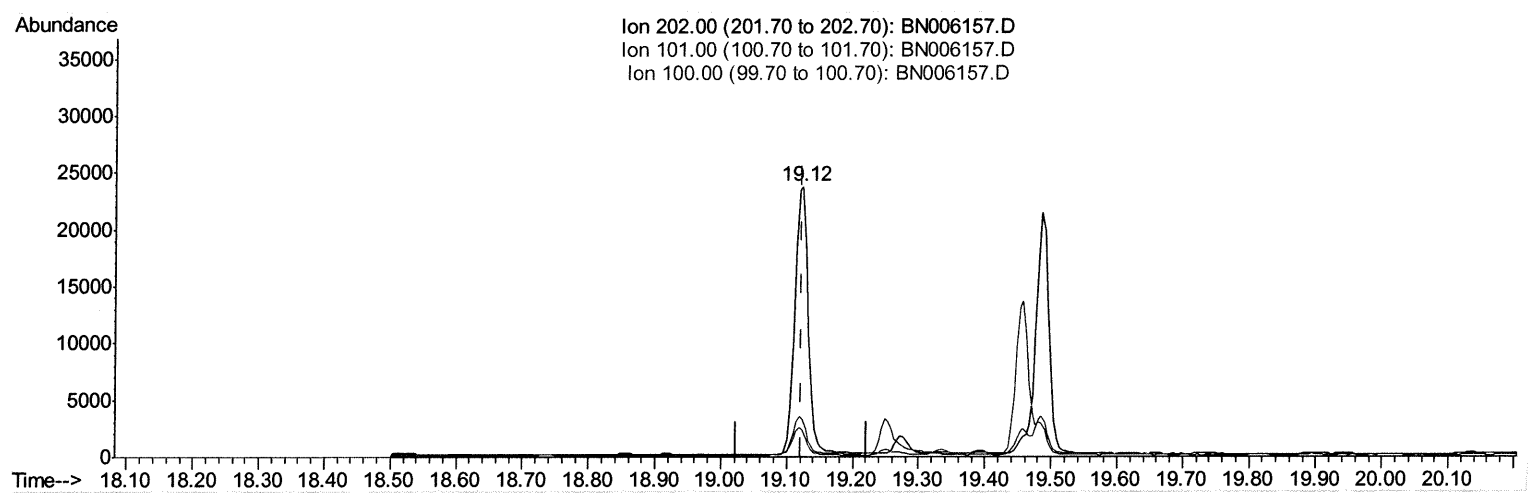

(15) Fluoranthene (C)

19.123min (+0.000) 0.43ng/ul m *Ju 06/10/19*

response 33954

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	14.00
100.00	8.70	10.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

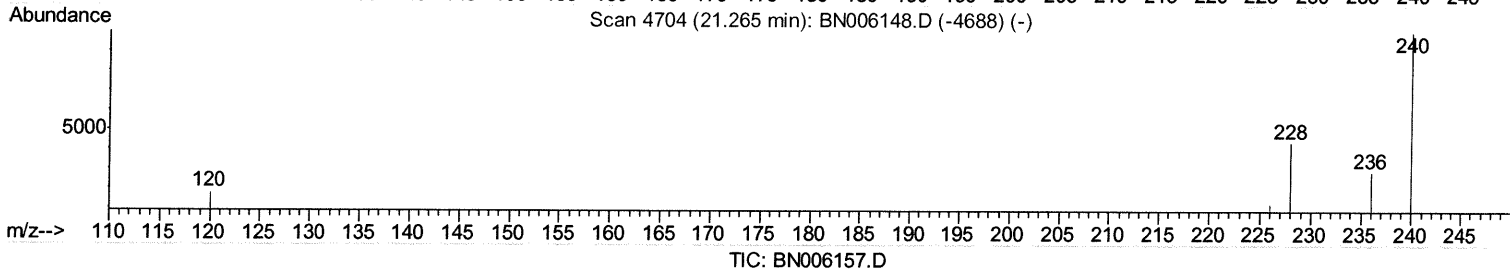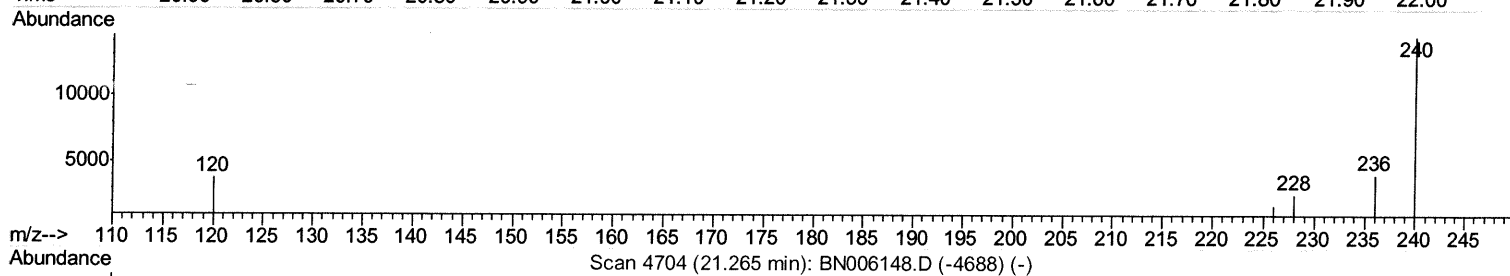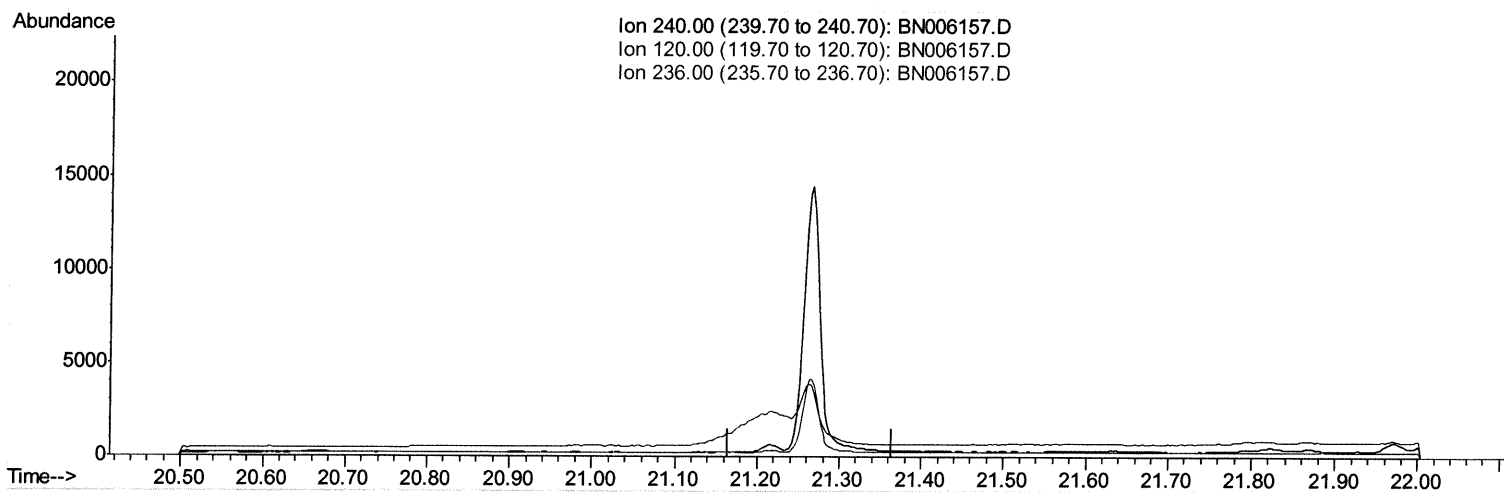

(16) Chrysene-d12 (I)

21.265min (-21.265) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:40:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

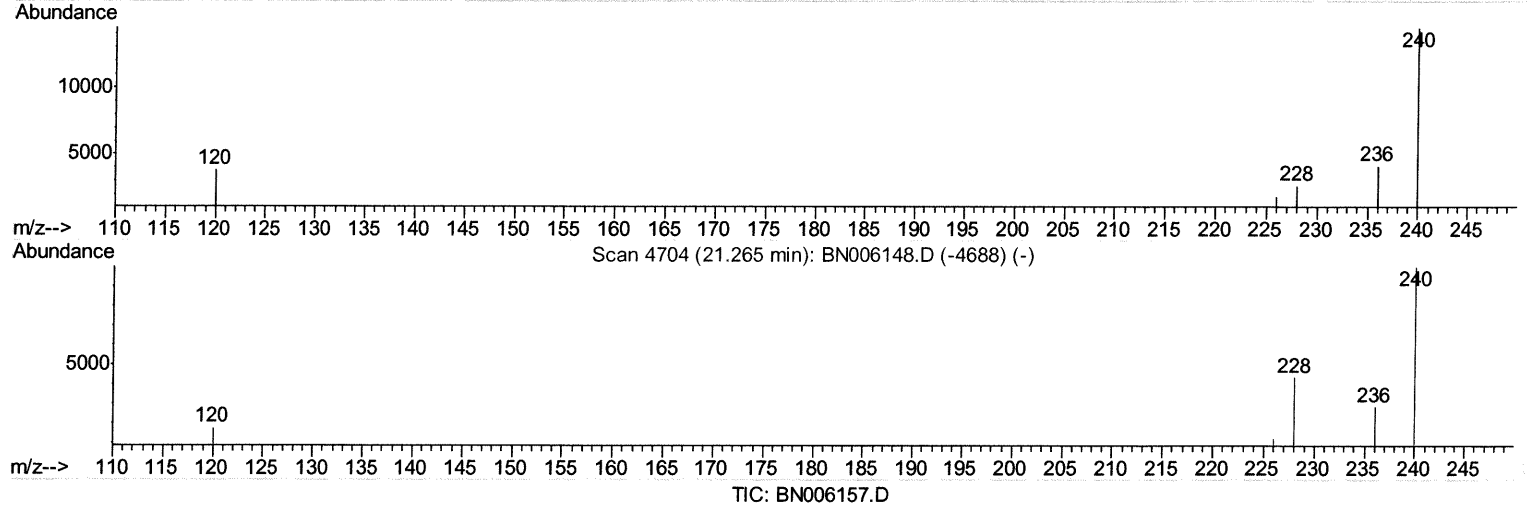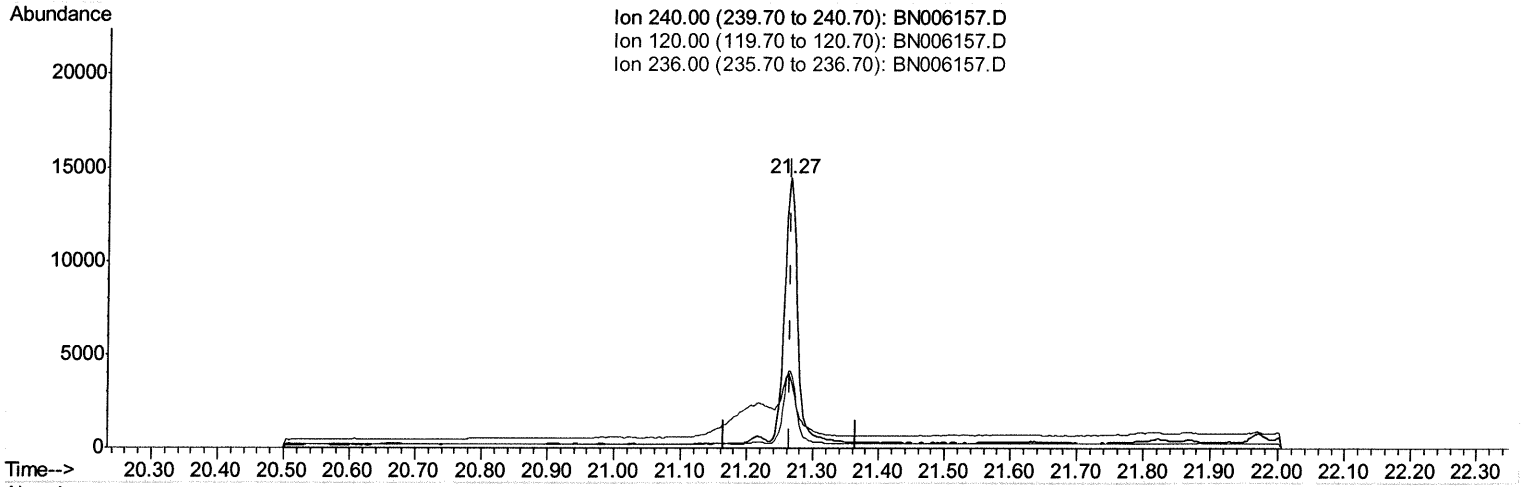

(16) Chrysene-d12 (I)

21.265min (+0.000) 0.40ng/ul m *JU* 06/10/19

response 19953

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	26.52#
236.00	30.10	28.75
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:42:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

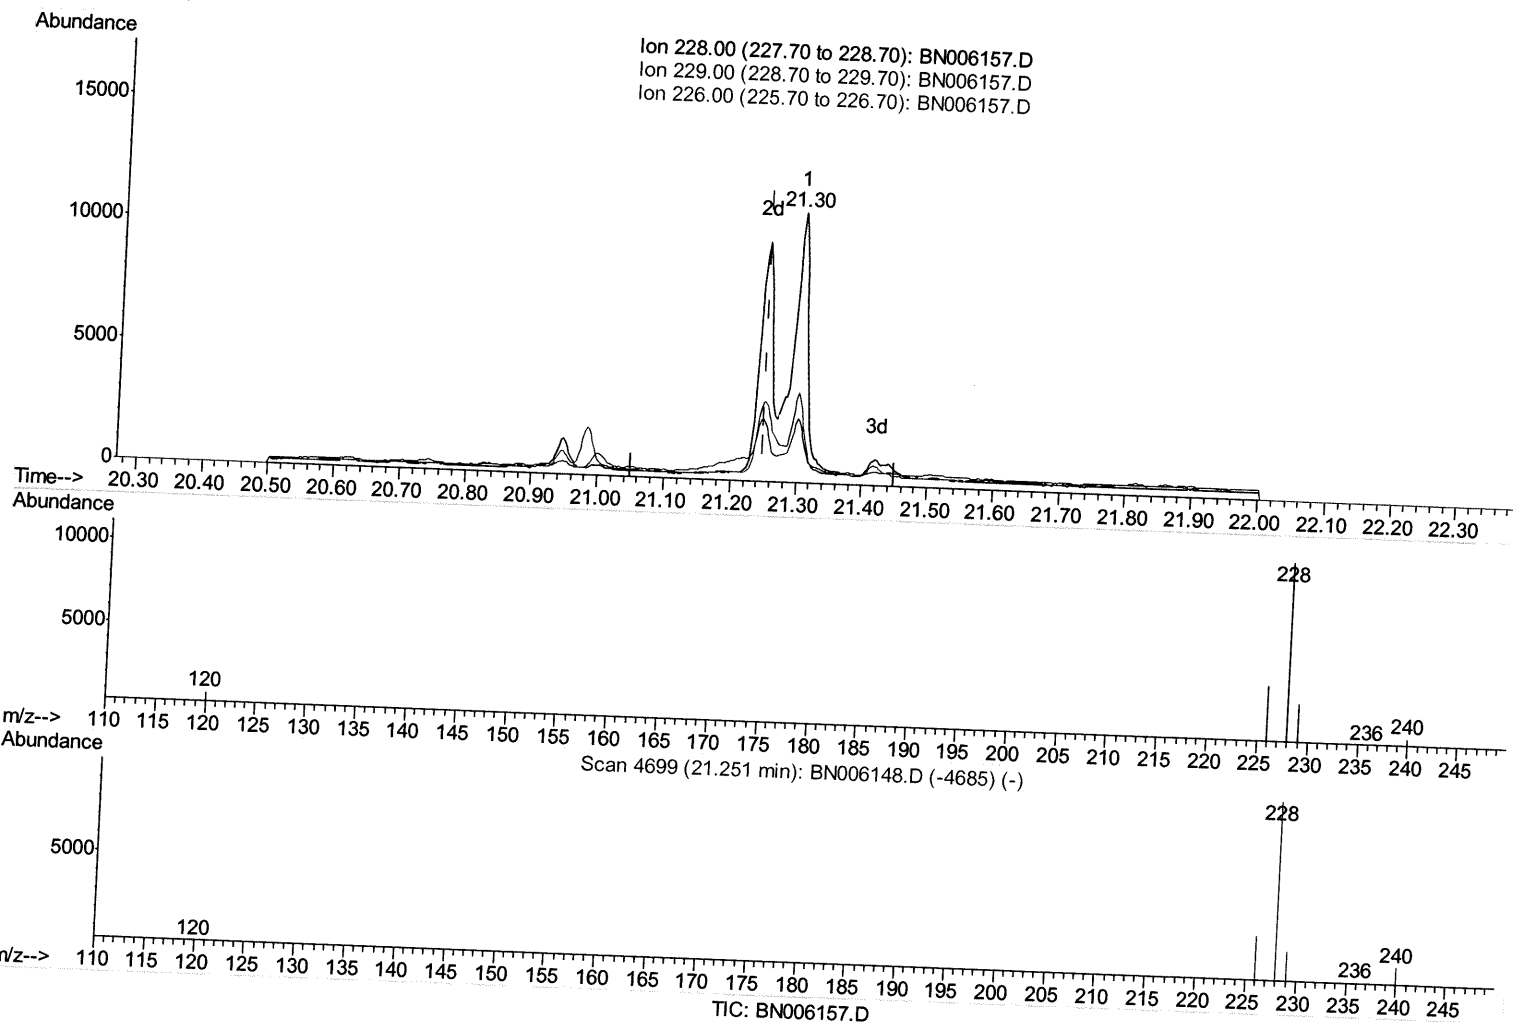

(18) Benzo(a)anthracene

21.300min (+0.050) 0.19ng/ul

response 16546

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	23.86
226.00	28.50	33.13
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:42:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

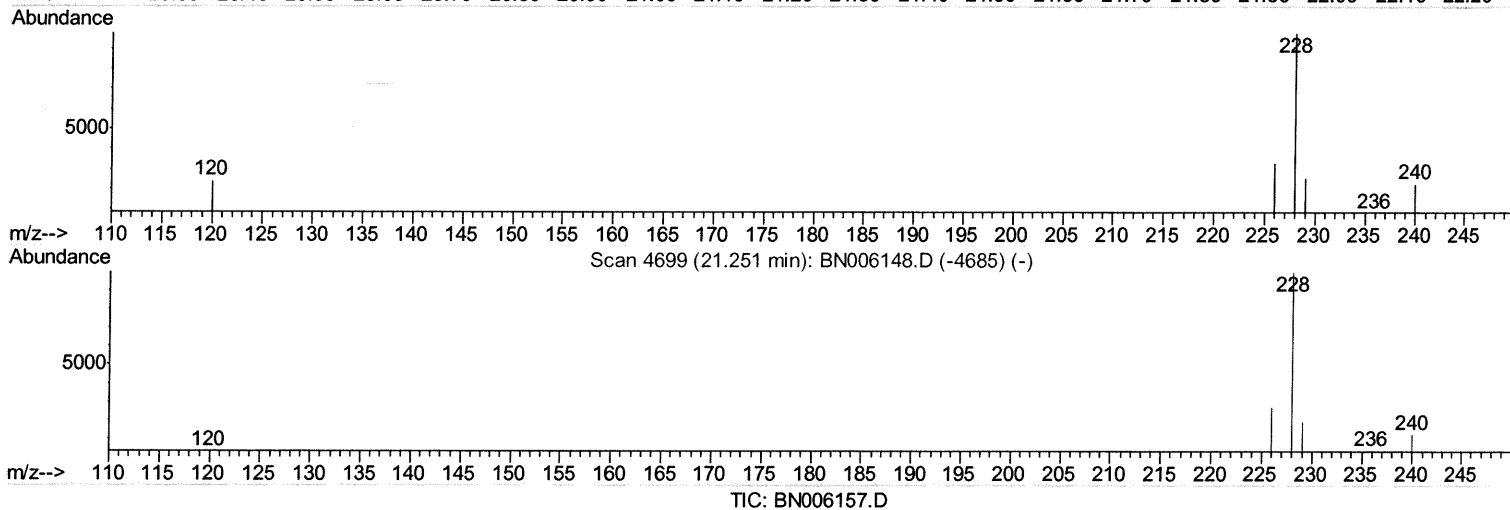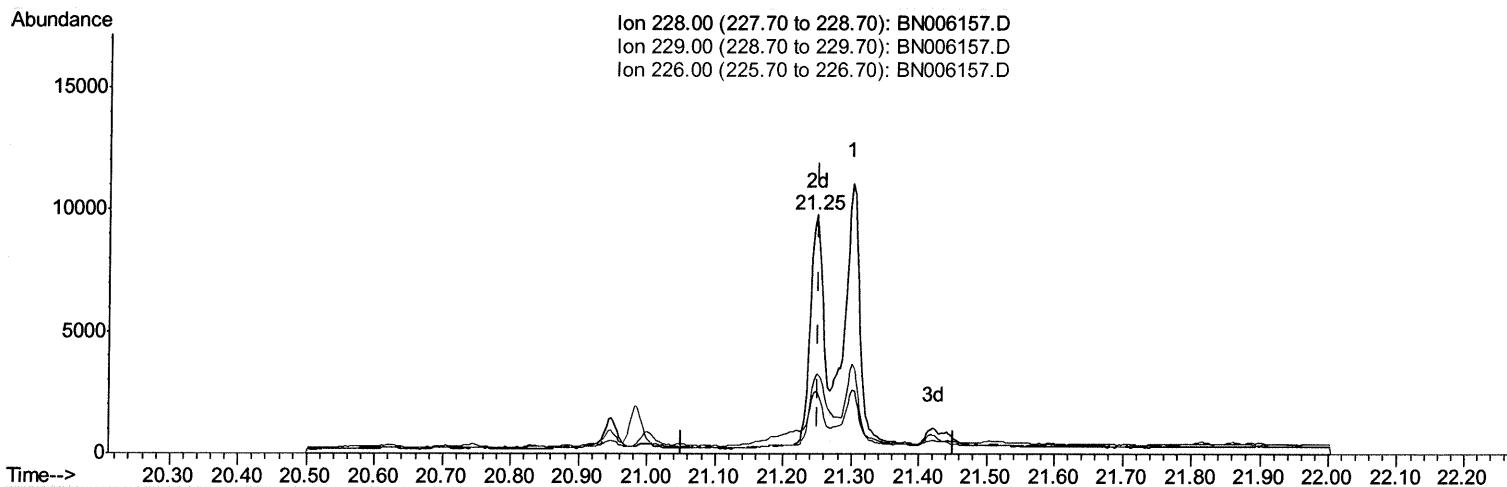

(18) Benzo(a)anthracene

21.248min (-0.003) 0.14ng/ul m *JU* 06/10/19

response 12704

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	26.19#
226.00	28.50	33.54
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1




Instrument :
 BNA_N
 ClientSampled :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:42:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

Ion 264.00 (263.70 to 264.70): BN006157.D
 Ion 260.00 (259.70 to 260.70): BN006157.D
 Ion 265.00 (264.70 to 265.70): BN006157.D

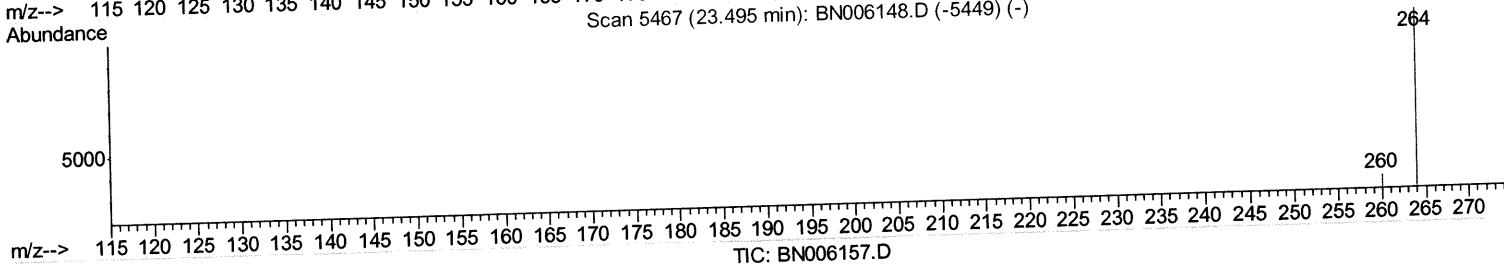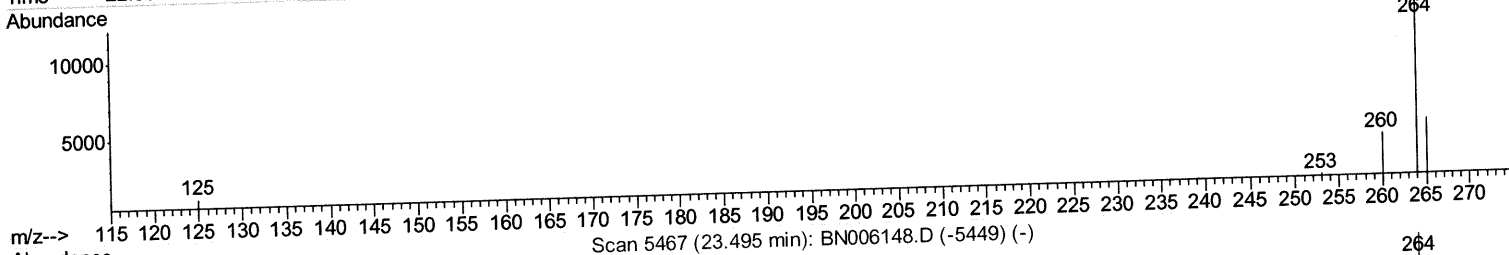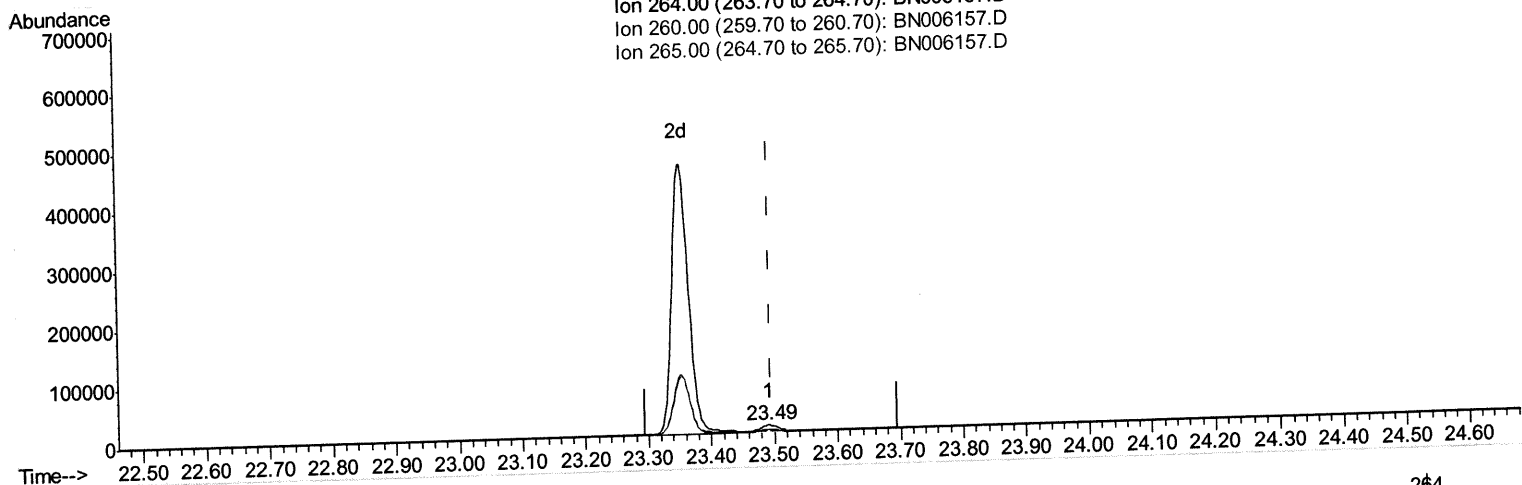

(20) Perylene-d12 (I)

23.492min (-0.003) 0.40ng/ul

response 27508

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.79
265.00	44.70	34.05#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:42:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

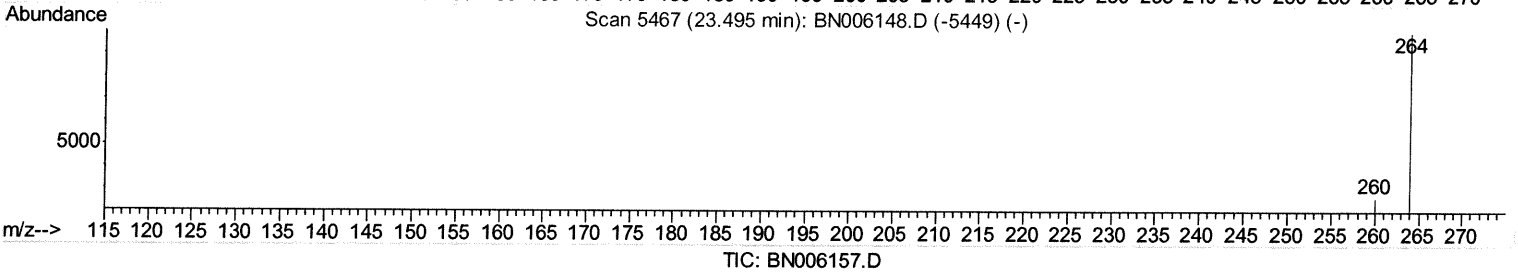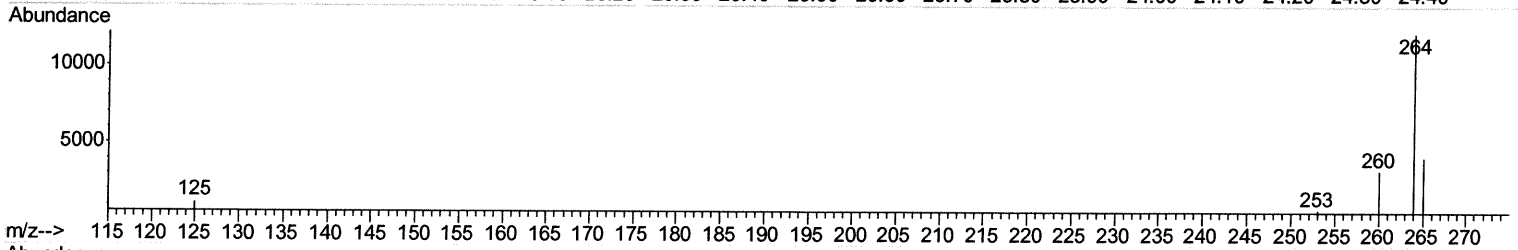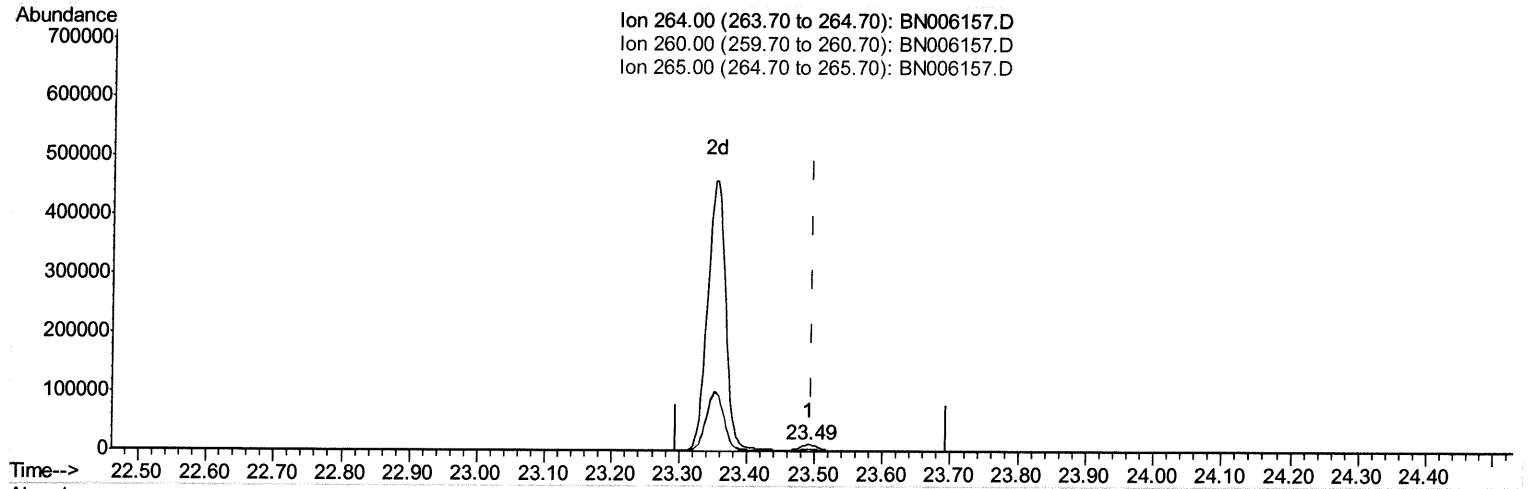

(20) Perylene-d12 (I)

23.492min (-0.003) 0.40ng/ul m *JU* 06/10/19

response 18033

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.79
265.00	44.70	34.05#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:43:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

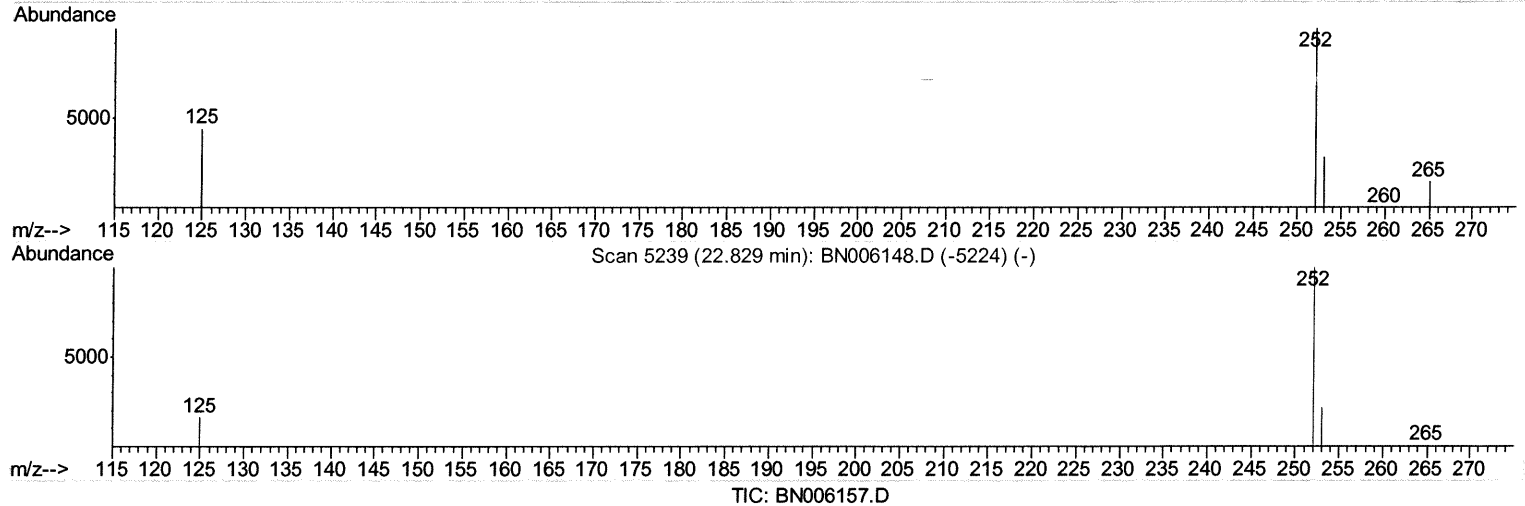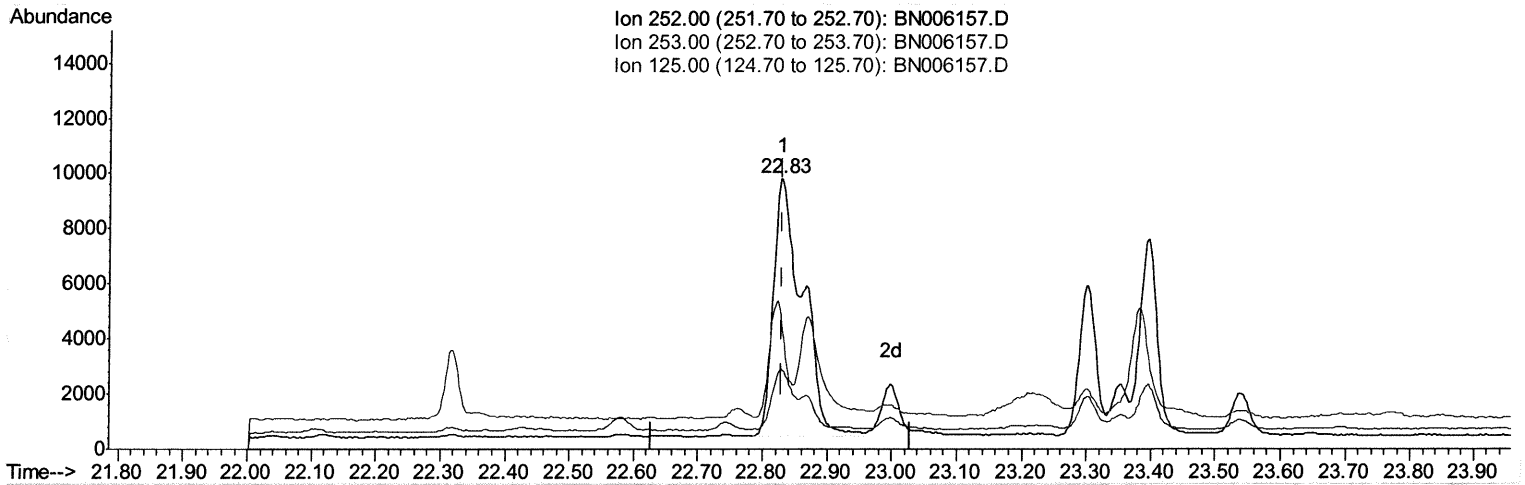

(21) Benzo(b)fluoranthene

22.829min (+0.000) 0.39ng/ul

response 29461

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	29.70
125.00	20.50	45.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:43:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

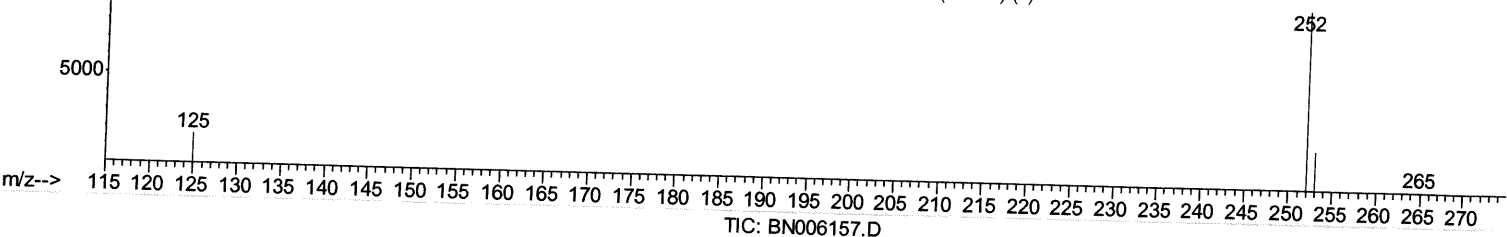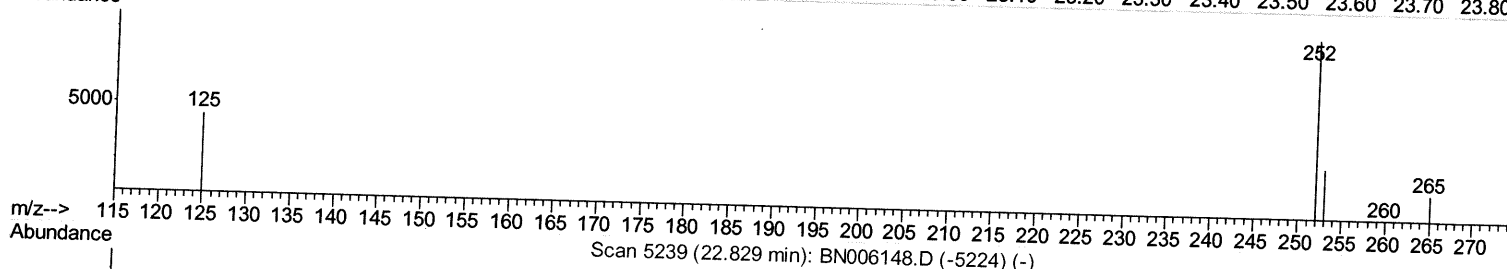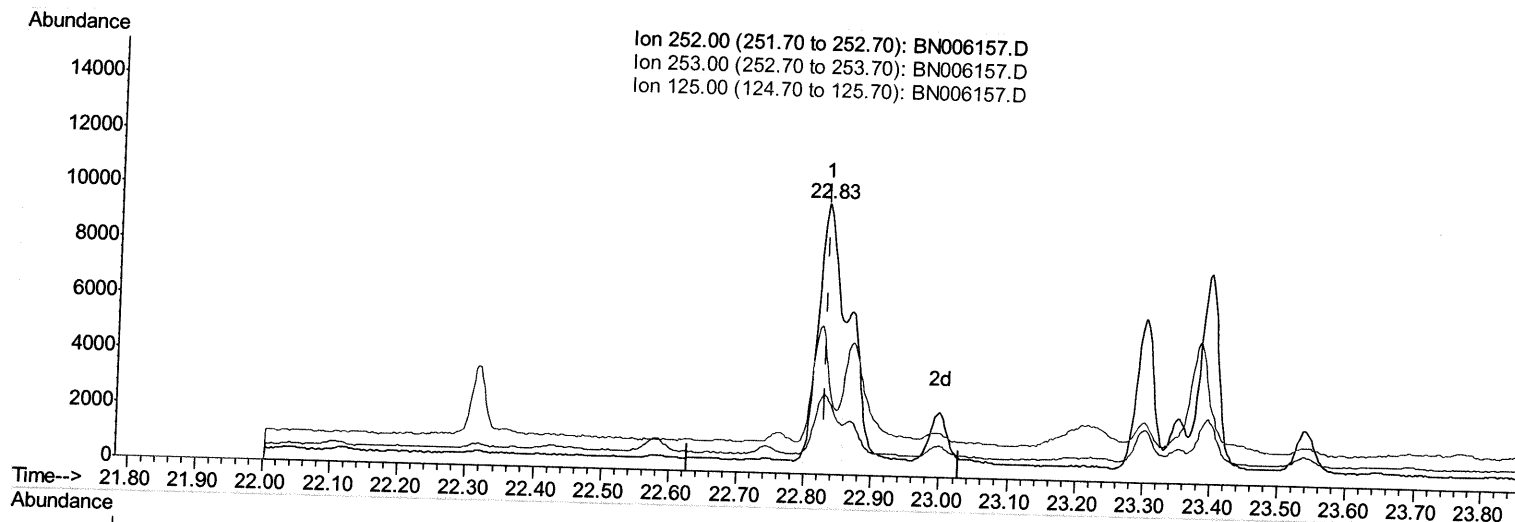

(21) Benzo(b)fluoranthene

22.829min (+0.000) 0.27ng/ul m ^{JU} 06/10/19

response 20573

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	29.70
125.00	20.50	45.59#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:43:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

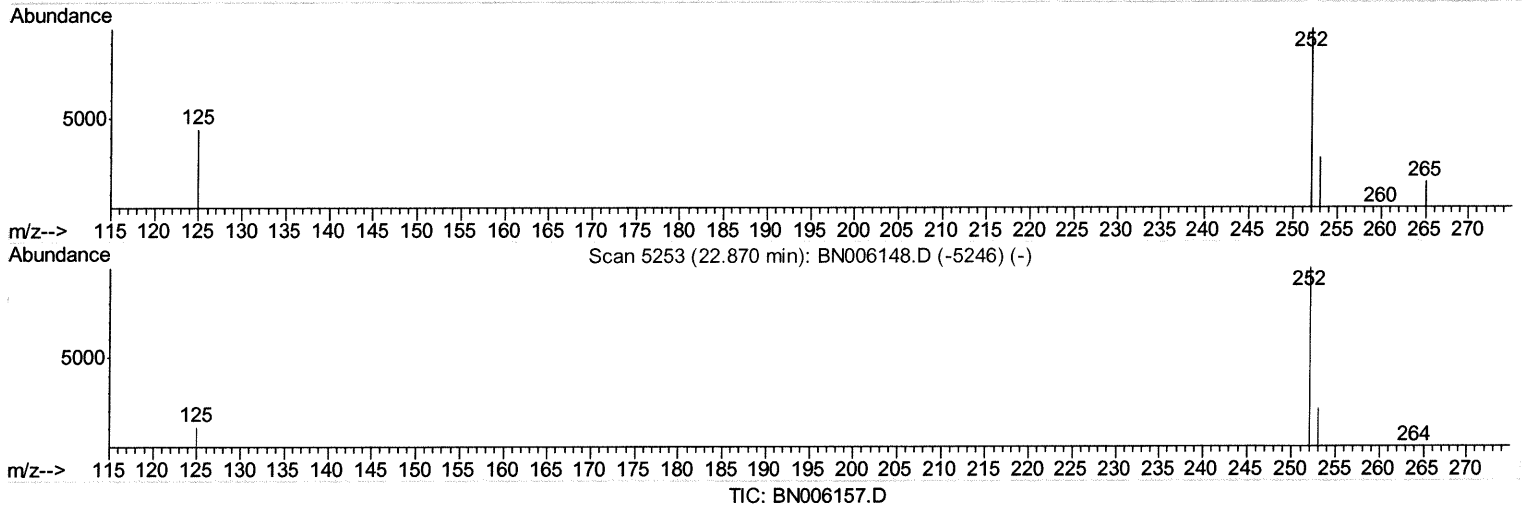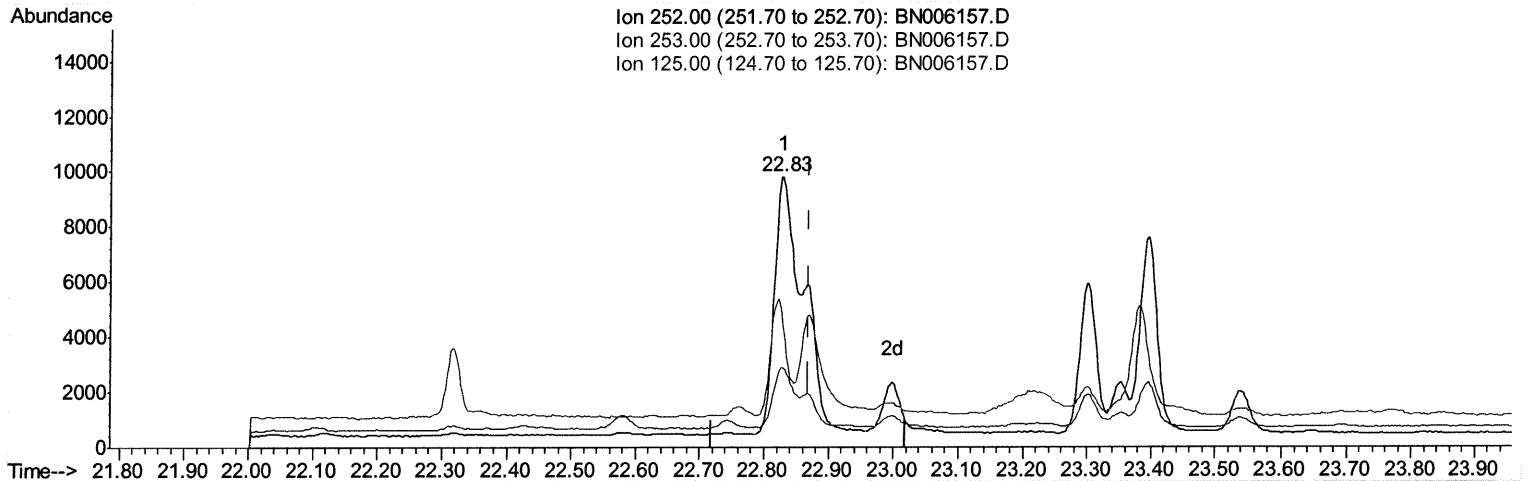

(22) Benzo(k)fluoranthene

22.829min (-0.041) 0.40ng/ul

response 29461

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	29.70
125.00	17.90	45.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:43:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

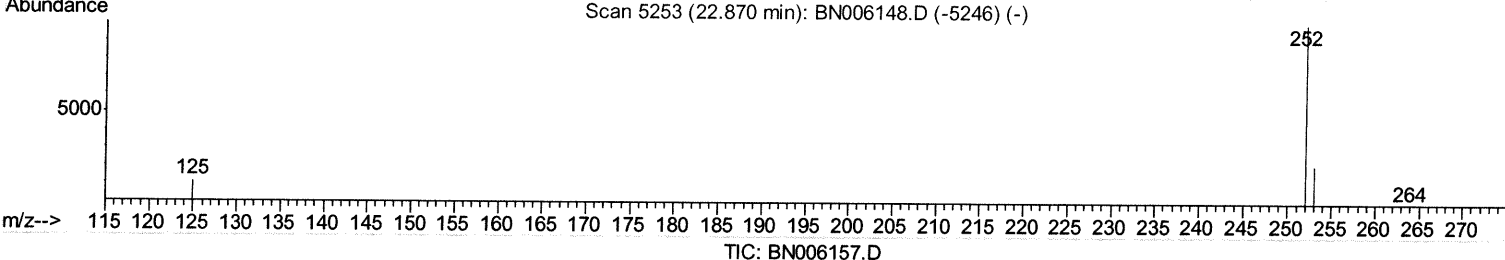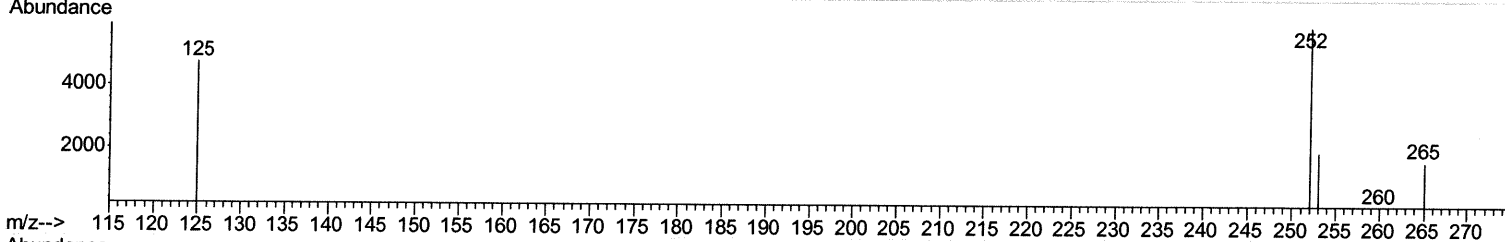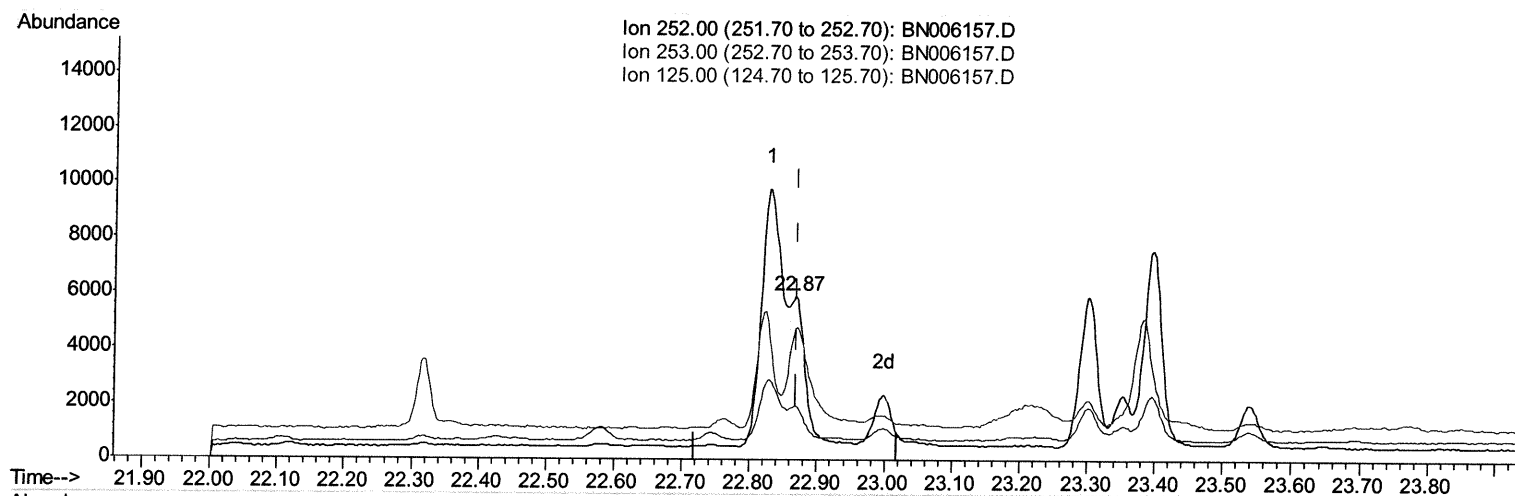

(22) Benzo(k)fluoranthene

22.867min (-0.003) 0.11ng/ul m *JU 06/10/19*

response 7983

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	33.17#
125.00	17.90	79.52#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006157.D
 Acq On : 07 Jun 2019 04:39
 Operator : JU/SJ
 Sample : K3016-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51C6

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:01 PM

Quant Time: Jun 07 06:44:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	5929	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	21699	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10915	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	22335m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	19953m>	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	18033m>	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	5831	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	12917m>	0.22	ng/ul	0.00
Target Compounds				Qvalue		
7) Acenaphthylene	14.01	152	4368	0.072	ng/ul#	93
12) Phenanthrene	17.09	178	13415	0.187	ng/ul	98
13) Anthracene	17.18	178	3217m>	0.047	ng/ul	
15) Fluoranthene	19.12	202	33954m>	0.429	ng/ul	
17) Pyrene	19.49	202	30256	0.288	ng/ul	96
18) Benzo(a)anthracene	21.25	228	12704m>	0.144	ng/ul	
19) Chrysene	21.30	228	17190	0.207	ng/ul	95
21) Benzo(b)fluoranthene	22.83	252	20573m>	0.274	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	7983m>	0.109	ng/ul	
23) Benzo(a)pyrene	23.40	252	13210	0.189	ng/ul#	78
24) Indeno(1,2,3-cd)pyrene	25.72	276	10068	0.133	ng/ul	98
25) Dibenzo(a,h)anthracene	25.73	278	2901	0.048	ng/ul#	33
26) Benzo(g,h,i)perylene	26.41	276	9461	0.149	ng/ul#	90

JU 06/10/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed