


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006173.D
Acq On : 07 Jun 2019 18:45
Operator : JU/SJ
Sample : K3201-09DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleID :
C0AC0DL

Manual Integrations
APPROVED

mohammad
6/11/2019 5:08:43 PM

Quant Time: Jun 08 02:55:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

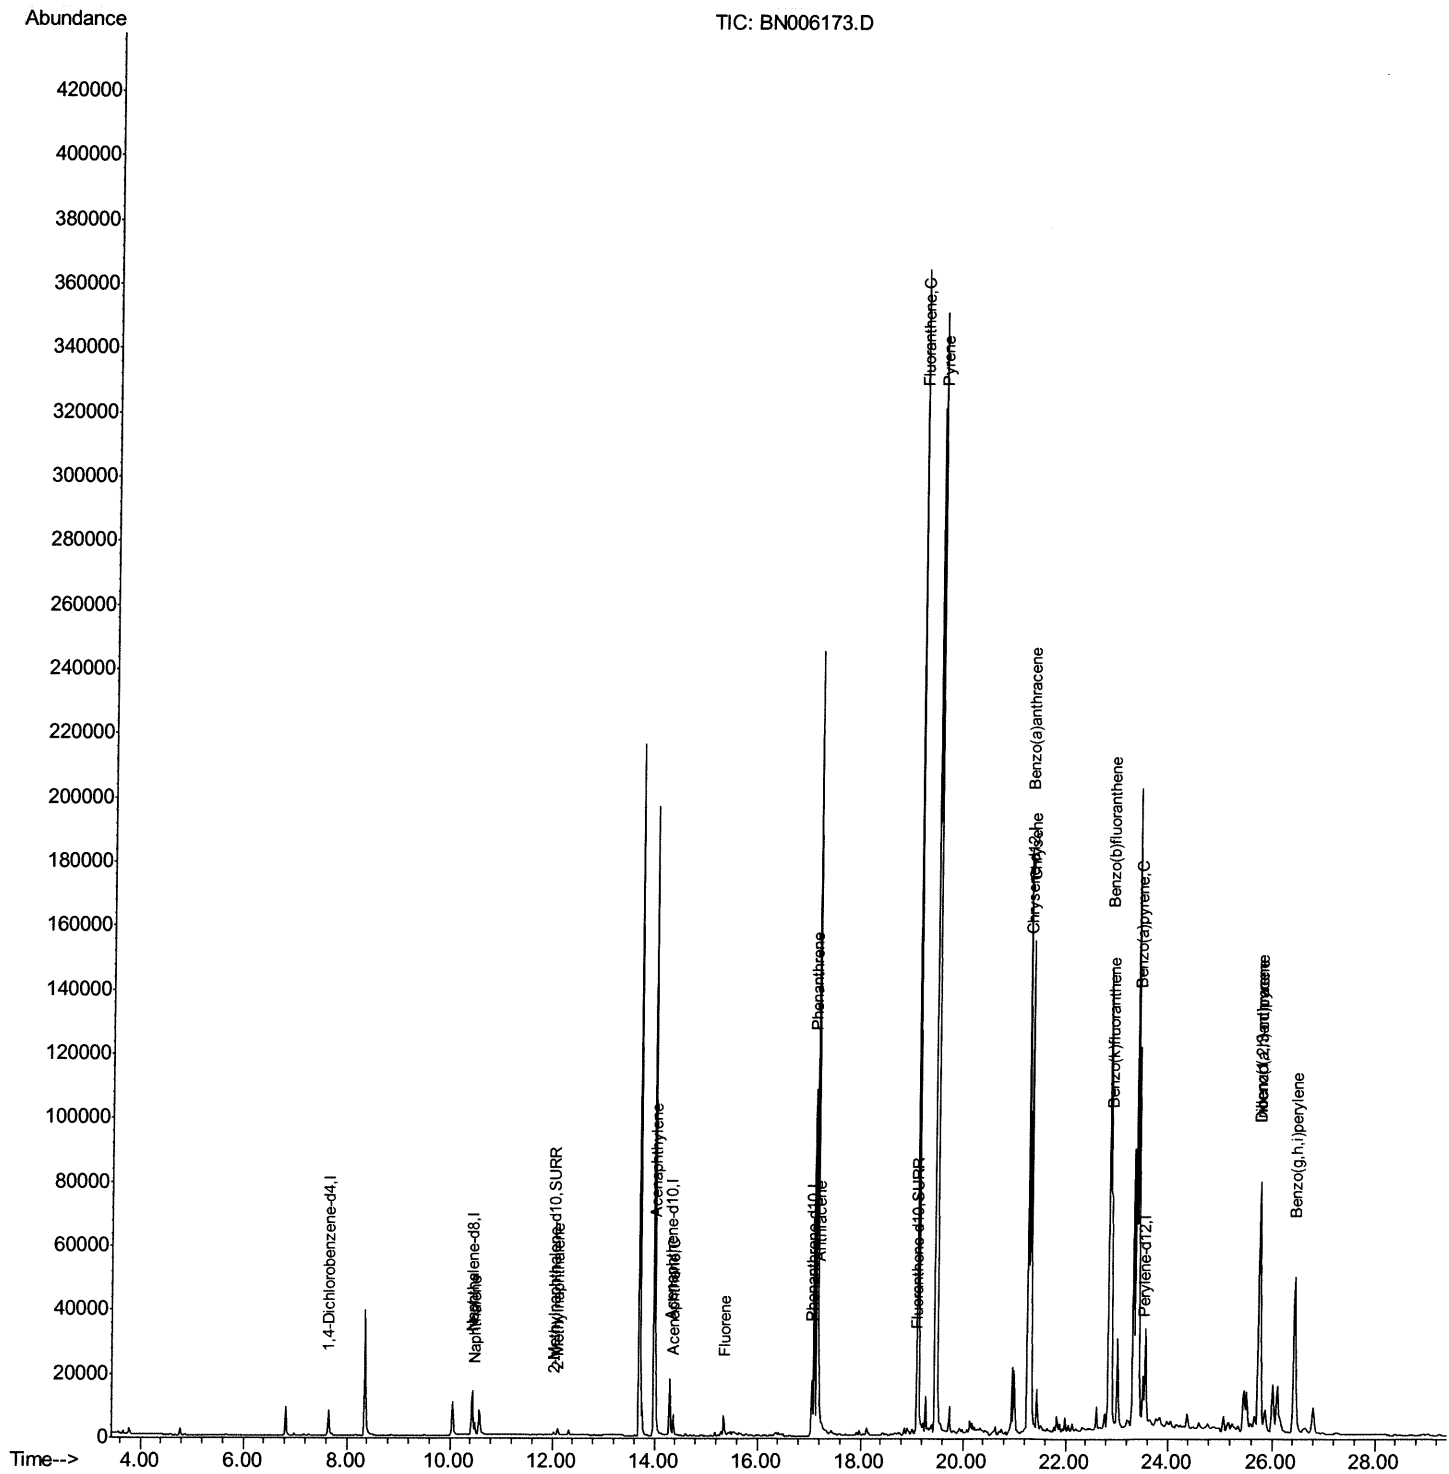

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006173.D
 Acq On : 07 Jun 2019 18:45
 Operator : JU/SJ
 Sample : K3201-09DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0DL

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:43 PM

Quant Time: Jun 08 02:03:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

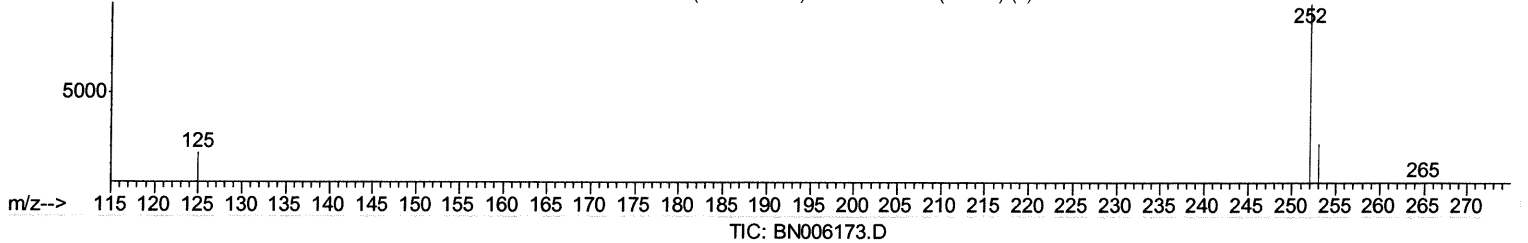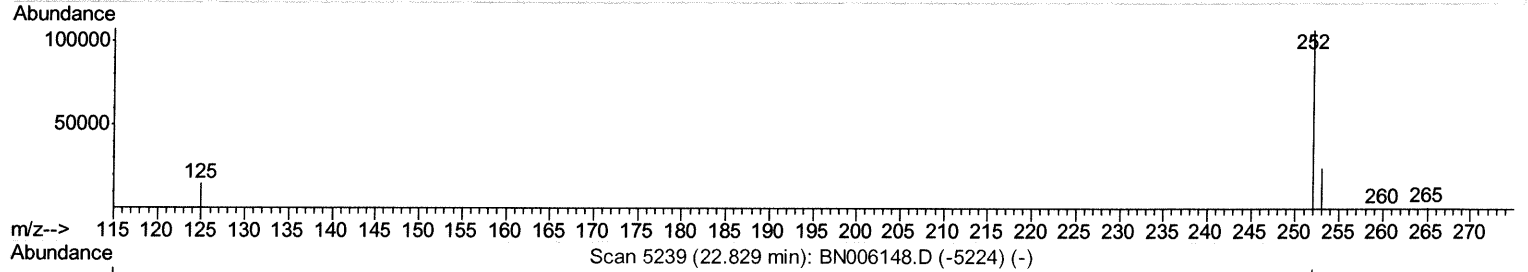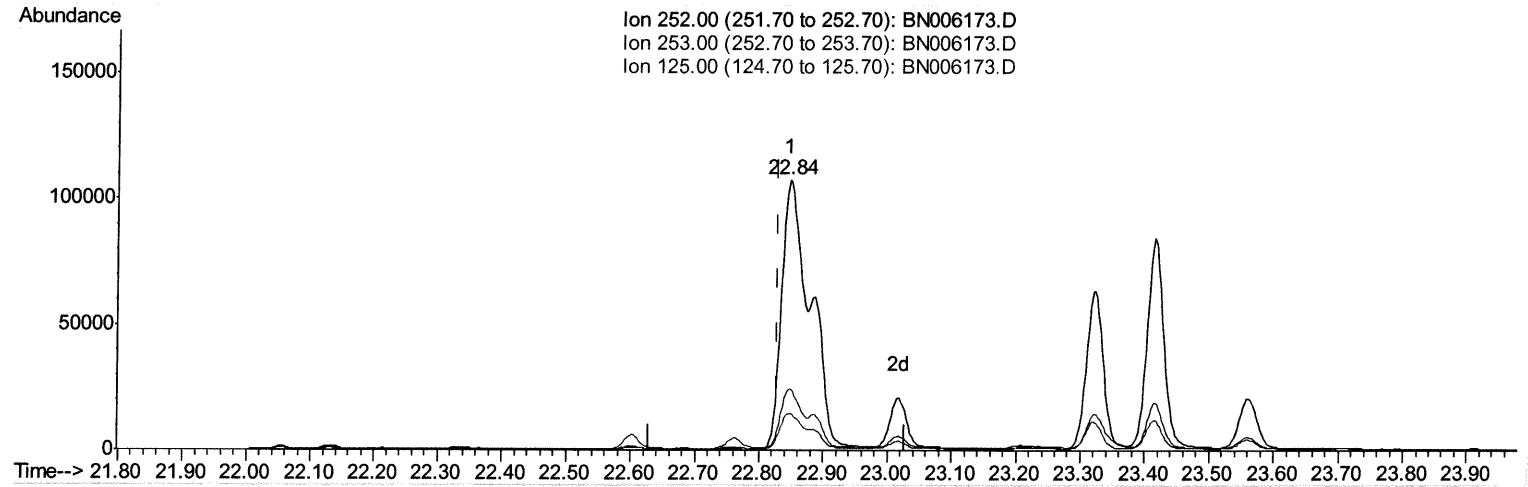

(21) Benzo(b)fluoranthene

22.845min (+0.016) 3.33ng/ul

response 330461

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.58
125.00	20.50	13.51
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006173.D
 Acq On : 07 Jun 2019 18:45
 Operator : JU/SJ
 Sample : K3201-09DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0DL

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:43 PM

Quant Time: Jun 08 02:03:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

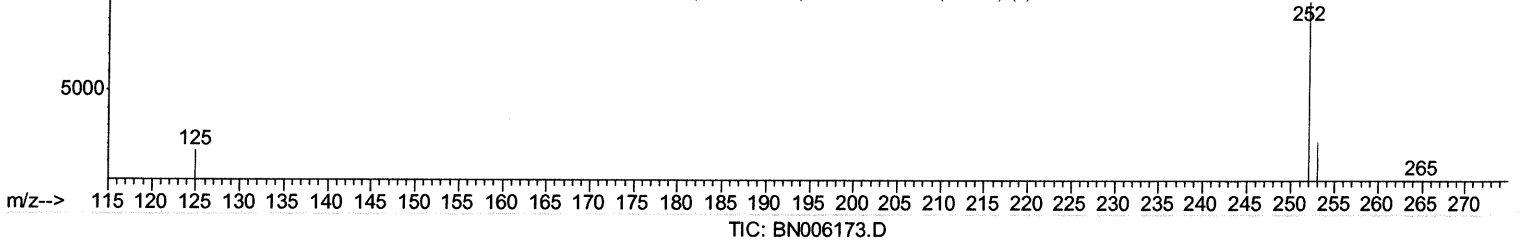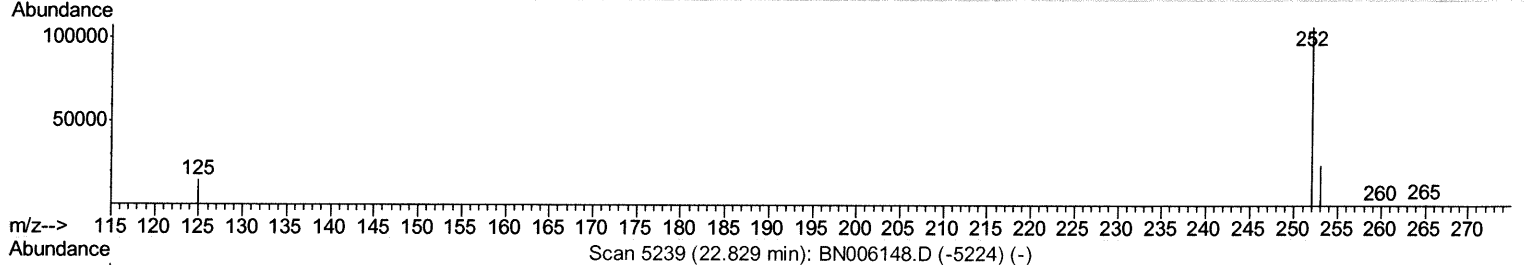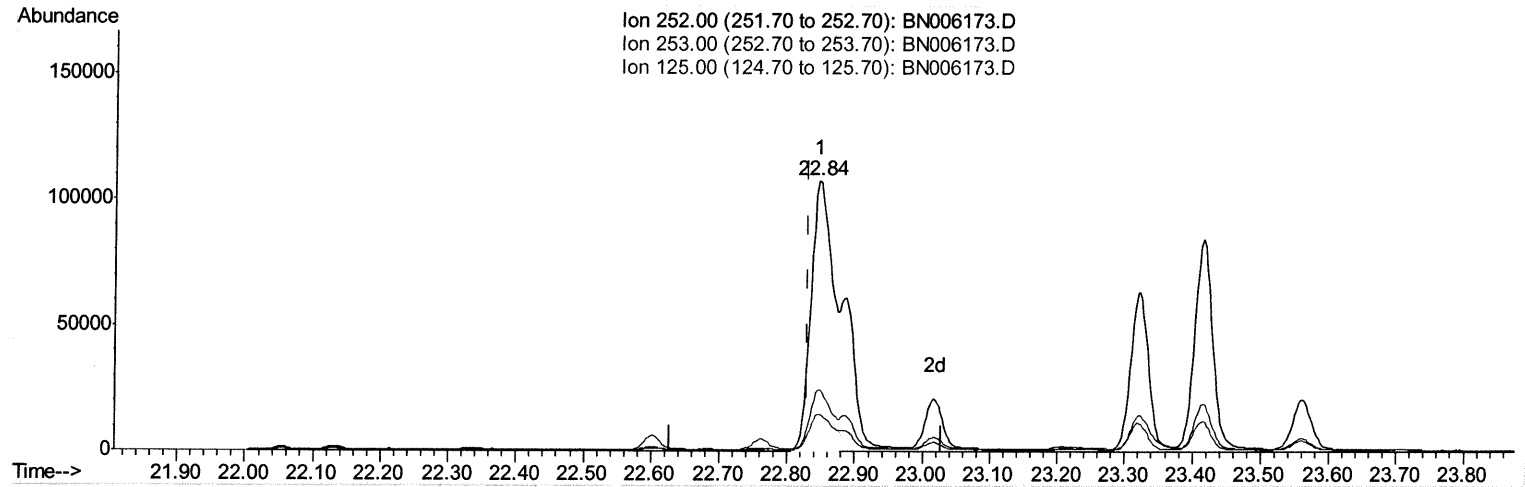

(21) Benzo(b)fluoranthene

22.845min (+0.016) 2.47ng/ul m *JU 06/10/19*

response 245784

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.58
125.00	20.50	13.51
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006173.D
 Acq On : 07 Jun 2019 18:45
 Operator : JU/SJ
 Sample : K3201-09DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC0DL

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:43 PM

Quant Time: Jun 08 02:03:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

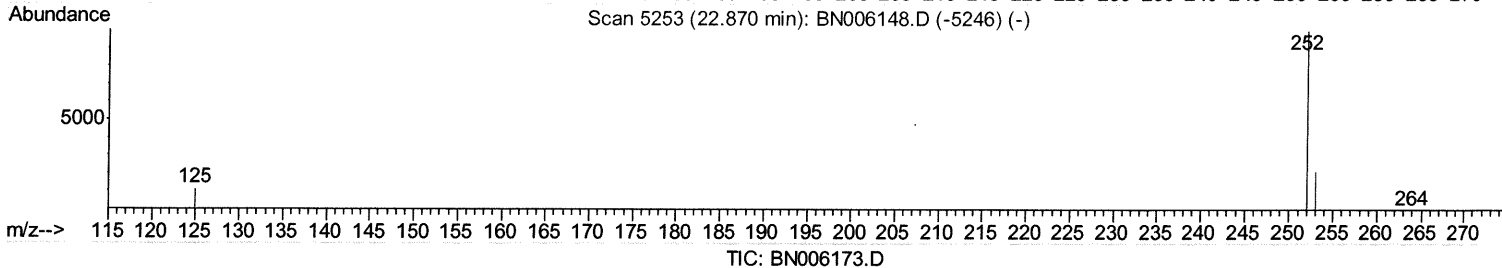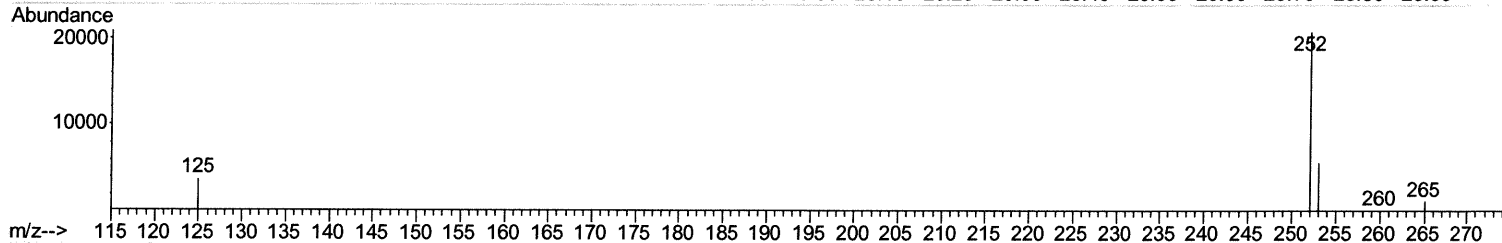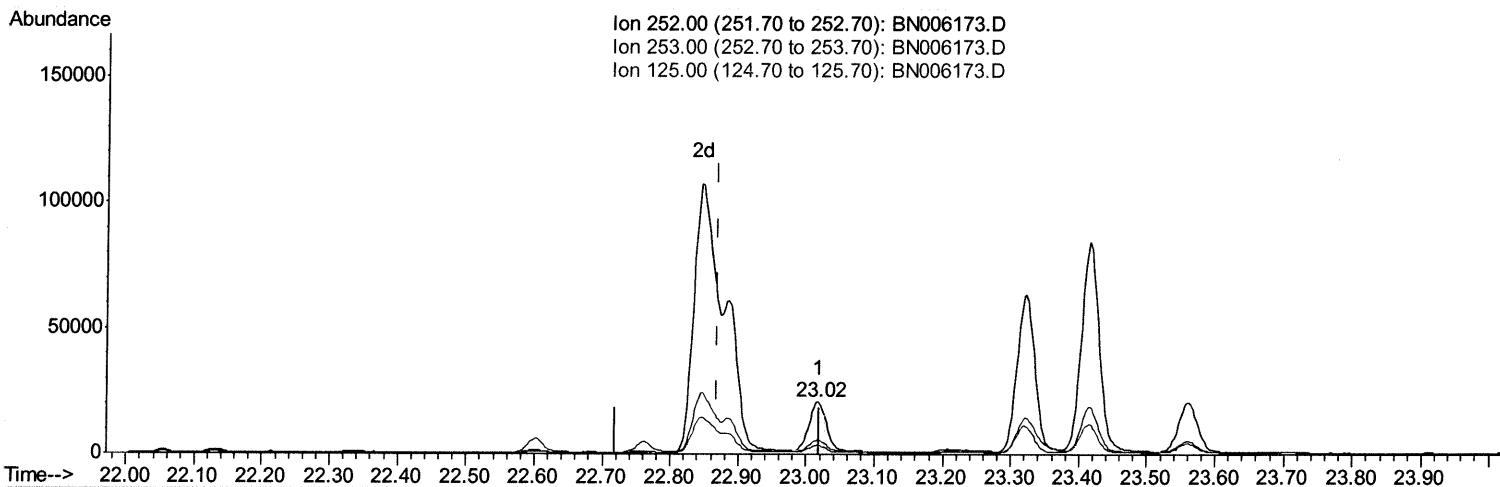

(22) Benzo(k)fluoranthene

23.017min (+0.148) 0.28ng/ul

response 27341

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	27.11
125.00	17.90	17.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
Data File : BN006173.D
Acq On : 07 Jun 2019 18:45
Operator : JU/SJ
Sample : K3201-09DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC0DL

Manual Integrations
APPROVED

mohammad
6/11/2019 5:08:43 PM

Quant Time: Jun 08 02:03:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 07 01:31:14 2019
Response via : Initial Calibration

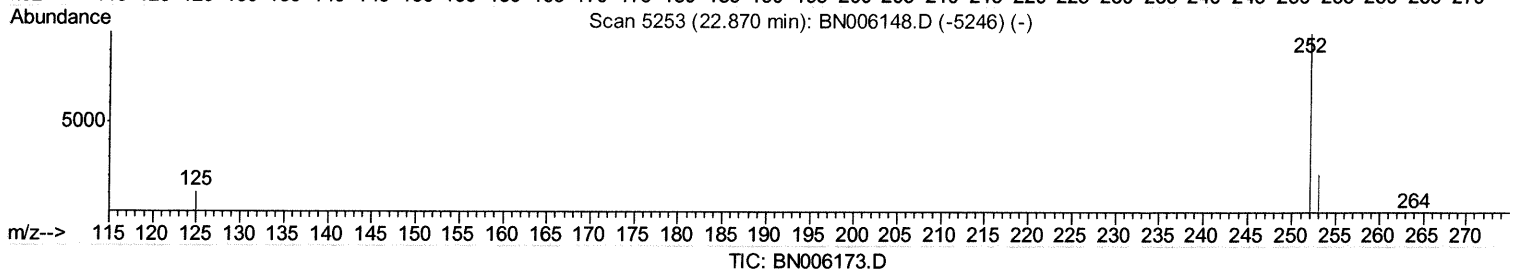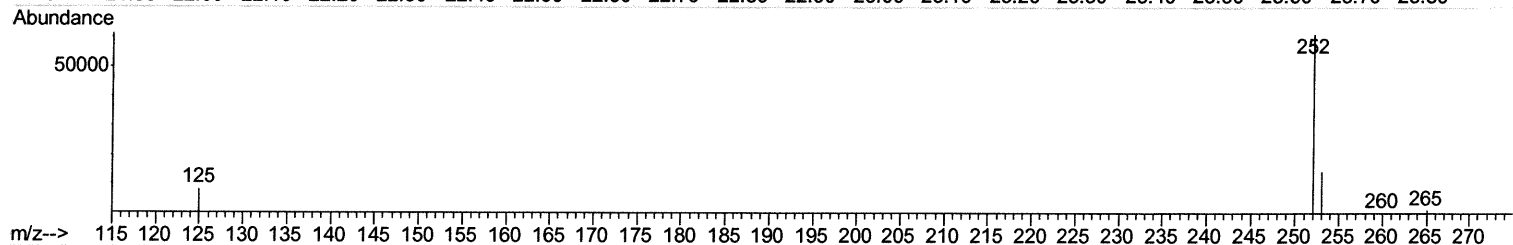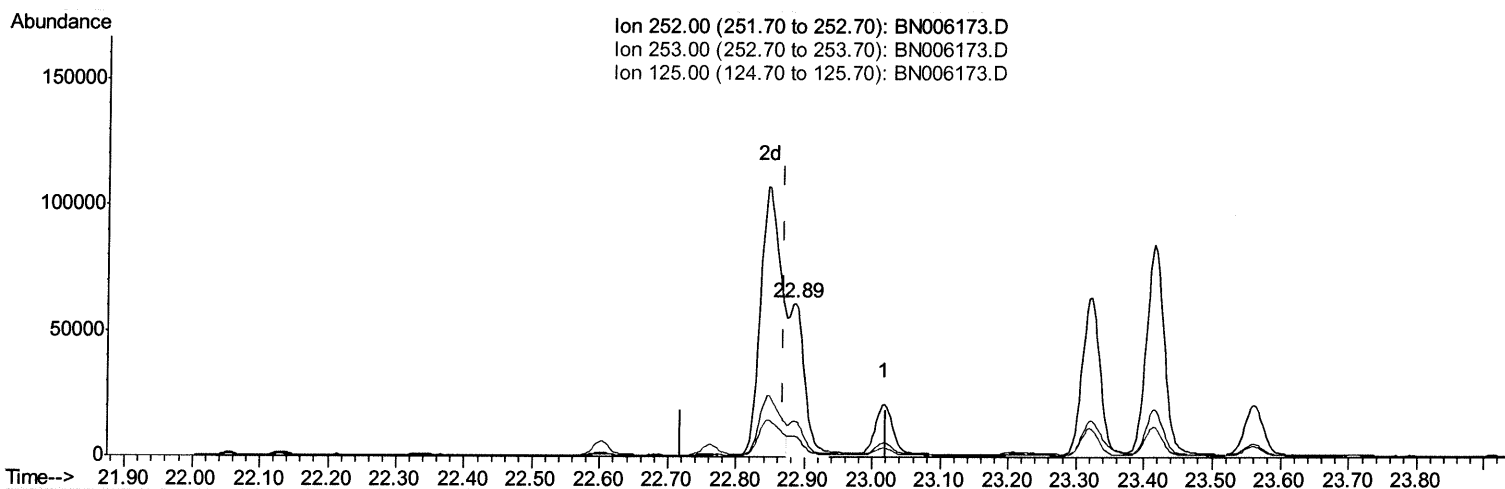

(22) Benzo(k)fluoranthene

22.886min (+0.016) 0.99ng/ul m

JU
06/10/19

response 95597

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.23
125.00	17.90	13.49#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060619\
 Data File : BN006173.D
 Acq On : 07 Jun 2019 18:45
 Operator : JU/SJ
 Sample : K3201-09DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 C0AC0DL

Manual Integrations
 APPROVED

mohammad
 6/11/2019 5:08:43 PM

Quant Time: Jun 08 02:55:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 07 01:31:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	5090	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	19307	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	9853	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	20947	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	17679	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	23817	0.40	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.03	152	1497	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	3543	0.06	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.48	128	5157	0.097	ng/ul#	95
5) 2-Methylnaphthalene	12.10	142	1841	0.050	ng/ul	98
7) Acenaphthylene	14.01	152	27861	0.509	ng/ul	100
8) Acenaphthene	14.36	153	3861	0.102	ng/ul	99
9) Fluorene	15.35	166	4381	0.099	ng/ul#	95
12) Phenanthrene	17.09	178	117850	1.753	ng/ul	100
13) Anthracene	17.18	178	32732	0.510	ng/ul	99
15) Fluoranthene	19.12	202	312570	4.210	ng/ul	98
17) Pyrene	19.49	202	283832	3.048	ng/ul	99
18) Benzo(a)anthracene	21.26	228	155794	1.992	ng/ul	99
19) Chrysene	21.31	228	170218	2.319	ng/ul	98
21) Benzo(b)fluoranthene	22.84	252	245784m	2.475	ng/ul	
22) Benzo(k)fluoranthene	22.89	252	95597m	0.988	ng/ul	
23) Benzo(a)pyrene	23.42	252	152555	1.649	ng/ul#	85
24) Indeno(1,2,3-cd)pyrene	25.75	276	127017	1.269	ng/ul#	87
25) Dibenzo(a,h)anthracene	25.75	278	30476	0.381	ng/ul	95
26) Benzo(g,h,i)perylene	26.43	276	99363	1.185	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 06/10/19