
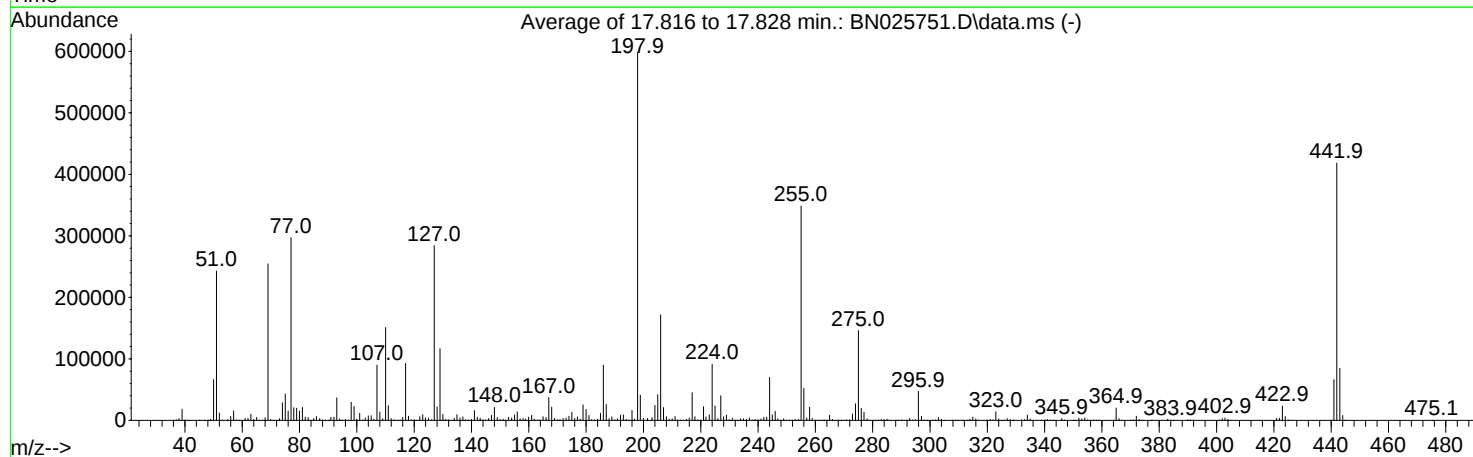


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060623\
 Data File : BN025751.D
 Acq On : 06 Jun 2023 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 15:34:02 2023

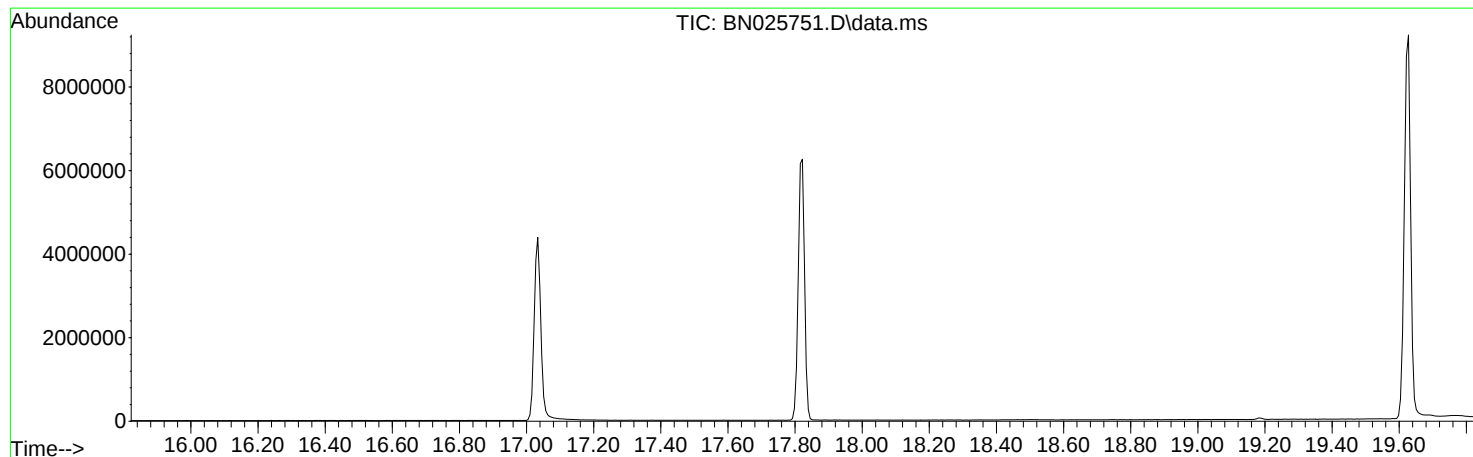

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	242666	PASS
68	69	0.00	2	1.6	4196	PASS
69	198	0.00	100	42.5	254485	PASS
70	69	0.00	2	0.5	1256	PASS
127	198	10	80	47.5	284160	PASS
197	198	0.00	2	0.4	2099	PASS
198	198	100	100	100.0	598144	PASS
199	198	5	9	6.8	40821	PASS
275	198	10	60	24.4	146061	PASS
365	198	1	100	3.3	19976	PASS
441	198	0.01	100	11.1	66408	PASS
442	442	50	100	100.0	418325	PASS
443	442	15	24	20.2	84685	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_N	<u>BN025751.D</u>
Compound Name	Response	Retention Time
DDT	1493640	20.863
DDD	25304	20.416
DDE	3569	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28873	1522513	1.90

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060623\
 Data File : BN025751.D
 Acq On : 06 Jun 2023 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 08:06:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 07 08:06:04 2023
 Response via : Initial Calibration

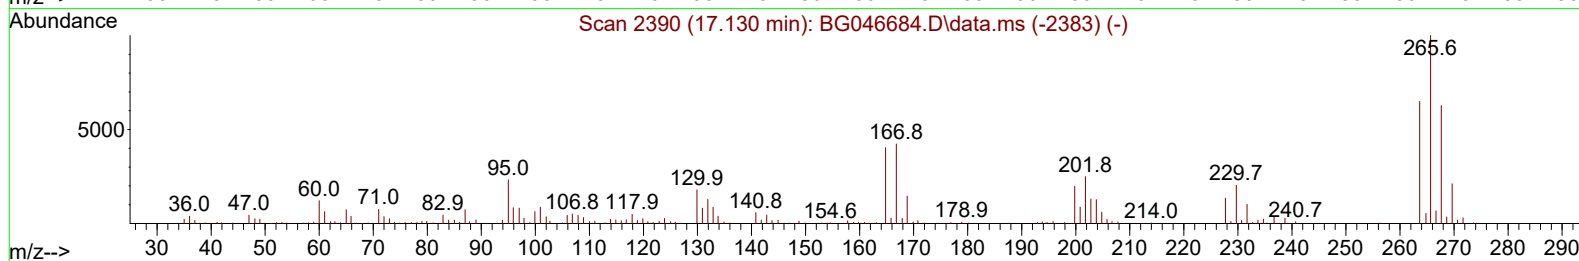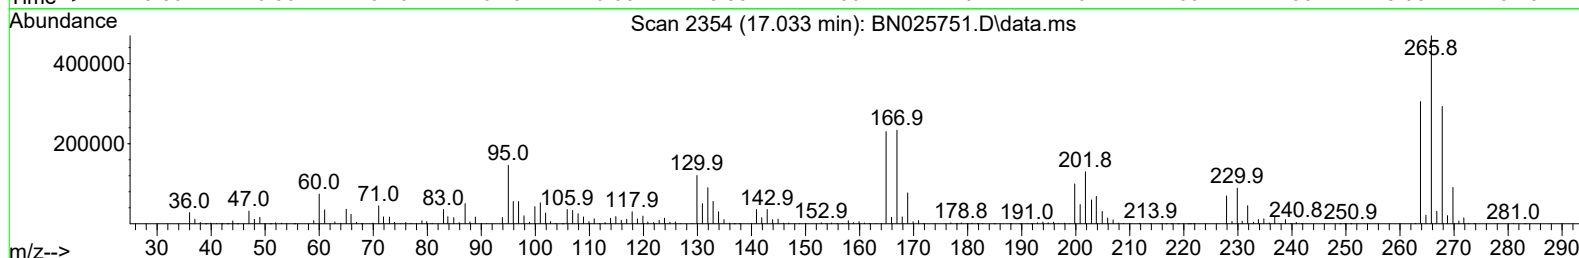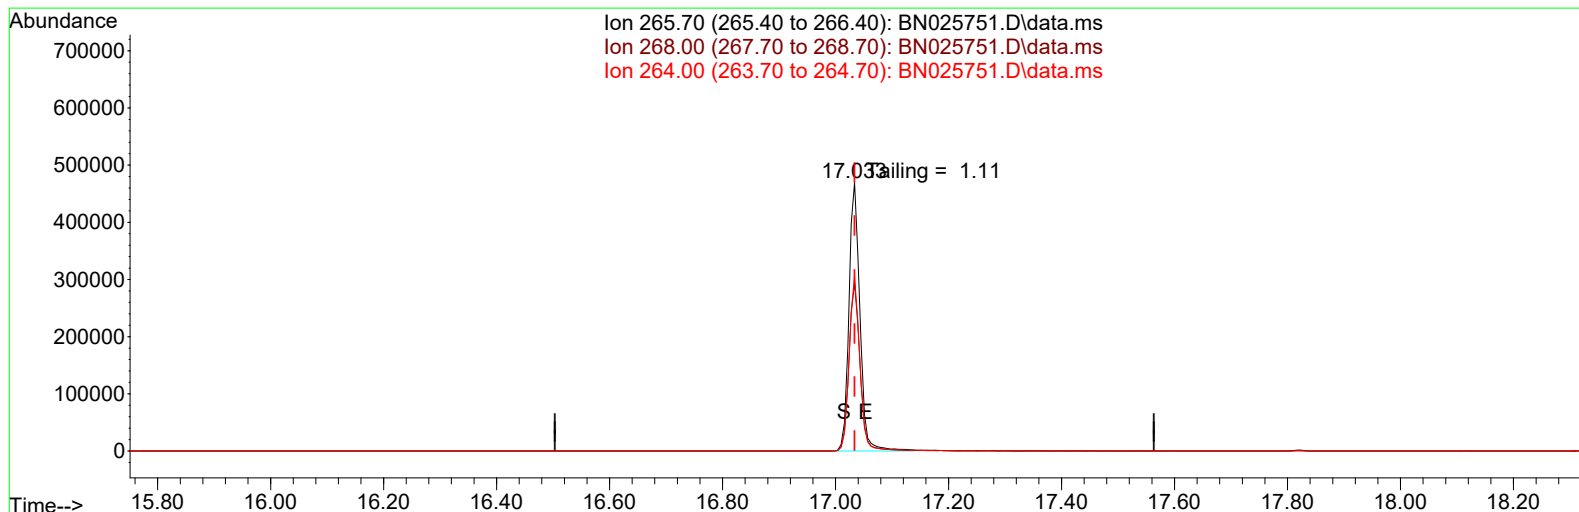

TIC: BN025751.D\data.ms

(70) Pentachlorophenol (C)

17.033min (0.000) 17875.78 ng




response 636331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.41
264.00	61.60	65.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060623\
 Data File : BN025751.D
 Acq On : 06 Jun 2023 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 08:06:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 07 08:06:04 2023
 Response via : Initial Calibration

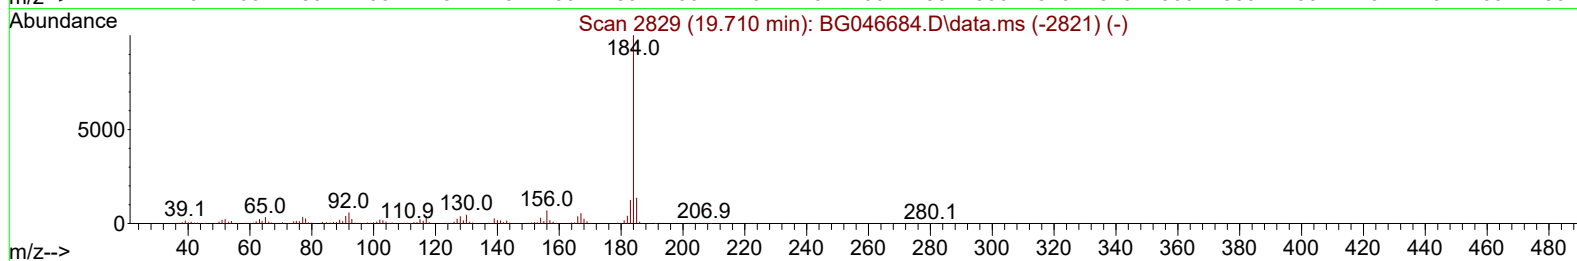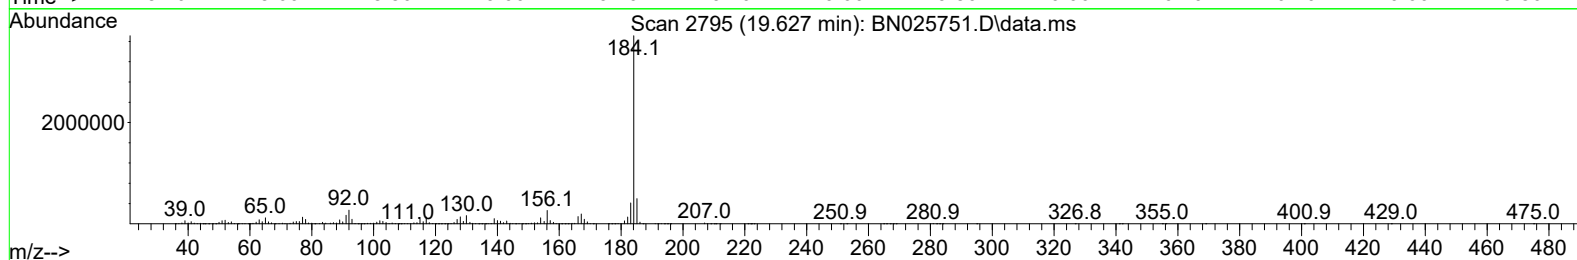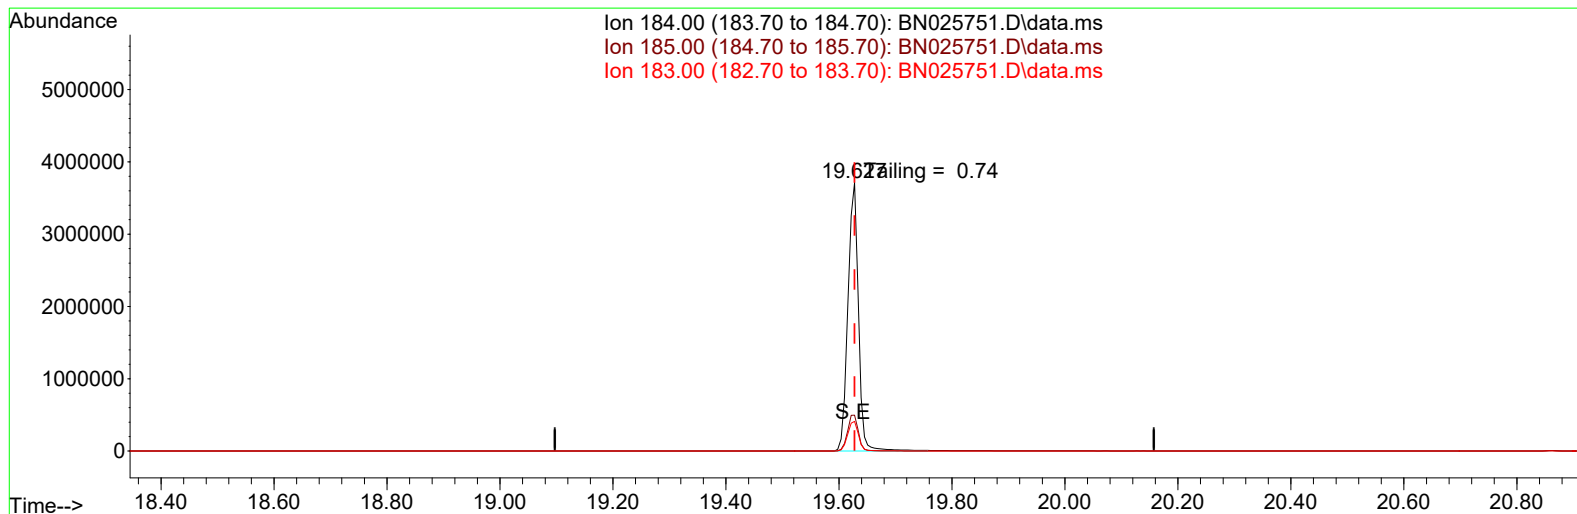

TIC: BN025751.D\data.ms

(77) Benzidine

19.627min (0.000) 0.00 ng

response 4842350

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.40
183.00	13.20	11.03
0.00	0.00	0.00