
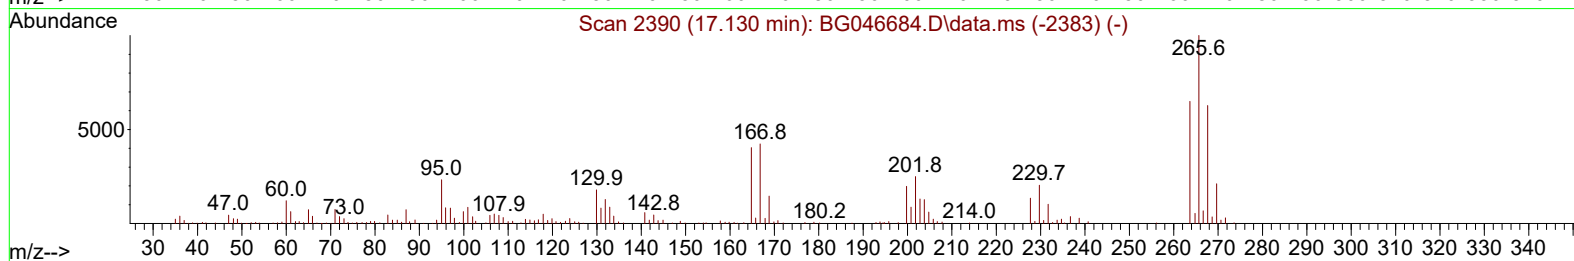
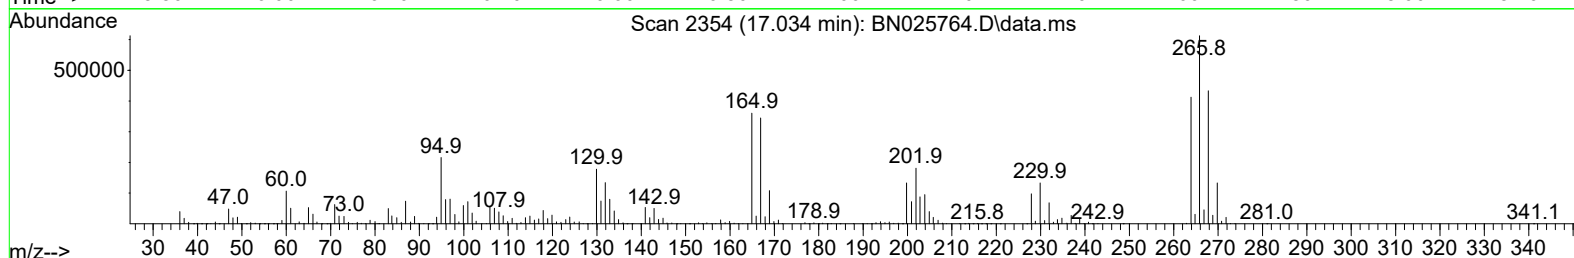


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
Data File : BN025764.D
Acq On : 07 Jun 2023 08:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 04:18:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 04:18:15 2023
Response via : Initial Calibration

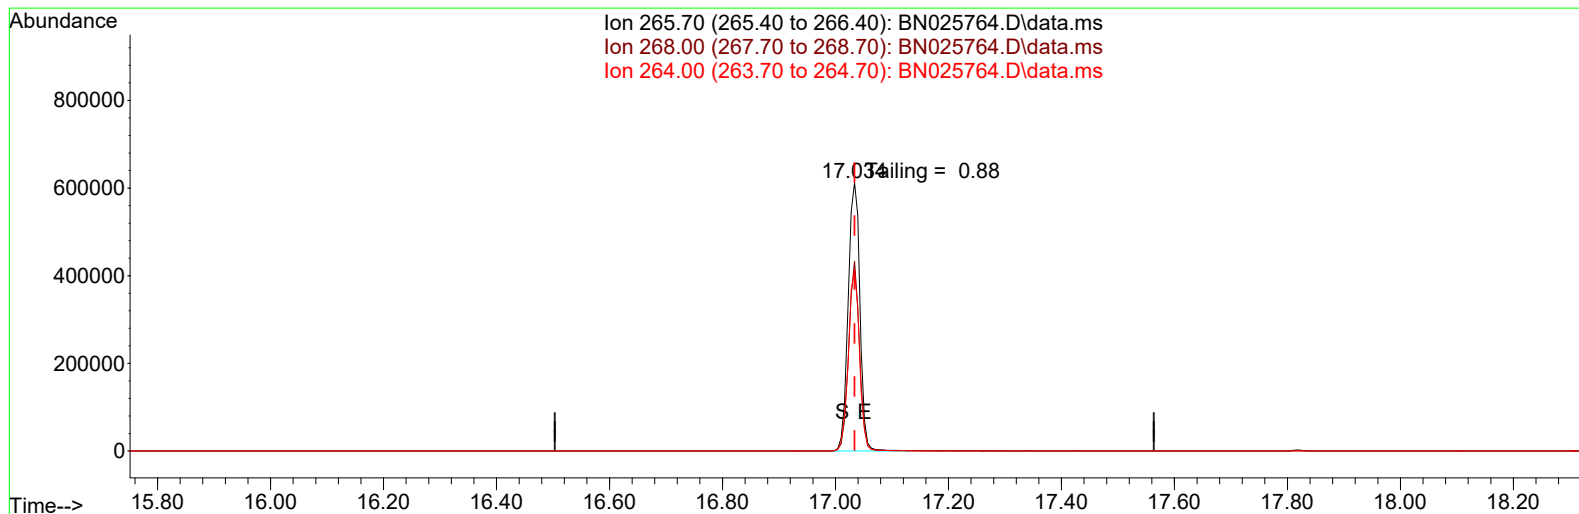

TIC: BN025764.D\data.ms

(70) Pentachlorophenol (C)




17.034min (0.000) 19047.85 ng

response 885984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.74
264.00	61.60	67.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
Data File : BN025764.D
Acq On : 07 Jun 2023 08:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 04:18:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 04:18:15 2023
Response via : Initial Calibration

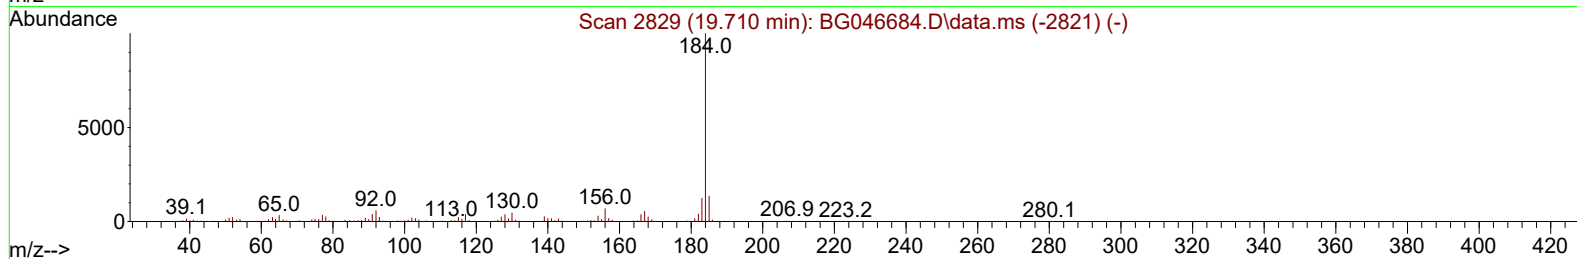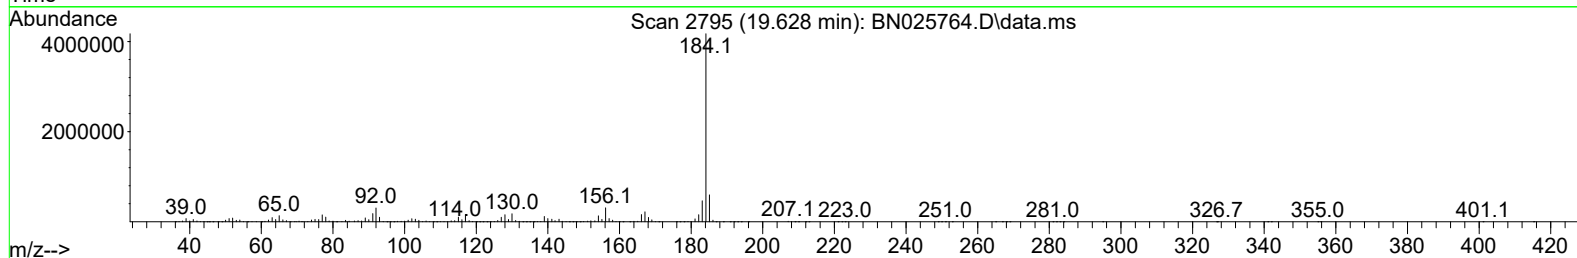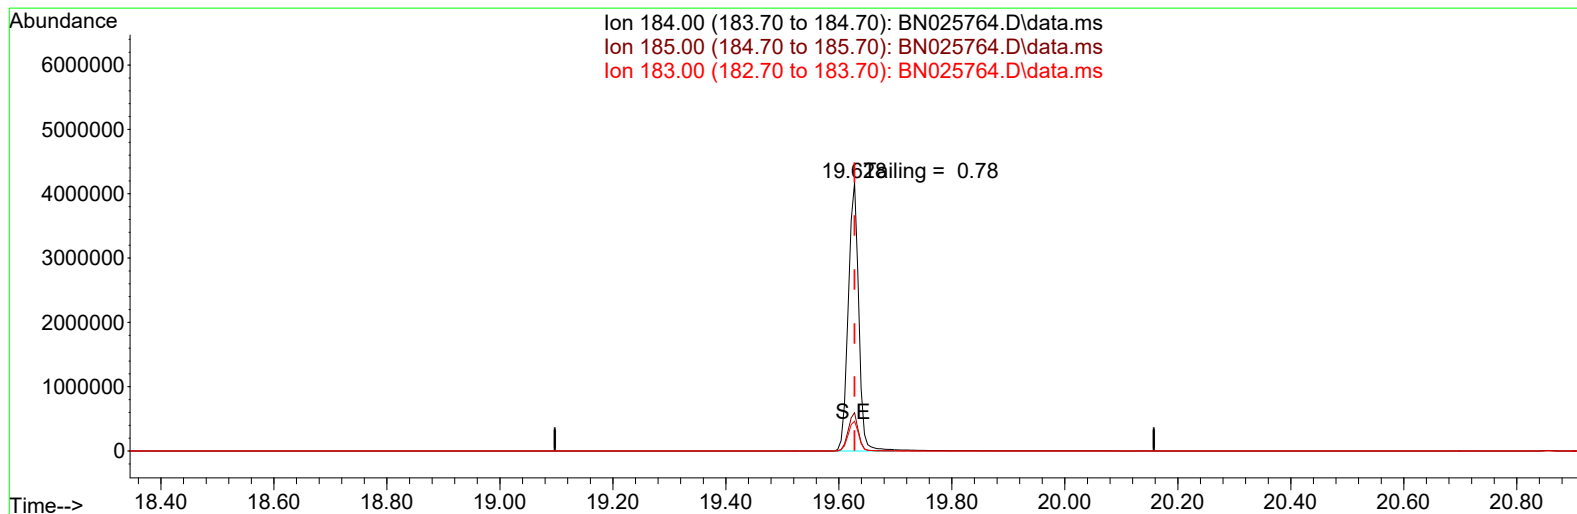

TIC: BN025764.D\data.ms

(77) Benzidine**19.628min (0.000) 1363071.35 ng****response 5336182**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	11.17
0.00	0.00	0.00