


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
 Data File : BN025764.D
 Acq On : 07 Jun 2023 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 15:34:02 2023

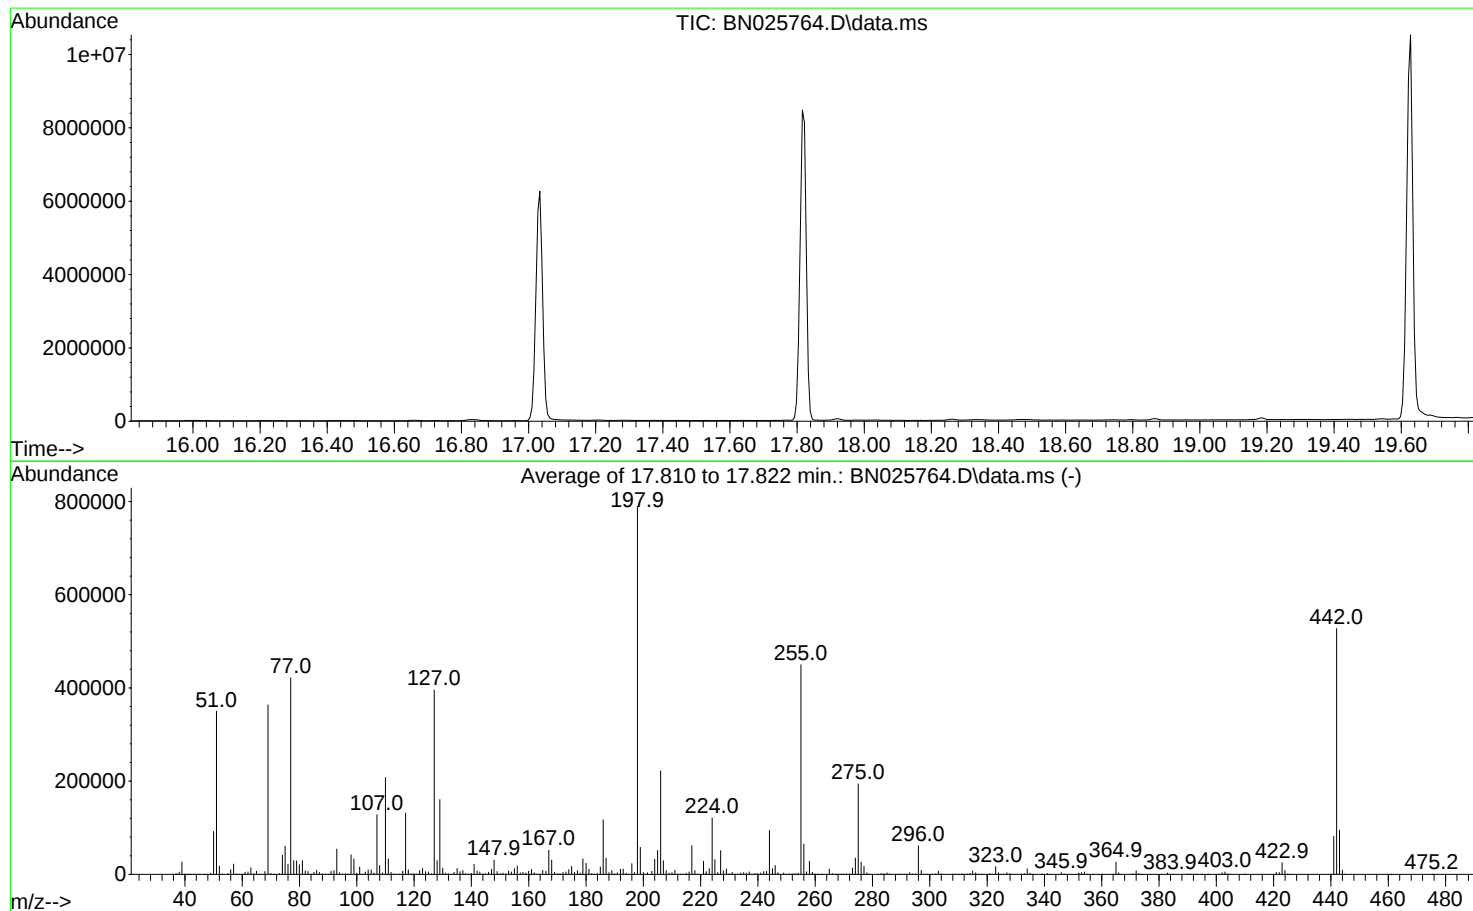

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	349675	PASS
68	69	0.00	2	1.7	6182	PASS
69	198	0.00	100	46.1	363563	PASS
70	69	0.00	2	0.5	1937	PASS
127	198	10	80	50.1	395392	PASS
197	198	0.00	2	0.5	3828	PASS
198	198	100	100	100.0	789248	PASS
199	198	5	9	7.4	58187	PASS
275	198	10	60	24.6	193968	PASS
365	198	1	100	3.3	26093	PASS
441	198	0.01	100	10.3	81421	PASS
442	442	50	100	100.0	527403	PASS
443	442	15	24	18.0	94925	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/7/2023	BNA_N	<u>BN025764.D</u>
Compound Name	Response	Retention Time
DDT	1895718	20.857
DDD	29210	20.469
DDE	2771	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31981	1927699	1.66

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
Data File : BN025764.D
Acq On : 07 Jun 2023 08:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 08 04:18:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 04:18:15 2023
Response via : Initial Calibration

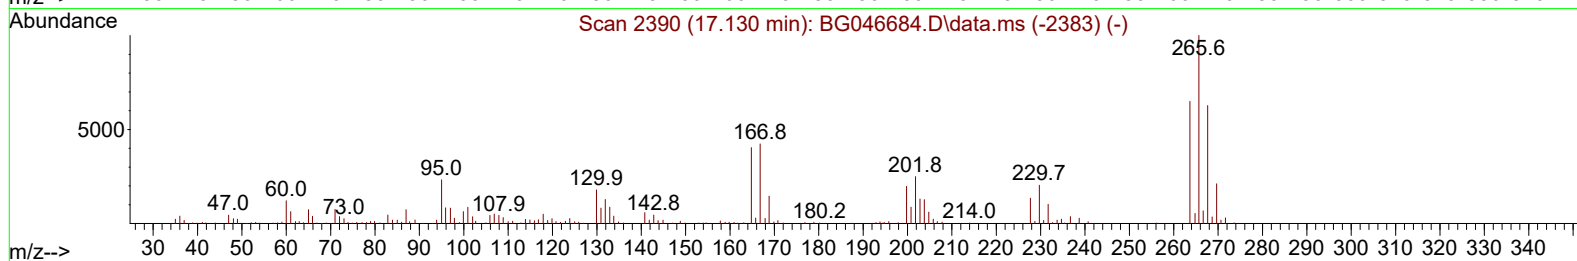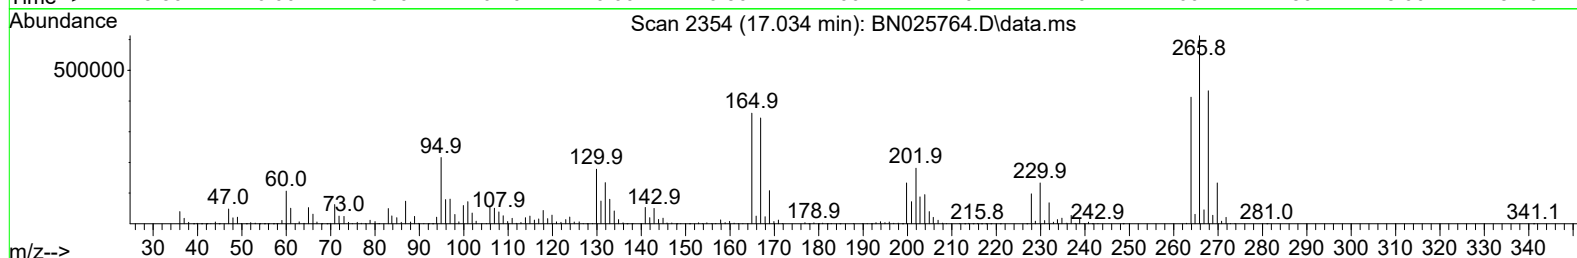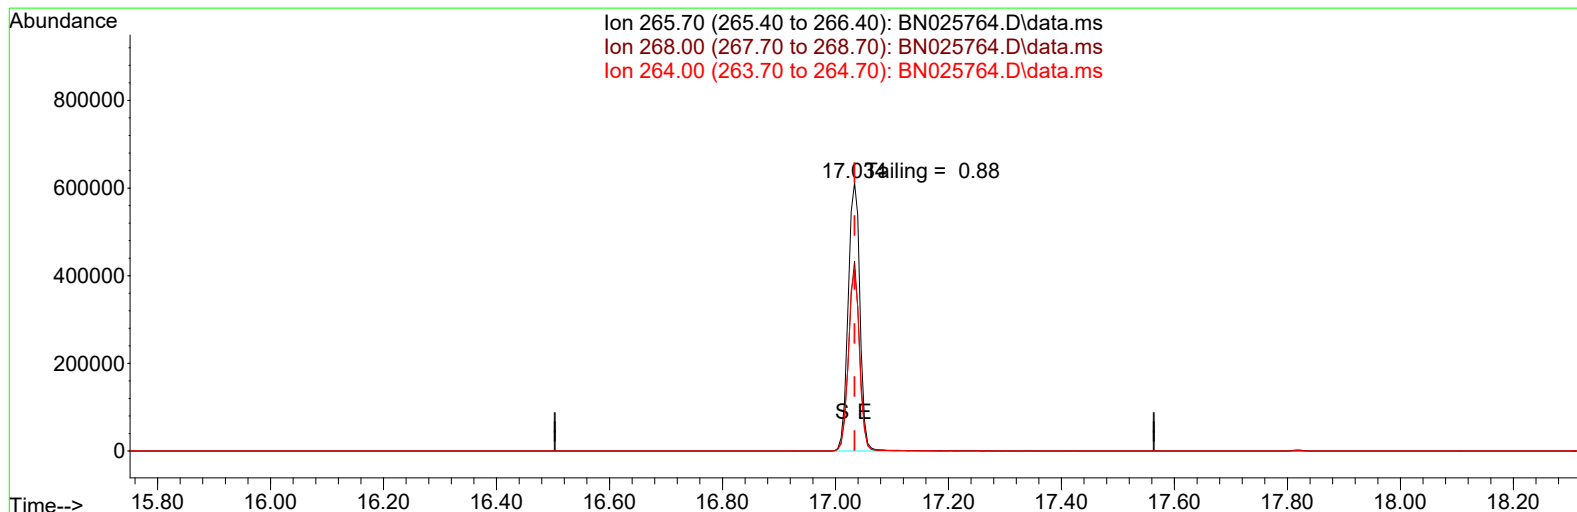

TIC: BN025764.D\data.ms

(70) Pentachlorophenol (C)

17.034min (0.000) 19047.85 ng




response 885984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.74
264.00	61.60	67.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
 Data File : BN025764.D
 Acq On : 07 Jun 2023 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 08 04:18:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 04:18:15 2023
 Response via : Initial Calibration

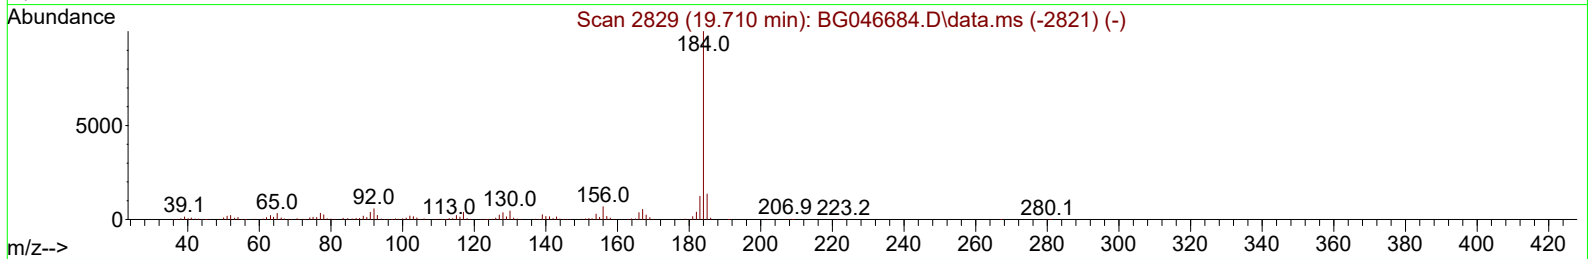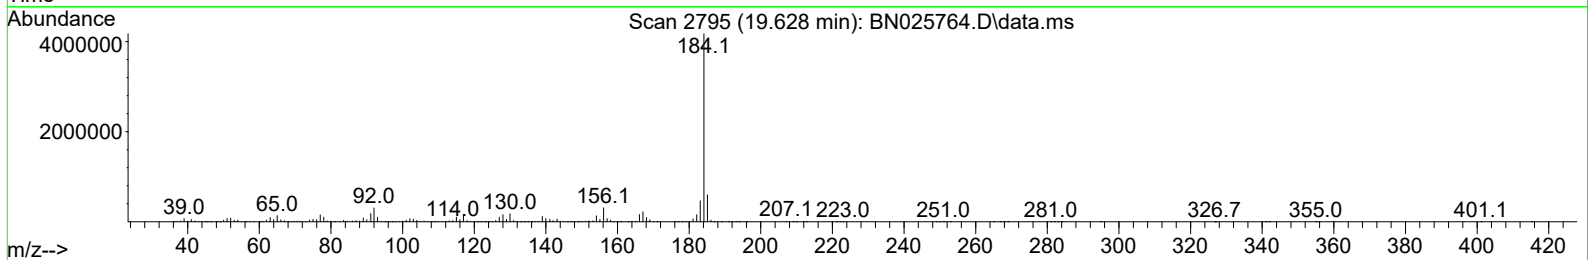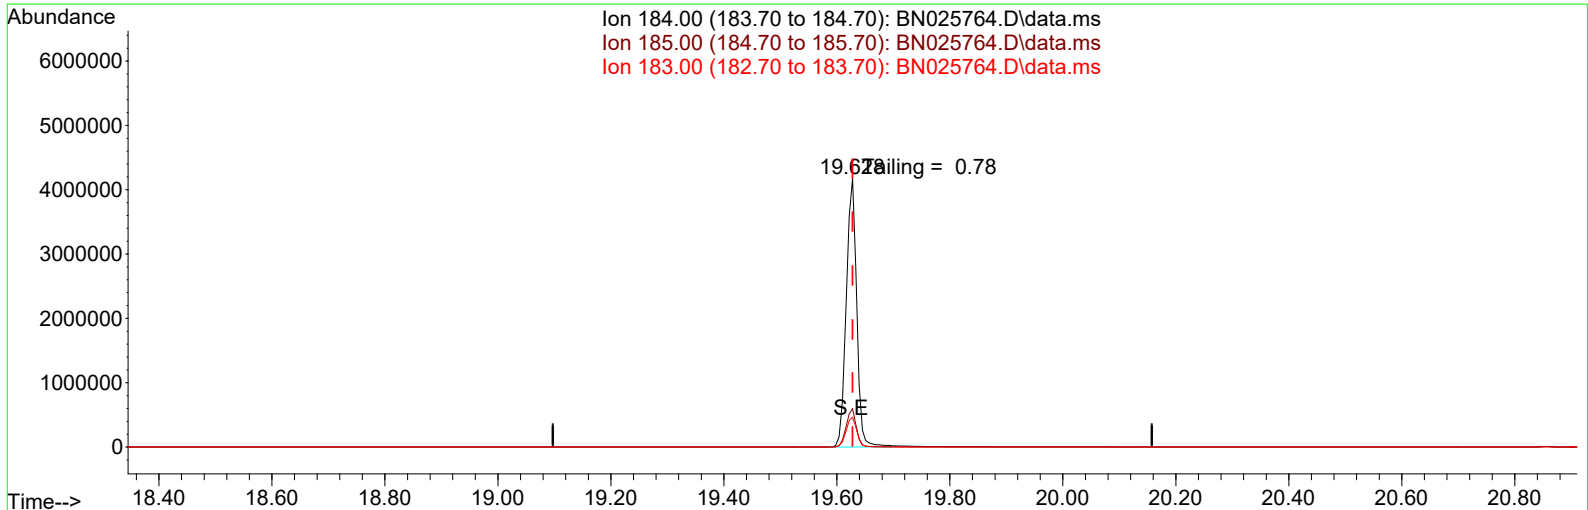

TIC: BN025764.D\data.ms

(77) Benzidine

19.628min (0.000) 1363071.35 ng

response 5336182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	11.17
0.00	0.00	0.00