
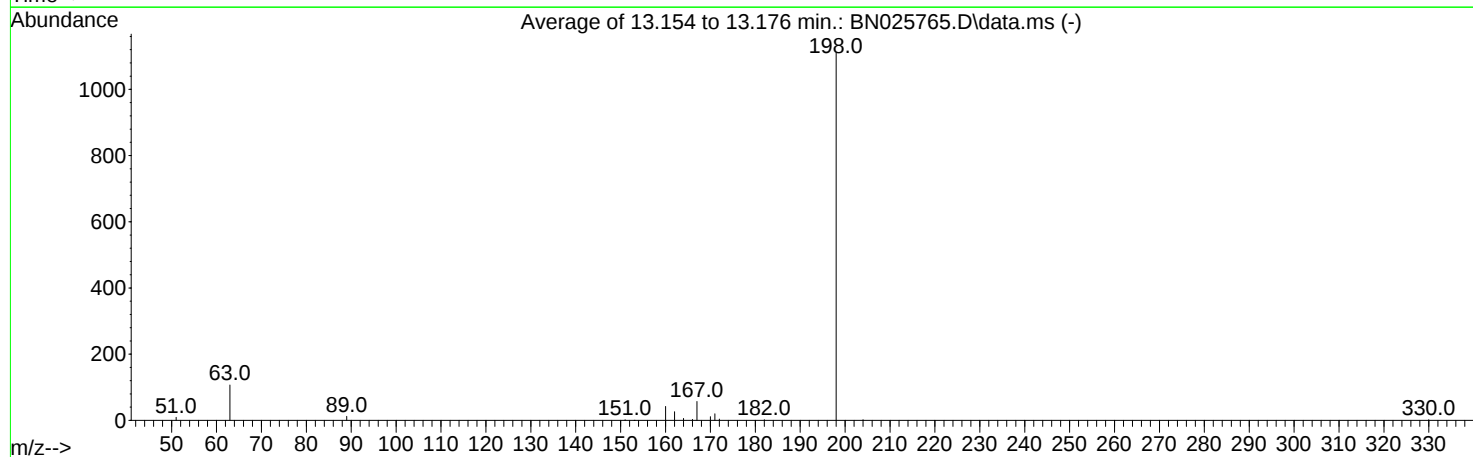


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
 Data File : BN025765.D
 Acq On : 07 Jun 2023 09:20
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 06 15:34:02 2023

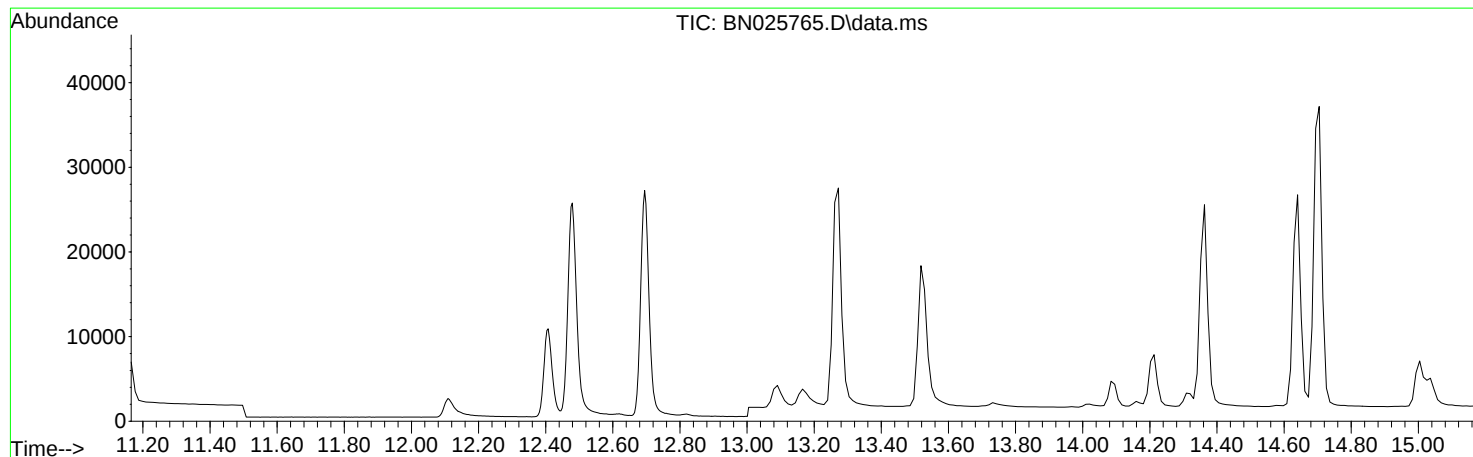

AutoFind: Scans 1420, 1421, 1422; Background Corrected with Scan 1417

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	0.8	9	FAIL*
68.00	69.00	COMPARISON MASS IS NOT PRESENT!!!				
69	198	0.00	100	0.0	0	PASS
70.00	69.00	COMPARISON MASS IS NOT PRESENT!!!				
127	198	10	80	0.0	0	FAIL*
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1111	PASS
199	198	5	9	0.0	0	FAIL*
275	198	10	60	0.0	0	FAIL*
365	198	1	100	0.0	0	FAIL*
441	198	0.01	100	0.0	0	FAIL*
442.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				
443.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/7/2023	BNA_N	<u>BN025764.D</u>
Compound Name	Response	Retention Time
DDT	1895718	20.857
DDD	29210	20.469
DDE	2771	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31981	1927699	1.66

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
 Data File : BN025764.D
 Acq On : 07 Jun 2023 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Quant Time: Jun 08 04:18:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 04:18:15 2023
 Response via : Initial Calibration

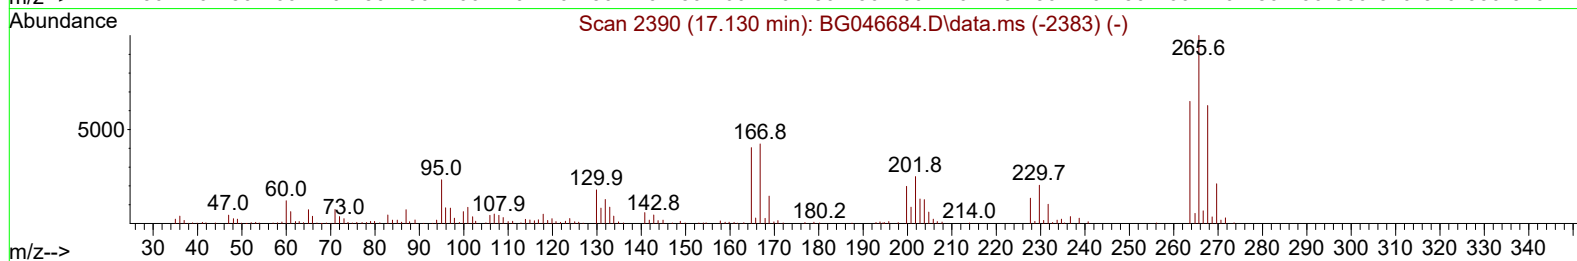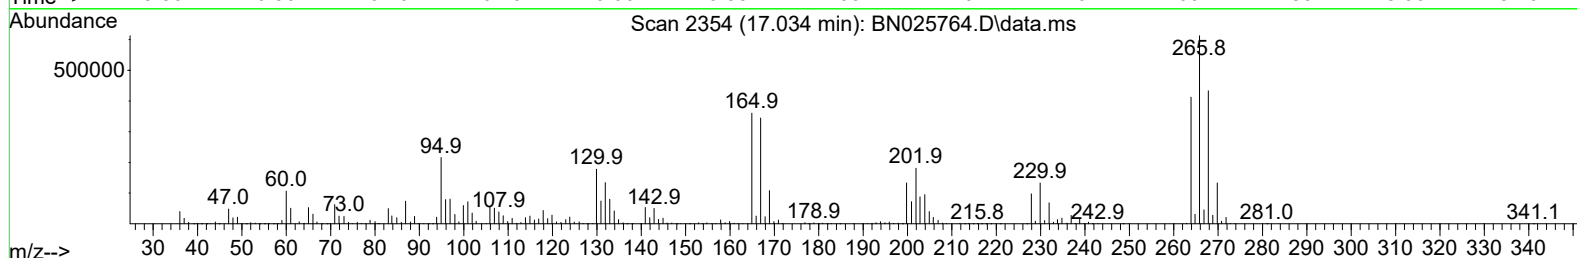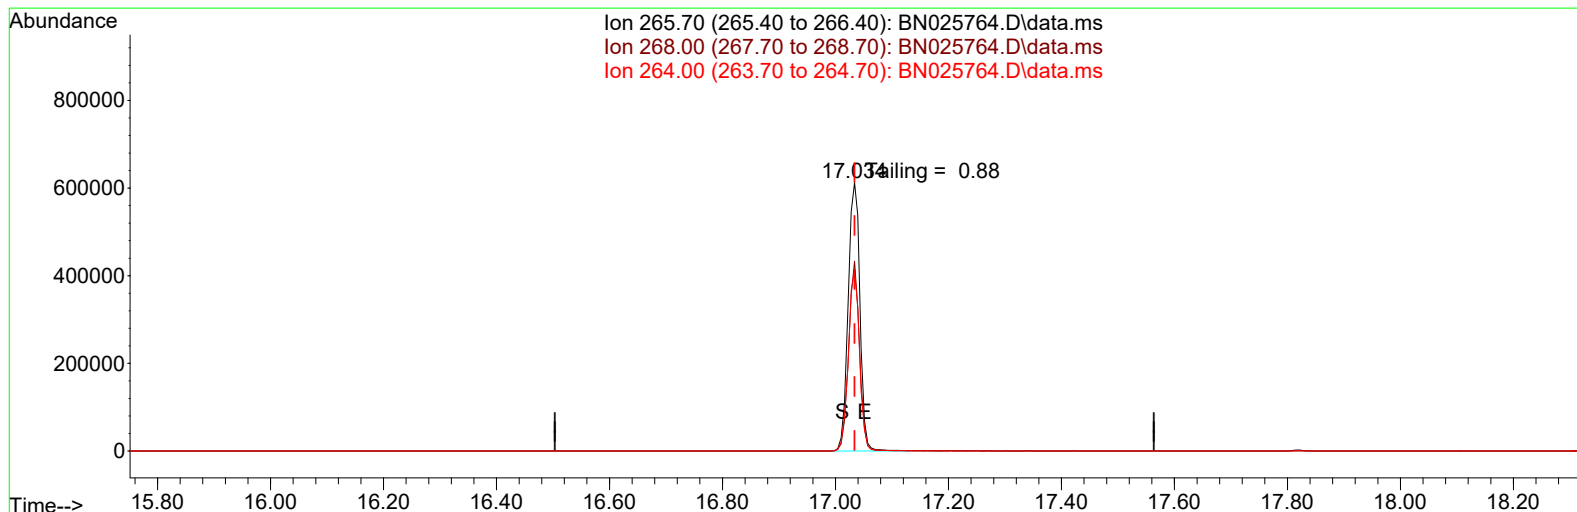

TIC: BN025764.D\data.ms

(70) Pentachlorophenol (C)

17.034min (0.000) 19047.85 ng




response 885984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.74
264.00	61.60	67.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060723\
Data File : BN025764.D
Acq On : 07 Jun 2023 08:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Quant Time: Jun 08 04:18:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 04:18:15 2023
Response via : Initial Calibration

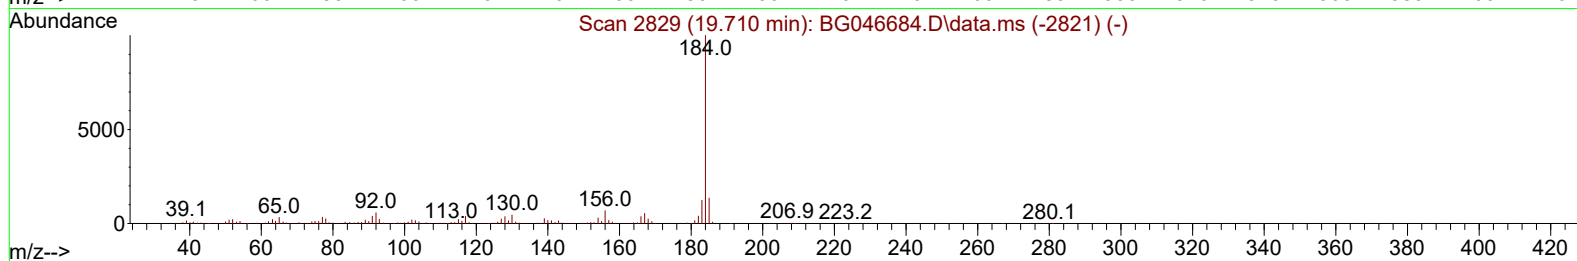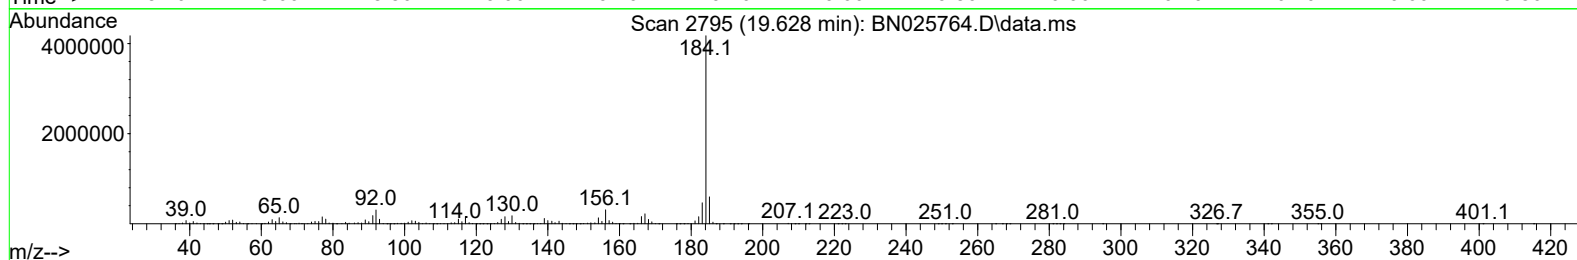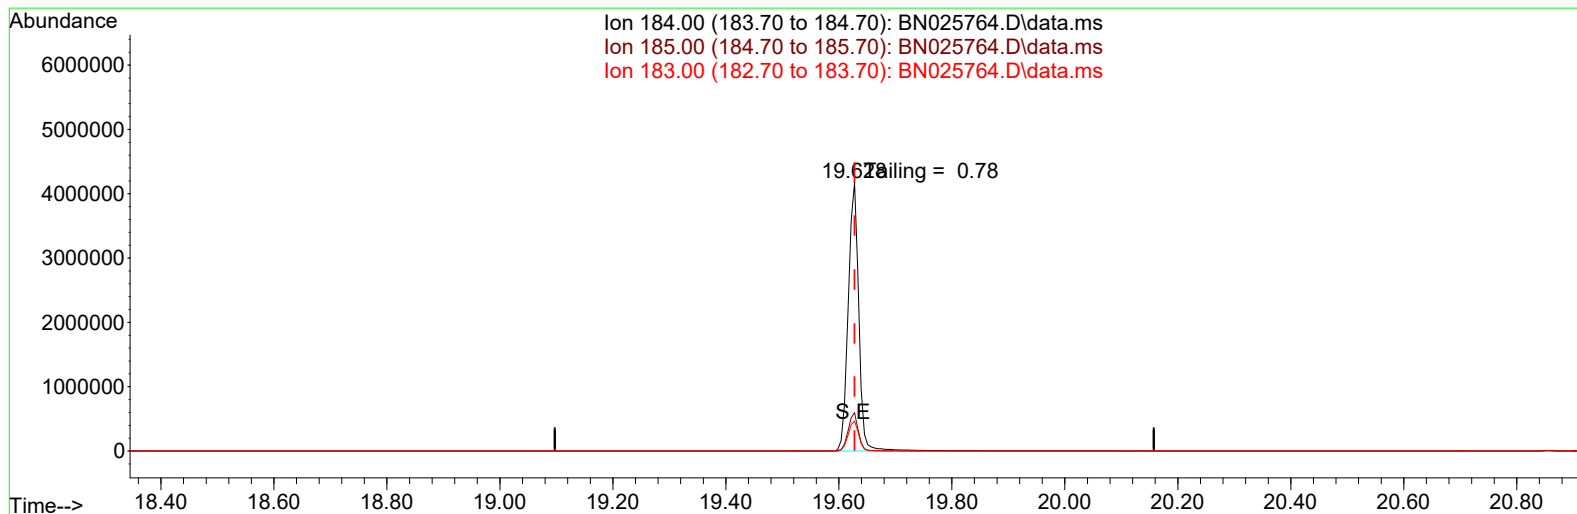

TIC: BN025764.D\data.ms

(77) Benzidine

19.628min (0.000) 1363071.35 ng

response 5336182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	11.17
0.00	0.00	0.00