


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (QT Reviewed)
Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:29:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

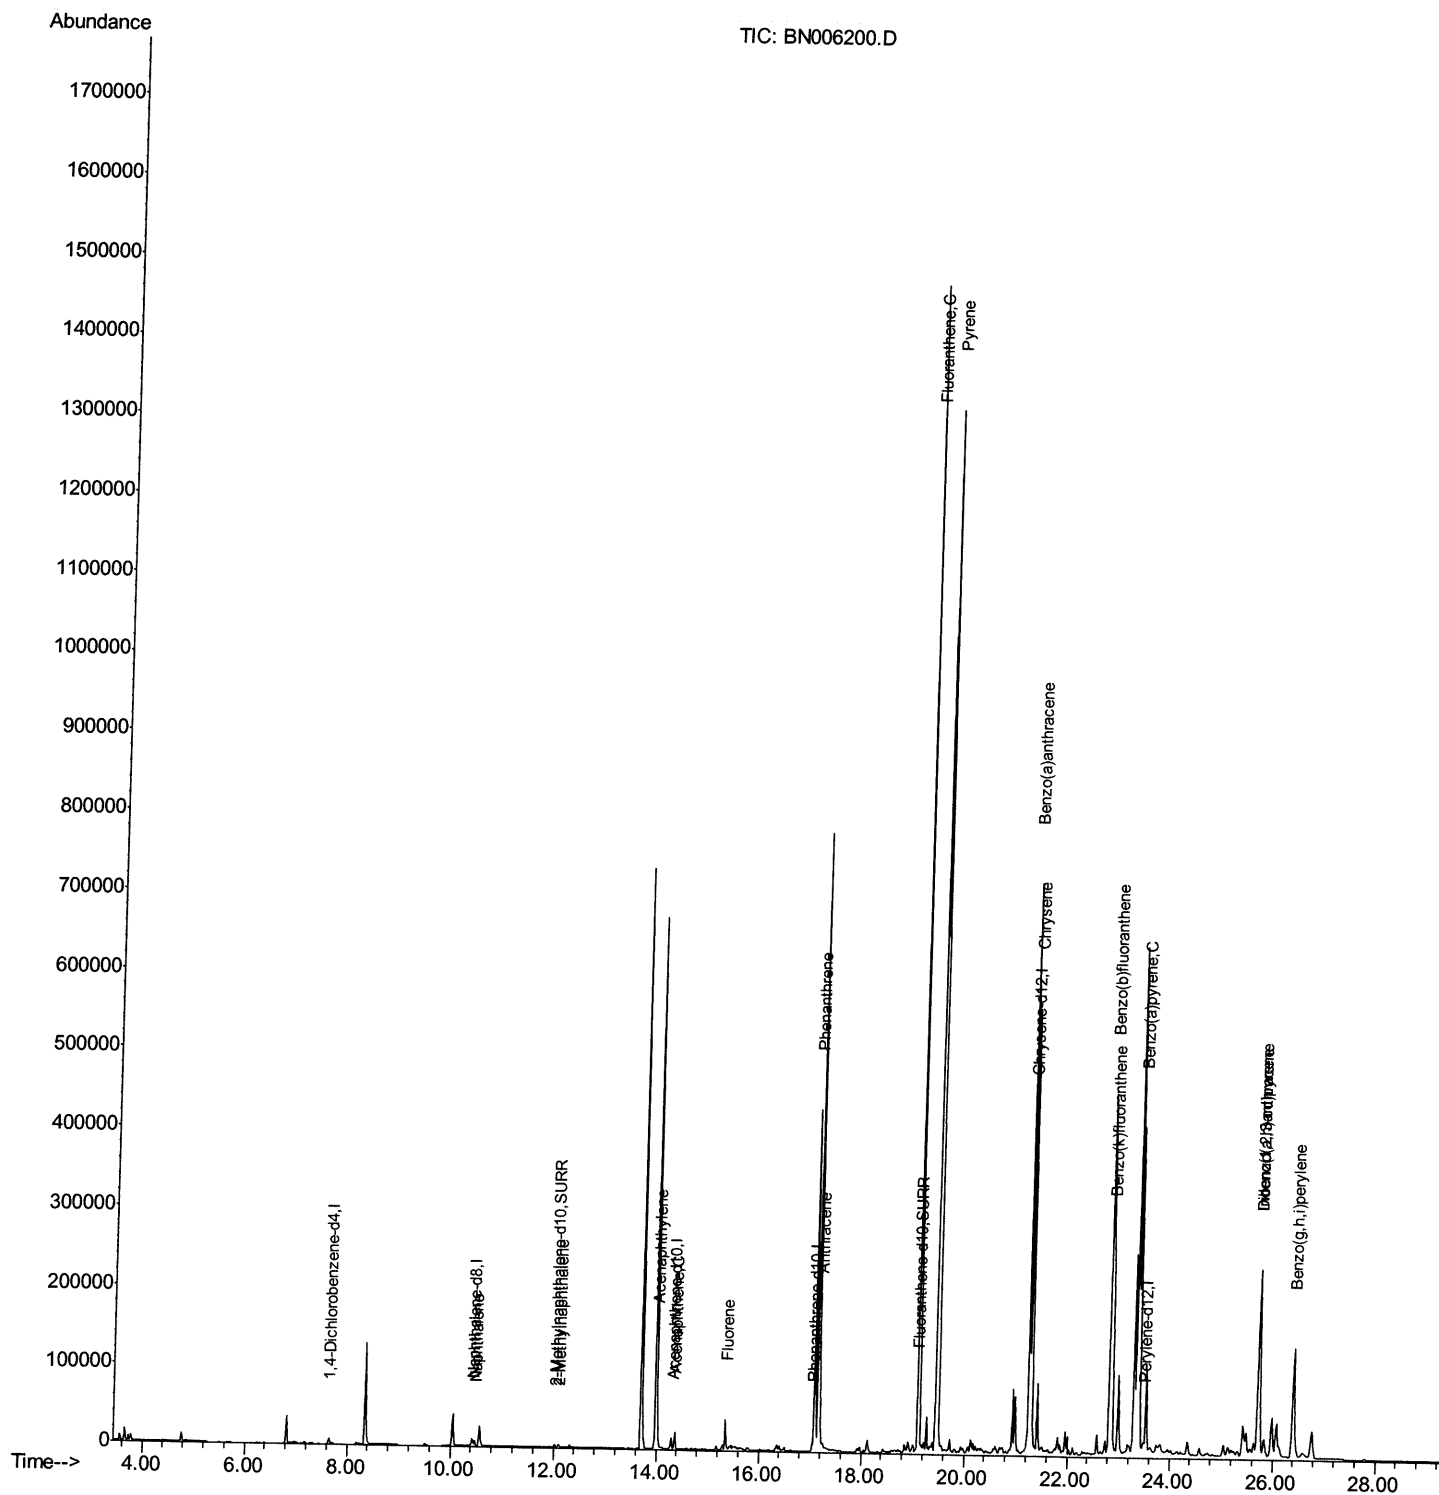

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)


Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:14:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

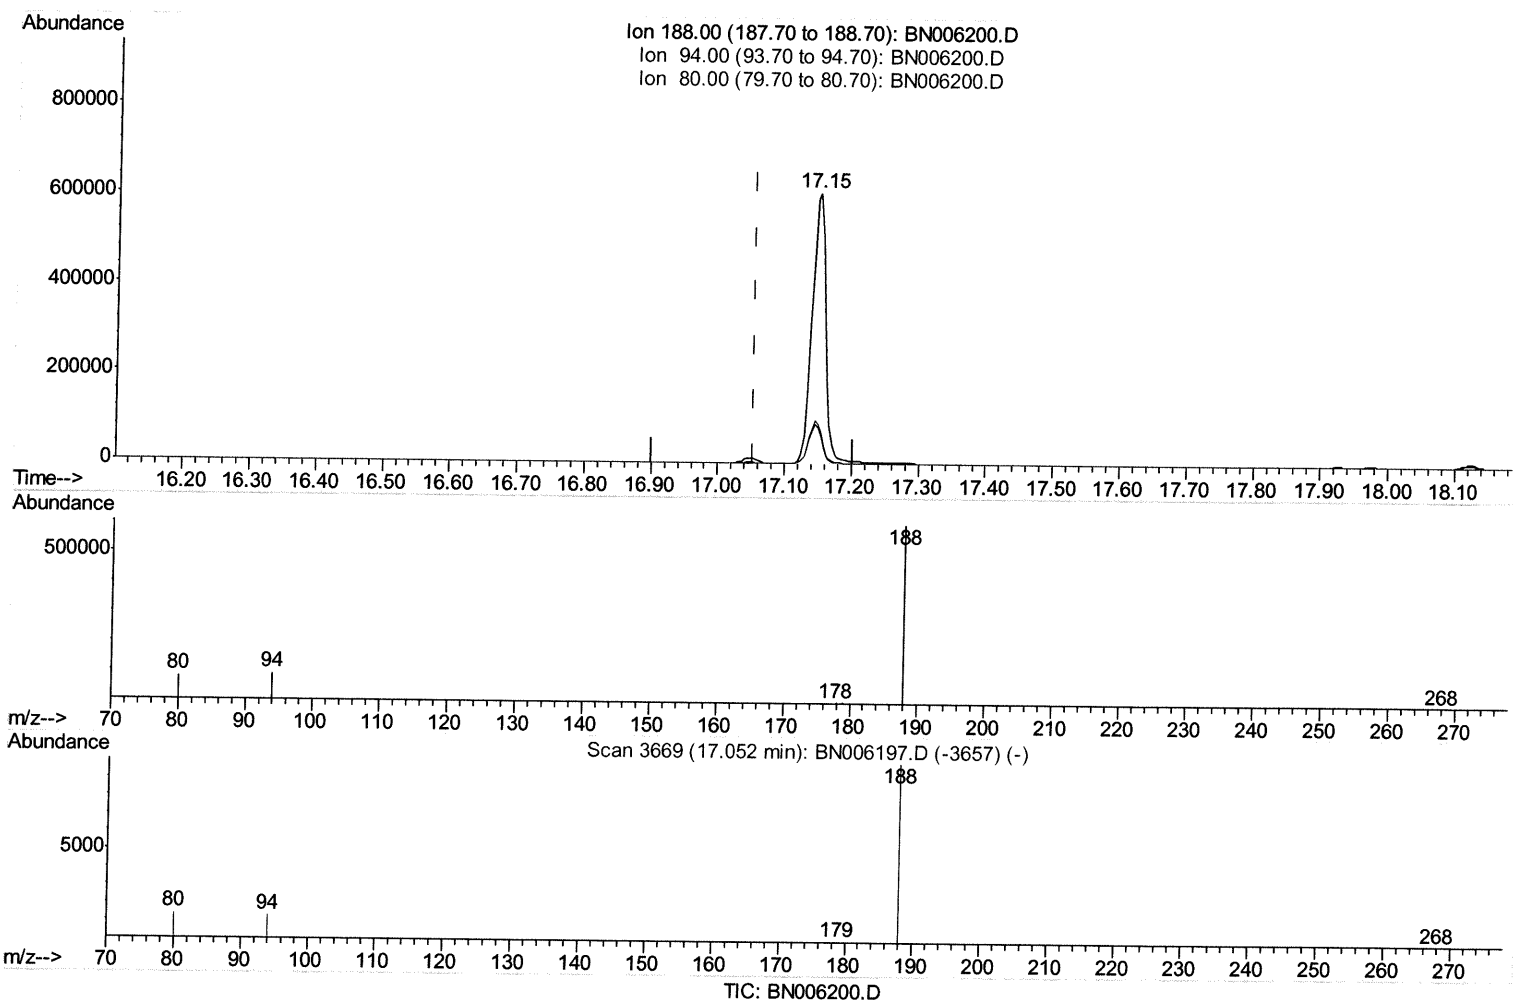

(10) Phenanthrene-d10 (I)

17.149min (+0.097) 0.40ng/ul

response 862304

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.64
80.00	13.60	13.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:14:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

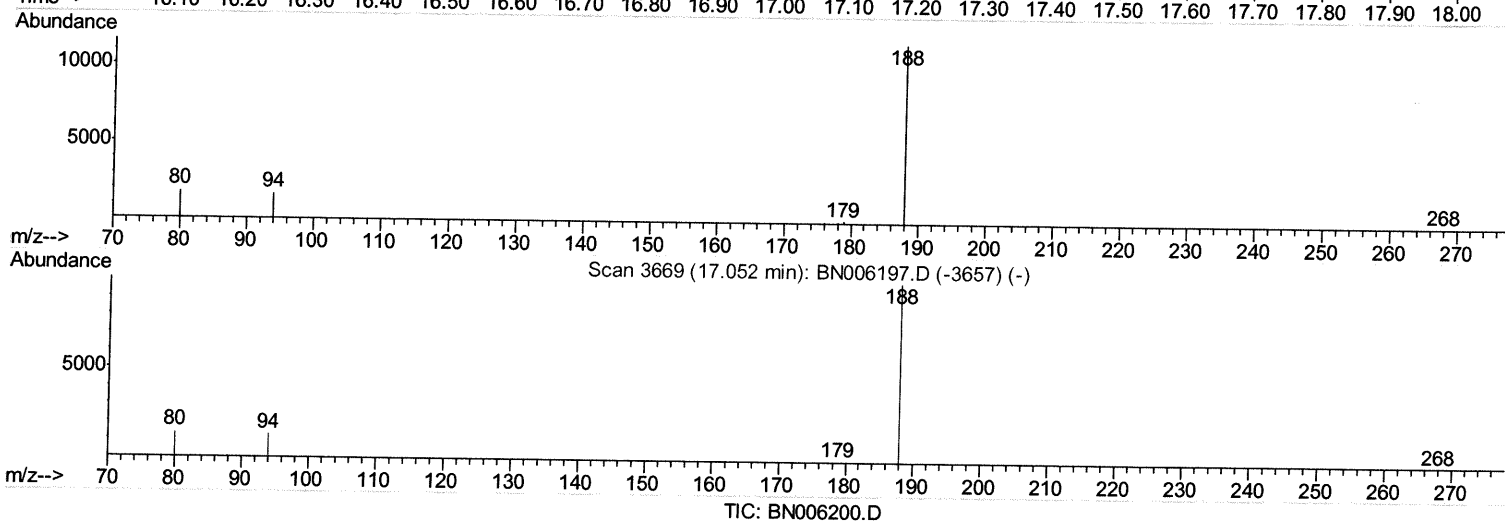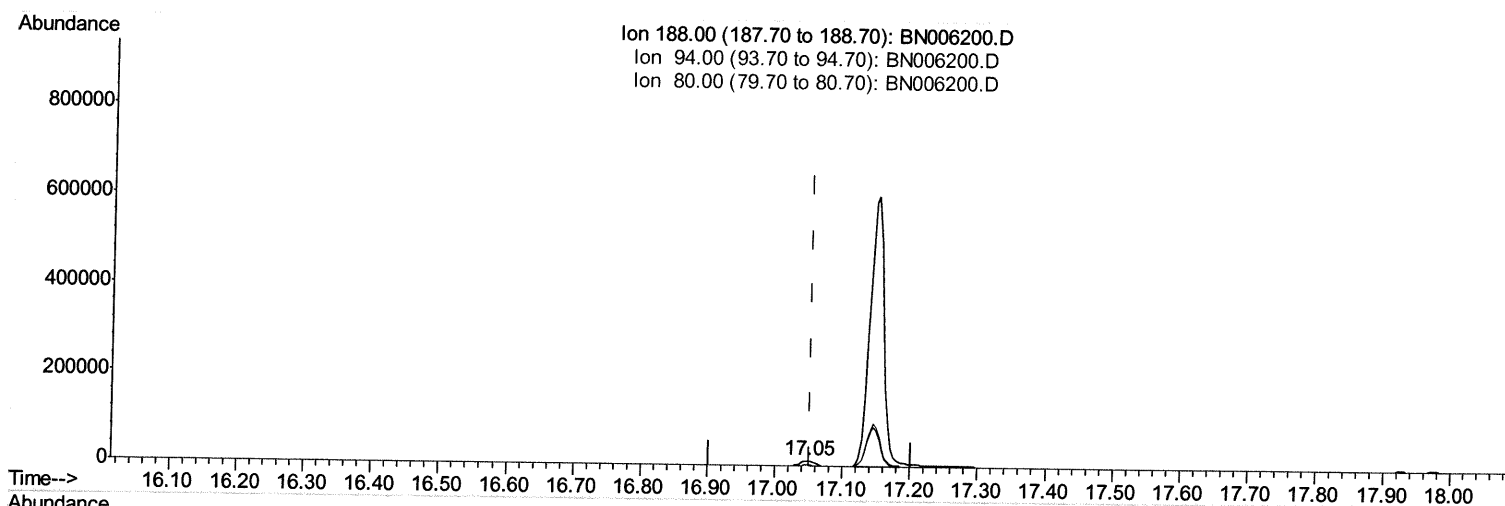

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m *JU* 06/10/19

response 16691

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.16
80.00	13.60	15.70
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)


Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

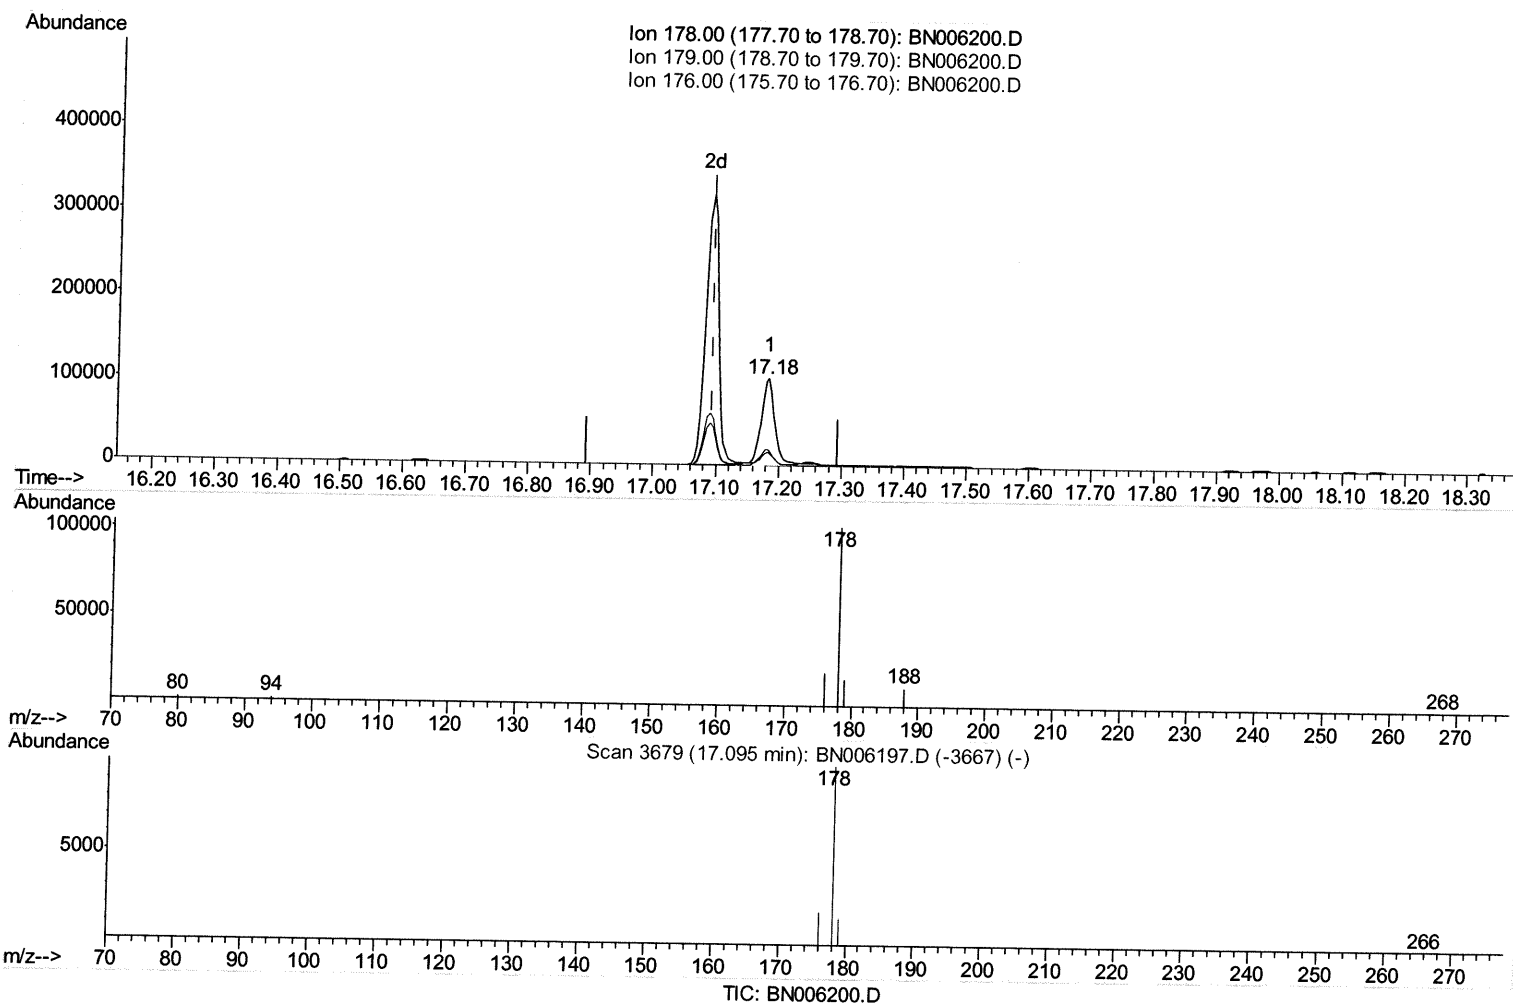

(12) Phenanthrene

17.183min (+0.089) 3.07ng/ul

response 164486

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.42
176.00	19.10	18.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)


Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

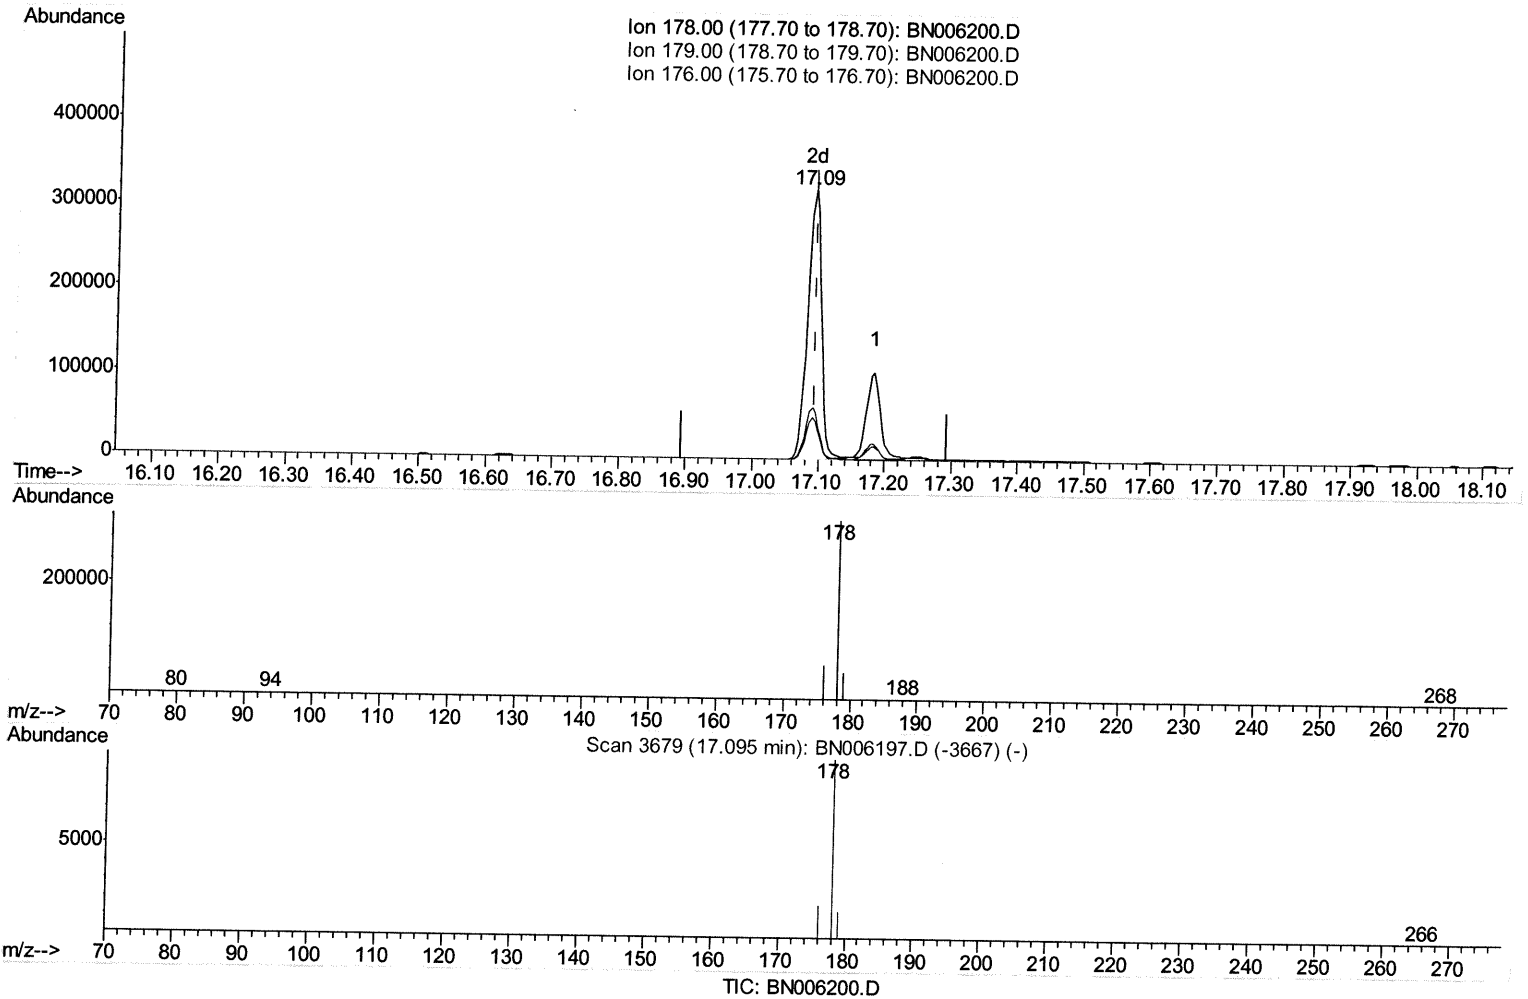

(12) Phenanthrene

17.090min (-0.004) 8.50ng/ul m

JU
06/10/19

response 455387

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.26
176.00	19.10	19.29
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)


Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

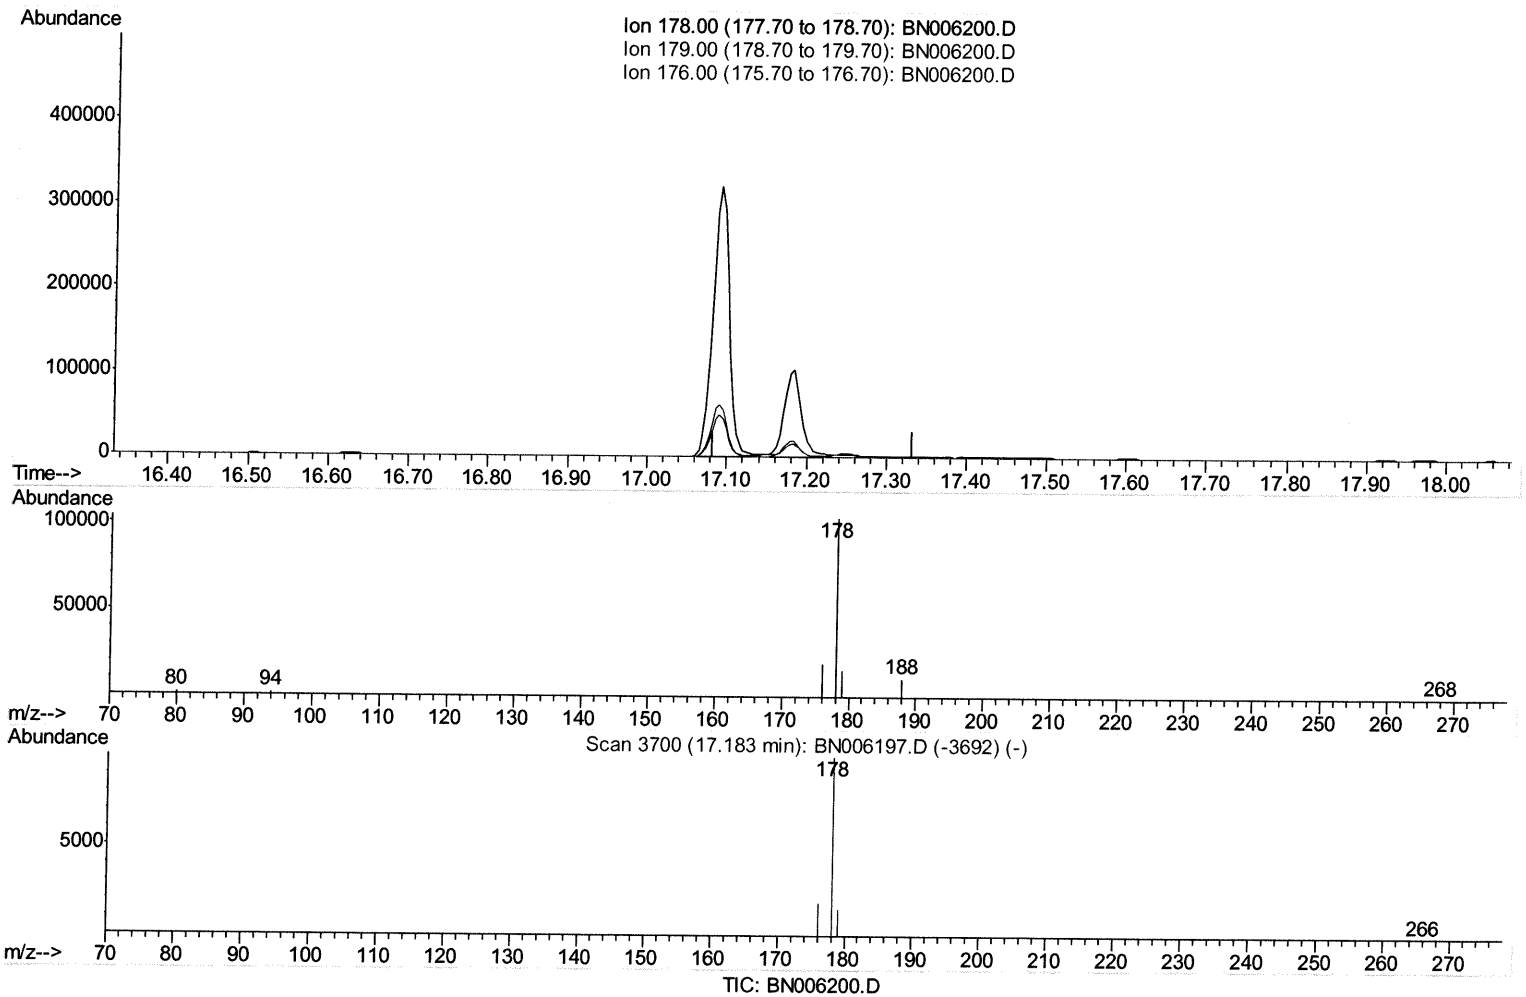

(13) Anthracene

17.183min (-17.183) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.30	0.00#
176.00	18.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

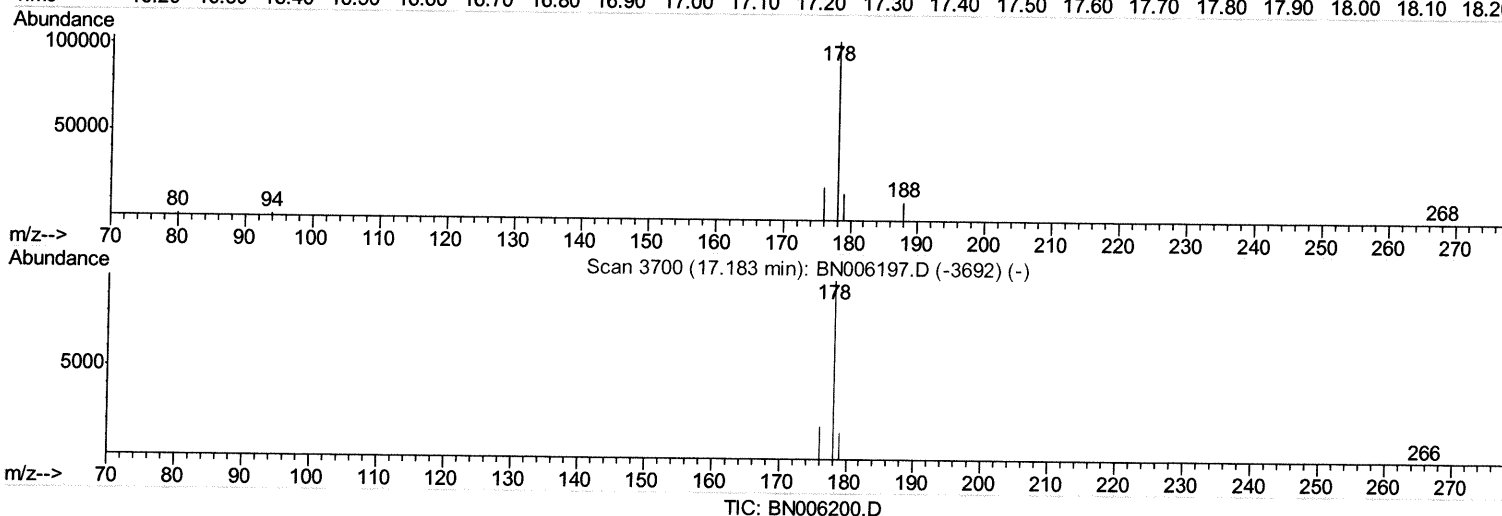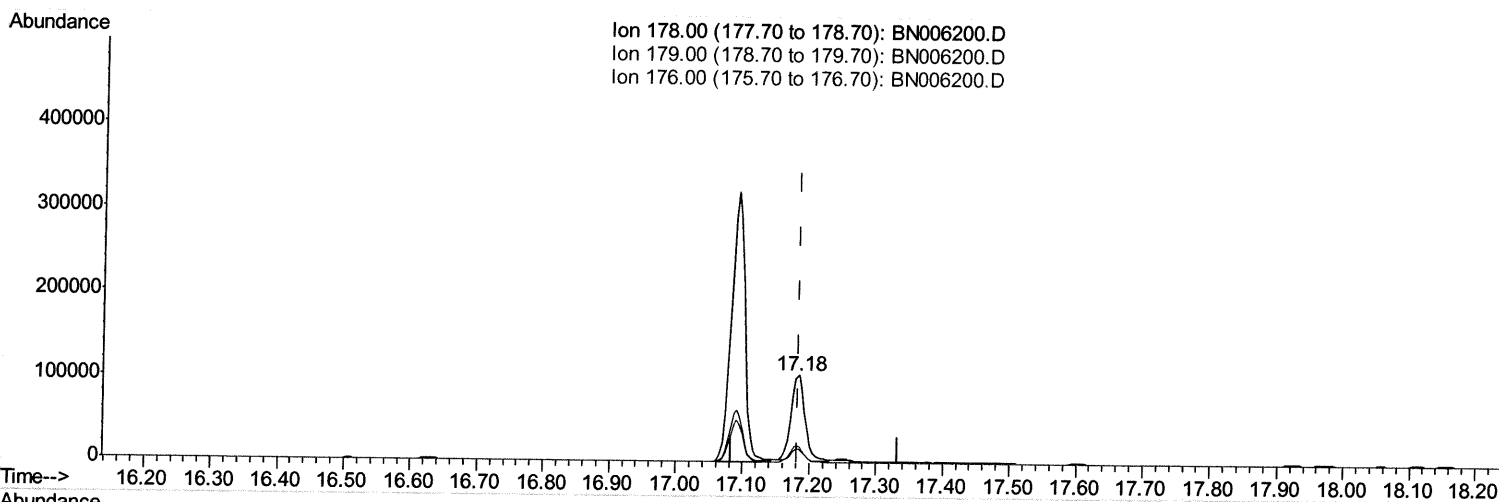

(13) Anthracene

17.183min (-0.000) 3.14ng/ul m

JU
06/10/19

response 160502

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	15.42
176.00	18.90	18.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

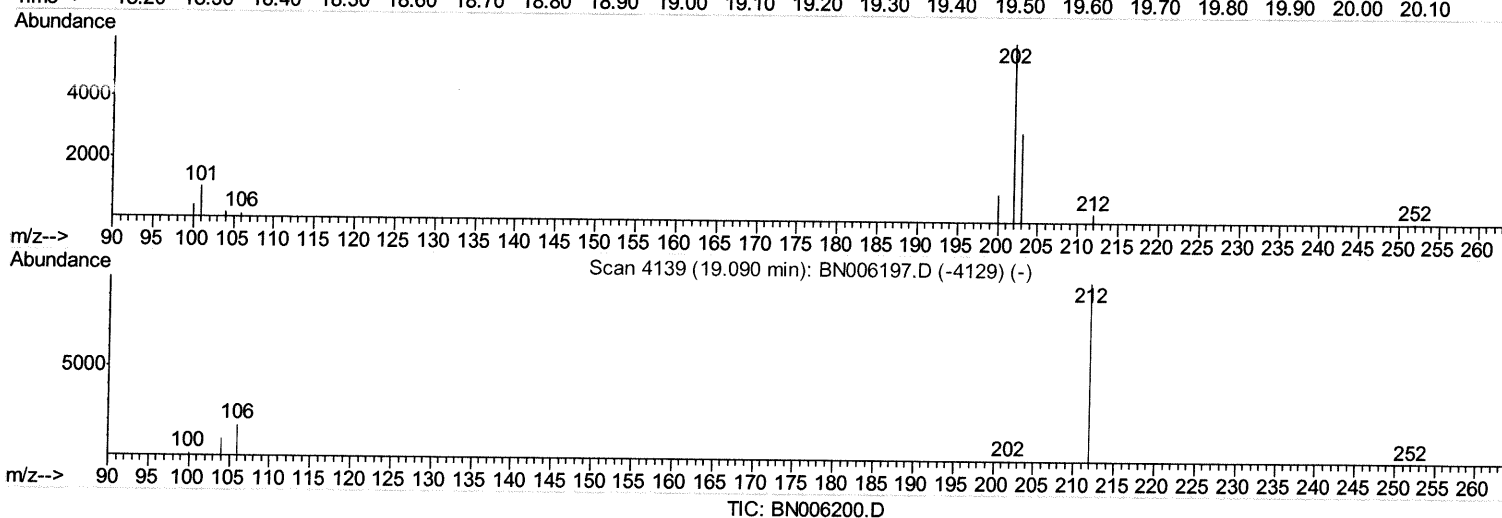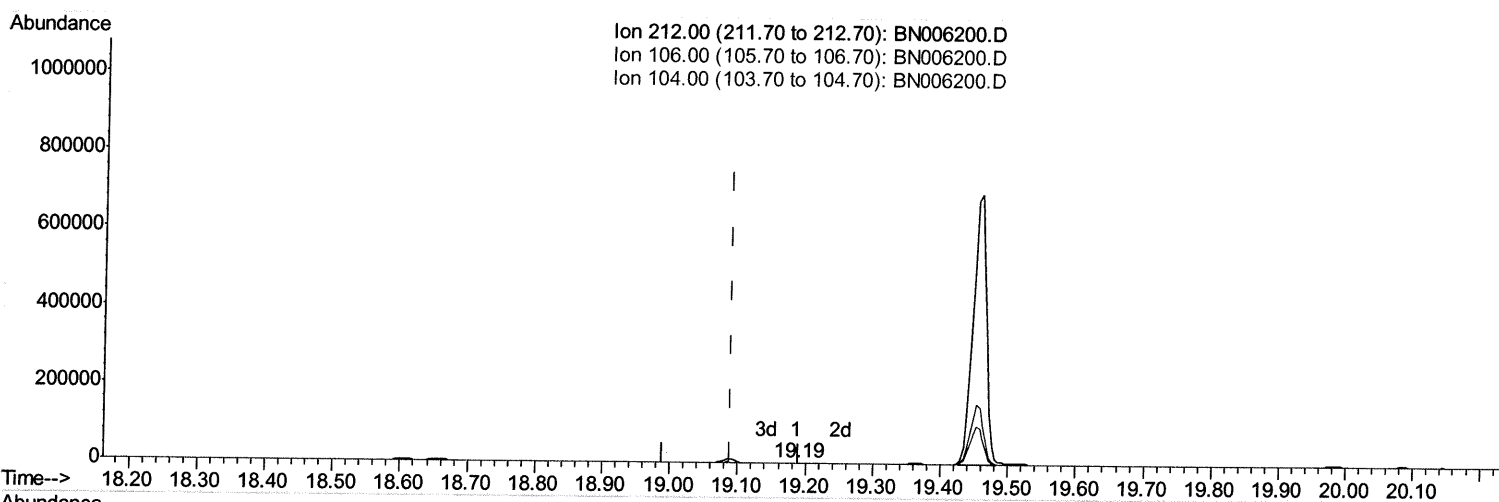

(14) Fluoranthene-d10 (SURR)

19.188min (+0.098) 0.01ng/ul

response 402

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	17.41
104.00	9.90	25.87#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

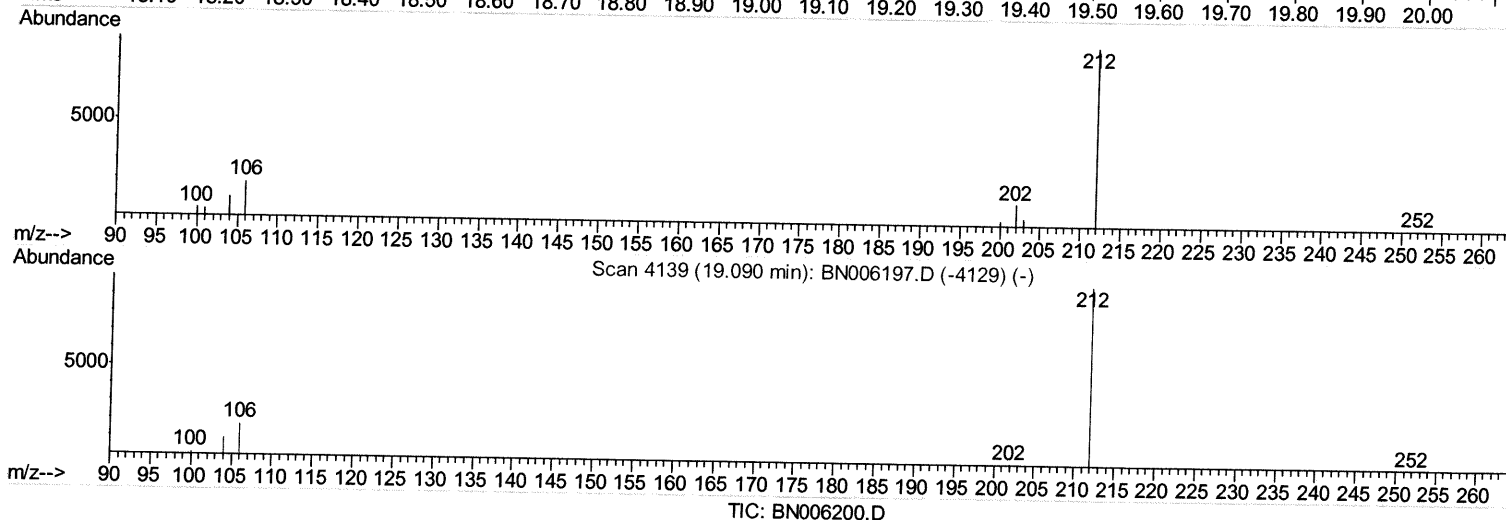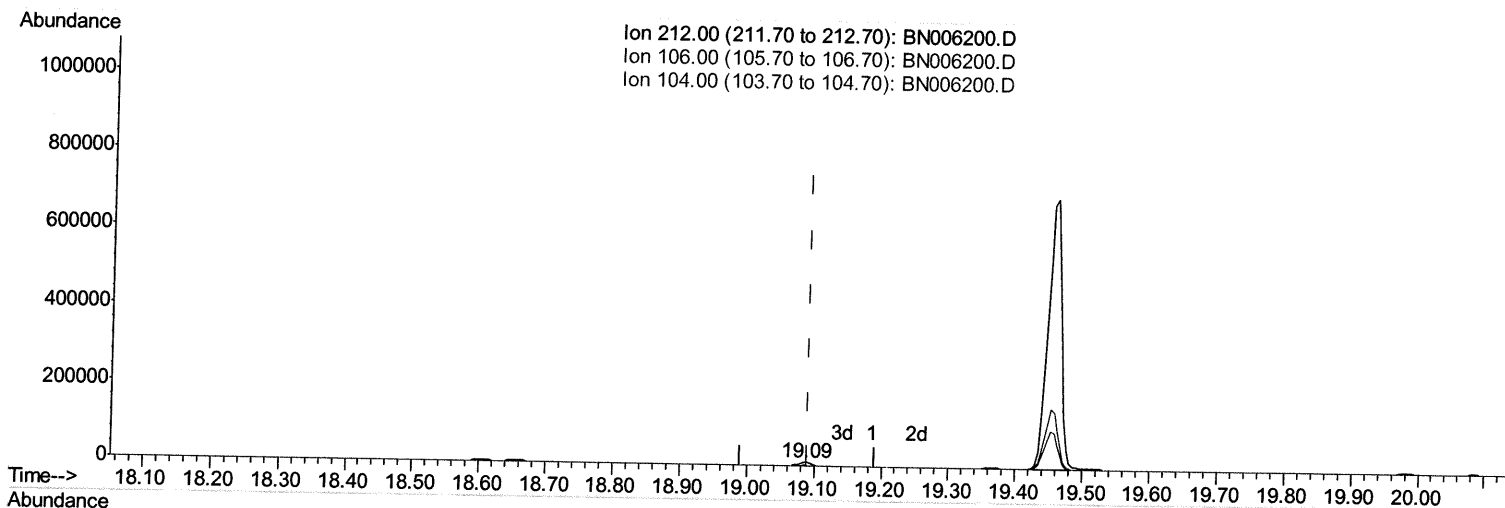

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.29ng/ul m ⁵⁰ 06/10/19

response 13191

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.53#
104.00	9.90	0.79#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

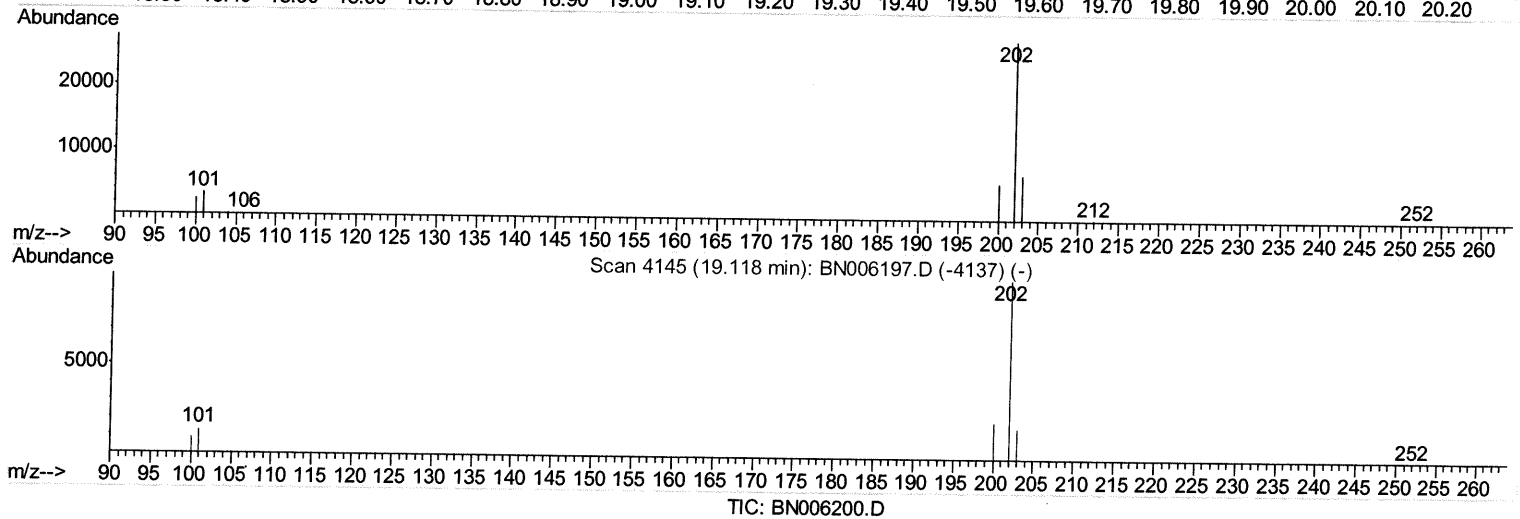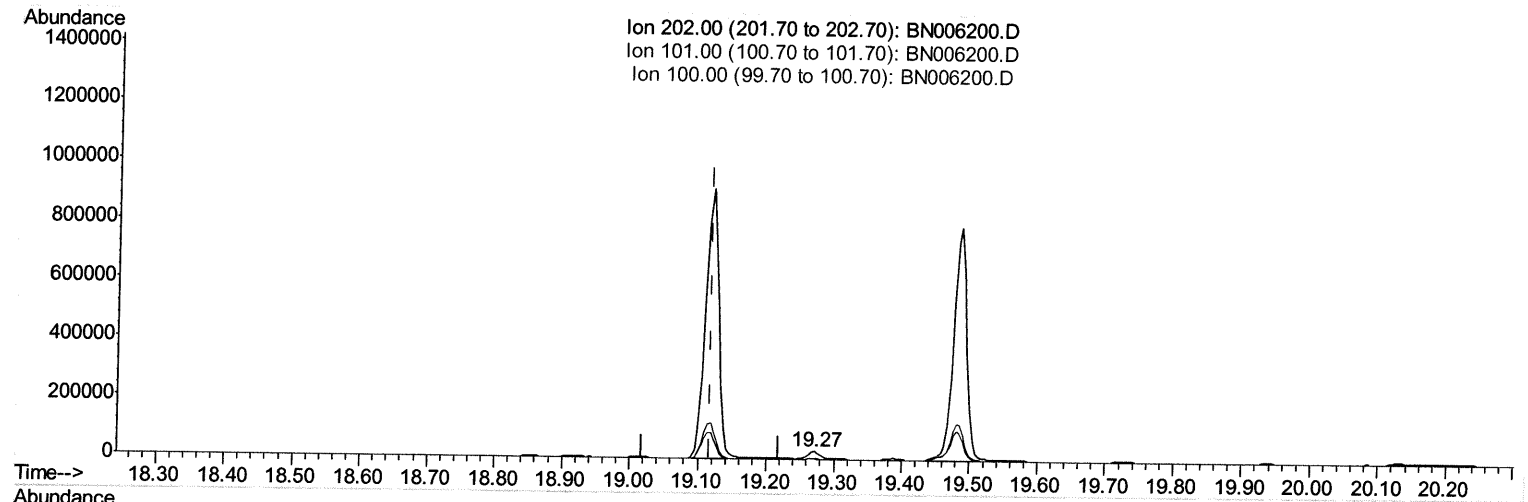

(15) Fluoranthene (C)

19.271min (+0.153) 0.56ng/ul

response 33139

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	12.28
100.00	8.70	8.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

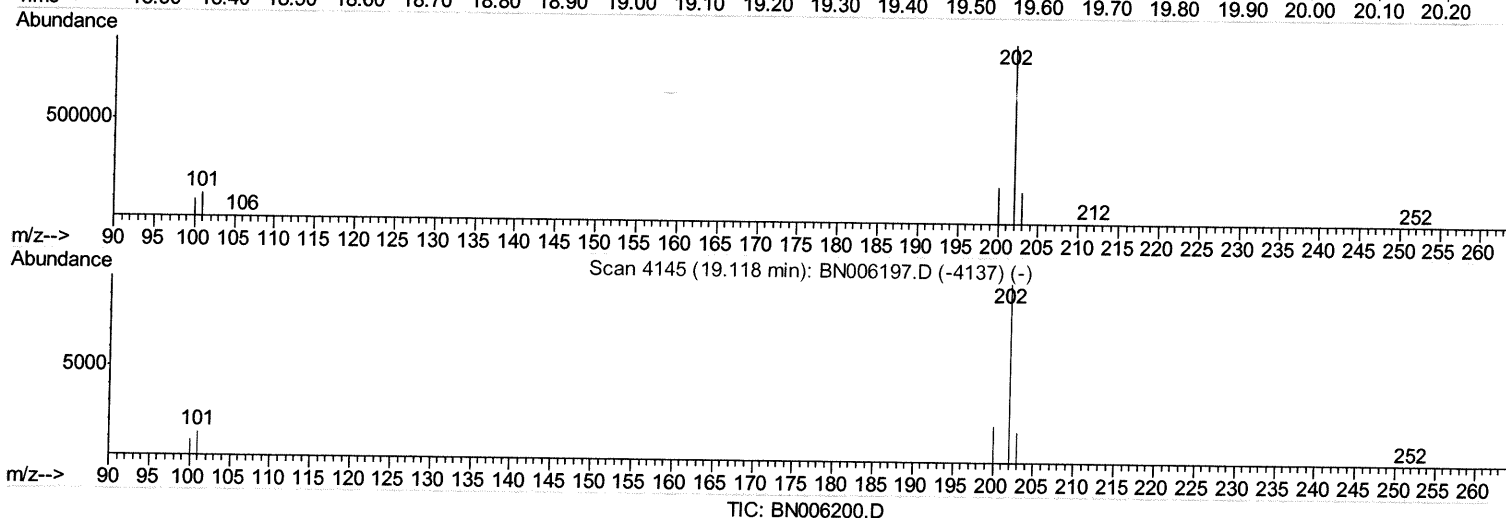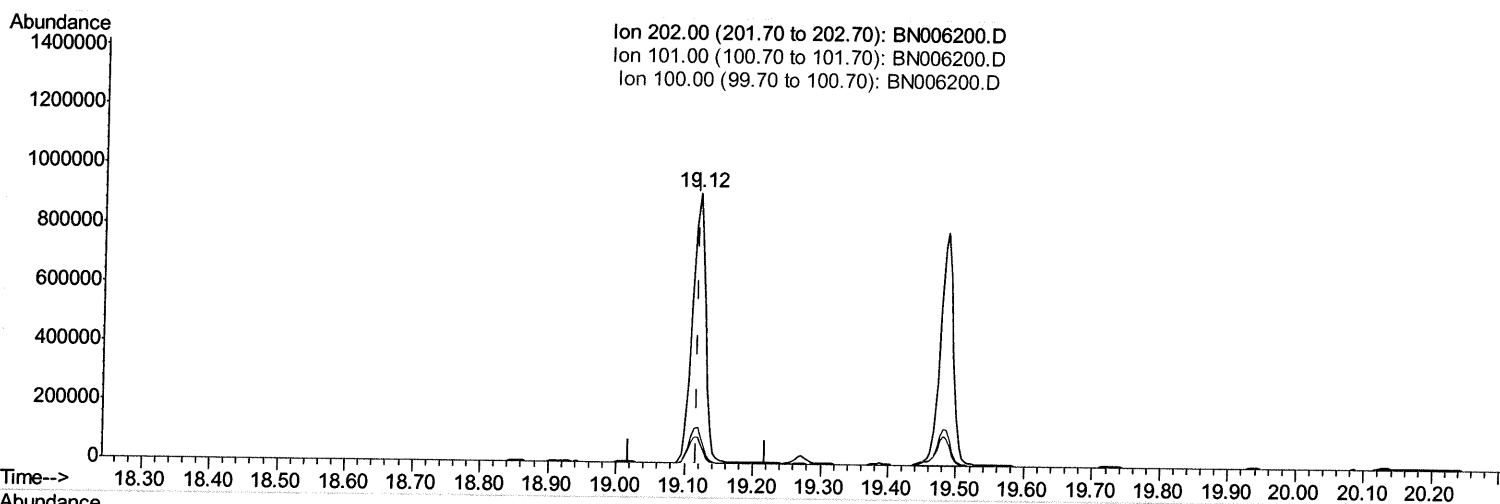

(15) Fluoranthene (C)

19.118min (-0.000) 20.65ng/ul m *JU 06/10/19*

response 1221600

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	13.17
100.00	8.70	9.56
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

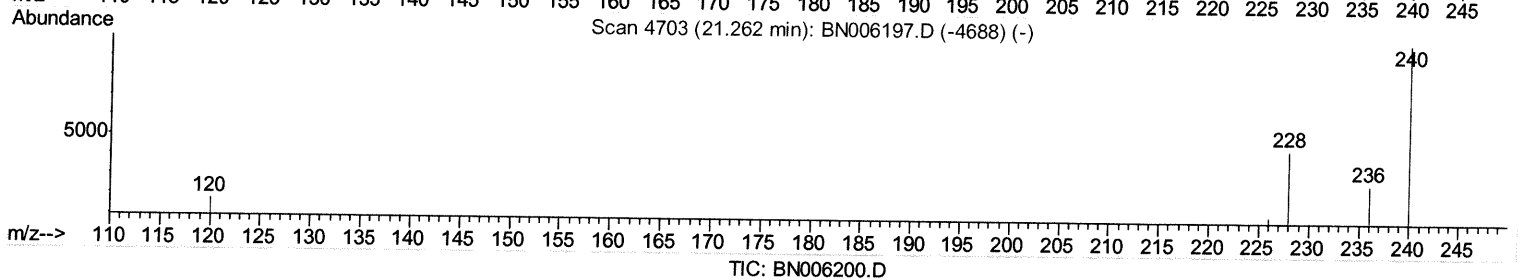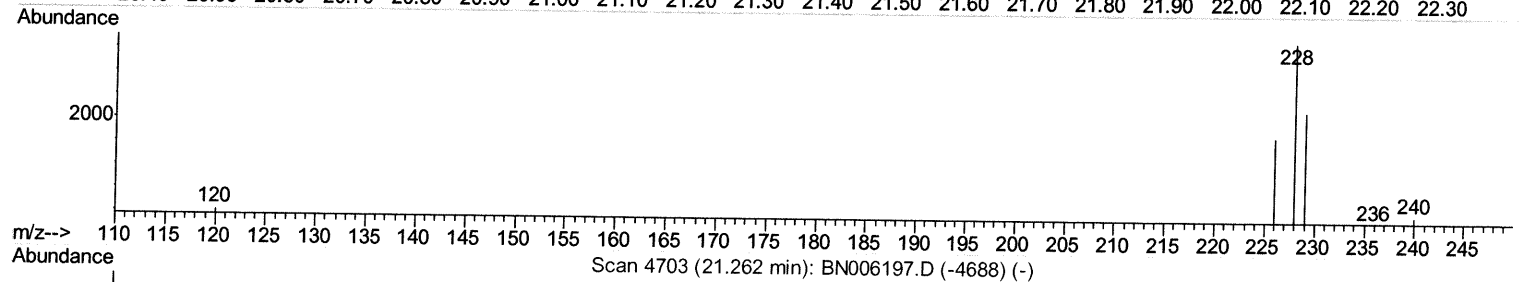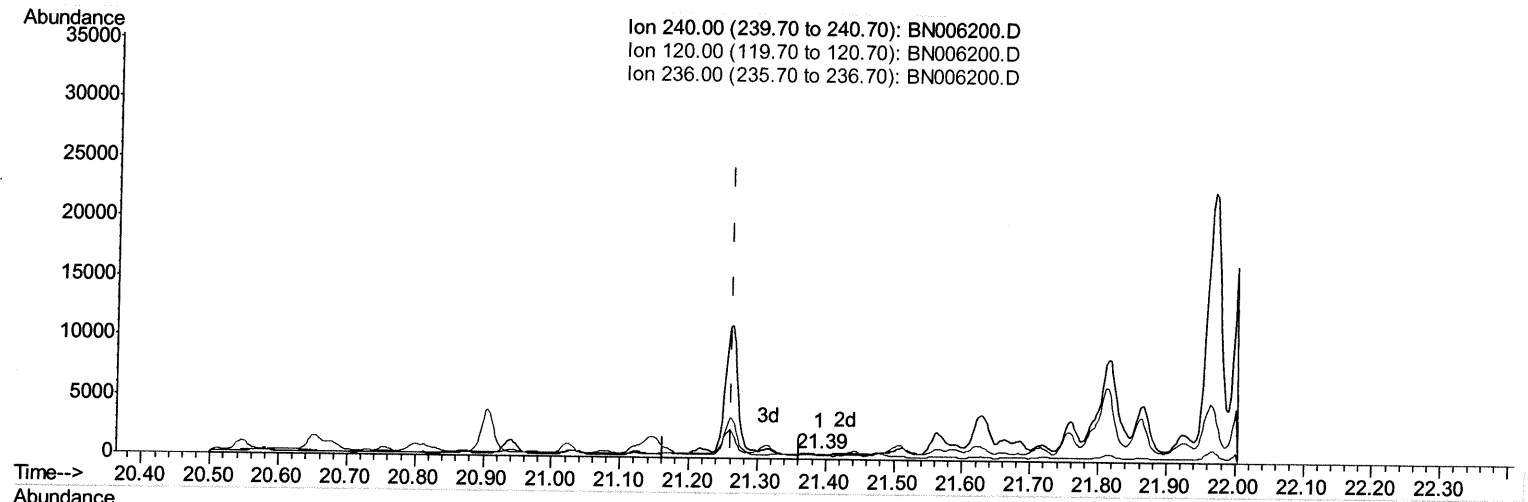

(16) Chrysene-d12 (I)

21.391min (+0.128) 0.40ng/ul

response 218

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	94.85#
236.00	30.10	74.72#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)


Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:26:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

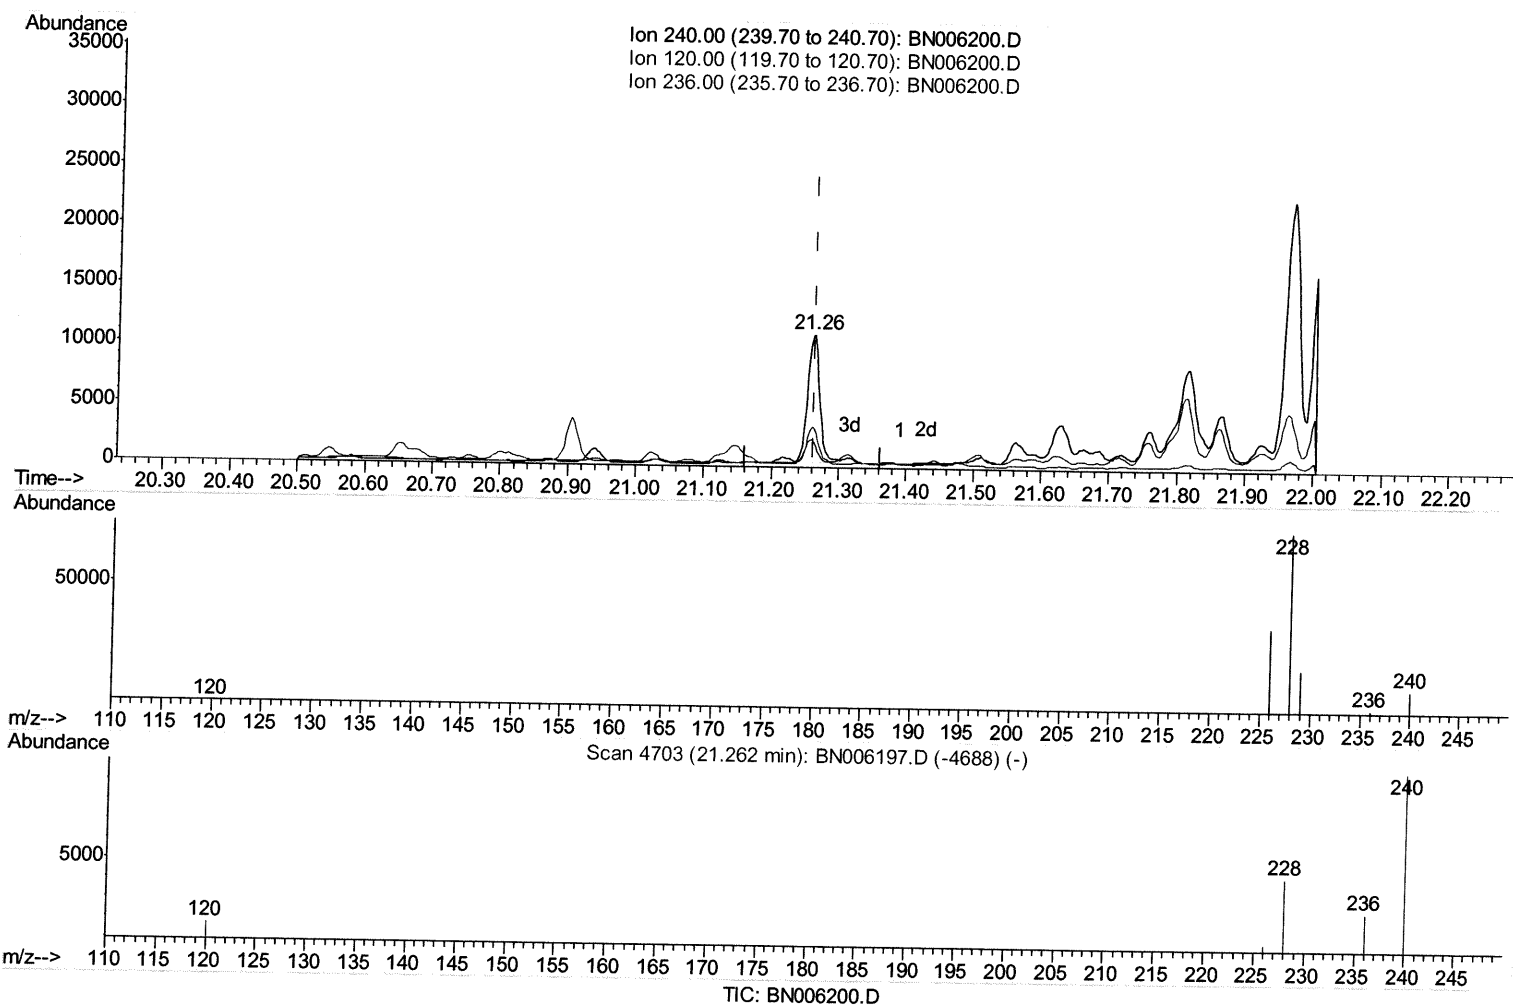

(16) Chrysene-d12 (I)

21.262min (-0.000) 0.40ng/ul m

response 13524

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	19.43
236.00	30.10	30.03
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

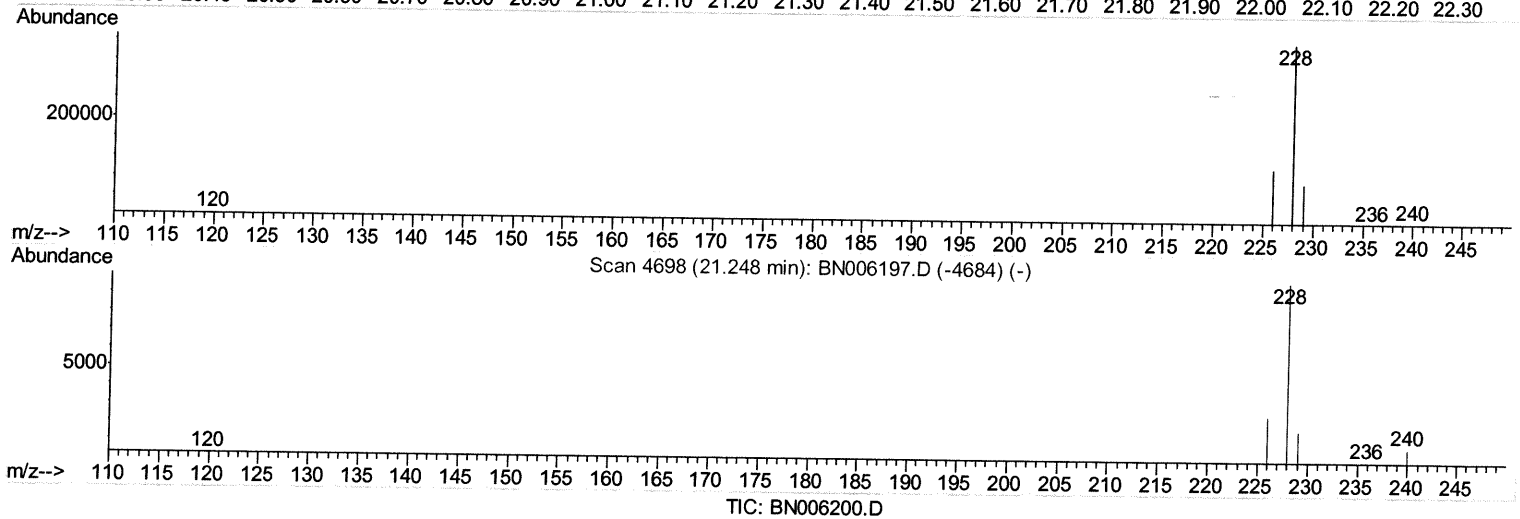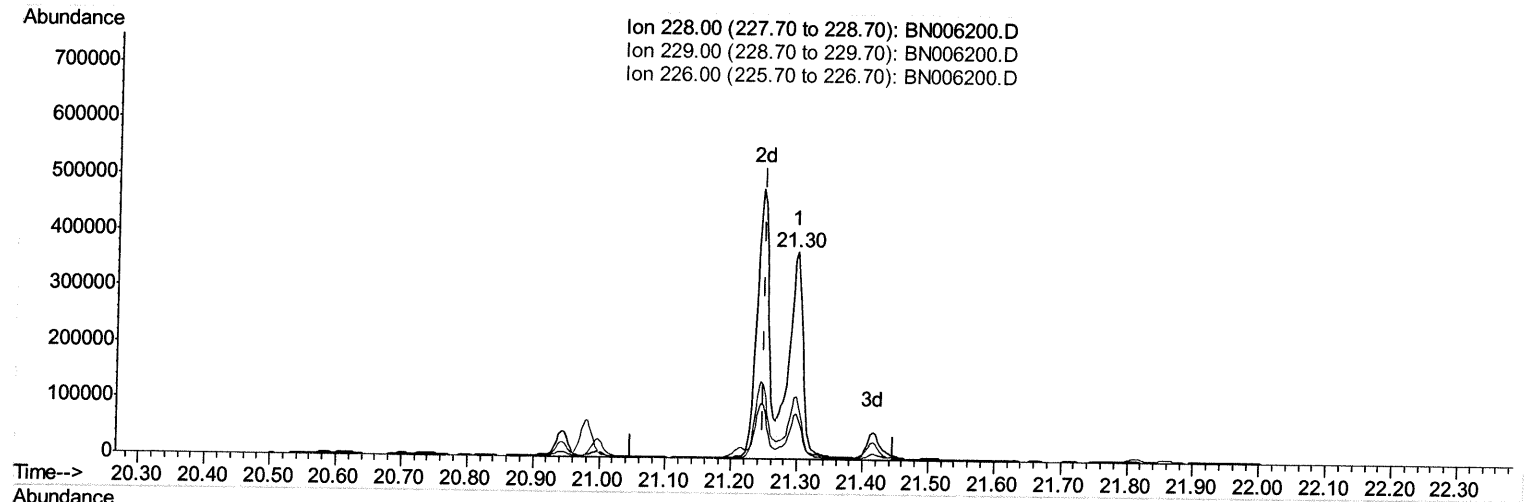

(18) Benzo(a)anthracene

21.297min (+0.050) 9.14ng/ul

response 546679

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	22.02
226.00	28.50	30.53
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)


Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

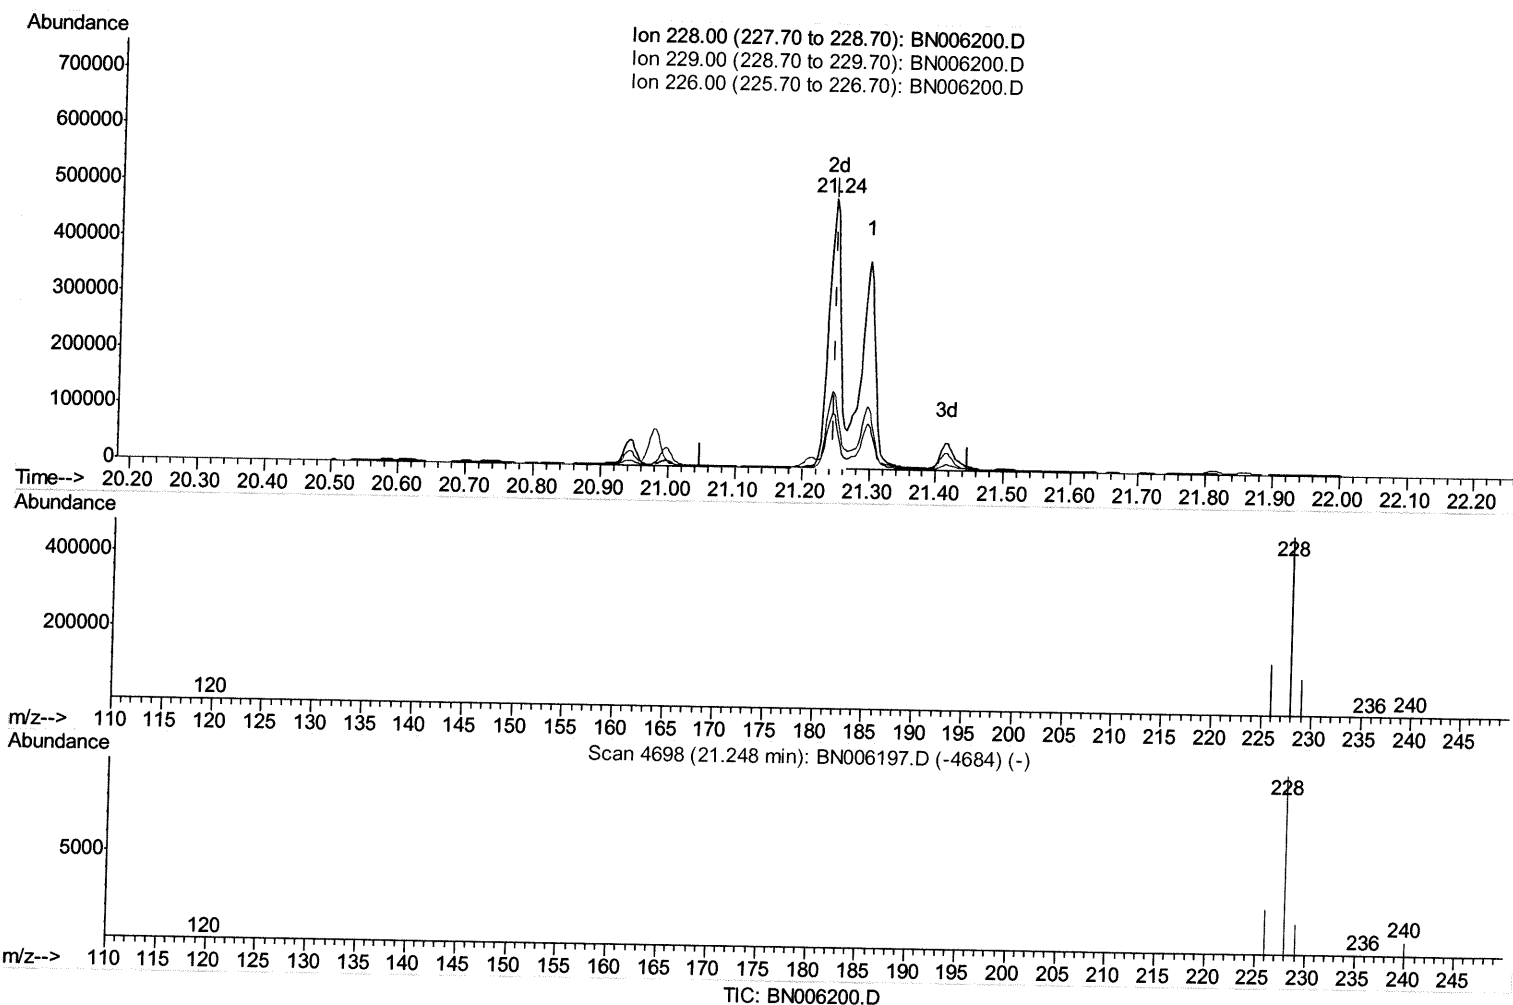

(18) Benzo(a)anthracene

21.245min (-0.003) 10.19ng/ul m *JU 06/10/19*

response 609525

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	20.57
226.00	28.50	28.78
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

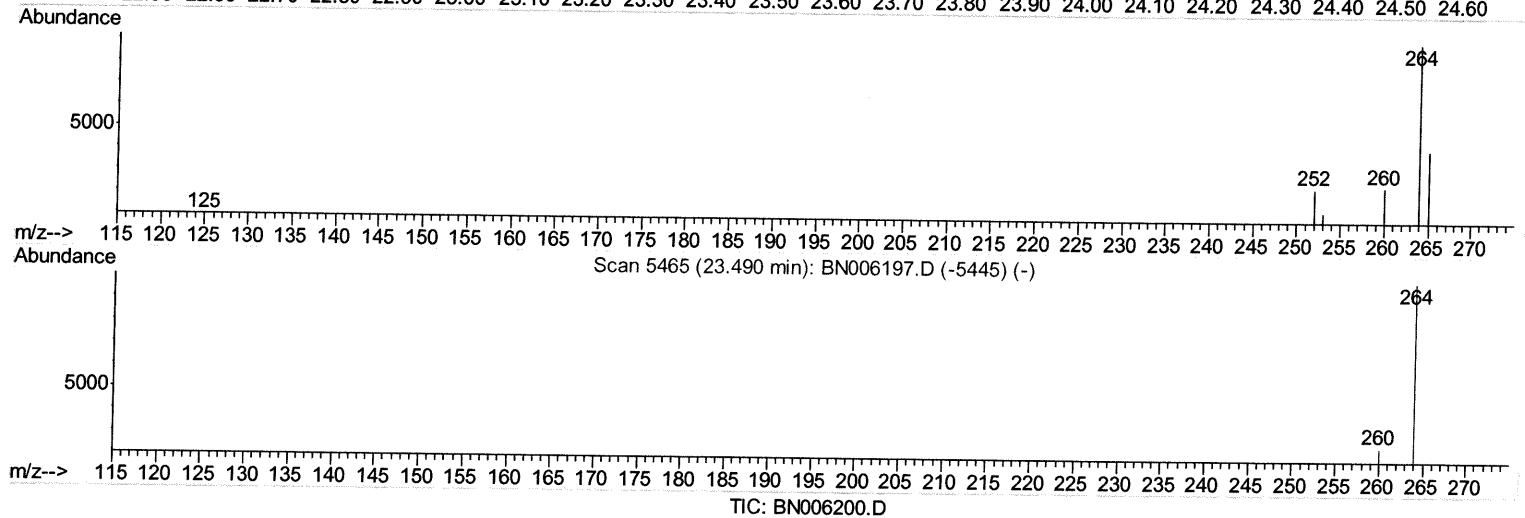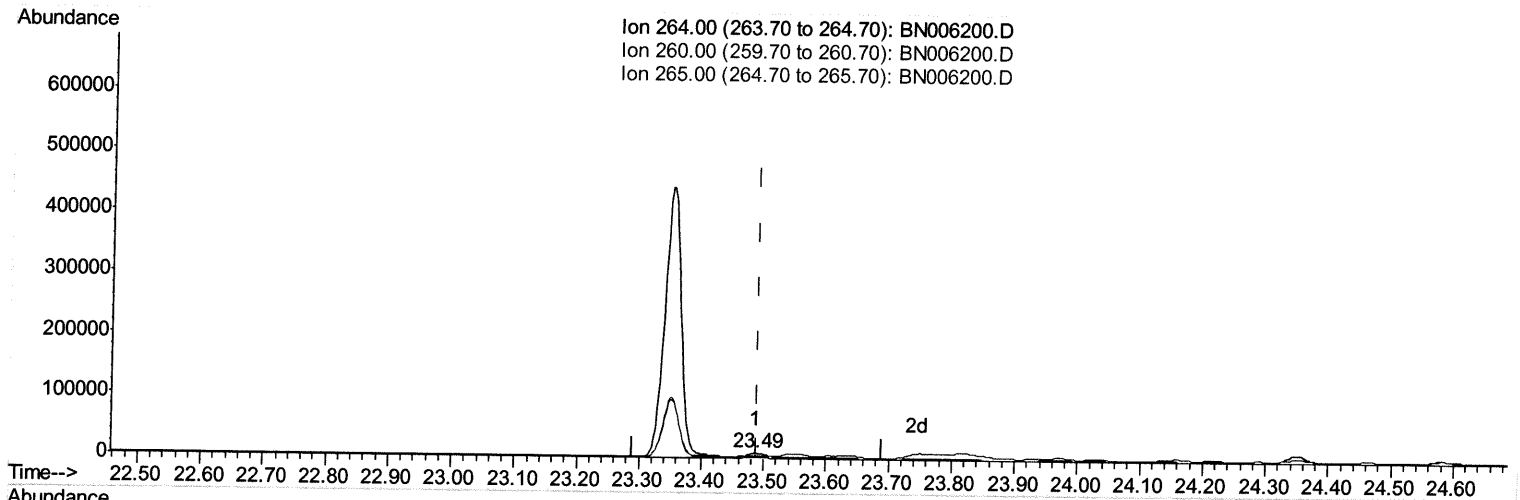

(20) Perylene-d12 (I)

23.487min (-0.003) 0.40ng/ul

response 26680

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.66
265.00	44.70	46.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

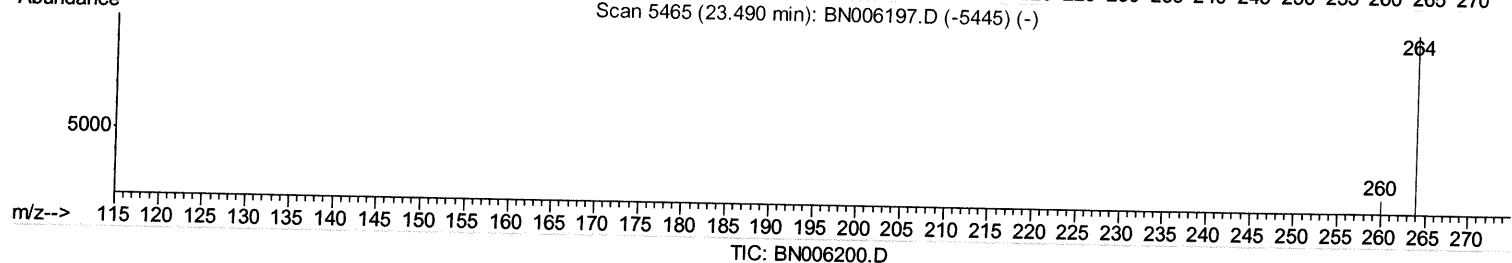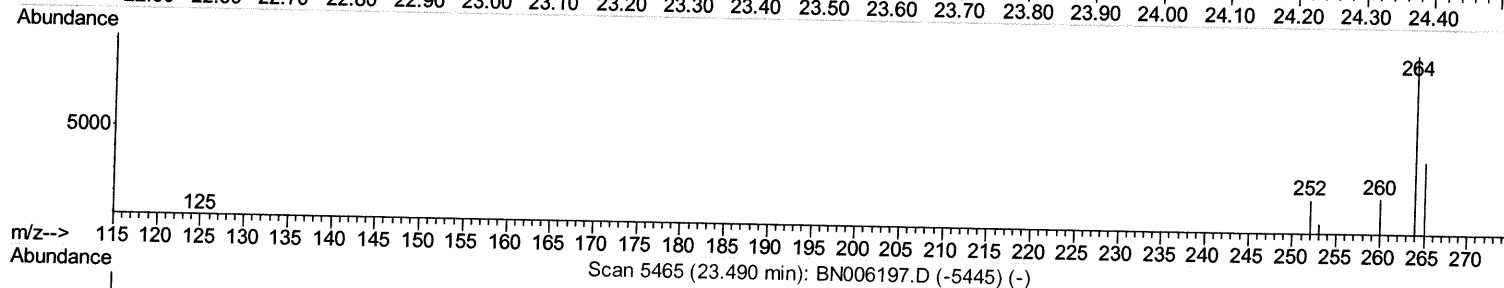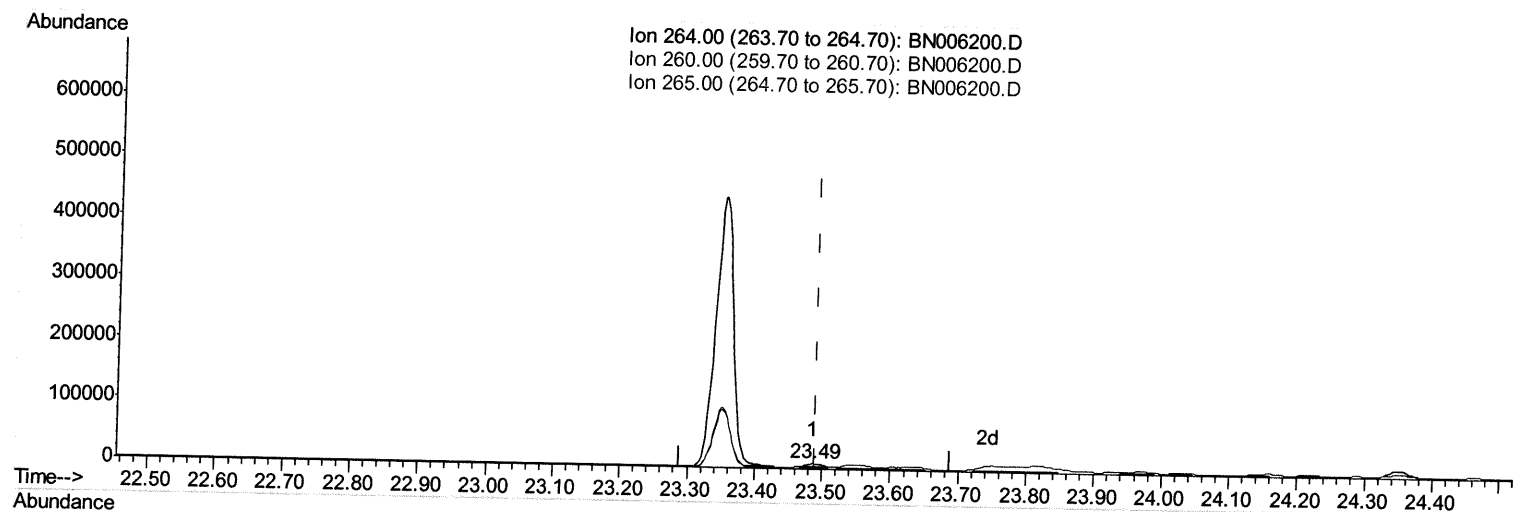

(20) Perylene-d12 (I)

23.487min (-0.003) 0.40ng/ul m 06/10/19

response 12606

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	27.66
265.00	44.70	46.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

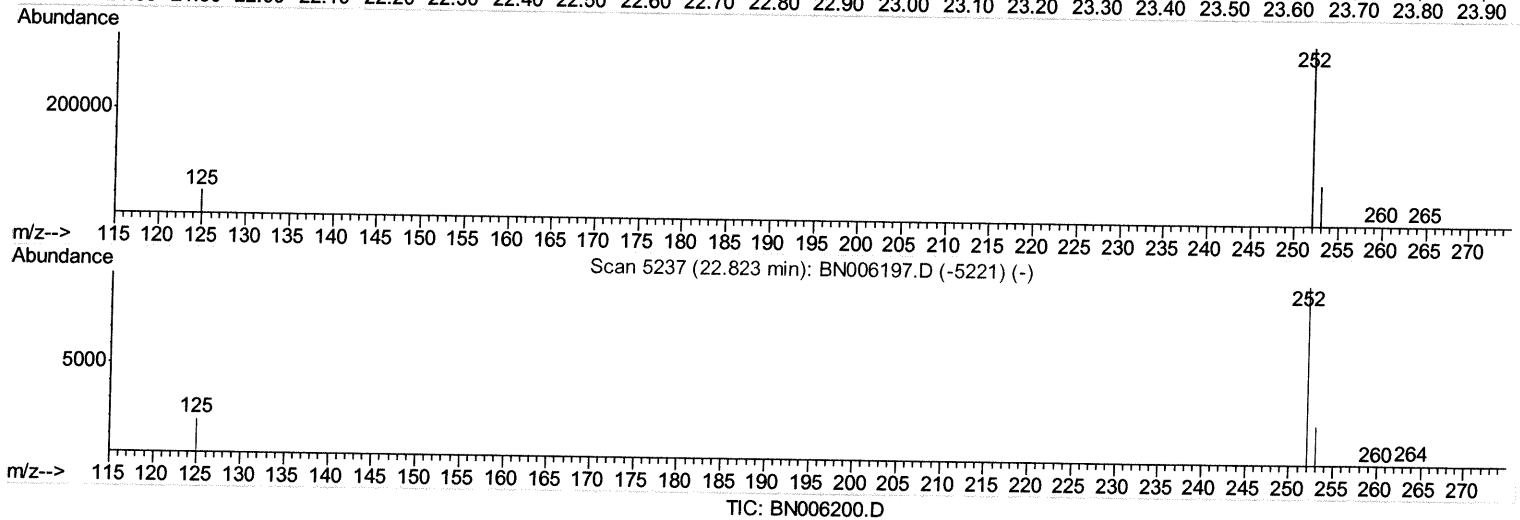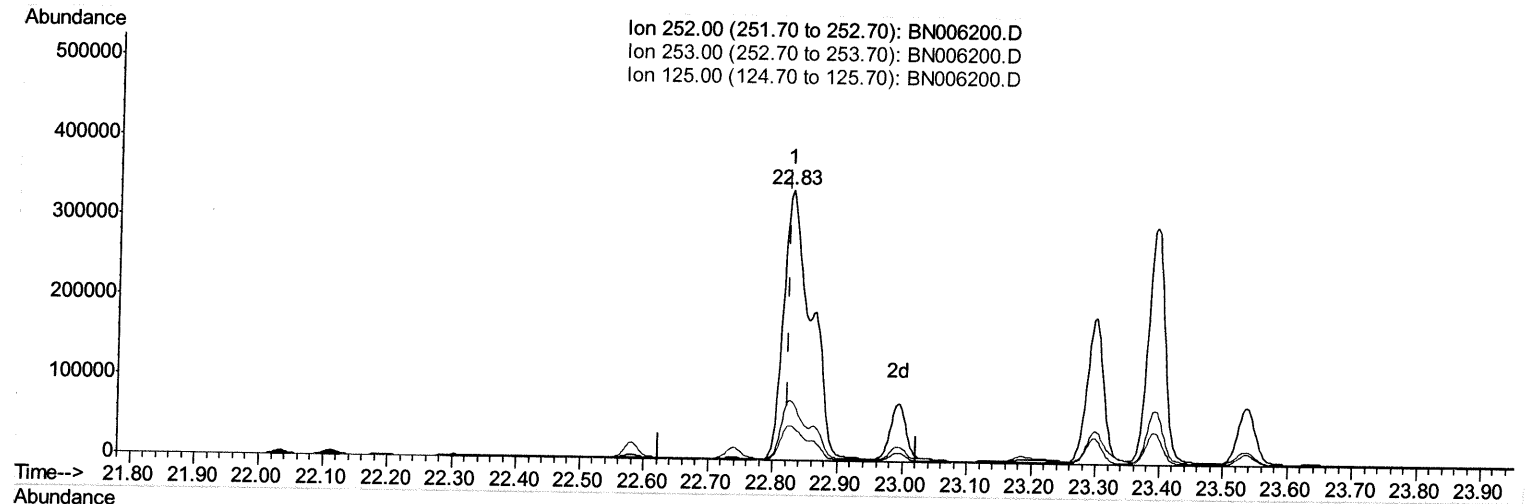

(21) Benzo(b)fluoranthene

22.826min (+0.003) 18.93ng/ul

response 995096

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.44
125.00	20.50	12.95
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

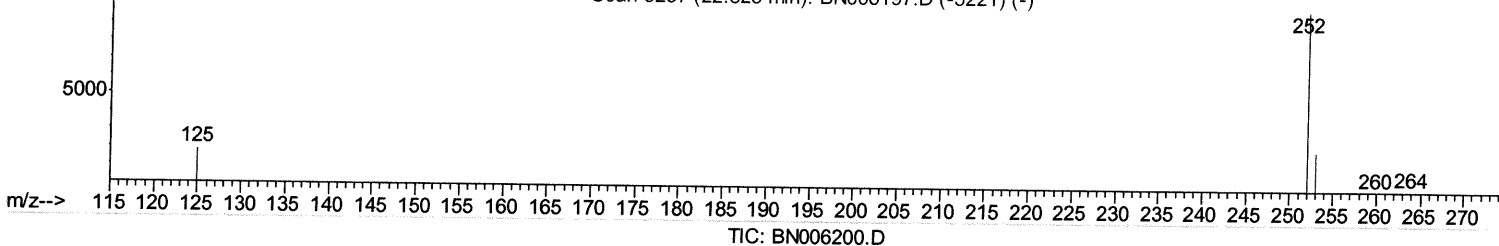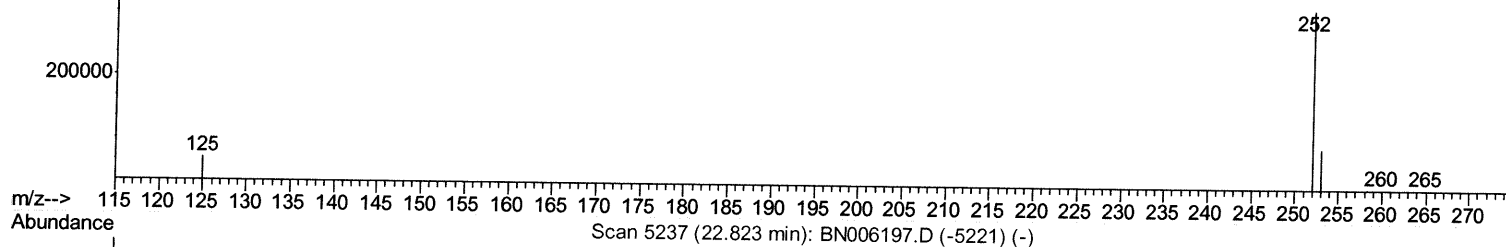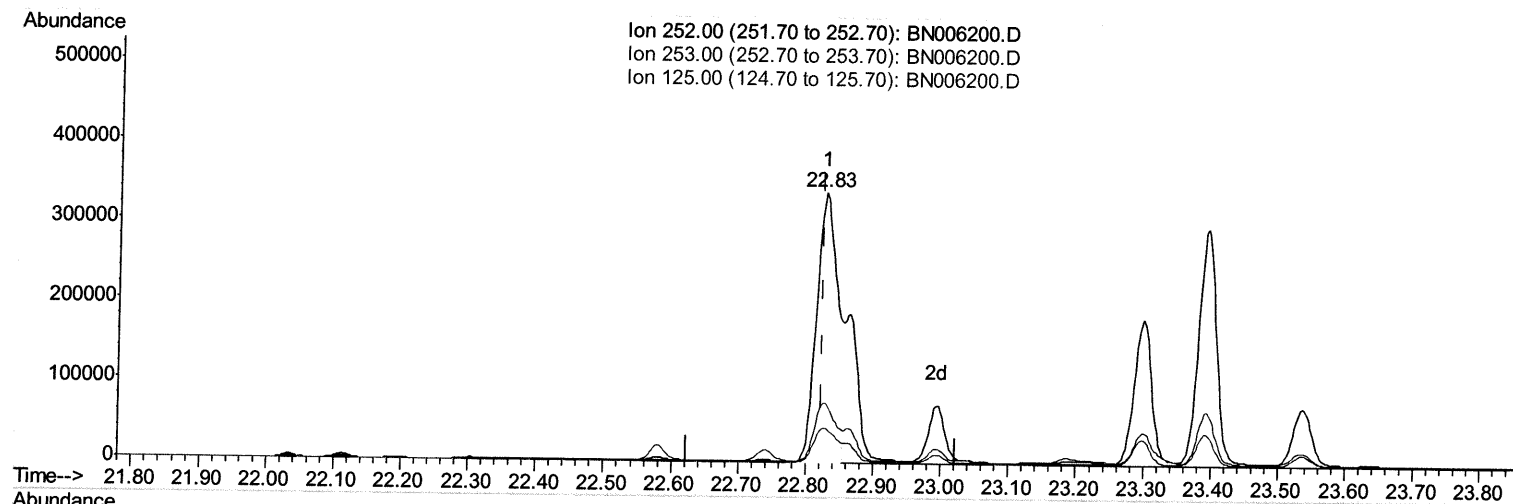

(21) Benzo(b)fluoranthene

22.826min (+0.003) 13.67ng/ul m 06/10/19

response 718693

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	22.44
125.00	20.50	12.95
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

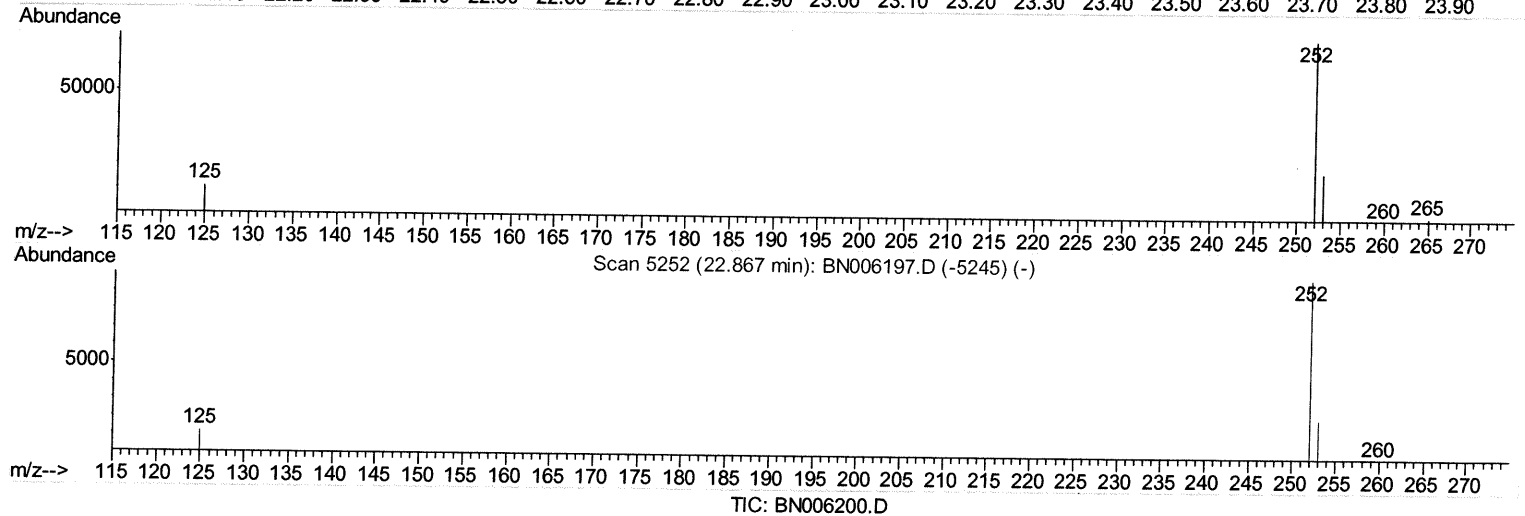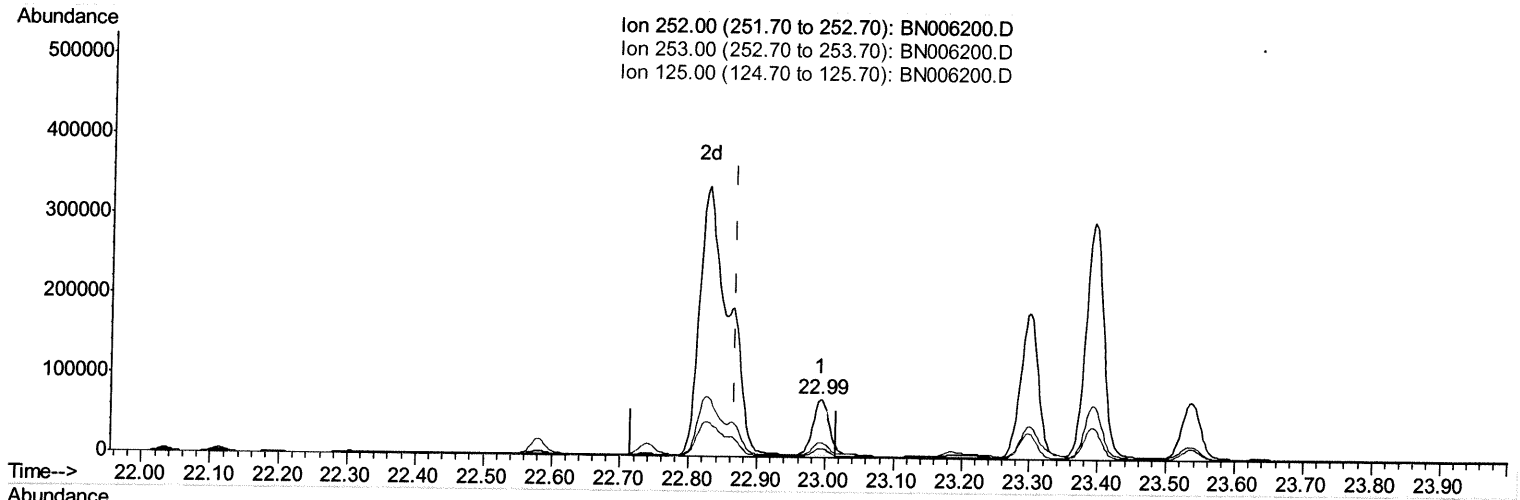

(22) Benzo(k)fluoranthene

22.992min (+0.126) 1.75ng/ul

response 89762

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	26.18
125.00	17.90	15.60
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006200.D
Acq On : 08 Jun 2019 21:23
Operator : JU/SJ
Sample : K3016-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleID :
A51D0

Manual Integrations
APPROVED

mohammad
6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:28:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

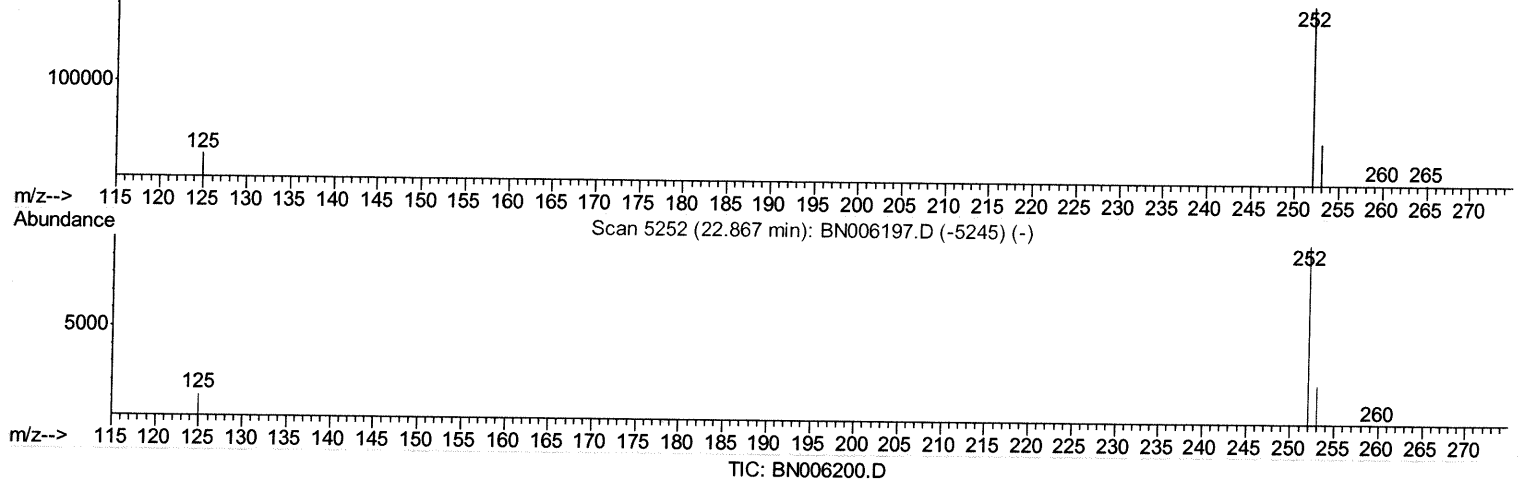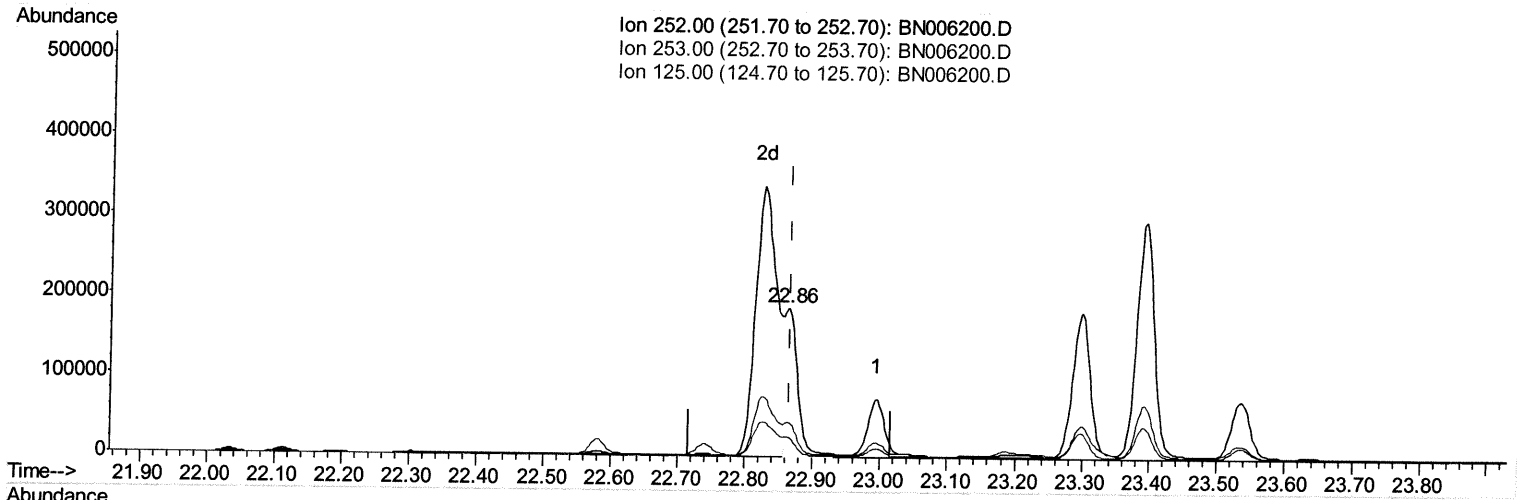

(22) Benzo(k)fluoranthene

22.864min (-0.003) 4.94ng/ul m

JU
06/10/19

response 253011

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.30
125.00	17.90	12.93#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
 Quantitation Report (QT Reviewed)
 Data File : BN006200.D
 Acq On : 08 Jun 2019 21:23
 Operator : JU/SJ
 Sample : K3016-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 A51D0

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:32:37 PM

Quant Time: Jun 09 05:29:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	3840	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14550	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	7857	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	16691m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	13524m>	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	12606m>	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	5007	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	13191m>	0.29	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.47	128	8600	0.214	ng/ul	98
5) 2-Methylnaphthalene	12.10	142	3324	0.119	ng/ul	100
7) Acenaphthylene	14.01	152	59605	1.365	ng/ul	100
8) Acenaphthene	14.36	153	12780	0.422	ng/ul	99
9) Fluorene	15.35	166	25400	0.717	ng/ul	97
12) Phenanthrene	17.09	178	455387m>	8.499	ng/ul	
13) Anthracene	17.18	178	160502m>	3.137	ng/ul	
15) Fluoranthene	19.12	202	1221600m>	20.648	ng/ul	
17) Pyrene	19.49	202	1077299	15.123	ng/ul	100
18) Benzo(a)anthracene	21.24	228	609525m>	10.190	ng/ul	
19) Chrysene	21.30	228	539548	9.609	ng/ul	98
21) Benzo(b)fluoranthene	22.83	252	718693m>	13.673	ng/ul	
22) Benzo(k)fluoranthene	22.86	252	253011m>	4.942	ng/ul	
23) Benzo(a)pyrene	23.39	252	536531	10.960	ng/ul#	85
24) Indeno(1,2,3-cd)pyrene	25.72	276	345859	6.527	ng/ul#	89
25) Dibenzo(a,h)anthracene	25.72	278	87169	2.058	ng/ul	94
26) Benzo(g,h,i)perylene	26.40	276	269294	6.068	ng/ul	94

Ju 06/10/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed