

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (QT Reviewed)


Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:54:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

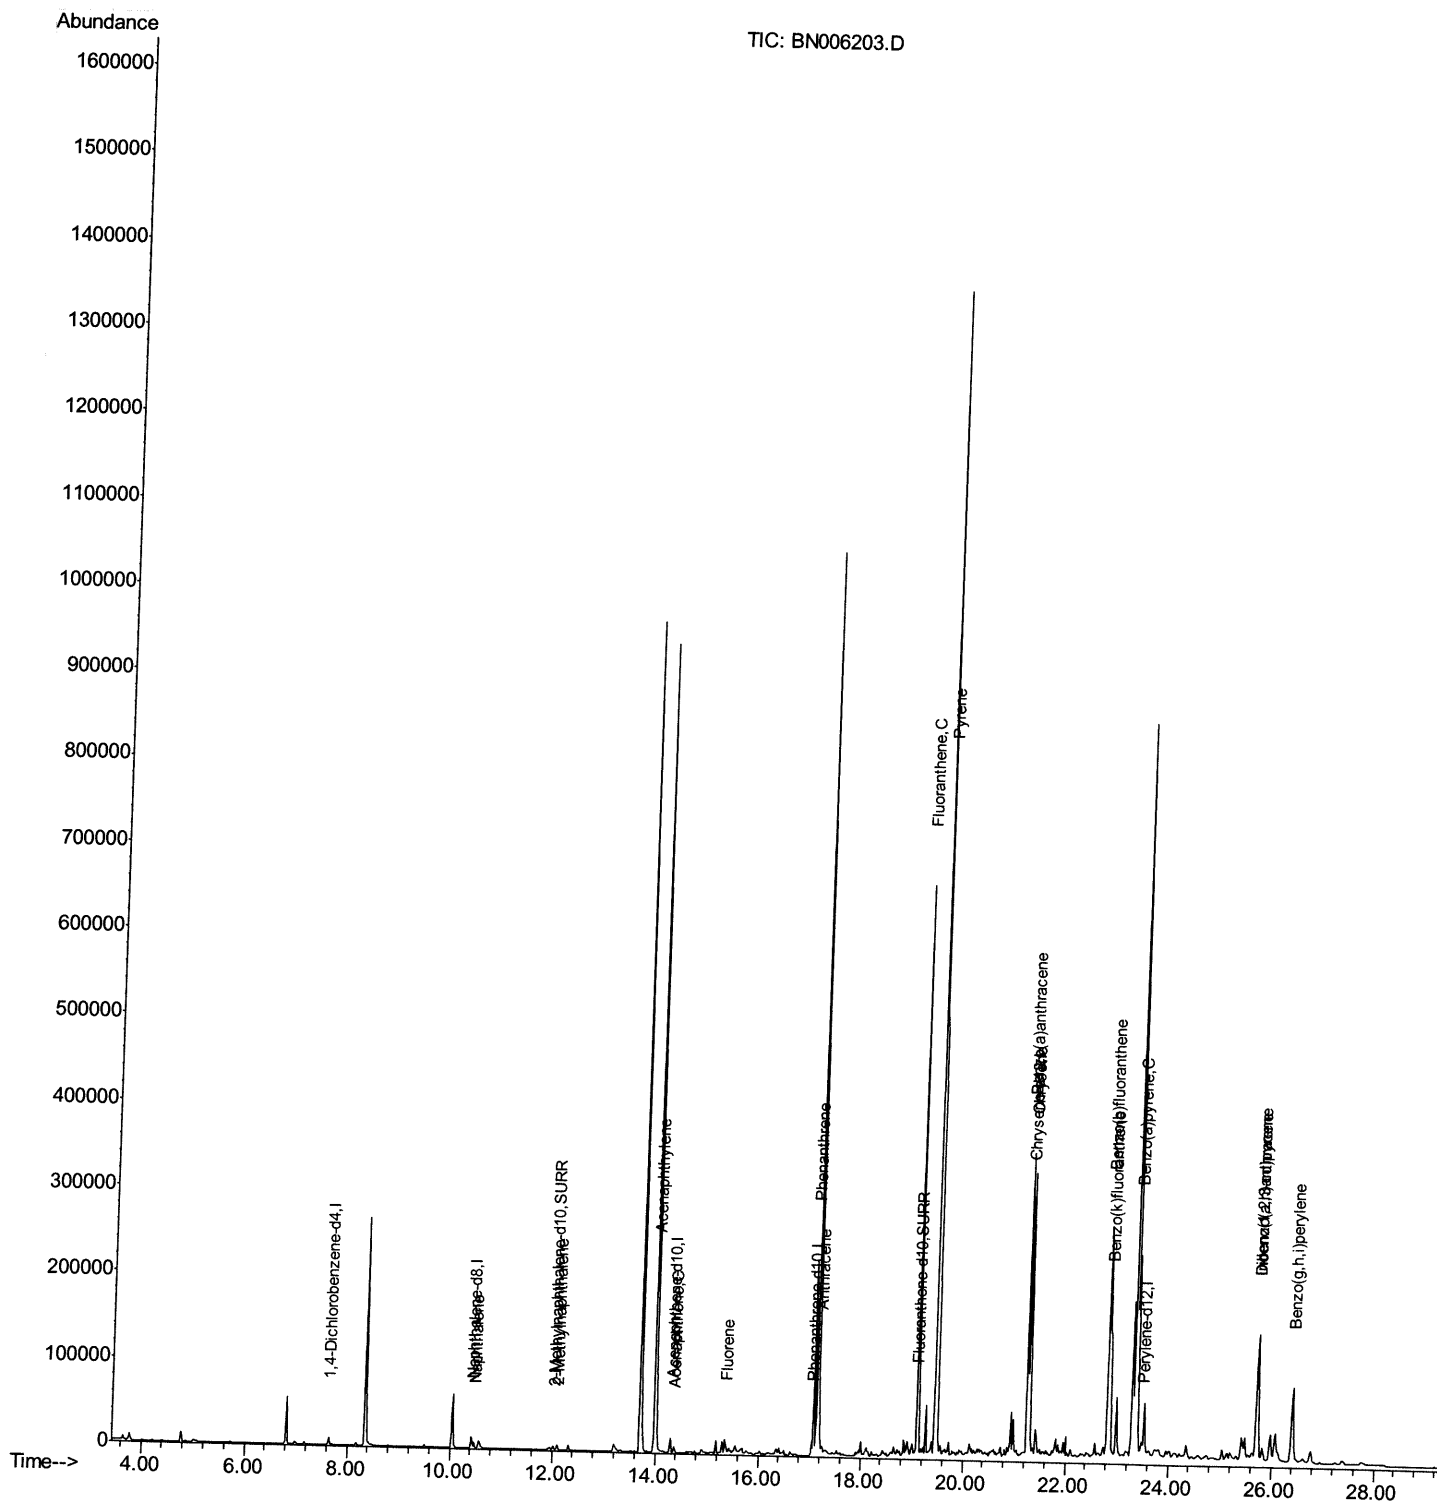

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

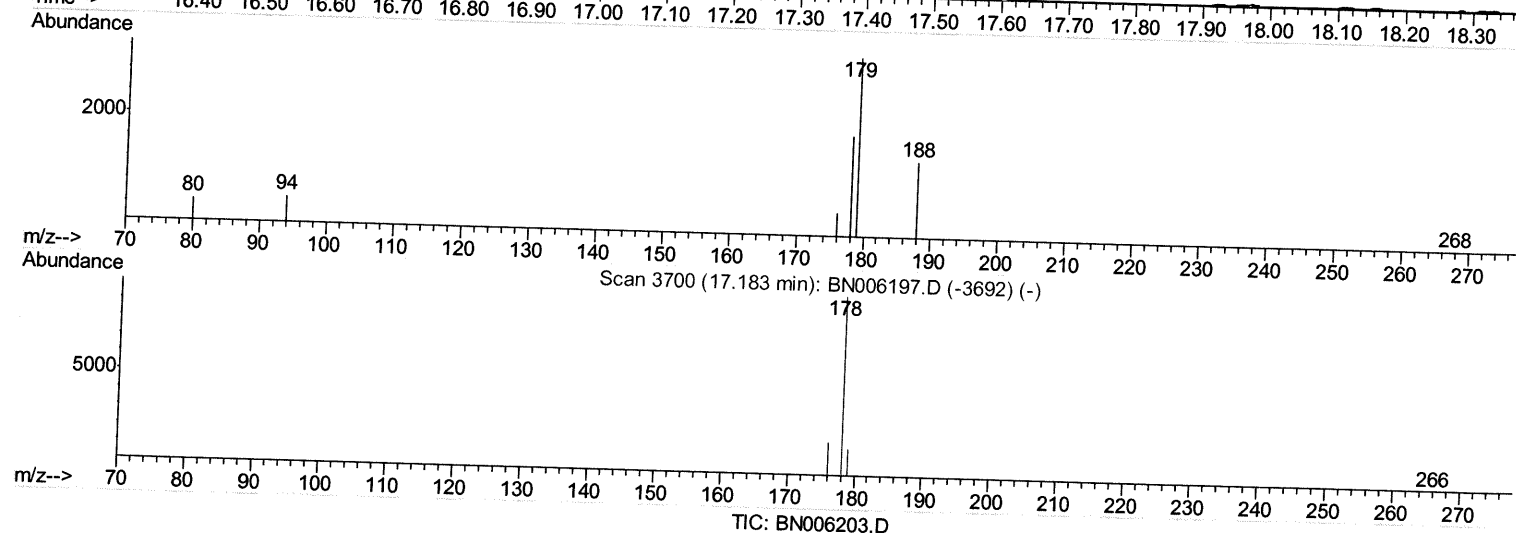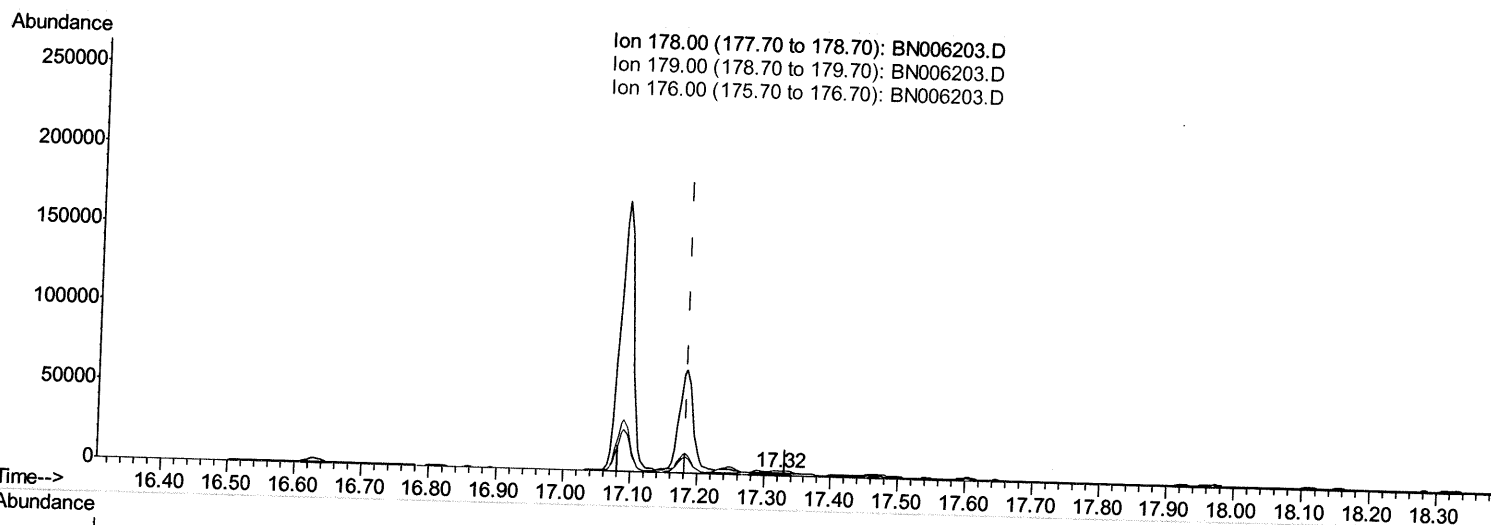

(13) Anthracene

17.323min (+0.139) 0.04ng/ul

response 2843

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	175.94#
176.00	18.90	26.15#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

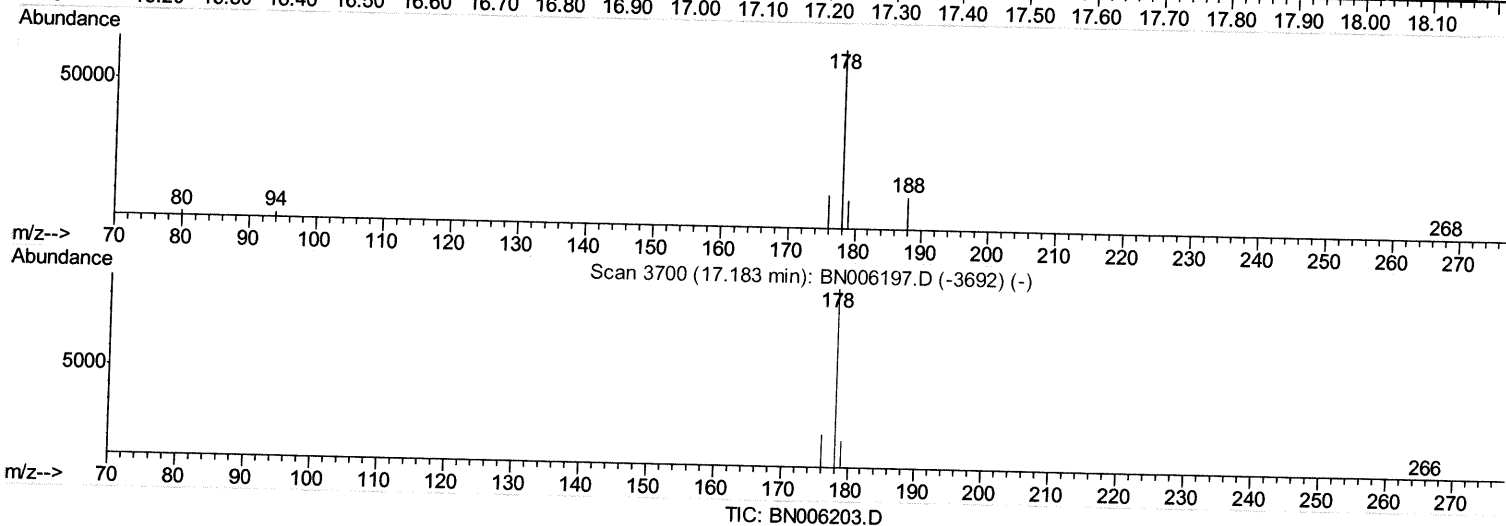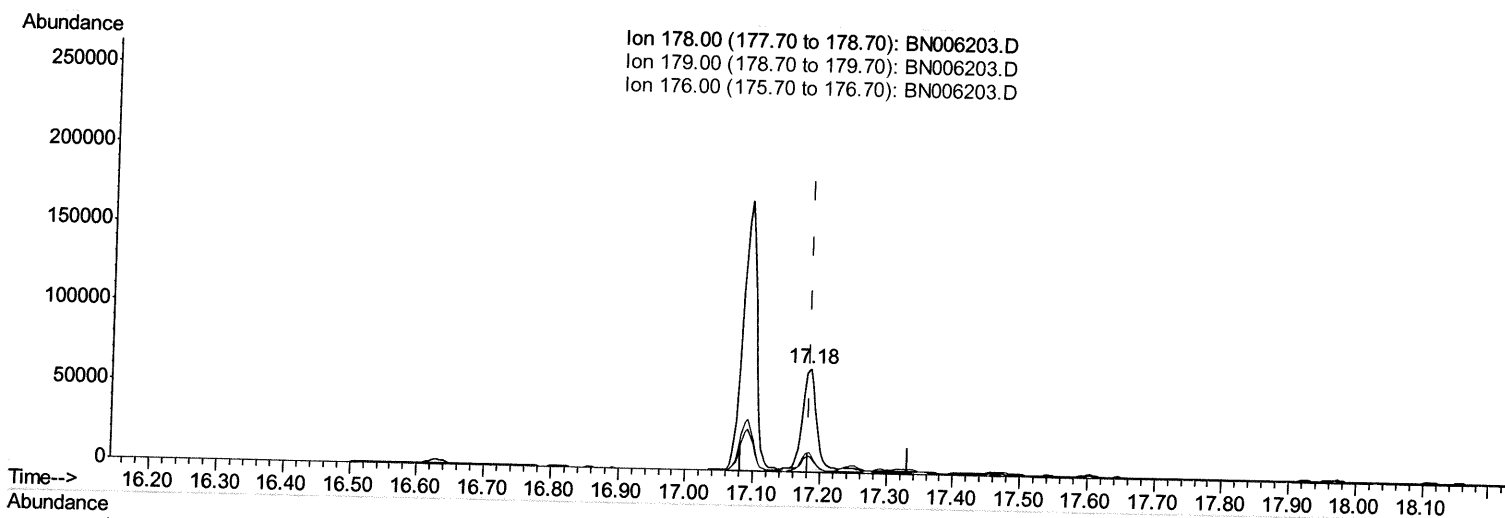

(13) Anthracene

17.183min (0.000) 1.42ng/ul m ^{JU} 06/10/19

response 89711

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	15.58
176.00	18.90	18.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)

Data File : BN006203.D

Acq On : 08 Jun 2019 23:06

Operator : JU/SJ

Sample : K3016-04

Misc :

ALS Vial : 21 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM



Quant Time: Jun 09 05:45:14 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Jun 09 05:10:30 2019

Response via : Initial Calibration

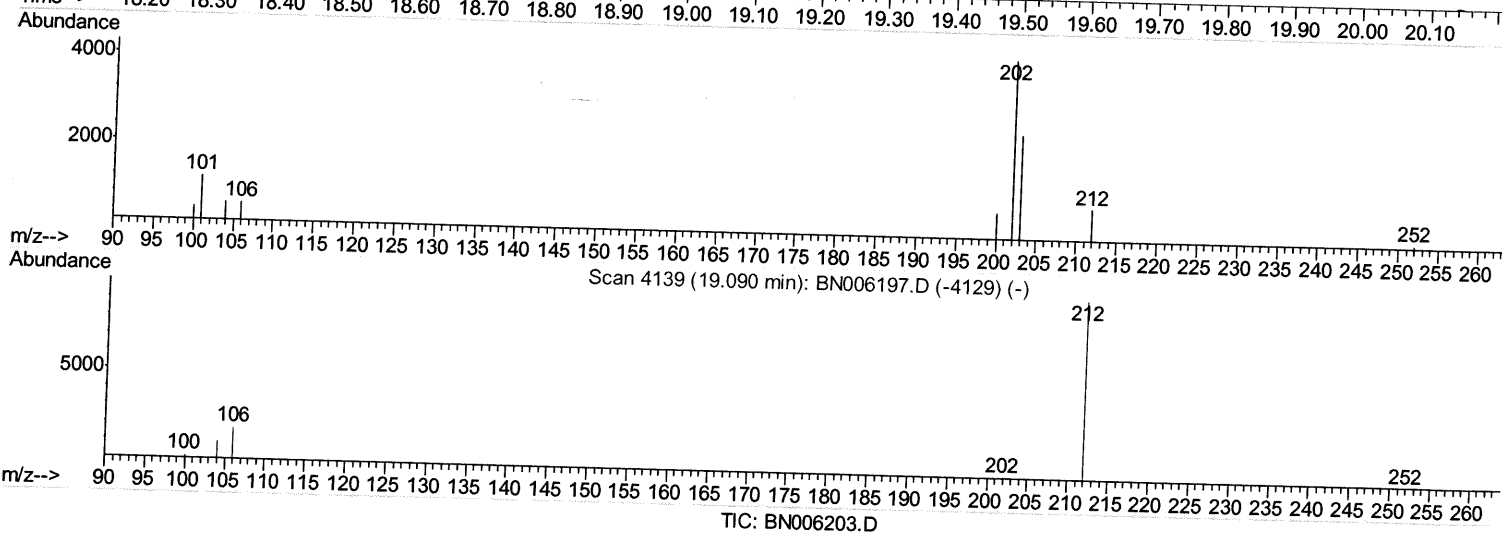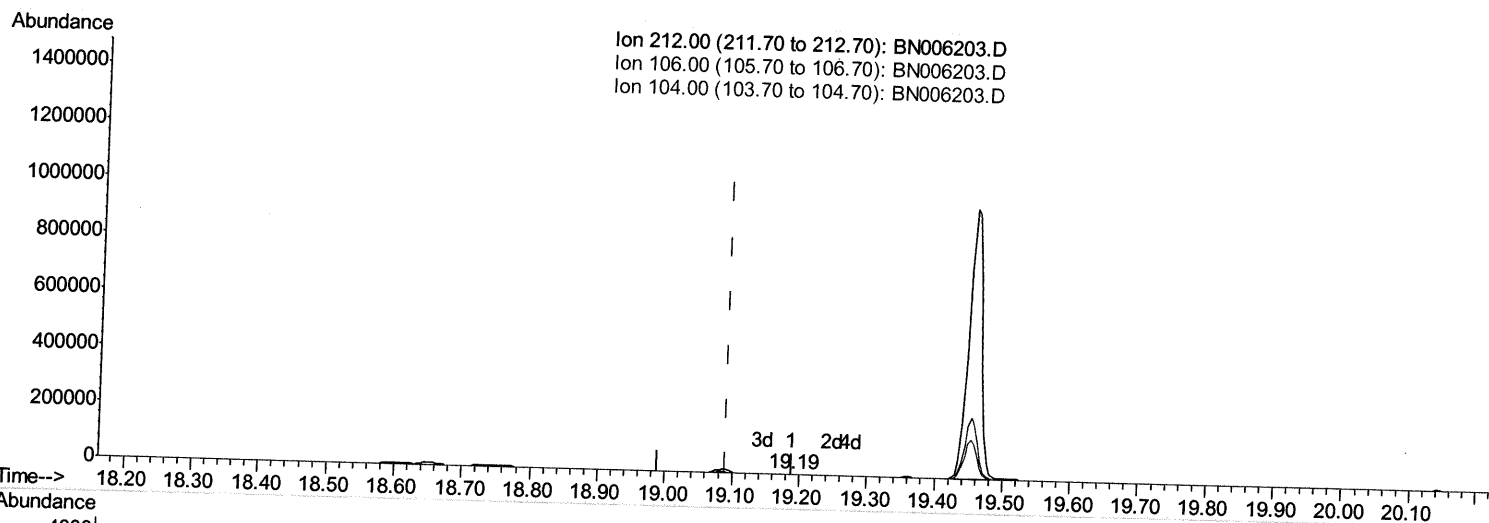

(14) Fluoranthene-d10 (SURR)

19.188min (+0.098) 0.02ng/ul

response 1102

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	14.97
104.00	9.90	46.28#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

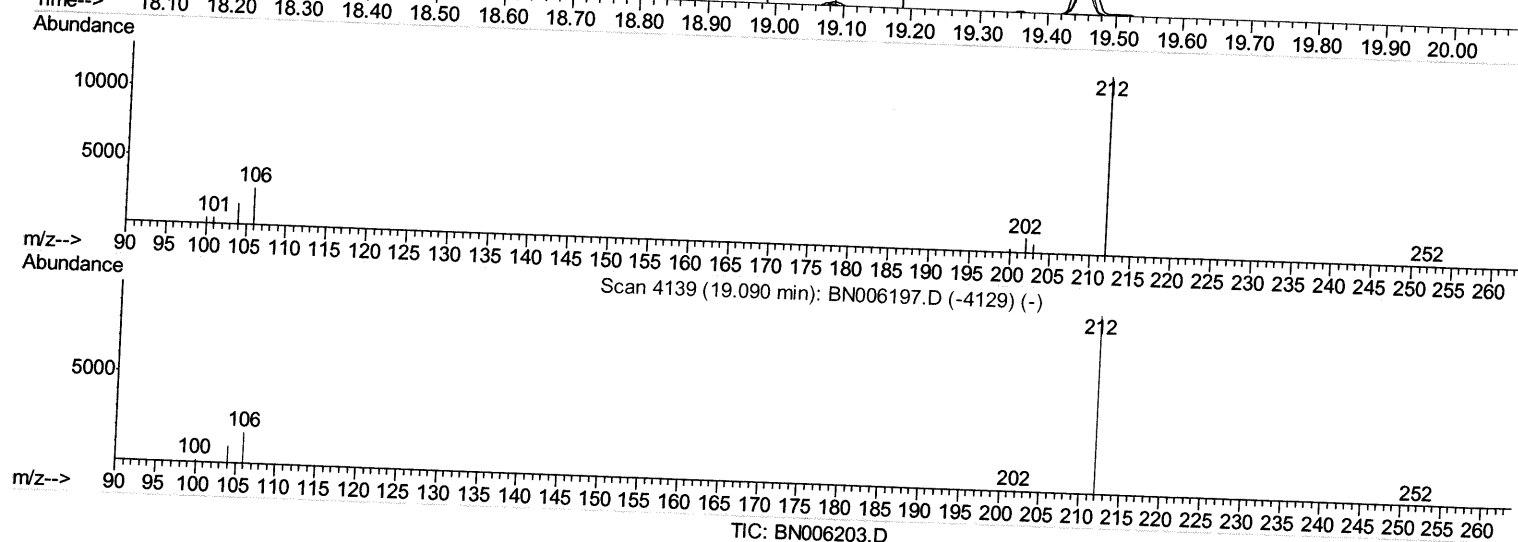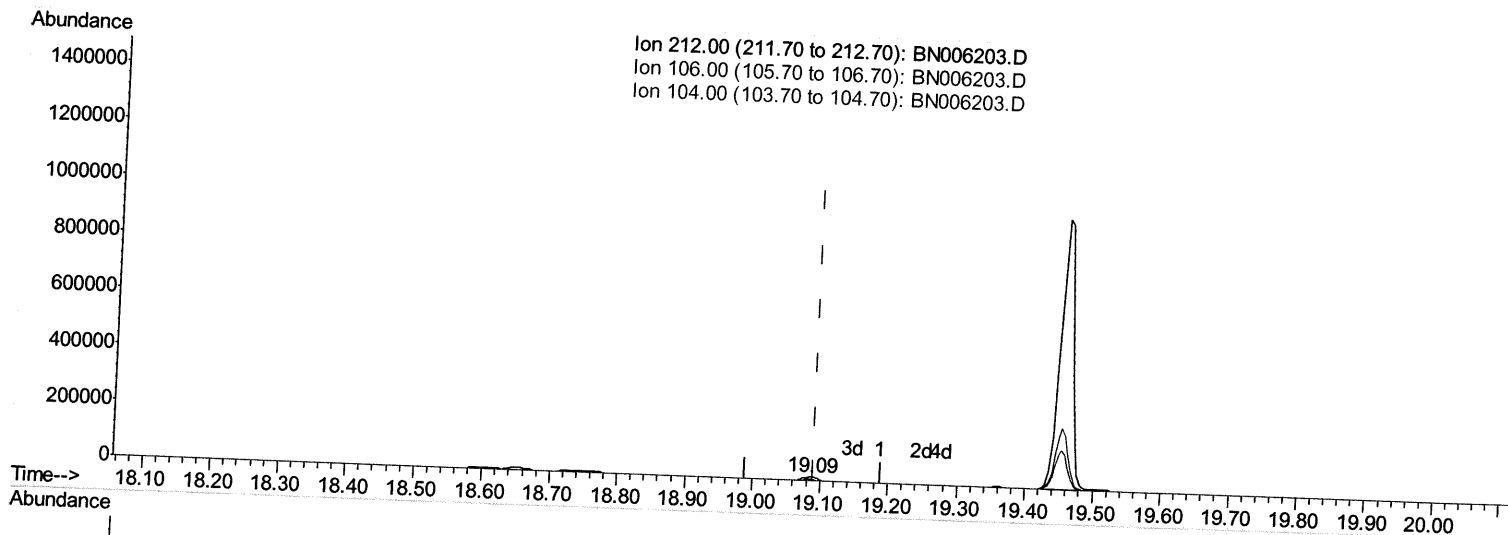

(14) Fluoranthene-d10 (SURR)

19.086min (-0.005) 0.33ng/ul m ^{JU} 06/10/19

response 18316

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.90#
104.00	9.90	2.78#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

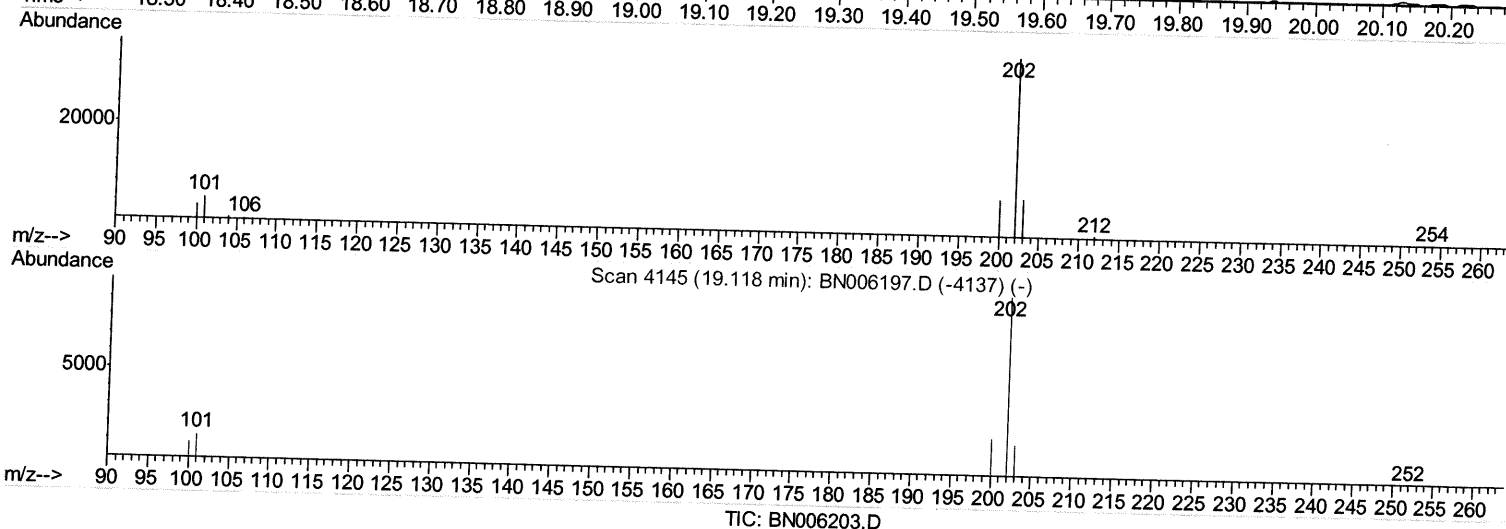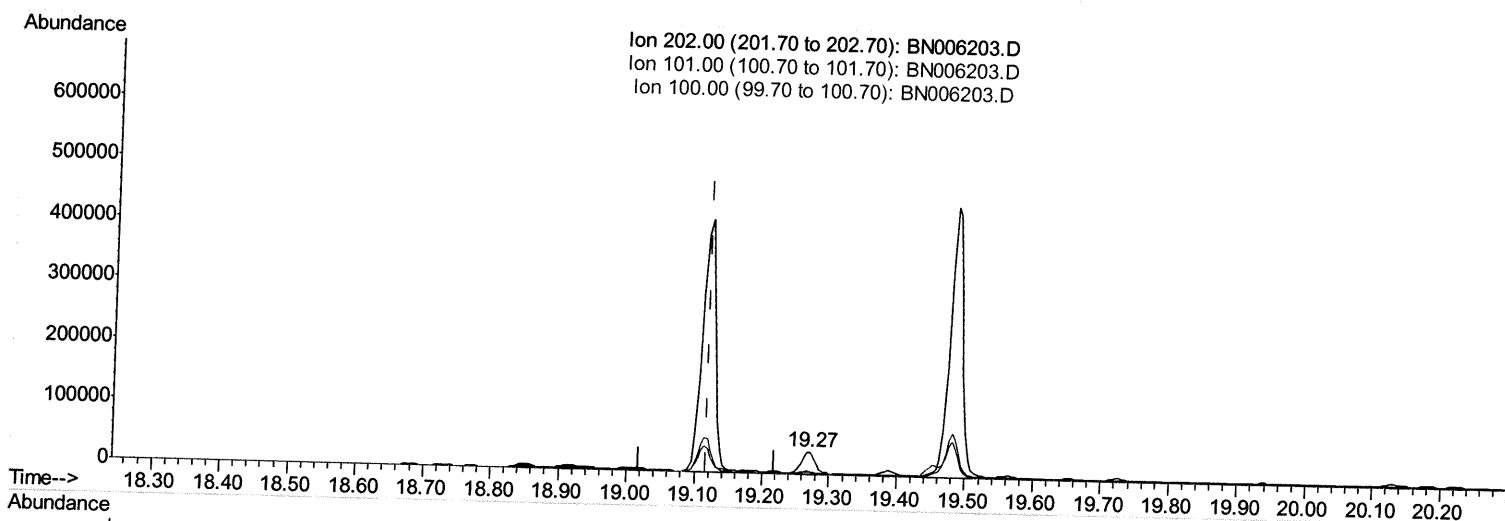

(15) Fluoranthene (C)

19.271min (+0.153) 0.65ng/ul

response 47347

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	12.87
100.00	8.70	9.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

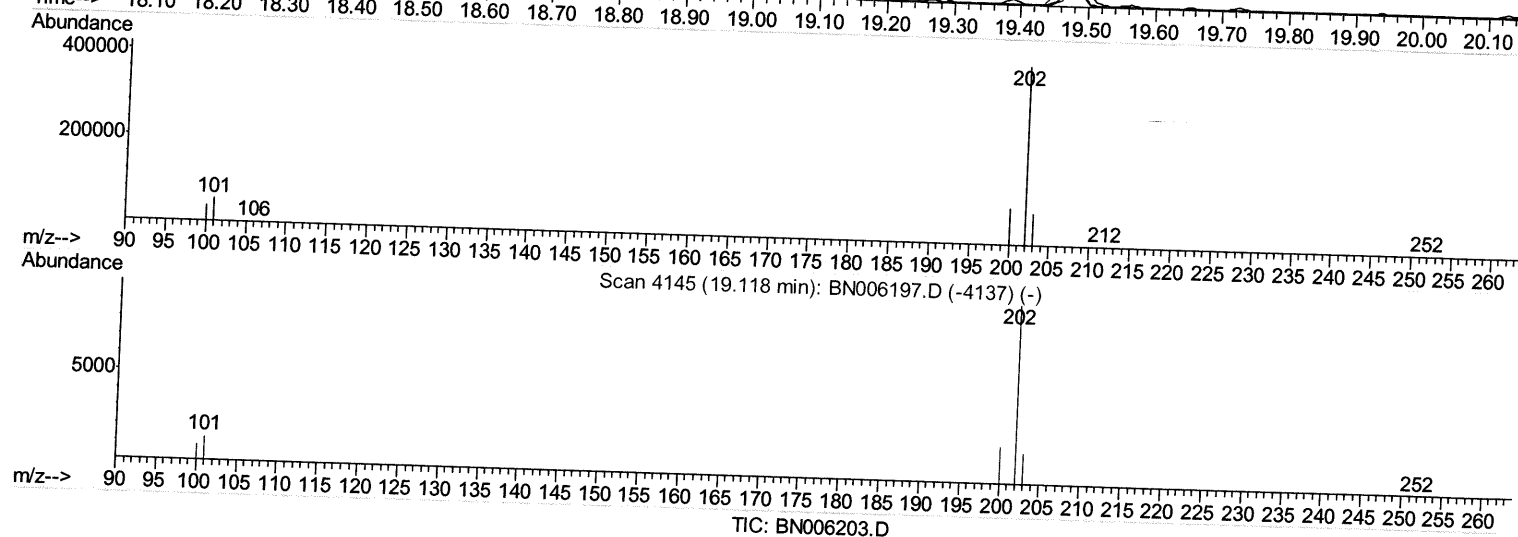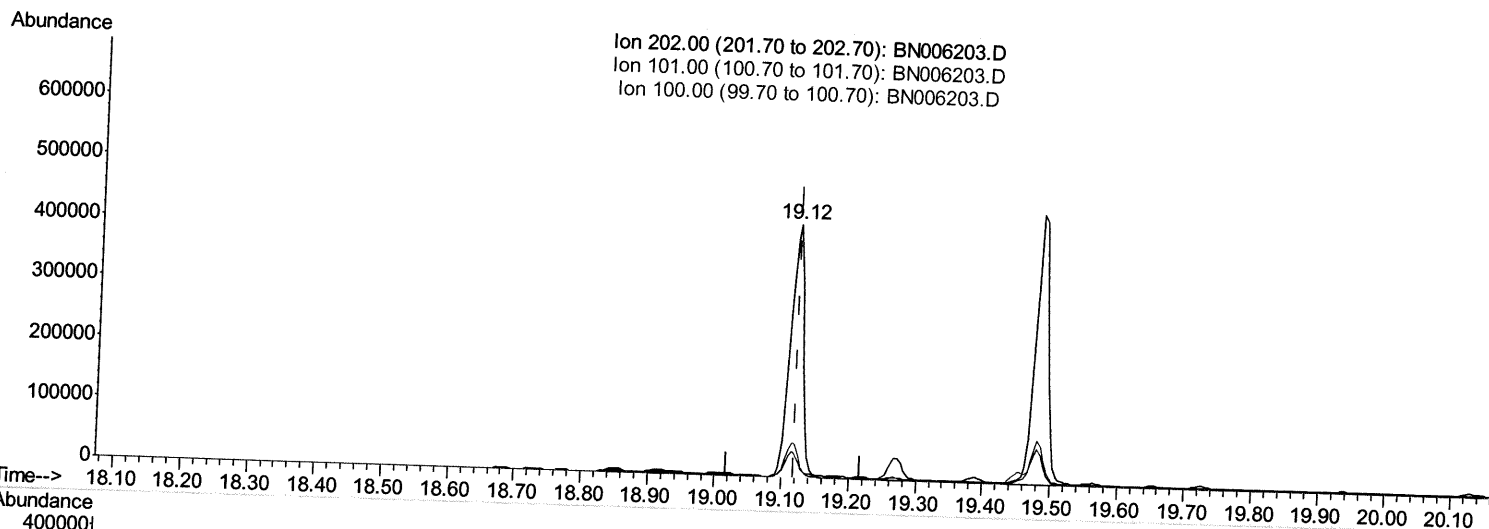

(15) Fluoranthene (C)

19.118min (0.000) 7.55ng/ul m *JU 06/10/19*

response 552376

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	12.91
100.00	8.70	9.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)

Data File : BN006203.D

Acq On : 08 Jun 2019 23:06

Operator : JU/SJ

Sample : K3016-04

Misc :

ALS Vial : 21 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampled :

A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM



Quant Time: Jun 09 05:45:14 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Jun 09 05:10:30 2019

Response via : Initial Calibration

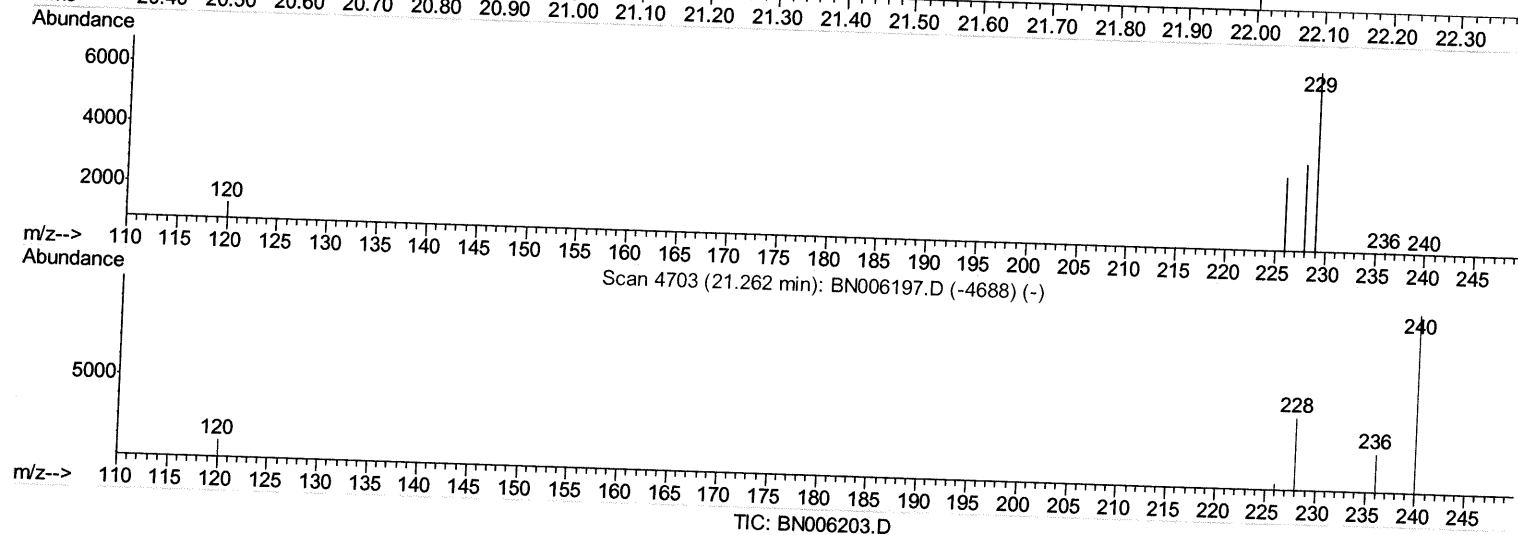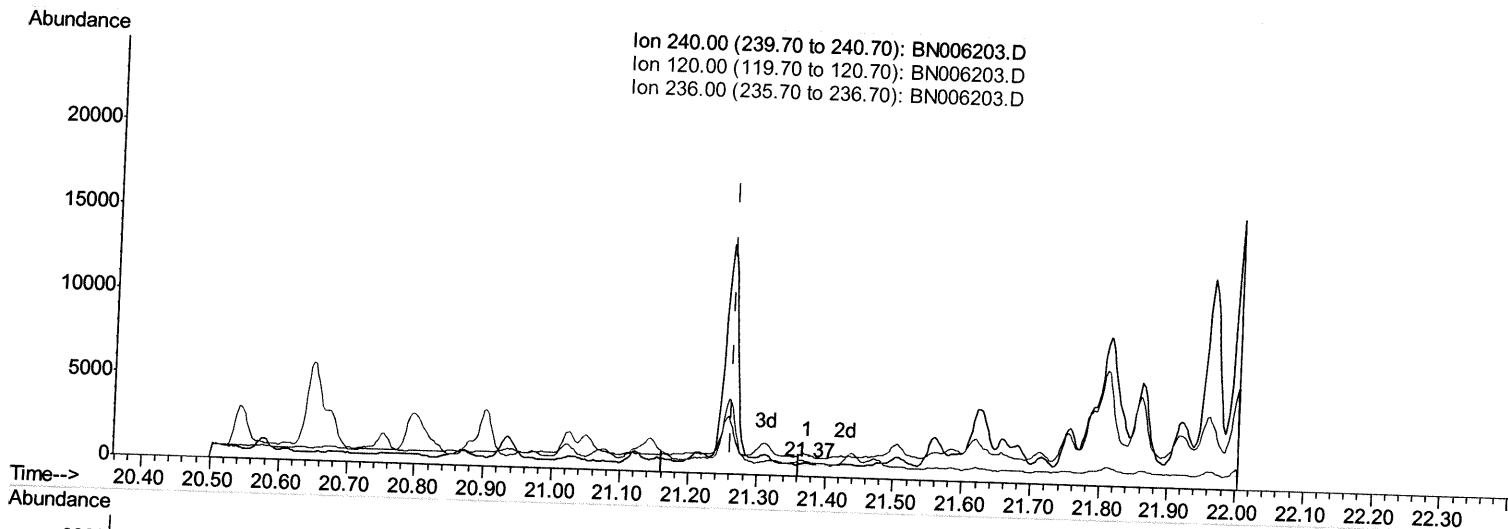

(16) Chrysene-d12 (I)

21.373min (+0.111) 0.40ng/ul

response 168

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	165.10#
236.00	30.10	104.08#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

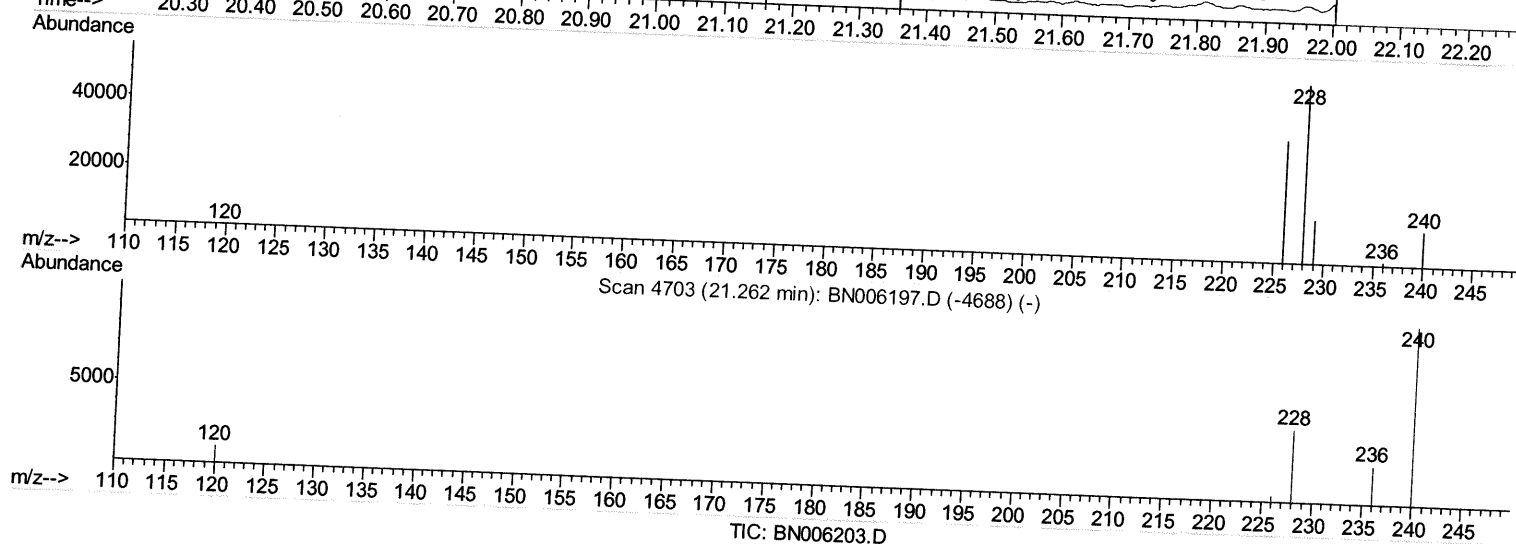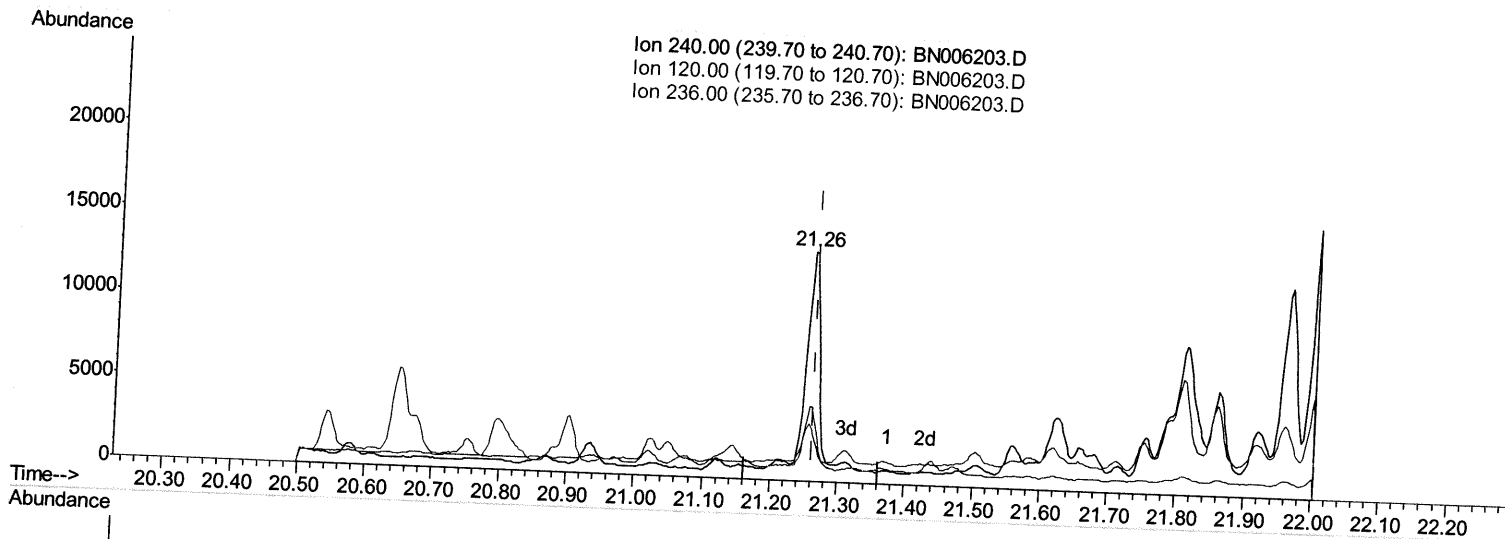

(16) Chrysene-d12 (I)

21.257min (-0.006) 0.40ng/ul m ^{JU} 06/10/19

response 16440

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	24.91#
236.00	30.10	32.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:46:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

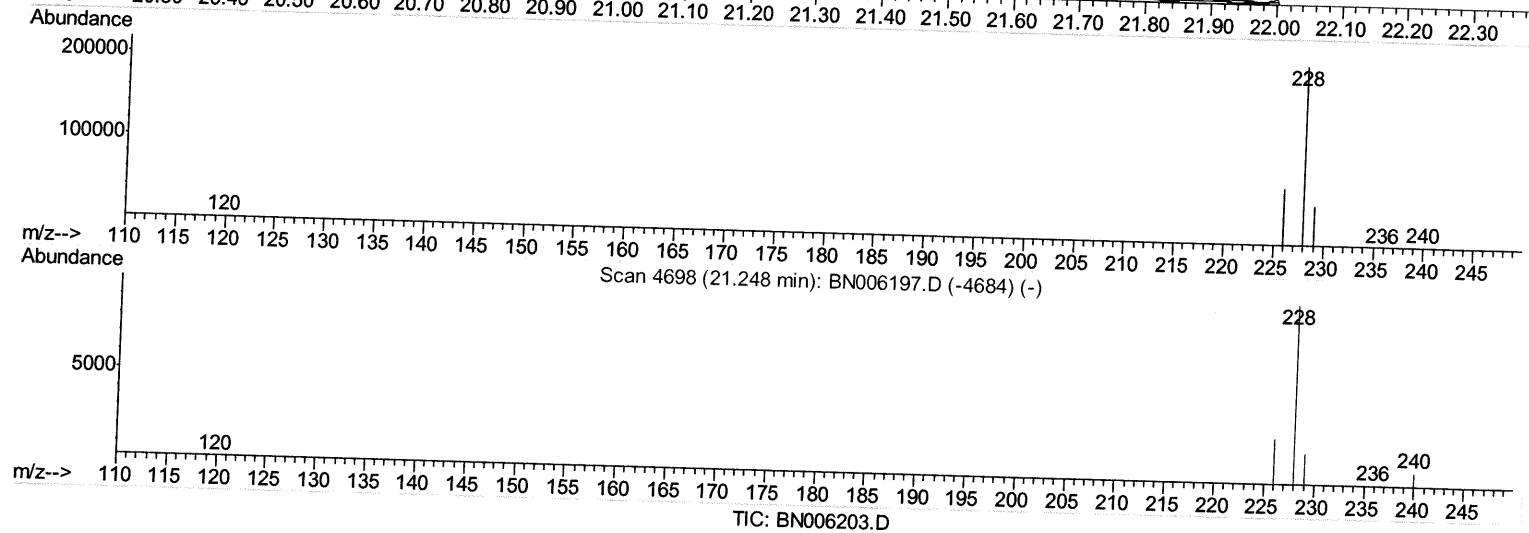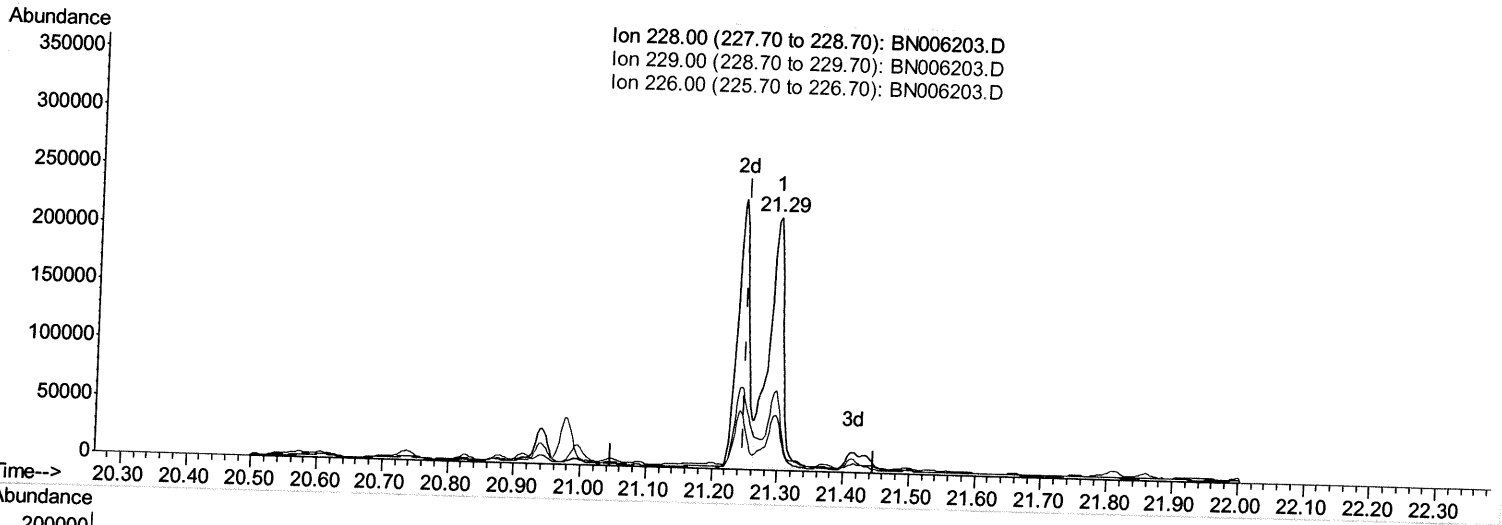

(18) Benzo(a)anthracene

21.295min (+0.047) 4.75ng/ul

response 345387

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	22.03
226.00	28.50	31.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:46:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

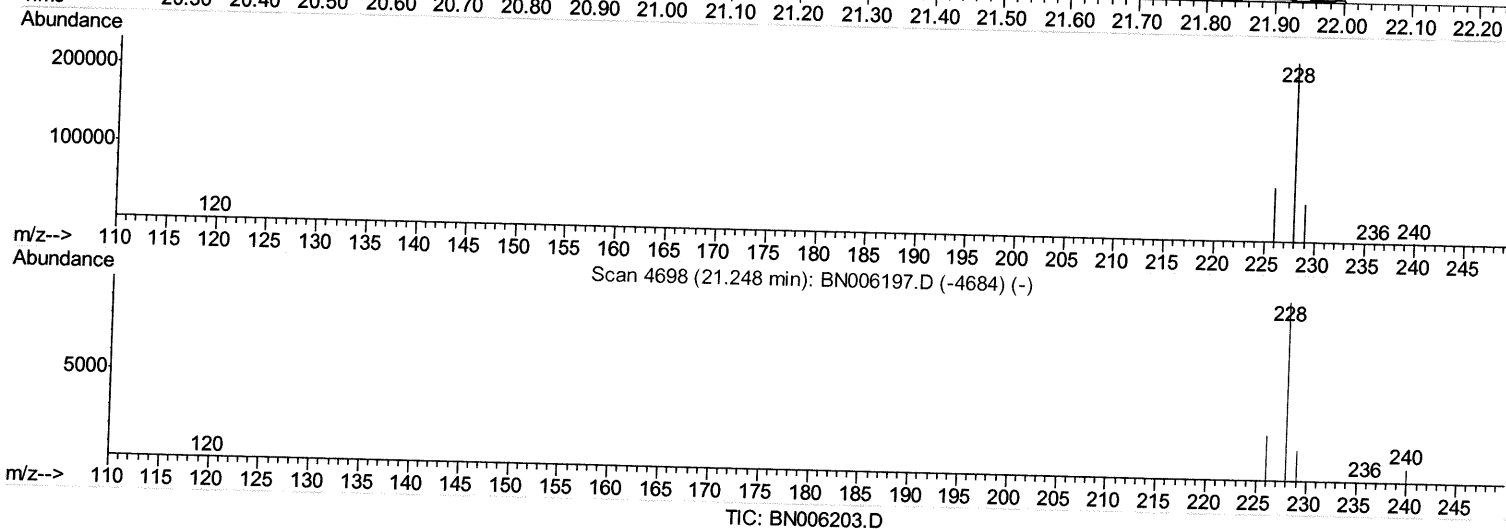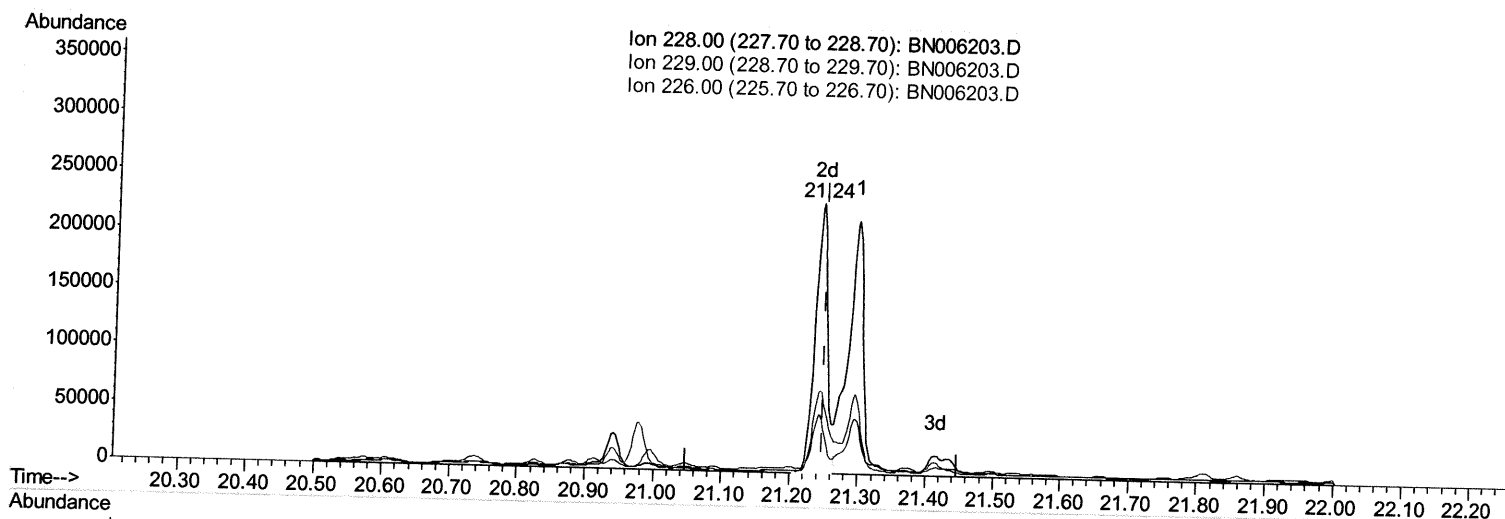

(18) Benzo(a)anthracene

21.242min (-0.006) 4.06ng/ul m ⁵⁰06/10/19

response 295566

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.71
226.00	28.50	30.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:46:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

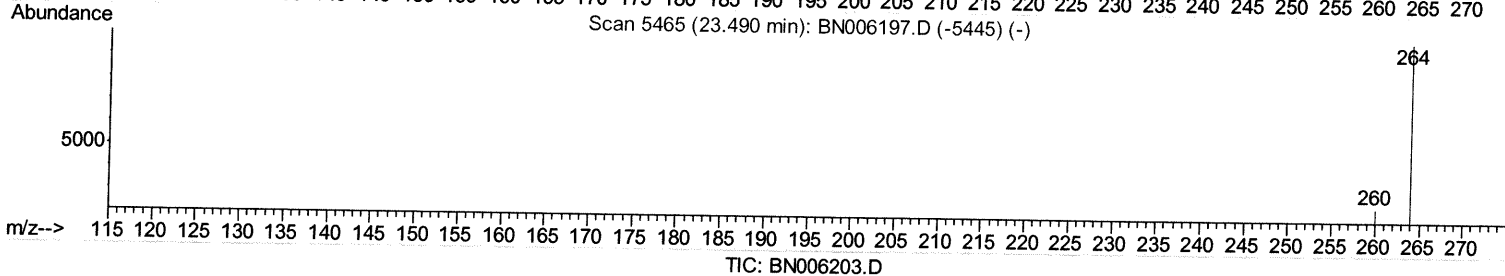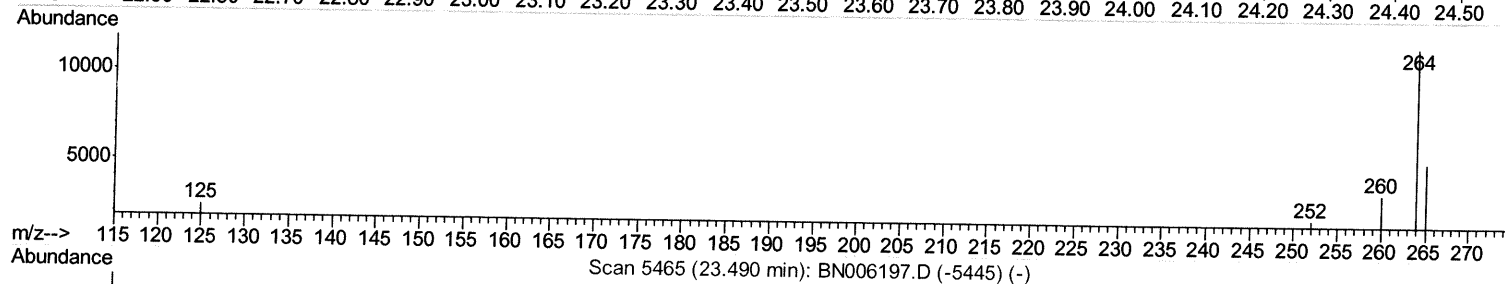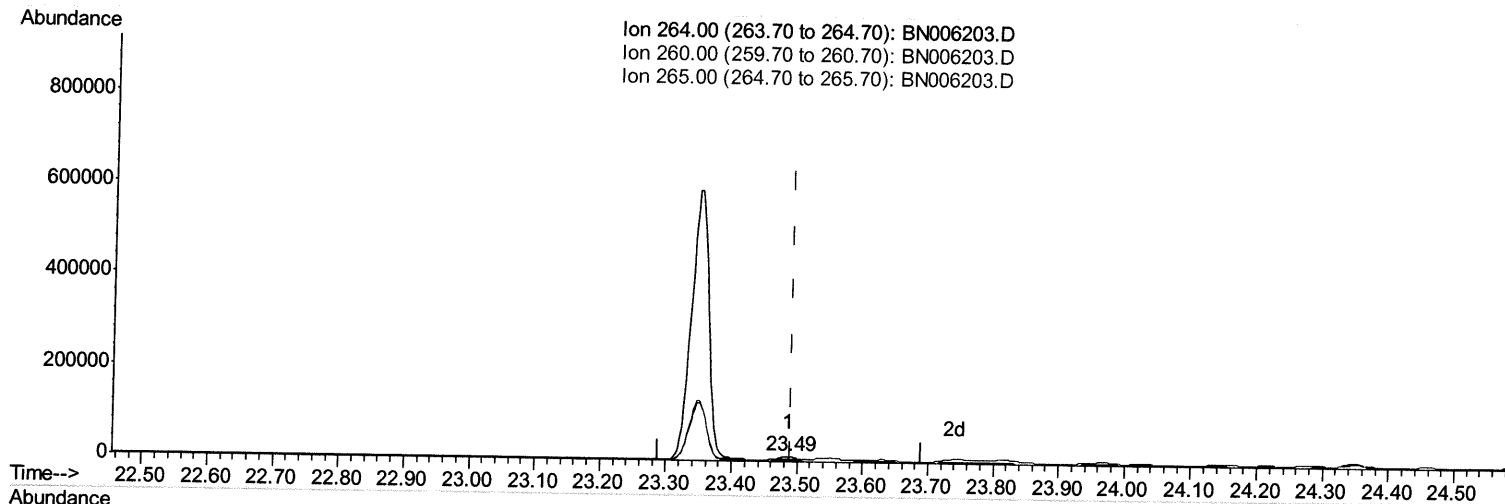

(20) Perylene-d12 (I)

23.487min (-0.003) 0.40ng/ul

response 22209

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	30.23
265.00	44.70	45.13
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:46:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

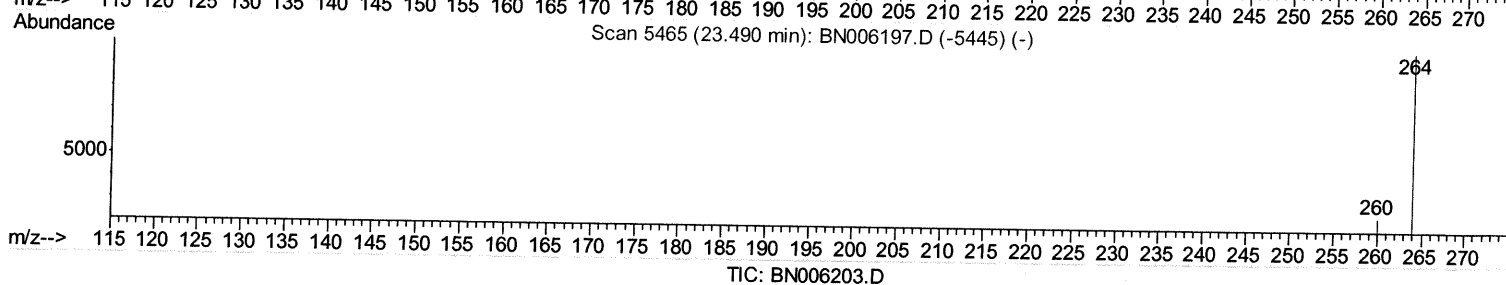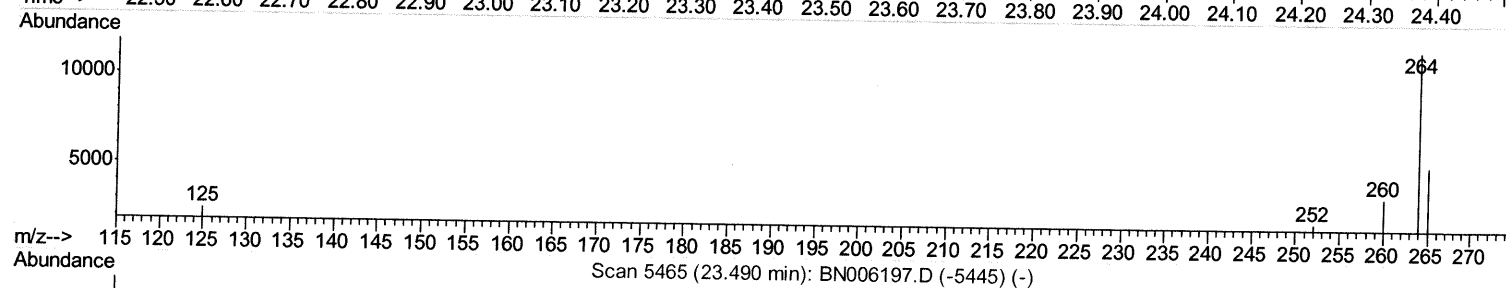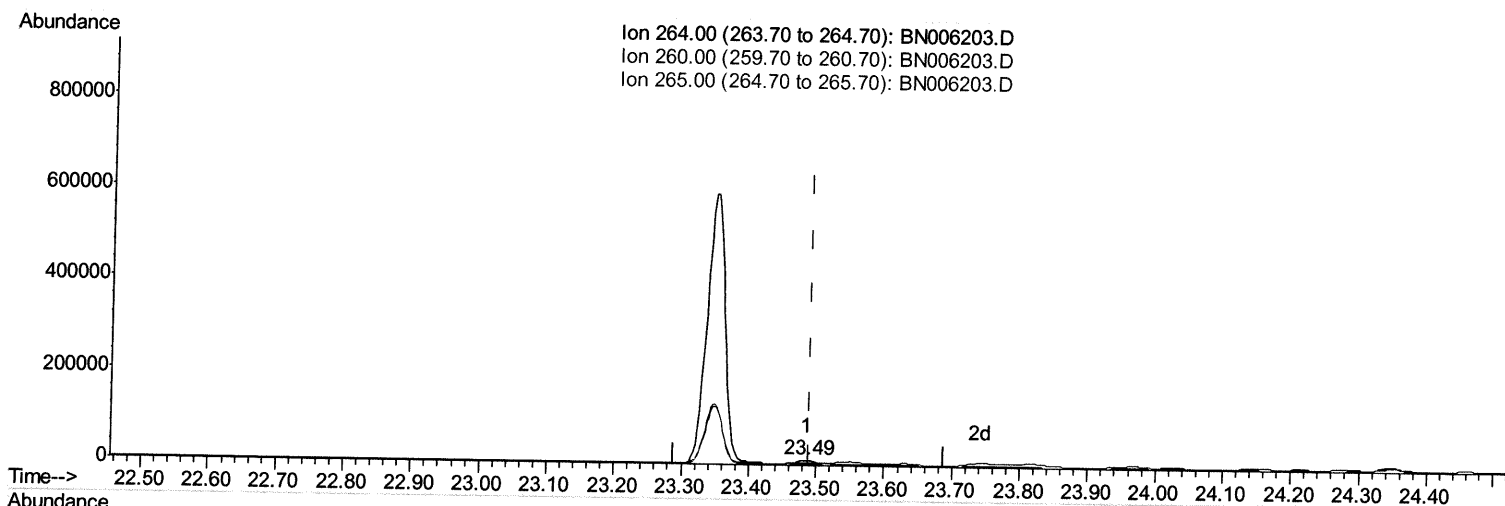

(20) Perylene-d12 (I)

23.487min (-0.003) 0.40ng/ul m *JU* 06/10/19

response 16765

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	30.23
265.00	44.70	45.13
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:47:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

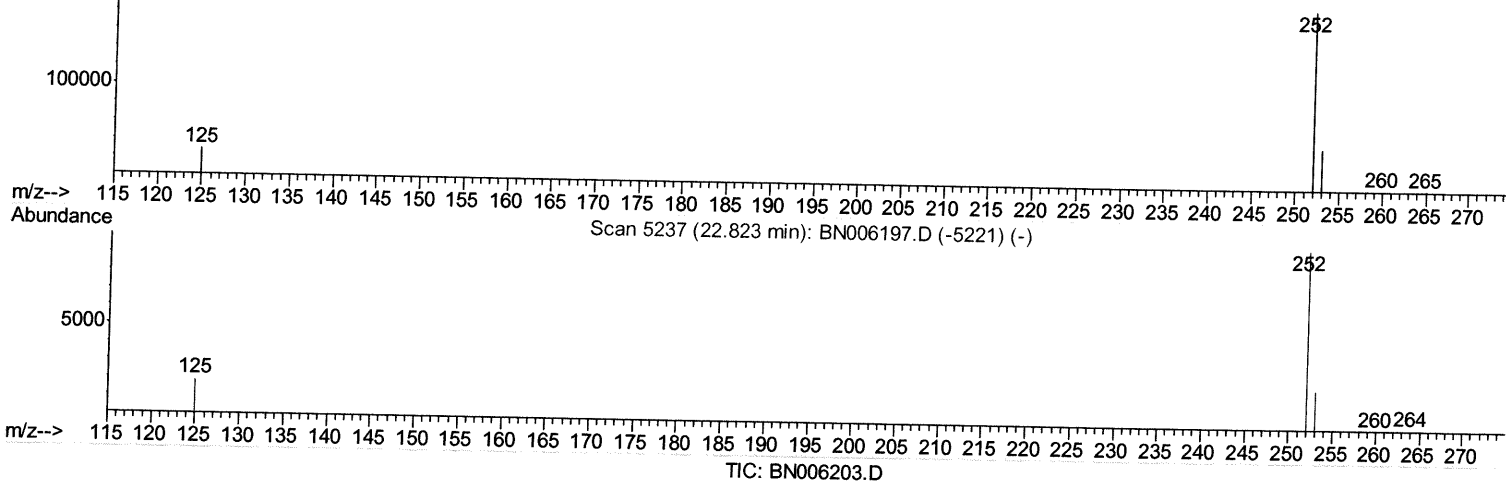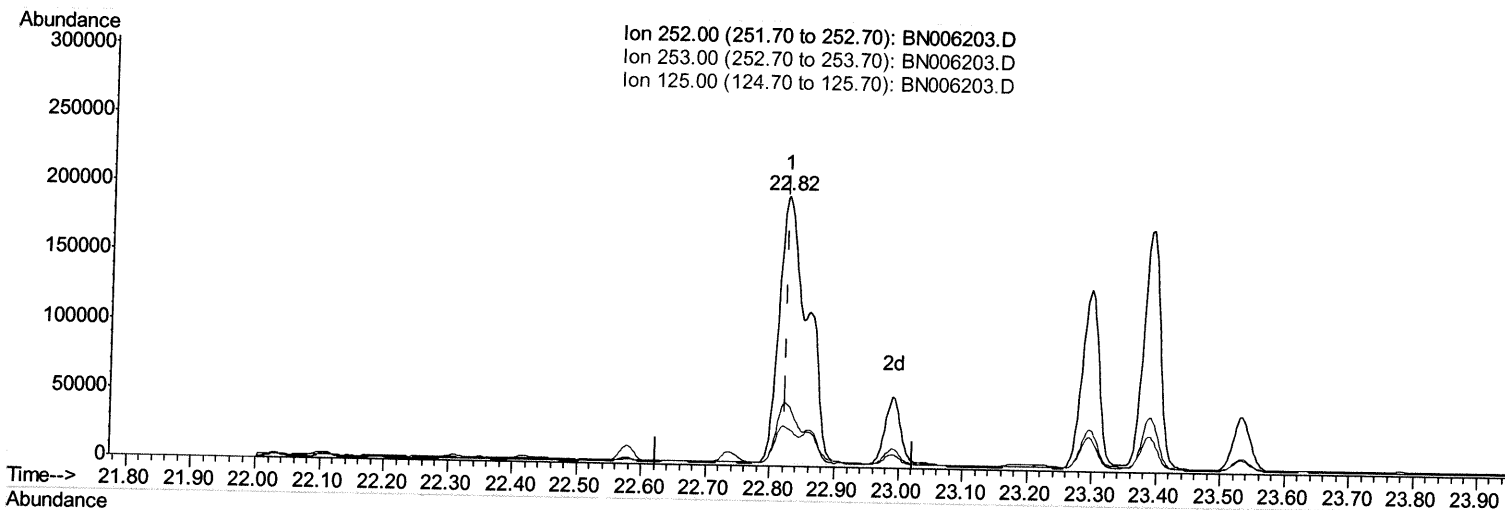

(21) Benzo(b)fluoranthene

22.823min (0.000) 8.49ng/ul

response 593717

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	23.59
125.00	20.50	14.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\

Quantitation Report (Qedit)

Data File : BN006203.D

Acq On : 08 Jun 2019 23:06

Operator : JU/SJ

Sample : K3016-04

Misc :

ALS Vial : 21 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM



Quant Time: Jun 09 05:47:45 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Jun 09 05:10:30 2019

Response via : Initial Calibration

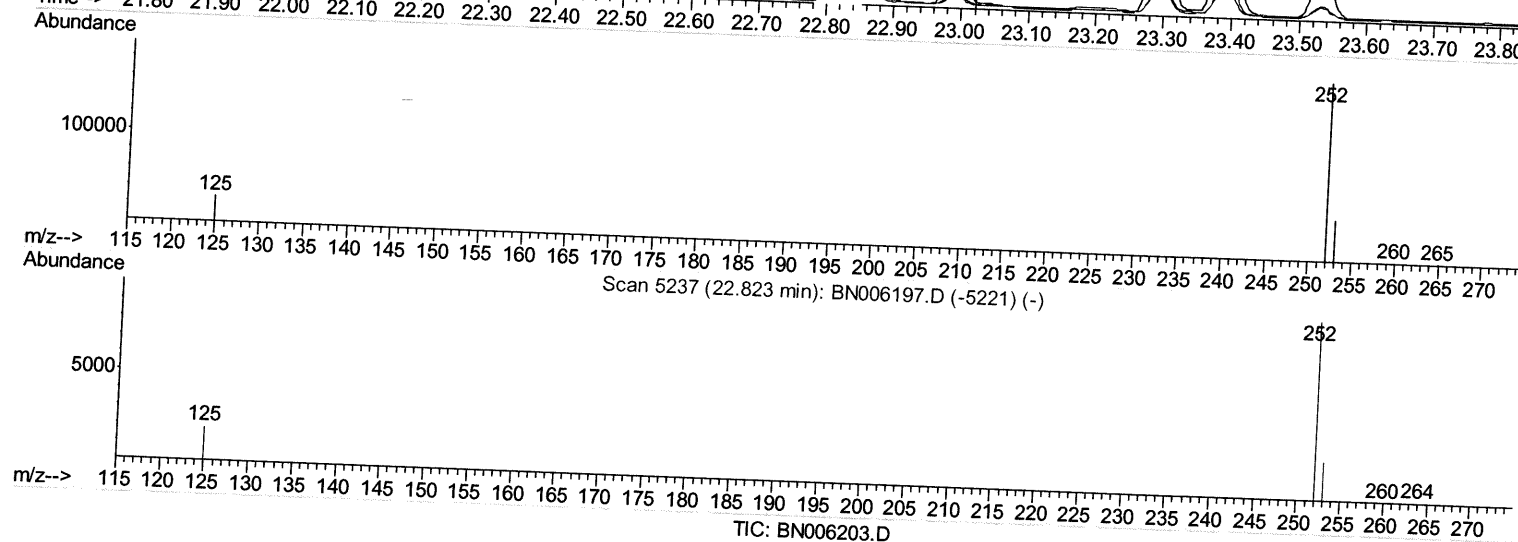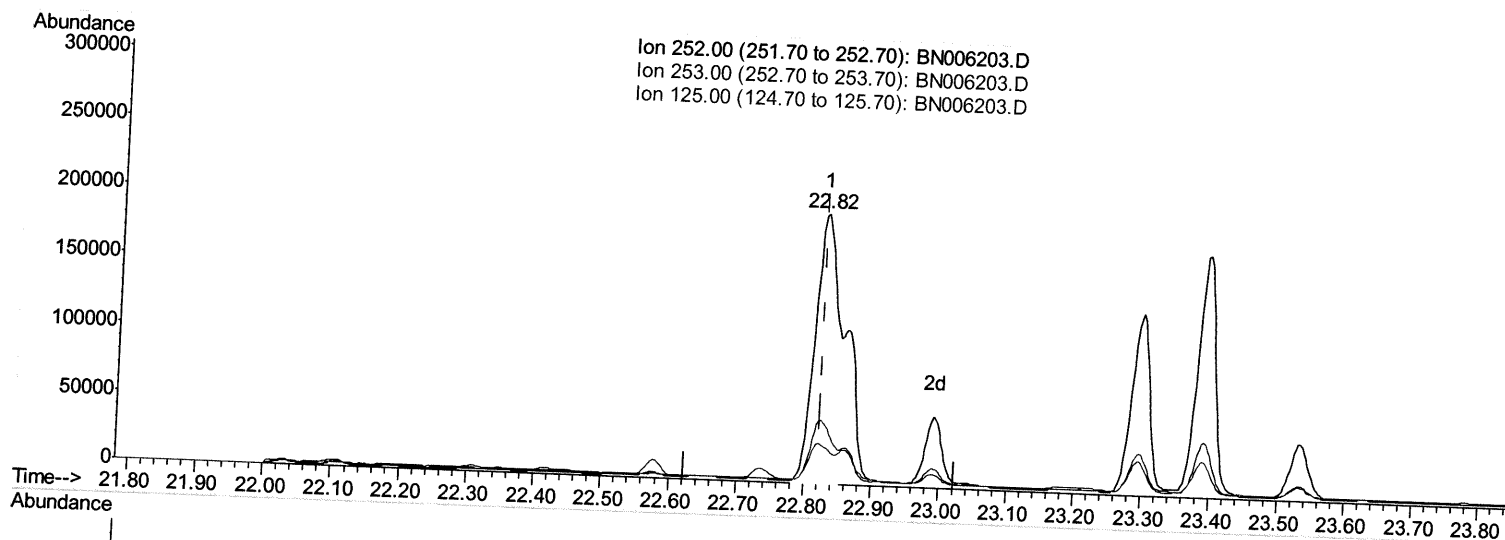

(21) Benzo(b)fluoranthene

22.823min (0.000) 6.48ng/ul m *JU 06/10/19*

response 452773

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	23.59
125.00	20.50	14.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:47:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

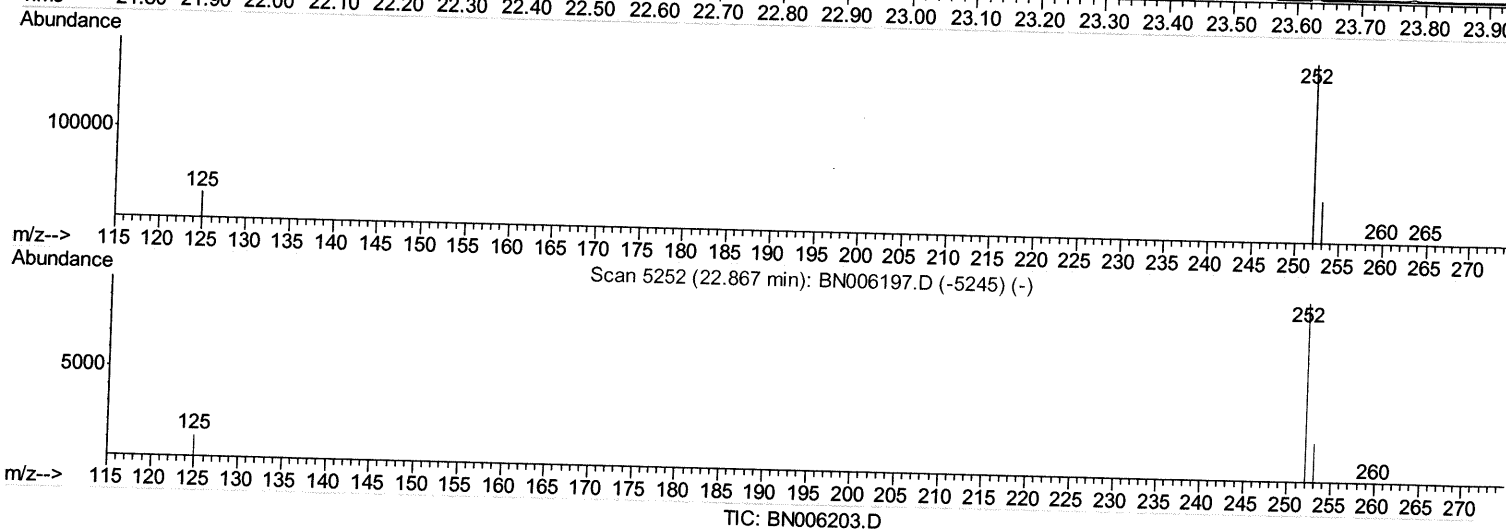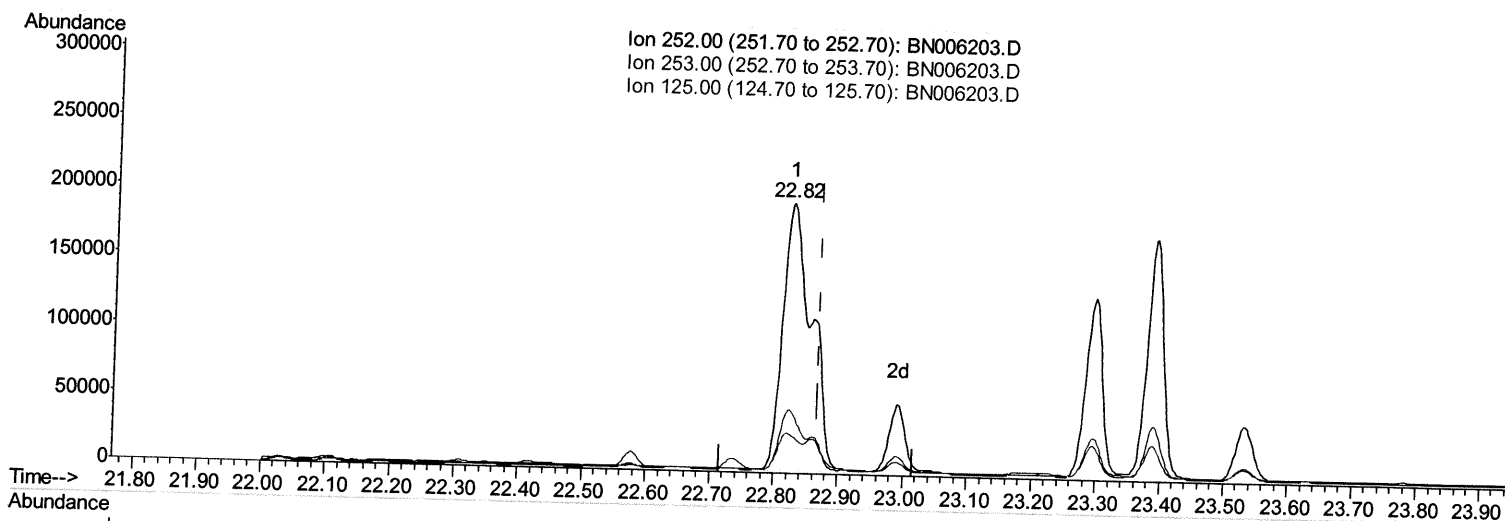

(22) Benzo(k)fluoranthene

22.823min (-0.044) 8.72ng/ul

response 593632

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.59
125.00	17.90	14.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:47:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

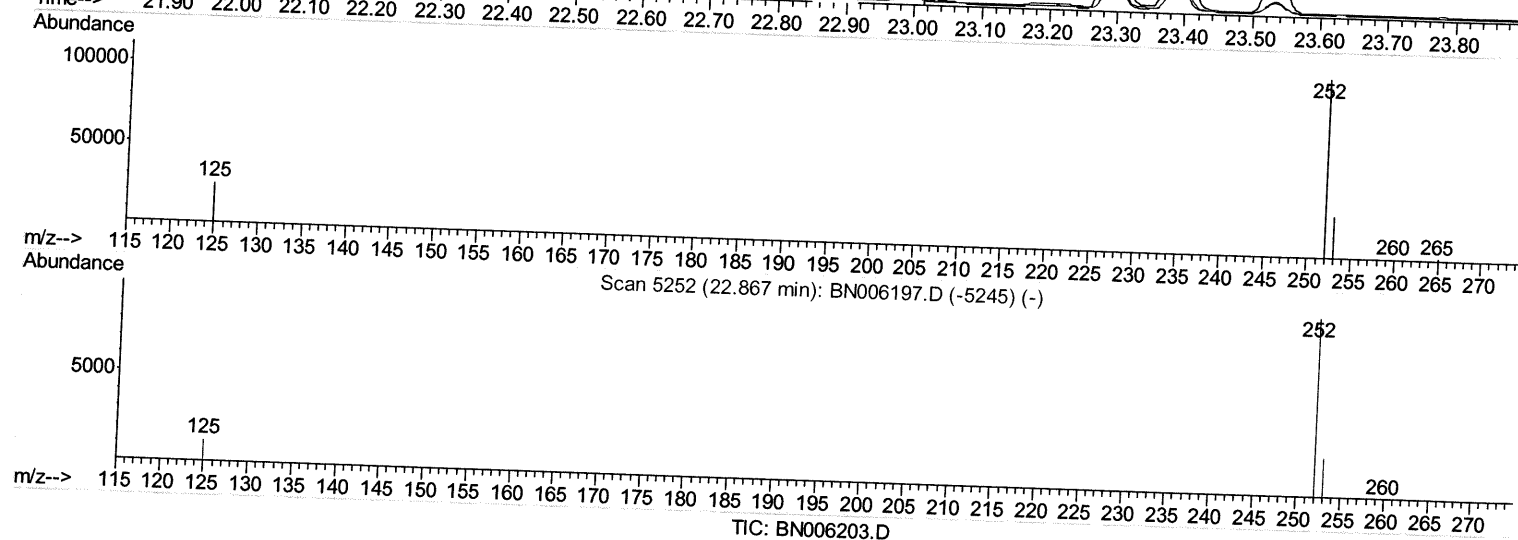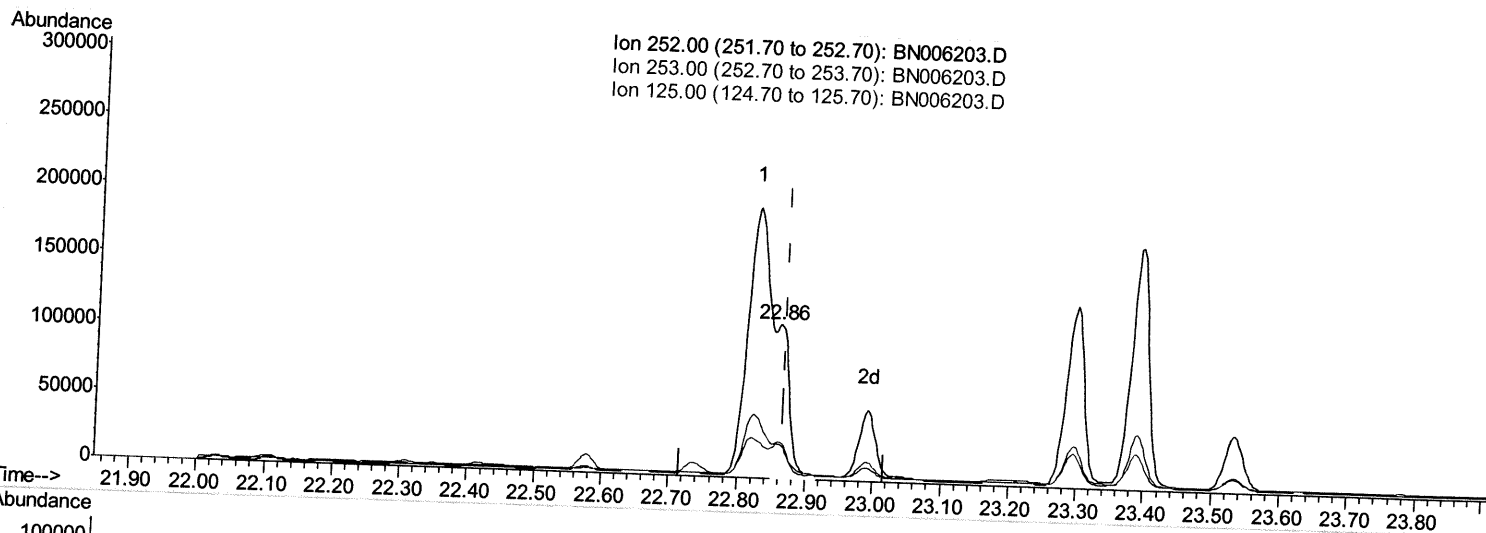

(22) Benzo(k)fluoranthene

22.858min (-0.009) 2.52ng/ul m

JU
06/10/19

response 171490

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.89
125.00	17.90	22.44#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:15:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

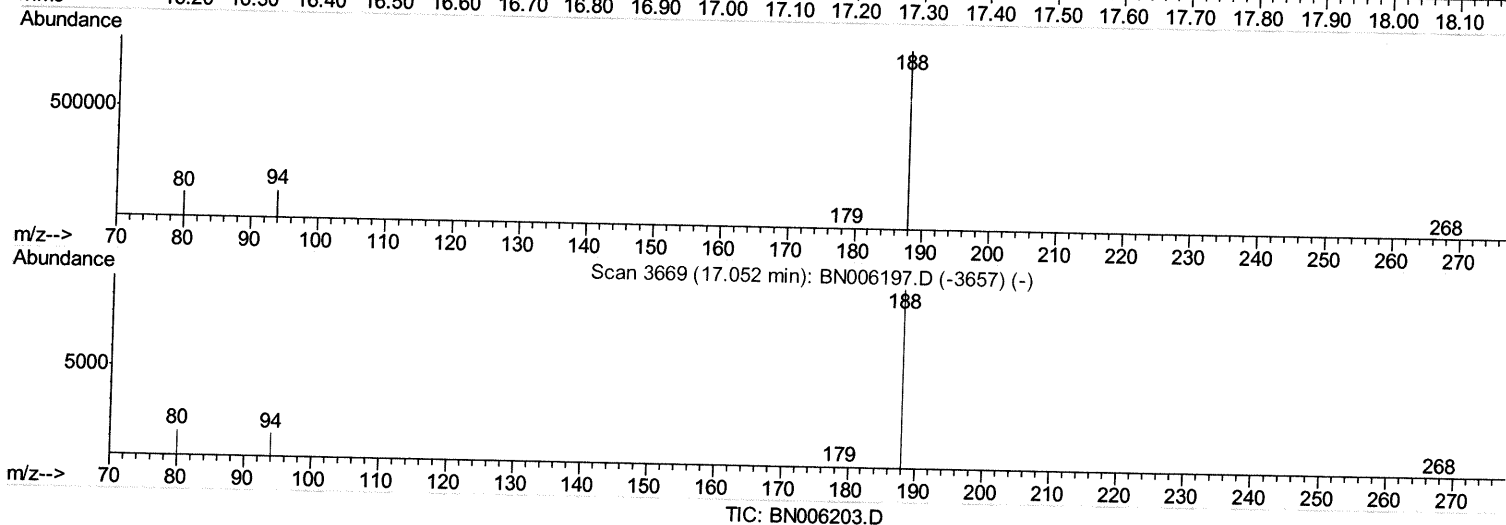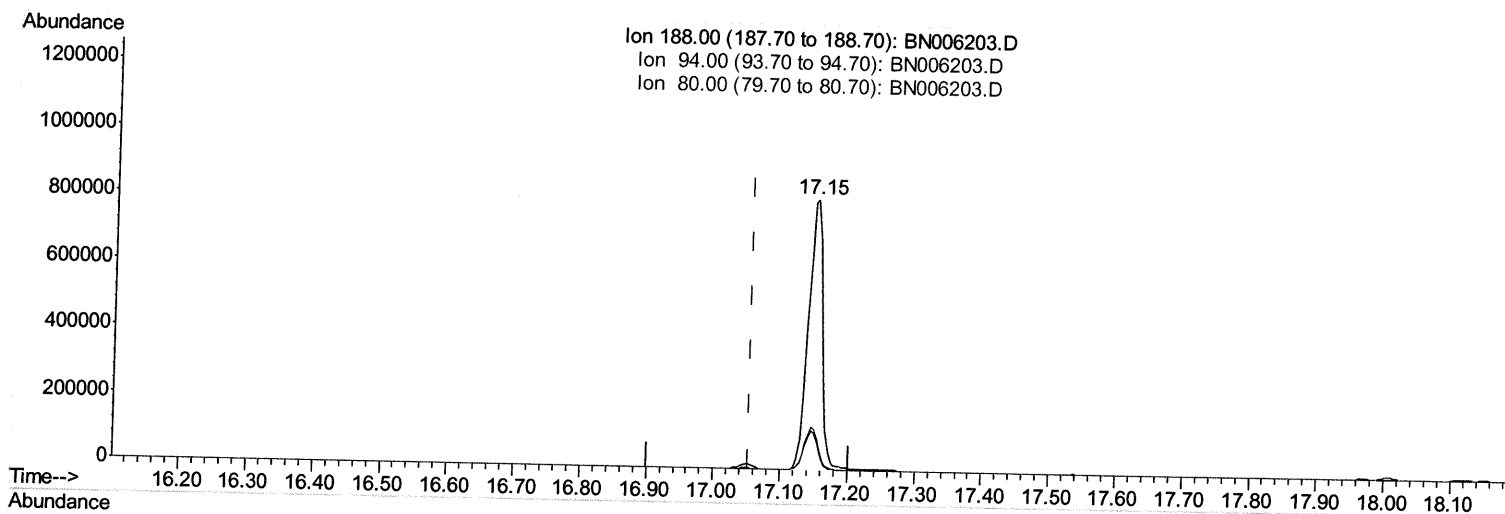

(10) Phenanthrene-d10 (I)

17.149min (+0.097) 0.40ng/ul

response 1178918

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.18
80.00	13.60	13.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:15:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

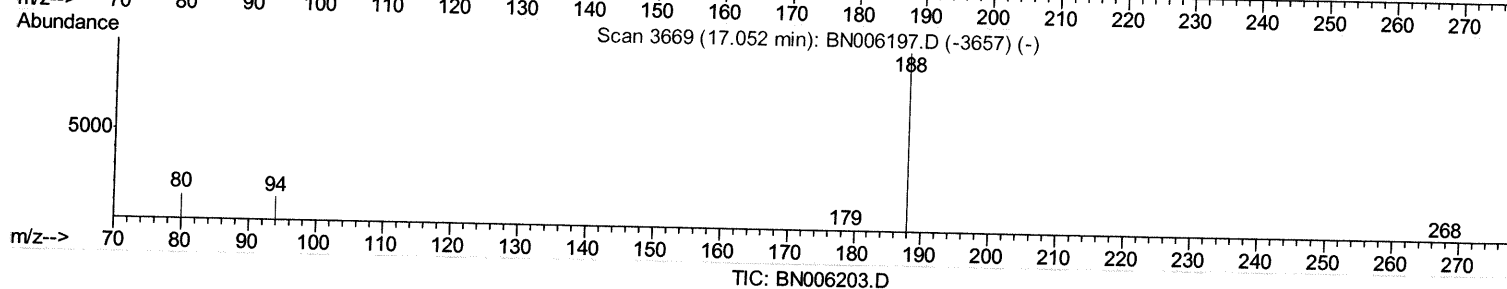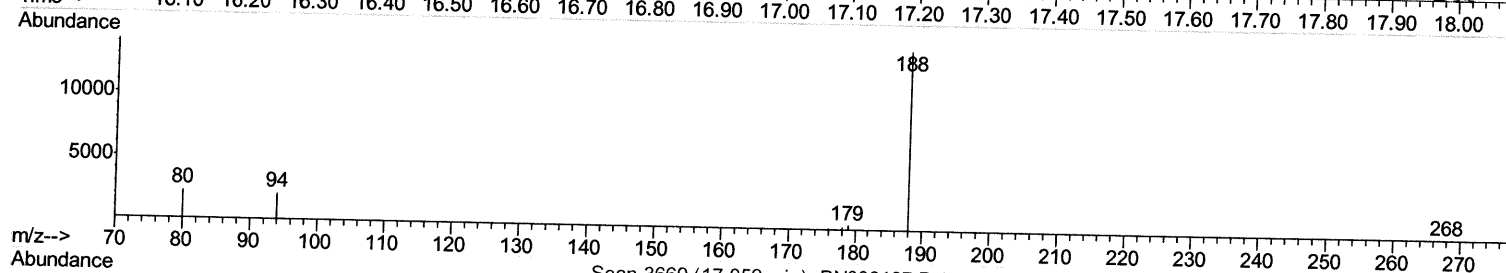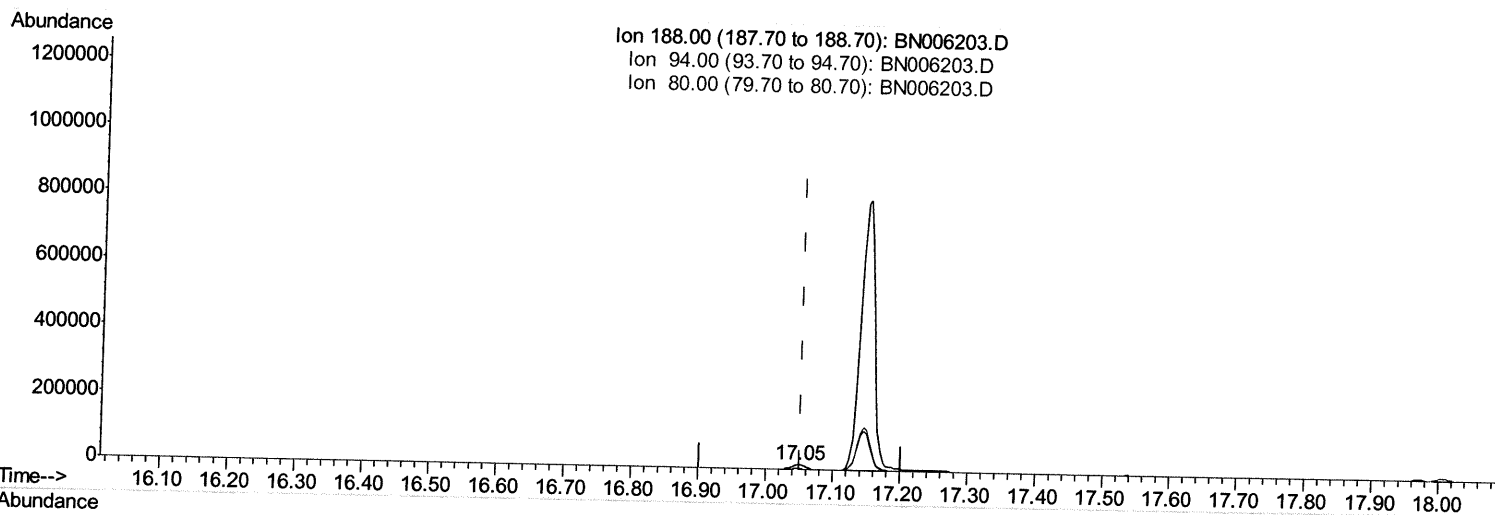

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m *JU*
06/10/19

response 20630

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.96
80.00	13.60	16.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

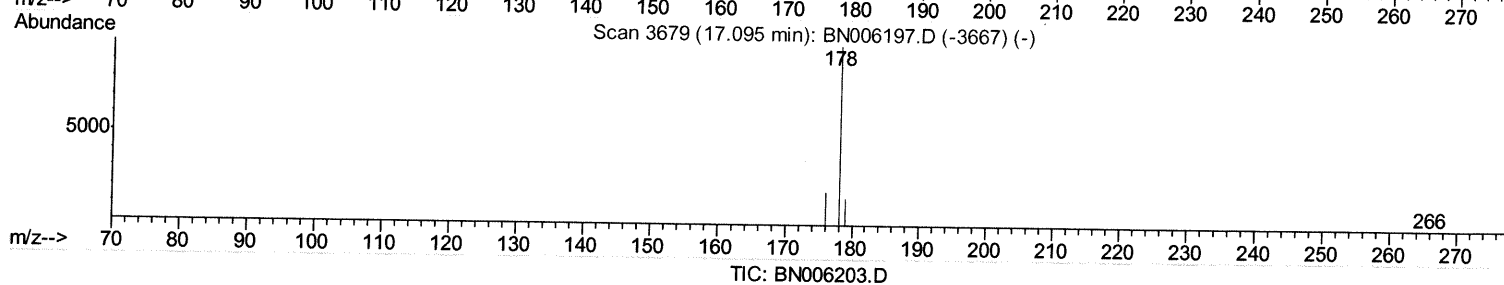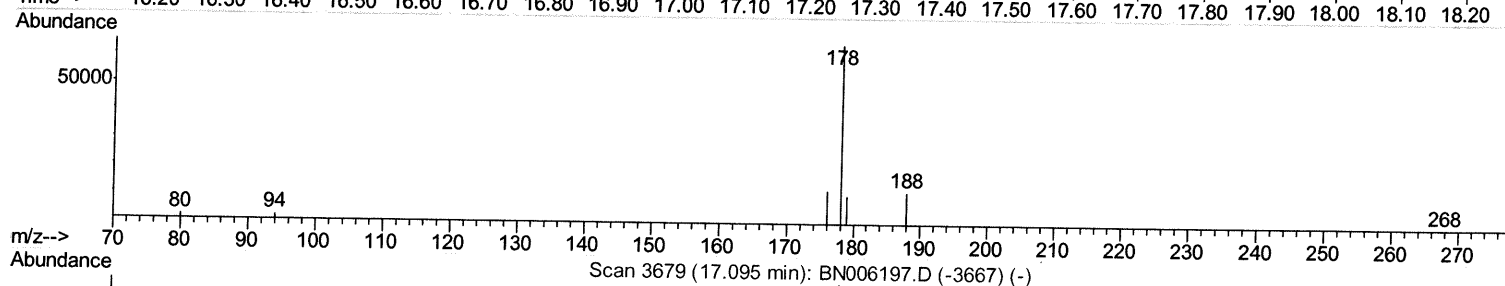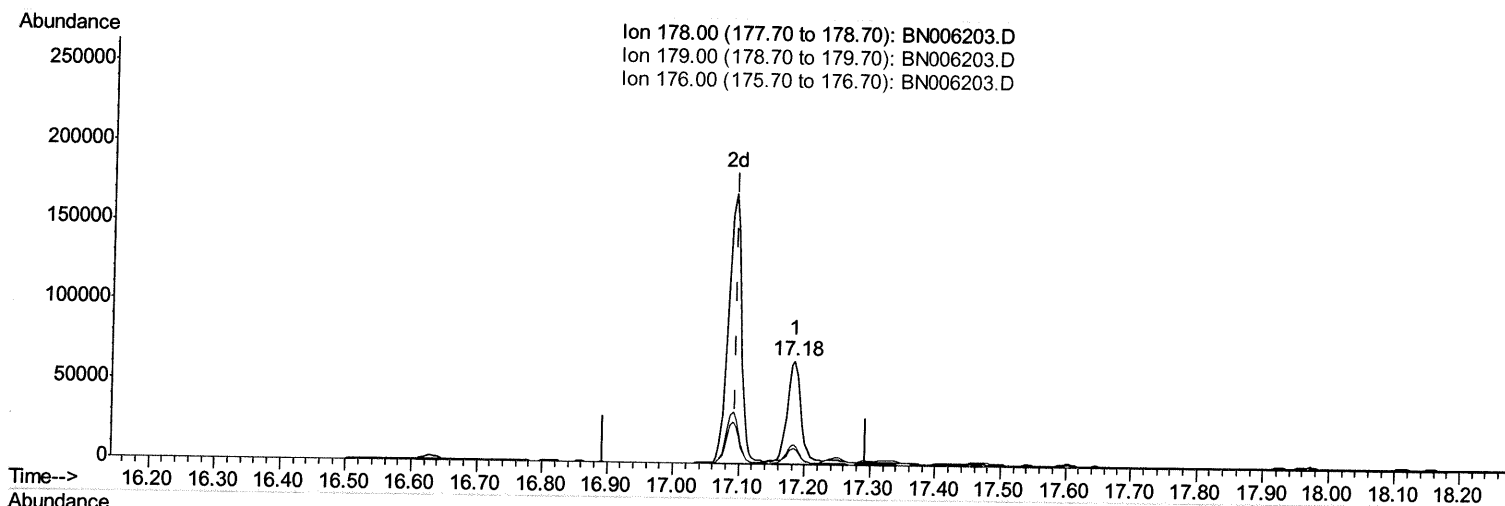

(12) Phenanthrene

17.183min (+0.089) 1.47ng/ul

response 97213

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.58
176.00	19.10	18.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:45:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

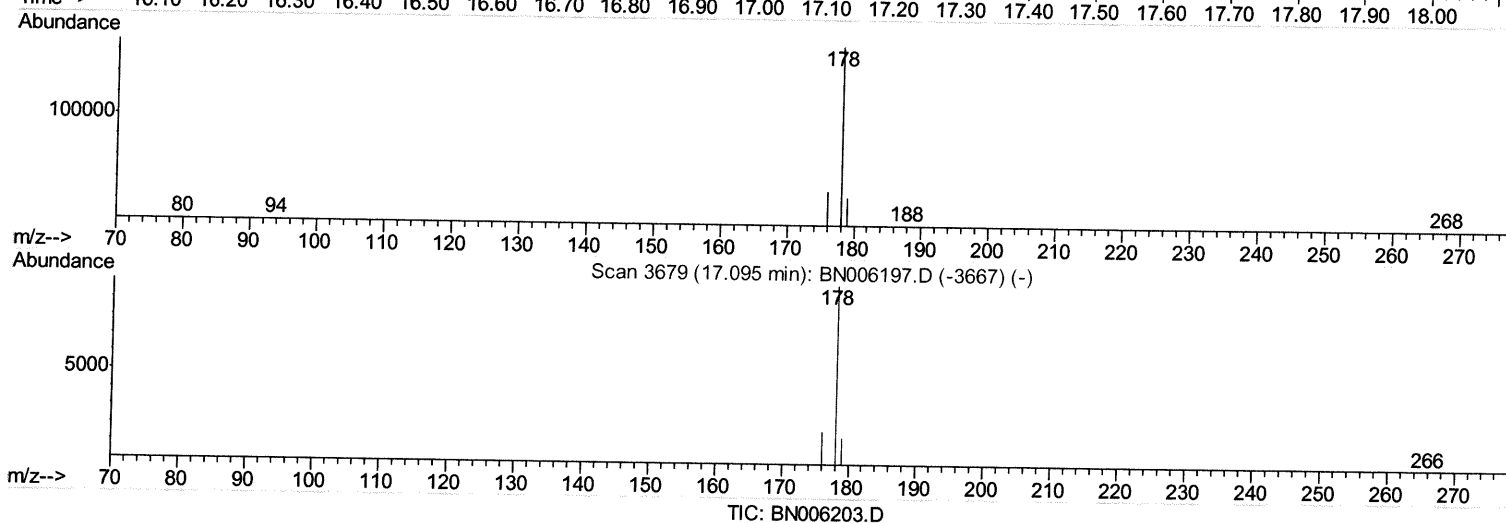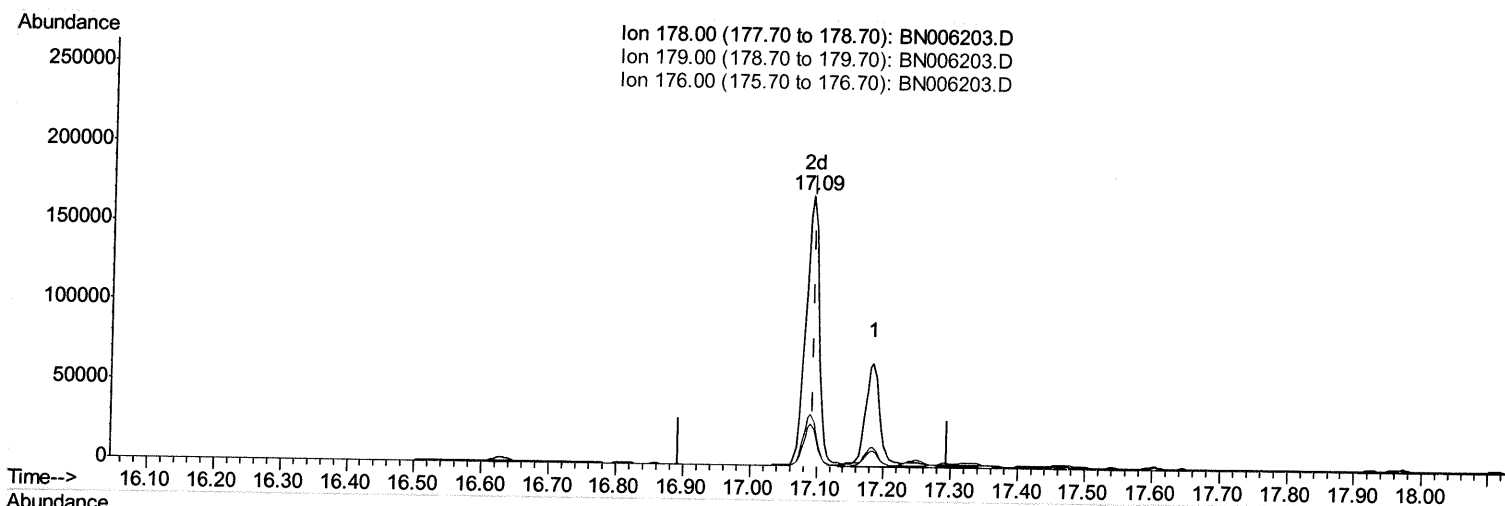

(12) Phenanthrene

17.090min (-0.004) 3.57ng/ul m *Ju* 06/10/19

response 236333

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.51
176.00	19.10	19.12
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (QT Reviewed)

Data File : BN006203.D
Acq On : 08 Jun 2019 23:06
Operator : JU/SJ
Sample : K3016-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51C3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:31:59 PM

Quant Time: Jun 09 05:54:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4654	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	17643	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	9633	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	20630m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	16440m>	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	16765m>	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	7334	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	18316m>	0.33	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.47	128	9820	0.202	ng/ul	96
5) 2-Methylnaphthalene	12.10	142	4763	0.140	ng/ul	97
7) Acenaphthylene	14.01	152	101004	1.886	ng/ul	100
8) Acenaphthene	14.36	153	4455	0.120	ng/ul	97
9) Fluorene	15.35	166	14785	0.340	ng/ul#	93
12) Phenanthrene	17.09	178	236333m>	3.569	ng/ul	
13) Anthracene	17.18	178	89711m>	1.419	ng/ul	
15) Fluoranthene	19.12	202	552376m>	7.554	ng/ul	
17) Pyrene	19.48	202	590713	6.821	ng/ul	97
18) Benzo(a)anthracene	21.24	228	295566m>	4.065	ng/ul	
19) Chrysene	21.29	228	341330	5.000	ng/ul	98
21) Benzo(b)fluoranthene	22.82	252	452773m>	6.477	ng/ul	
22) Benzo(k)fluoranthene	22.86	252	171490m>	2.519	ng/ul	
23) Benzo(a)pyrene	23.39	252	312605	4.801	ng/ul#	86
24) Indeno(1,2,3-cd)pyrene	25.71	276	225073	3.194	ng/ul#	89
25) Dibenzo(a,h)anthracene	25.72	278	57686	1.024	ng/ul	100
26) Benzo(g,h,i)perylene	26.40	276	173013	2.931	ng/ul	95

Ju 06/10/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed