


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060819\
Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 10 02:40:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

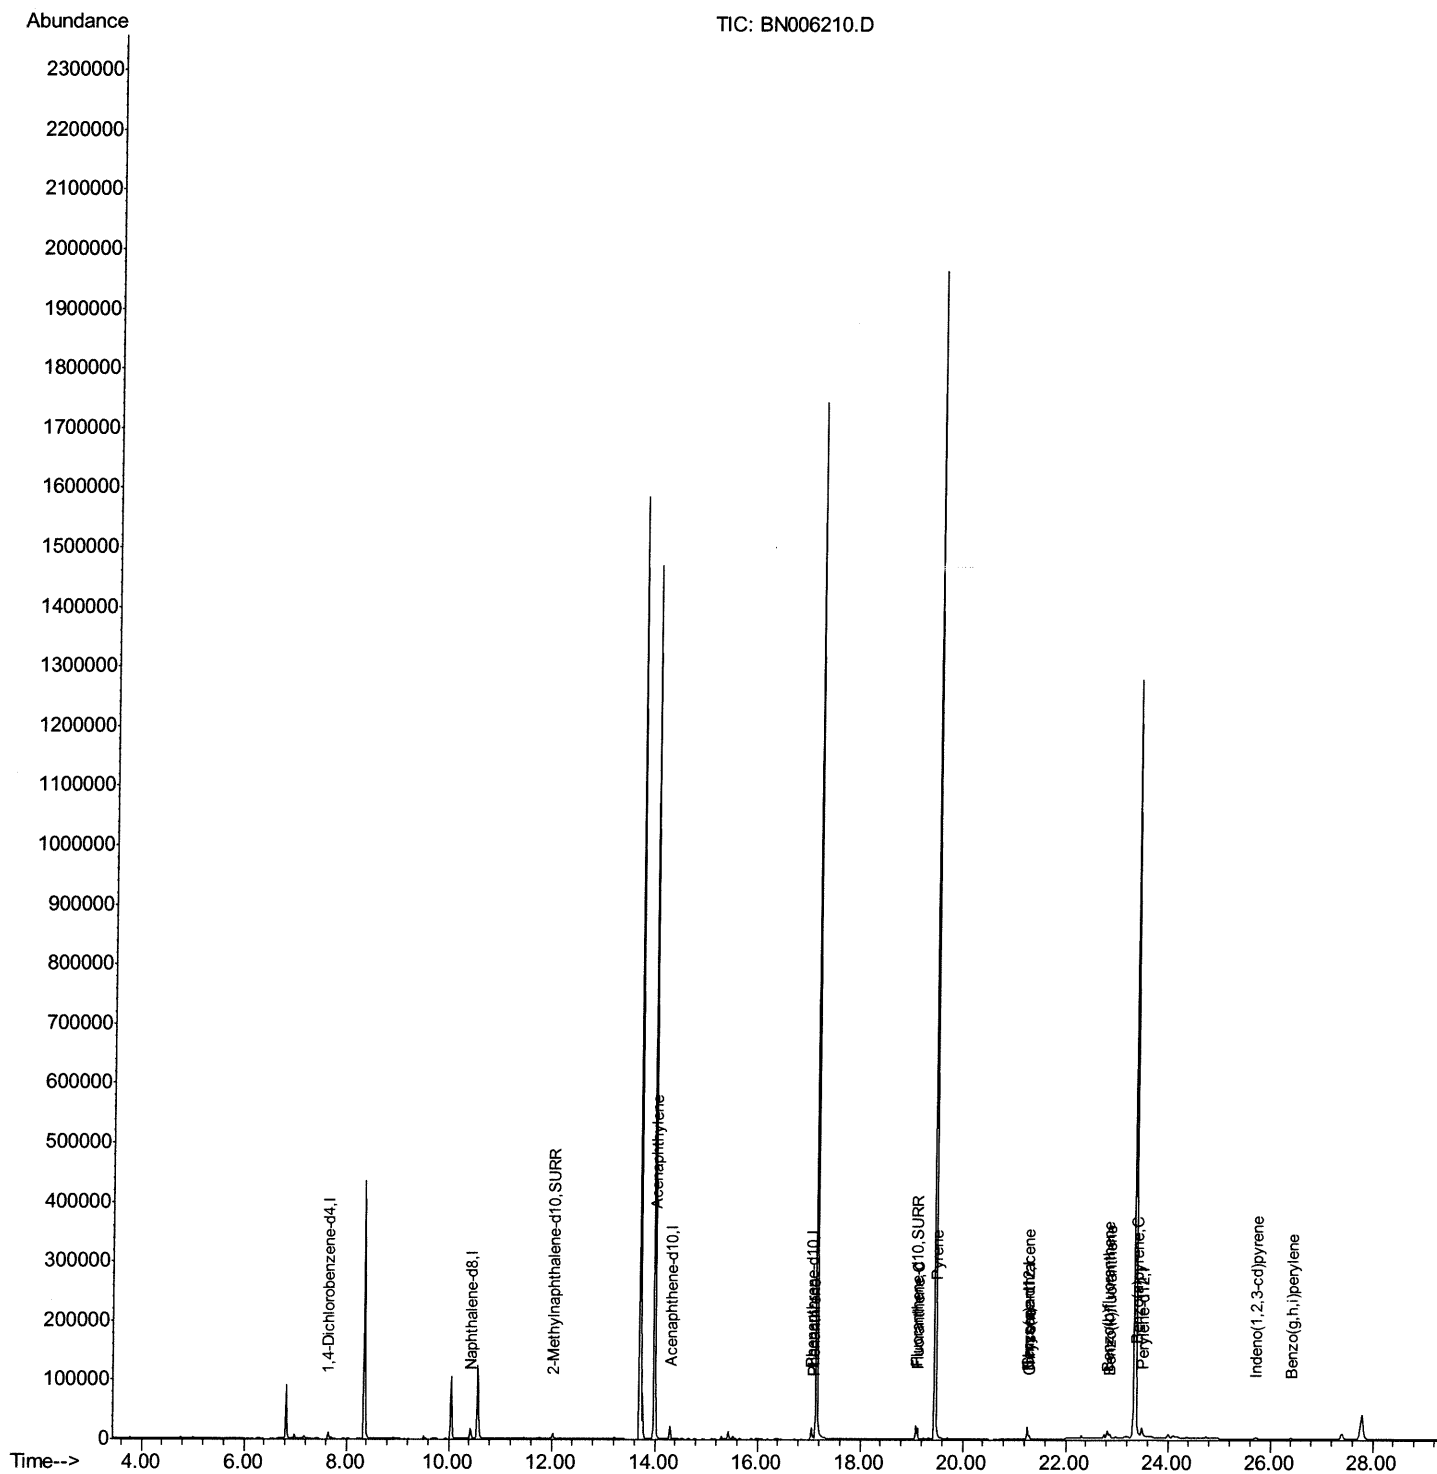

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 05:16:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

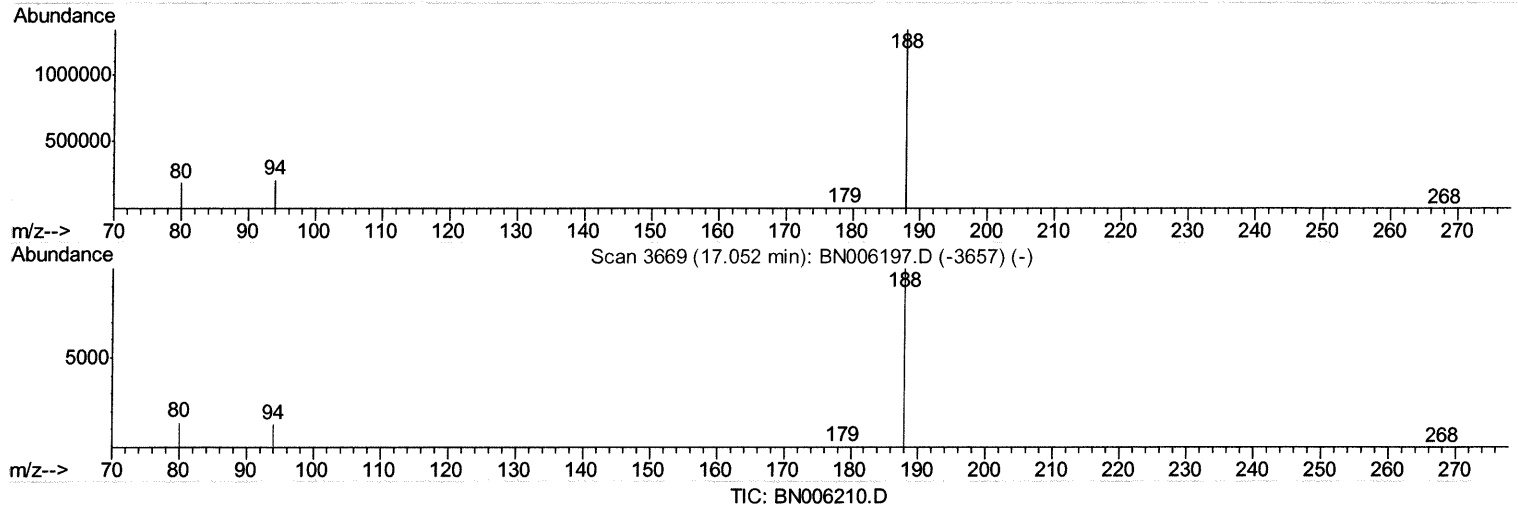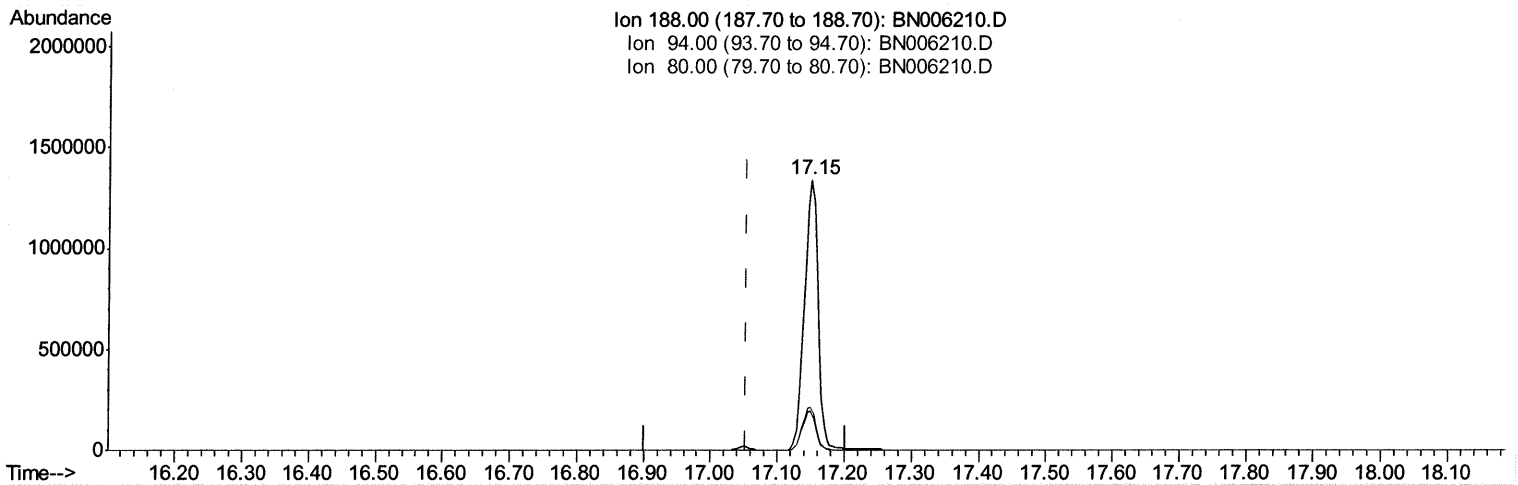

(10) Phenanthrene-d10 (I)

17.149min (+0.097) 0.40ng/ul

response 1913336

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	15.85#
80.00	13.60	14.34
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 05:16:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

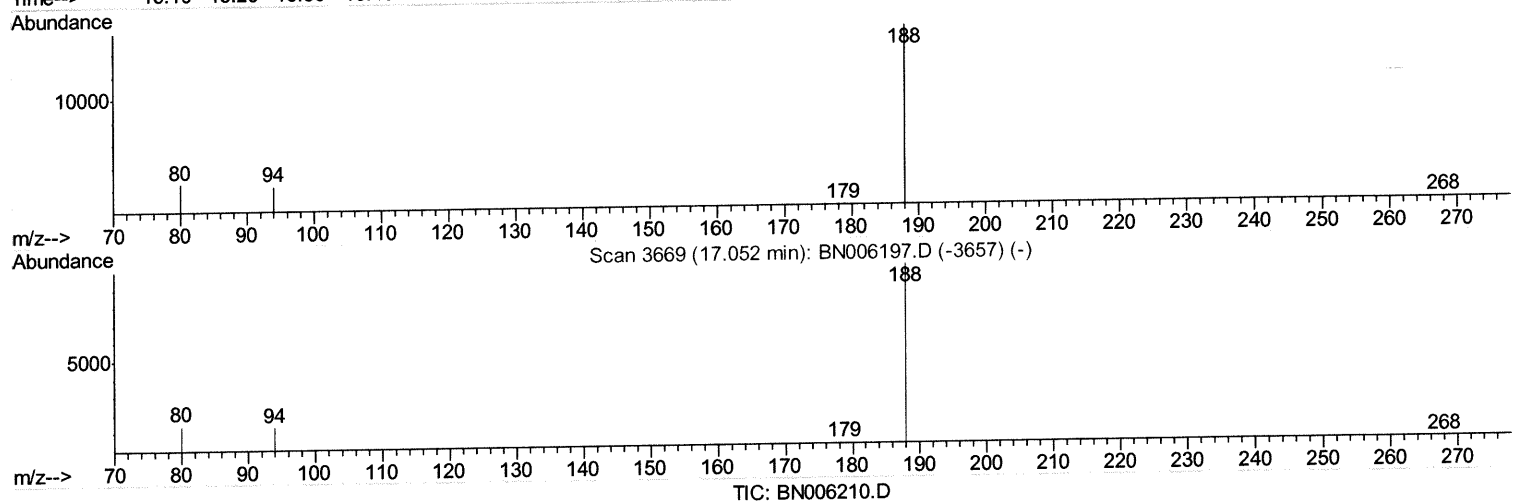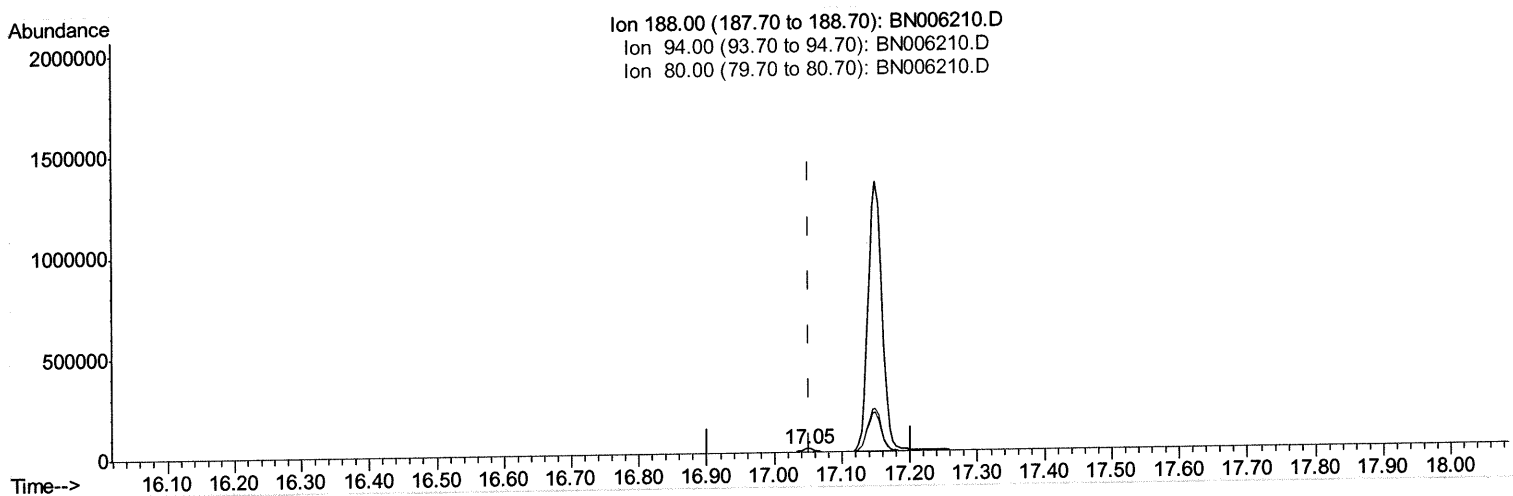

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m

JU
06/10/19

response 22701

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.31
80.00	13.60	15.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:28:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

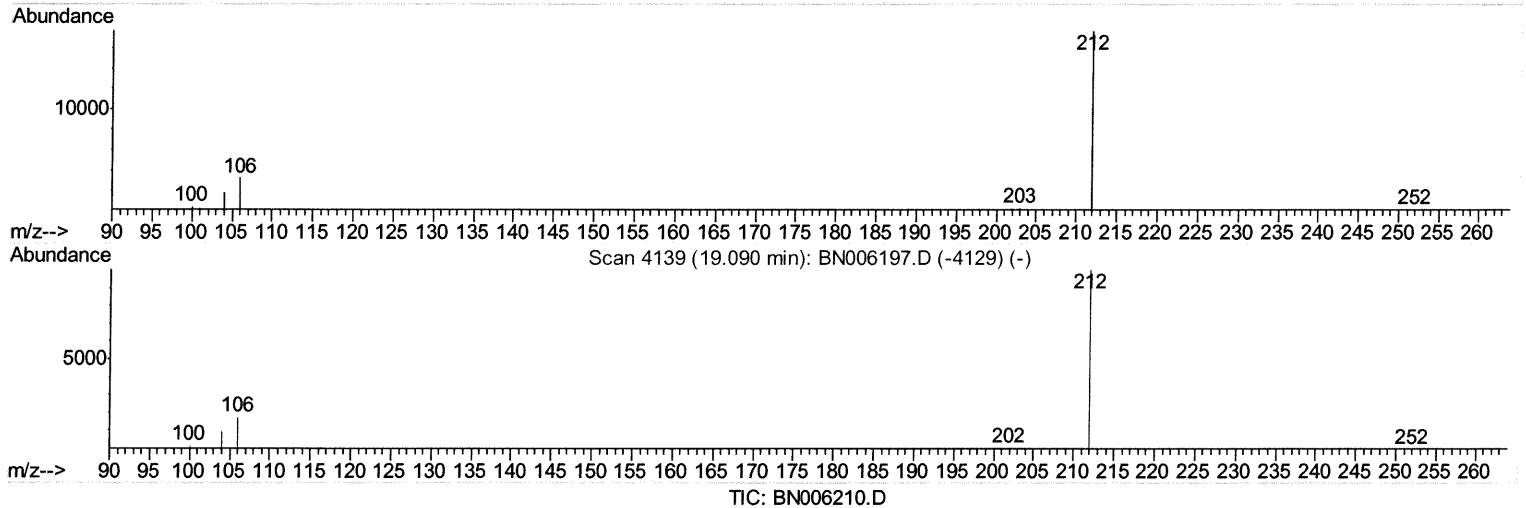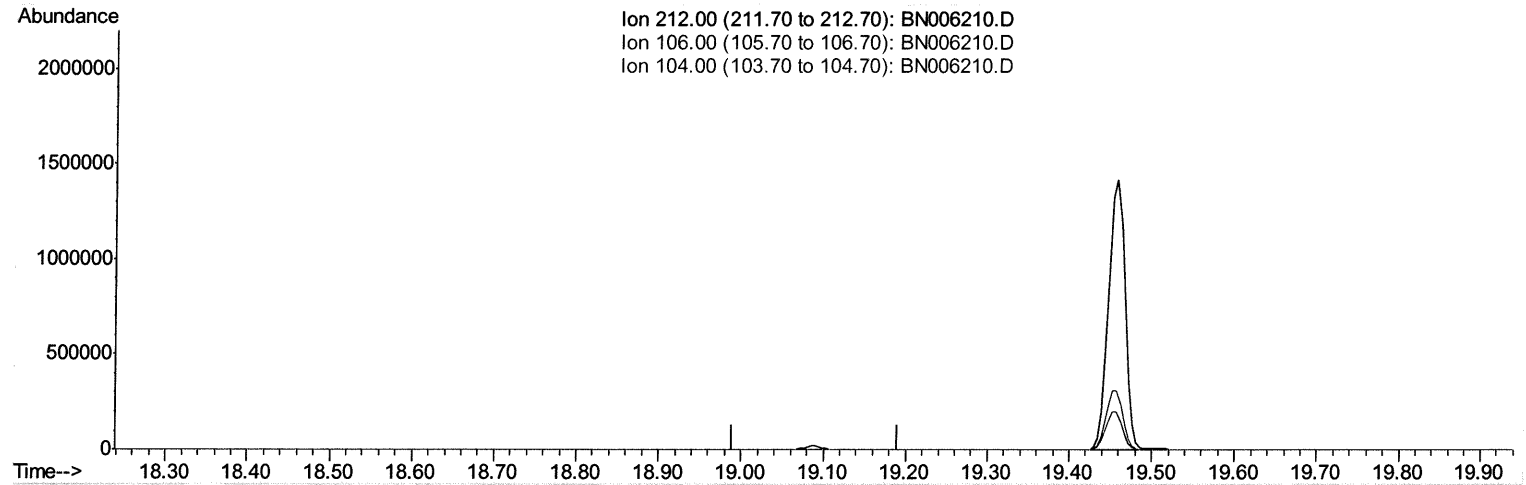

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:28:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

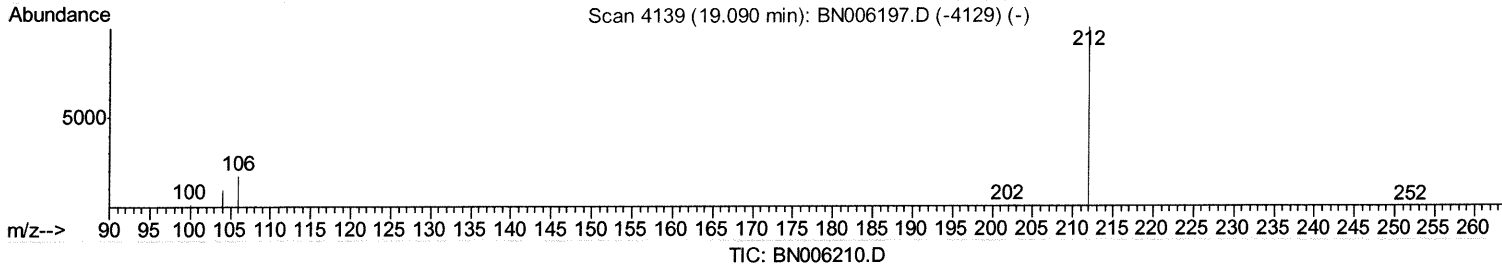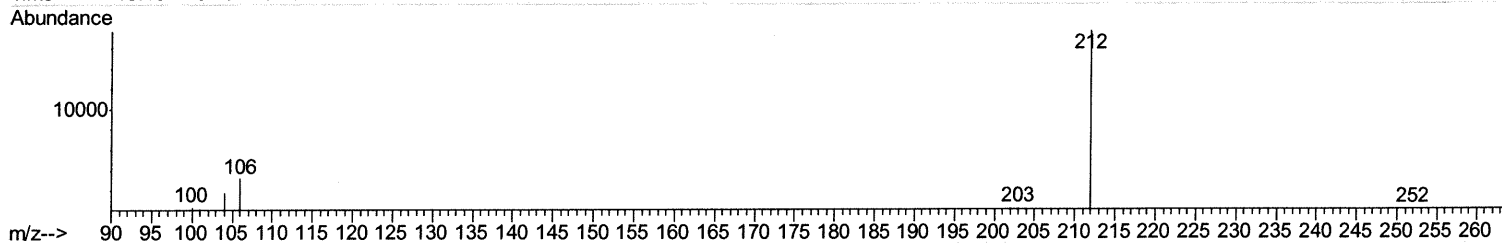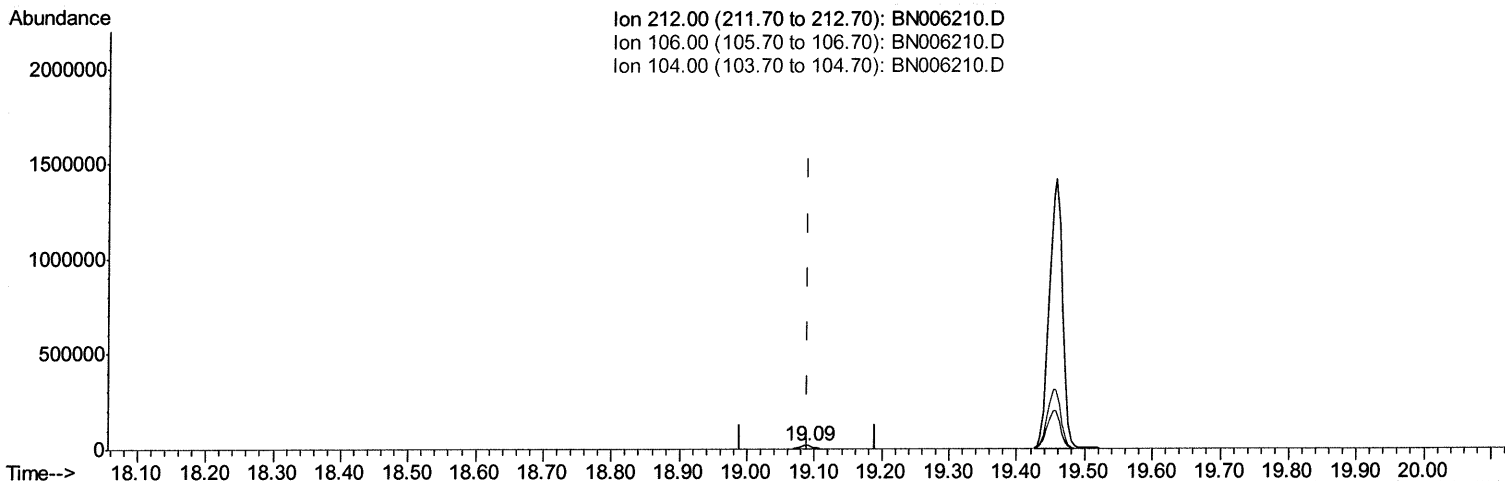

(14) Fluoranthene-d10 (SURR)

19.090min (-0.000) 0.41ng/ul m

JU
06/10/19

response 25034

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:28:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

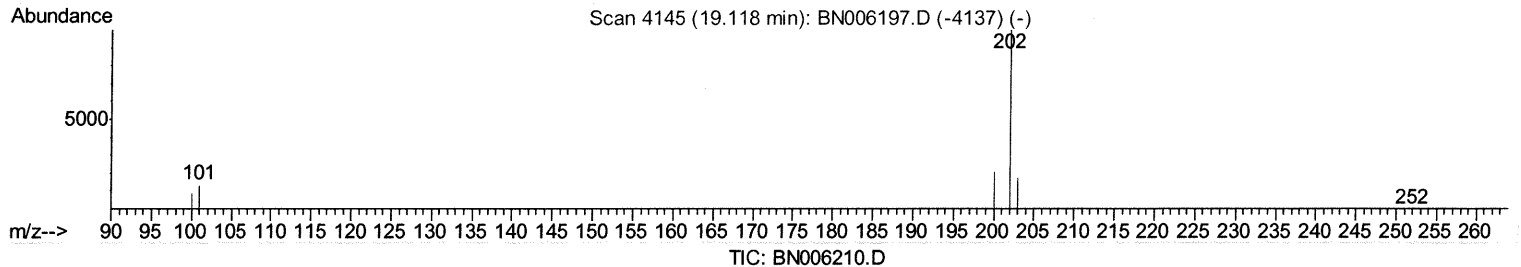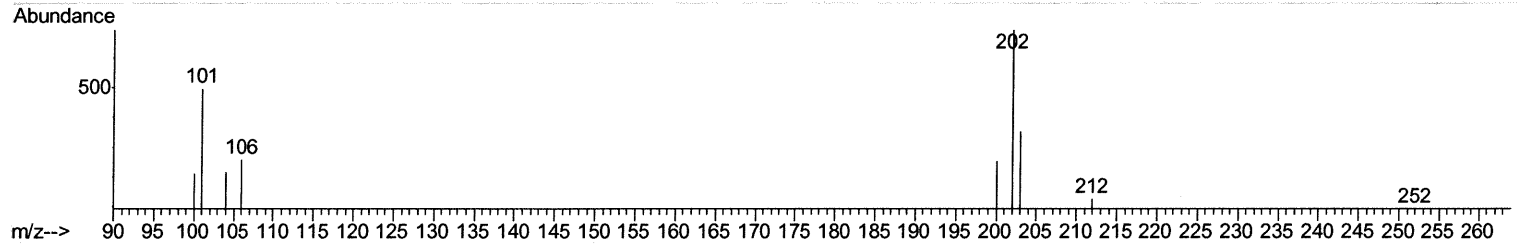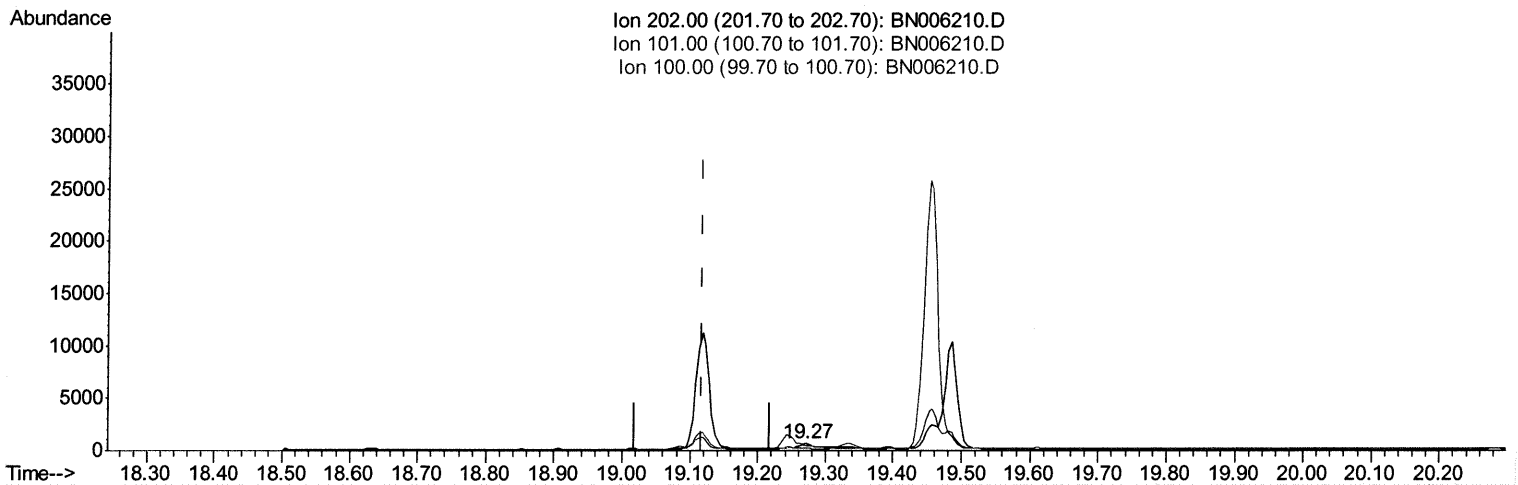

(15) Fluoranthene (C)

19.271min (+0.153) 0.01ng/ul

response 690

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	71.65#
100.00	8.70	30.22#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:28:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

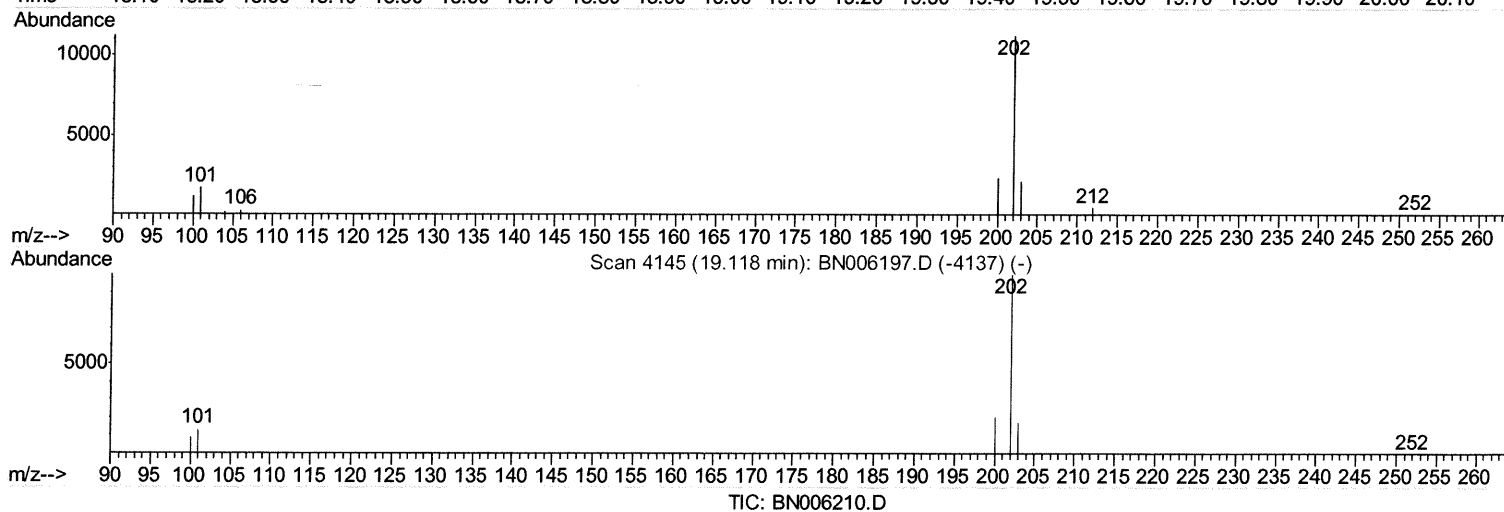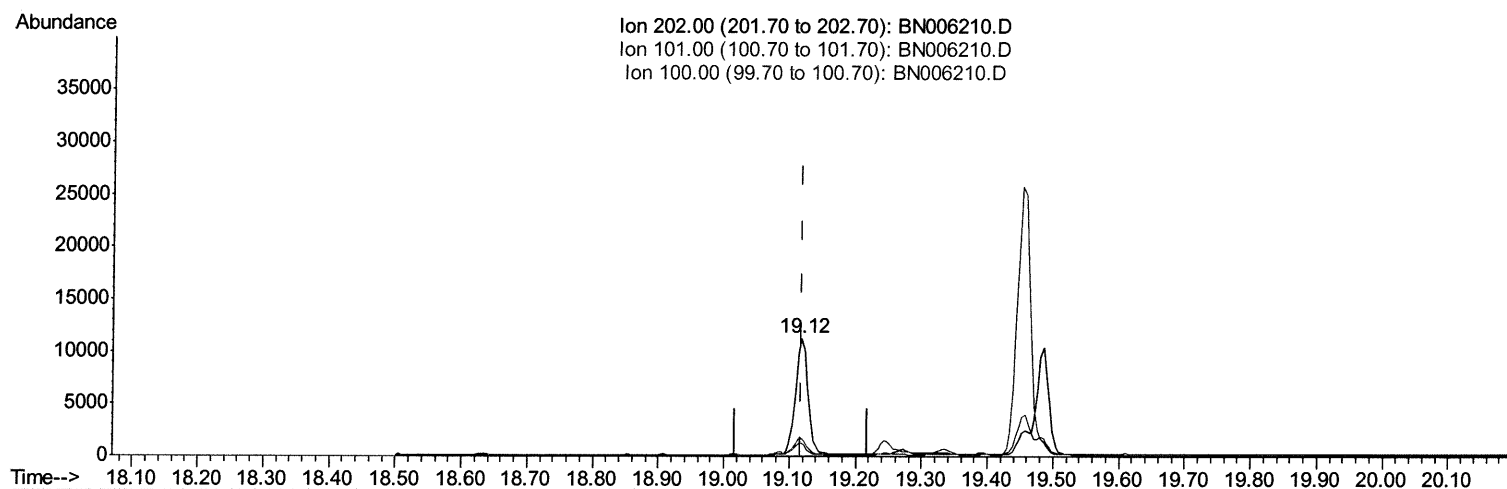

(15) Fluoranthene (C)

19.118min (-0.000) 0.19ng/ul m

JU
06/10/19

response 15303

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	15.48
100.00	8.70	11.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:28:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

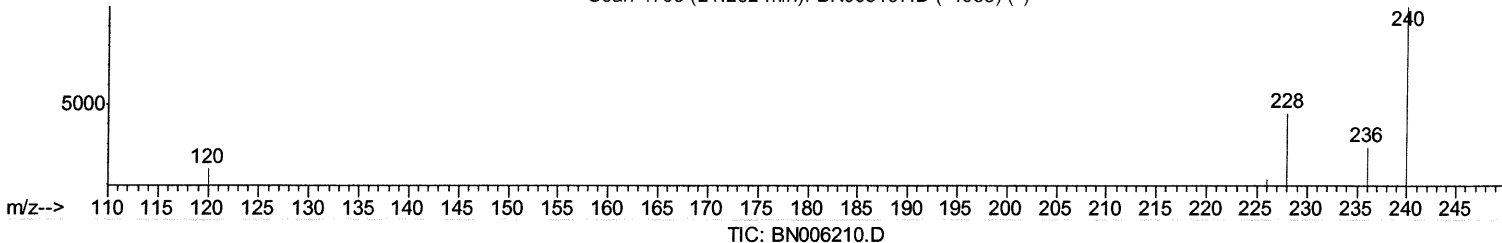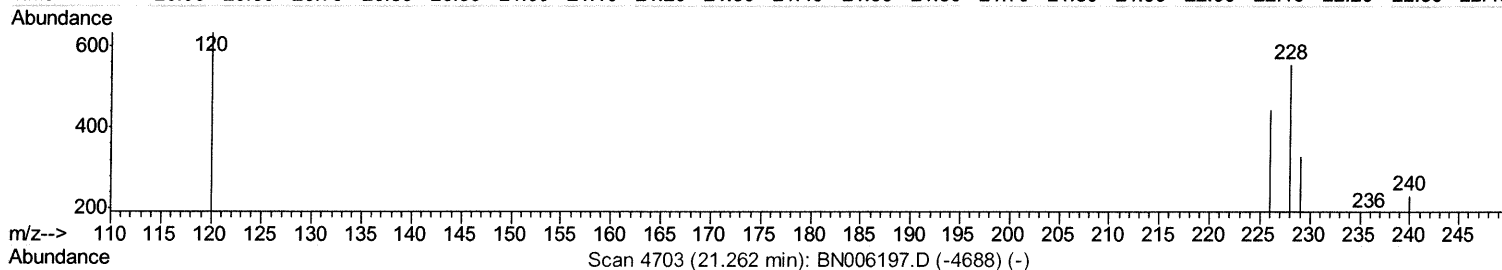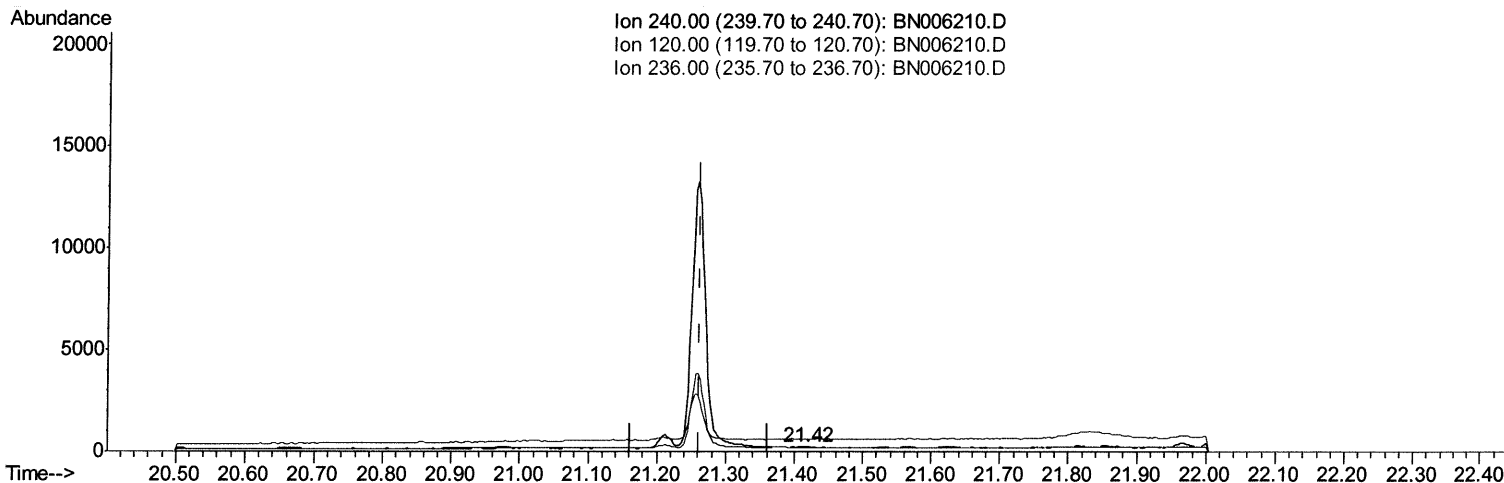

(16) Chrysene-d12 (I)

21.417min (+0.155) 0.40ng/ul

response 35

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	272.84#
236.00	30.10	82.76#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:28:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

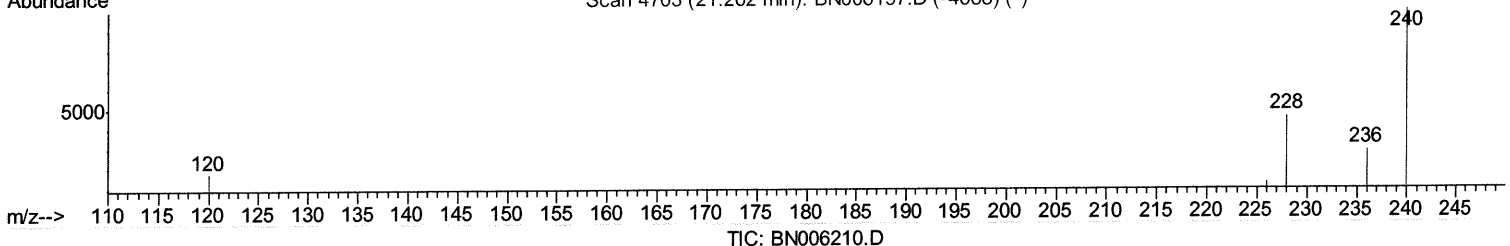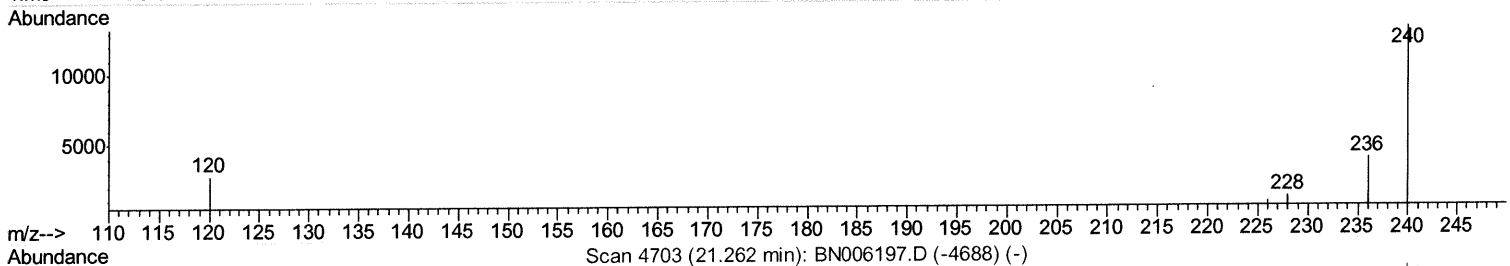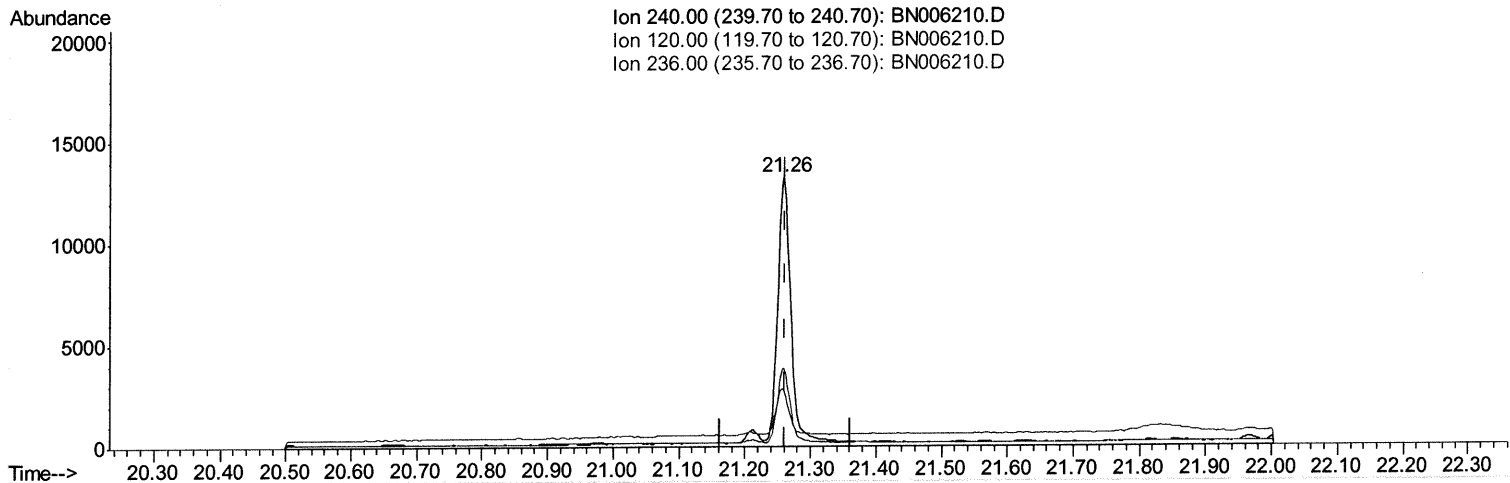

(16) Chrysene-d12 (I)

21.259min (-0.003) 0.40ng/ul m

JU
06/10/19

response 18285

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	21.12
236.00	30.10	29.26
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

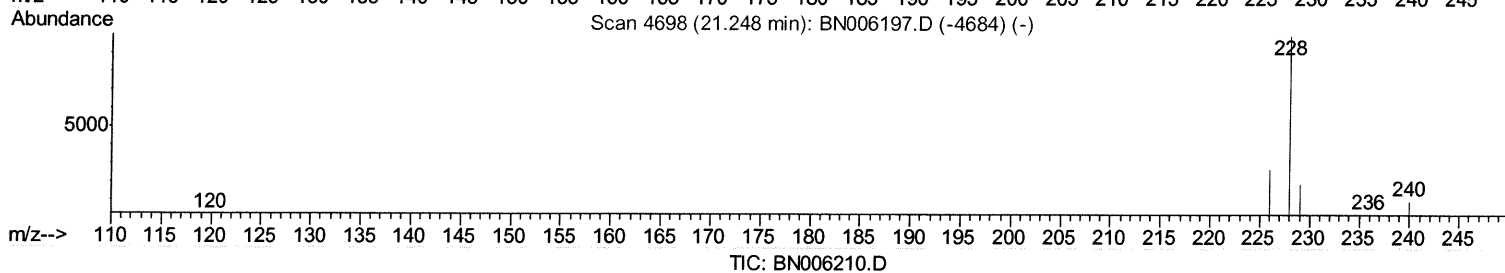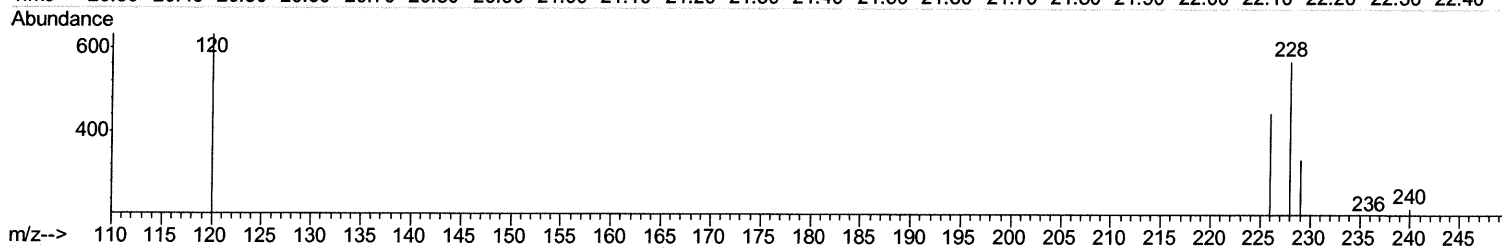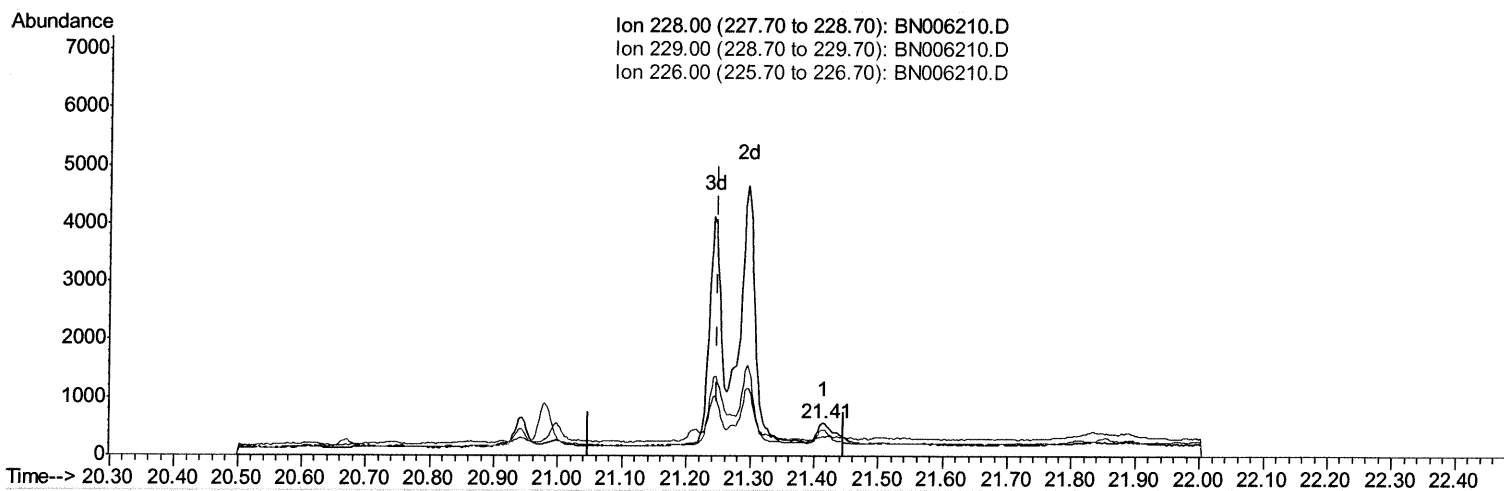

(18) Benzo(a)anthracene

21.414min (+0.166) 0.01ng/ul

response 679

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	58.77#
226.00	28.50	78.60#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

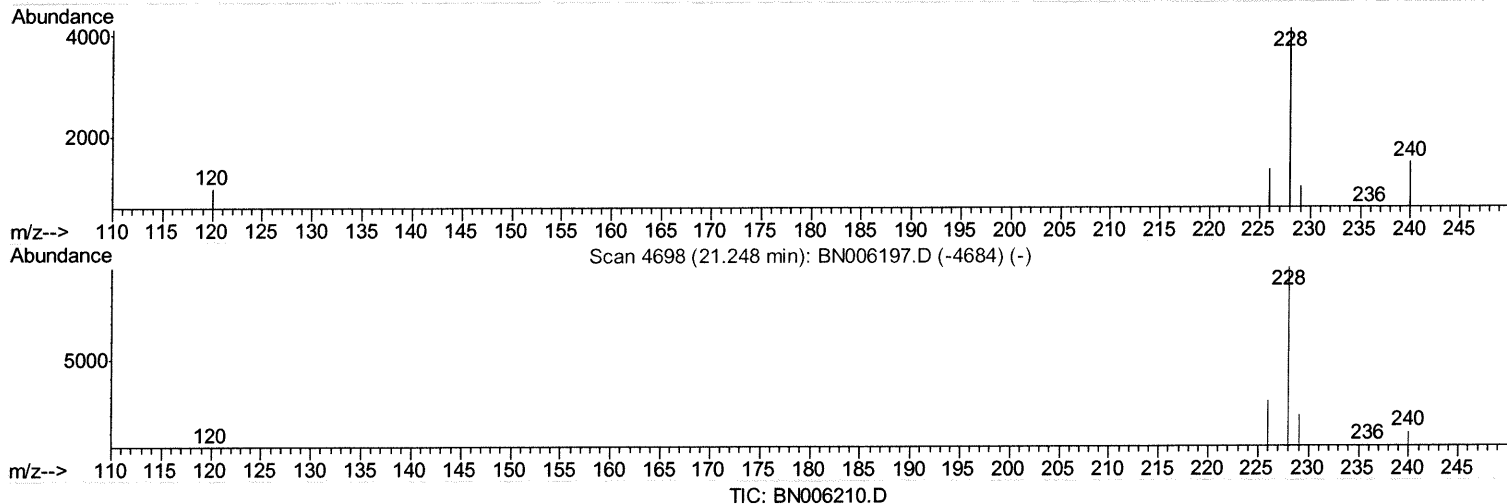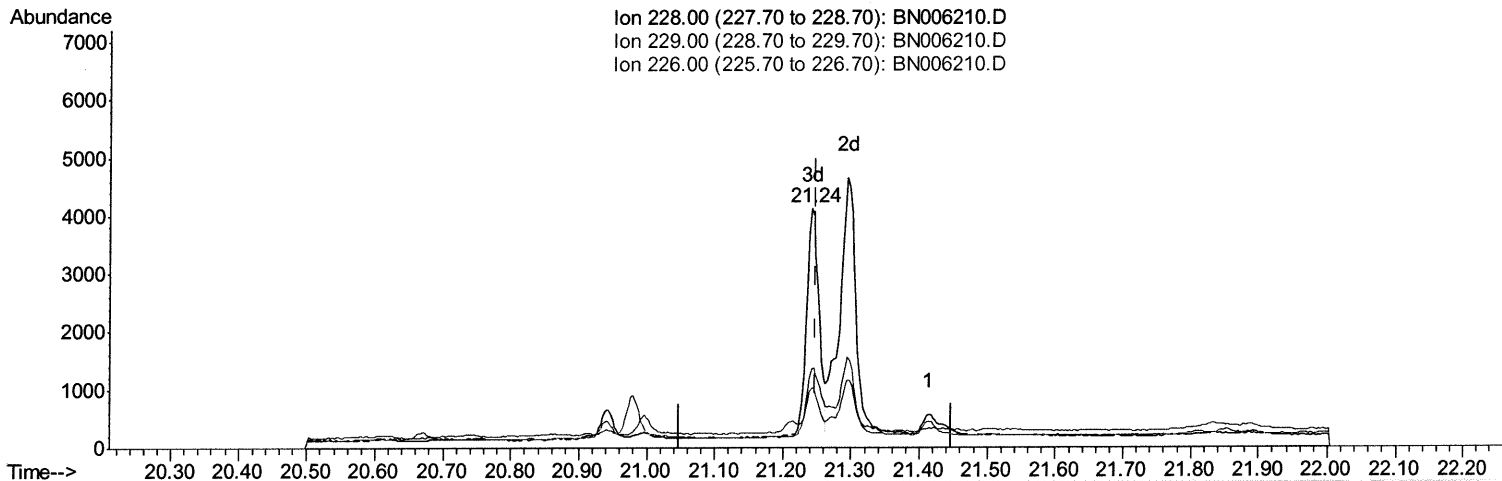

(18) Benzo(a)anthracene

21.242min (-0.006) 0.06ng/ul m *Ju 06/10/19*

response 4969

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	24.76#
226.00	28.50	32.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

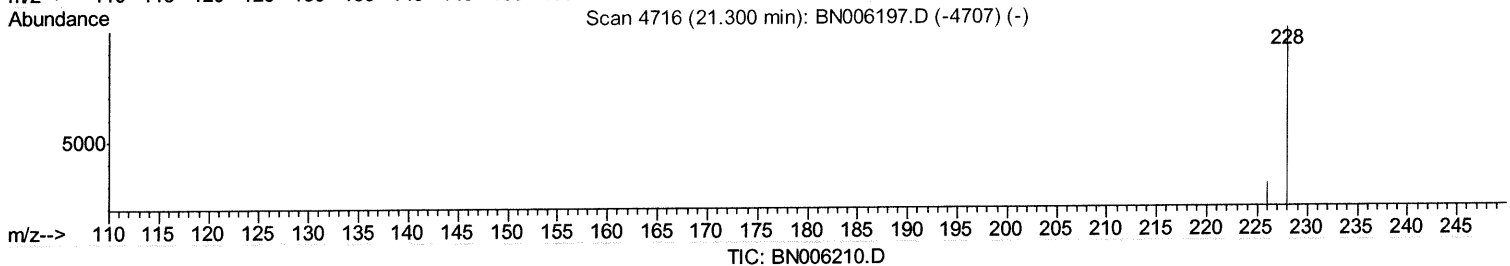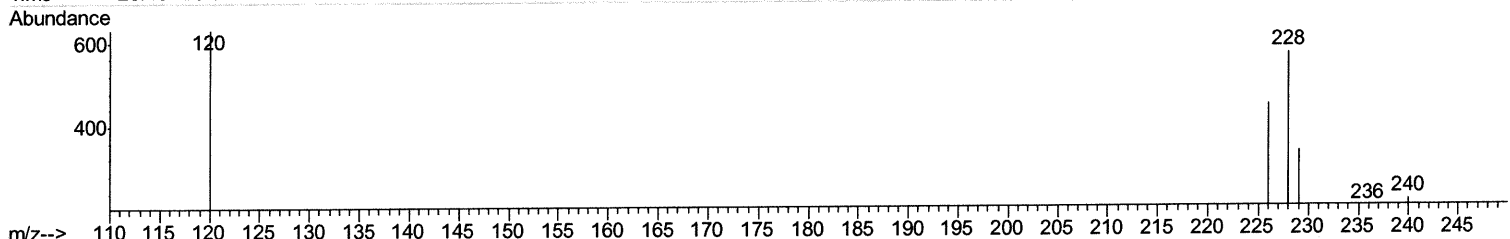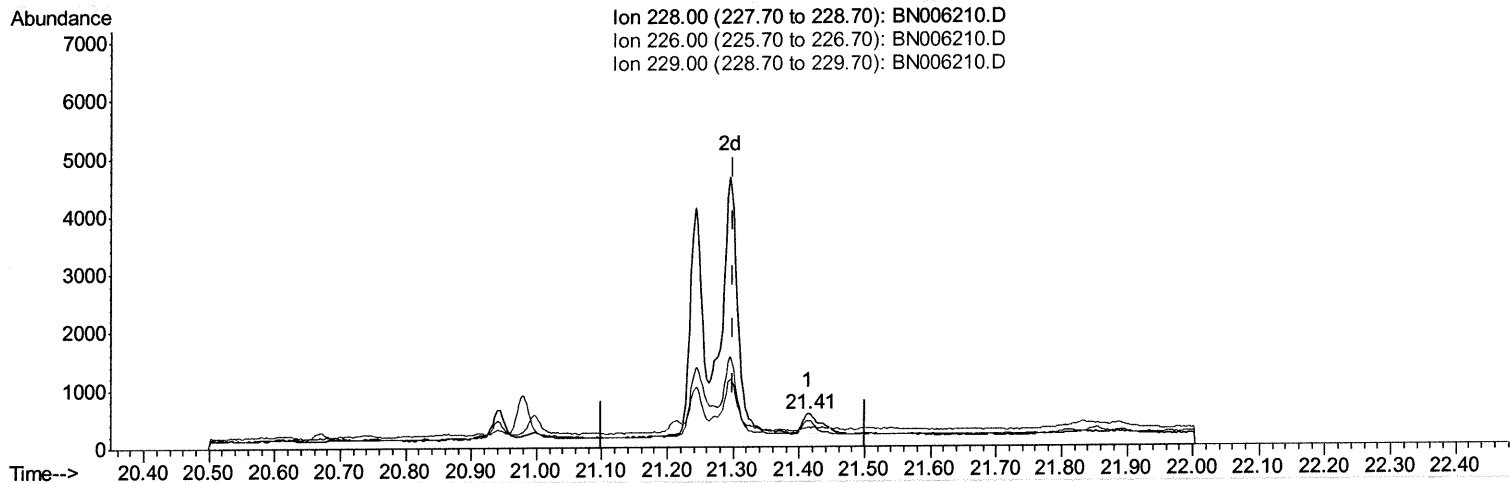

(19) Chrysene

21.414min (+0.114) 0.01ng/ul

response 679

Ion	Exp%	Act%
228.00	100	100
226.00	31.30	78.60#
229.00	20.40	58.77#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

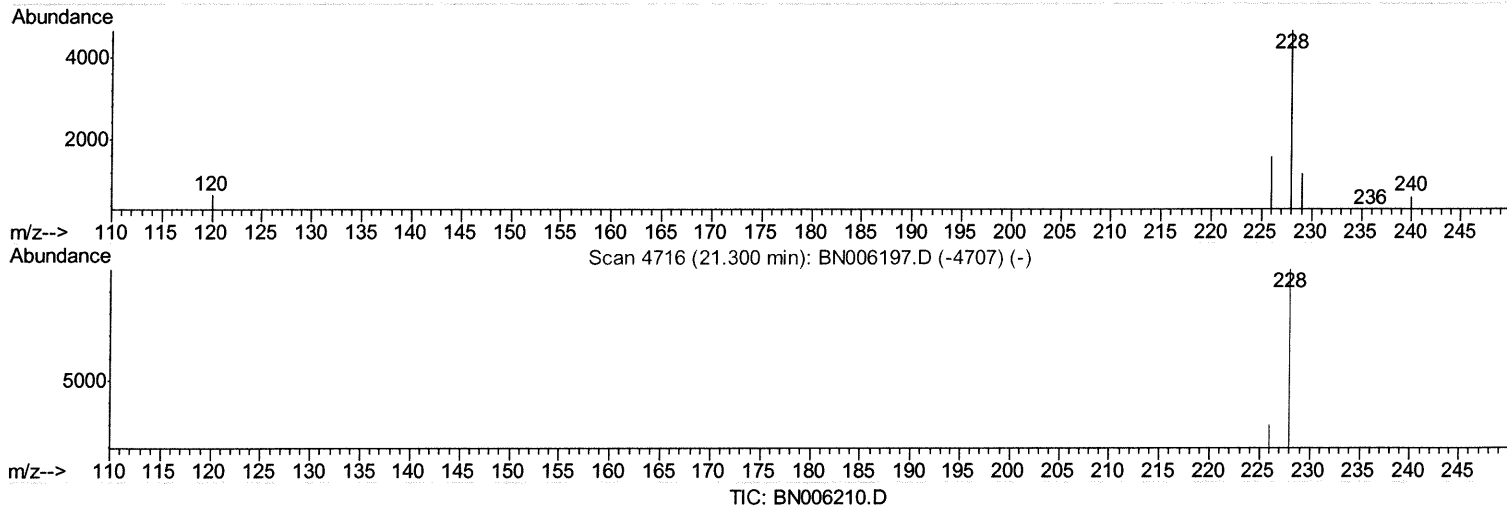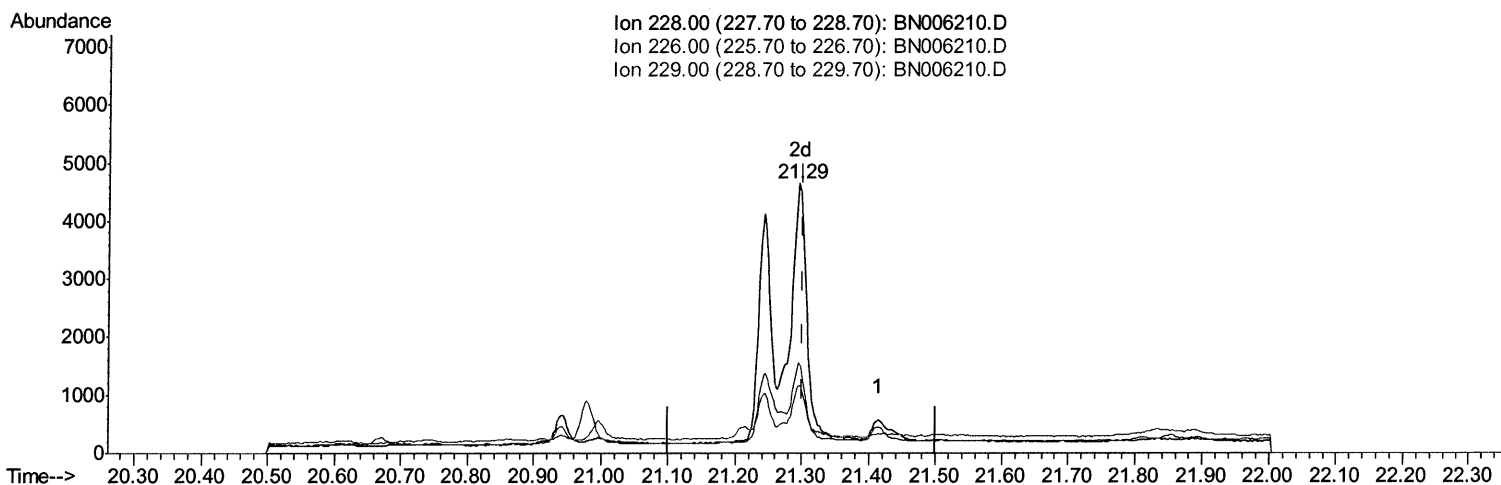

(19) Chrysene

21.294min (-0.006) 0.10ng/ul m ^{JU} 06/10/19

response 7601

Ion	Exp%	Act%
228.00	100	100
226.00	31.30	33.88
229.00	20.40	25.24#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A51E3


Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

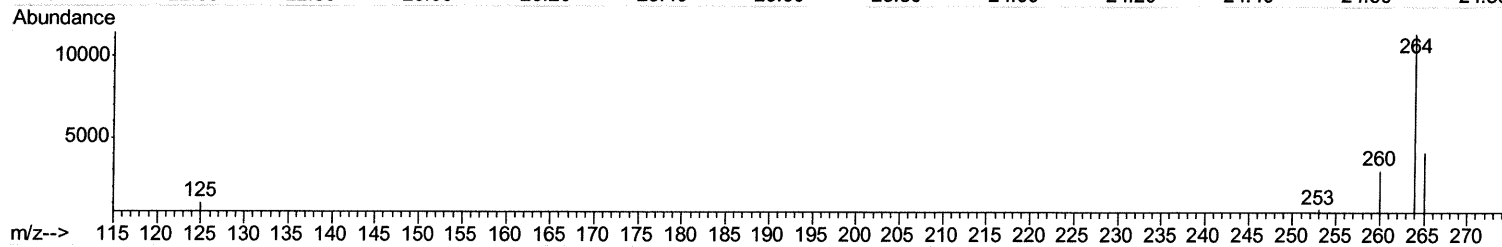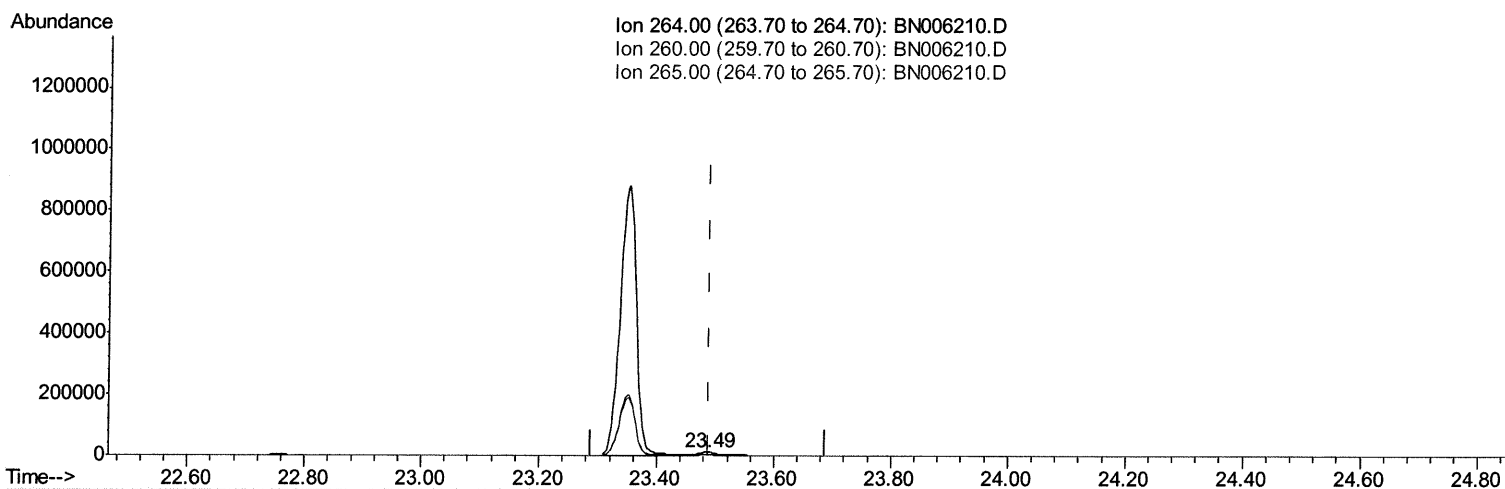

Scan 5465 (23.490 min): BN006197.D (-5445) (-)

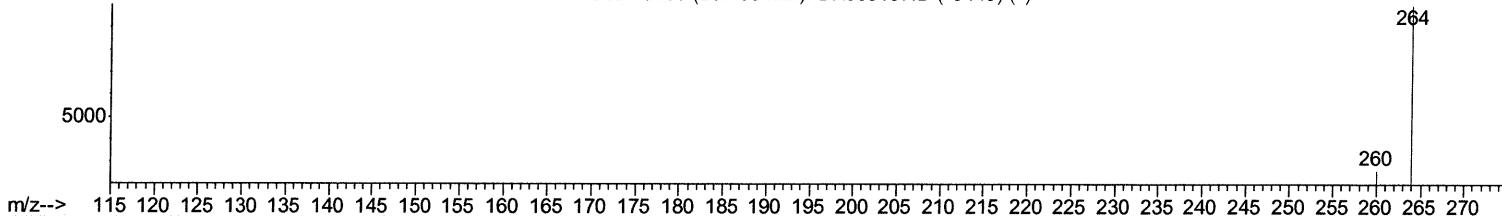

TIC: BN006210.D

(20) Perylene-d12 (I)

23.486min (-0.003) 0.40ng/ul

response 30037

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.45
265.00	44.70	36.51
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)



Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3


Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:29:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

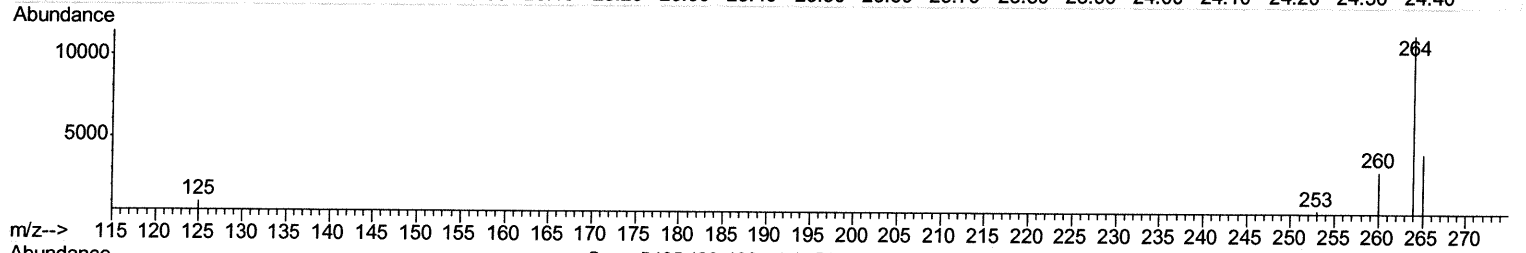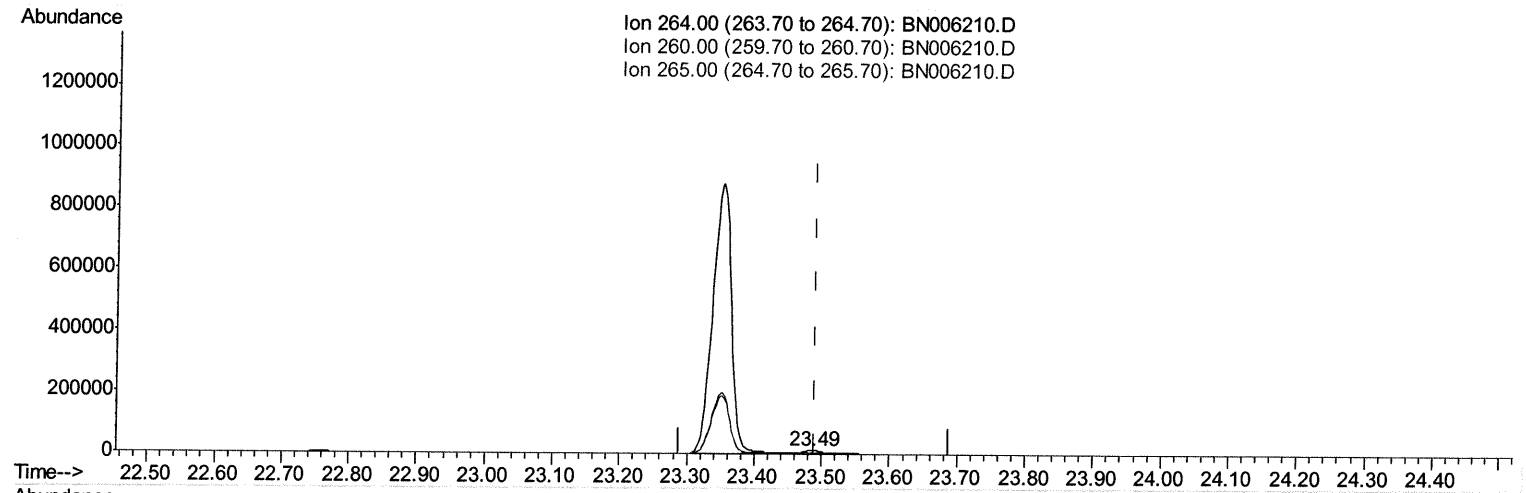

Scan 5465 (23.490 min): BN006197.D (-5445) (-)

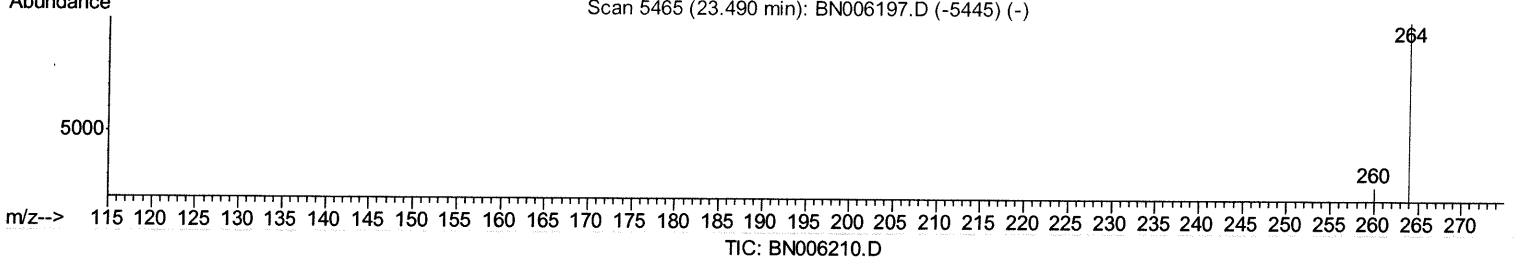

(20) Perylene-d12 (I)

23.486min (-0.003) 0.40ng/ul m

J0
06/10/19

response 14991

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.45
265.00	44.70	36.51
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:30:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

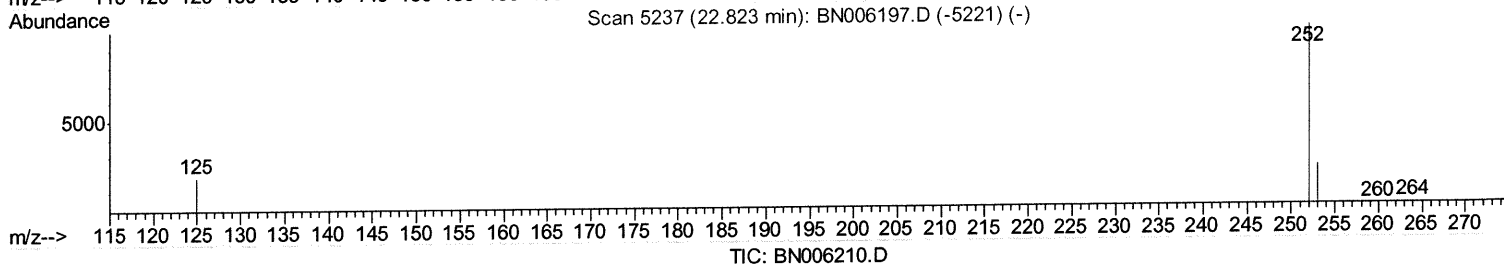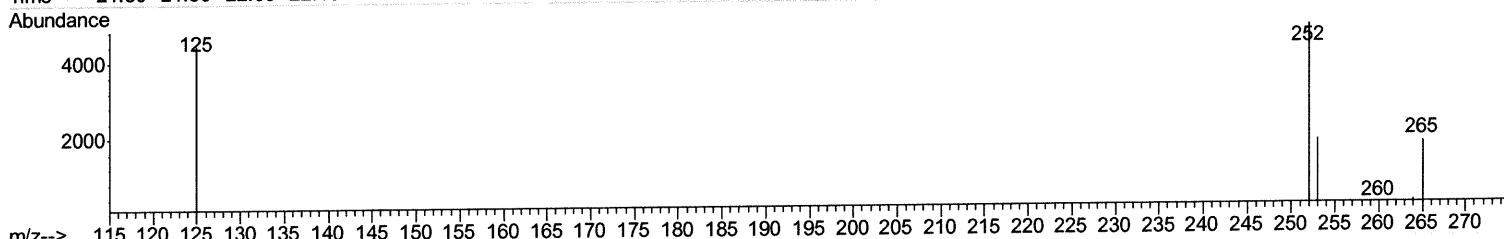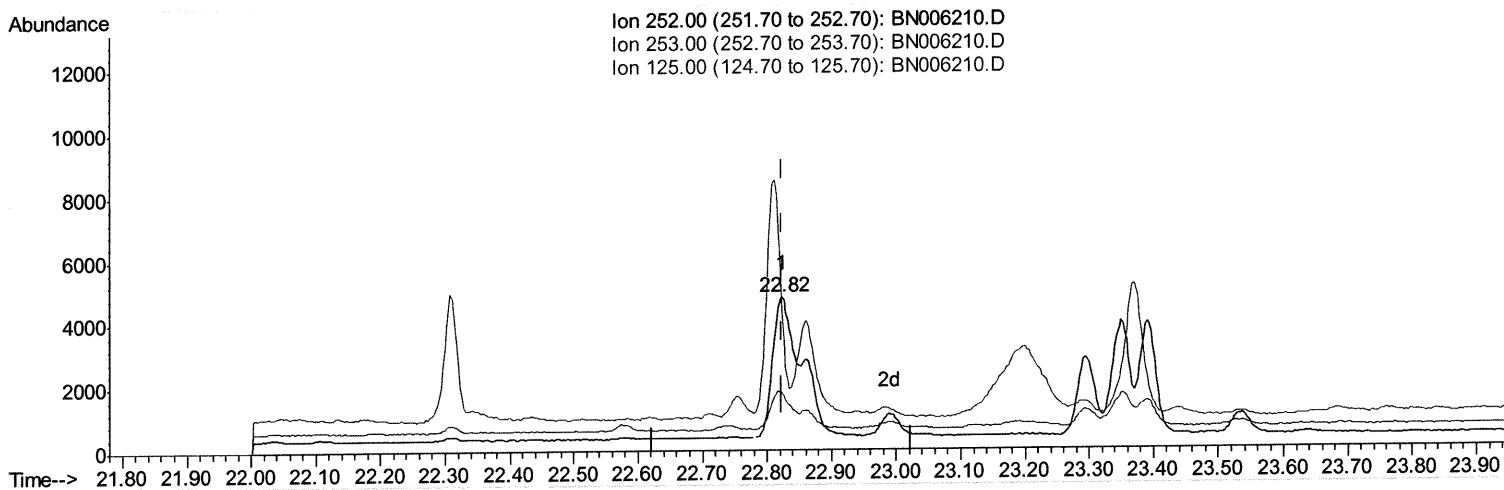

(21) Benzo(b)fluoranthene

22.823min (-0.000) 0.22ng/ul

response 13865

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	37.49
125.00	20.50	91.81#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:30:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

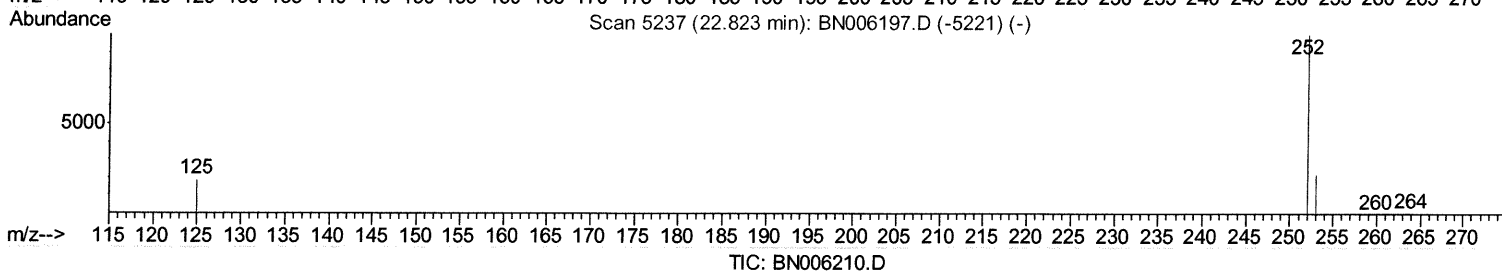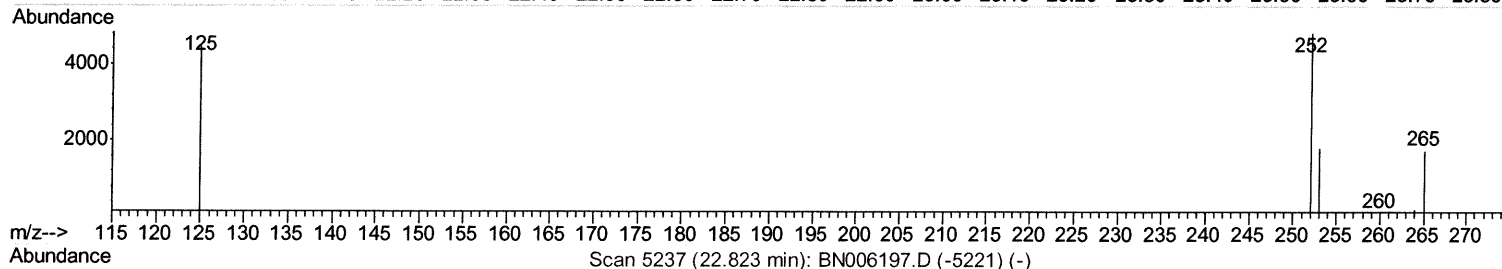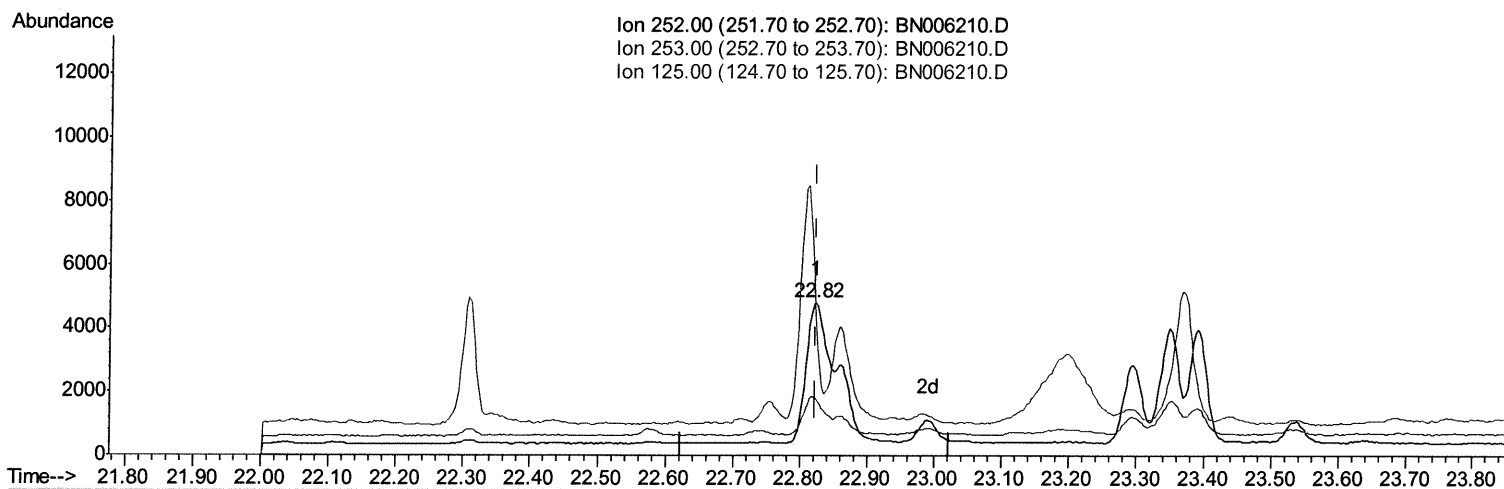

(21) Benzo(b)fluoranthene

22.823min (-0.000) 0.16ng/ul m *Jo* 06/10/19

response 10118

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	37.49
125.00	20.50	91.81#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:30:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

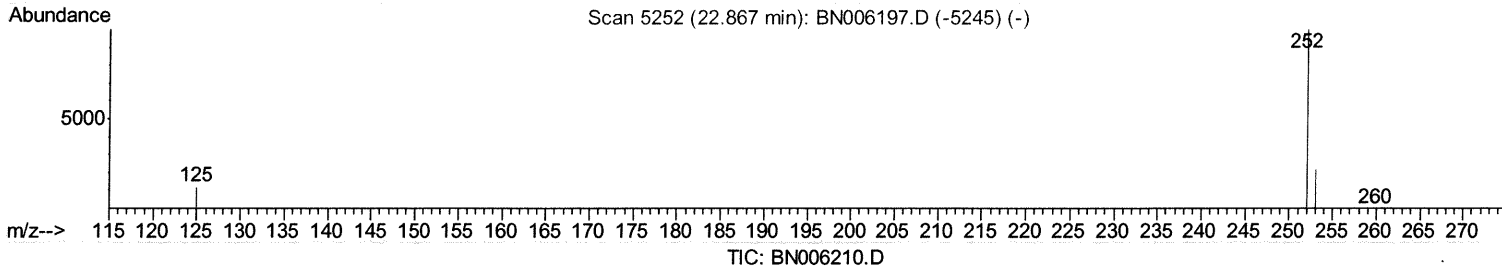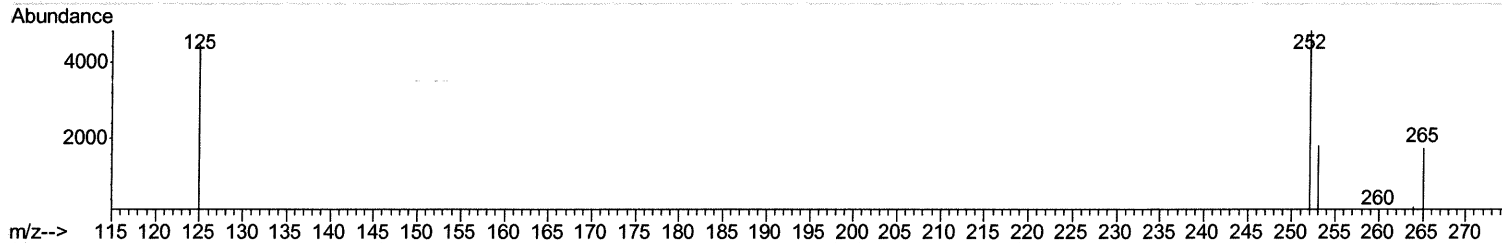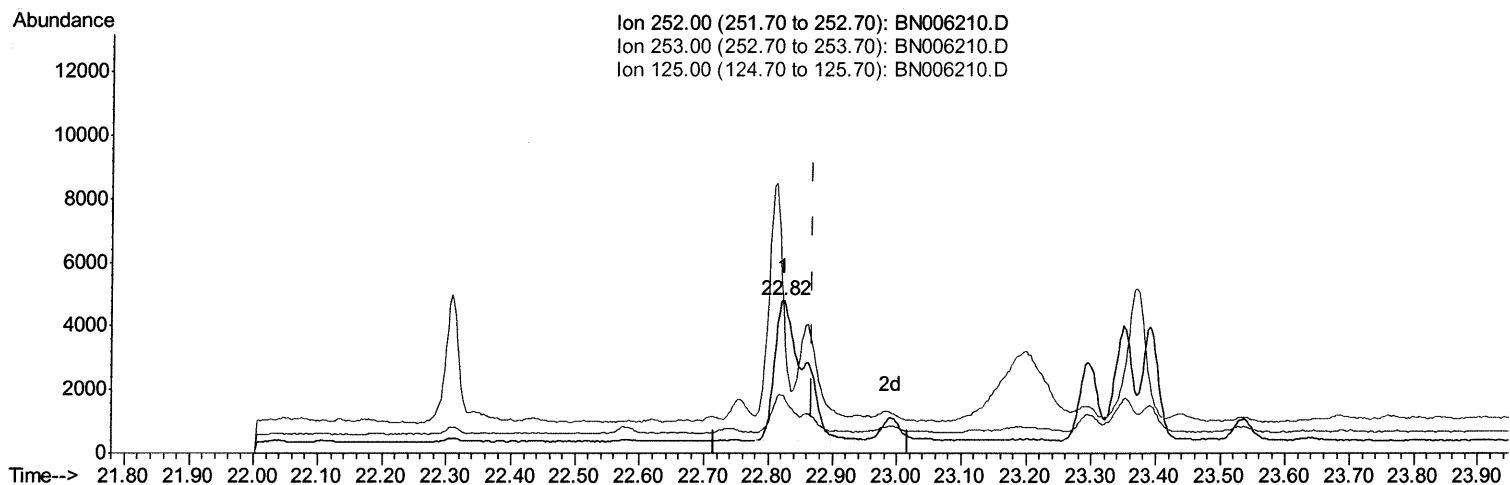

(22) Benzo(k)fluoranthene
22.823min (-0.044) 0.23ng/ul

response 13856

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	37.49#
125.00	17.90	91.81#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060819\
Quantitation Report (Qedit)




Data File : BN006210.D
Acq On : 09 Jun 2019 03:07
Operator : JU/SJ
Sample : K3017-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51E3

Manual Integrations
APPROVED

mohammad
6/11/2019 4:33:05 PM

Quant Time: Jun 09 06:30:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

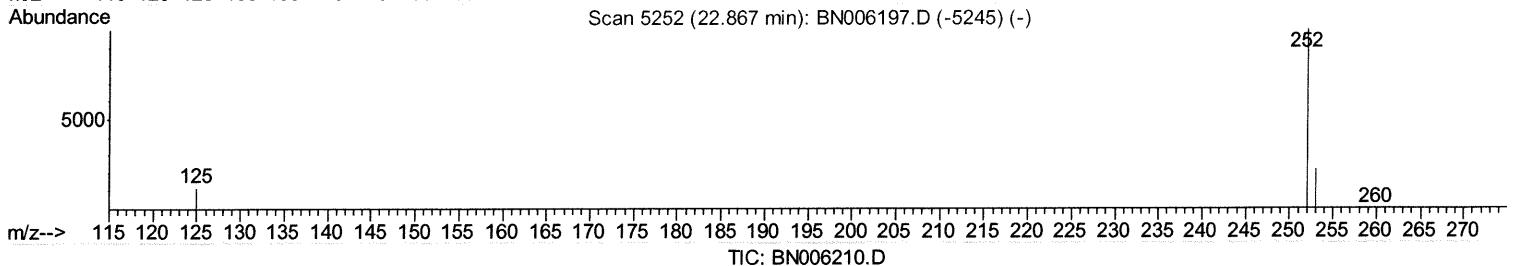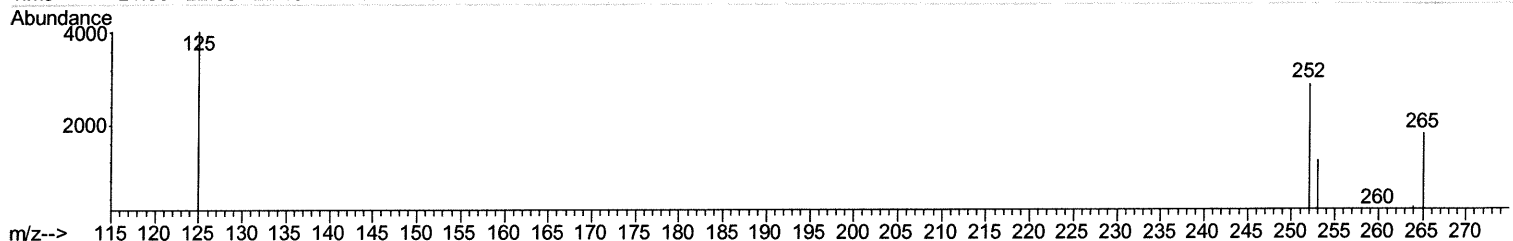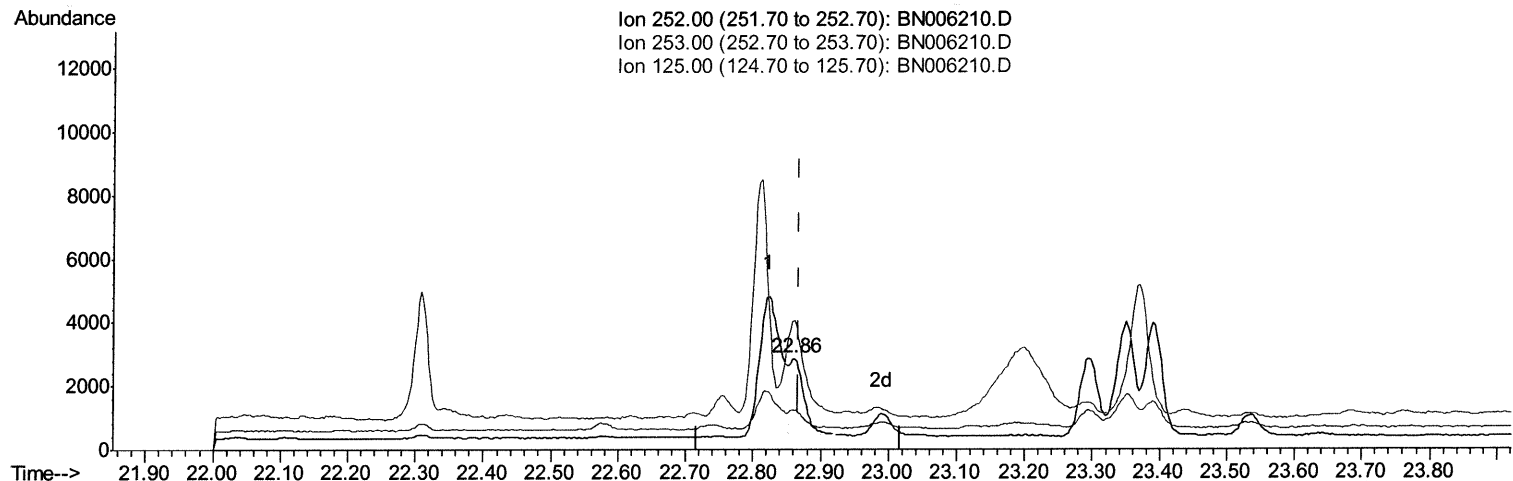

(22) Benzo(k)fluoranthene

22.861min (-0.006) 0.06ng/ul m

JU
06/10/19

response 3573

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	42.83#
125.00	17.90	140.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060819\
 Data File : BN006210.D
 Acq On : 09 Jun 2019 03:07
 Operator : JU/SJ
 Sample : K3017-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51E3

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:33:05 PM

Quant Time: Jun 10 02:40:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5702	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	22318	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	11993	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	22701m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	18285m>	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	14991m>	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.02	152	12364	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	25034m>	0.41	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.01	152	1608	0.024	ng/ul#	82
12) Phenanthrene	17.09	178	7021	0.096	ng/ul	96
15) Fluoranthene	19.12	202	15303m>	0.190	ng/ul	
17) Pyrene	19.49	202	15512	0.161	ng/ul	97
18) Benzo(a)anthracene	21.24	228	4969m>	0.061	ng/ul	
19) Chrysene	21.29	228	7601m>	0.100	ng/ul	
21) Benzo(b)fluoranthene	22.82	252	10118m>	0.162	ng/ul	
22) Benzo(k)fluoranthene	22.86	252	3573m>	0.059	ng/ul	
23) Benzo(a)pyrene	23.39	252	5918	0.102	ng/ul#	59
24) Indeno(1,2,3-cd)pyrene	25.72	276	4761	0.076	ng/ul#	83
26) Benzo(g,h,i)perylene	26.41	276	4742	0.090	ng/ul#	81

JU 06/10/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed