

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060824\
 Data File : BN031852.D
 Acq On : 08 Jun 2024 10:36
 Operator : MA/JU
 Sample : PB161227BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	29	34	42	rVB	125926	180215	1.69%	0.130%
2	3.587	98	102	124	rBV	1754556	2683607	25.16%	1.941%
3	3.905	152	156	162	rVB	24350	36294	0.34%	0.026%
4	6.681	621	628	633	rBV9	7607	17061	0.16%	0.012%
5	6.846	648	656	667	rBV	2317040	3726637	34.93%	2.695%
6	7.010	673	684	694	rBV	1819753	2886977	27.06%	2.088%
7	7.205	709	717	729	rBV	2386694	3829553	35.90%	2.770%
8	7.669	789	796	809	rVB	2171024	3447797	32.32%	2.494%
9	8.381	909	917	931	rBV	2858068	4811933	45.11%	3.480%
10	8.828	985	993	1004	rBV	2235633	3671530	34.42%	2.655%
11	9.546	1106	1115	1126	rBV	1837153	3104934	29.10%	2.246%
12	10.075	1197	1205	1224	rBV	2742394	4825622	45.23%	3.490%
13	10.451	1261	1269	1280	rBV	3231426	5520147	51.74%	3.992%
14	10.598	1286	1294	1309	rBV	2912355	5031809	47.17%	3.639%
15	11.251	1401	1405	1409	rBV6	8760	16638	0.16%	0.012%
16	12.045	1535	1540	1552	rVB	54689	98436	0.92%	0.071%
17	13.275	1746	1749	1757	rVB3	7701	13706	0.13%	0.010%
18	13.728	1819	1826	1837	rBV	4485898	6644219	62.28%	4.805%
19	14.010	1865	1874	1885	rBV	5465350	8509875	79.77%	6.155%
20	14.316	1918	1926	1933	rBV	5080051	7580348	71.06%	5.482%
21	14.428	1940	1945	1951	rVB10	6141	12022	0.11%	0.009%
22	14.528	1955	1962	1982	rBV	2237804	3618086	33.92%	2.617%
23	15.310	2088	2095	2105	rBV	6849189	10102960	94.70%	7.307%
24	15.439	2110	2117	2130	rVV	1882050	2638432	24.73%	1.908%
25	15.545	2131	2135	2145	rVB	41079	75378	0.71%	0.055%
26	16.004	2208	2213	2217	rBV8	6431	11311	0.11%	0.008%
27	16.098	2221	2229	2233	rBV6	8749	15808	0.15%	0.011%
28	16.745	2334	2339	2342	rVB2	10079	14003	0.13%	0.010%
29	16.845	2350	2356	2362	rBV2	17588	32557	0.31%	0.024%
30	17.063	2386	2393	2403	rBV	5848483	8691984	81.48%	6.286%
31	17.163	2403	2410	2422	rVV2	7293617	10668081	100.00%	7.715%
32	17.328	2433	2438	2449	rBV3	45094	112509	1.05%	0.081%
33	17.439	2455	2457	2463	rVB2	12525	19357	0.18%	0.014%
34	17.963	2543	2546	2551	rBV7	12518	19242	0.18%	0.014%
35	18.298	2598	2603	2608	rBV4	33114	59267	0.56%	0.043%
36	19.022	2722	2726	2733	rBV2	104514	174427	1.64%	0.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060824\
Data File : BN031852.D
Acq On : 08 Jun 2024 10:36
Operator : MA/JU
Sample : PB161227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.098	2734	2739	2744	rVB	93623	138027	1.29%	0.100%
38	19.398	2787	2790	2794	rBV3	31772	40967	0.38%	0.030%
39	19.463	2795	2801	2809	rBV	7489832	10499621	98.42%	7.594%
40	21.298	3108	3113	3122	rVB2	4733843	7003336	65.65%	5.065%
41	24.039	3570	3579	3591	rVB	3875356	9670048	90.64%	6.994%
42	24.239	3604	3613	3625	rBV	3135154	8014844	75.13%	5.797%




Sum of corrected areas: 138269605

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060824\
Data File : BN031852.D
Acq On : 08 Jun 2024 10:36
Operator : MA/JU
Sample : PB161227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

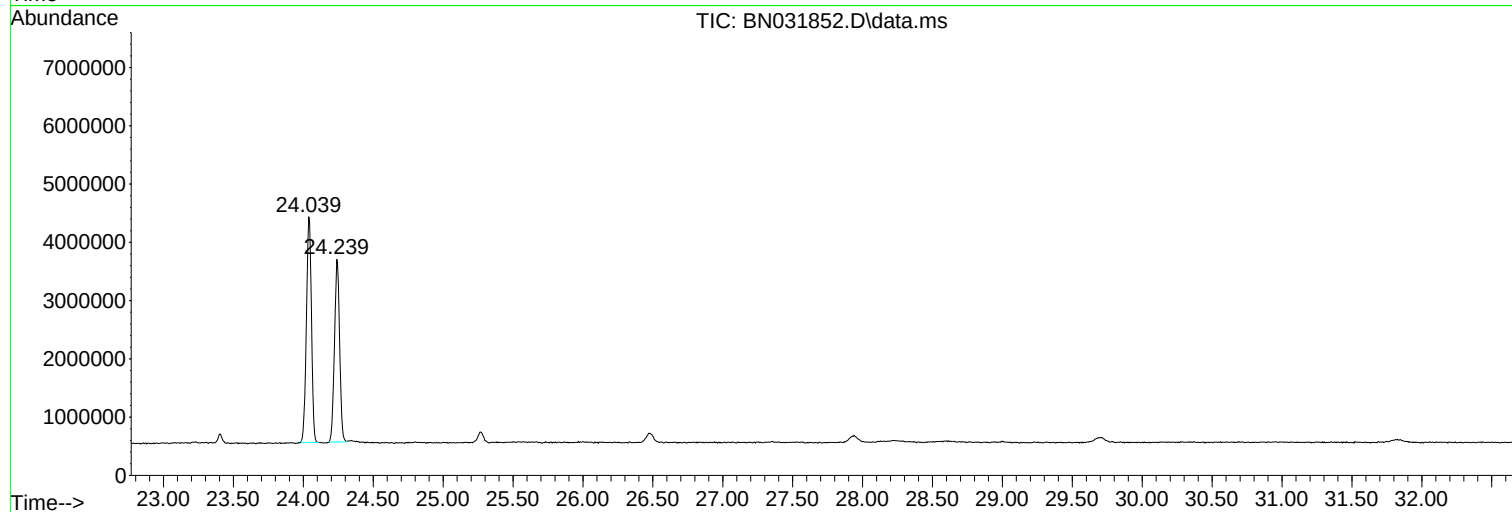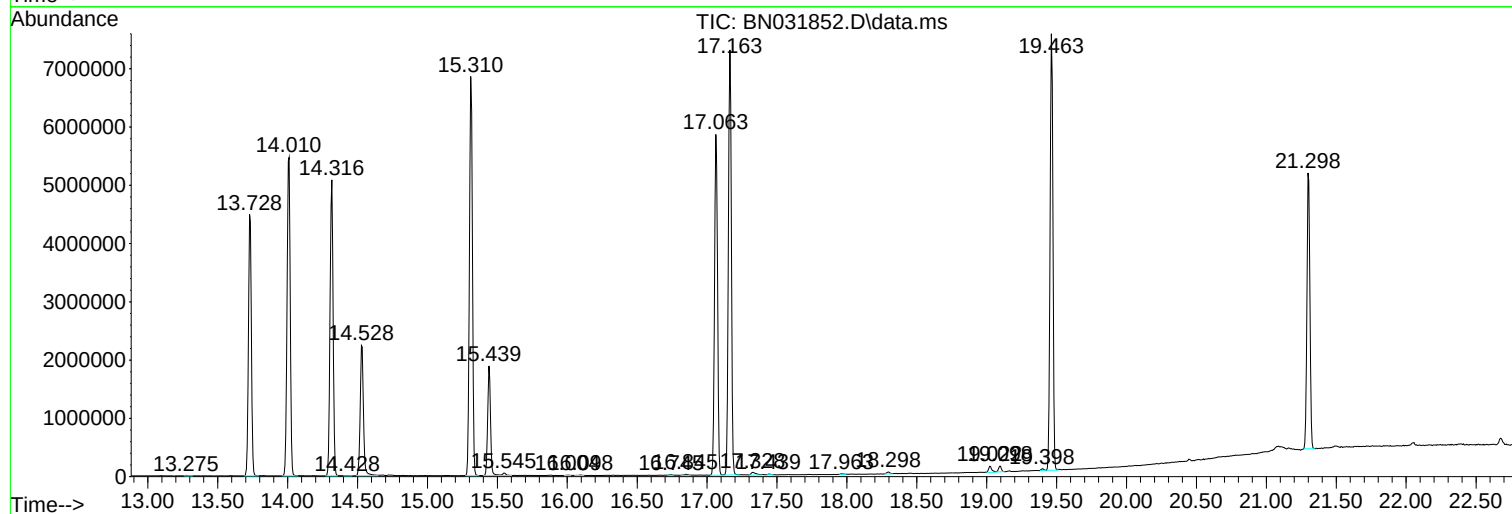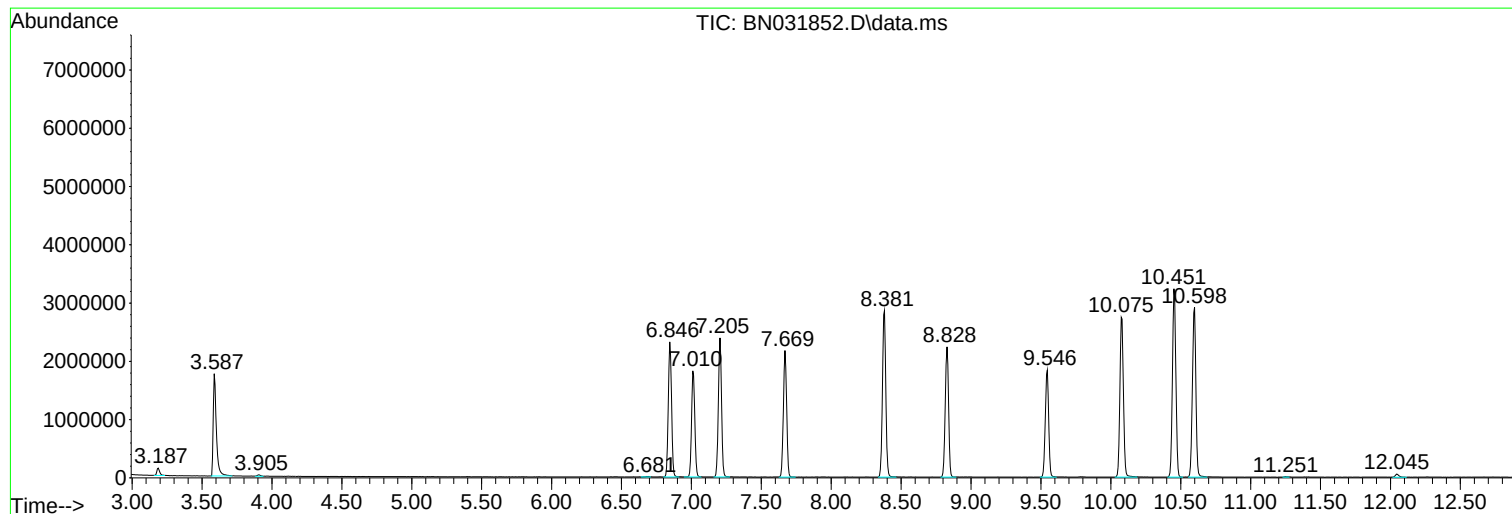

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060824\
Data File : BN031852.D
Acq On : 08 Jun 2024 10:36
Operator : MA/JU
Sample : PB161227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060824\
Data File : BN031852.D
Acq On : 08 Jun 2024 10:36
Operator : MA/JU
Sample : PB161227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc