

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006231.D
 Acq On : 10 Jun 2019 20:01
 Operator : JU/SJ
 Sample : K3017-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 11 00:19:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3774	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14578	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	7615	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	892901	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.35	264	792775	0.40	ng/ul	-0.13
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	5051	0.23	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
7) Acenaphthylene	14.01	152	1299	0.031	ng/ul#	82
8) Acenaphthene	14.36	153	1638	0.056	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006231.D
Acq On : 10 Jun 2019 20:01
Operator : JU/SJ
Sample : K3017-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 11 00:19:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

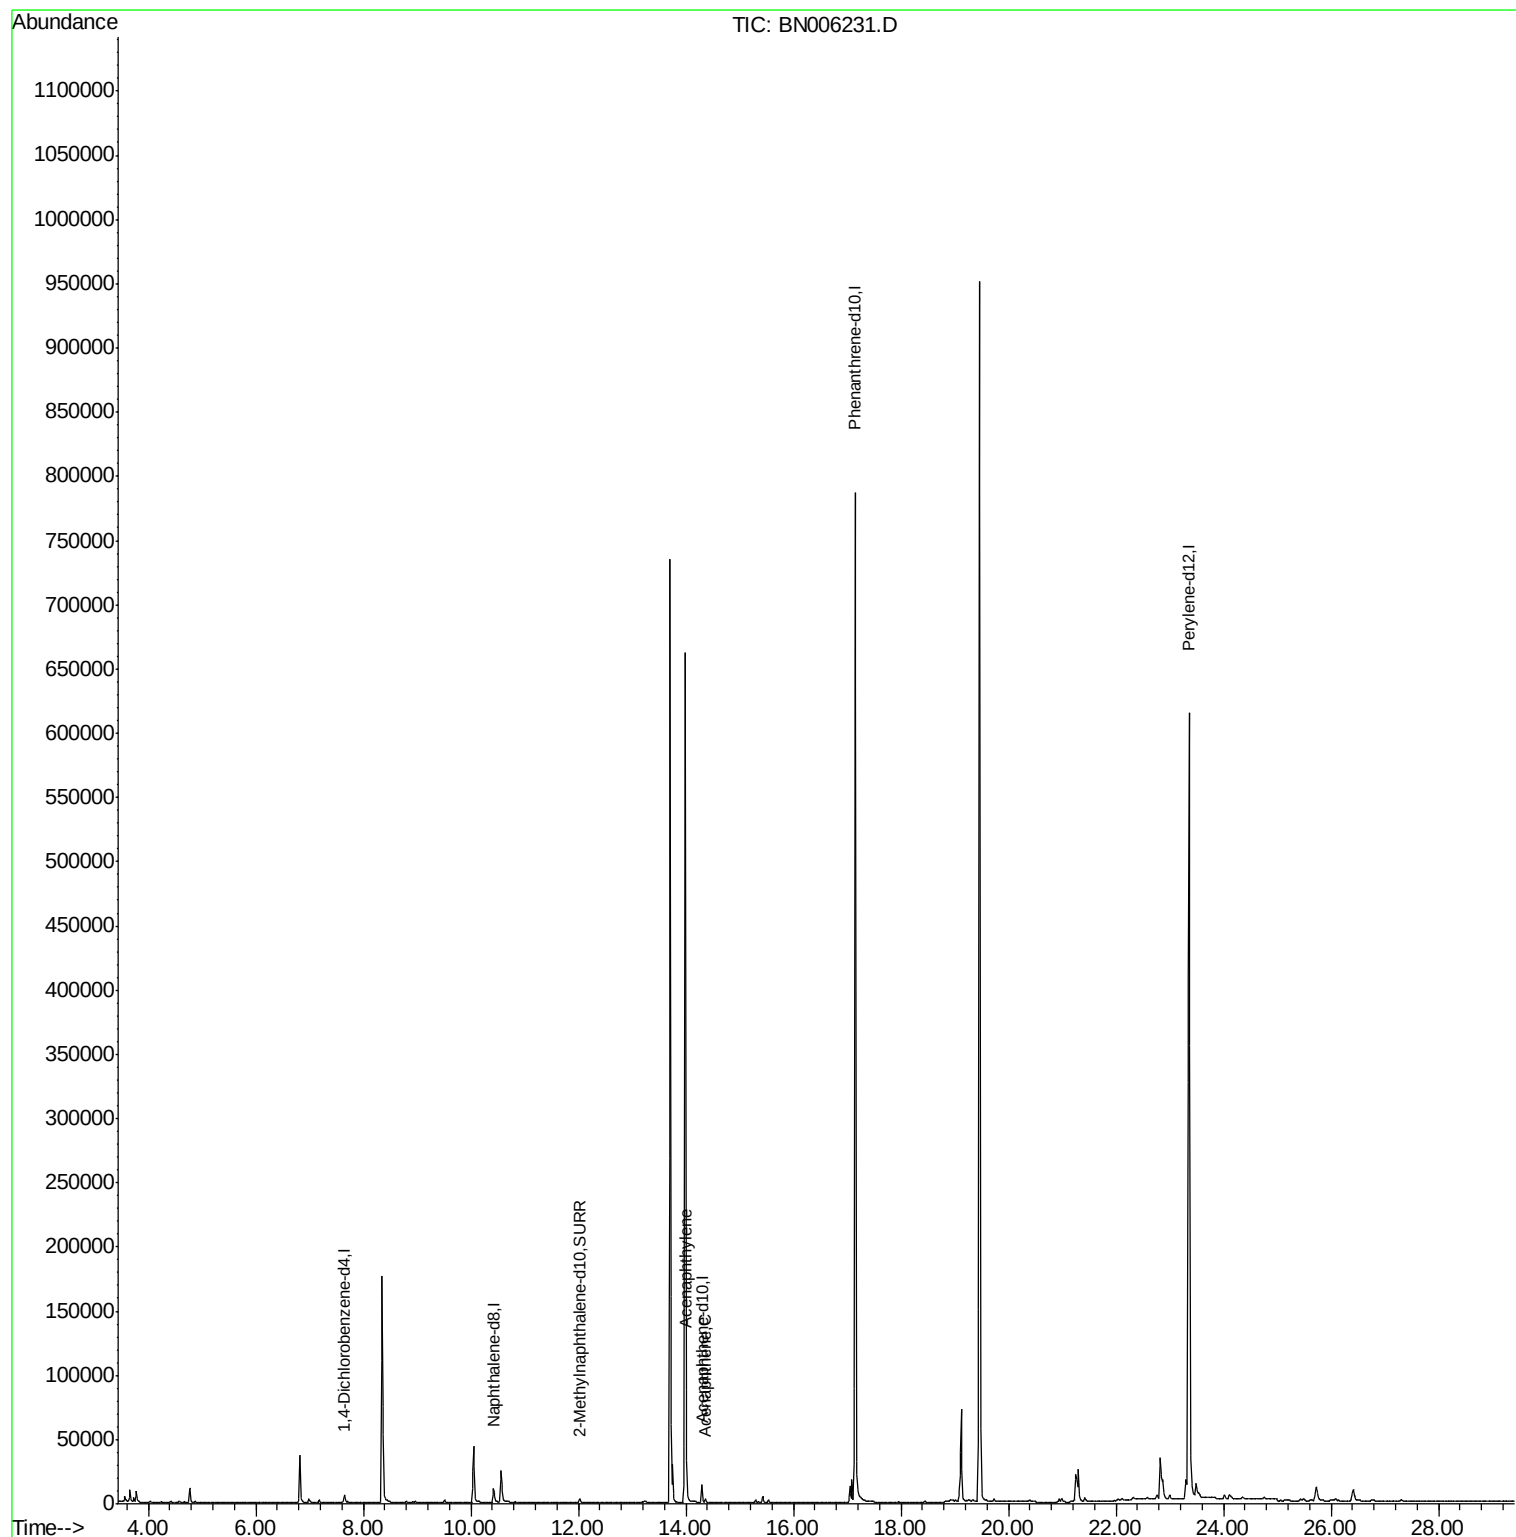

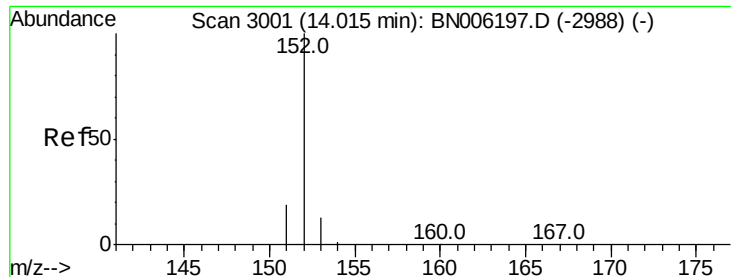

#7

Acenaphthylene

Concen: 0.031 ng/ul

RT: 14.01 min Scan# 3001

Delta R.T. -0.00 min

Lab File: BN006231.D

Acq: 10 Jun 2019 20:01

Instrument :

BNA_N

ClientSampleId :


Tot Ion:152 Resp: 1299

Ion Ratio Lower Upper

152 100

151 27.0 15.8 23.8#



153 22.2 10.8 16.2#

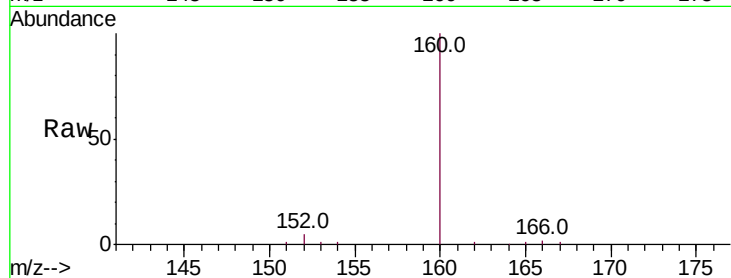


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

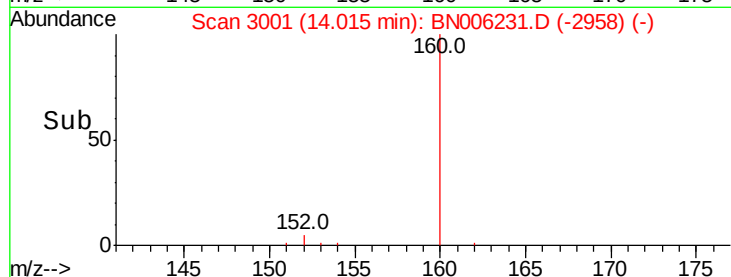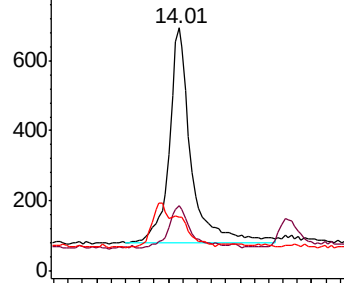

Time-->

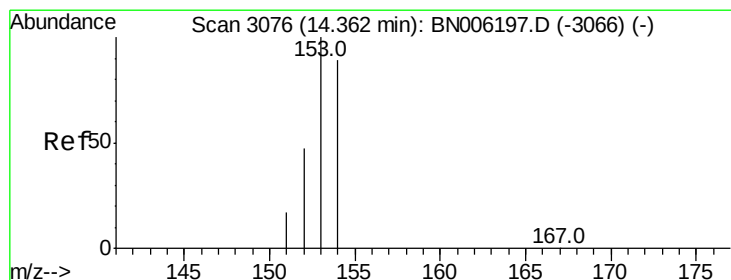

#8

Acenaphthene

Concen: 0.056 ng/ul

RT: 14.36 min Scan# 3075

Delta R.T. -0.00 min

Lab File: BN006231.D

Acq: 10 Jun 2019 20:01


Tgt Ion:153 Resp: 1638

Ion Ratio Lower Upper

153 100

152 51.7 39.1 58.7



154 87.6 71.1 106.7

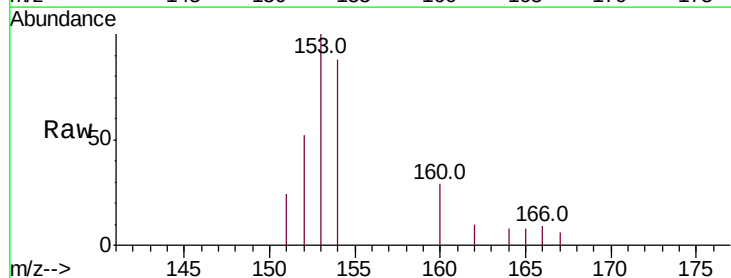

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

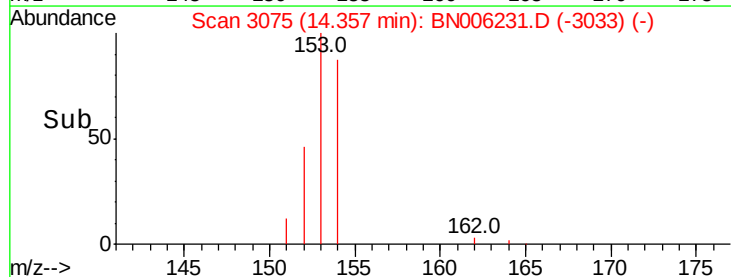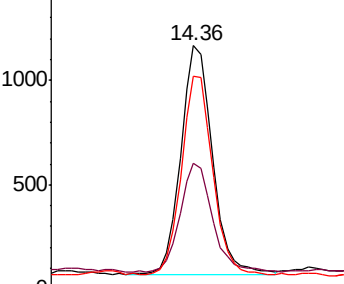

Time-->