


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006222.D
Acq On : 10 Jun 2019 14:50
Operator : JU/SJ
Sample : K3016-16DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D3DL

Manual Integrations
APPROVED

mohammad
6/11/2019 4:27:59 PM

Quant Time: Jun 11 00:53:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

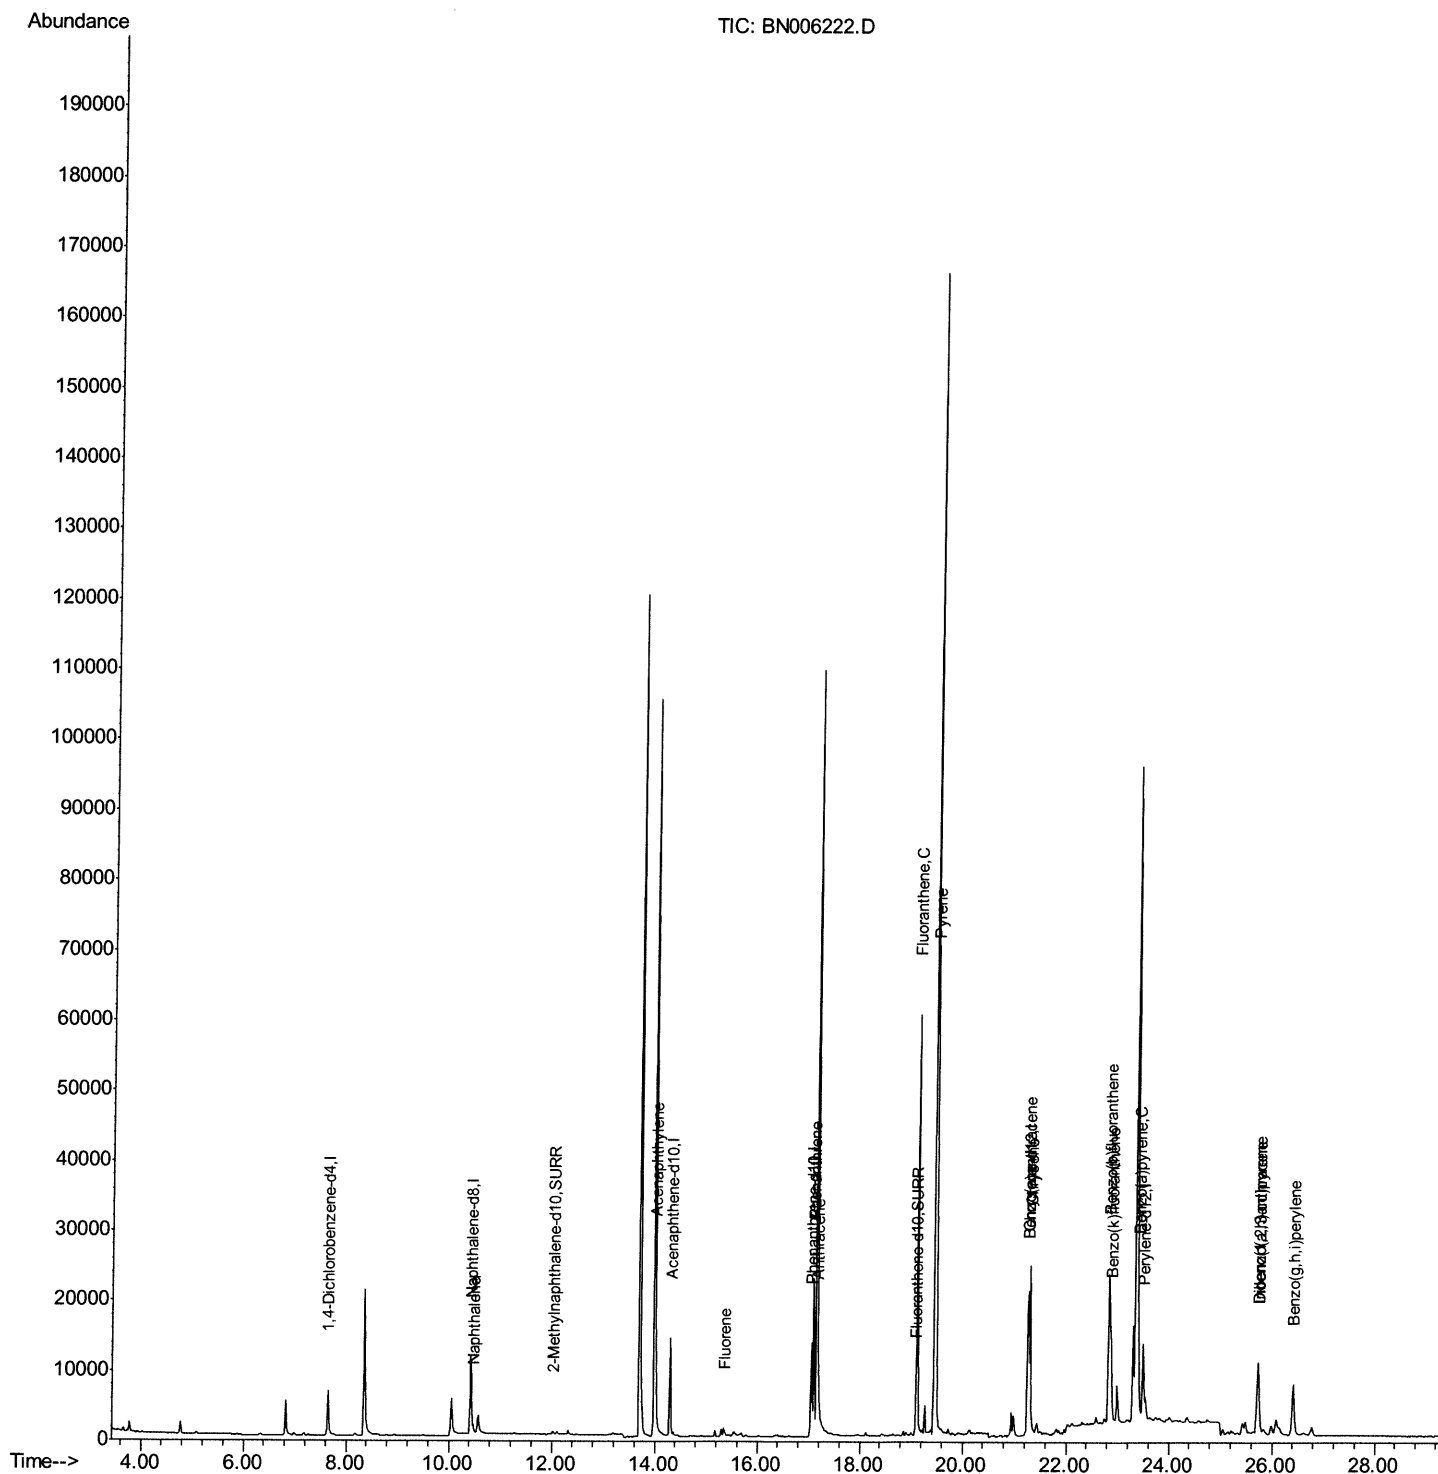

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006222.D
 Acq On : 10 Jun 2019 14:50
 Operator : JU/SJ
 Sample : K3016-16DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 A51D3DL

Manual Integrations
APPROVED

mohammad
 6/11/2019 4:27:59 PM

Quant Time: Jun 11 00:18:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

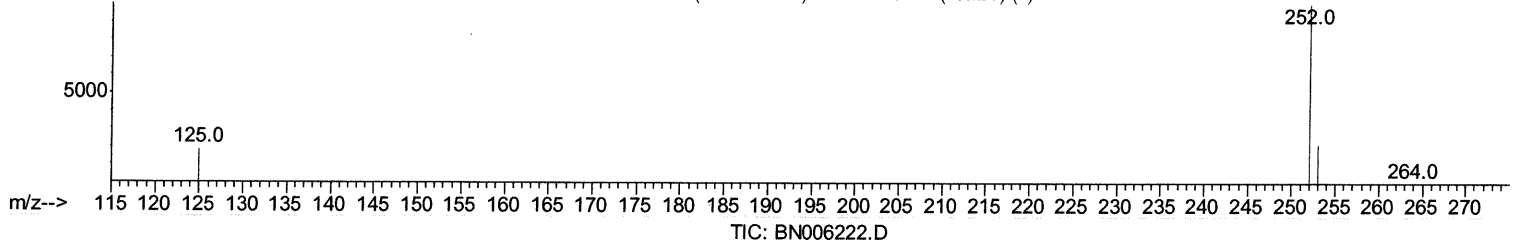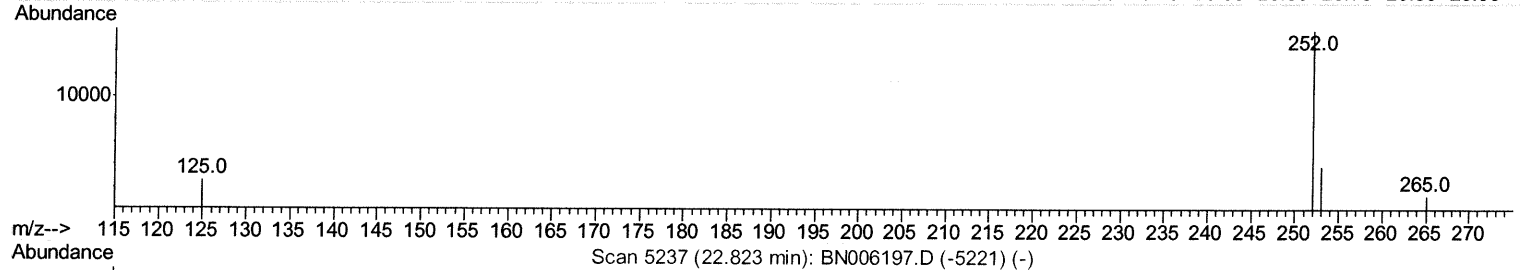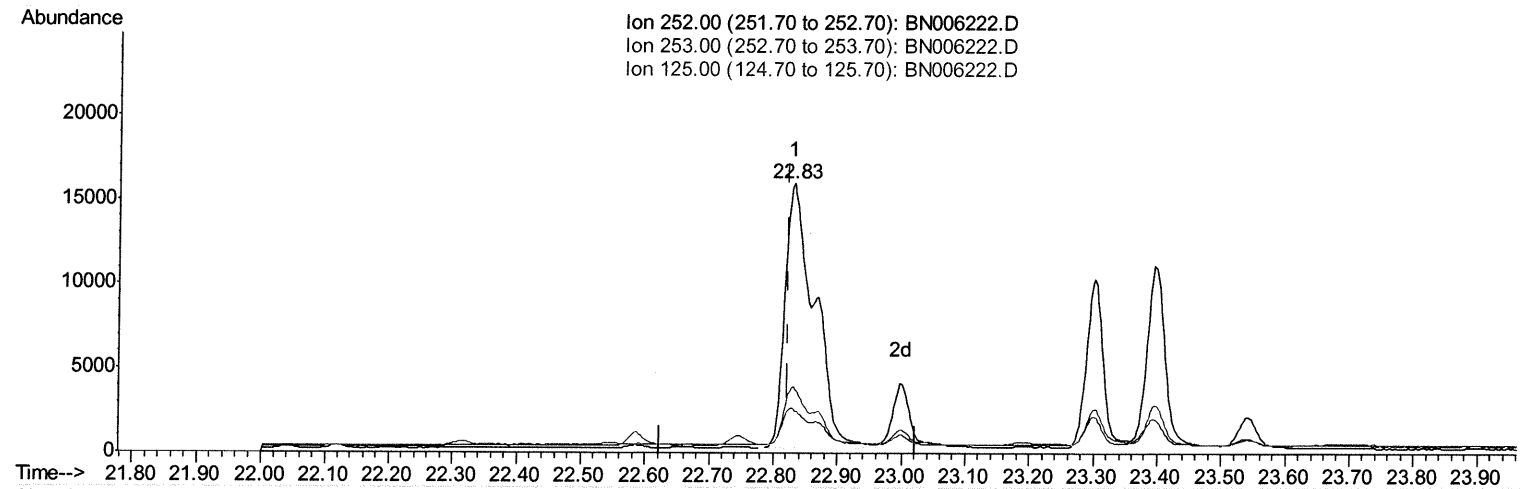

(21) Benzo(b)fluoranthene
 22.830min (+0.008) 0.73ng/ul
 response 50611

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	24.78
125.00	20.50	16.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006222.D
Acq On : 10 Jun 2019 14:50
Operator : JU/SJ
Sample : K3016-16DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51D3DL

Manual Integrations
APPROVED

mohammad
6/11/2019 4:27:59 PM

Quant Time: Jun 11 00:18:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

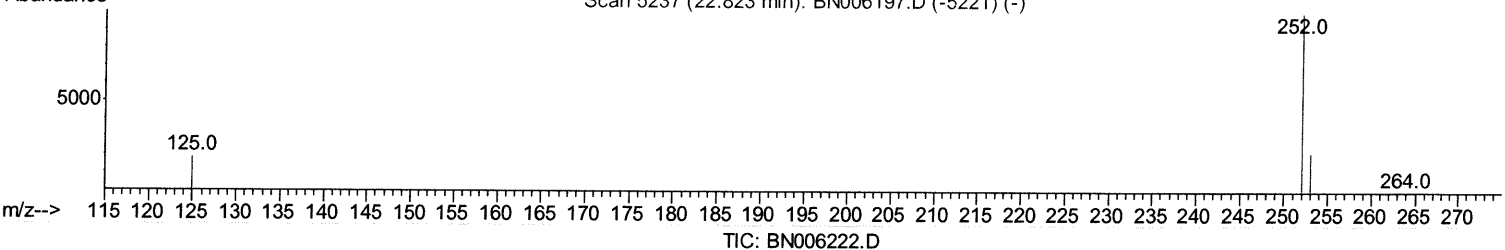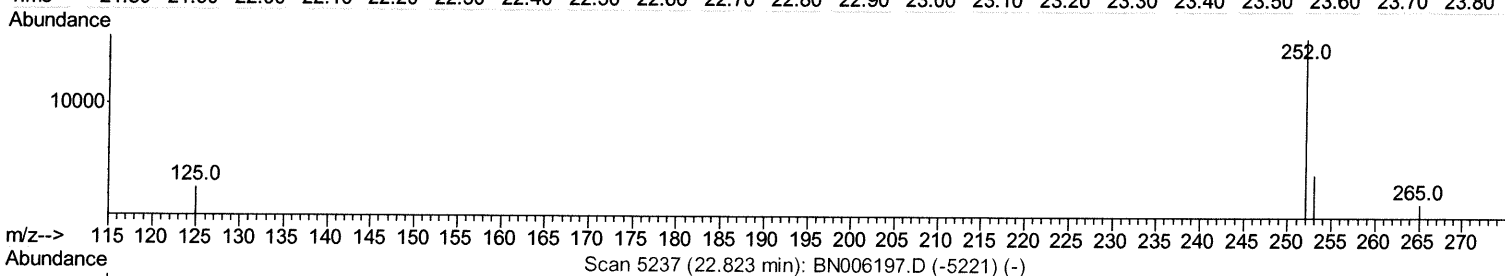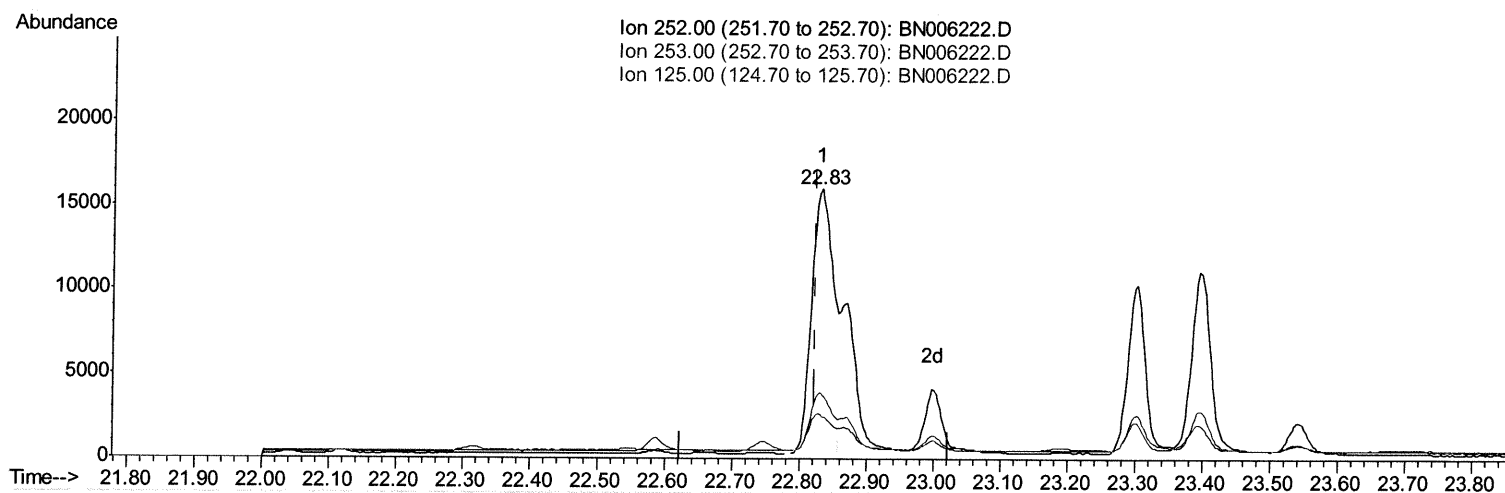

(21) Benzo(b)fluoranthene

22.830min (+0.008) 0.51ng/ul m

JU
06/11/19

response 34987

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	24.78
125.00	20.50	16.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006222.D
 Acq On : 10 Jun 2019 14:50
 Operator : JU/SJ
 Sample : K3016-16DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 A51D3DL

Manual Integrations
APPROVED

mohammad
 6/11/2019 4:27:59 PM

Quant Time: Jun 11 00:18:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

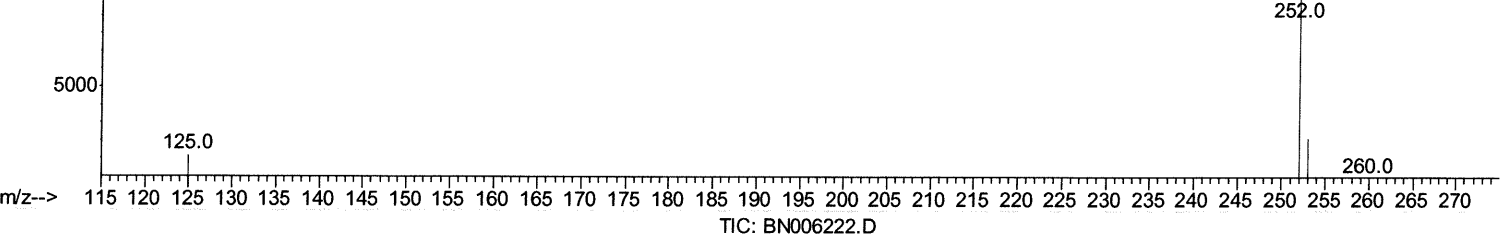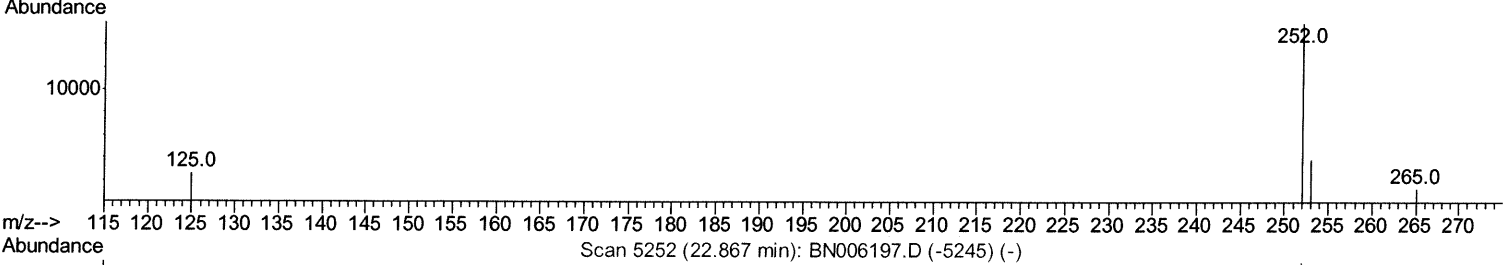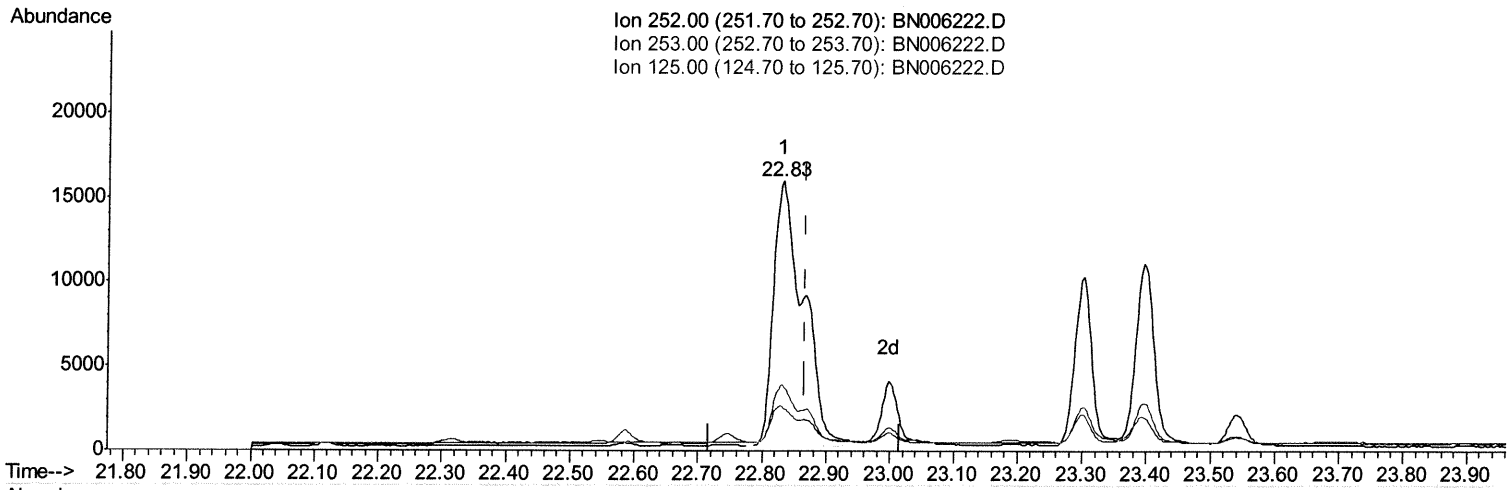

(22) Benzo(k)fluoranthene
 22.830min (-0.036) 0.75ng/ul
 response 50693

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	24.78
125.00	17.90	16.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006222.D
 Acq On : 10 Jun 2019 14:50
 Operator : JU/SJ
 Sample : K3016-16DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51D3DL

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:27:59 PM

Quant Time: Jun 11 00:18:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

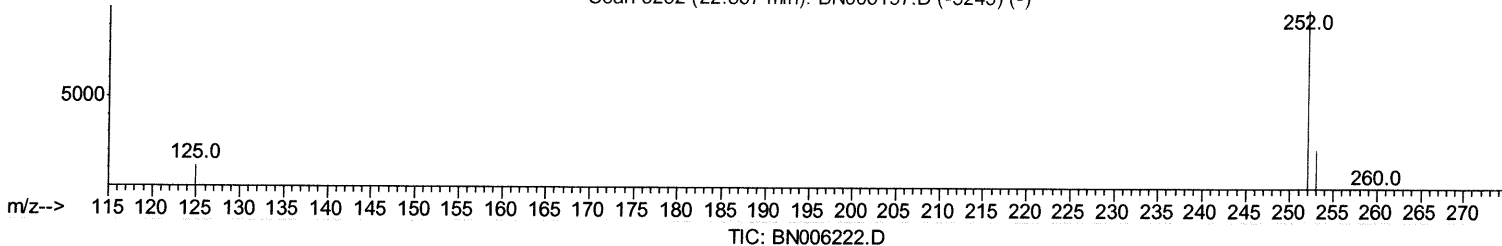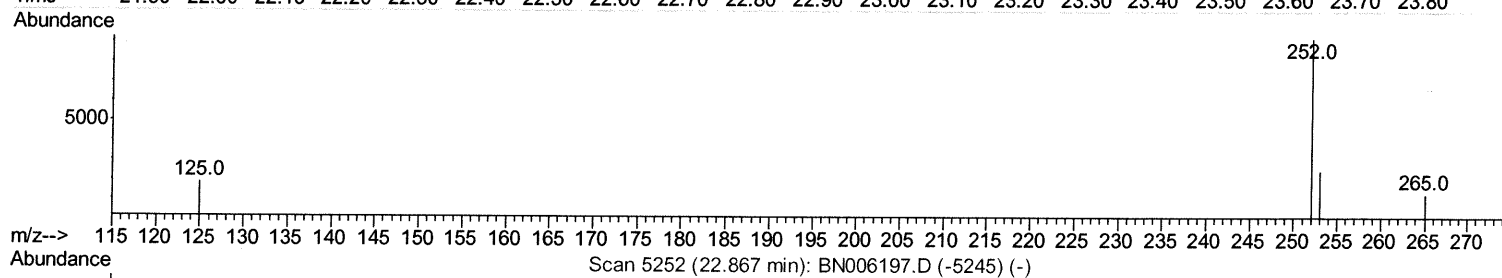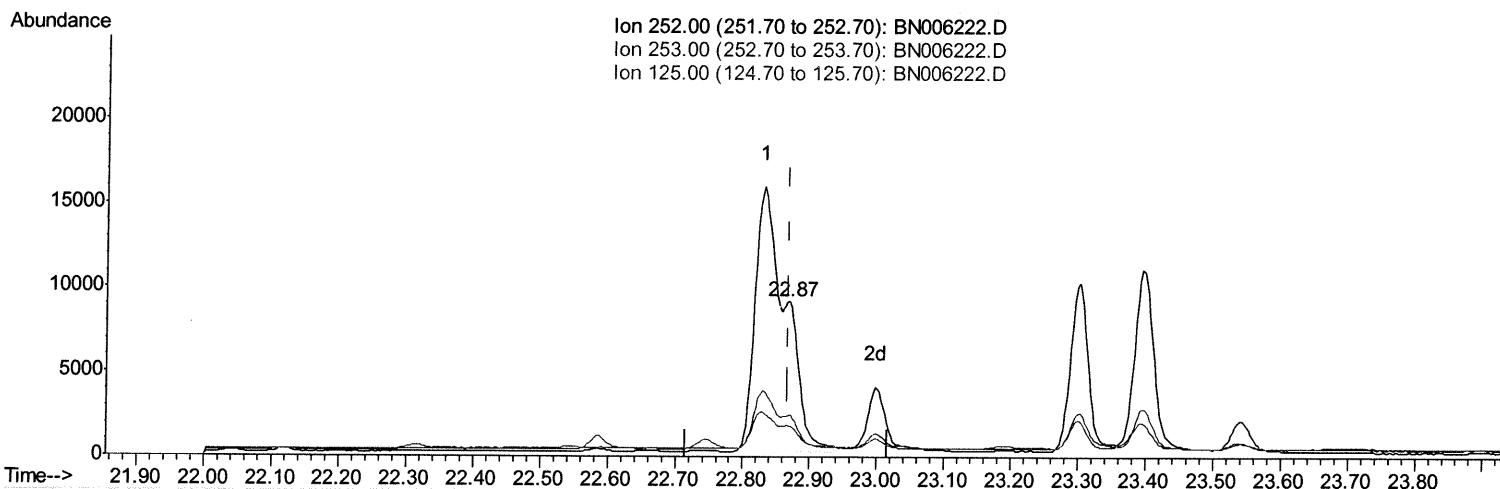

(22) Benzo(k)fluoranthene

22.868min (+0.002) 0.25ng/ul m

JU
 06/11/19

response 16820

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	26.70
125.00	17.90	19.86
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006222.D
 Acq On : 10 Jun 2019 14:50
 Operator : JU/SJ
 Sample : K3016-16DL 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51D3DL

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:27:59 PM

Quant Time: Jun 11 00:53:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4222	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15832	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	7947	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	16189	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	12936	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	16588	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.03	152	842	0.03	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	1705	0.04	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.47	128	1698	0.039	ng/ul#	86
7) Acenaphthylene	14.01	152	12960	0.293	ng/ul	100
9) Fluorene	15.35	166	1076	0.030	ng/ul#	90
12) Phenanthrene	17.09	178	25696	0.494	ng/ul	100
13) Anthracene	17.18	178	8284	0.167	ng/ul	97
15) Fluoranthene	19.12	202	53163	0.926	ng/ul	96
17) Pyrene	19.49	202	49660	0.729	ng/ul	99
18) Benzo(a)anthracene	21.25	228	14158	0.247	ng/ul	95
19) Chrysene	21.30	228	26894	0.501	ng/ul	98
21) Benzo(b)fluoranthene	22.83	252	34987m>	0.506	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	16820m>	0.250	ng/ul	
23) Benzo(a)pyrene	23.39	252	20908	0.325	ng/ul#	92
24) Indeno(1,2,3-cd)pyrene	25.73	276	17846	0.256	ng/ul#	88
25) Dibenzo(a,h)anthracene	25.73	278	4008	0.072	ng/ul#	85
26) Benzo(a,h,i)perylene	26.41	276	15520	0.266	ng/ul	98

JU 06/11/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed