


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006233.D
Acq On : 10 Jun 2019 21:10
Operator : JU/SJ
Sample : K3017-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51F1

Manual Integrations
APPROVED

mohammad
6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:11:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

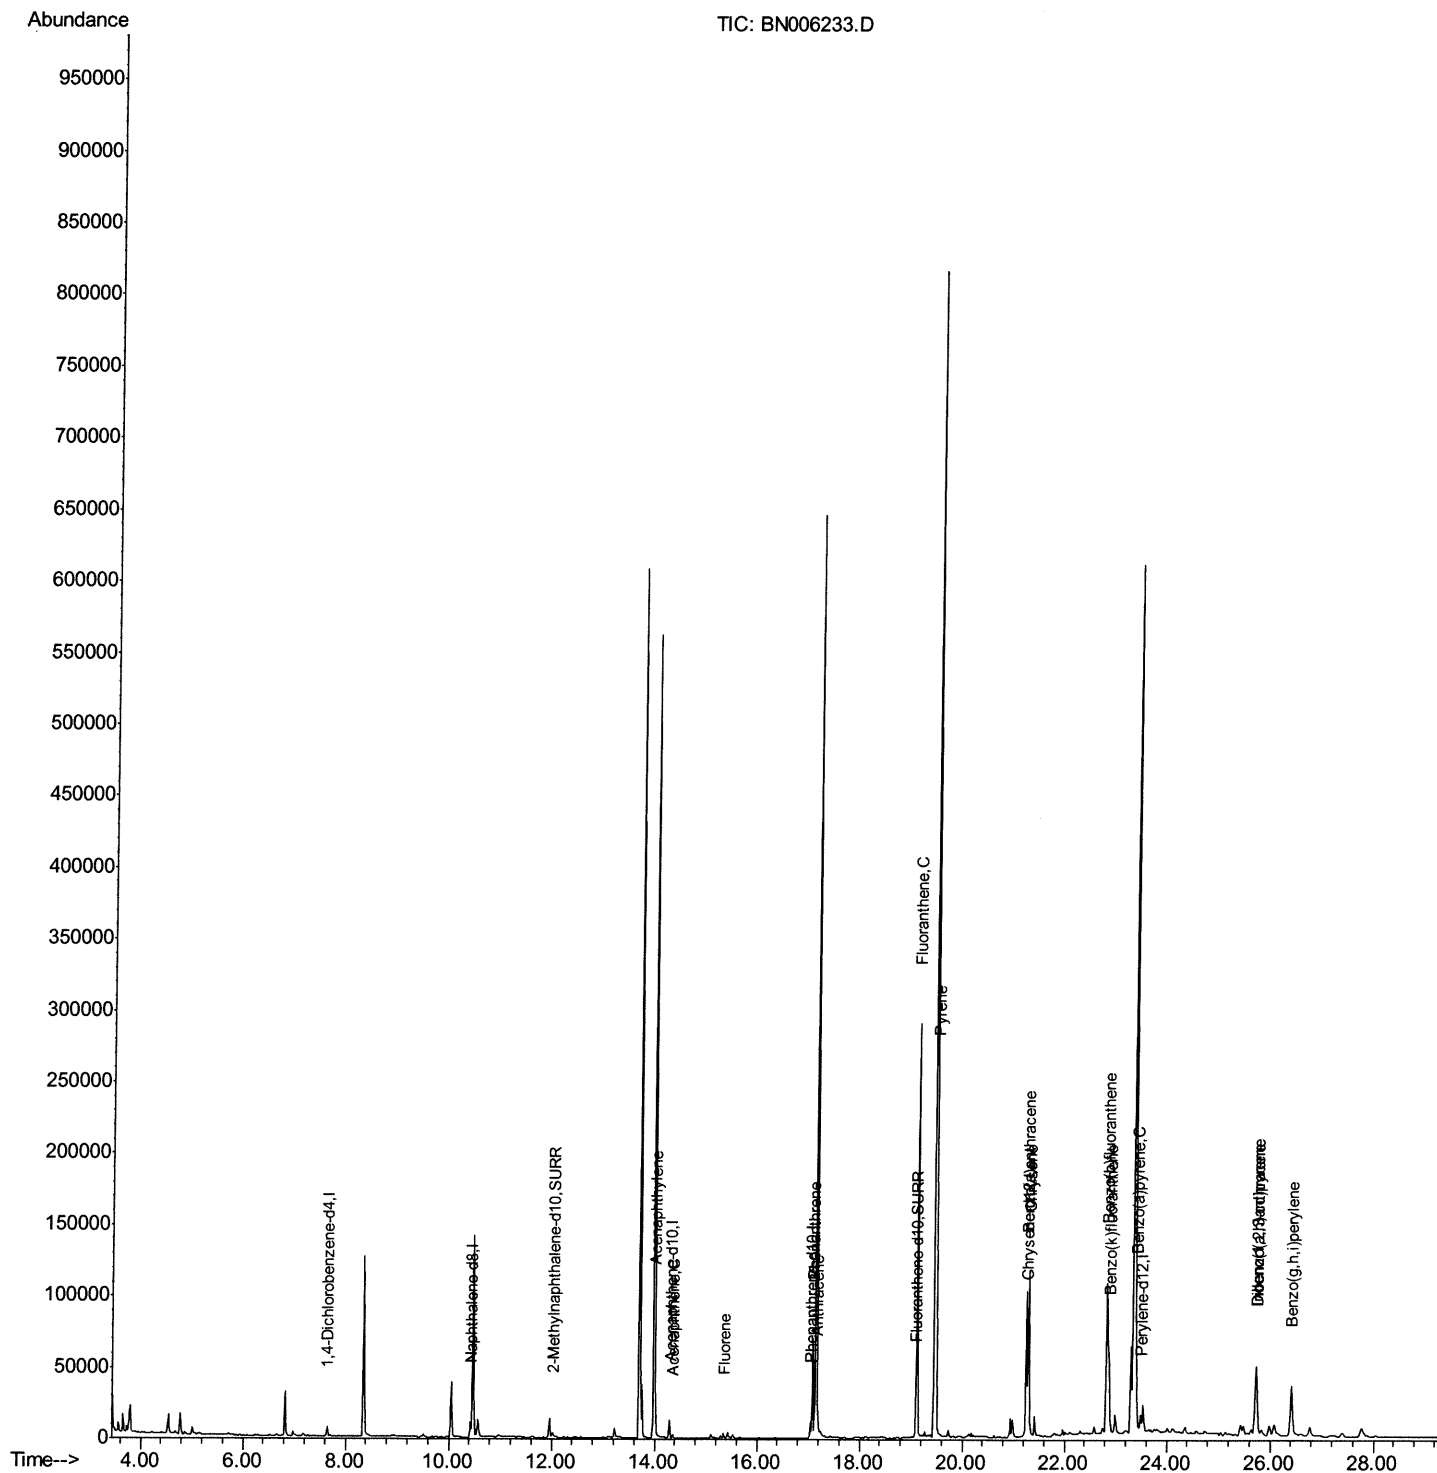

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 00:19:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

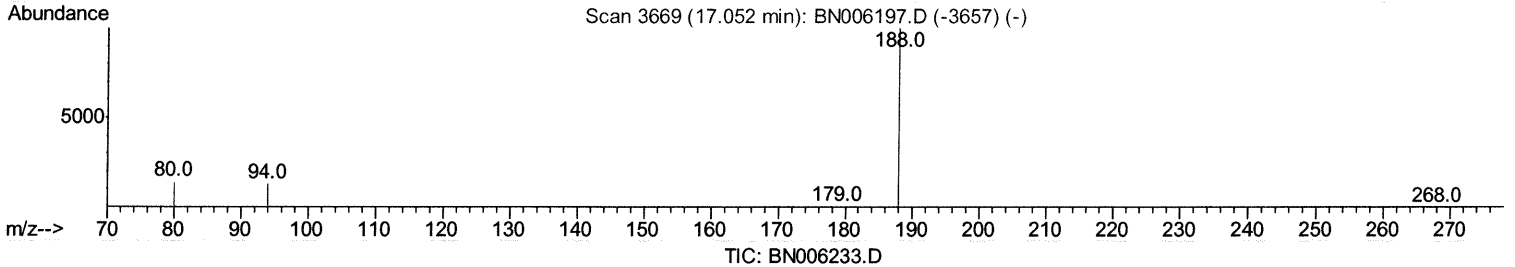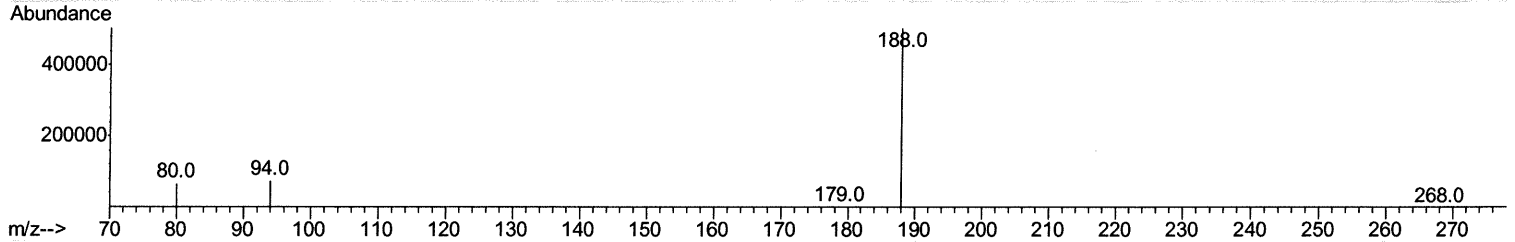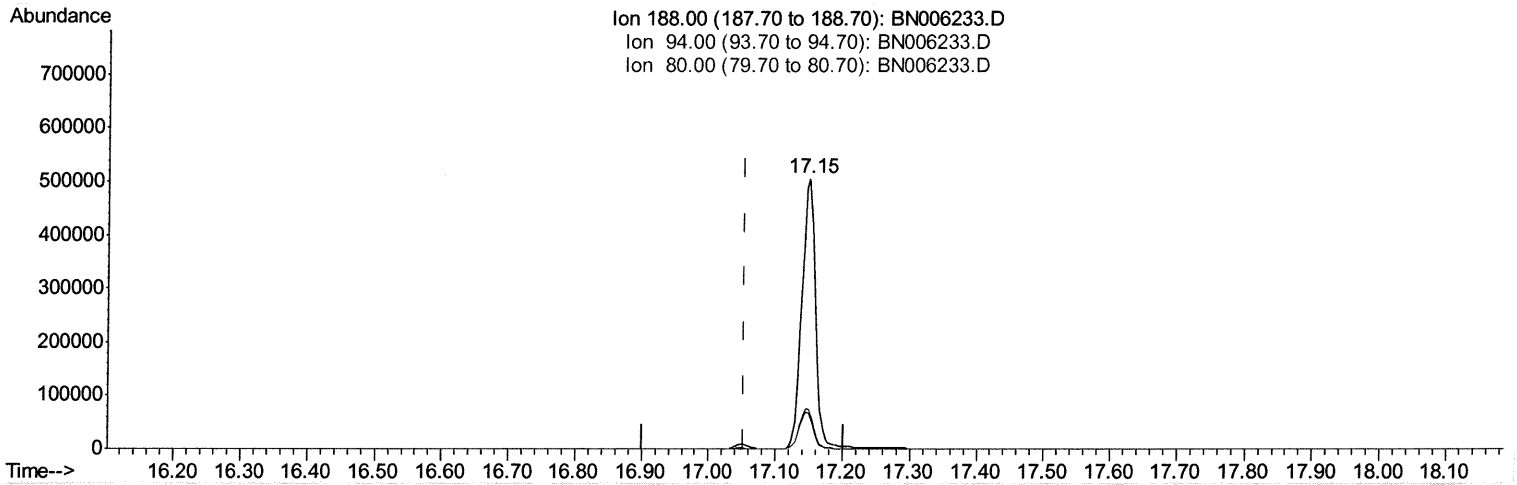

(10) Phenanthrene-d10 (I)

17.149min (+0.097) 0.40ng/ul

response 711065

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.60
80.00	13.60	13.08
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006233.D
Acq On : 10 Jun 2019 21:10
Operator : JU/SJ
Sample : K3017-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51F1

Manual Integrations
APPROVED

mohammad
6/11/2019 4:28:49 PM

Quant Time: Jun 11 00:19:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

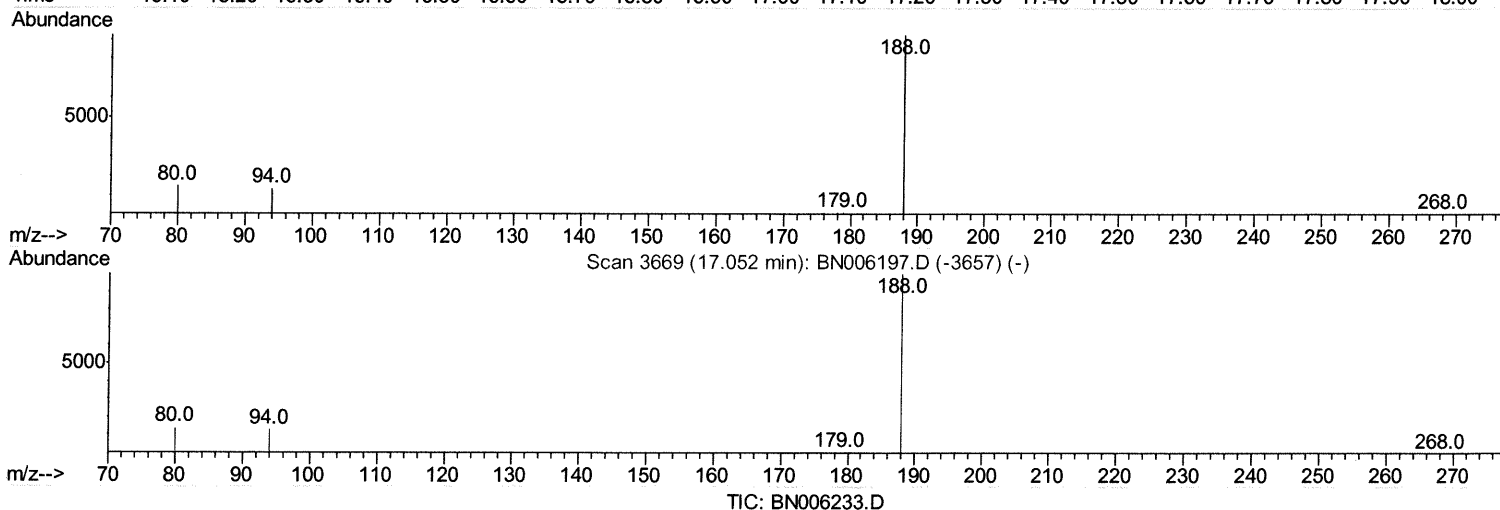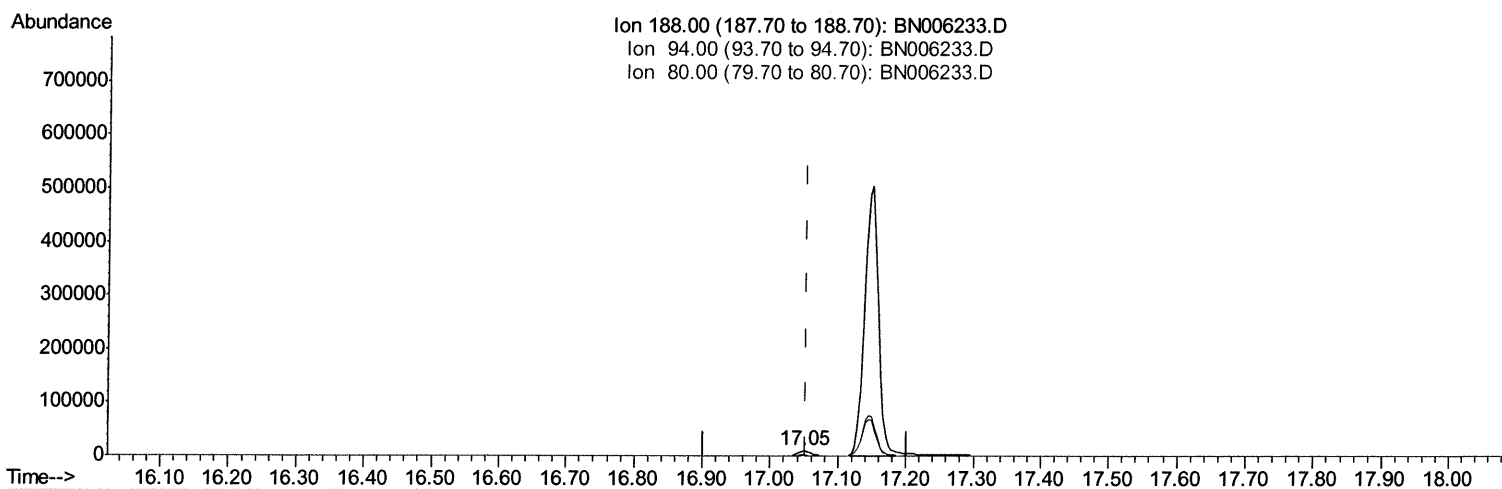

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m

JU
06/11/19

response 13107

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.46
80.00	13.60	16.03
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006233.D
Acq On : 10 Jun 2019 21:10
Operator : JU/SJ
Sample : K3017-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51F1

Manual Integrations
APPROVED

mohammad
6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

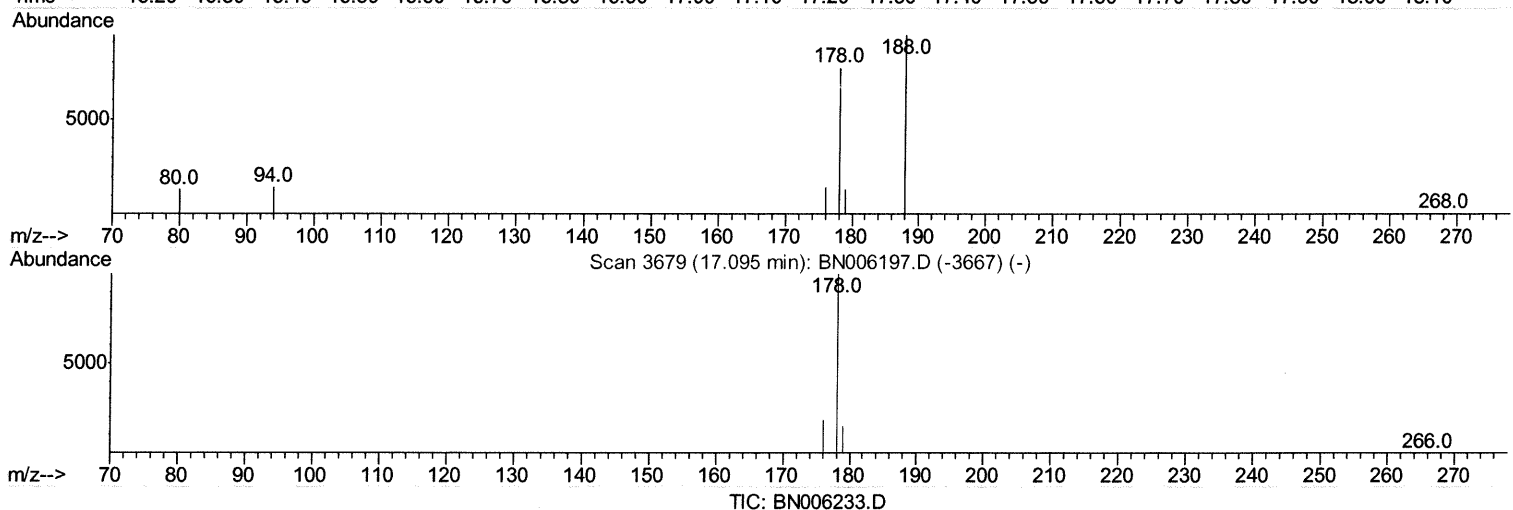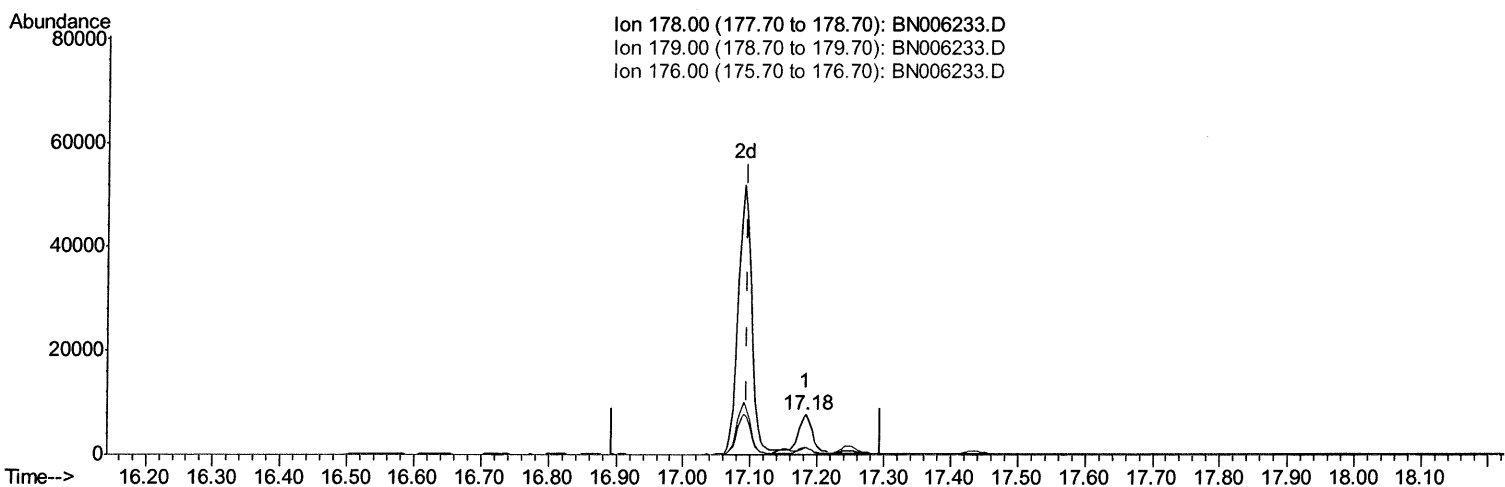

(12) Phenanthrene

17.183min (+0.088) 0.25ng/ul

response 10309

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	17.54
176.00	19.10	19.32
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

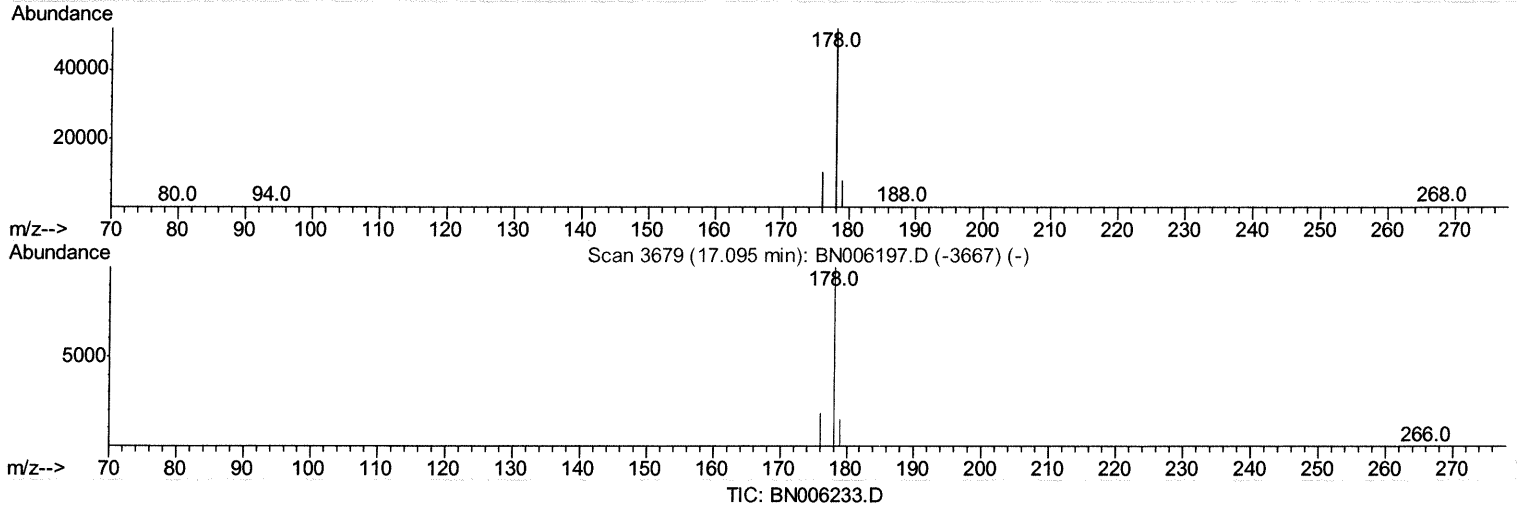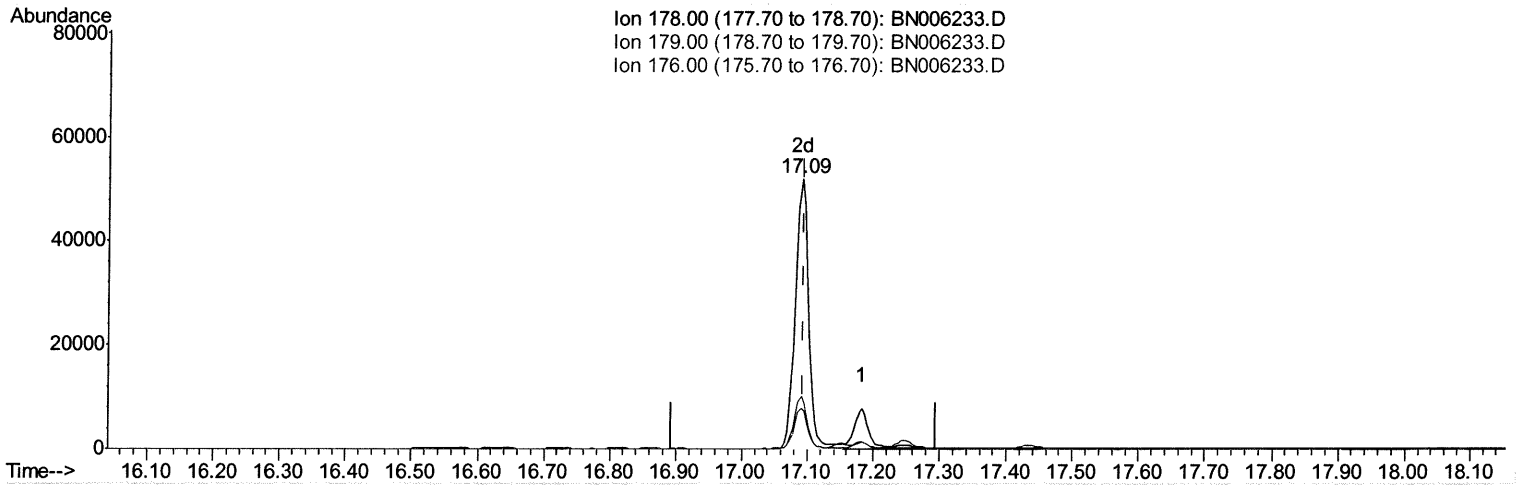

(12) Phenanthrene

17.090min (-0.004) 1.75ng/ul m *JU 06/11/19*

response 73437

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	15.23
176.00	19.10	19.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

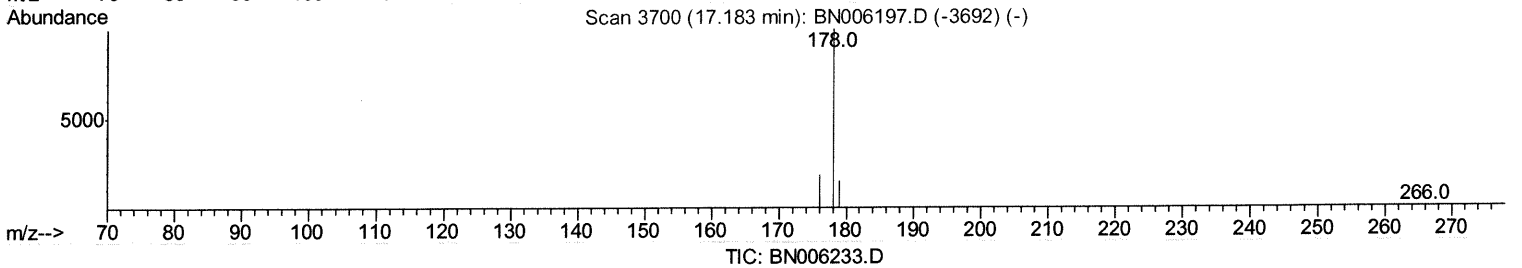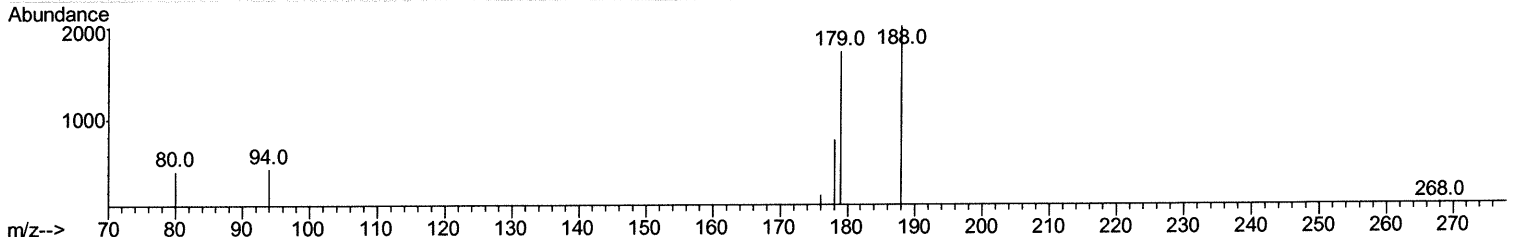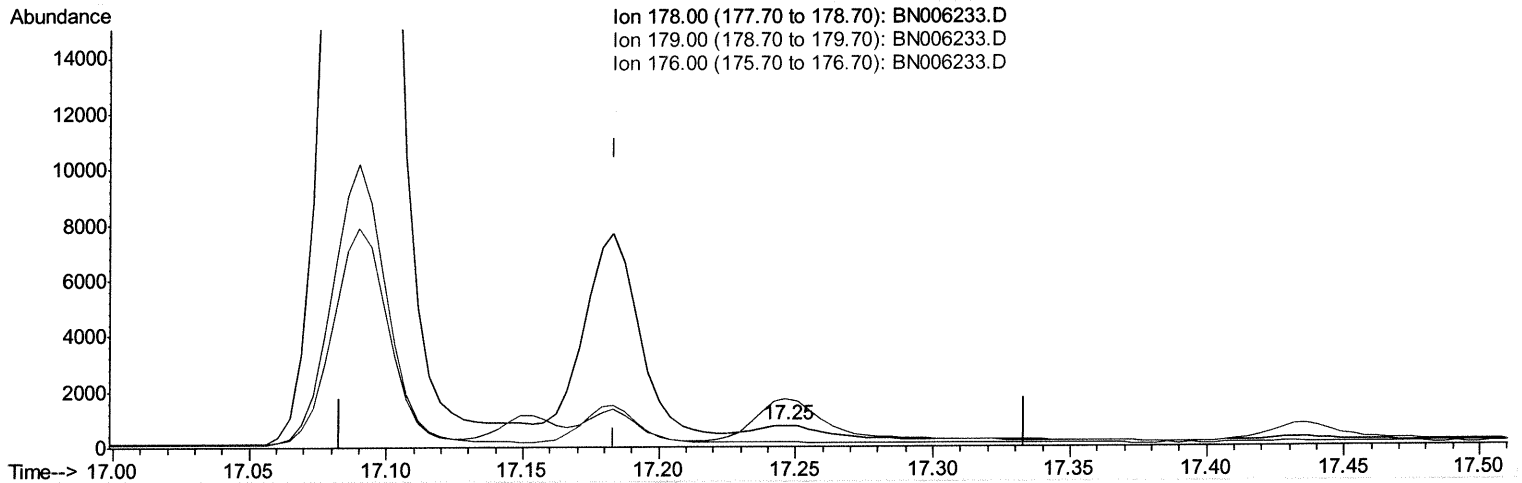

(13) Anthracene

17.246min (+0.063) 0.04ng/ul

response 1549

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	226.63#
176.00	18.90	21.41
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

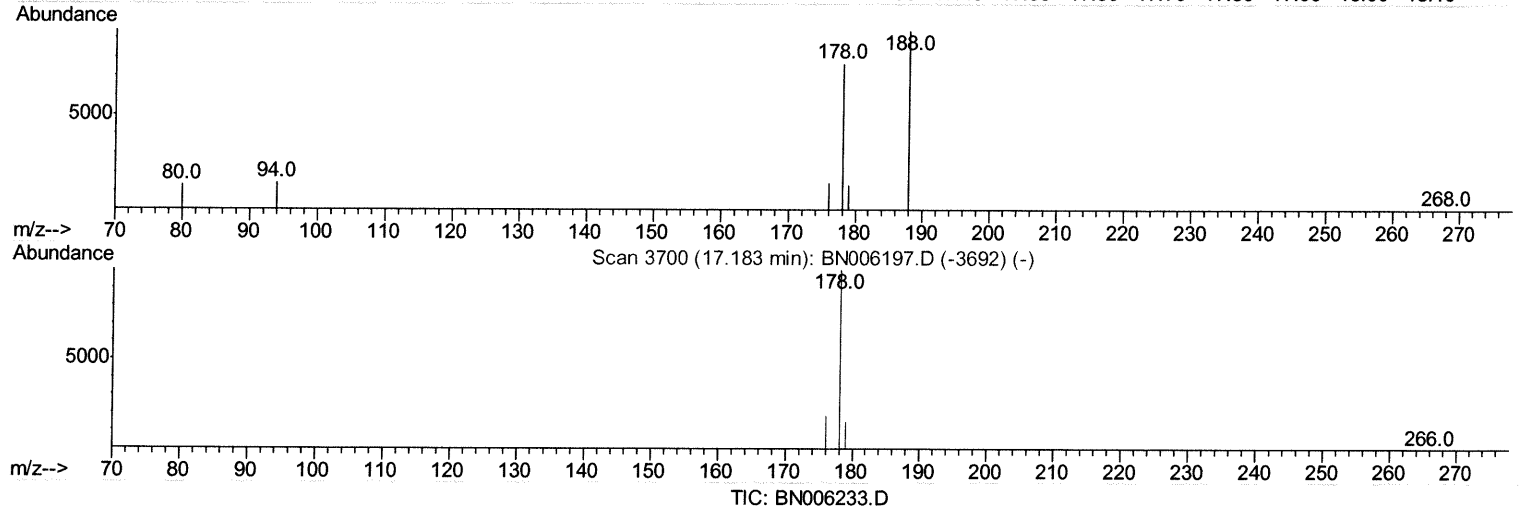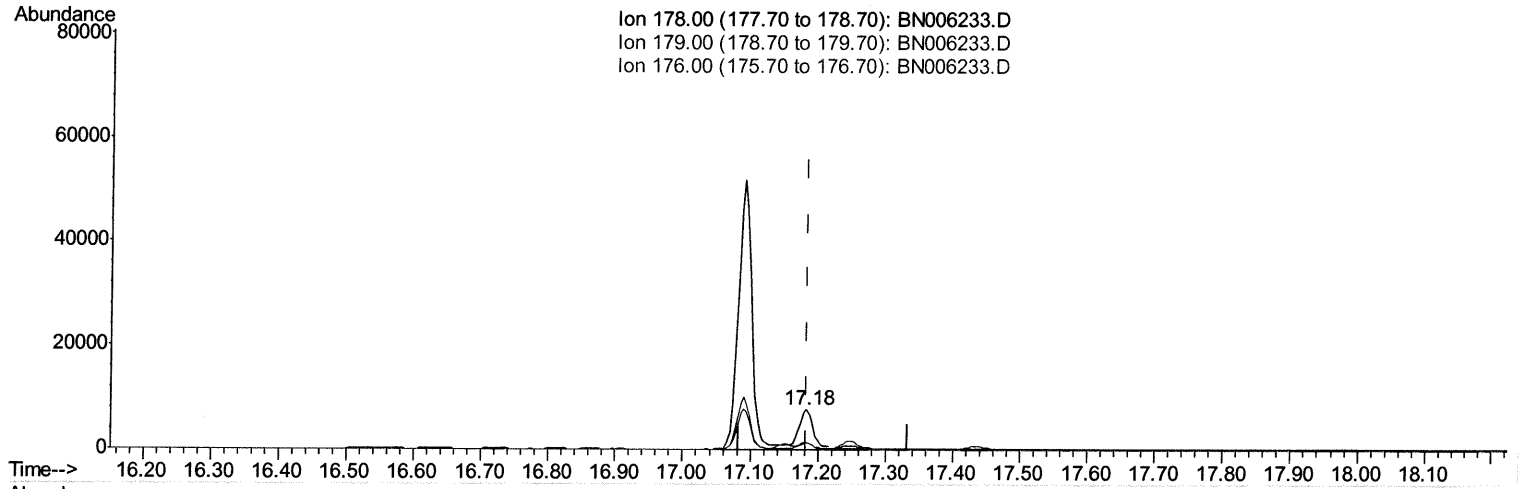

(13) Anthracene

17.183min (-0.000) 0.25ng/ul m ^{JU} 06/11/19

response 10083

Ion	Exp%	Act%
178.00	100	100
179.00	15.30	17.54
176.00	18.90	19.32
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

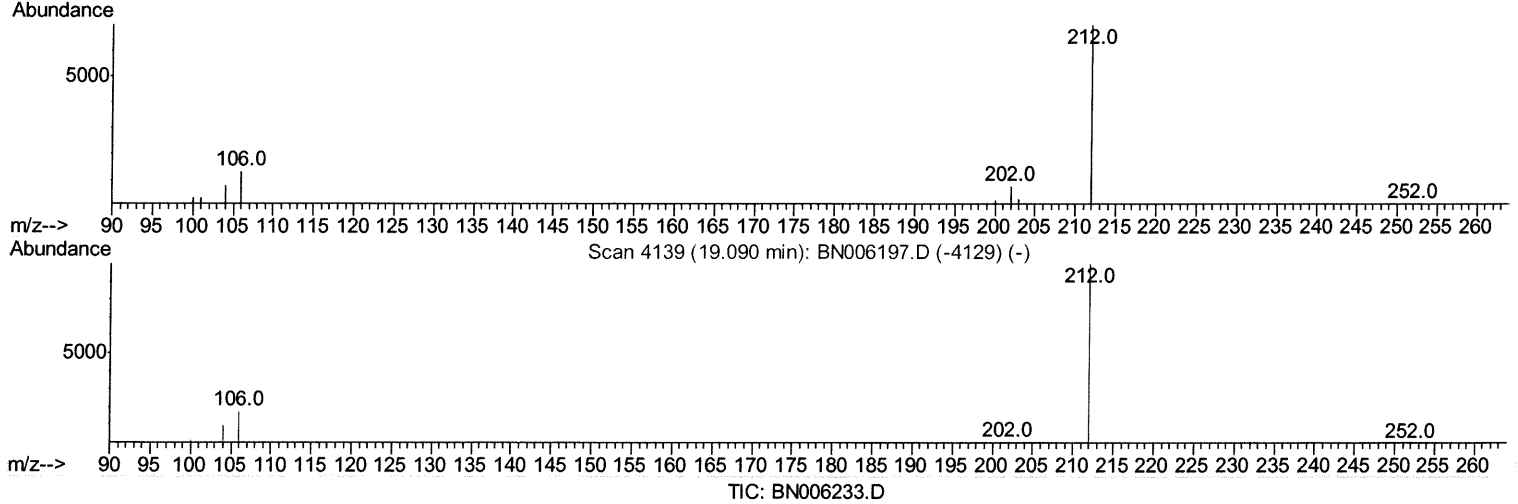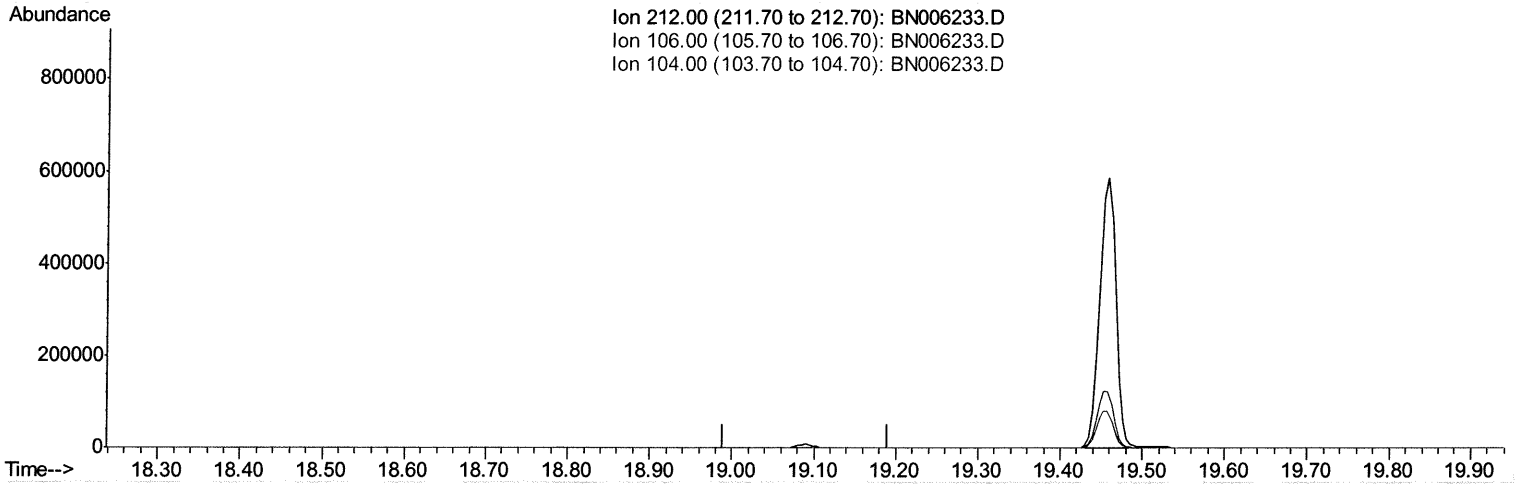

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

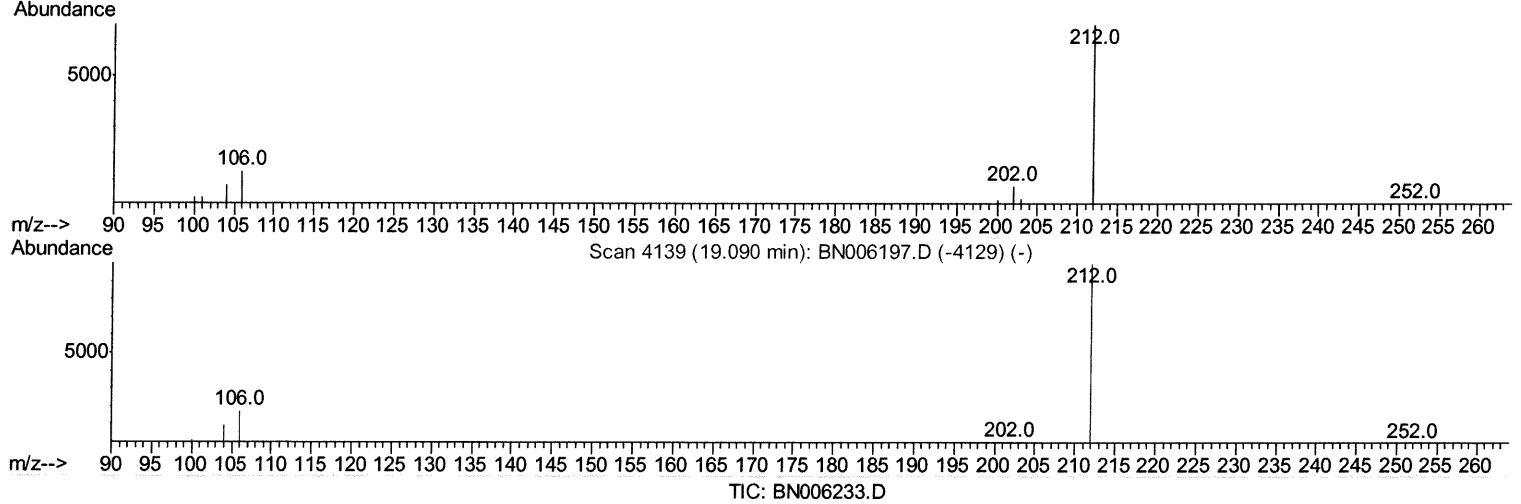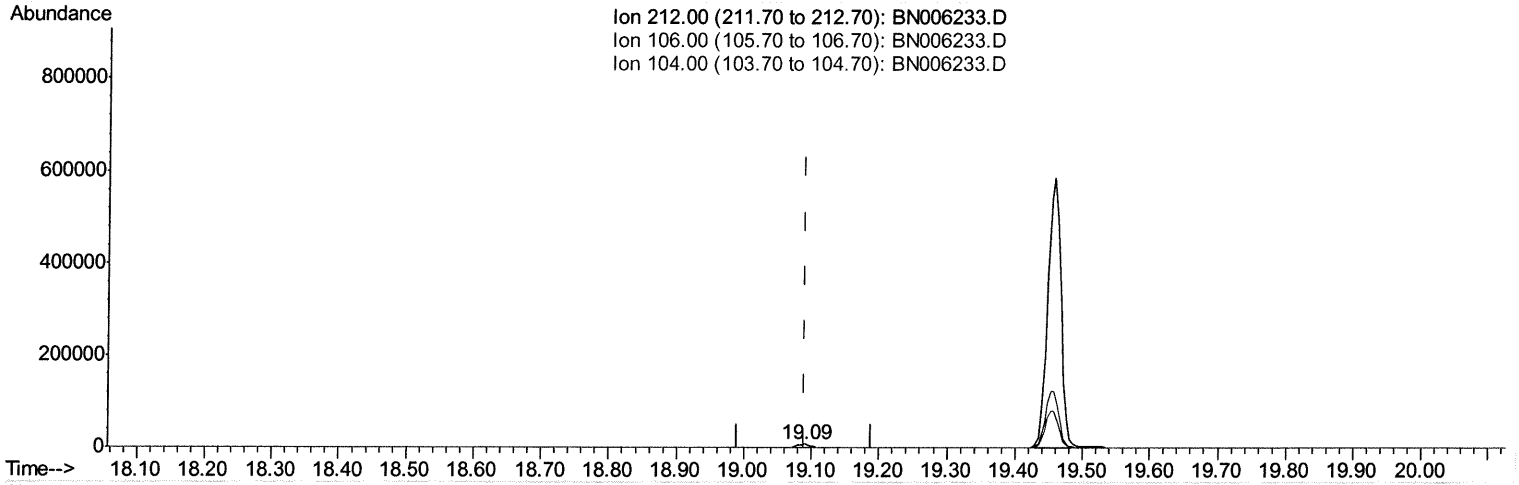

(14) Fluoranthene-d10 (SURR)

19.090min (-0.000) 0.28ng/ul m

JU
 06/11/19

response 9858

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

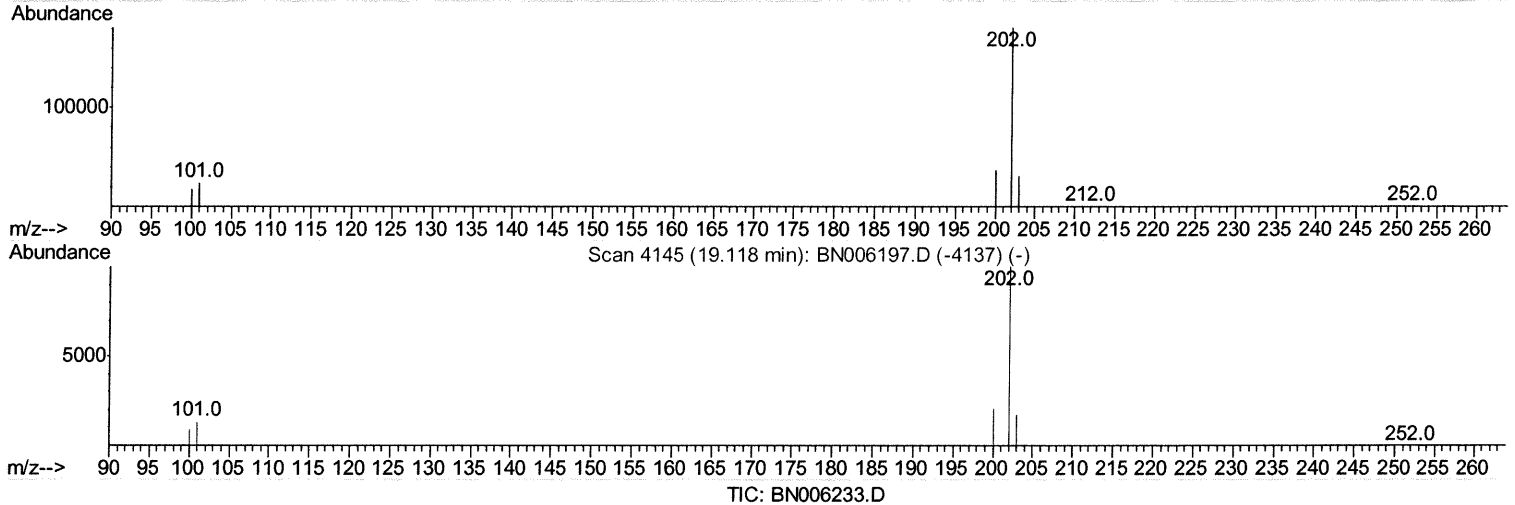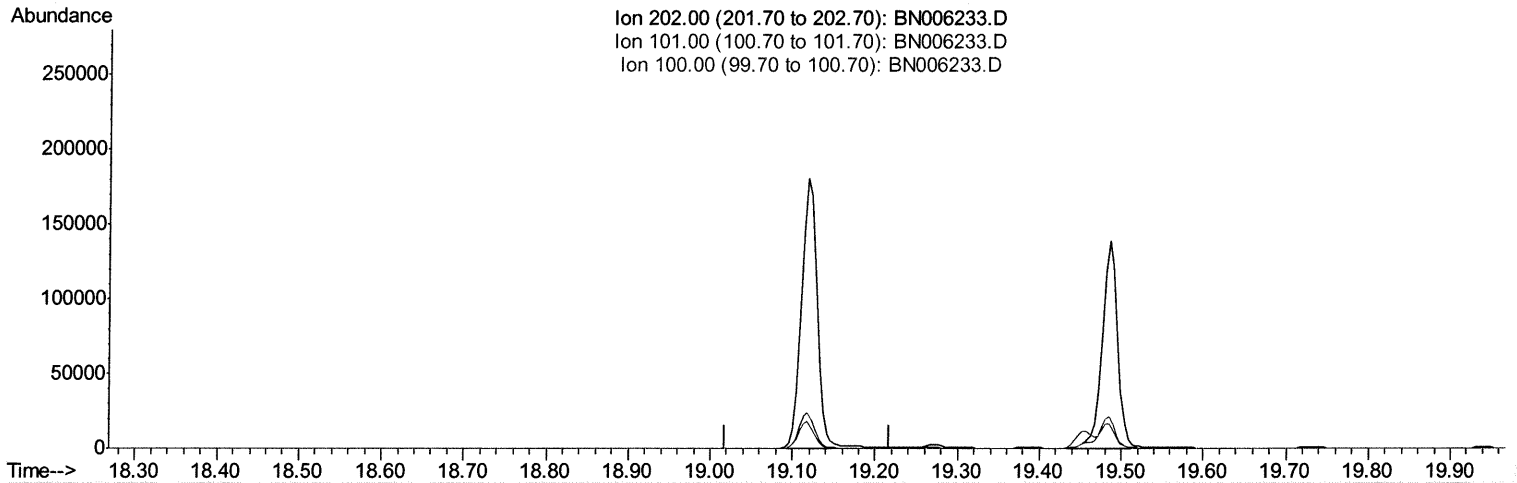

(15) Fluoranthene (C)

19.118min (-19.118) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.10	0.00
100.00	8.70	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

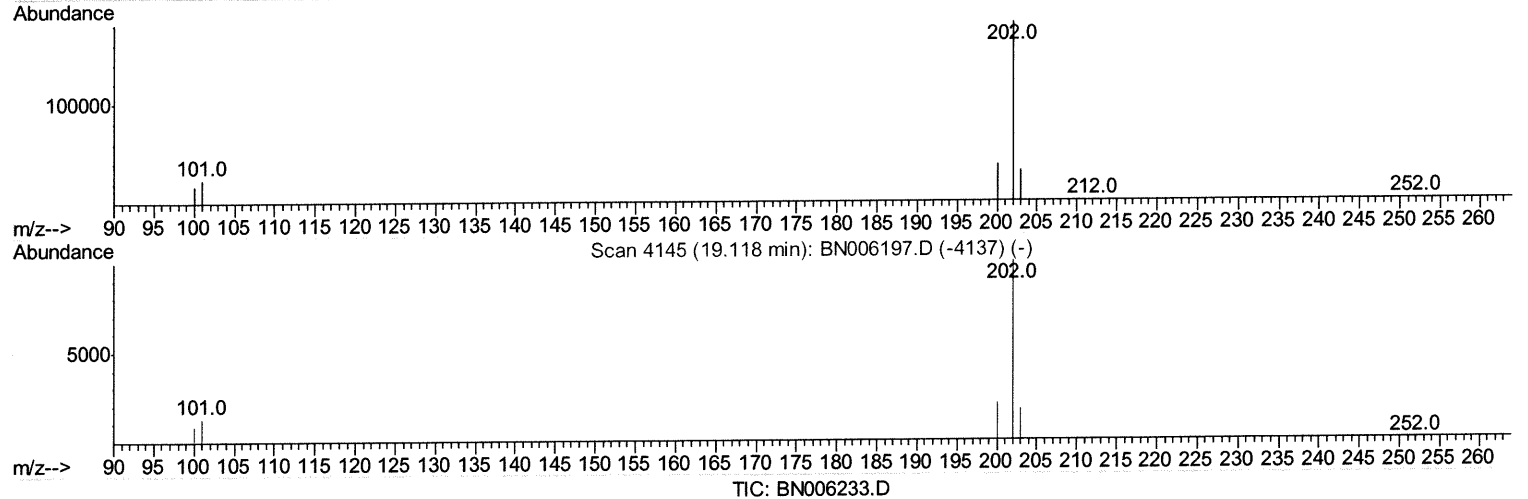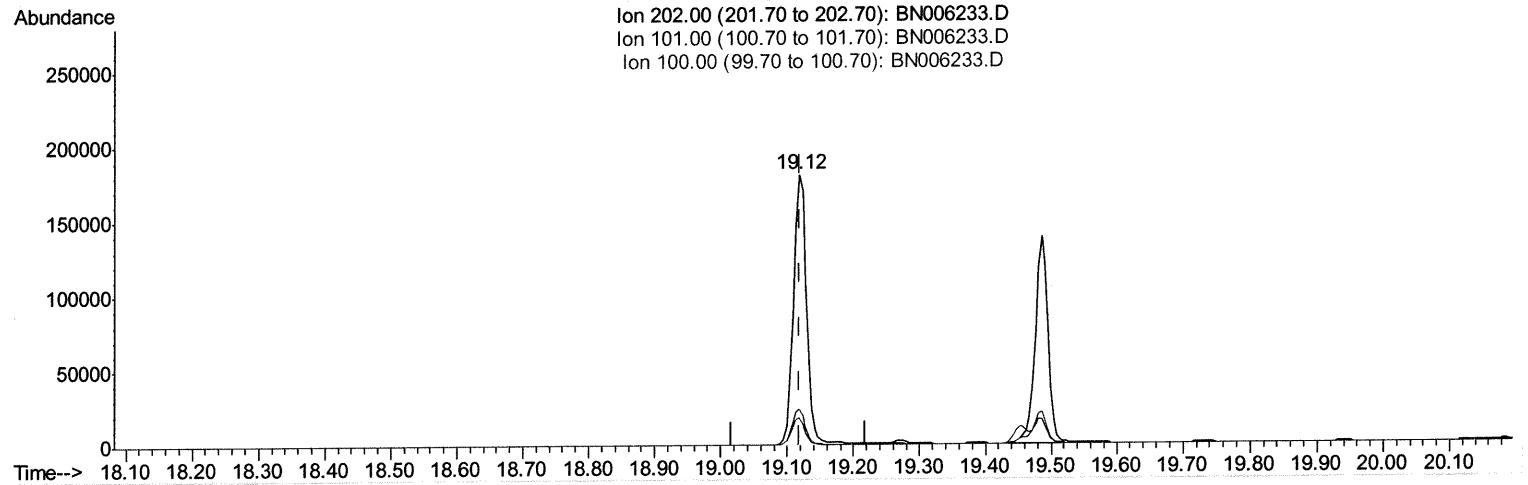

(15) Fluoranthene (C)

19.118min (-0.000) 5.11ng/ul m

response 237259

Ion	Exp%	Act%
202.00	100	100
101.00	12.10	13.30
100.00	8.70	9.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
Data File : BN006233.D
Acq On : 10 Jun 2019 21:10
Operator : JU/SJ
Sample : K3017-20
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A51F1

Manual Integrations
APPROVED

mohammad
6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 05:10:30 2019
Response via : Initial Calibration

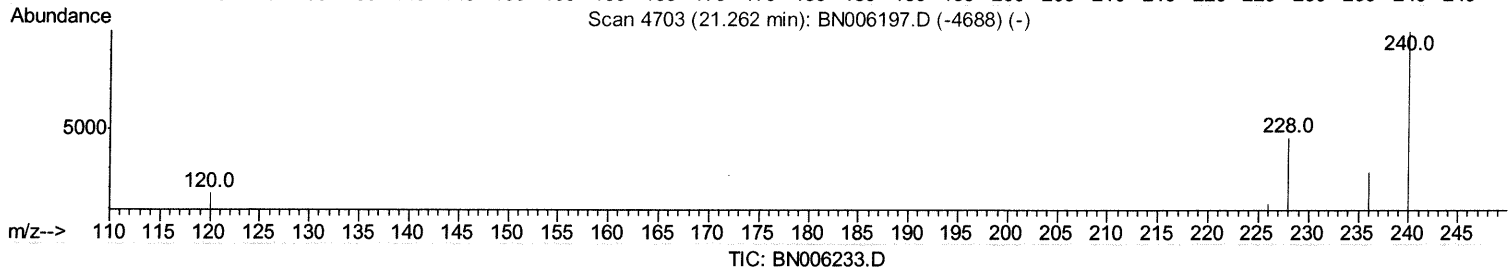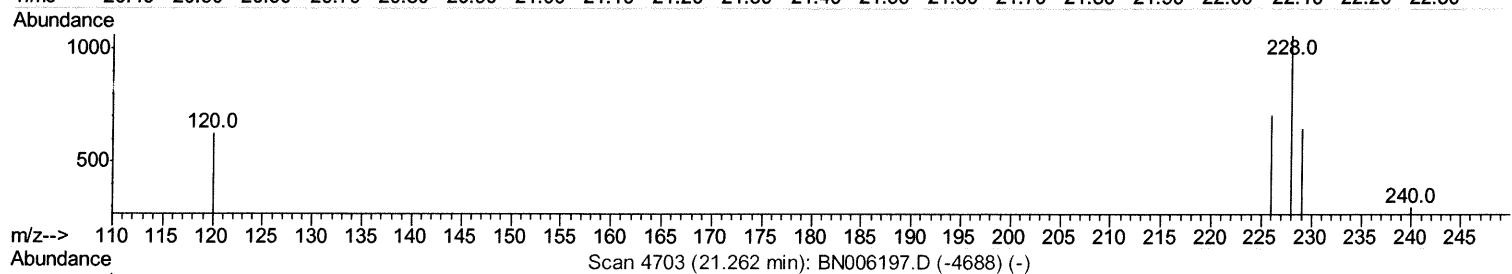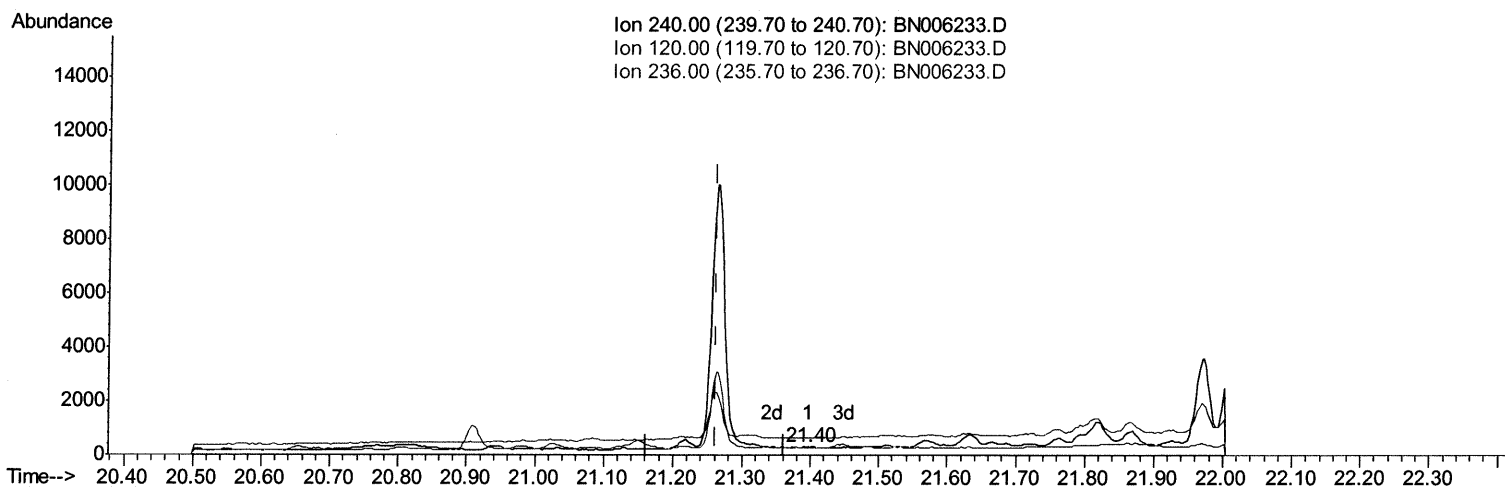

(16) Chrysene-d12 (I)

21.397min (+0.134) 0.40ng/ul

response 39

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	207.97#
236.00	30.10	89.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:08:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

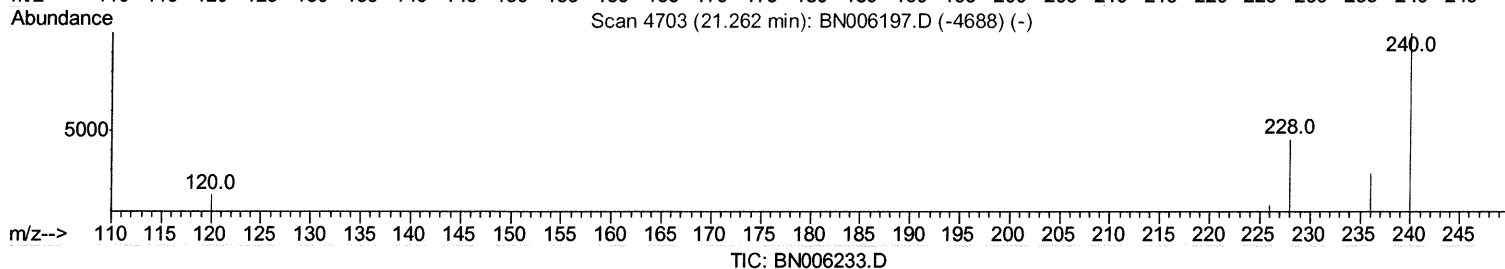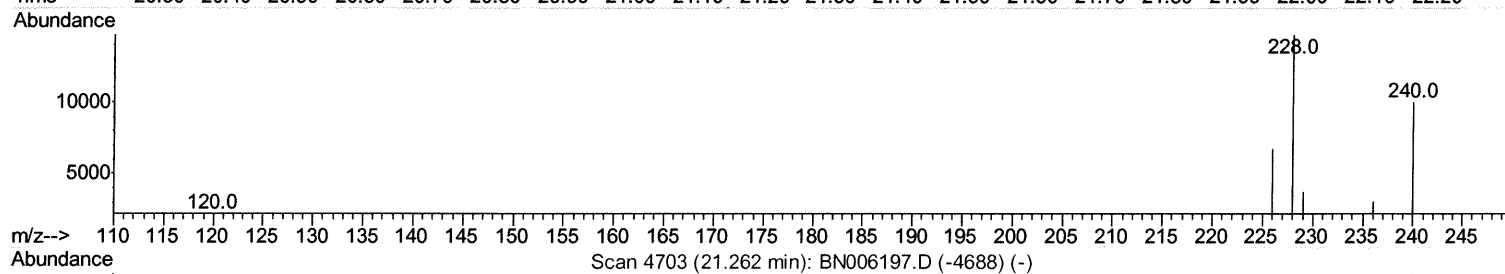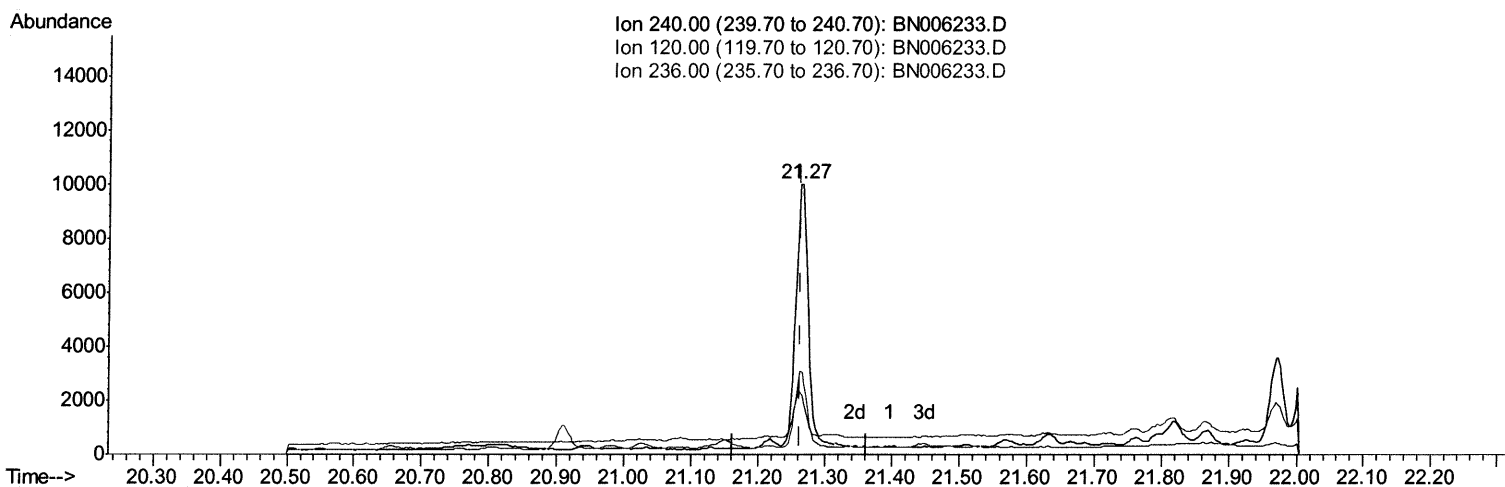

(16) Chrysene-d12 (I)

21.265min (+0.003) 0.40ng/ul m *JU 06/11/19*

response 12317

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	21.88
236.00	30.10	30.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:09:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

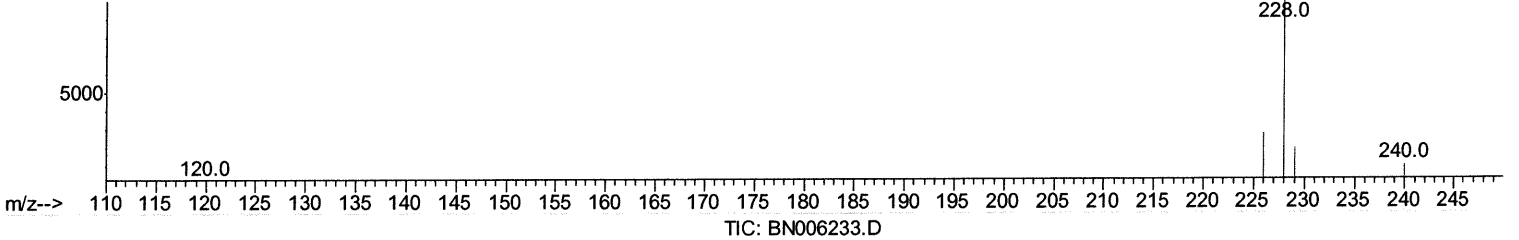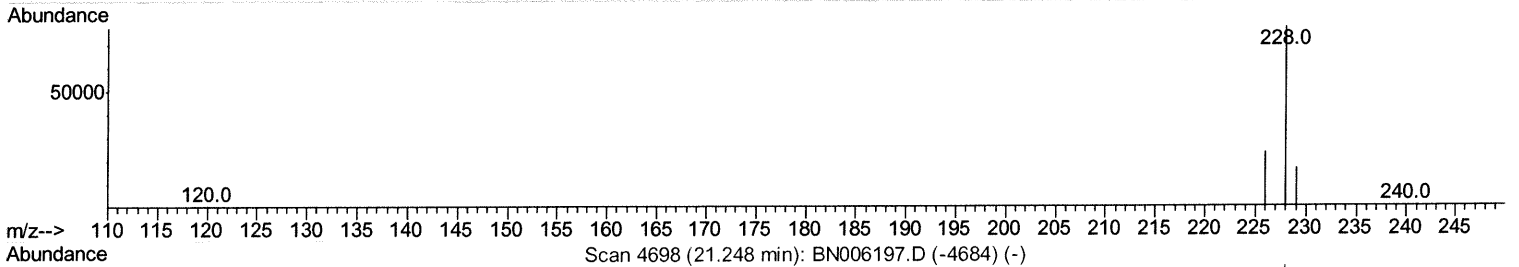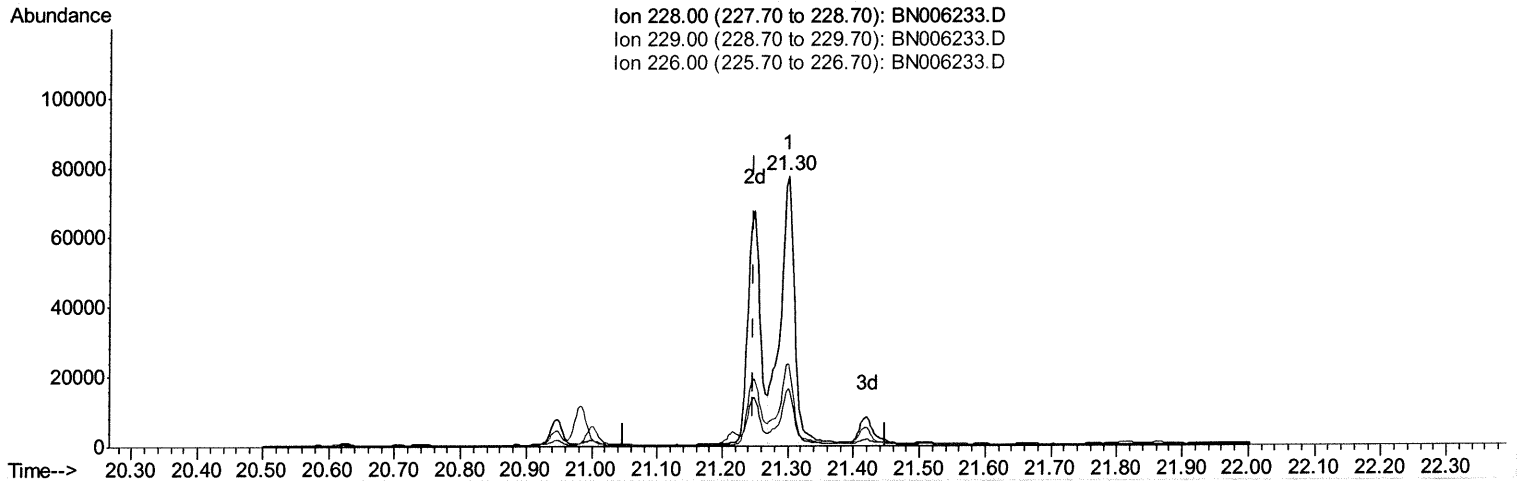

(18) Benzo(a)anthracene
 21.300min (+0.052) 2.20ng/ul
 response 120071

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	21.40
226.00	28.50	30.66
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:09:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

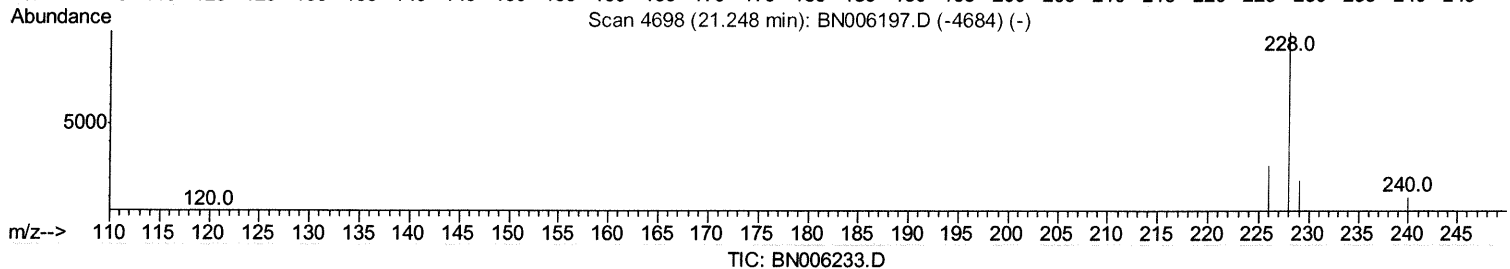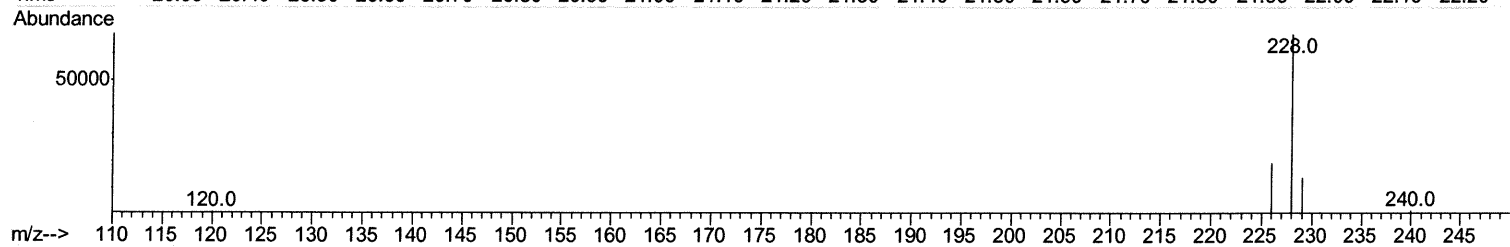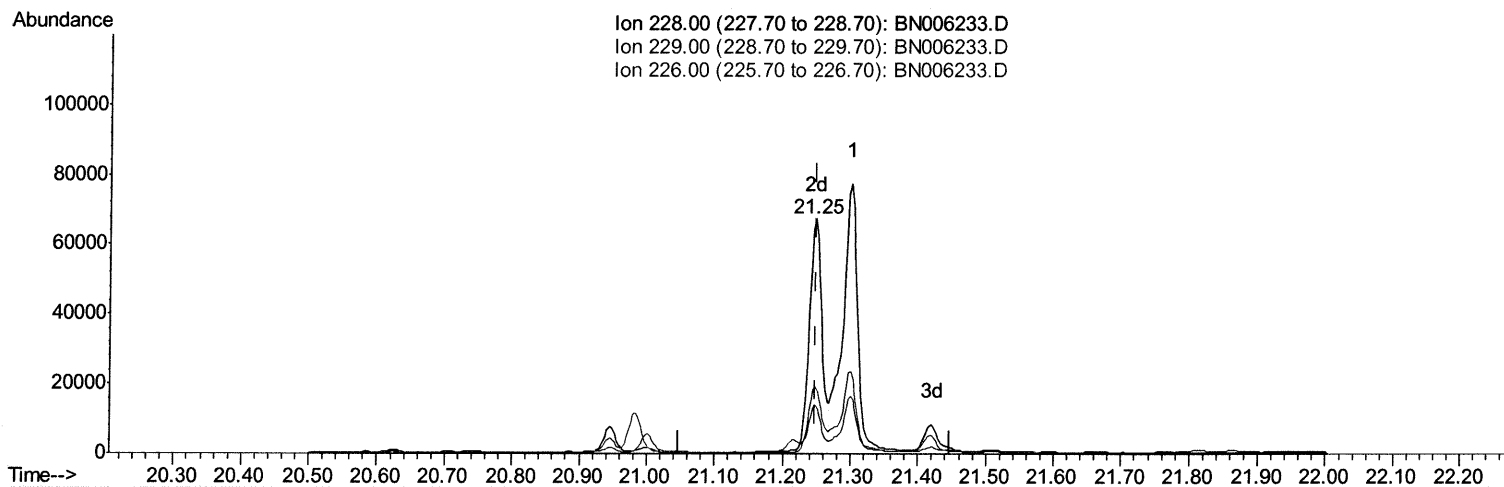

(18) Benzo(a)anthracene

21.248min (-0.000) 1.64ng/ul m *JU* 06/11/19

response 89181

Ion	Exp%	Act%
228.00	100	100
229.00	20.60	20.82
226.00	28.50	28.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:09:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

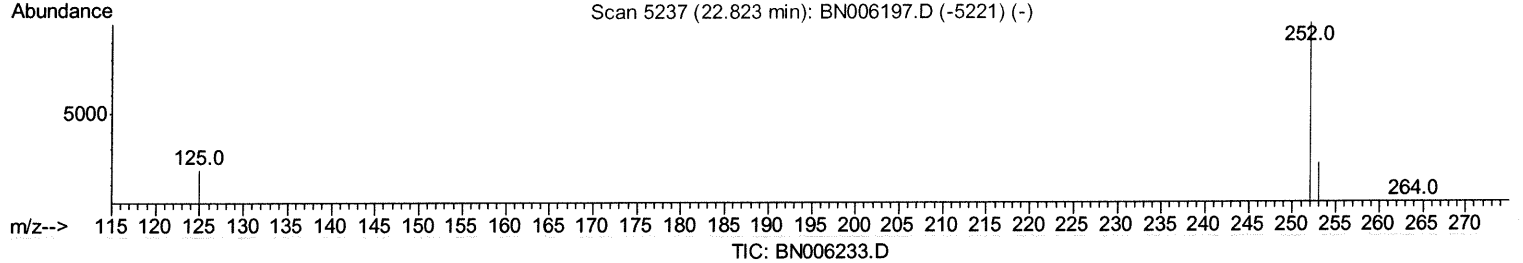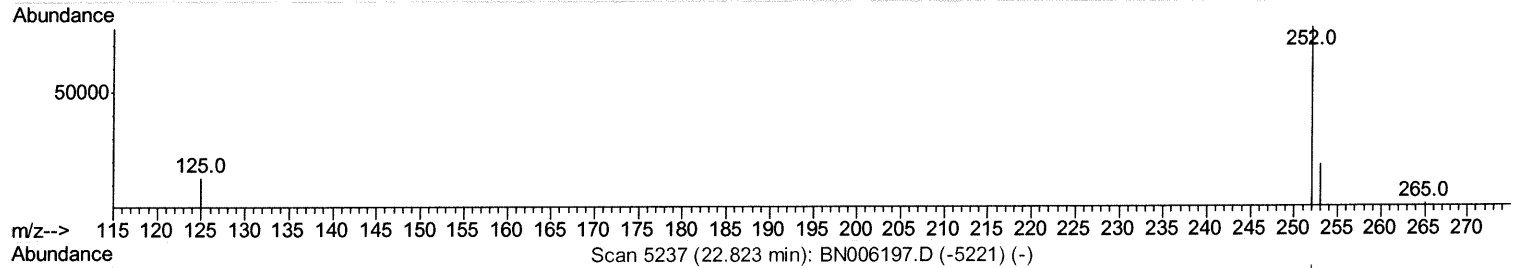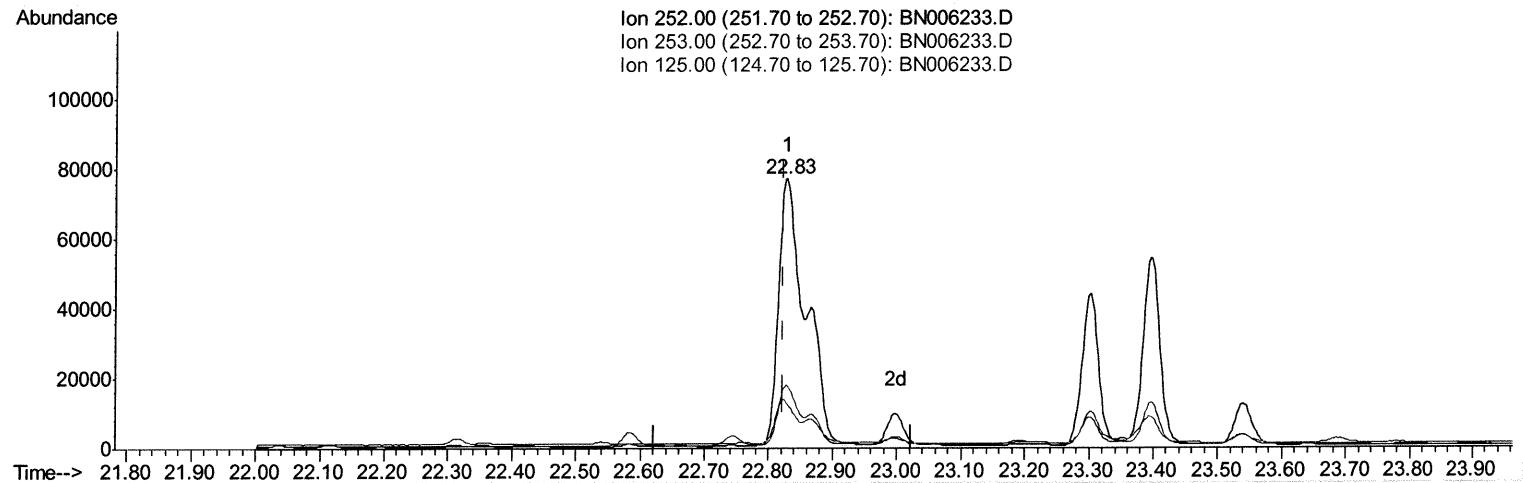

(21) Benzo(b)fluoranthene
 22.829min (+0.006) 2.80ng/ul
 response 227039

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	23.50
125.00	20.50	17.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:09:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

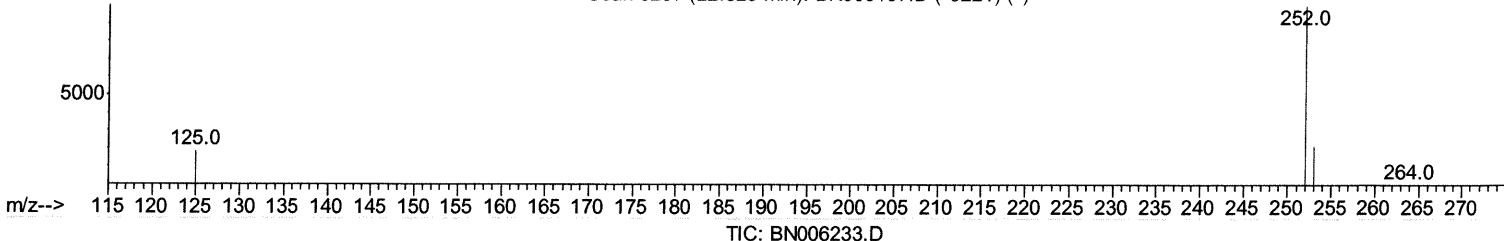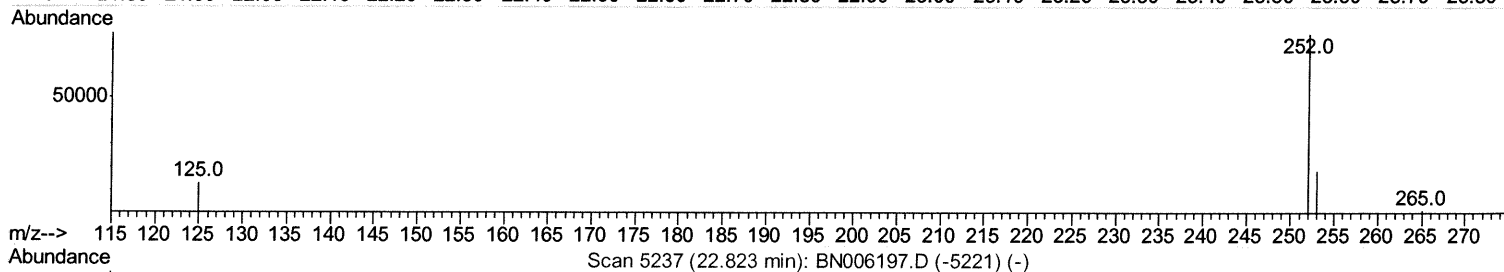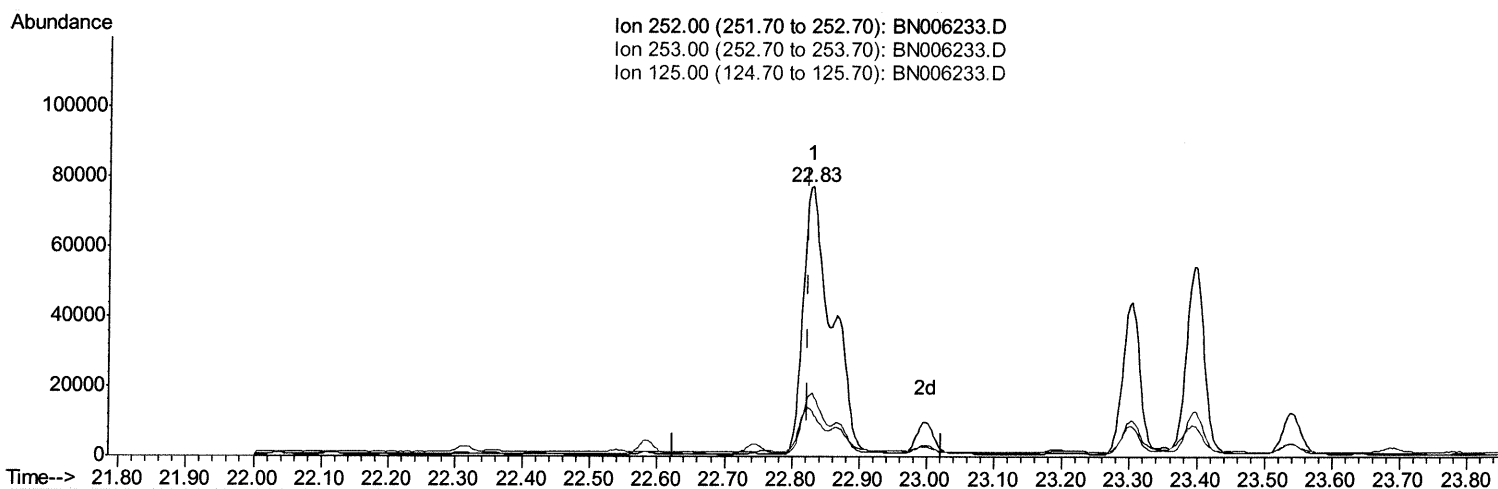

(21) Benzo(b)fluoranthene

22.829min (+0.006) 2.07ng/ul m

JU
 06/11/19

response 167568

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	23.50
125.00	20.50	17.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:09:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

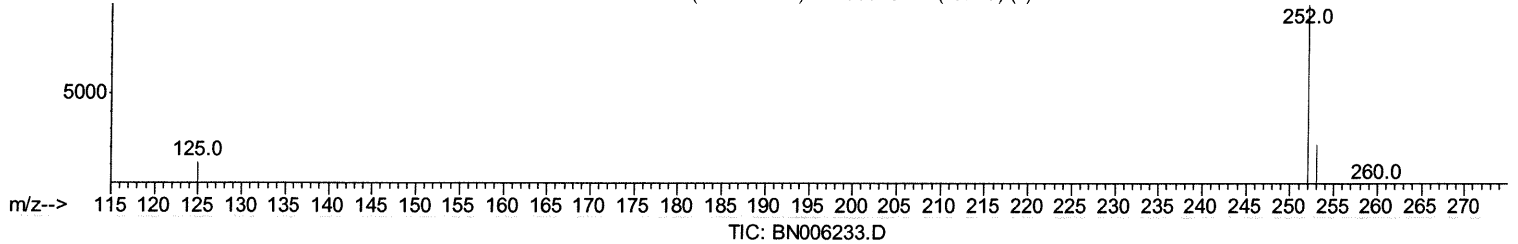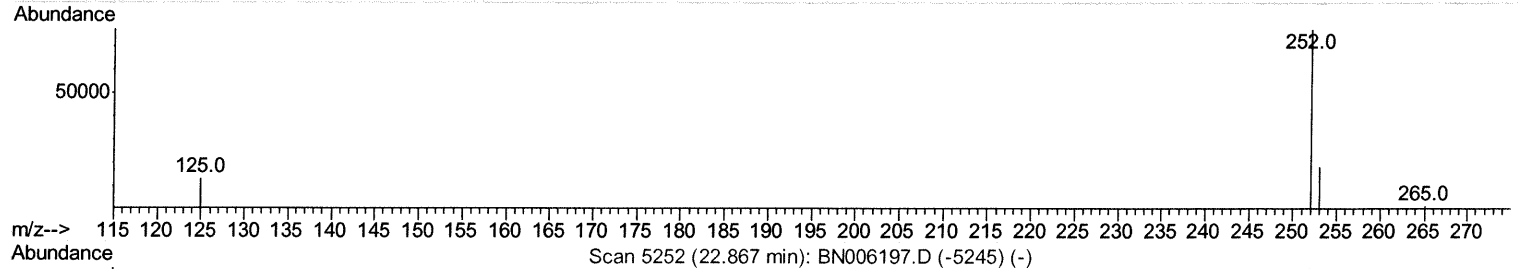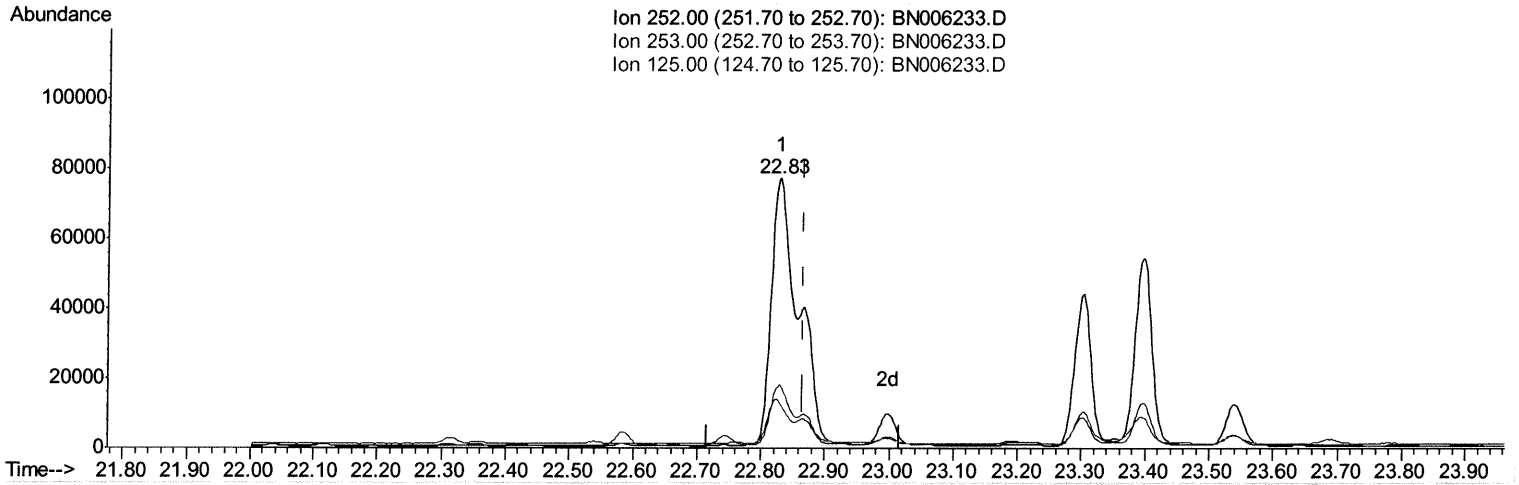

(22) Benzo(k)fluoranthene
 22.829min (-0.038) 2.88ng/ul
 response 227088

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	23.50
125.00	17.90	17.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:09:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

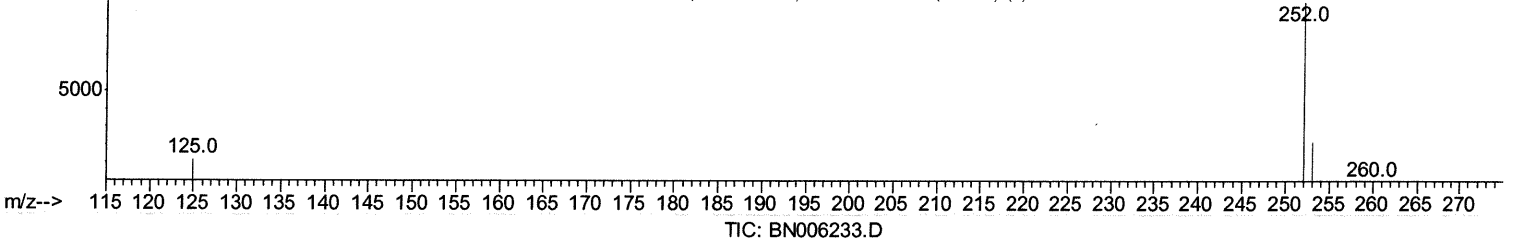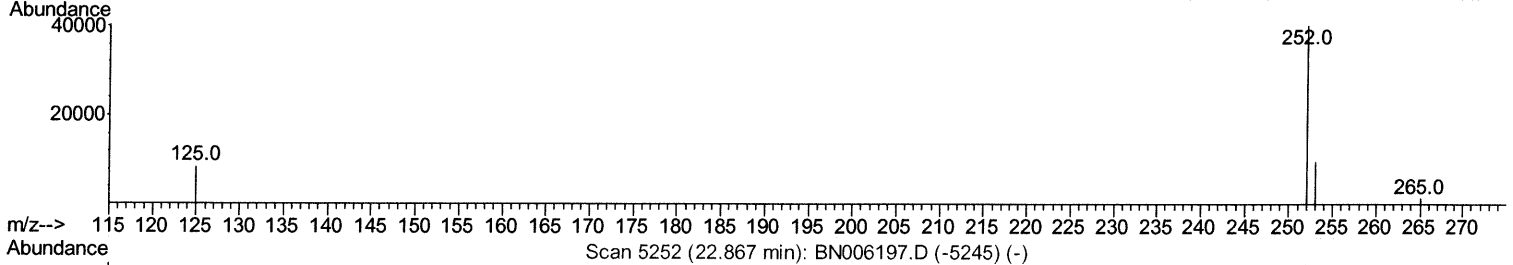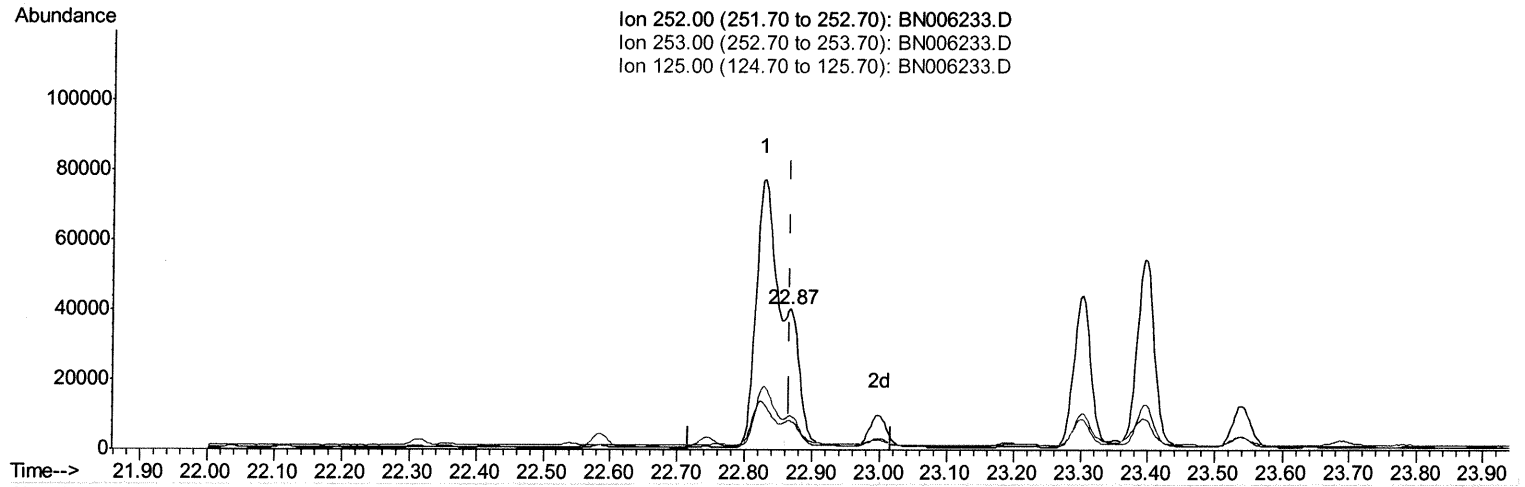

(22) Benzo(k)fluoranthene

22.867min (-0.000) 0.71ng/ul m *JU 06/11/19*

response 55724

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	24.38
125.00	17.90	21.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061019\
 Data File : BN006233.D
 Acq On : 10 Jun 2019 21:10
 Operator : JU/SJ
 Sample : K3017-20
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A51F1

Manual Integrations
 APPROVED

mohammad
 6/11/2019 4:28:49 PM

Quant Time: Jun 11 02:11:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jun 09 05:10:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4004	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15188	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	6823	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	13107m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	12317m>	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	19440	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	4811	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	9858m>	0.28	ng/ul	0.00
Target Compounds						
					Ovalue	
7) Acenaphthylene	14.01	152	6210	0.164	ng/ul	97
8) Acenaphthene	14.36	153	1277	0.049	ng/ul	96
9) Fluorene	15.35	166	2055	0.067	ng/ul#	98
12) Phenanthrene	17.09	178	73437m>	1.745	ng/ul	
13) Anthracene	17.18	178	10083m>	0.251	ng/ul	
15) Fluoranthene	19.12	202	237259m>	5.107	ng/ul	
17) Pyrene	19.49	202	186858	2.880	ng/ul	100
18) Benzo(a)anthracene	21.25	228	89181m>	1.637	ng/ul	
19) Chrysene	21.30	228	117216	2.292	ng/ul	98
21) Benzo(b)fluoranthene	22.83	252	167568m>	2.067	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	55724m>	0.706	ng/ul	
23) Benzo(a)pyrene	23.40	252	99217	1.314	ng/ul#	88
24) Indeno(1,2,3-cd)pyrene	25.72	276	82117	1.005	ng/ul#	87
25) Dibenzo(a,h)anthracene	25.73	278	18109	0.277	ng/ul#	90
26) Benzo(a,h,i)perylene	26.41	276	71697	1.048	ng/ul	96

JU 06/11/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed