

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020085.D
 Acq On : 09 Jun 2022 17:53
 Operator : CG/JU
 Sample : N3212-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 10 02:43:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	3716	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	12697	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.451	164	7988	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.192	188	17330	0.400	ng/ul	0.00
17) Chrysene-d12	21.379	240	14618	0.400	ng/ul	0.00
23) Perylene-d12	23.706	264	12244	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.286	96	22213	5.246	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.207	152	6389	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.220	212	17411	0.394	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.583	202	2213	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.560	252	4127	0.080	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020085.D
Acq On : 09 Jun 2022 17:53
Operator : CG/JU
Sample : N3212-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 10 02:43:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration




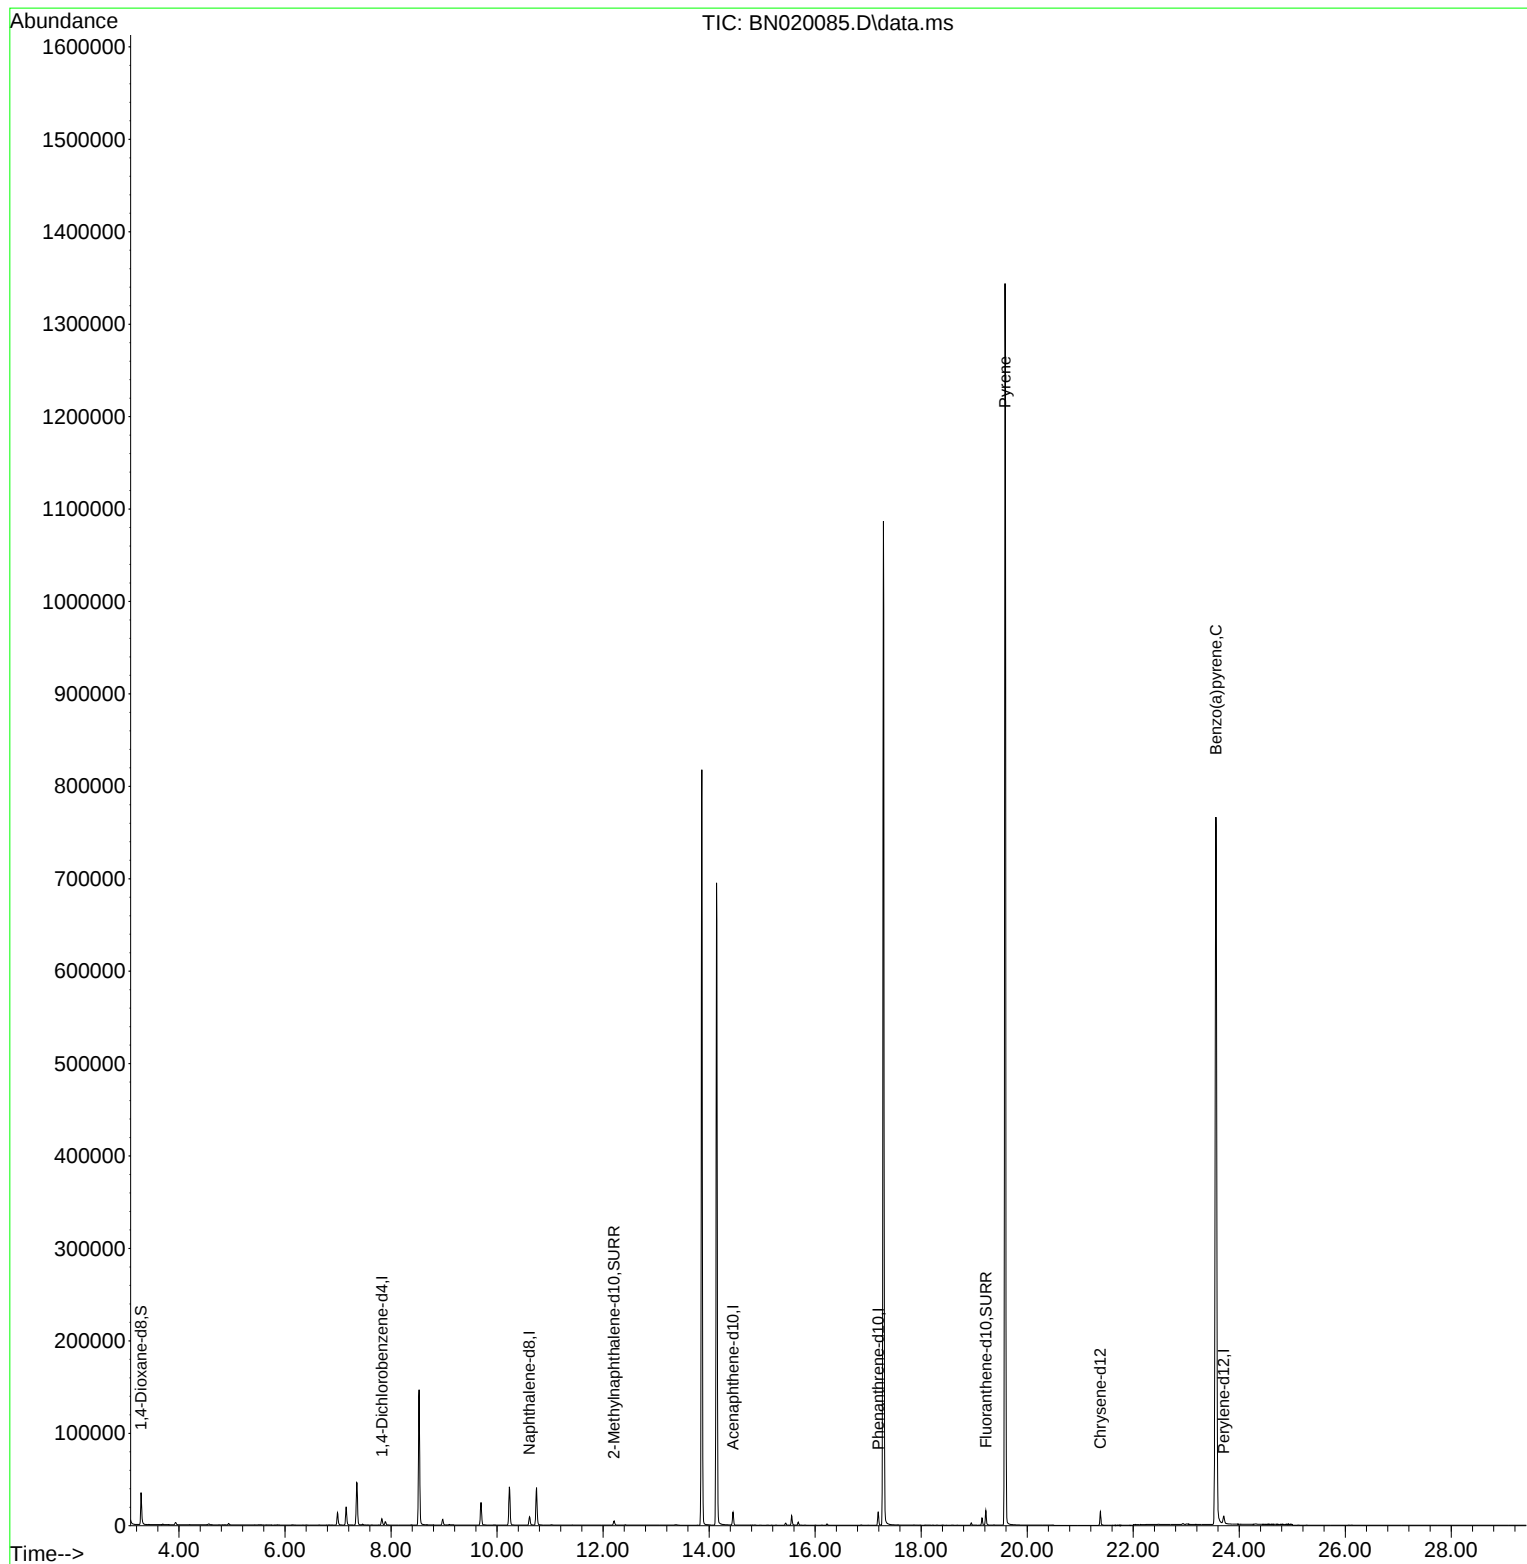


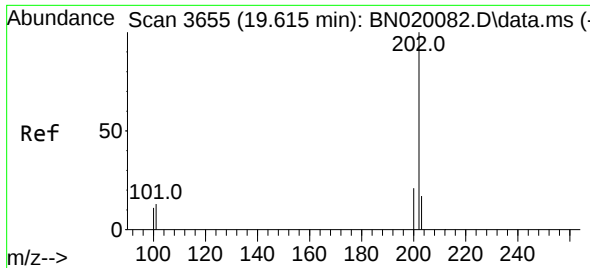

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.583 min Scan# 3648
Delta R.T. -0.032 min
Lab File: BN020085.D
Acq: 09 Jun 2022 17:53

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 2213
Ion Ratio Lower Upper
202 100
101 175.6 11.4 17.0#
100 1290.0 9.0 13.4#

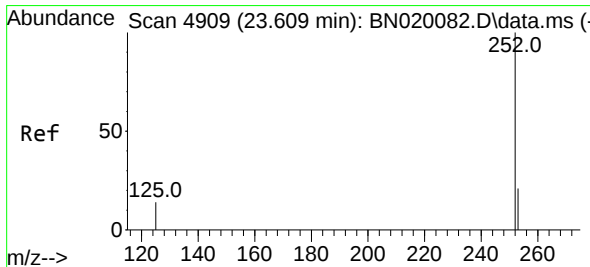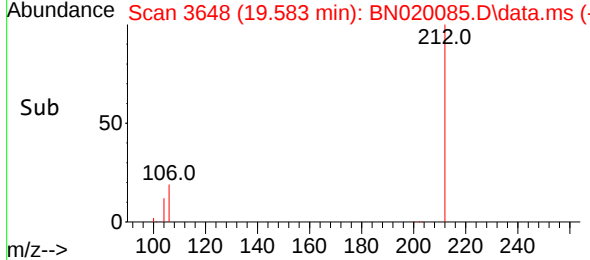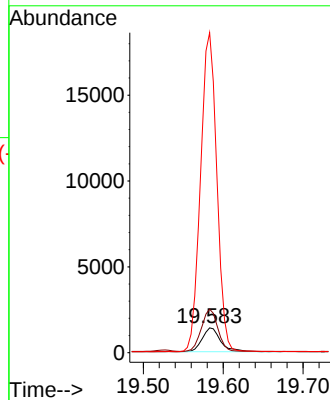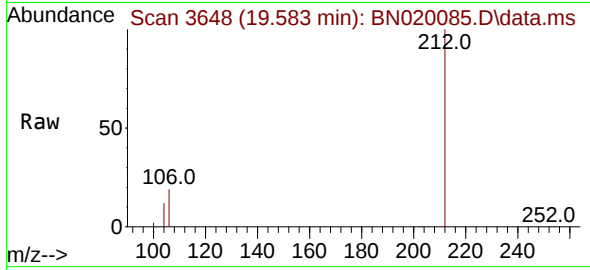

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.560 min Scan# 4892
Delta R.T. -0.049 min
Lab File: BN020085.D
Acq: 09 Jun 2022 17:53

Tgt Ion:252 Resp: 4127
Ion Ratio Lower Upper
252 100
253 43.9 23.4 35.0#
125 34.5 28.3 42.5

