

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020086.D
 Acq On : 09 Jun 2022 18:30
 Operator : CG/JU
 Sample : N3212-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 10 02:43:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	3865	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	13172	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.451	164	8269	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.192	188	17835	0.400	ng/ul	0.00
17) Chrysene-d12	21.381	240	15019	0.400	ng/ul	0.00
23) Perylene-d12	23.708	264	12981	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.285	96	17615	3.999	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	5763	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.220	212	15638	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.583	202	2811	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.558	252	4565	0.084	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020086.D
Acq On : 09 Jun 2022 18:30
Operator : CG/JU
Sample : N3212-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 10 02:43:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration




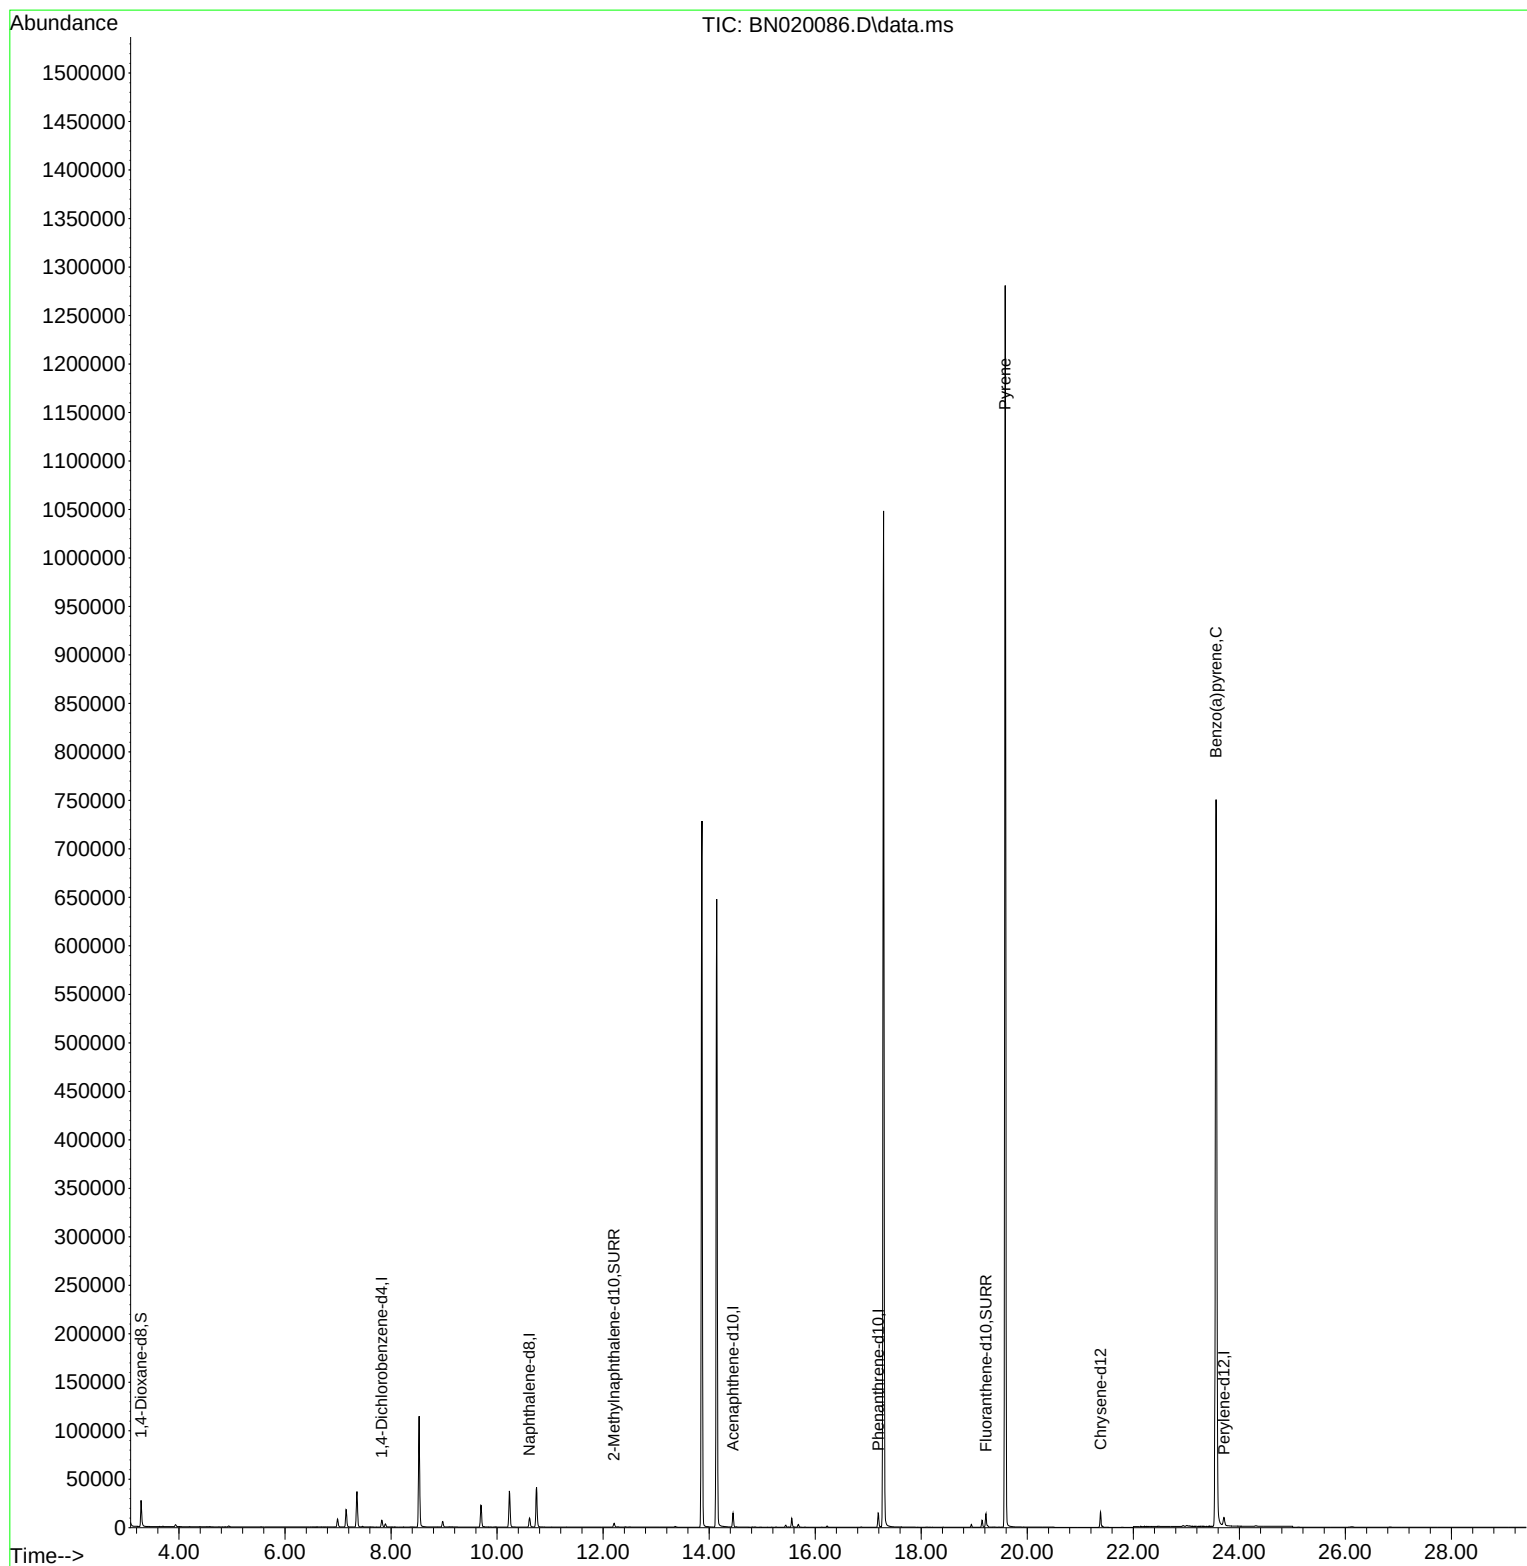


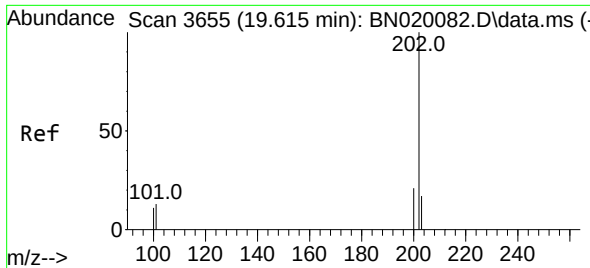

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.583 min Scan# 30
Delta R.T. -0.032 min
Lab File: BN020086.D
Acq: 09 Jun 2022 18:30

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 2811
Ion Ratio Lower Upper
202 100
101 173.4 11.4 17.0#
100 1288.4 9.0 13.4#

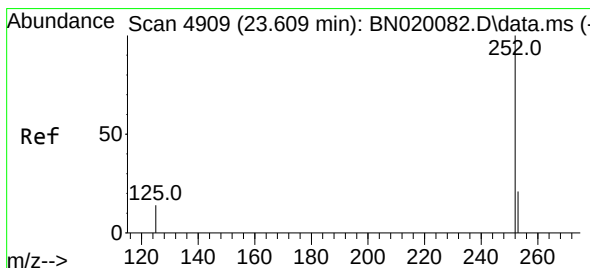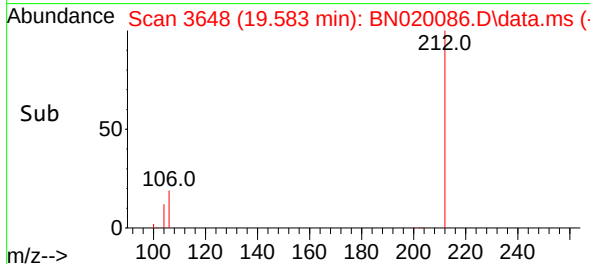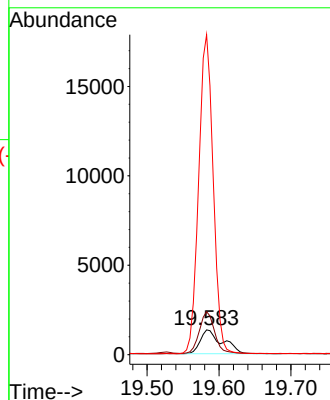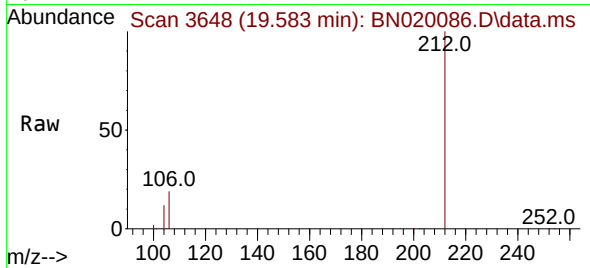

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.558 min Scan# 4891
Delta R.T. -0.051 min
Lab File: BN020086.D
Acq: 09 Jun 2022 18:30

Tgt Ion:252 Resp: 4565
Ion Ratio Lower Upper
252 100
253 42.6 23.4 35.0#
125 32.2 28.3 42.5

