

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020088.D
 Acq On : 09 Jun 2022 19:43
 Operator : CG/JU
 Sample : N3212-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 10 02:43:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	3870	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	13189	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.452	164	8267	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.188	188	17824	0.400	ng/ul	0.00
17) Chrysene-d12	21.377	240	14944	0.400	ng/ul	0.00
23) Perylene-d12	23.704	264	12351	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.285	96	18148	4.115	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	5389	0.256	ng/ul	0.00
18) Fluoranthene-d10	19.221	212	15469	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.584	202	2270	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.555	252	3914	0.075	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020088.D
Acq On : 09 Jun 2022 19:43
Operator : CG/JU
Sample : N3212-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 10 02:43:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration




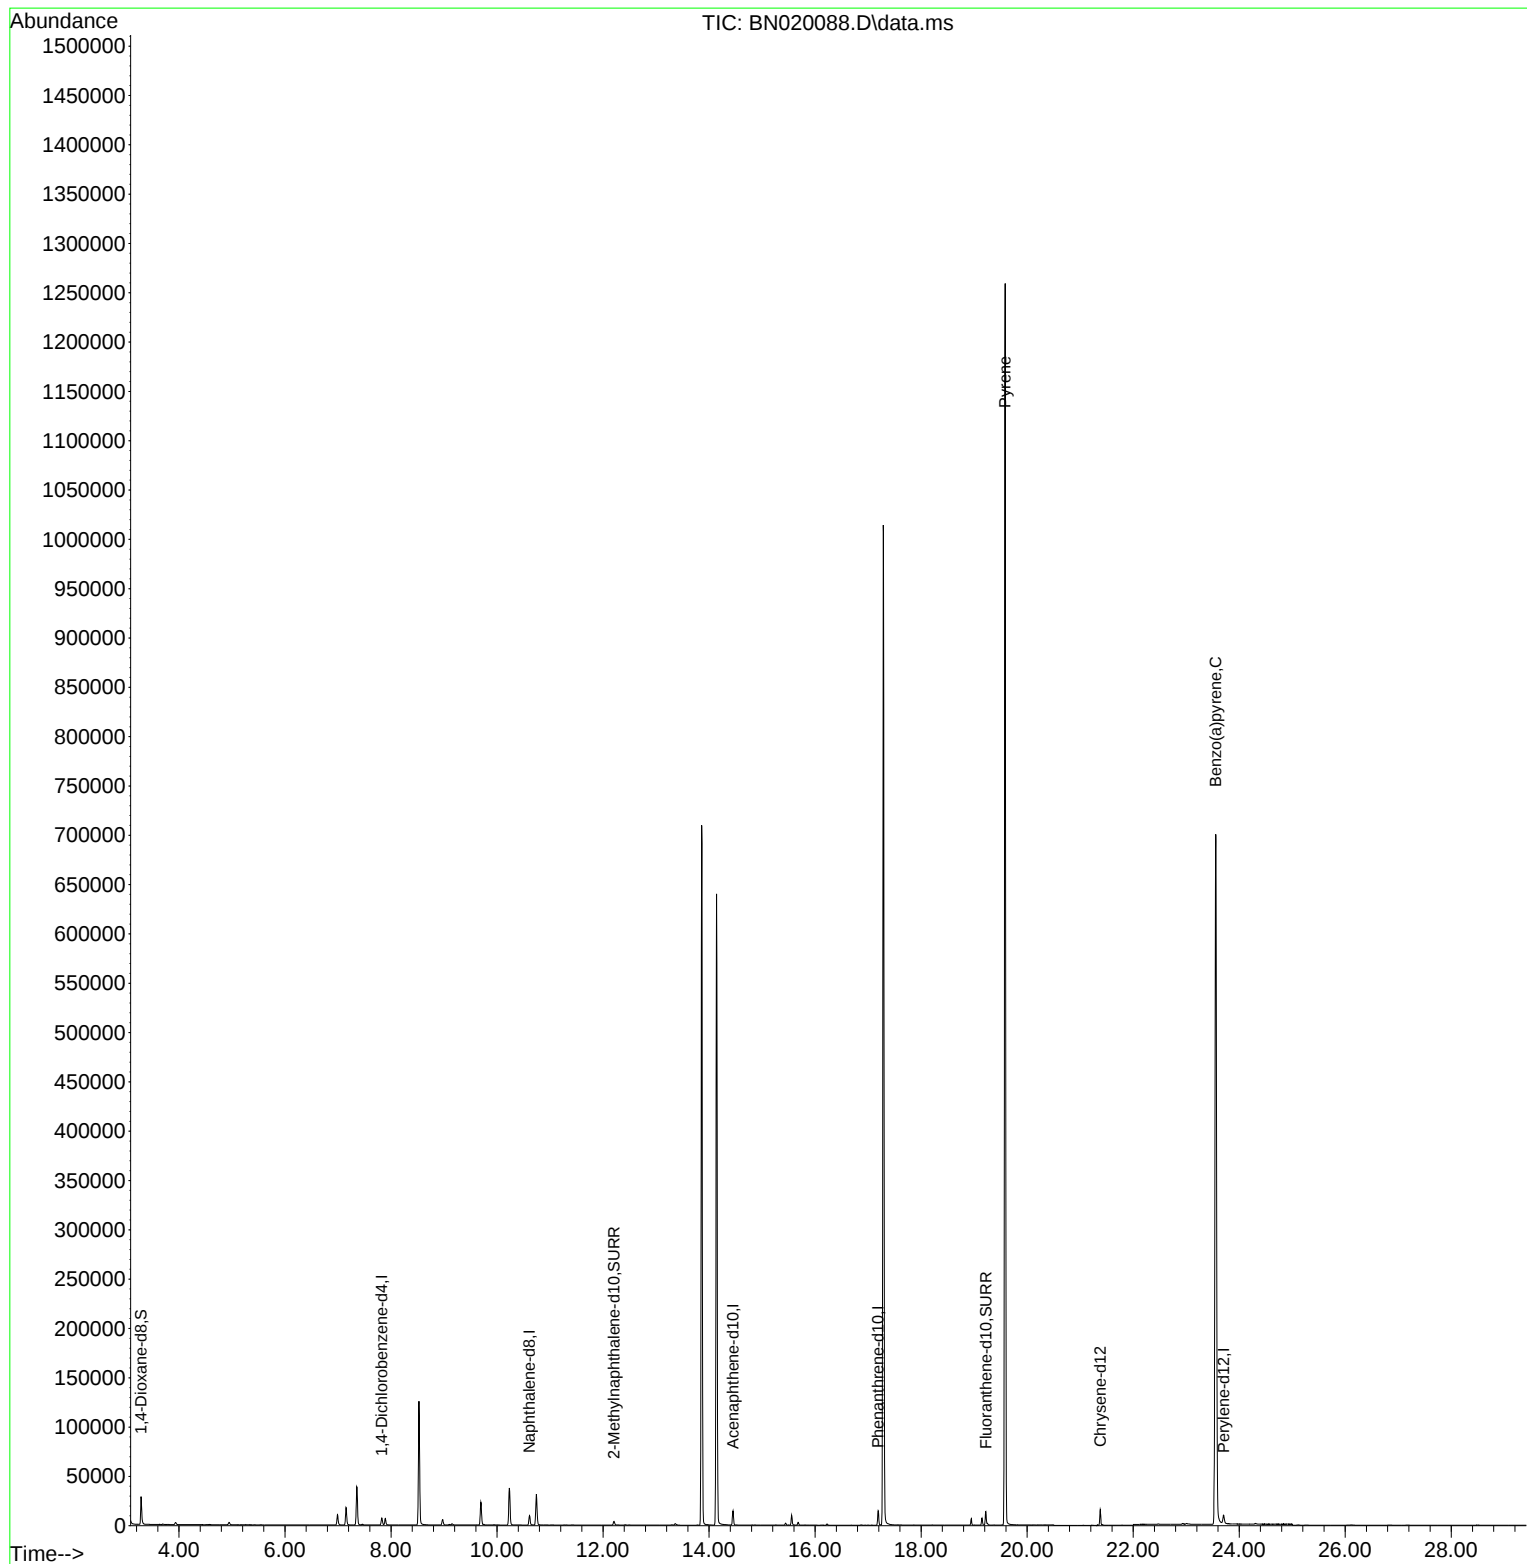


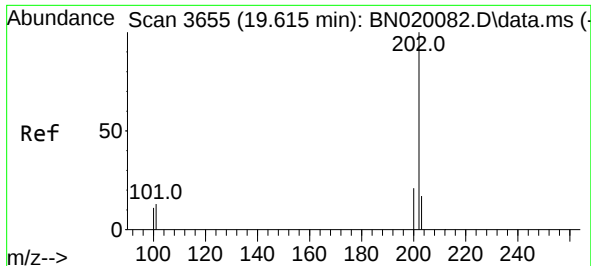

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.584 min Scan# 3648
Delta R.T. -0.032 min
Lab File: BN020088.D
Acq: 09 Jun 2022 19:43

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 2270
Ion Ratio Lower Upper
202 100
101 172.7 11.4 17.0#
100 1248.9 9.0 13.4#

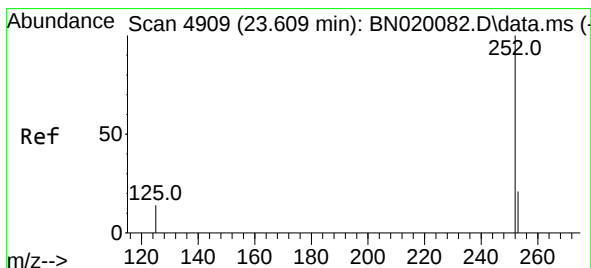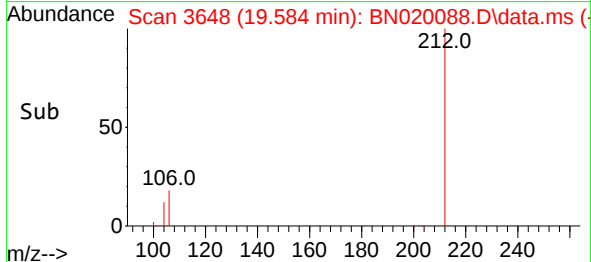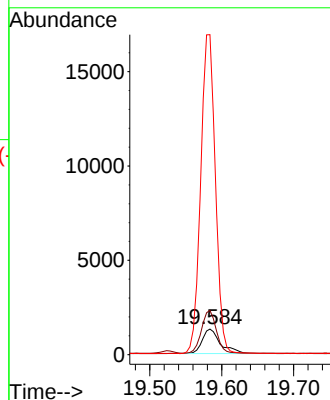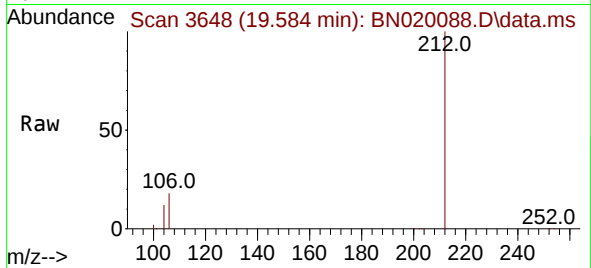

#26
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.555 min Scan# 4890
Delta R.T. -0.055 min
Lab File: BN020088.D
Acq: 09 Jun 2022 19:43

Tgt Ion:252 Resp: 3914
Ion Ratio Lower Upper
252 100
253 43.5 23.4 35.0#
125 34.9 28.3 42.5

