




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020087.D
 Acq On : 09 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3212-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A51

Manual IntegrationsAPPROVED

Quant Time: Jun 10 02:43:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

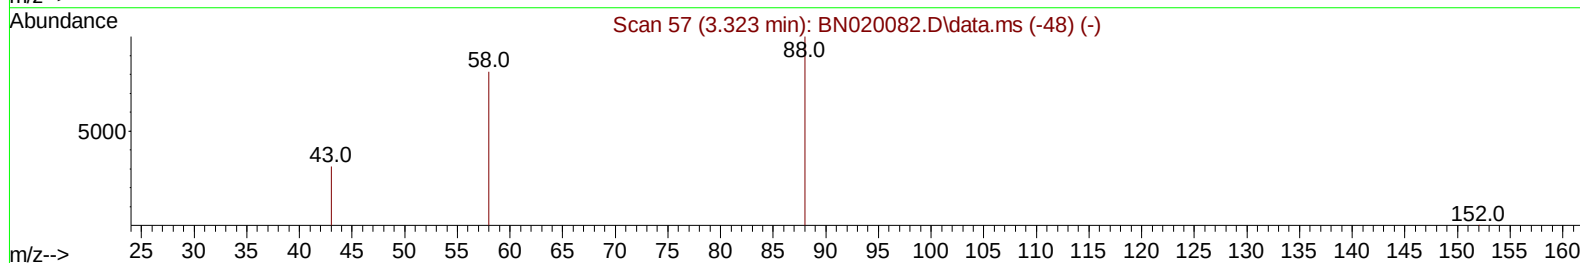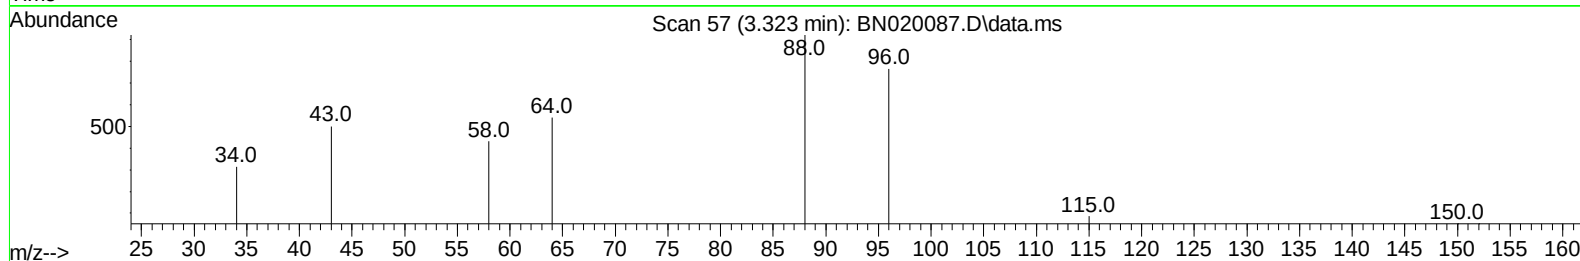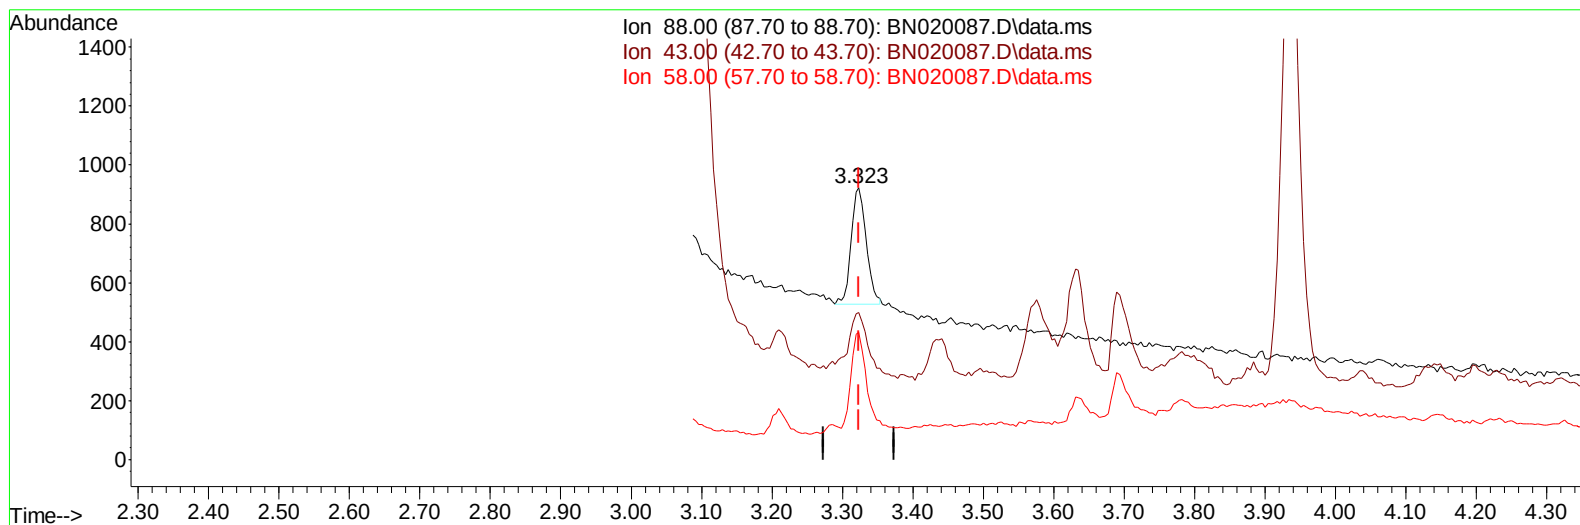

TIC: BN020087.D\data.ms

(2) 1,4-Dioxane

3.323min (+ 0.000) 0.12 ng/u1

response 580

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	54.23
58.00	49.80	46.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020087.D
Acq On : 09 Jun 2022 19:06
Operator : CG/JU
Sample : N3212-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A51

Manual IntegrationsAPPROVED

Quant Time: Jun 10 02:43:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

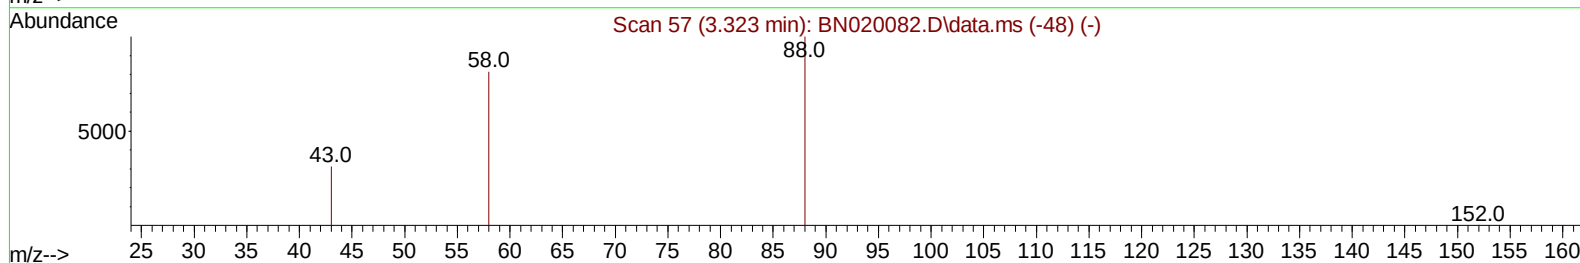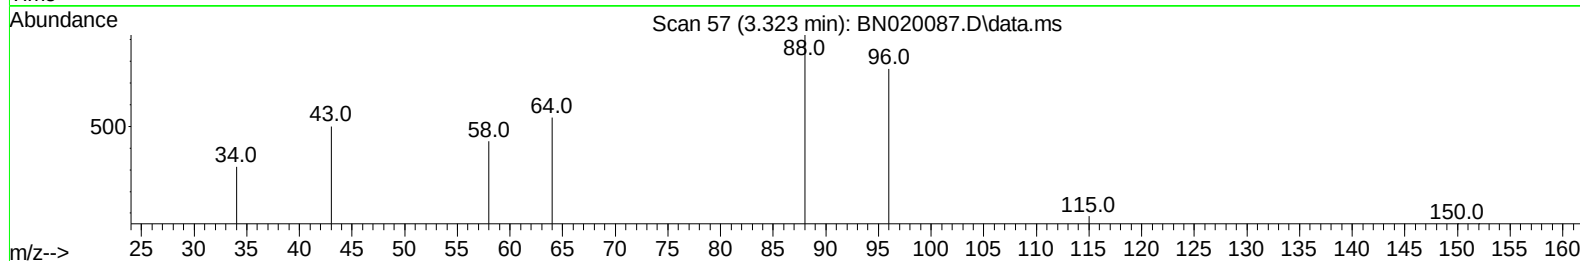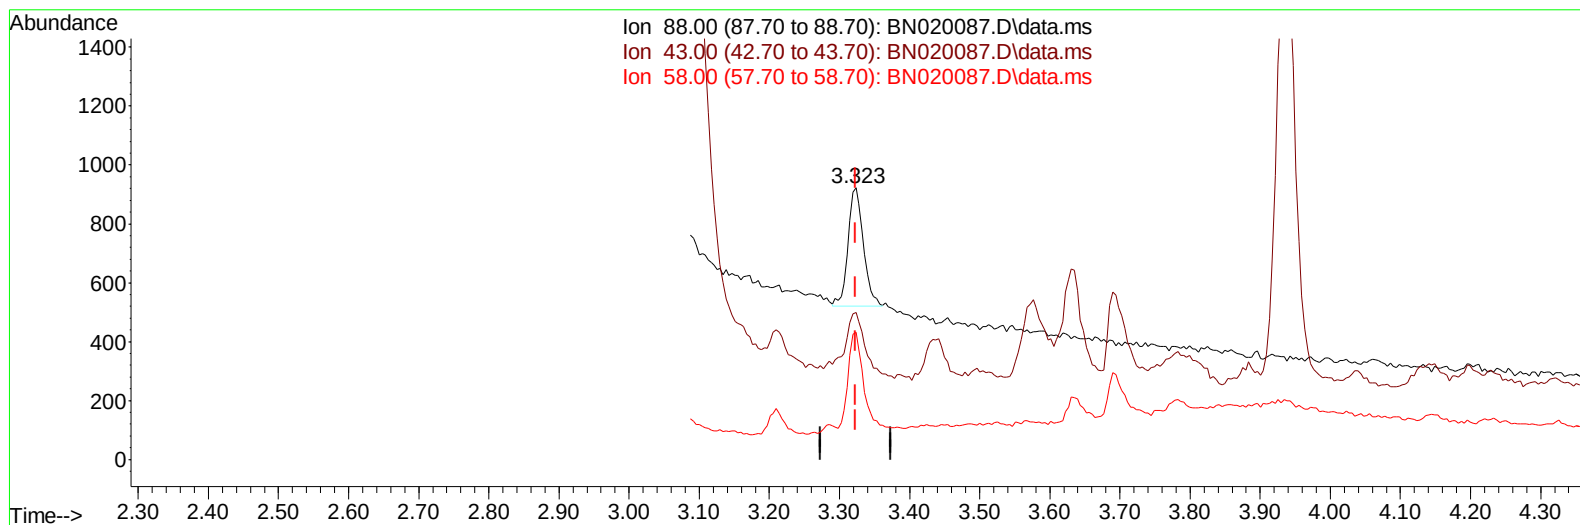

TIC: BN020087.D\data.ms

(2) 1,4-Dioxane

3.323min (+ 0.000) 0.13 ng/ul m

response 609

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	54.23
58.00	49.80	46.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
 Data File : BN020087.D
 Acq On : 09 Jun 2022 19:06
 Operator : CG/JU
 Sample : N3212-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A51

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

Quant Time: Jun 10 02:43:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 02:40:52 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.825	152		3907	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136		13441	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.451	164		8567	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.187	188		18860	0.400	ng/ul	0.00
17) Chrysene-d12	21.381	240		16107	0.400	ng/ul	0.00
23) Perylene-d12	23.708	264		13343	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.285	96		23365	5.248	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.207	152		7668	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.220	212		21143	0.434	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.323	88		609m	0.130	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061022\
Data File : BN020087.D
Acq On : 09 Jun 2022 19:06
Operator : CG/JU
Sample : N3212-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A51

Manual IntegrationsAPPROVED

Quant Time: Jun 10 02:43:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN053122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 02:40:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

